

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030521\
 Data File : PS014140.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Mar 2021 09:59
 Operator : DD\AJ
 Sample : HSTDICC750
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 11:41:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS030521.M
 Quant Title : 8080.M
 QLast Update : Fri Mar 05 11:40:03 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.204	6.901	747.8E6	281.7E6	750.000	750.000
Target Compounds							
1) T	Dalapon	3.026	2.619	793.0E6	353.4E6	682.500	682.500
2) T	3,5-DICHL...	6.421	6.058	951.5E6	396.6E6	697.500	697.500
3) T	4-Nitroph...	7.038	6.516	348.4E6	165.9E6	682.500	682.500
5) T	DICAMBA	7.392	7.067	2809.5E6	1133.8E6	705.000	705.000
6) T	MCPD	7.560	7.160	209.5E6	92026338	70.500	70.500
7) T	MCPA	7.709	7.375	301.0E6	134.9E6	69.750	69.750
8) T	DICHLORPROP	8.083	7.691	677.7E6	282.9E6	705.000	705.000
9) T	2,4-D	8.316	7.989	765.3E6	337.8E6	705.000	705.000
10) T	Pentachlo...	8.621	8.412	10408.4E6	3880.0E6	712.500	712.500
11) T	2,4,5-TP ...	9.170	8.773	4049.9E6	1571.8E6	712.500	712.500
12) T	2,4,5-T	9.457	9.155	4260.6E6	1554.0E6	712.500	712.500
13) T	2,4-DB	10.011	9.661	754.2E6	203.4E6	712.500	712.500
14) T	DINOSEB	11.162	9.988	3217.9E6	1104.1E6	705.000	705.000
15) T	Picloram	10.997	10.984	5885.0E6	2391.3E6	712.500	712.500
16) T	DCPA	11.427	10.914	6073.6E6	2391.8E6	720.000	720.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030521\
Data File : PS014140.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Mar 2021 09:59
Operator : DD\AJ
Sample : HSTDICC750
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 11:41:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS030521.M
Quant Title : 8080.M
QLast Update : Fri Mar 05 11:40:03 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

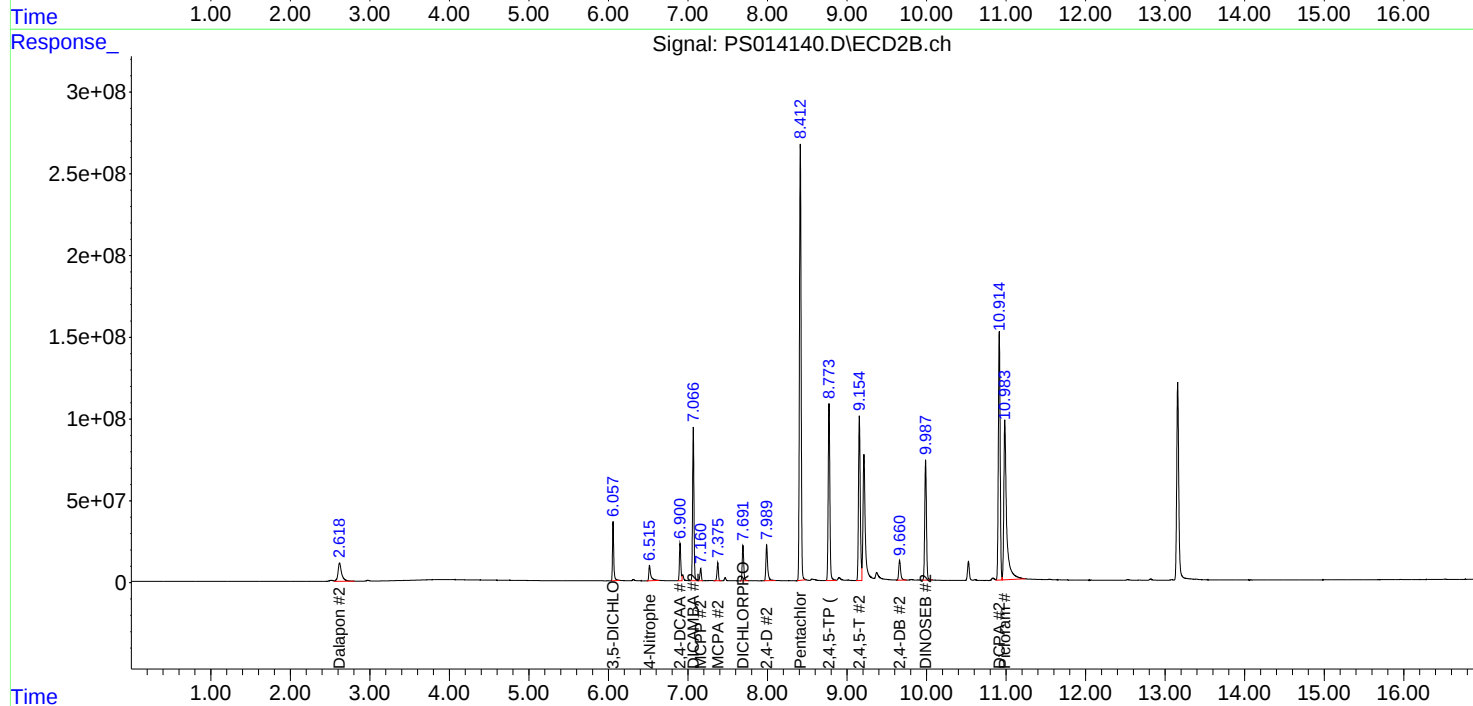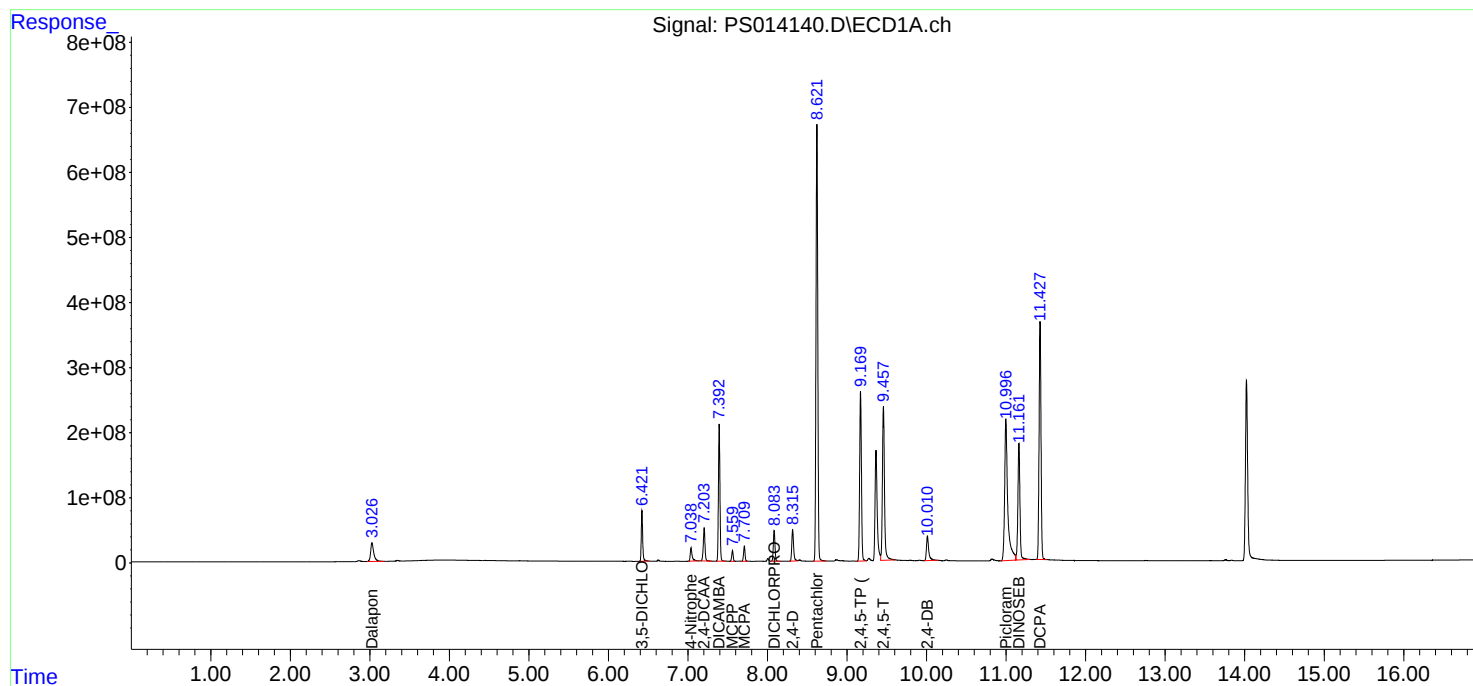


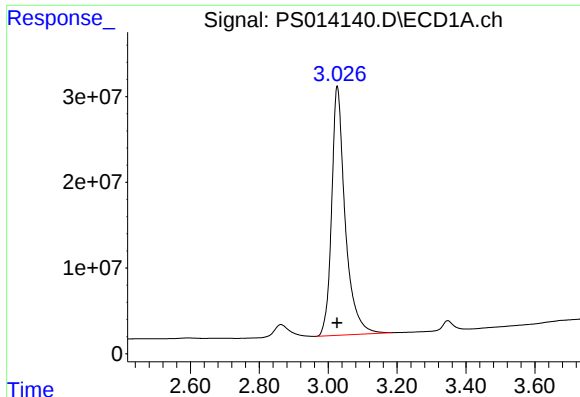

#1 Dalapon


R.T.: 3.026 min
Delta R.T.: 0.000 min
Response: 792962683
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

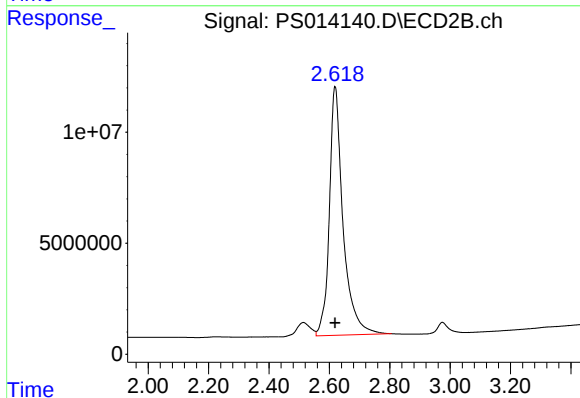


#1 Dalapon

R.T.: 2.619 min
Delta R.T.: 0.000 min
Response: 353376893
Conc: 682.50 ng/ml

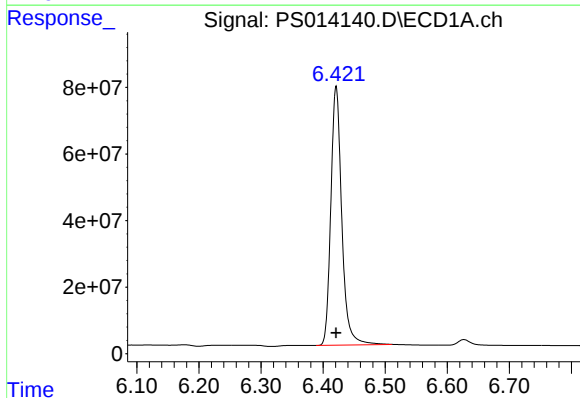


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.421 min
Delta R.T.: 0.000 min
Response: 951458880
Conc: 697.50 ng/ml

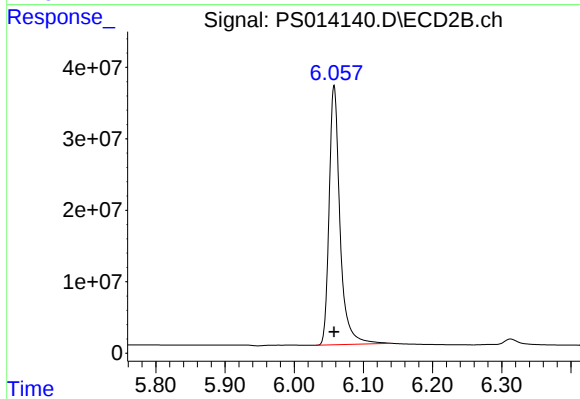

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.058 min
Delta R.T.: 0.000 min
Response: 396637675
Conc: 697.50 ng/ml

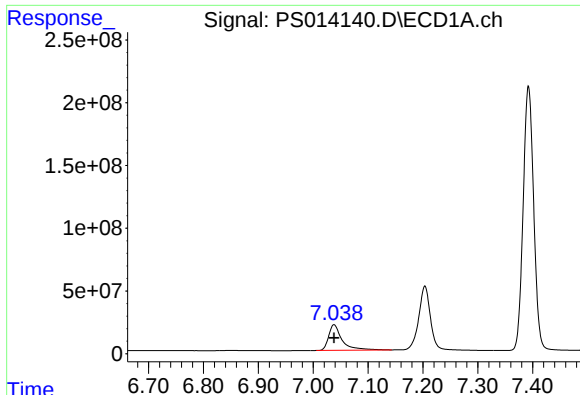

#3 4-Nitrophenol


R.T.: 7.038 min
Delta R.T.: 0.000 min
Response: 348392693
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

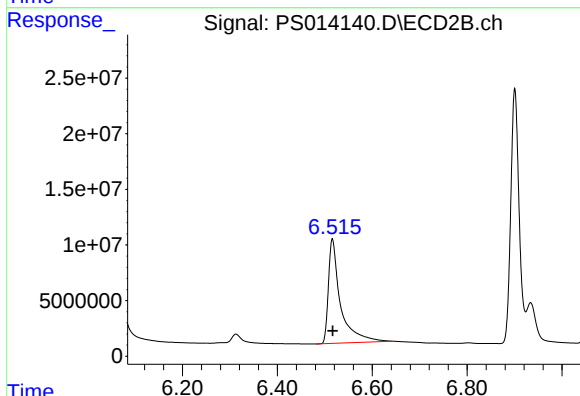


#3 4-Nitrophenol

R.T.: 6.516 min
Delta R.T.: 0.000 min
Response: 165874251
Conc: 682.50 ng/ml

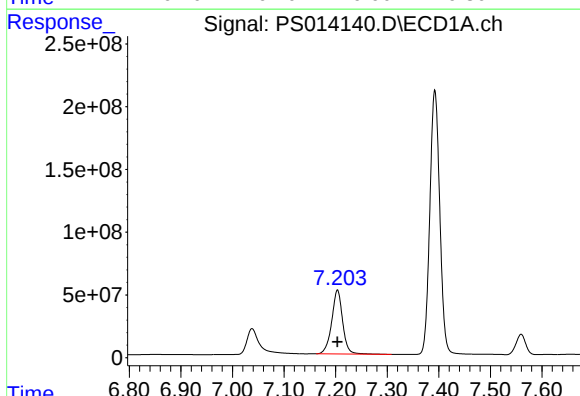


#4 2,4-DCAA

R.T.: 7.204 min
Delta R.T.: 0.000 min
Response: 747823590
Conc: 750.00 ng/ml

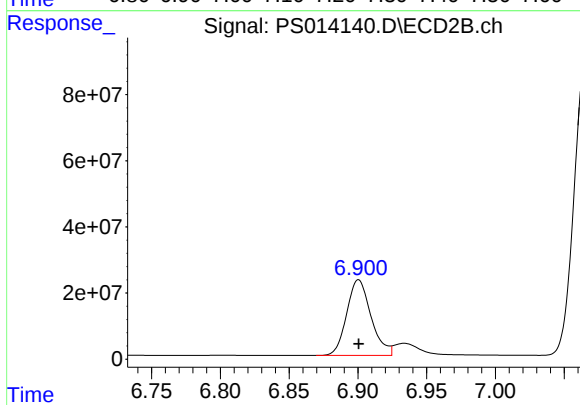

#4 2,4-DCAA


R.T.: 6.901 min
Delta R.T.: 0.000 min
Response: 281670286
Conc: 750.00 ng/ml

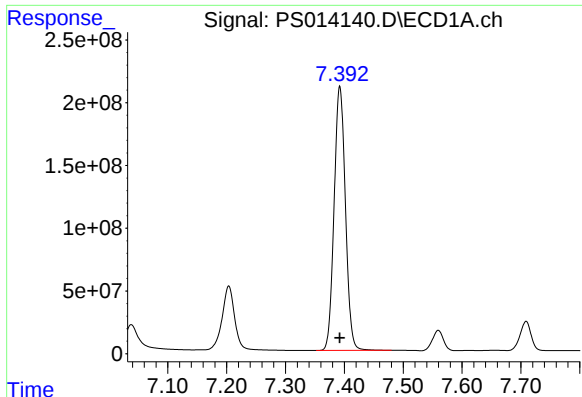

#5 DICAMBA


R.T.: 7.392 min
Delta R.T.: 0.000 min
Response: 2809511170
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

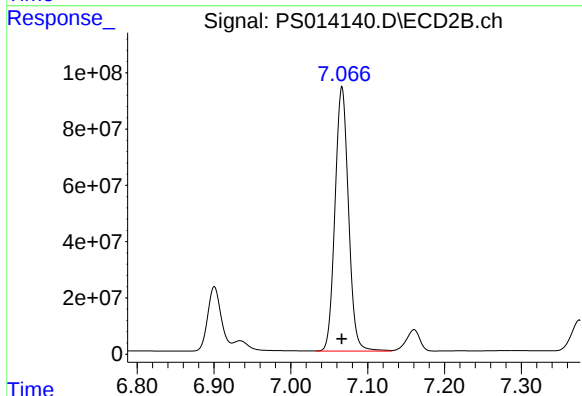


#5 DICAMBA

R.T.: 7.067 min
Delta R.T.: 0.000 min
Response: 1133794464
Conc: 705.00 ng/ml

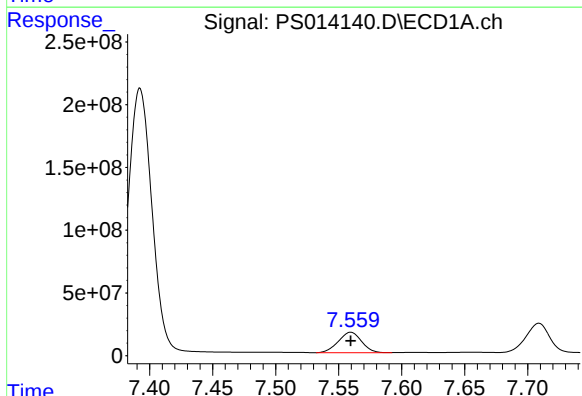


#6 MCP

R.T.: 7.560 min
Delta R.T.: 0.000 min
Response: 209504442
Conc: 70.50 ug/ml

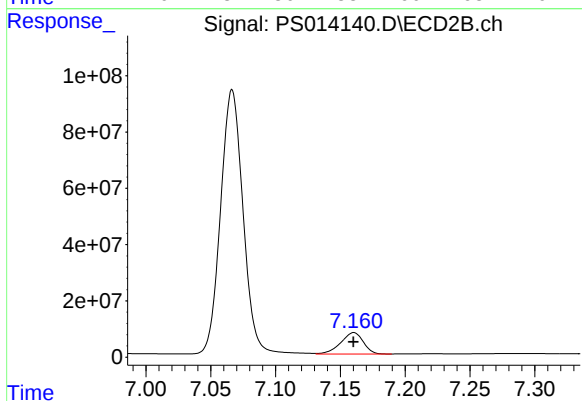

#6 MCP


R.T.: 7.160 min
Delta R.T.: 0.000 min
Response: 92026338
Conc: 70.50 ug/ml

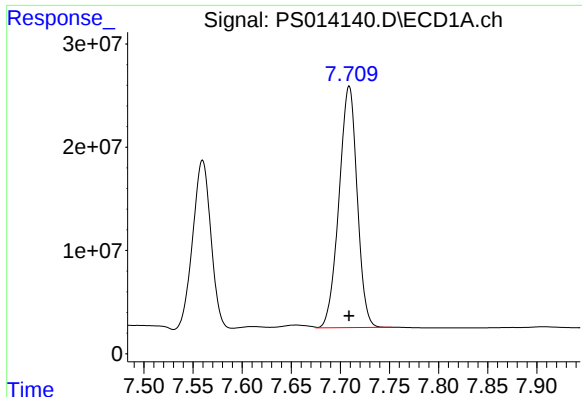

#7 MCPA


R.T.: 7.709 min
Delta R.T.: 0.000 min
Response: 301046957
Conc: 69.75 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

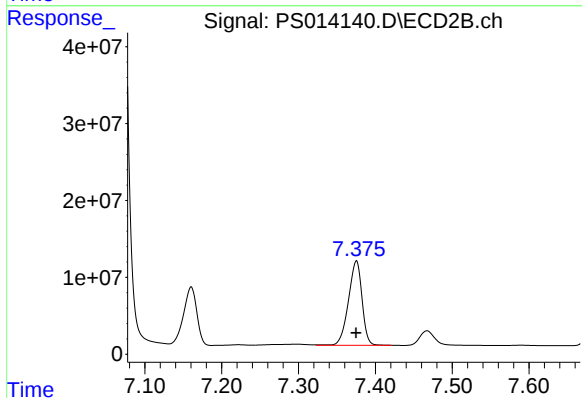


#7 MCPA

R.T.: 7.375 min
Delta R.T.: 0.000 min
Response: 134879542
Conc: 69.75 ug/ml

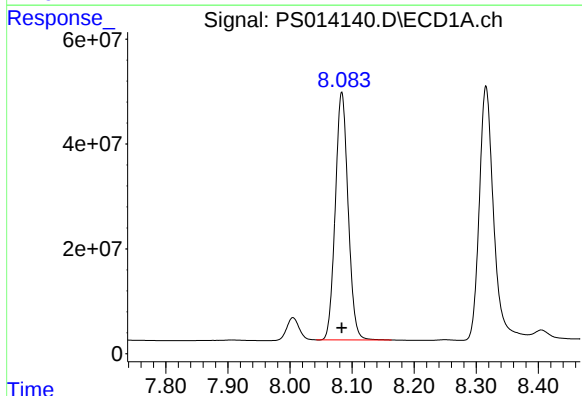


#8 DICHLORPROP

R.T.: 8.083 min
Delta R.T.: 0.000 min
Response: 677659623
Conc: 705.00 ng/ml

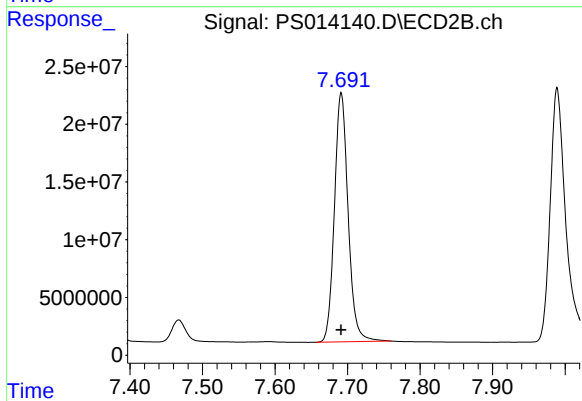

#8 DICHLORPROP


R.T.: 7.691 min
Delta R.T.: 0.000 min
Response: 282919777
Conc: 705.00 ng/ml

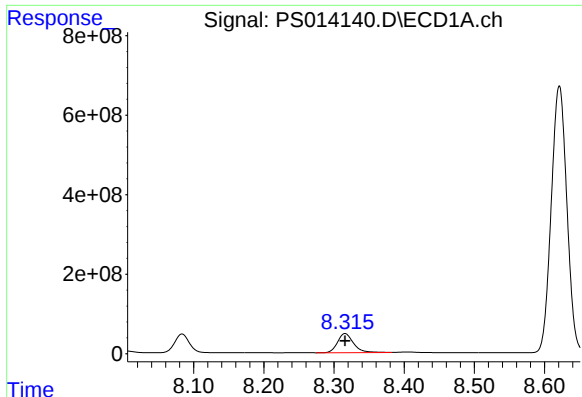

#9 2,4-D


R.T.: 8.316 min
Delta R.T.: 0.000 min
Response: 765276667
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

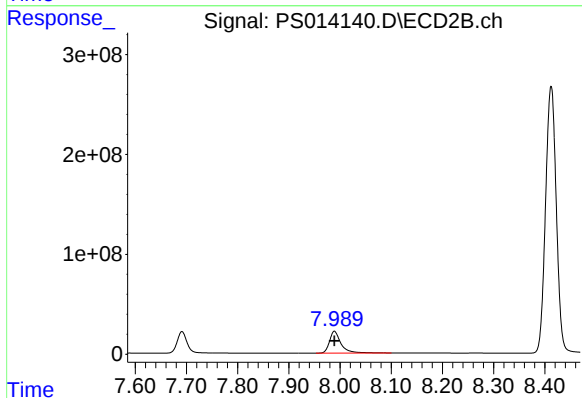


#9 2,4-D

R.T.: 7.989 min
Delta R.T.: 0.000 min
Response: 337824201
Conc: 705.00 ng/ml

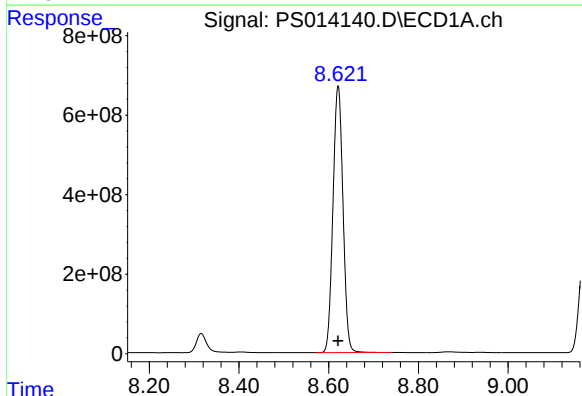


#10 Pentachlorophenol

R.T.: 8.621 min
Delta R.T.: 0.000 min
Response: 10408429258
Conc: 712.50 ng/ml

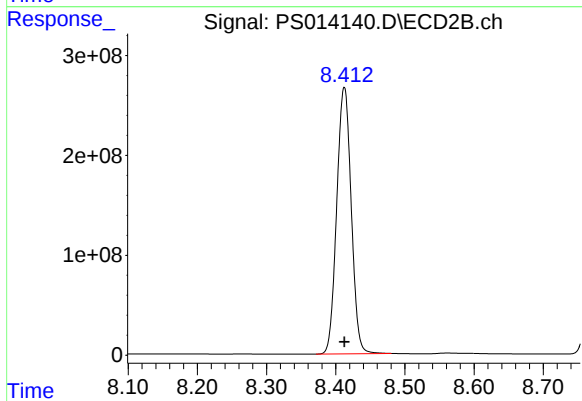

#10 Pentachlorophenol


R.T.: 8.412 min
Delta R.T.: 0.000 min
Response: 3880031603
Conc: 712.50 ng/ml

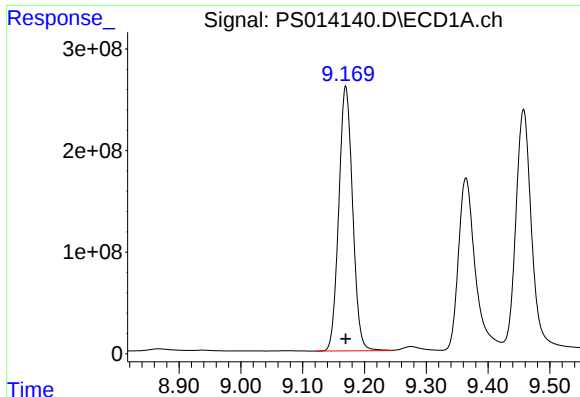

#11 2,4,5-TP (SILVEX)


R.T.: 9.170 min
Delta R.T.: 0.000 min
Response: 4049857299
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

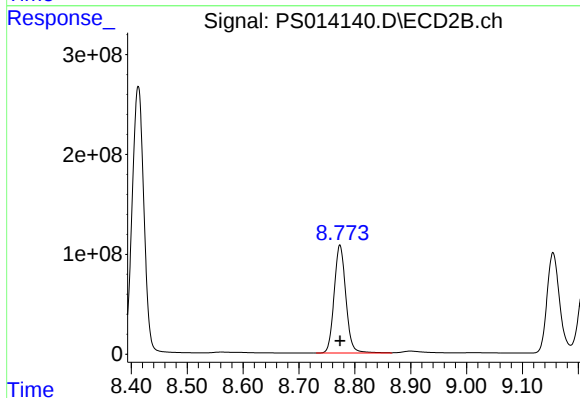


#11 2,4,5-TP (SILVEX)

R.T.: 8.773 min
Delta R.T.: 0.000 min
Response: 1571822962
Conc: 712.50 ng/ml

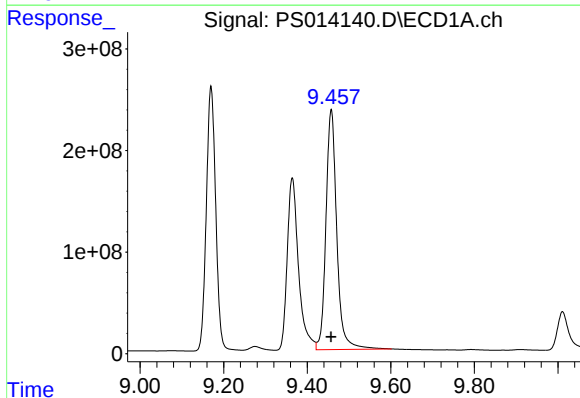


#12 2,4,5-T

R.T.: 9.457 min
Delta R.T.: 0.000 min
Response: 4260578067
Conc: 712.50 ng/ml

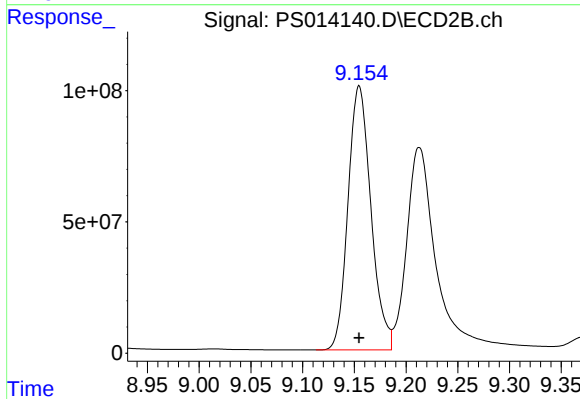

#12 2,4,5-T


R.T.: 9.155 min
Delta R.T.: 0.000 min
Response: 1553995214
Conc: 712.50 ng/ml

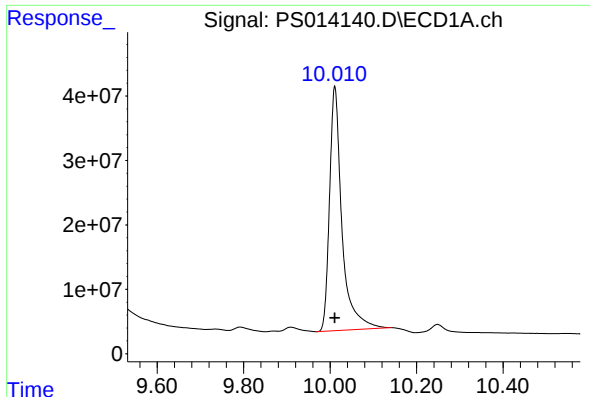

#13 2,4-DB


R.T.: 10.011 min
Delta R.T.: 0.000 min
Response: 754175973
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

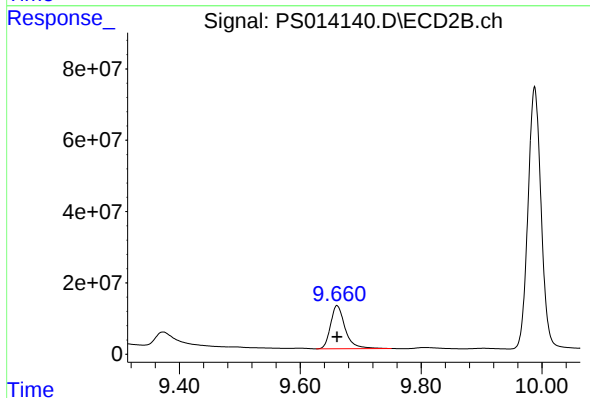


#13 2,4-DB

R.T.: 9.661 min
Delta R.T.: 0.000 min
Response: 203436787
Conc: 712.50 ng/ml

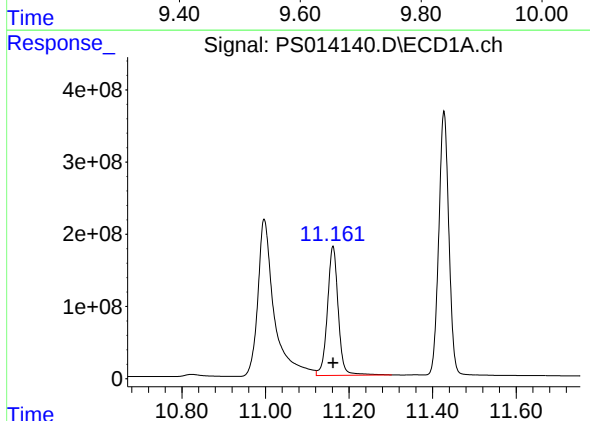


#14 DINOSEB

R.T.: 11.162 min
Delta R.T.: 0.000 min
Response: 3217879433
Conc: 705.00 ng/ml

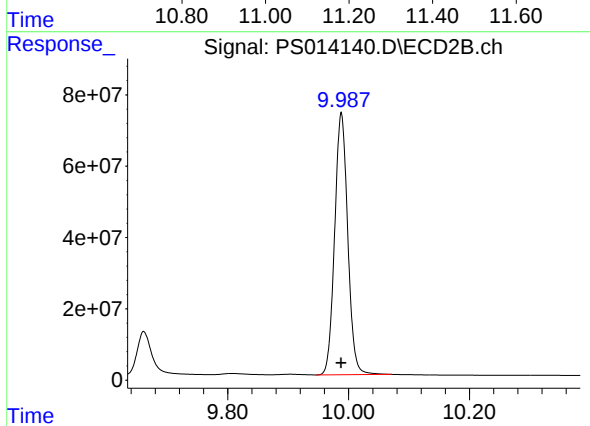

#14 DINOSEB


R.T.: 9.988 min
Delta R.T.: 0.000 min
Response: 1104094009
Conc: 705.00 ng/ml

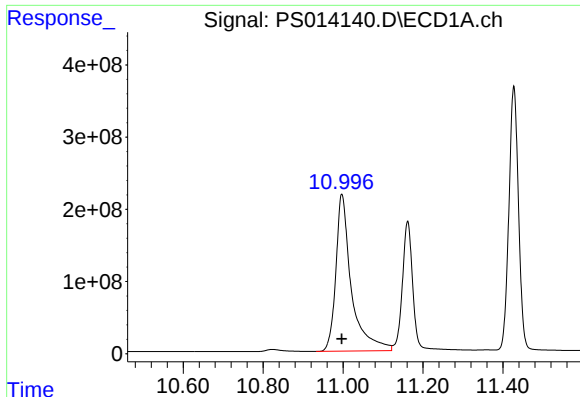

#15 Picloram


R.T.: 10.997 min
Delta R.T.: 0.000 min
Response: 5885029334
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

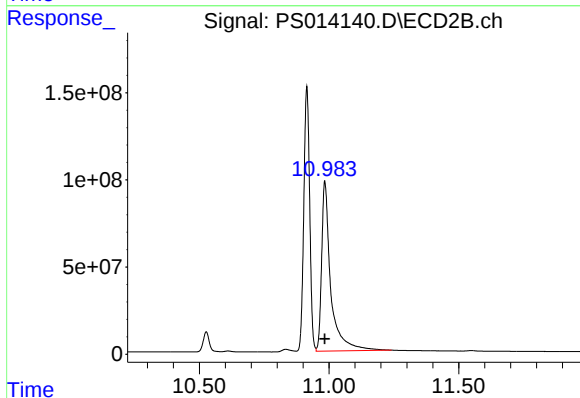


#15 Picloram

R.T.: 10.984 min
Delta R.T.: 0.000 min
Response: 2391251084
Conc: 712.50 ng/ml

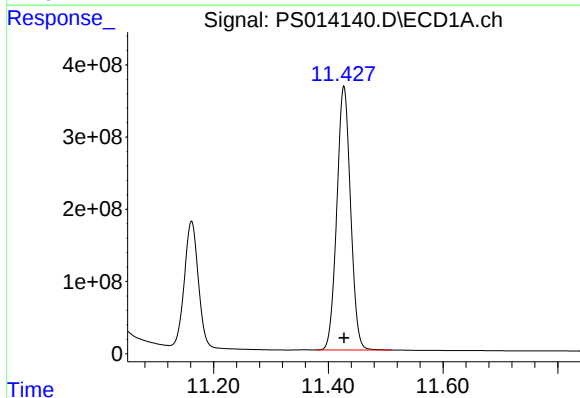

#16 DCPA

R.T.: 11.427 min
Delta R.T.: 0.000 min
Response: 6073602416
Conc: 720.00 ng/ml

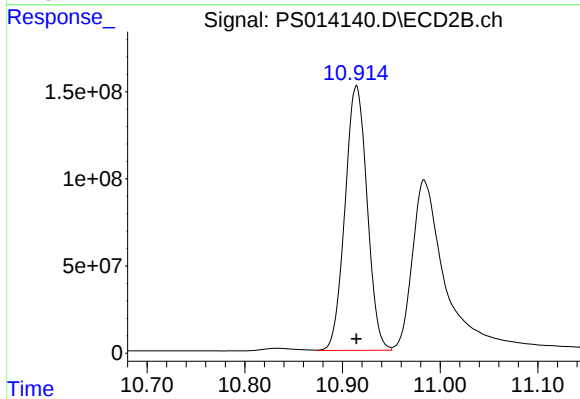

#16 DCPA

R.T.: 10.914 min
Delta R.T.: 0.000 min
Response: 2391811299
Conc: 720.00 ng/ml