

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030525\
 Data File : PS029368.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Mar 2025 00:04
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 06 03:49:48 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022125.M
 Quant Title : 8080.M
 QLast Update : Sat Feb 22 01:02:20 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.160	7.626	2195.8E6	482.8E6	532.876	513.434
Target Compounds							
1) T	Dalapon	0.000	2.684f	0	10490180	N.D.	4.955
2) T	3,5-DICHL...	6.338	0.000	1260940	0	<MDL	N.D. #
3) T	4-Nitroph...	6.955	0.000	11830968	0	5.056	N.D. #
5) T	DICAMBA	7.338	7.827	-11346019	3590881	N.D.	<MDL
8) T	DICHLORPROP	8.030	8.579f	4725096	15452119	1.028	12.084 #
10) T	Pentachlo...	8.566	0.000	6658988	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.110f	9.756	17622227	25738427	<MDL	2.848 #
12) T	2,4,5-T	9.385f	0.000	14592263	0	<MDL	N.D. #
13) T	2,4-DB	10.026f	0.000	8675362	0	2.078	N.D. #
15) T	Picloram	10.995	0.000	4239867	0	<MDL	N.D. #
16) T	DCPA	11.484	0.000	2557720	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030525\
Data File : PS029368.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2025 00:04
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 06 03:49:48 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022125.M
Quant Title : 8080.M
QLast Update : Sat Feb 22 01:02:20 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

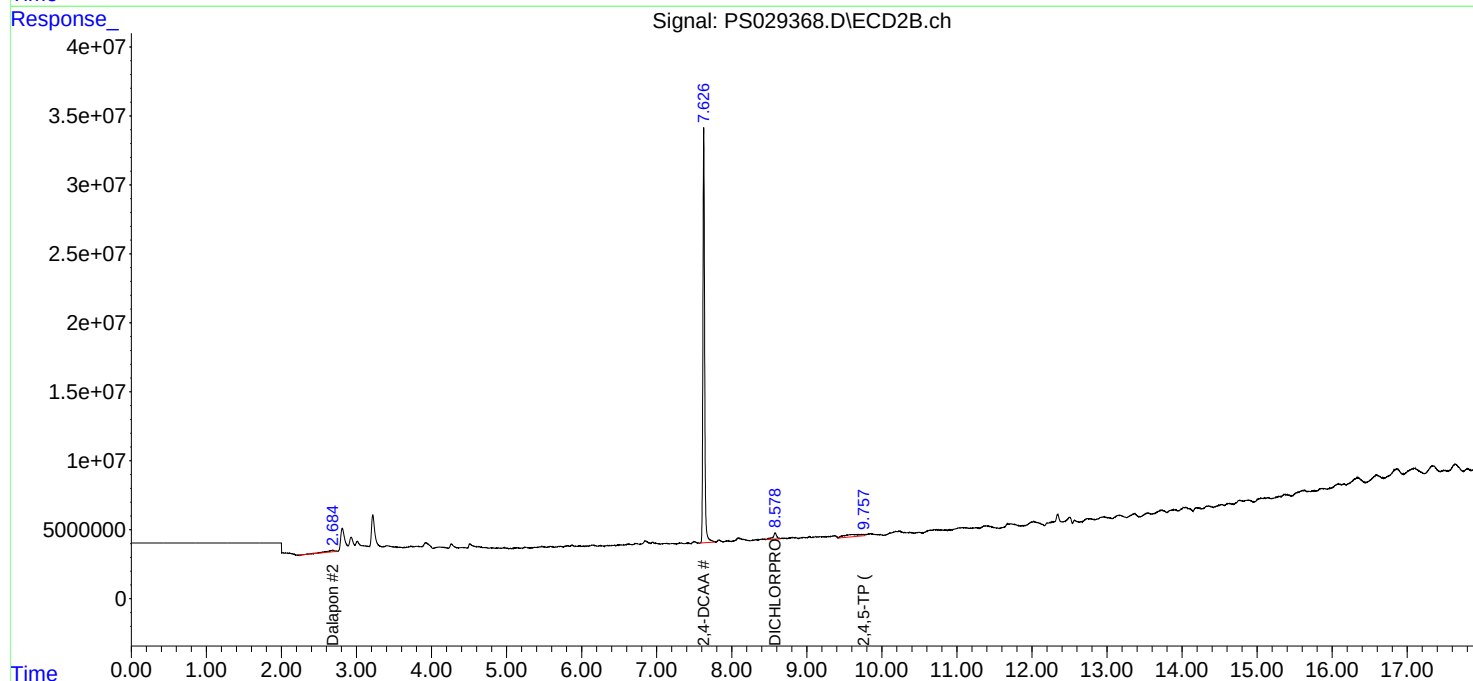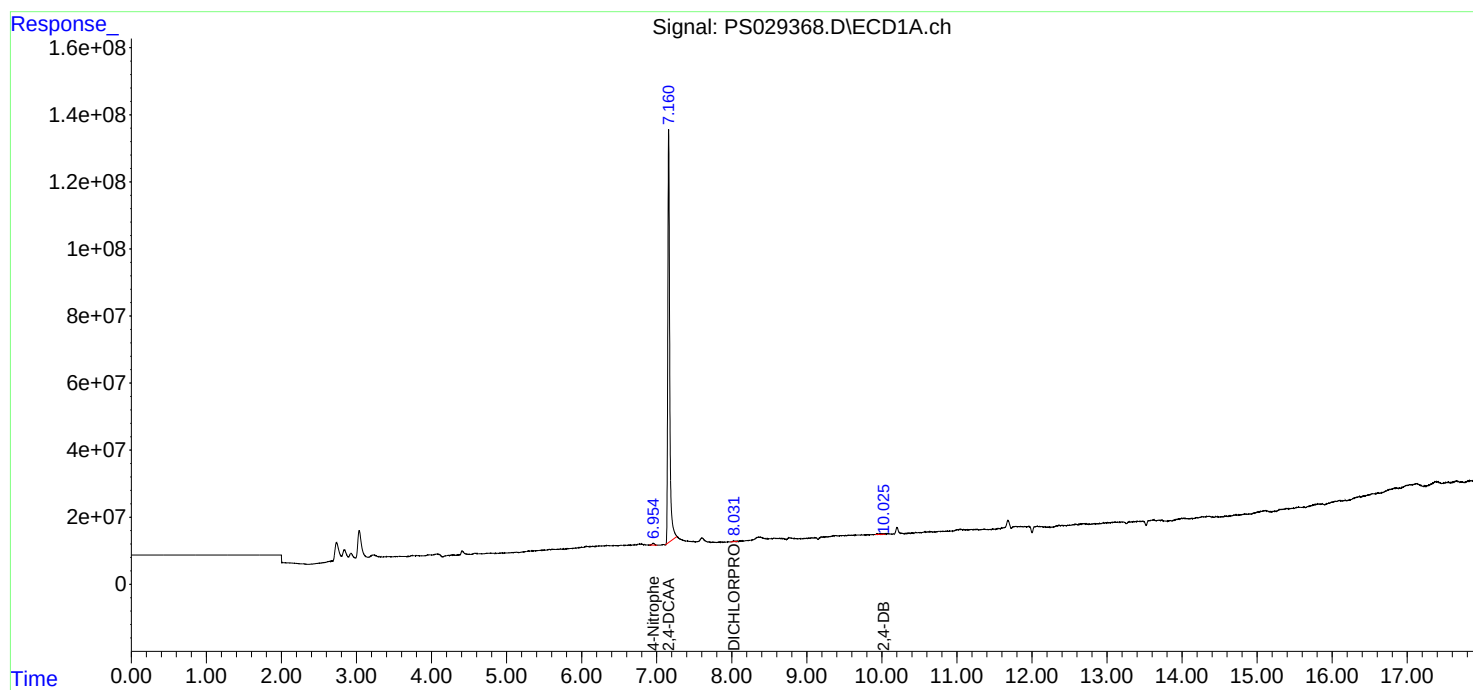


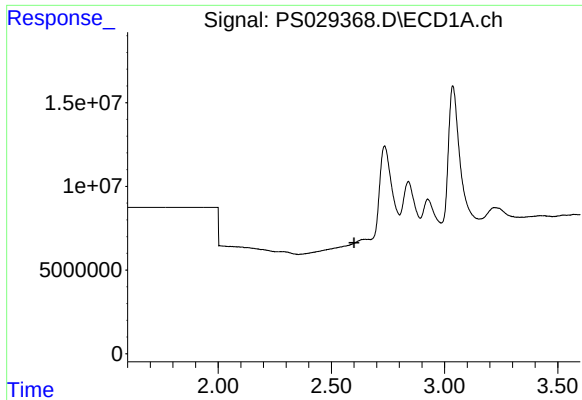

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.600 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

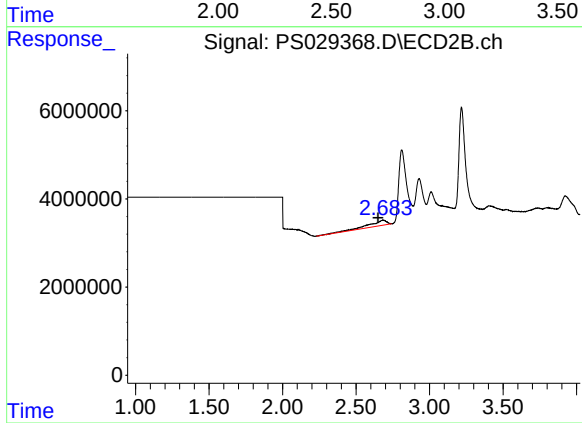


#1 Dalapon

R.T.: 2.684 min
Delta R.T.: 0.033 min
Response: 10490180
Conc: 4.95 ng/ml

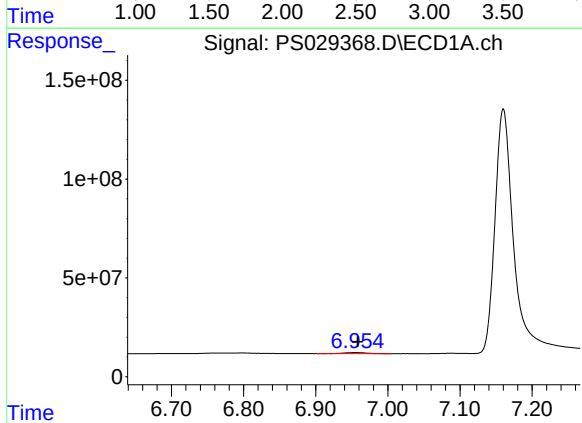


#3 4-Nitrophenol

R.T.: 6.955 min
Delta R.T.: -0.004 min
Response: 11830968
Conc: 5.06 ng/ml

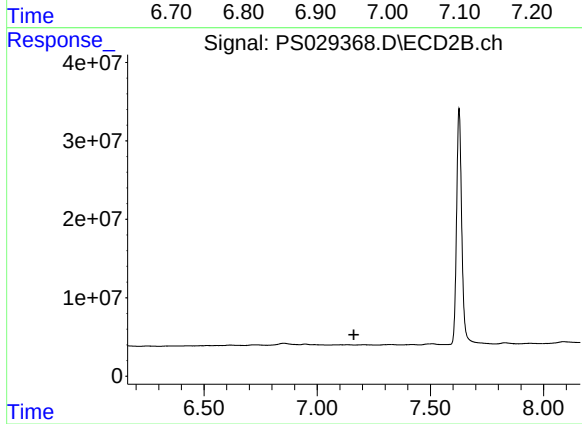

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.162 min
Response: 0
Conc: N.D.

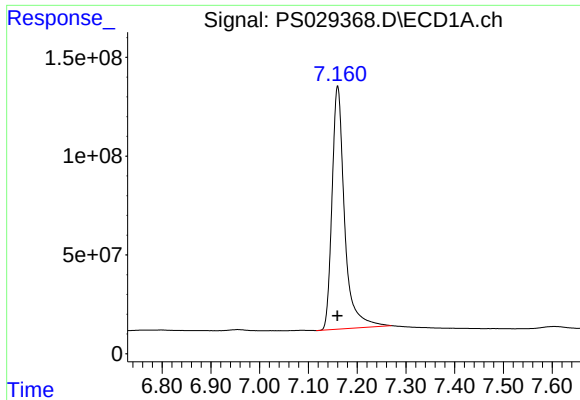

#4 2,4-DCAA


R.T.: 7.160 min
Delta R.T.: 0.000 min
Response: 2195755089
Conc: 532.88 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

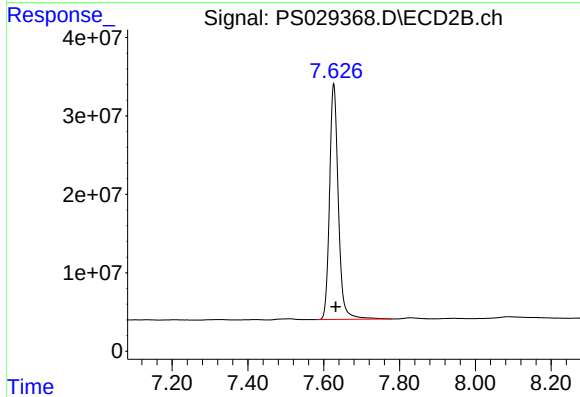


#4 2,4-DCAA

R.T.: 7.626 min
Delta R.T.: -0.005 min
Response: 482798861
Conc: 513.43 ng/ml

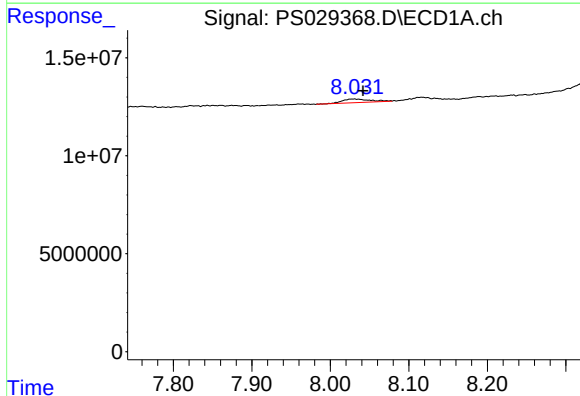


#8 DICHLORPROP

R.T.: 8.030 min
Delta R.T.: -0.012 min
Response: 4725096
Conc: 1.03 ng/ml

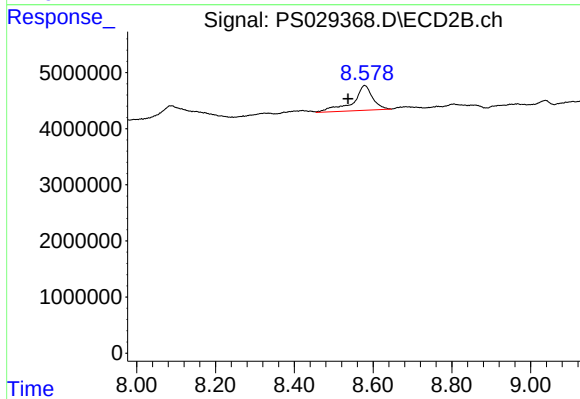

#8 DICHLORPROP


R.T.: 8.579 min
Delta R.T.: 0.042 min
Response: 15452119
Conc: 12.08 ng/ml

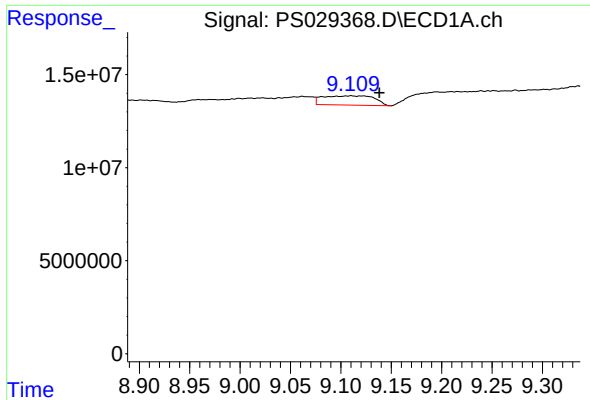

#11 2,4,5-TP (SILVEX)


R.T.: 9.110 min
Delta R.T.: -0.029 min
Response: 17622227
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

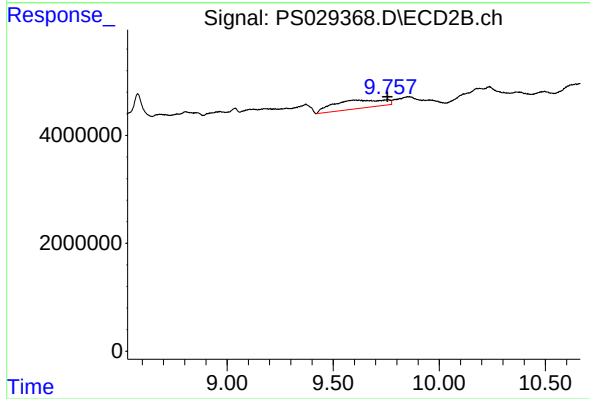


#11 2,4,5-TP (SILVEX)

R.T.: 9.756 min
Delta R.T.: 0.000 min
Response: 25738427
Conc: 2.85 ng/ml

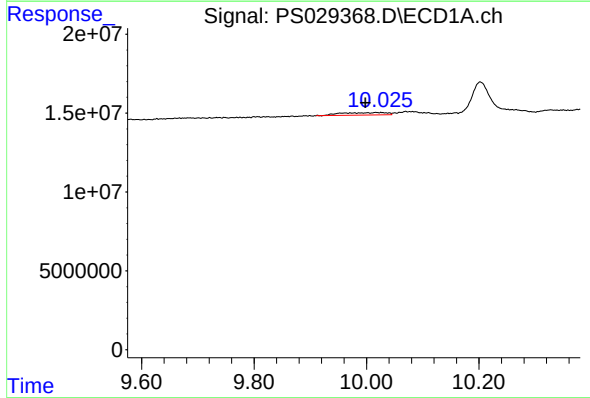

#13 2,4-DB

R.T.: 10.026 min
Delta R.T.: 0.028 min
Response: 8675362
Conc: 2.08 ng/ml

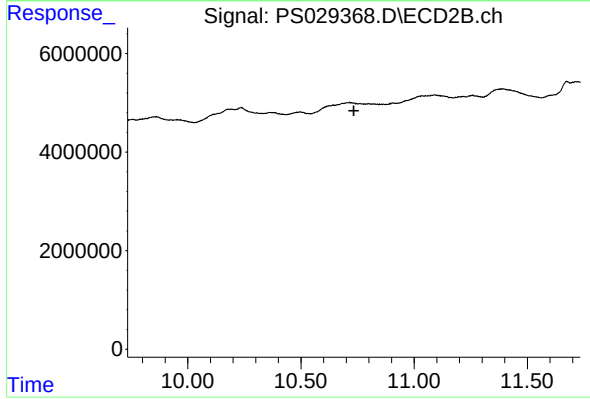

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 10.734 min
Response: 0
Conc: N.D.