

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030619\
 Data File : PS003429.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Mar 2019 12:51
 Operator : EI\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 02:26:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	10.799	0	1051666	N.D.	2.240 #
Target Compounds							
2) T	3,5-DICHL...	0.000	8.917	0	385896	N.D.	0.625 #
3) T	4-Nitroph...	0.000	9.961	0	131055	N.D.	0.583 #
5) T	DICAMBA	0.000	11.050	0	213778	N.D.	0.128 #
6) T	MCP	0.000	11.315	0	458763	N.D.	0.389 #
8) T	DICHLORPROP	0.000	12.160	0	246650	N.D.	0.597 #
9) T	2,4-D	0.000	12.712	0	139087	N.D.	0.265 #
10) T	Pentachlo...	0.000	13.184	0	176051	N.D.	0.027 #
11) T	2,4,5-TP ...	0.000	13.835	0	1483783	N.D.	0.583 #
12) T	2,4,5-T	0.000	14.364	0	486836	N.D.	0.241 #
13) T	2,4-DB	0.000	15.061	0	207488	N.D.	0.813 #
14) T	DINOSEB	0.000	15.491	0	129955	N.D.	0.073 #
15) T	Picloram	0.000	16.714	0	735354	N.D.	0.290 #
16) T	DCPA	0.000	16.630	0	359423	N.D.	0.116 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030619\
Data File : PS003429.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2019 12:51
Operator : EI\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 02:26:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

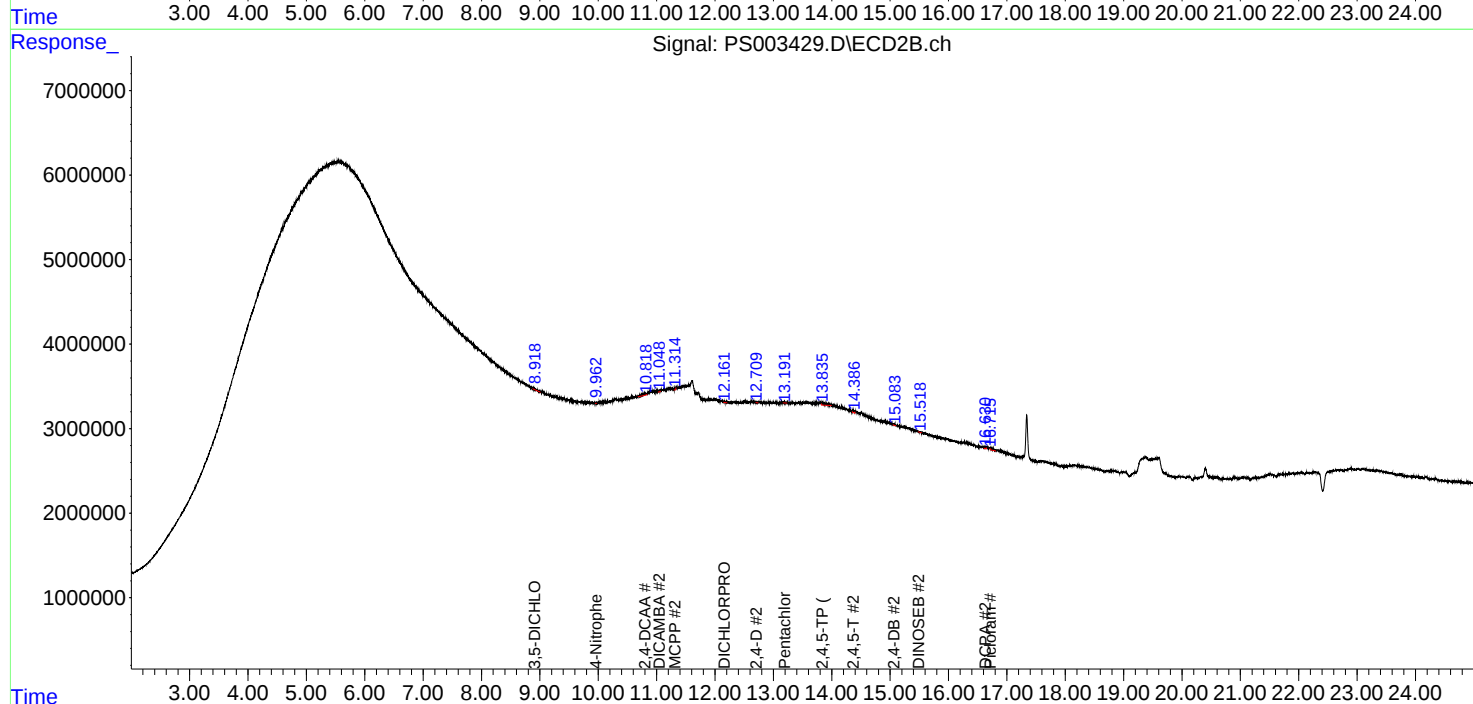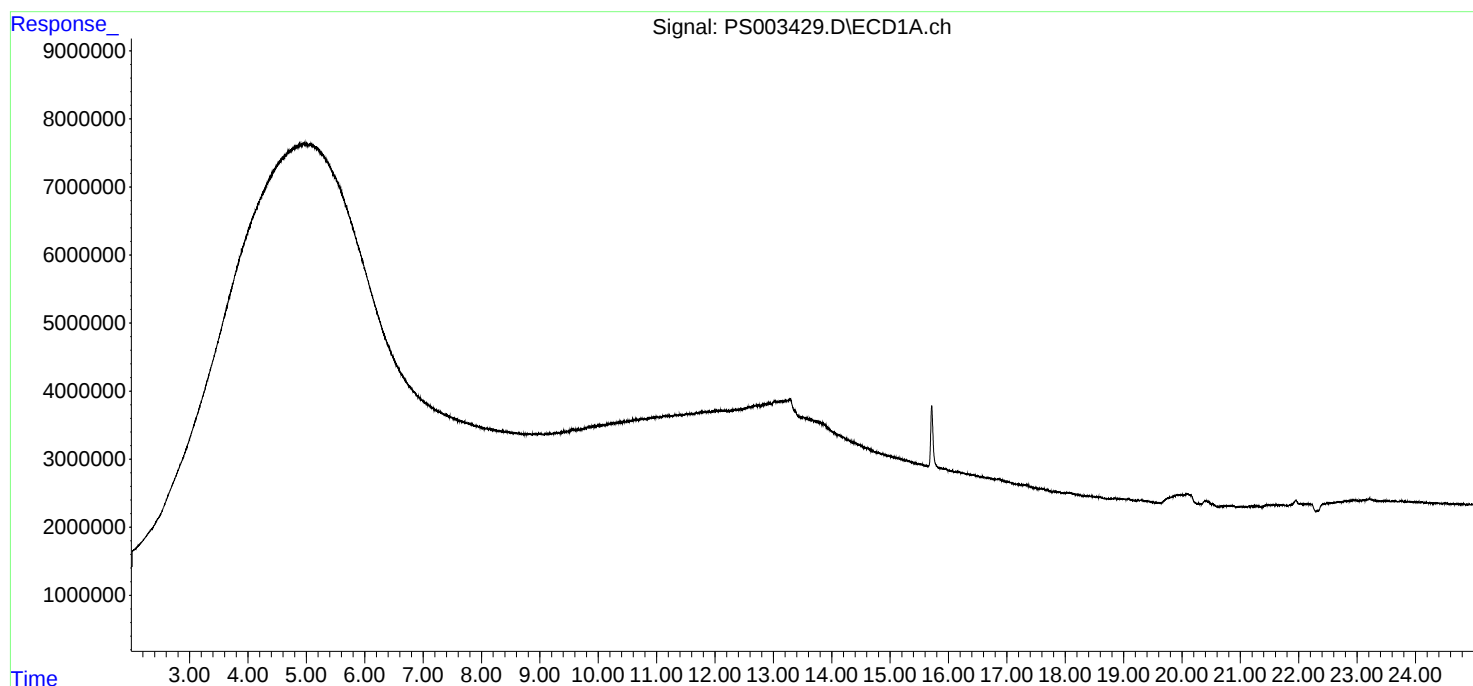


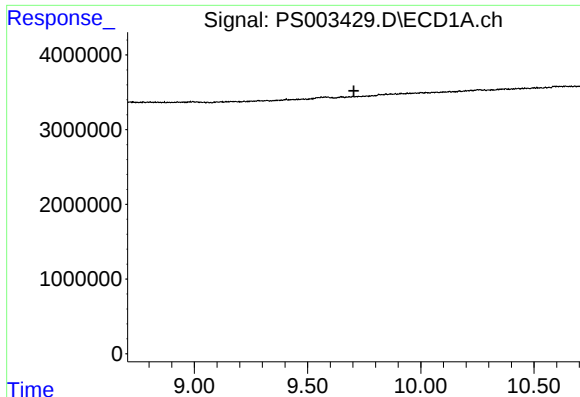

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.705 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

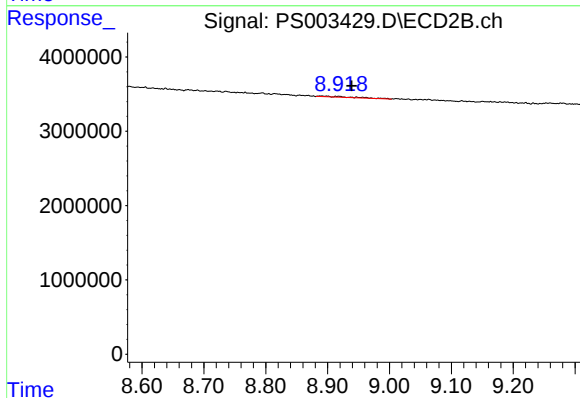


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 8.917 min
Delta R.T.: -0.022 min
Response: 385896
Conc: 0.62 ng/ml

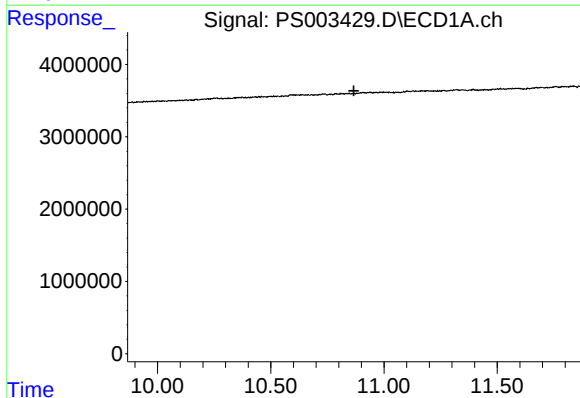


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

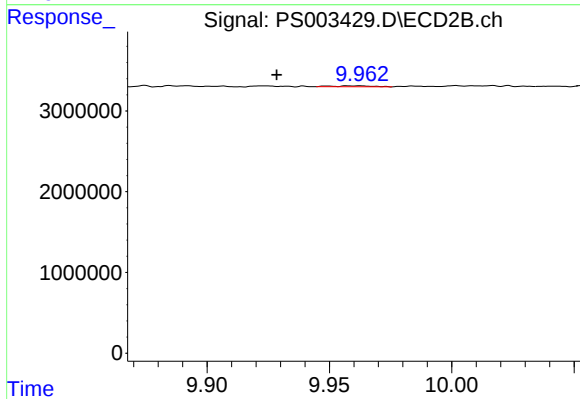

#3 4-Nitrophenol


R.T.: 9.961 min
Delta R.T.: 0.032 min
Response: 131055
Conc: 0.58 ng/ml

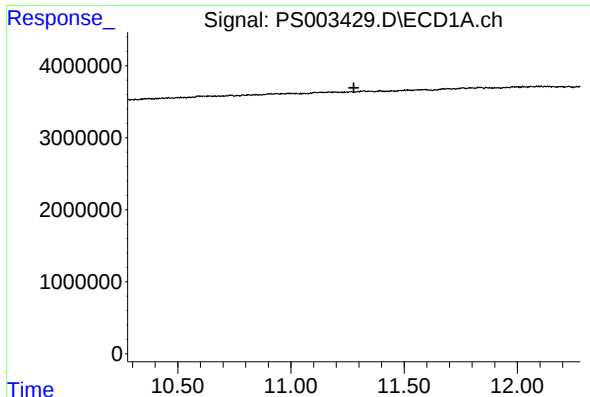

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 11.278 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

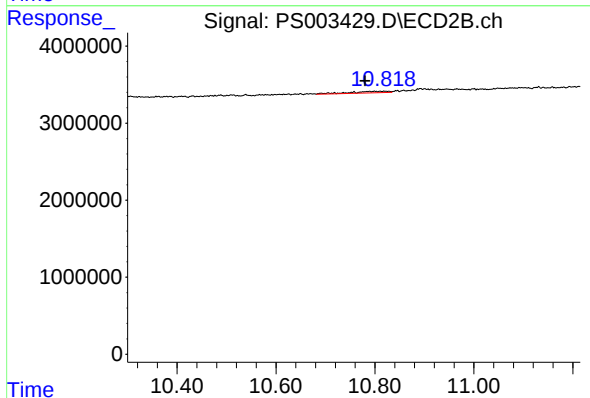


#4 2,4-DCAA

R.T.: 10.799 min
Delta R.T.: 0.020 min
Response: 1051666
Conc: 2.24 ng/ml

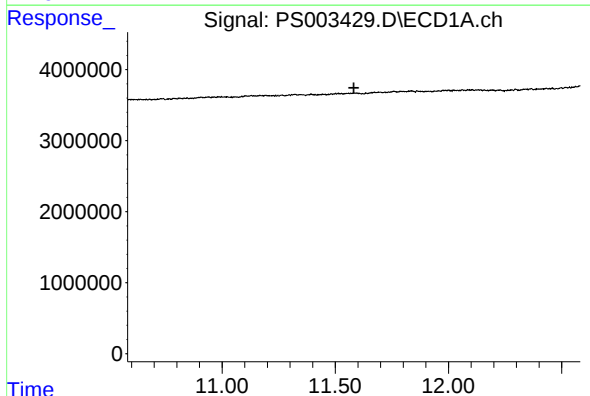


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 11.582 min
Response: 0
Conc: N.D.

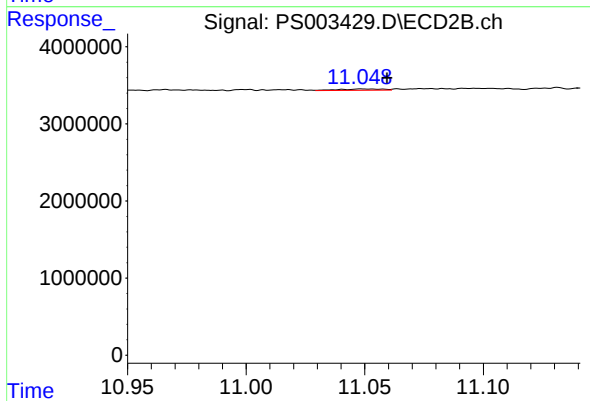

#5 DICAMBA


R.T.: 11.050 min
Delta R.T.: -0.009 min
Response: 213778
Conc: 0.13 ng/ml

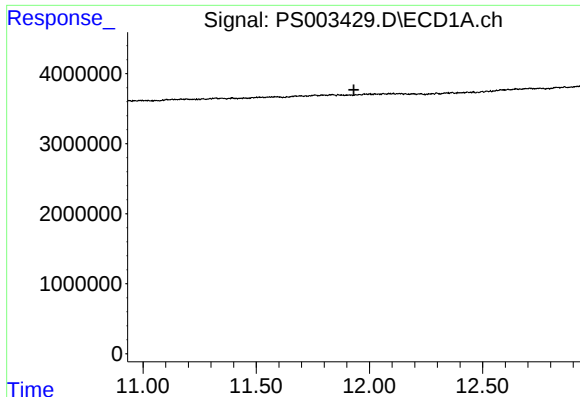

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.931 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

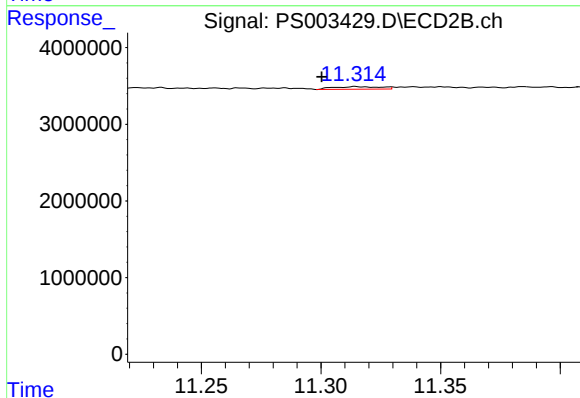


#6 MCP

R.T.: 11.315 min
Delta R.T.: 0.015 min
Response: 458763
Conc: 0.39 ug/ml

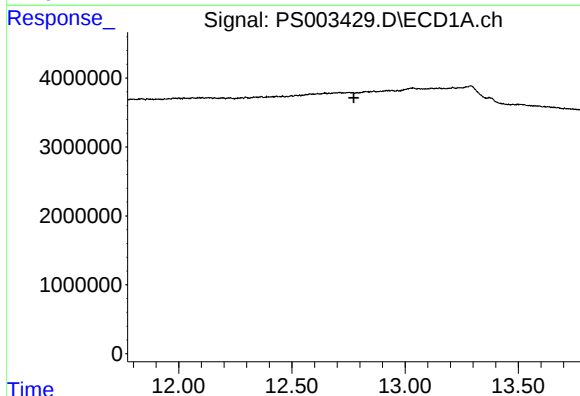


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 12.773 min
Response: 0
Conc: N.D.

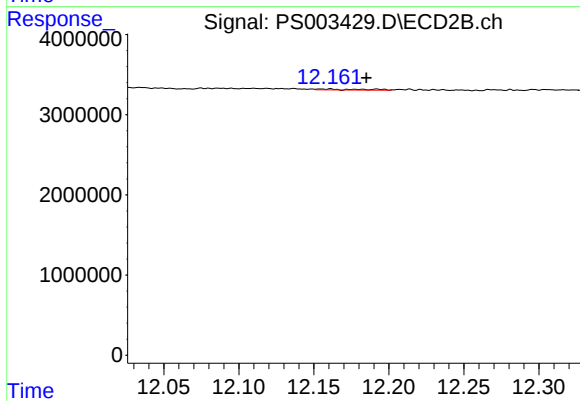

#8 DICHLORPROP


R.T.: 12.160 min
Delta R.T.: -0.025 min
Response: 246650
Conc: 0.60 ng/ml

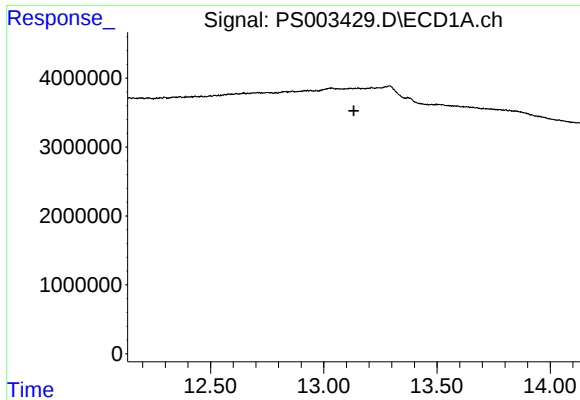

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.133 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

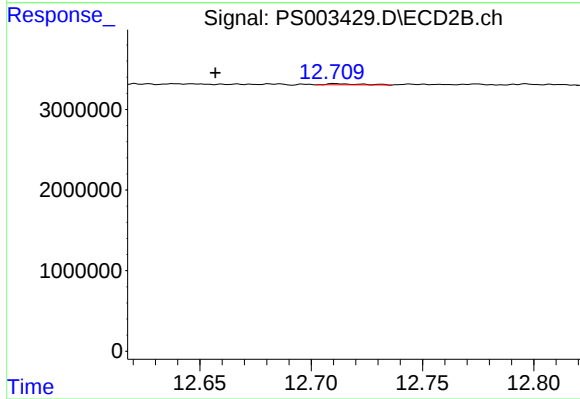


#9 2,4-D

R.T.: 12.712 min
Delta R.T.: 0.055 min
Response: 139087
Conc: 0.26 ng/ml

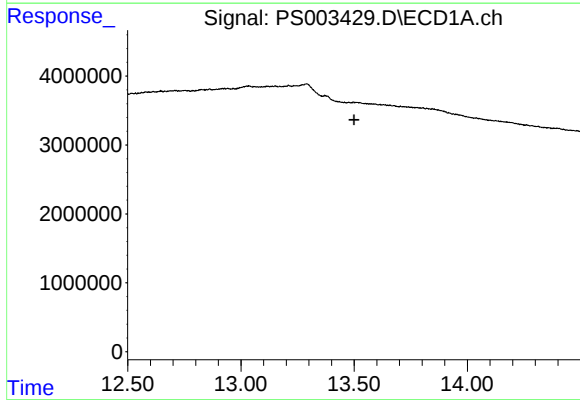


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 13.499 min
Response: 0
Conc: N.D.

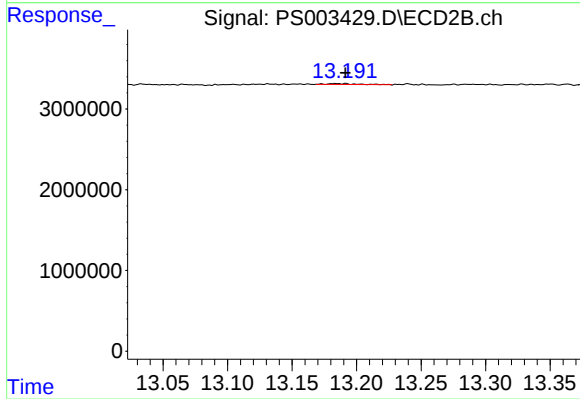

#10 Pentachlorophenol


R.T.: 13.184 min
Delta R.T.: -0.007 min
Response: 176051
Conc: 0.03 ng/ml

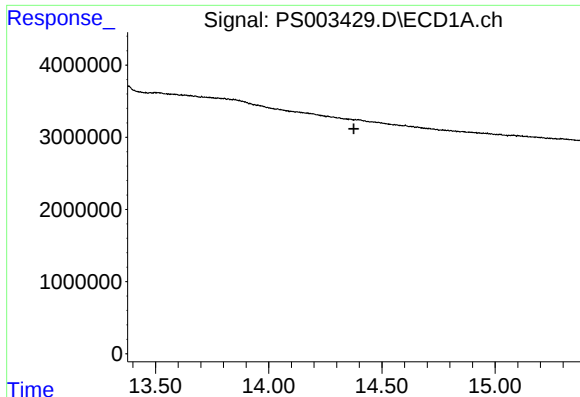

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

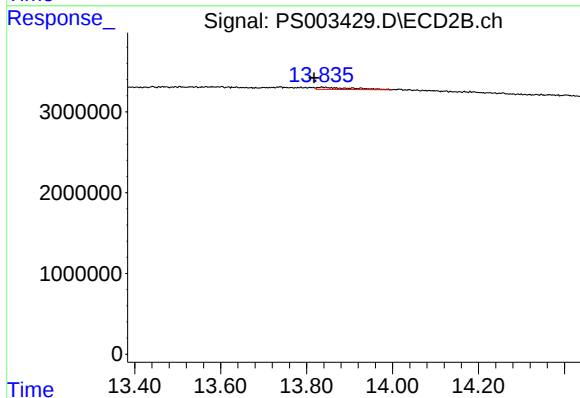


#11 2,4,5-TP (SILVEX)

R.T.: 13.835 min
Delta R.T.: 0.018 min
Response: 1483783
Conc: 0.58 ng/ml

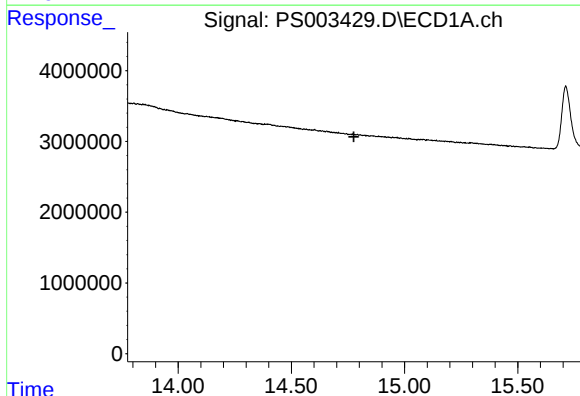


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

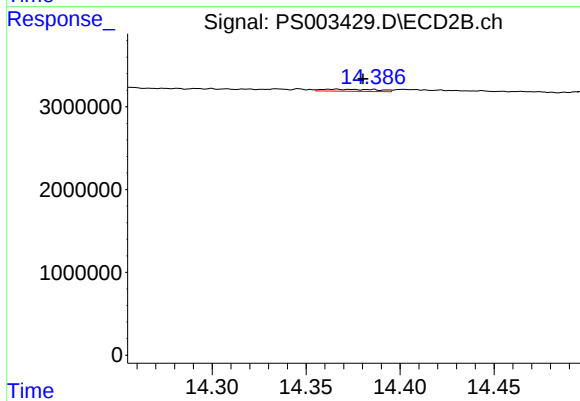

#12 2,4,5-T


R.T.: 14.364 min
Delta R.T.: -0.016 min
Response: 486836
Conc: 0.24 ng/ml

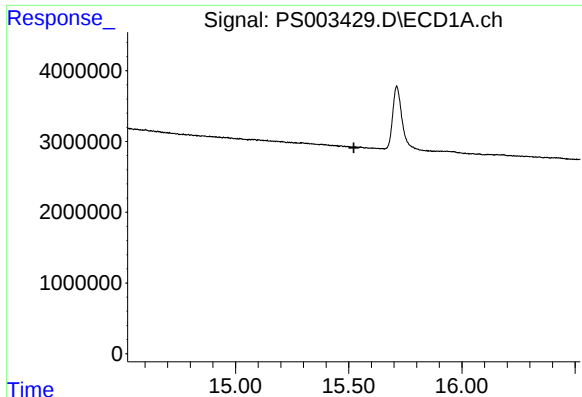

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.523 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

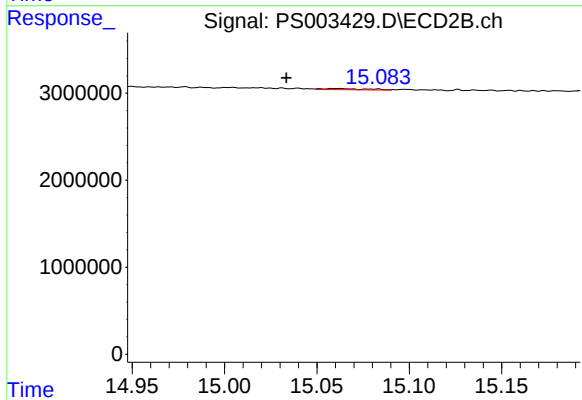


#13 2,4-DB

R.T.: 15.061 min
Delta R.T.: 0.027 min
Response: 207488
Conc: 0.81 ng/ml

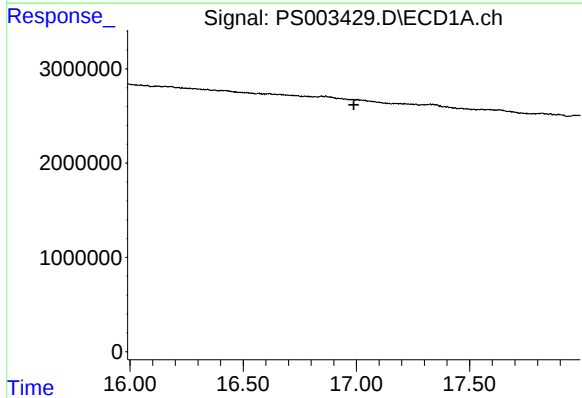


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

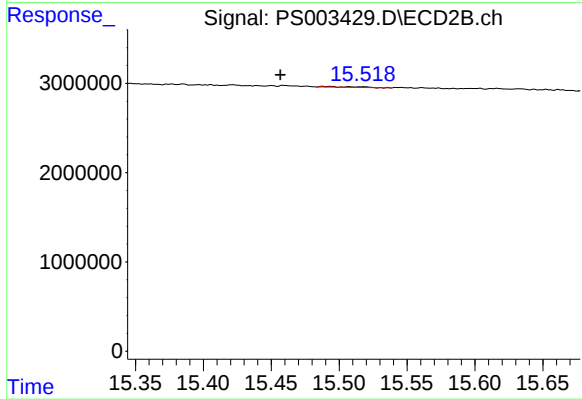

#14 DINOSEB


R.T.: 15.491 min
Delta R.T.: 0.034 min
Response: 129955
Conc: 0.07 ng/ml

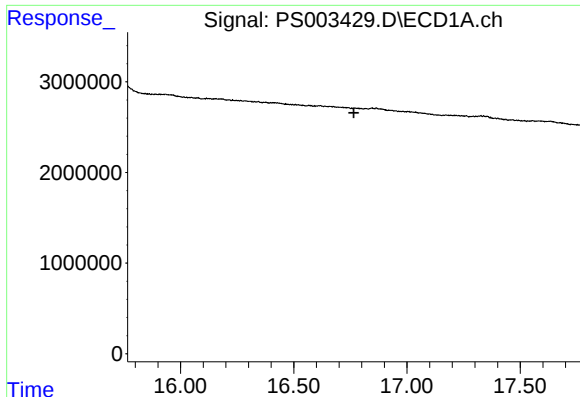

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.765 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

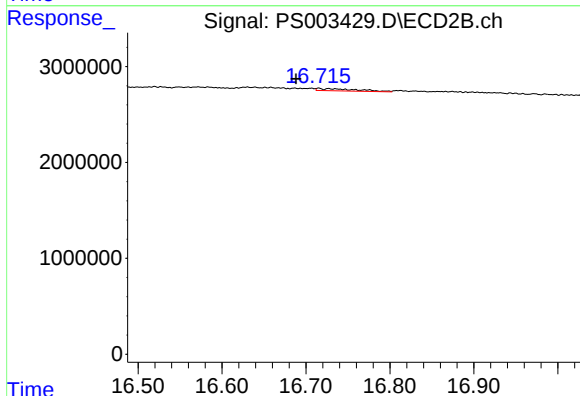


#15 Picloram

R.T.: 16.714 min
Delta R.T.: 0.026 min
Response: 735354
Conc: 0.29 ng/ml

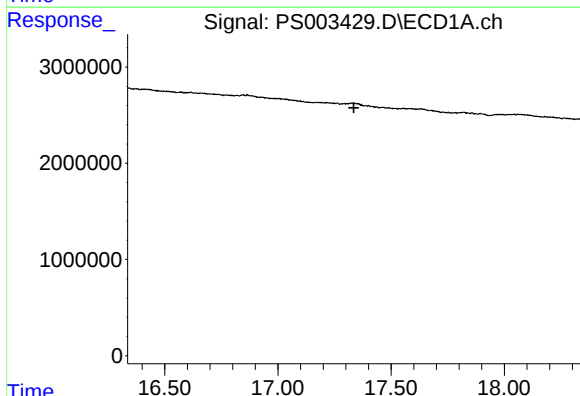

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.335 min
Response: 0
Conc: N.D.

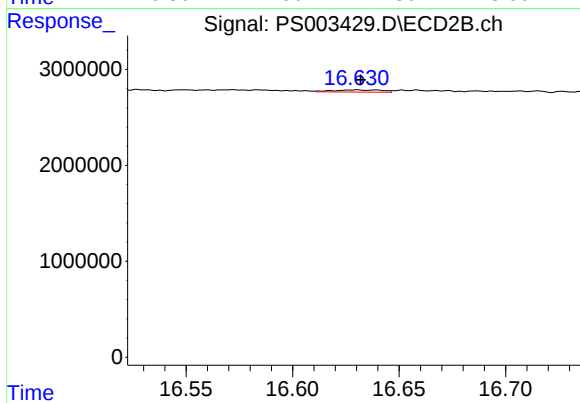

#16 DCPA

R.T.: 16.630 min
Delta R.T.: -0.002 min
Response: 359423
Conc: 0.12 ng/ml