

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030619\
 Data File : PS003430.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Mar 2019 13:22
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 02:26:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.286	10.781	215.3E6	208.2E6	490.381	443.291
Target Compounds							
2) T	3,5-DICHL...	0.000	8.995	0	130172	N.D.	0.211 #
3) T	4-Nitroph...	0.000	9.957	0	183644	N.D.	0.817 #
7) T	MCPA	0.000	11.666	0	531053	N.D.	0.308 #
8) T	DICHLORPROP	0.000	12.201	0	78031	N.D.	0.189 #
9) T	2,4-D	0.000	12.704	0	78420	N.D.	0.149 #
10) T	Pentachlo...	0.000	13.202	0	826086	N.D.	0.125 #
11) T	2,4,5-TP ...	0.000	13.843	0	442083	N.D.	0.174 #
13) T	2,4-DB	0.000	15.097	0	3016378	N.D.	11.812 #
14) T	DINOSEB	0.000	15.455	0	316756	N.D.	0.177 #
15) T	Picloram	0.000	16.640	0	1611796	N.D.	0.635 #
16) T	DCPA	0.000	16.640	0	1611796	N.D.	0.518 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030619\
Data File : PS003430.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2019 13:22
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 02:26:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

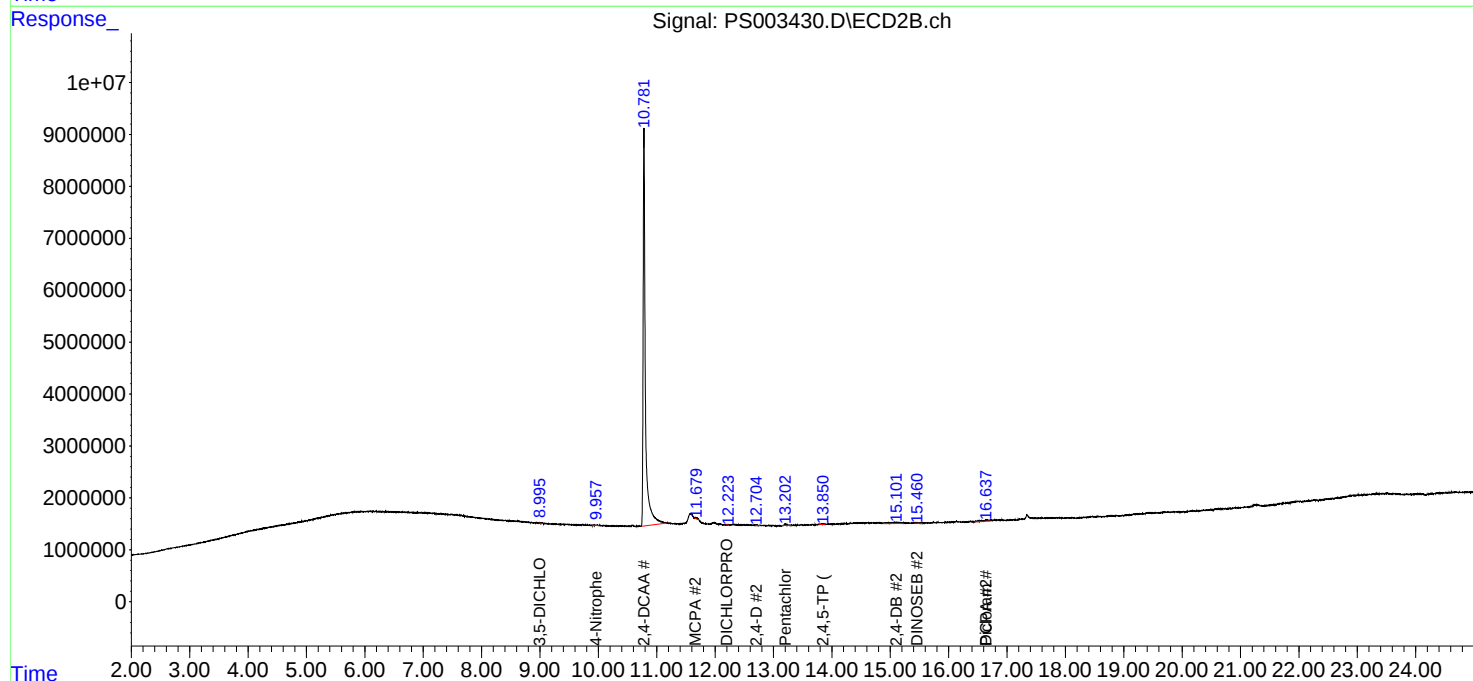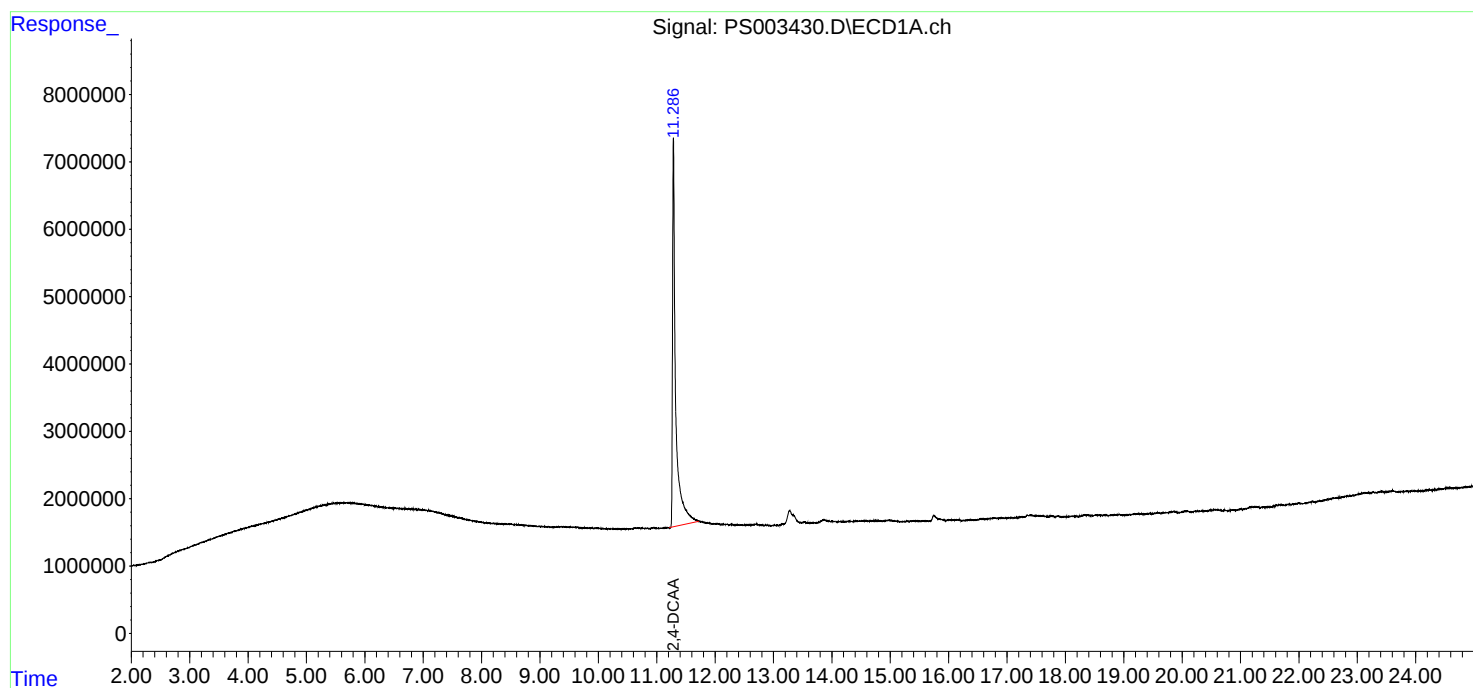


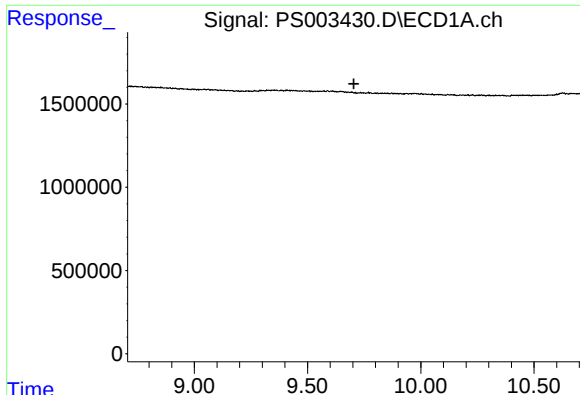

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.705 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

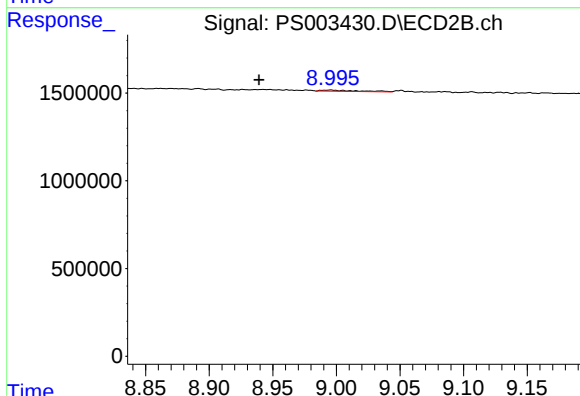


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 8.995 min
Delta R.T.: 0.056 min
Response: 130172
Conc: 0.21 ng/ml

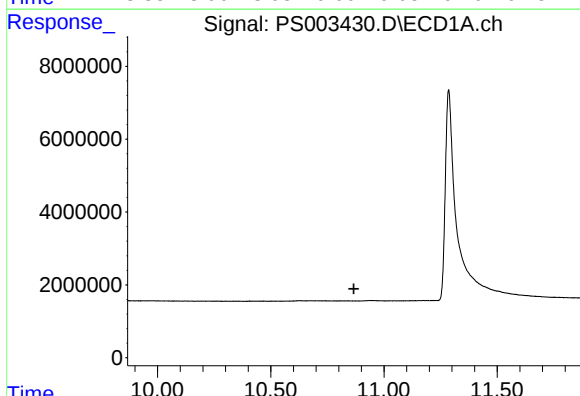


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

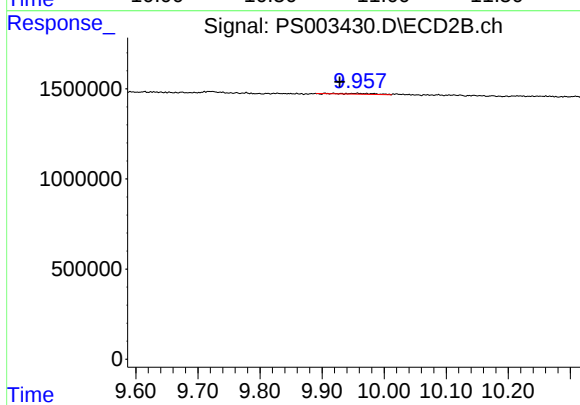

#3 4-Nitrophenol


R.T.: 9.957 min
Delta R.T.: 0.028 min
Response: 183644
Conc: 0.82 ng/ml

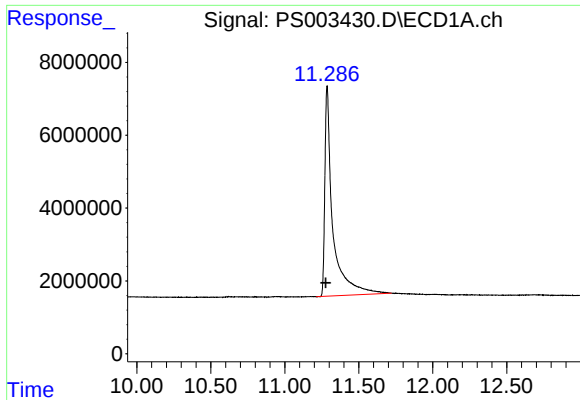

#4 2,4-DCAA


R.T.: 11.286 min
Delta R.T.: 0.008 min
Response: 215289123
Conc: 490.38 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

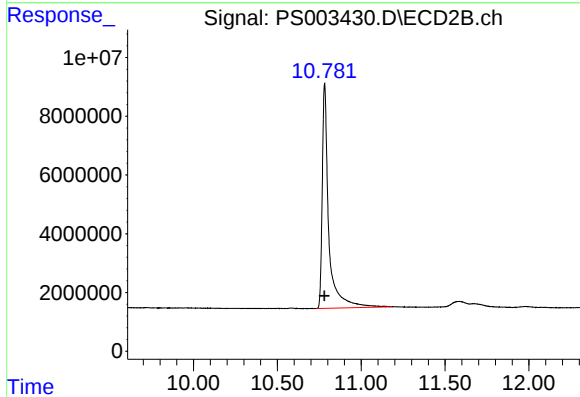


#4 2,4-DCAA

R.T.: 10.781 min
Delta R.T.: 0.002 min
Response: 208155786
Conc: 443.29 ng/ml

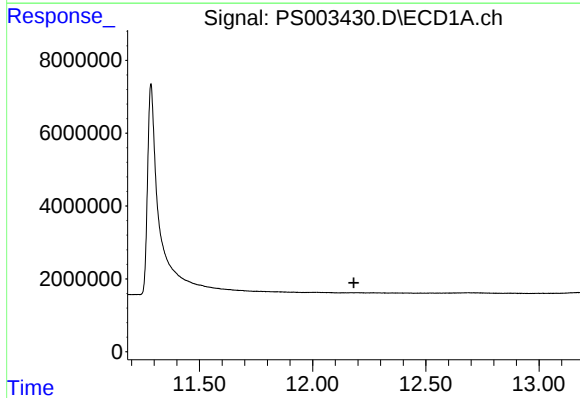


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.182 min
Response: 0
Conc: N.D.

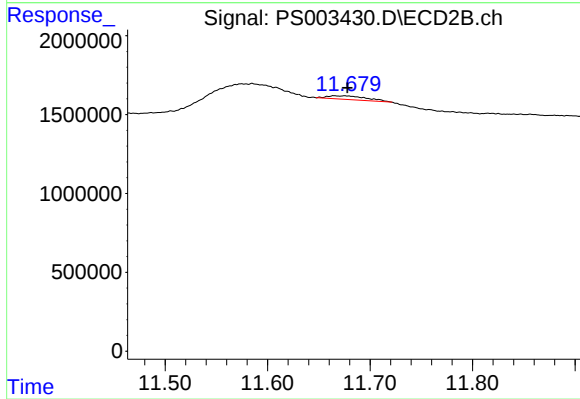

#7 MCPA


R.T.: 11.666 min
Delta R.T.: -0.012 min
Response: 531053
Conc: 0.31 ug/ml

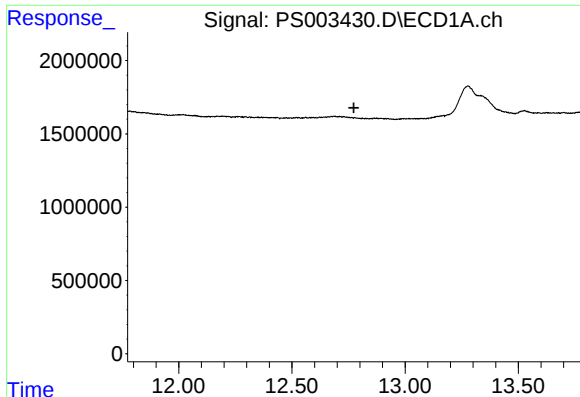

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.773 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

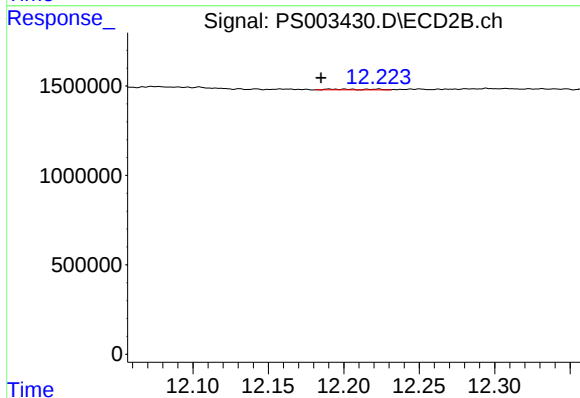


#8 DICHLORPROP

R.T.: 12.201 min
Delta R.T.: 0.016 min
Response: 78031
Conc: 0.19 ng/ml

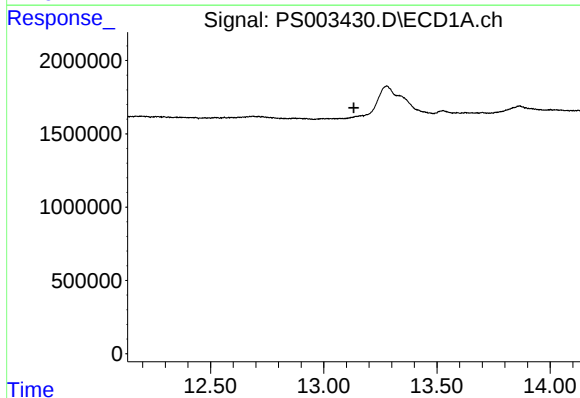


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 13.133 min
Response: 0
Conc: N.D.

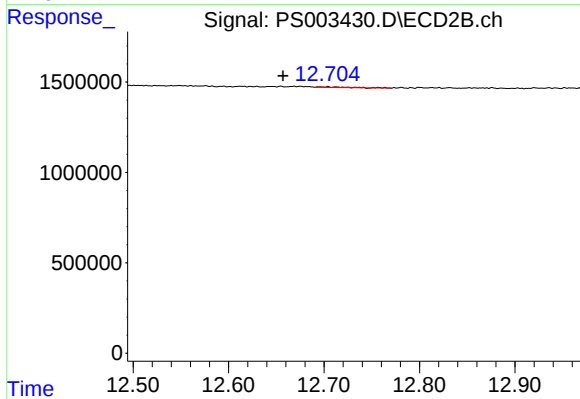

#9 2,4-D


R.T.: 12.704 min
Delta R.T.: 0.047 min
Response: 78420
Conc: 0.15 ng/ml

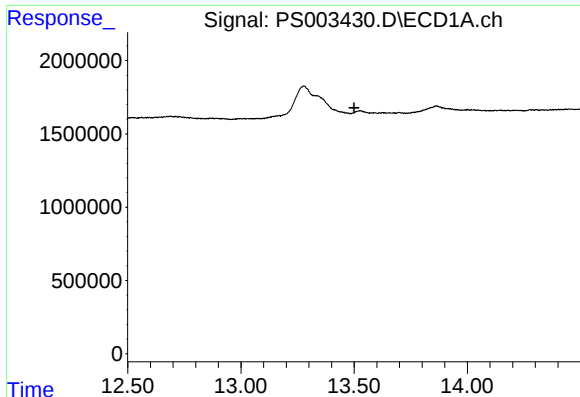

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.499 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

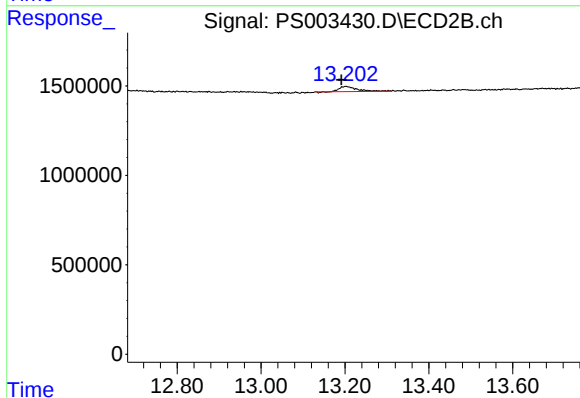


#10 Pentachlorophenol

R.T.: 13.202 min
Delta R.T.: 0.010 min
Response: 826086
Conc: 0.13 ng/ml

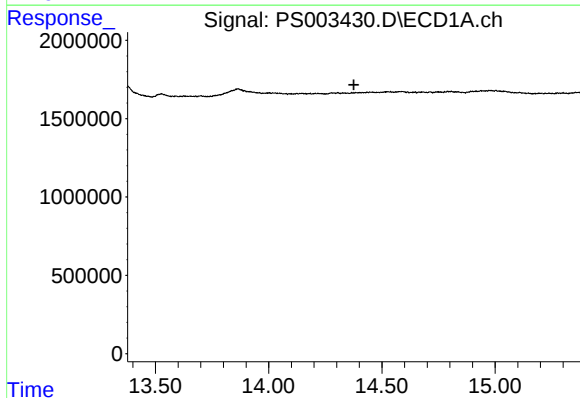


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

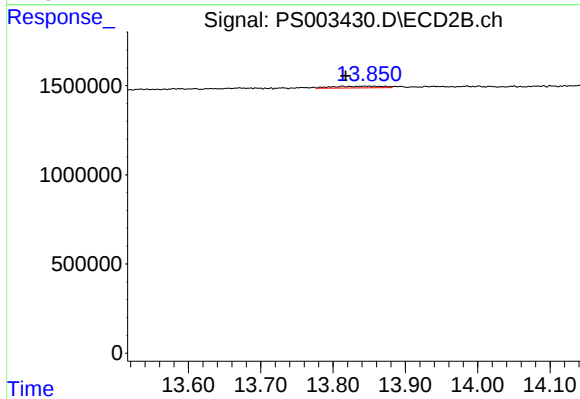

#11 2,4,5-TP (SILVEX)


R.T.: 13.843 min
Delta R.T.: 0.026 min
Response: 442083
Conc: 0.17 ng/ml

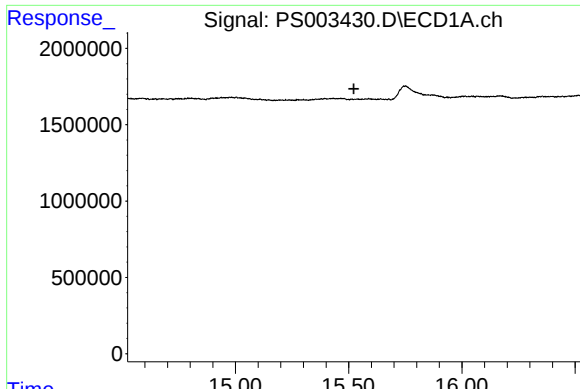

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.523 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

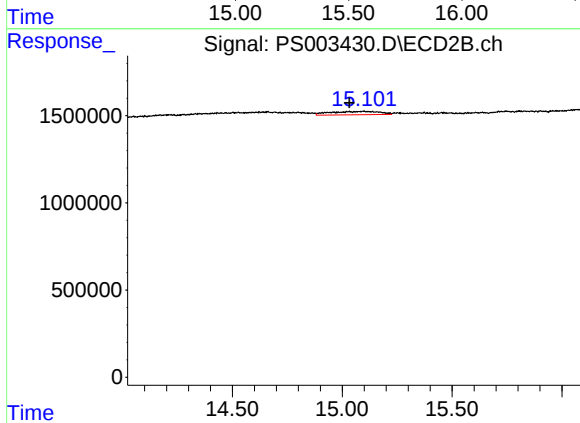


#13 2,4-DB

R.T.: 15.097 min
Delta R.T.: 0.064 min
Response: 3016378
Conc: 11.81 ng/ml

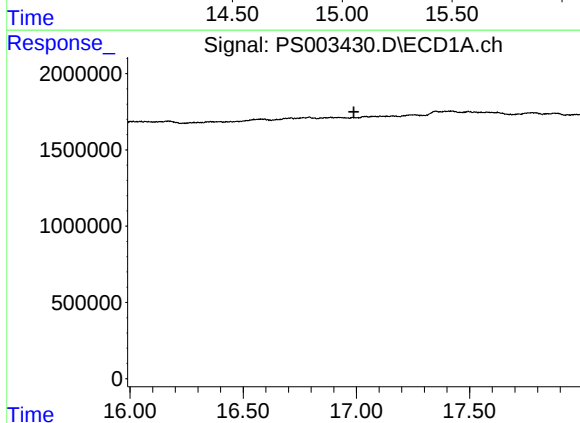


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

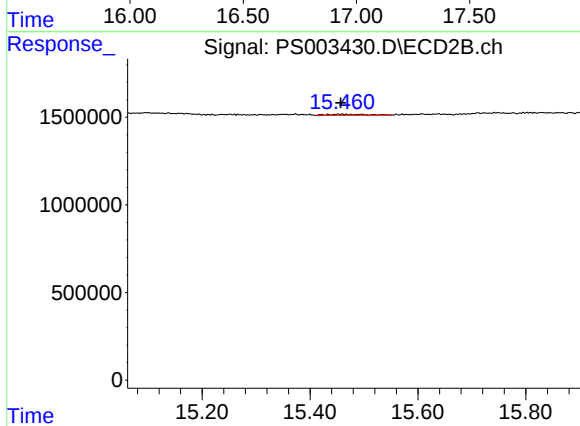

#14 DINOSEB


R.T.: 15.455 min
Delta R.T.: -0.002 min
Response: 316756
Conc: 0.18 ng/ml

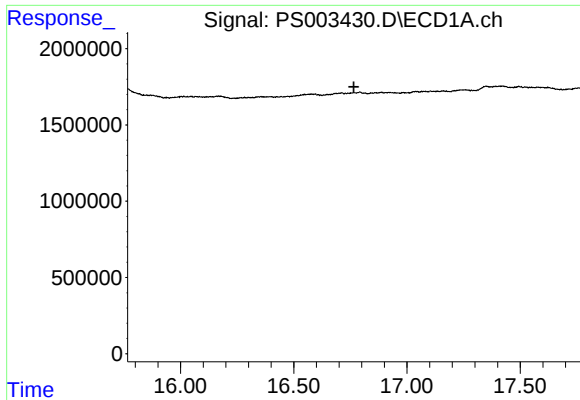

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.765 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

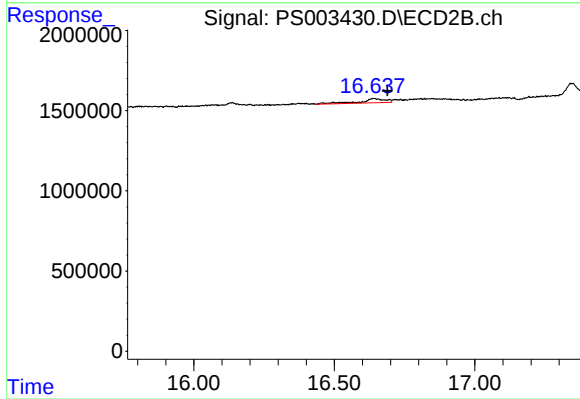


#15 Picloram

R.T.: 16.640 min
Delta R.T.: -0.049 min
Response: 1611796
Conc: 0.64 ng/ml

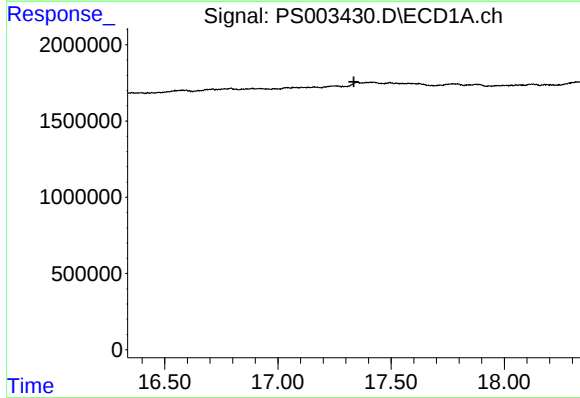

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.335 min
Response: 0
Conc: N.D.

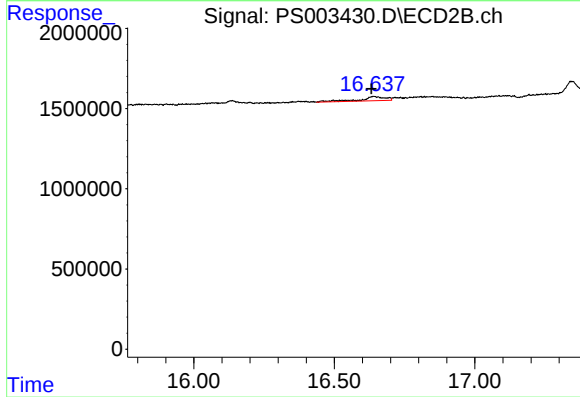

#16 DCPA

R.T.: 16.640 min
Delta R.T.: 0.008 min
Response: 1611796
Conc: 0.52 ng/ml