

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030619\
 Data File : PS003447.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Mar 2019 23:28
 Operator : EI\SJ
 Sample : K1707-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 S11

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 02:31:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.269	10.773	240.5E6	250.9E6	547.730	534.382
Target Compounds							
1) T	Dalapon	2.792	2.281	47427343	71376718	72.972	112.727 #
2) T	3,5-DICHL...	0.000	8.939	0	9411549	N.D.	15.242 #
3) T	4-Nitroph...	0.000	9.962	0	3712894	N.D.	16.514 #
5) T	DICAMBA	0.000	11.012	0	6907101	N.D.	4.134 #
6) T	MCPD	11.953	11.307	3553907	300863	2.707	0.255 #
9) T	2,4-D	0.000	12.635	0	1347308	N.D.	2.567 #
11) T	2,4,5-TP ...	0.000	13.832	0	613205	N.D.	0.241 #
12) T	2,4,5-T	0.000	14.374	0	14361861	N.D.	7.121 #
13) T	2,4-DB	15.467	0.000	15291449	0	64.577	N.D. #
14) T	DINOSEB	0.000	15.493	0	12591774	N.D.	7.055 #
15) T	Picloram	16.749	16.710	5123123	27734071	2.082	10.927 #
16) T	DCPA	17.293	0.000	34983590	0	10.616	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030619\
Data File : PS003447.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2019 23:28
Operator : EI\SJ
Sample : K1707-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
S11

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 02:31:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

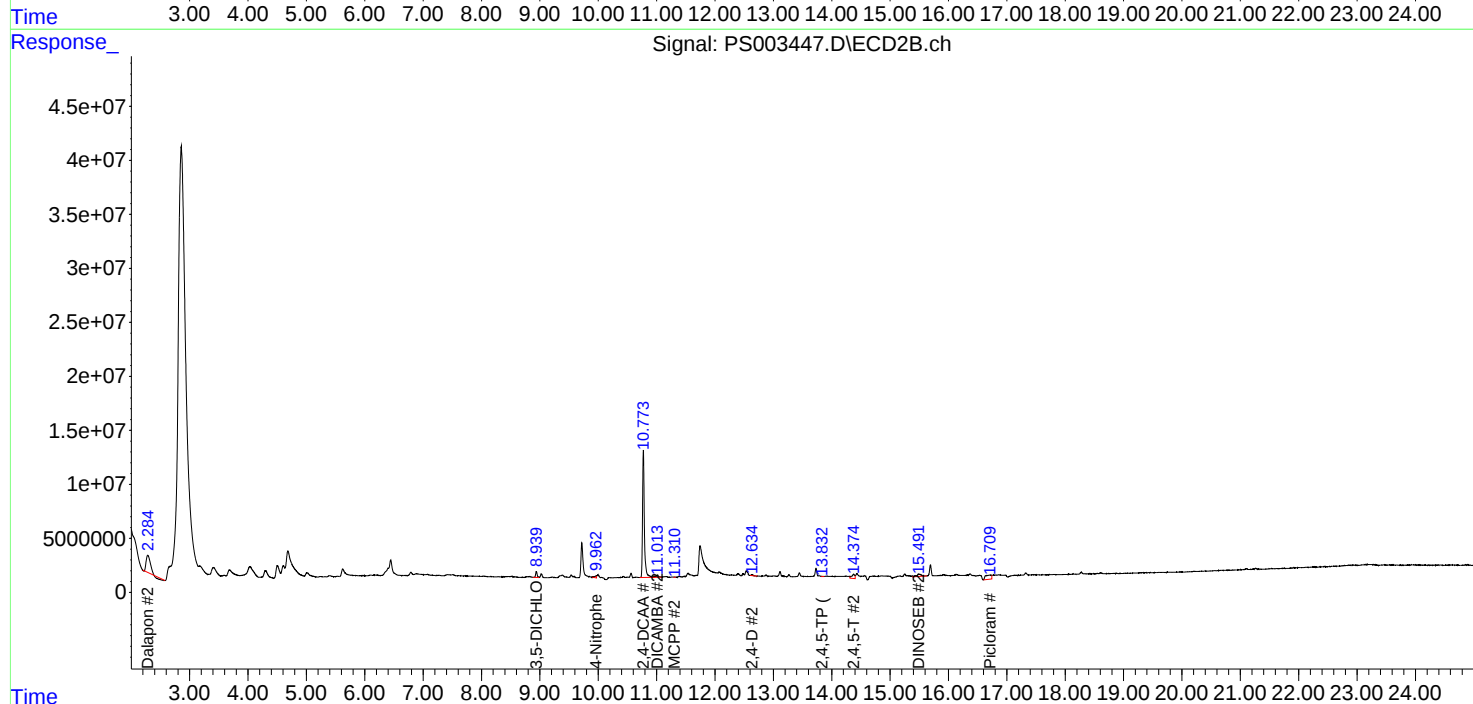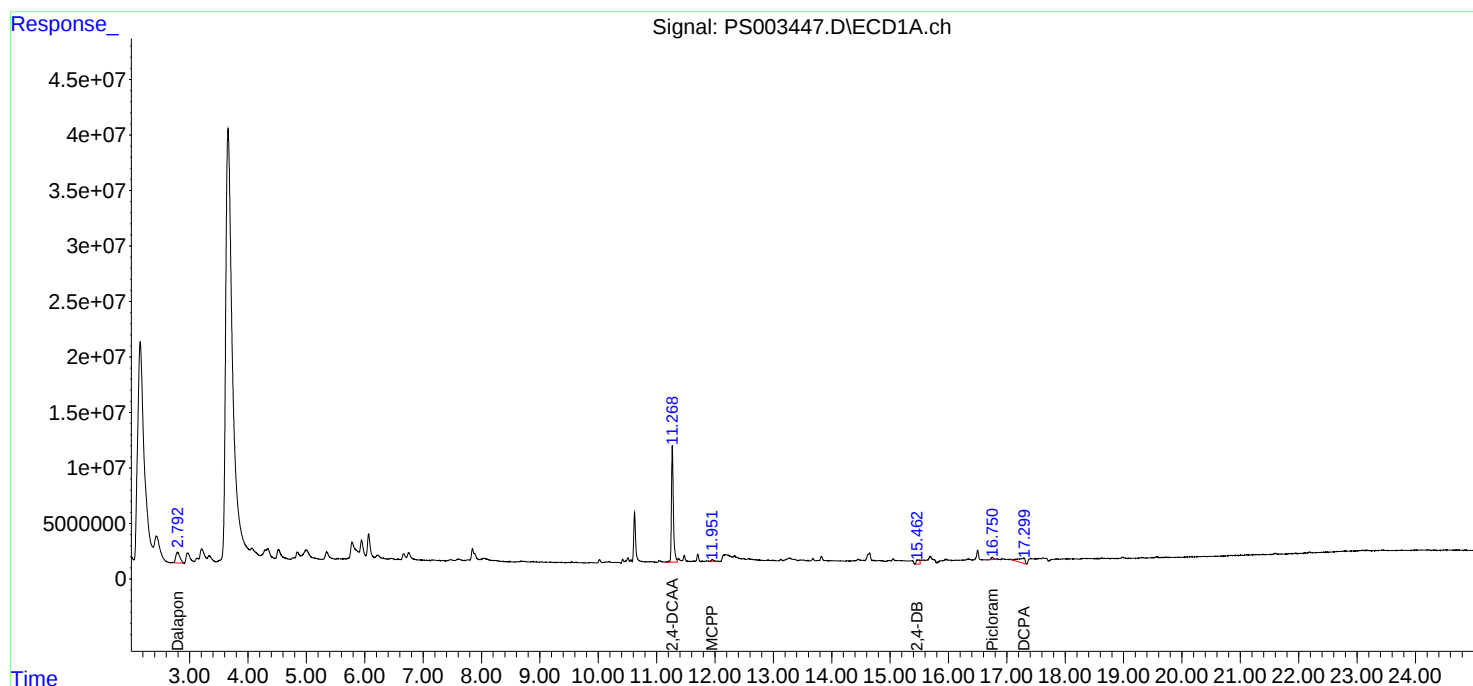


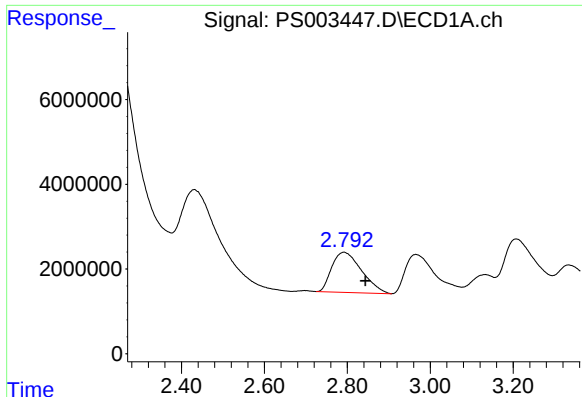

#1 Dalapon


R.T.: 2.792 min
Delta R.T.: -0.052 min
Response: 47427343
Conc: 72.97 ng/ml

Instrument :
ECD_S
ClientSampleId :
S11

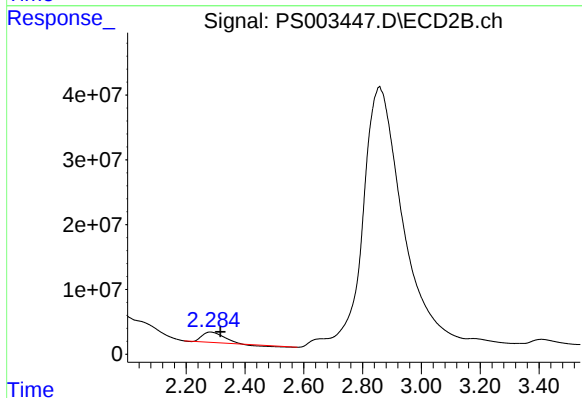


#1 Dalapon

R.T.: 2.281 min
Delta R.T.: -0.035 min
Response: 71376718
Conc: 112.73 ng/ml

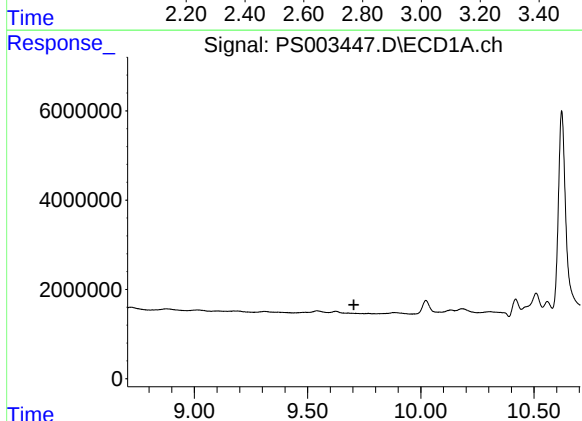


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.705 min
Response: 0
Conc: N.D.

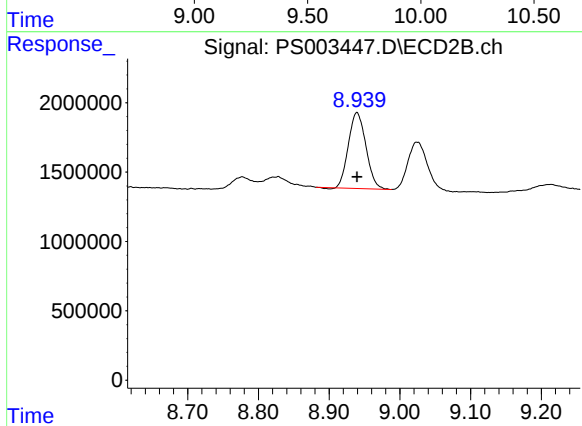

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.939 min
Delta R.T.: 0.000 min
Response: 9411549
Conc: 15.24 ng/ml

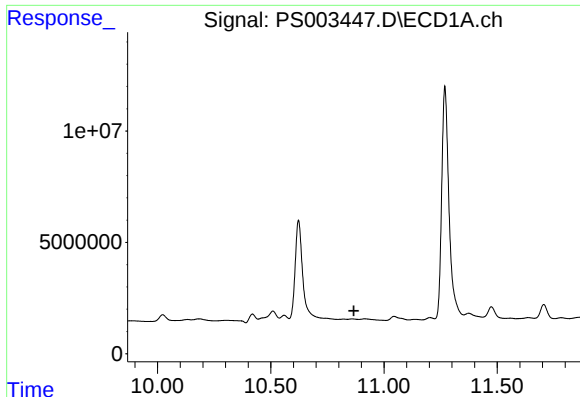

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
S11

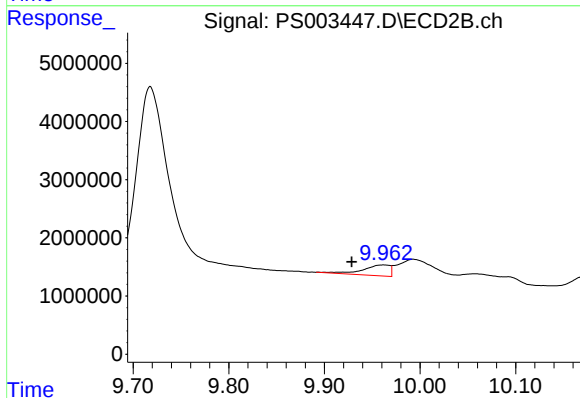


#3 4-Nitrophenol

R.T.: 9.962 min
Delta R.T.: 0.033 min
Response: 3712894
Conc: 16.51 ng/ml

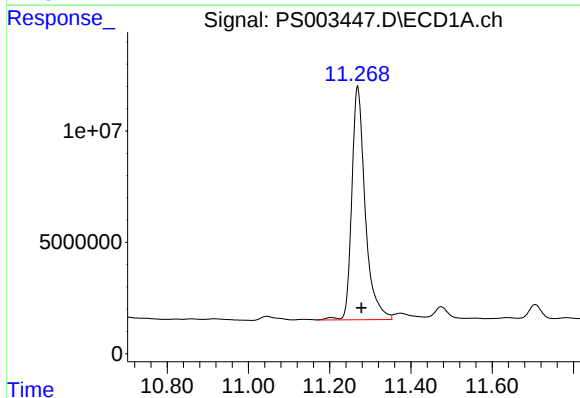


#4 2,4-DCAA

R.T.: 11.269 min
Delta R.T.: -0.008 min
Response: 240466868
Conc: 547.73 ng/ml

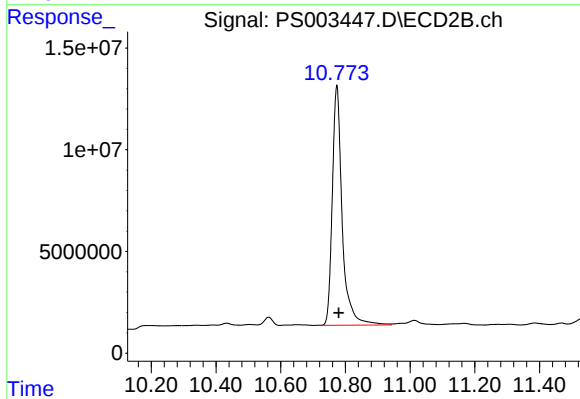

#4 2,4-DCAA


R.T.: 10.773 min
Delta R.T.: -0.006 min
Response: 250929409
Conc: 534.38 ng/ml

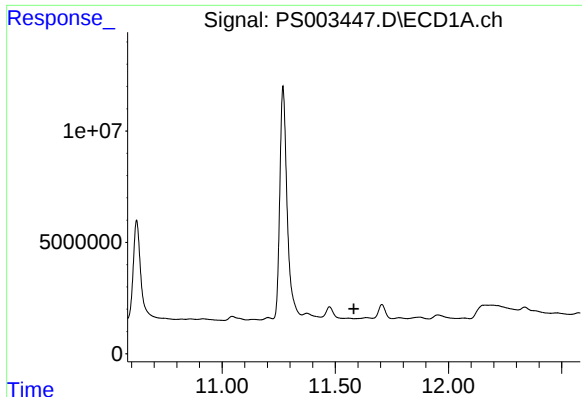

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.582 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
S11

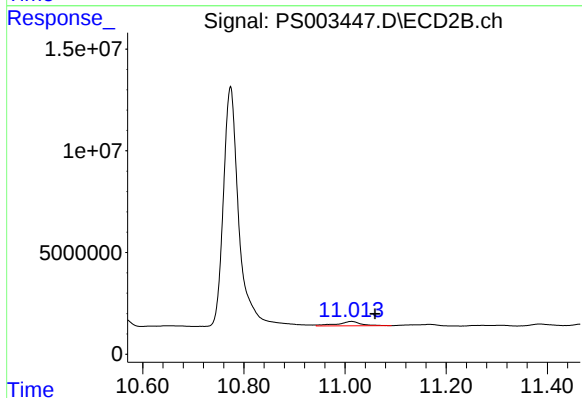


#5 DICAMBA

R.T.: 11.012 min
Delta R.T.: -0.047 min
Response: 6907101
Conc: 4.13 ng/ml

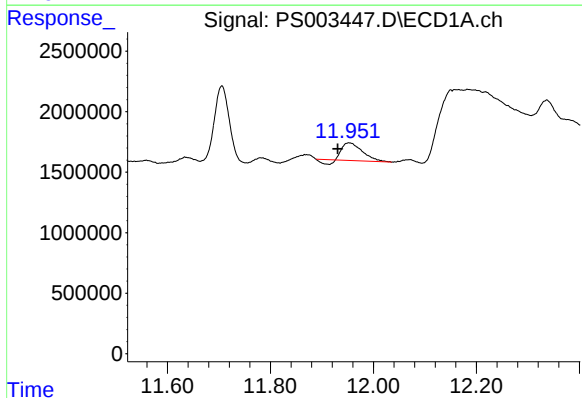


#6 MCP

R.T.: 11.953 min
Delta R.T.: 0.022 min
Response: 3553907
Conc: 2.71 ug/ml

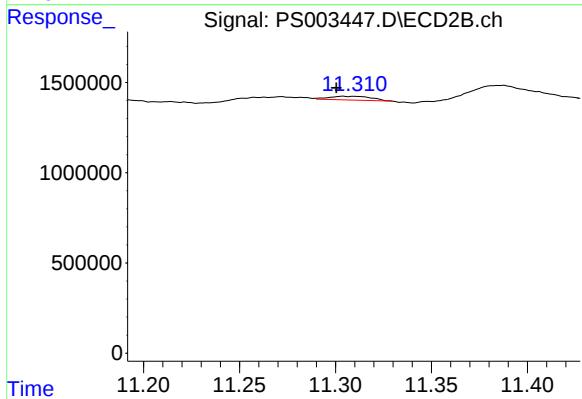

#6 MCP


R.T.: 11.307 min
Delta R.T.: 0.007 min
Response: 300863
Conc: 0.25 ug/ml

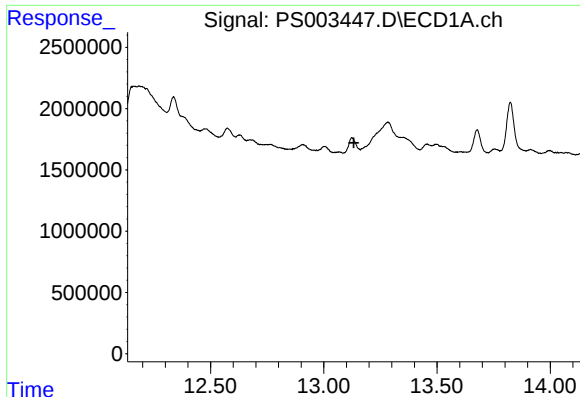

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.133 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
S11

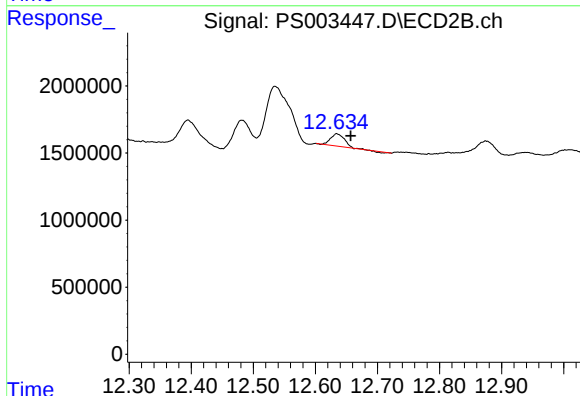


#9 2,4-D

R.T.: 12.635 min
Delta R.T.: -0.022 min
Response: 1347308
Conc: 2.57 ng/ml

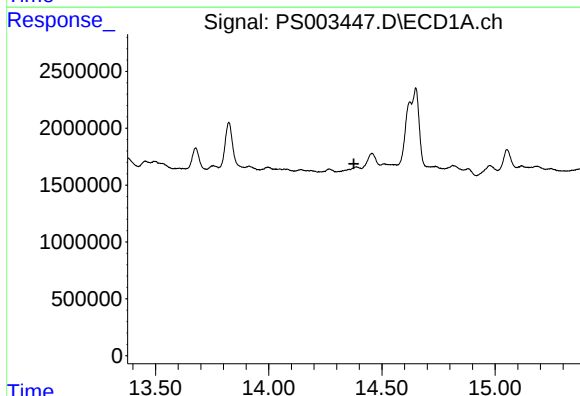


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

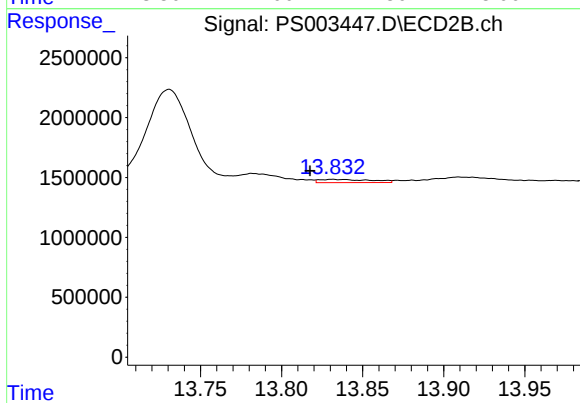

#11 2,4,5-TP (SILVEX)


R.T.: 13.832 min
Delta R.T.: 0.014 min
Response: 613205
Conc: 0.24 ng/ml

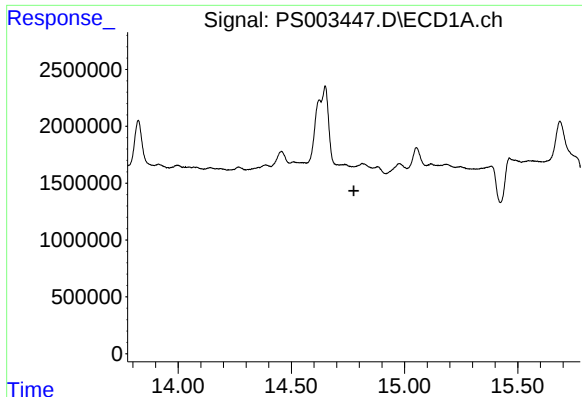

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
S11

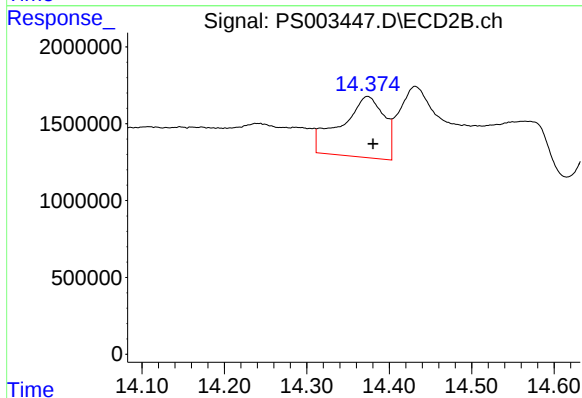


#12 2,4,5-T

R.T.: 14.374 min
Delta R.T.: -0.007 min
Response: 14361861
Conc: 7.12 ng/ml

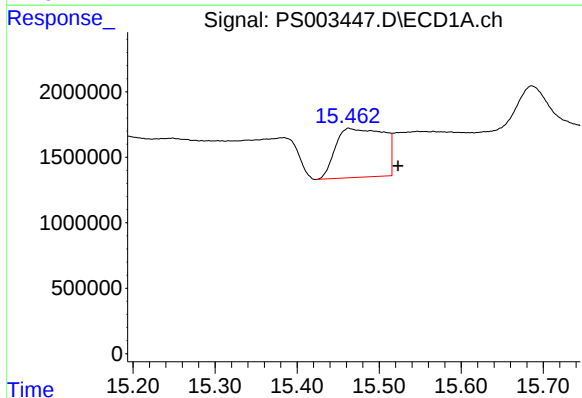


#13 2,4-DB

R.T.: 15.467 min
Delta R.T.: -0.057 min
Response: 15291449
Conc: 64.58 ng/ml

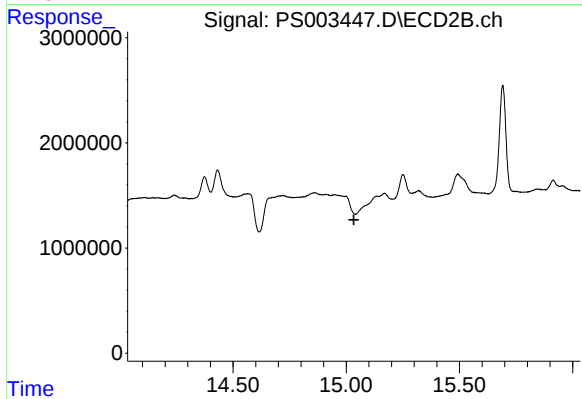

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.033 min
Response: 0
Conc: N.D.

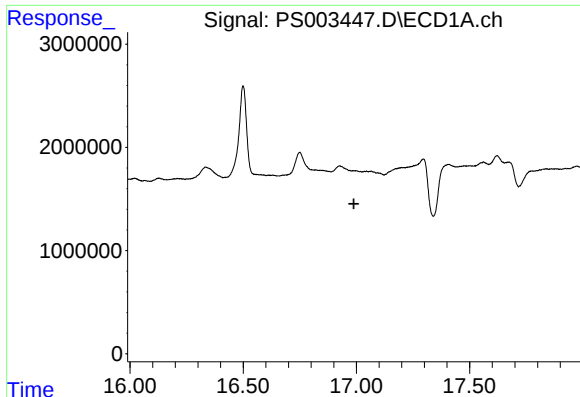

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
S11

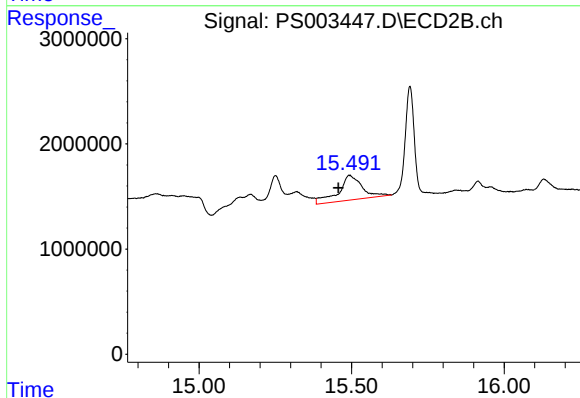


#14 DINOSEB

R.T.: 15.493 min
Delta R.T.: 0.036 min
Response: 12591774
Conc: 7.05 ng/ml

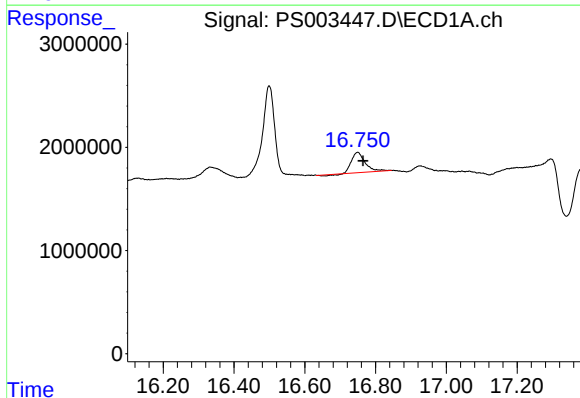


#15 Picloram

R.T.: 16.749 min
Delta R.T.: -0.016 min
Response: 5123123
Conc: 2.08 ng/ml

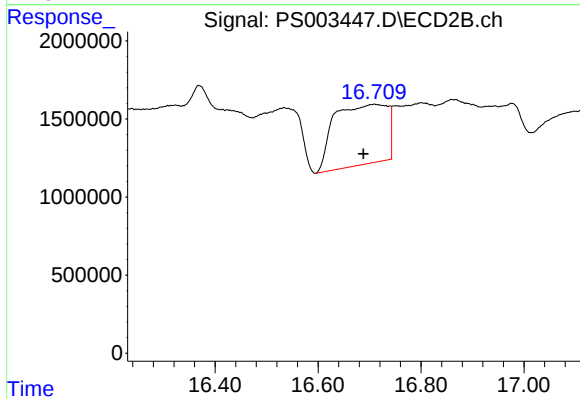

#15 Picloram


R.T.: 16.710 min
Delta R.T.: 0.021 min
Response: 27734071
Conc: 10.93 ng/ml

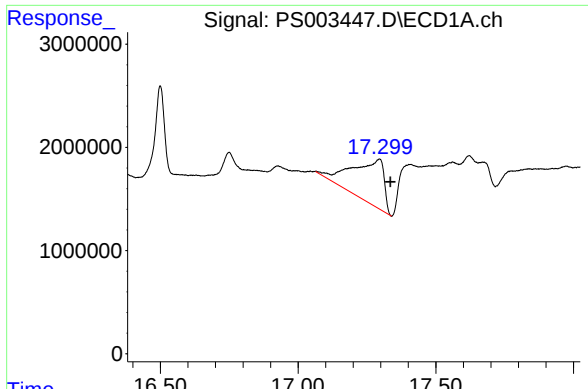

#16 DCPA

R.T.: 17.293 min
Delta R.T.: -0.042 min
Response: 34983590
Conc: 10.62 ng/ml

Instrument :
ECD_S
ClientSampleId :
S11

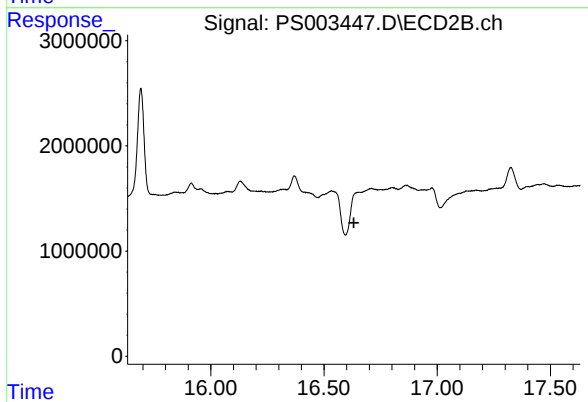

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 16.632 min
Response: 0
Conc: N.D.