

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030619\
 Data File : PS003448.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Mar 2019 23:59
 Operator : EI\SJ
 Sample : K1707-06
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 S12

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 02:32:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.307	10.811	244.9E6	258.8E6	557.888	551.072
Target Compounds							
1) T	Dalapon	2.828	2.319	44029053	59128348	67.743	93.382 #
2) T	3,5-DICHL...	0.000	8.977	0	9913393	N.D.	16.055 #
5) T	DICAMBA	11.512	11.050	14138482	6285436	8.021	3.762 #
6) T	MCP	11.994	11.299	5866845	212197	4.469	0.180 #
7) T	MCPA	12.185	0.000	69623320	0	35.100	N.D. #
10) T	Pentachlo...	0.000	13.205	0	69040	N.D.	0.010 #
11) T	2,4,5-TP ...	0.000	13.823	0	1235868	N.D.	0.485 #
12) T	2,4,5-T	0.000	14.412	0	13156353	N.D.	6.523 #
13) T	2,4-DB	15.506	0.000	16601033	0	70.107	N.D. #
15) T	Picloram	16.789	16.751	6867635	32140654	2.790	12.663 #
16) T	DCPA	17.332	16.566	33023526	22607491	10.022	7.268 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030619\
Data File : PS003448.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2019 23:59
Operator : EI\SJ
Sample : K1707-06
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
S12

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 02:32:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

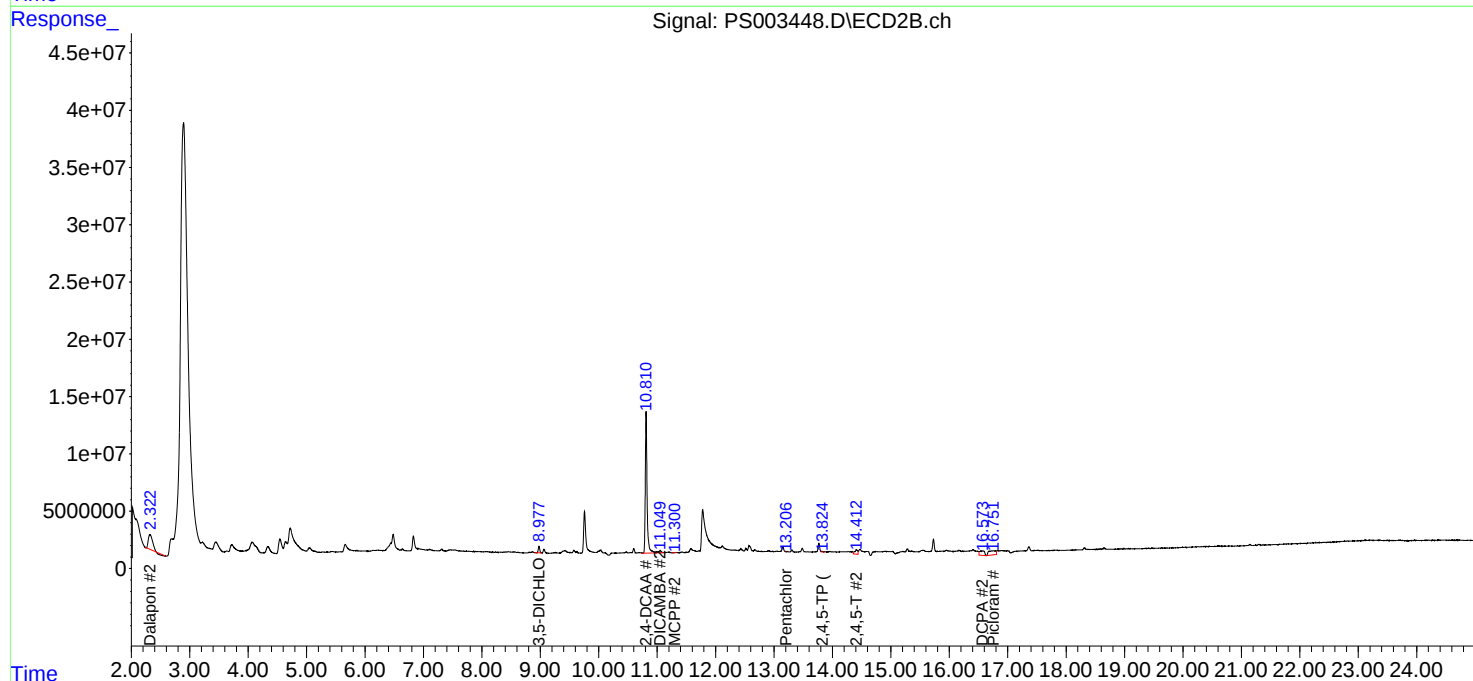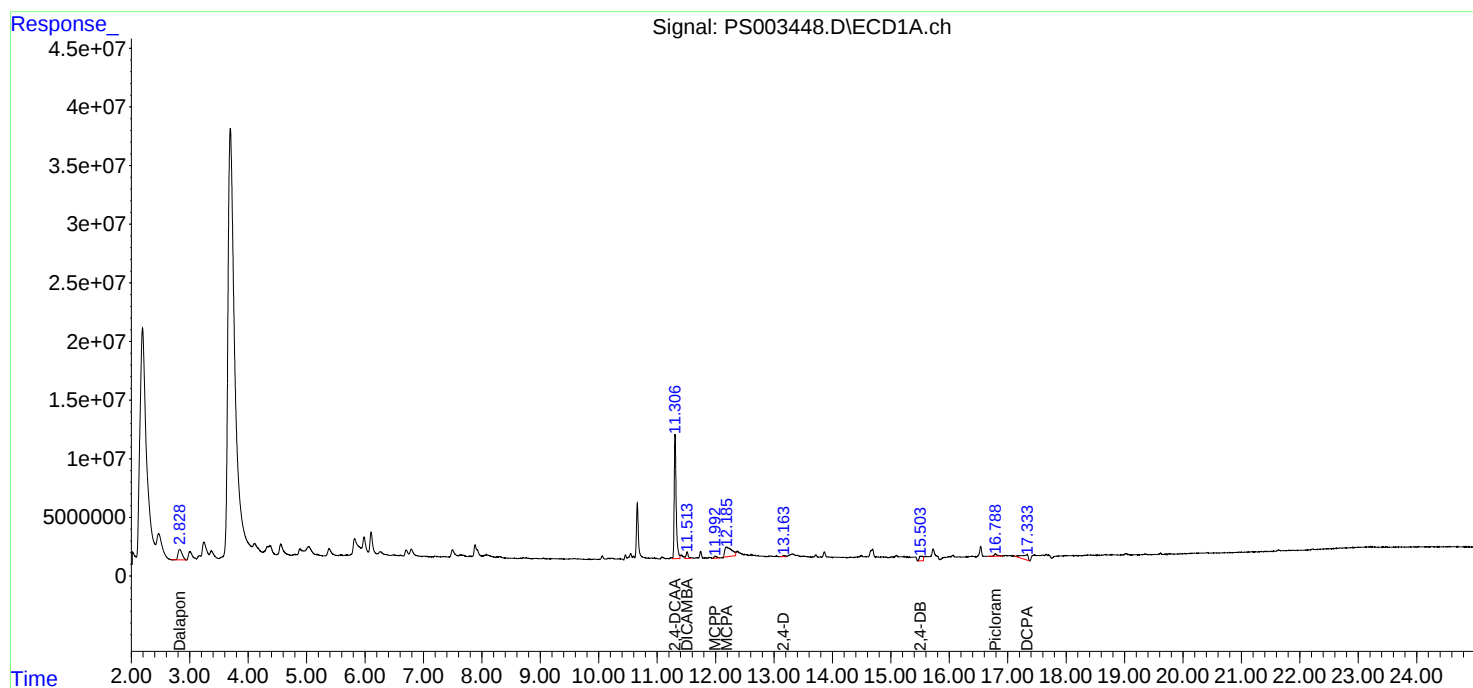


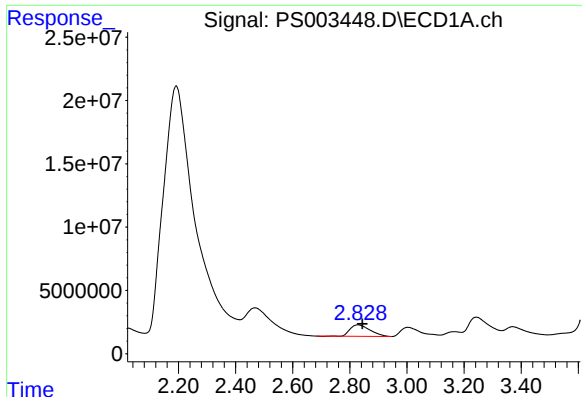

#1 Dalapon


R.T.: 2.828 min
Delta R.T.: -0.016 min
Response: 44029053
Conc: 67.74 ng/ml

Instrument :
ECD_S
ClientSampleId :
S12

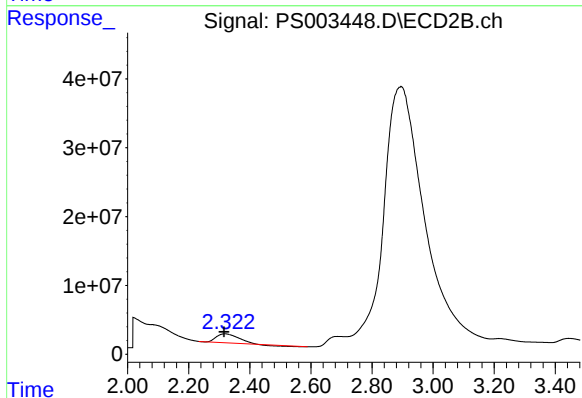


#1 Dalapon

R.T.: 2.319 min
Delta R.T.: 0.003 min
Response: 59128348
Conc: 93.38 ng/ml

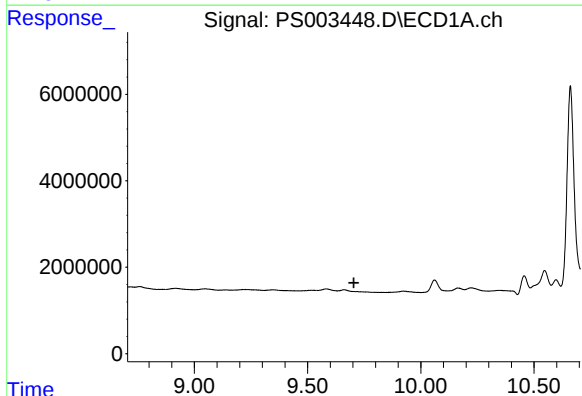


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.705 min
Response: 0
Conc: N.D.

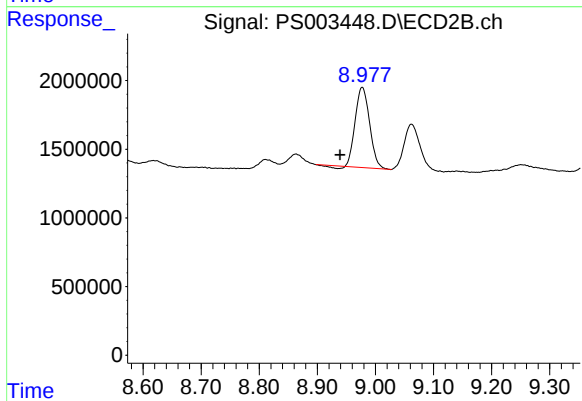

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.977 min
Delta R.T.: 0.038 min
Response: 9913393
Conc: 16.06 ng/ml

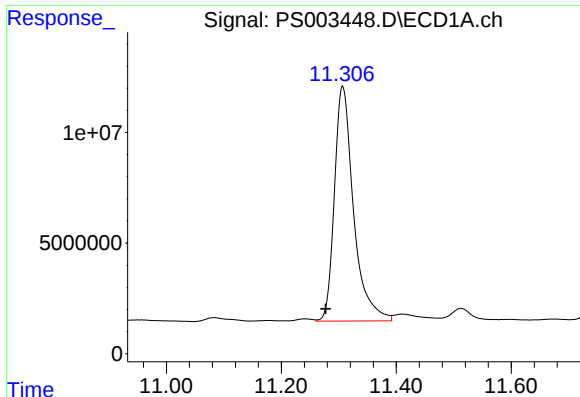

#4 2,4-DCAA


R.T.: 11.307 min
Delta R.T.: 0.029 min
Response: 244926510
Conc: 557.89 ng/ml

Instrument :
ECD_S
ClientSampleId :
S12

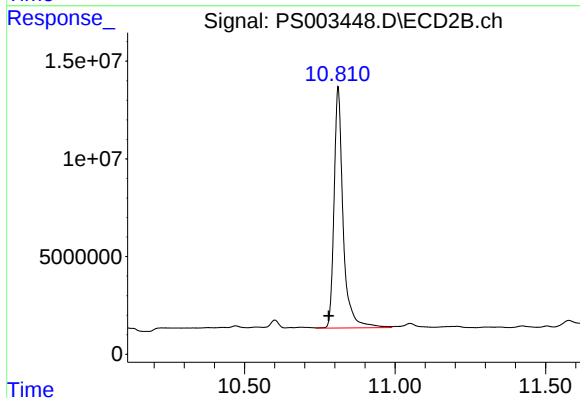


#4 2,4-DCAA

R.T.: 10.811 min
Delta R.T.: 0.031 min
Response: 258766481
Conc: 551.07 ng/ml

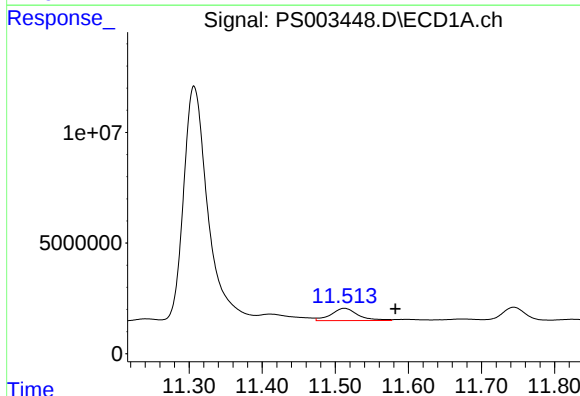


#5 DICAMBA

R.T.: 11.512 min
Delta R.T.: -0.070 min
Response: 14138482
Conc: 8.02 ng/ml

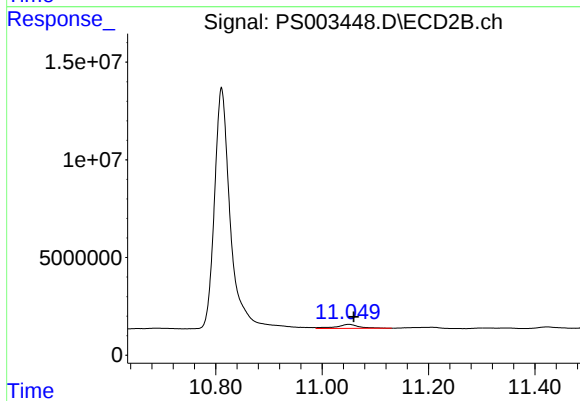

#5 DICAMBA


R.T.: 11.050 min
Delta R.T.: -0.010 min
Response: 6285436
Conc: 3.76 ng/ml

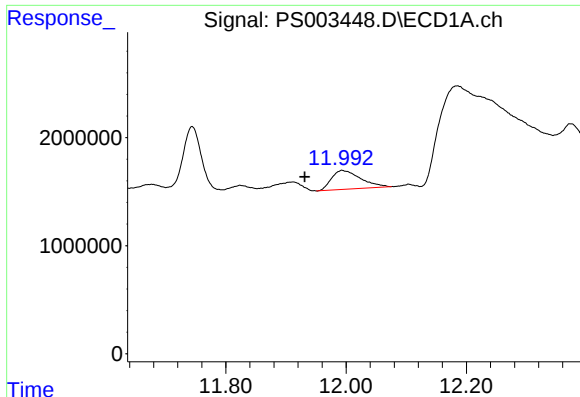

#6 MCPP


R.T.: 11.994 min
Delta R.T.: 0.063 min
Response: 5866845
Conc: 4.47 ug/ml

Instrument :
ECD_S
ClientSampleId :
S12

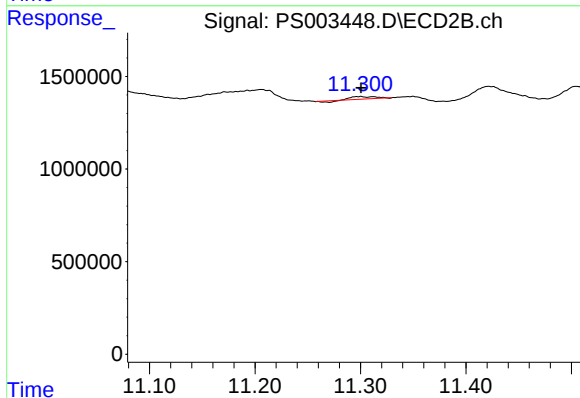


#6 MCPP

R.T.: 11.299 min
Delta R.T.: -0.001 min
Response: 212197
Conc: 0.18 ug/ml

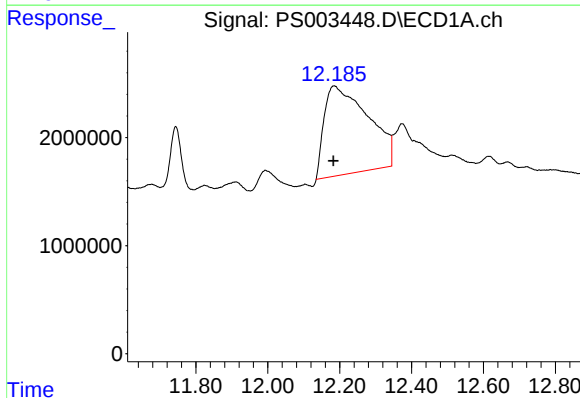


#7 MCPA

R.T.: 12.185 min
Delta R.T.: 0.002 min
Response: 69623320
Conc: 35.10 ug/ml

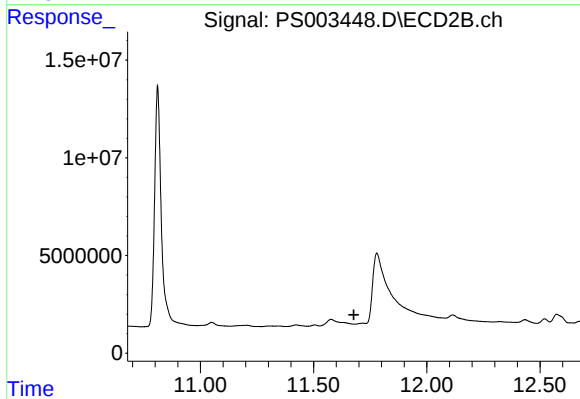

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 11.678 min
Response: 0
Conc: N.D.

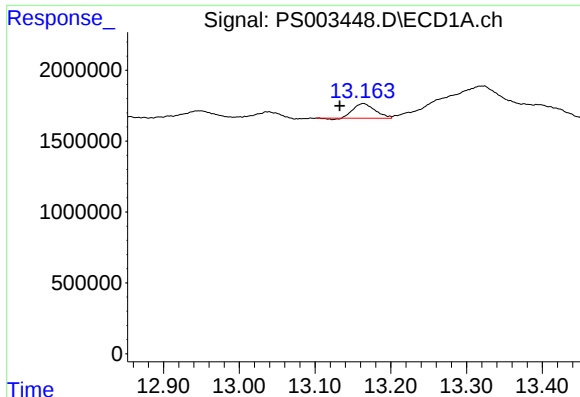

#9 2,4-D


R.T.: 13.164 min
Delta R.T.: 0.031 min
Response: 2032653
Conc: 4.38 ng/ml

Instrument :
ECD_S
ClientSampleId :
S12

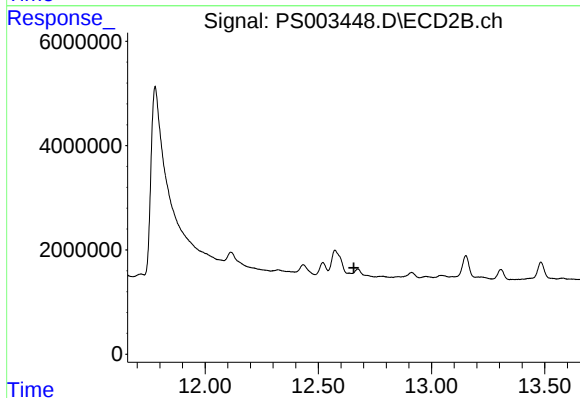


#9 2,4-D

R.T.: 12.674 min
Delta R.T.: 0.017 min
Response: -4624398
Conc: N.D.

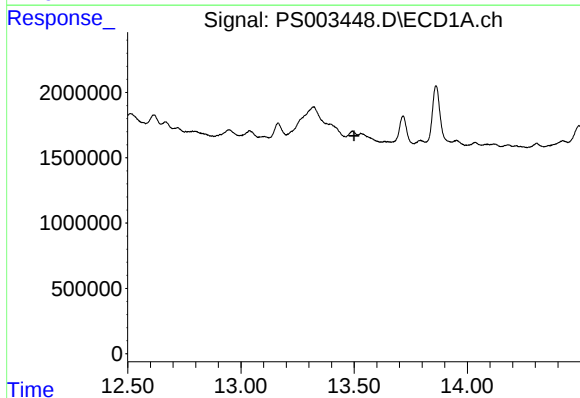


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.499 min
Response: 0
Conc: N.D.

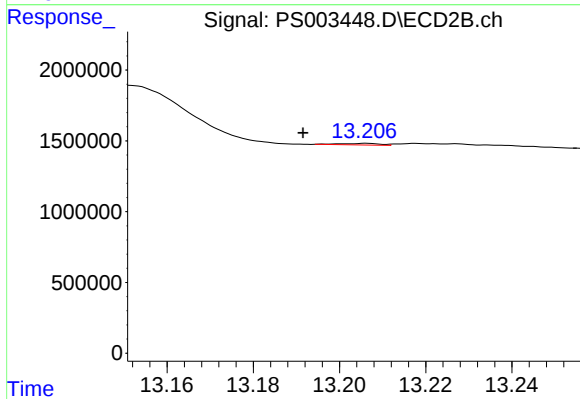

#10 Pentachlorophenol


R.T.: 13.205 min
Delta R.T.: 0.014 min
Response: 69040
Conc: 0.01 ng/ml

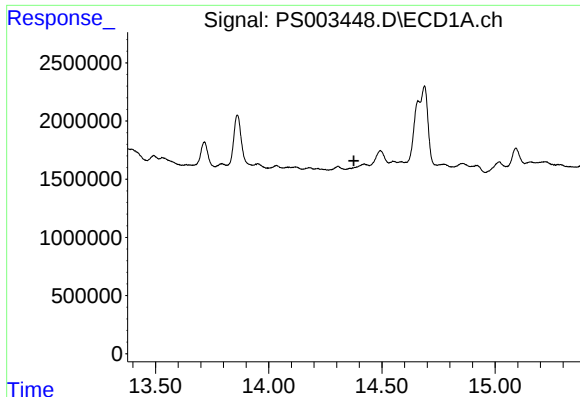

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
S12

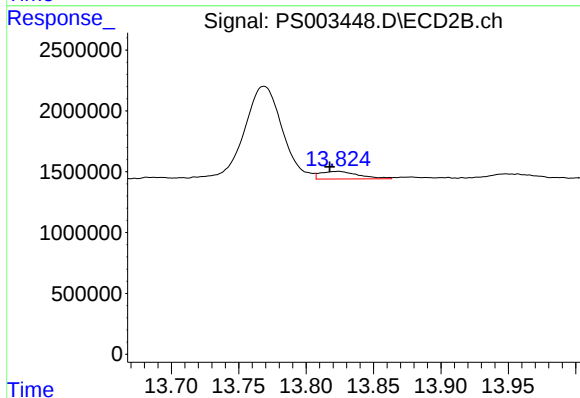


#11 2,4,5-TP (SILVEX)

R.T.: 13.823 min
Delta R.T.: 0.006 min
Response: 1235868
Conc: 0.49 ng/ml

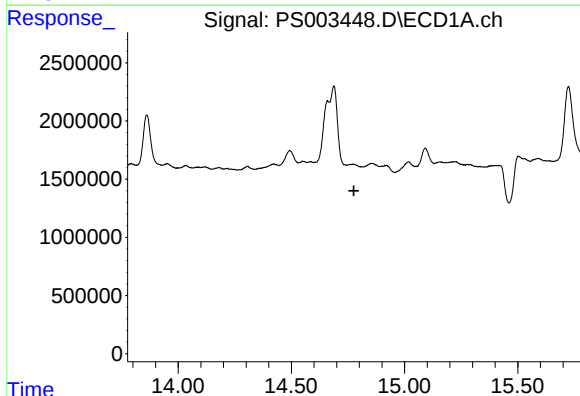


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

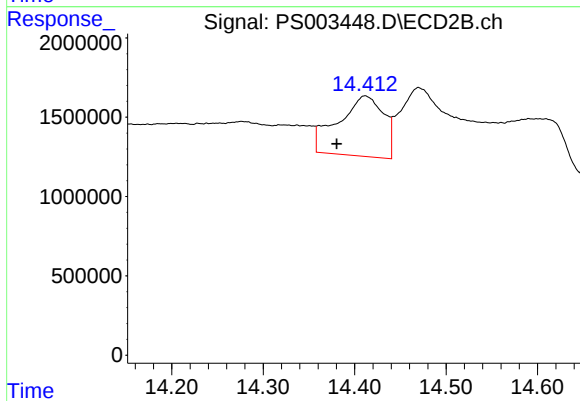

#12 2,4,5-T


R.T.: 14.412 min
Delta R.T.: 0.031 min
Response: 13156353
Conc: 6.52 ng/ml

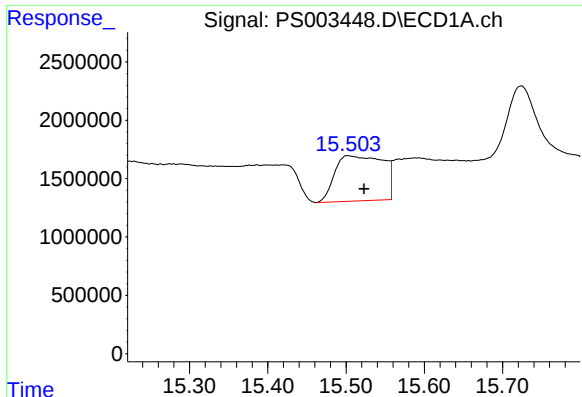

#13 2,4-DB


R.T.: 15.506 min
Delta R.T.: -0.017 min
Response: 16601033
Conc: 70.11 ng/ml

Instrument :
ECD_S
ClientSampleId :
S12

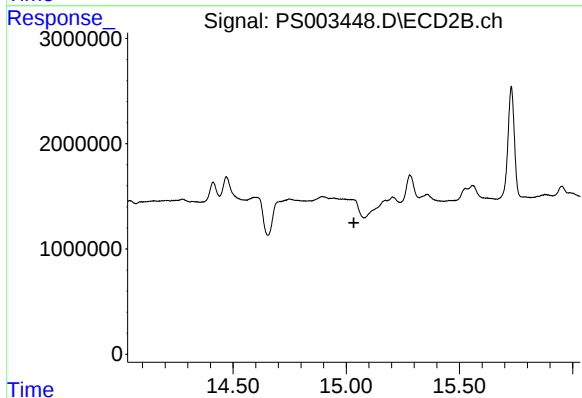


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.033 min
Response: 0
Conc: N.D.

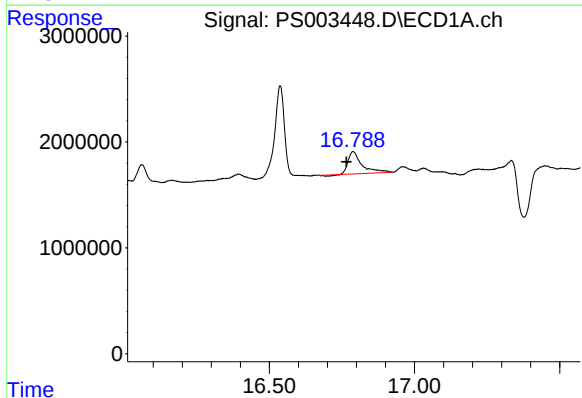


#15 Picloram

R.T.: 16.789 min
Delta R.T.: 0.024 min
Response: 6867635
Conc: 2.79 ng/ml

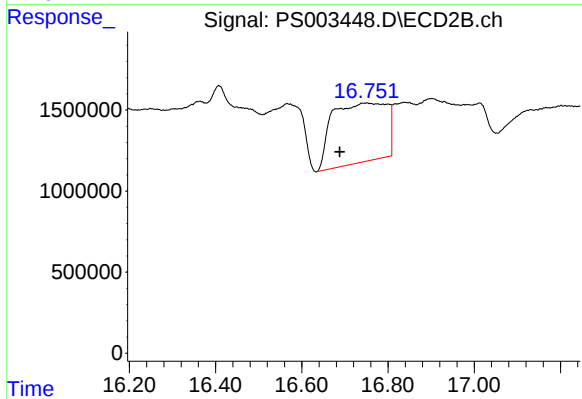

#15 Picloram


R.T.: 16.751 min
Delta R.T.: 0.062 min
Response: 32140654
Conc: 12.66 ng/ml

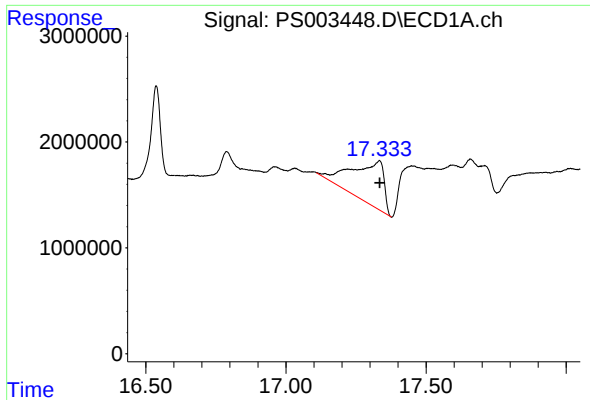

#16 DCPA

R.T.: 17.332 min
Delta R.T.: -0.003 min
Response: 33023526
Conc: 10.02 ng/ml

Instrument :
ECD_S
ClientSampleId :
S12

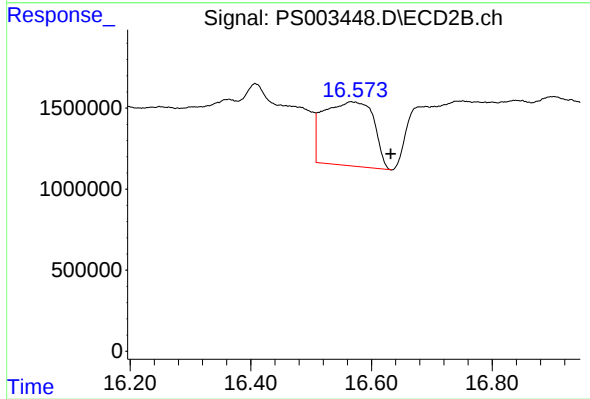

#16 DCPA

R.T.: 16.566 min
Delta R.T.: -0.066 min
Response: 22607491
Conc: 7.27 ng/ml