

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030619\
 Data File : PS003449.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Mar 2019 00:30
 Operator : EI\SJ
 Sample : K1753-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 Z-2-5

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 02:32:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.276	10.779	233.4E6	242.3E6	531.665	516.071
Target Compounds							
1) T	Dalapon	2.798	2.288	39945757	67189891	61.460	106.114 #
2) T	3,5-DICHL...	0.000	8.946	0	7261371	N.D.	11.760 #
5) T	DICAMBA	0.000	11.019	0	4622695	N.D.	2.767 #
6) T	MCP	11.965	11.315	2508627	616828	1.911	0.523 #
9) T	2,4-D	13.132	12.642	4829807	1953714	10.413	3.722 #
12) T	2,4,5-T	0.000	14.380	0	8844899	N.D.	4.386 #
13) T	2,4-DB	15.552	0.000	10648301	0	44.968	N.D. #
14) T	DINOSEB	0.000	15.424	0	1072570	N.D.	0.601 #
15) T	Picloram	16.752	16.746	8673106	21817553	3.524	8.596 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030619\
Data File : PS003449.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Mar 2019 00:30
Operator : EI\SJ
Sample : K1753-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
Z-2-5

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 02:32:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

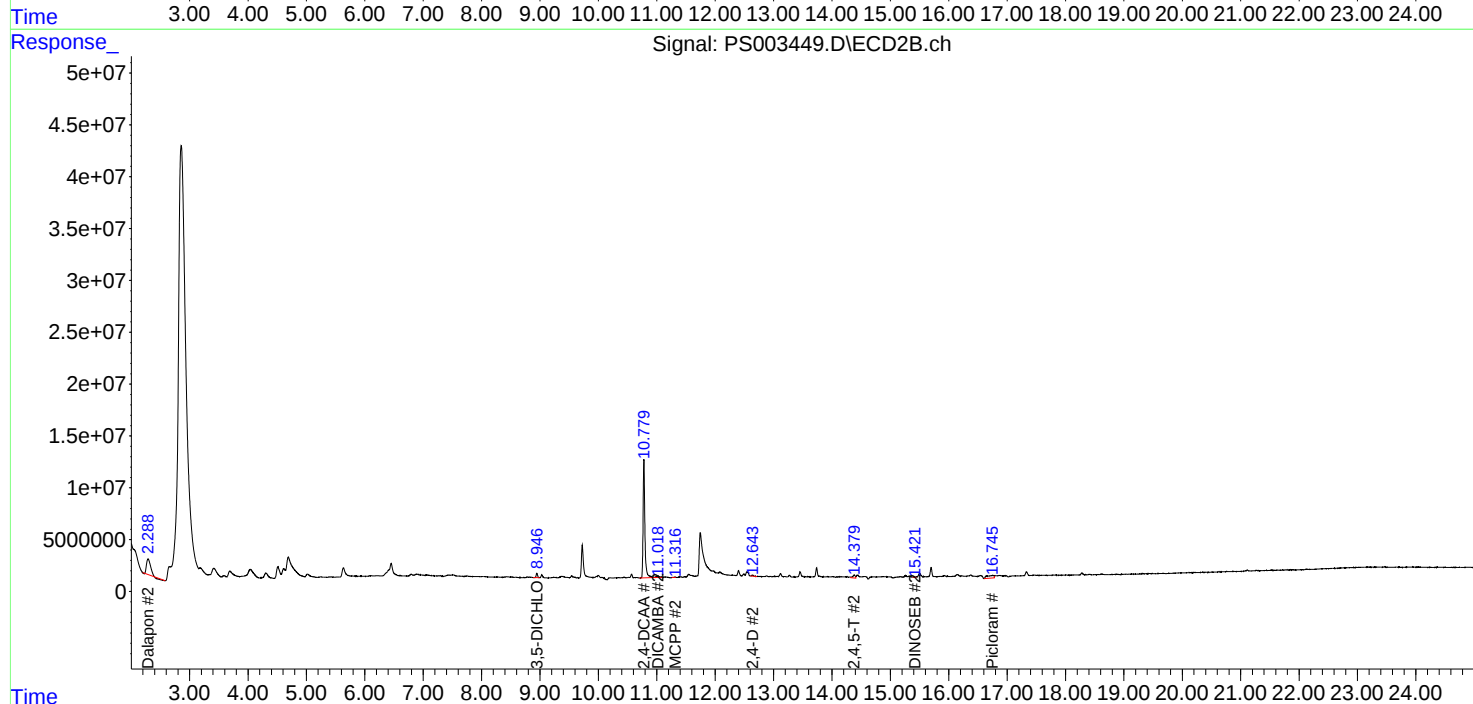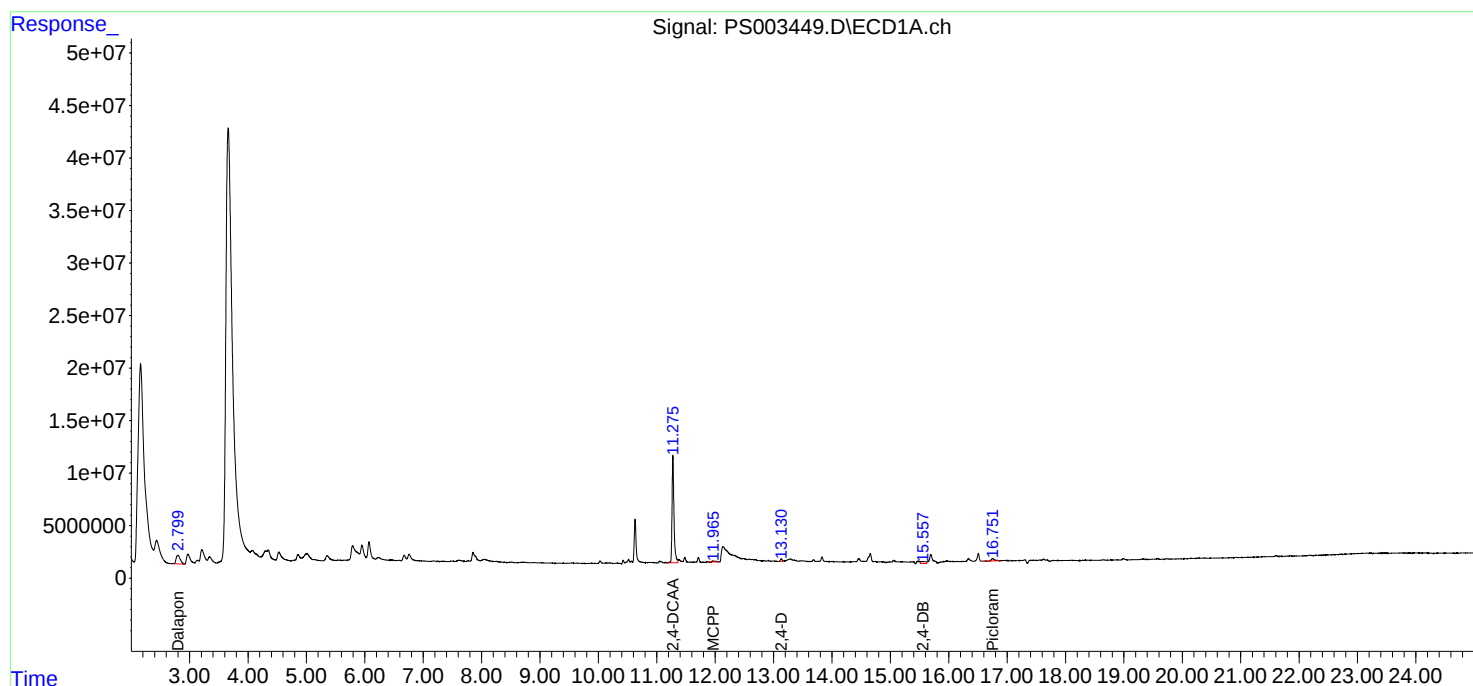


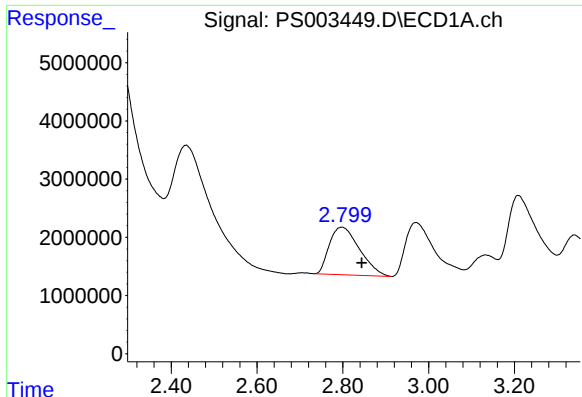

#1 Dalapon


R.T.: 2.798 min
Delta R.T.: -0.046 min
Response: 39945757
Conc: 61.46 ng/ml

Instrument :
ECD_S
ClientSampleId :
Z-2-5

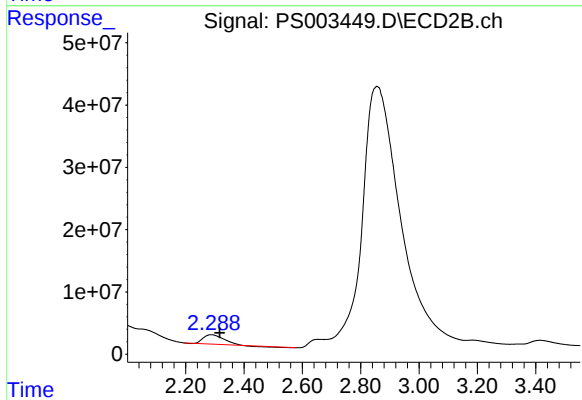


#1 Dalapon

R.T.: 2.288 min
Delta R.T.: -0.029 min
Response: 67189891
Conc: 106.11 ng/ml

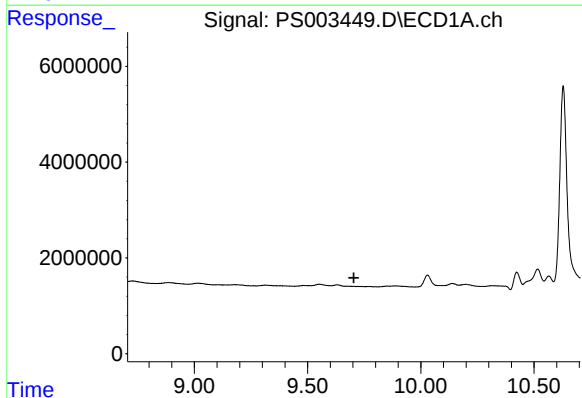


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.705 min
Response: 0
Conc: N.D.

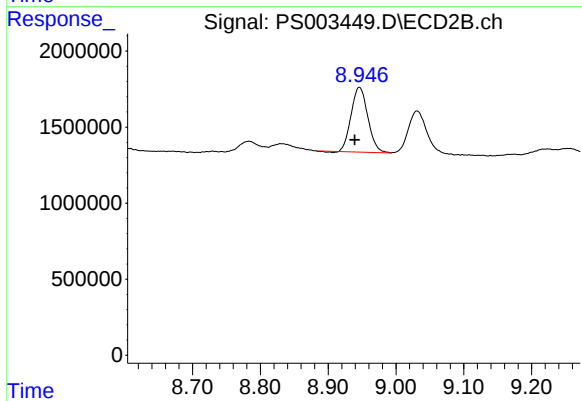

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.946 min
Delta R.T.: 0.007 min
Response: 7261371
Conc: 11.76 ng/ml

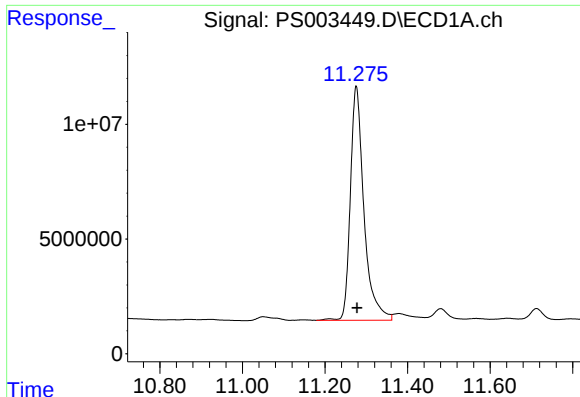

#4 2,4-DCAA


R.T.: 11.276 min
Delta R.T.: -0.002 min
Response: 233414072
Conc: 531.67 ng/ml

Instrument :
ECD_S
ClientSampleId :
Z-2-5

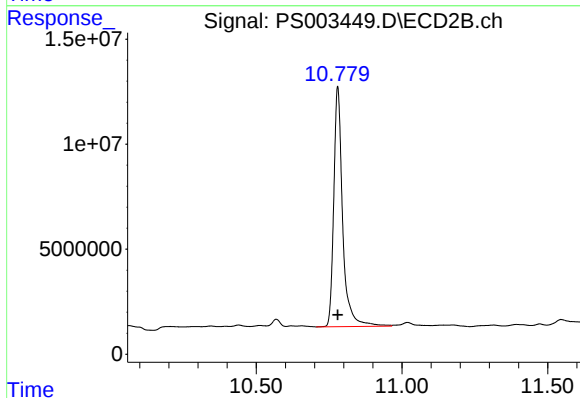


#4 2,4-DCAA

R.T.: 10.779 min
Delta R.T.: 0.000 min
Response: 242331159
Conc: 516.07 ng/ml

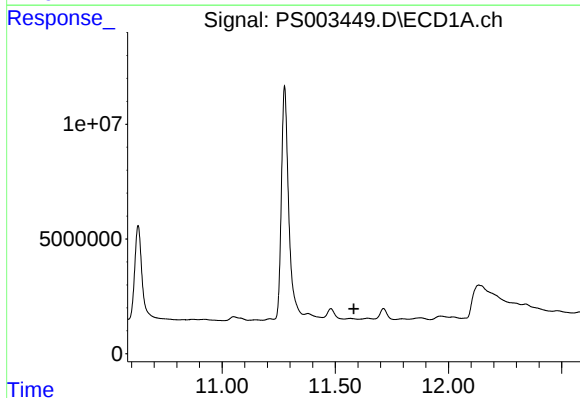


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.582 min
Response: 0
Conc: N.D.

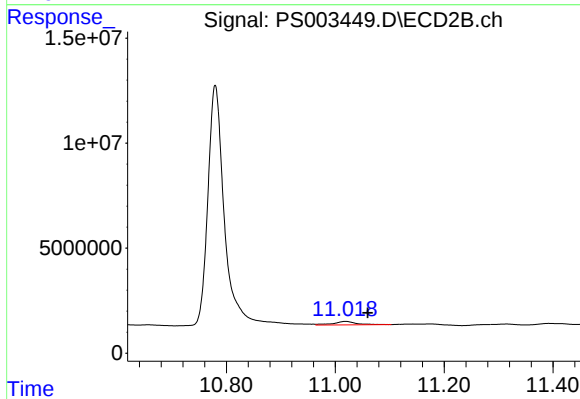

#5 DICAMBA


R.T.: 11.019 min
Delta R.T.: -0.041 min
Response: 4622695
Conc: 2.77 ng/ml

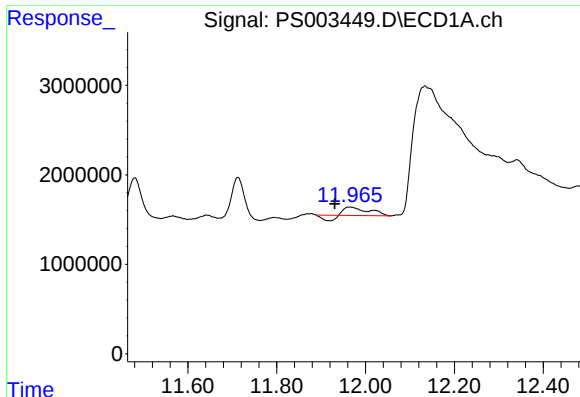

#6 MCP


R.T.: 11.965 min
Delta R.T.: 0.034 min
Response: 2508627
Conc: 1.91 ug/ml

Instrument :
ECD_S
ClientSampleId :
Z-2-5

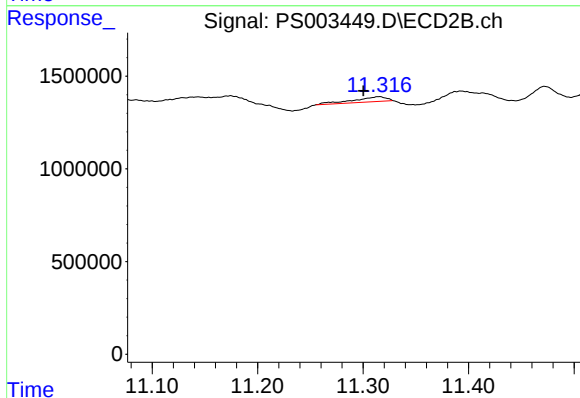


#6 MCP

R.T.: 11.315 min
Delta R.T.: 0.014 min
Response: 616828
Conc: 0.52 ug/ml

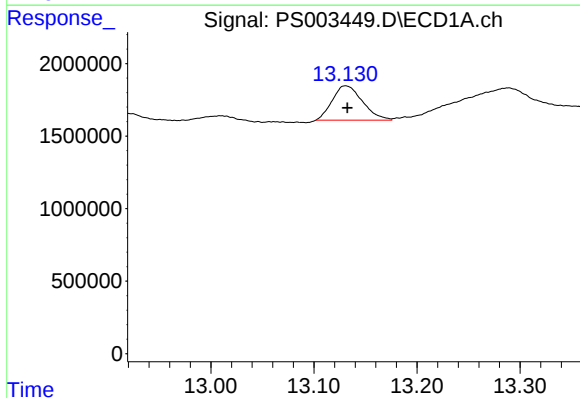


#9 2,4-D

R.T.: 13.132 min
Delta R.T.: 0.000 min
Response: 4829807
Conc: 10.41 ng/ml

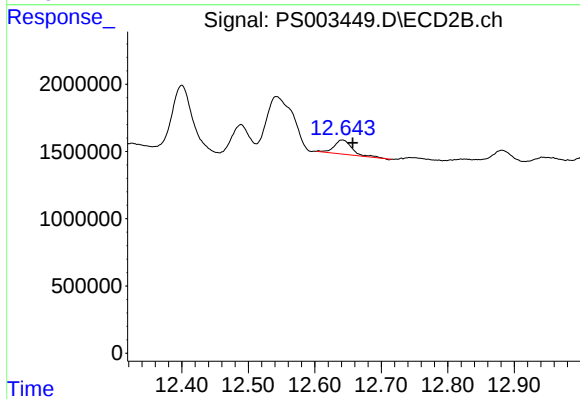

#9 2,4-D


R.T.: 12.642 min
Delta R.T.: -0.015 min
Response: 1953714
Conc: 3.72 ng/ml

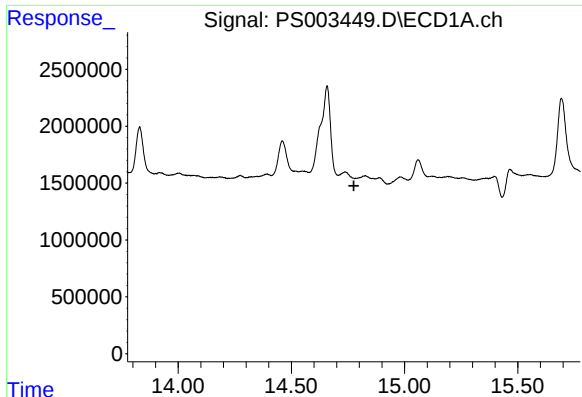

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
Z-2-5

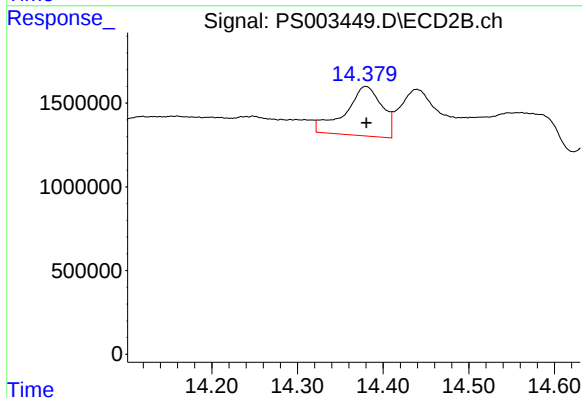


#12 2,4,5-T

R.T.: 14.380 min
Delta R.T.: 0.000 min
Response: 8844899
Conc: 4.39 ng/ml

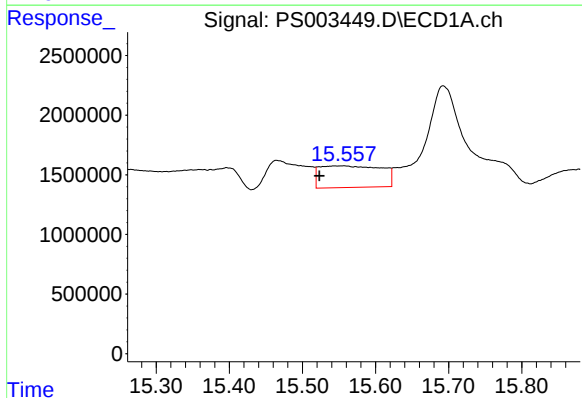


#13 2,4-DB

R.T.: 15.552 min
Delta R.T.: 0.029 min
Response: 10648301
Conc: 44.97 ng/ml

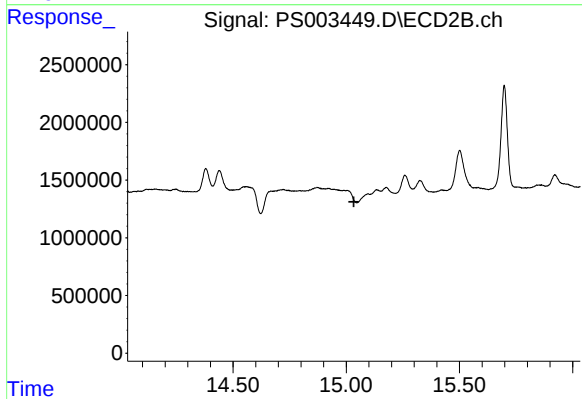

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.033 min
Response: 0
Conc: N.D.

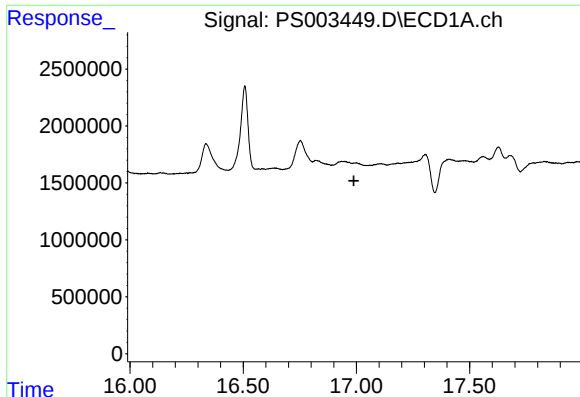

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
Z-2-5

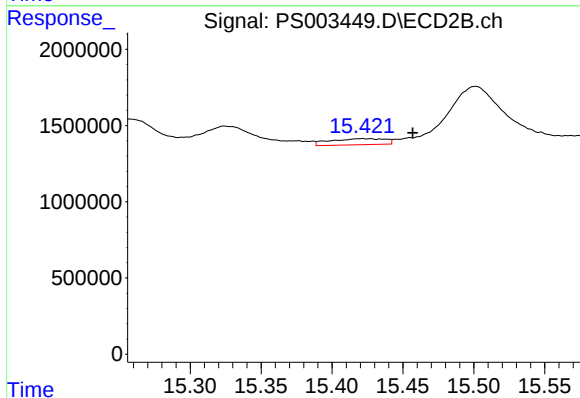


#14 DINOSEB

R.T.: 15.424 min
Delta R.T.: -0.033 min
Response: 1072570
Conc: 0.60 ng/ml

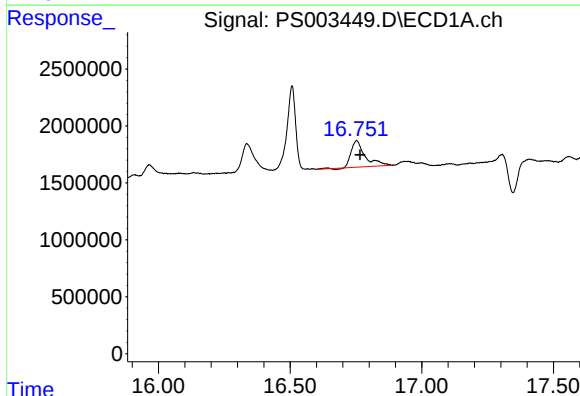

#15 Picloram

R.T.: 16.752 min
Delta R.T.: -0.013 min
Response: 8673106
Conc: 3.52 ng/ml

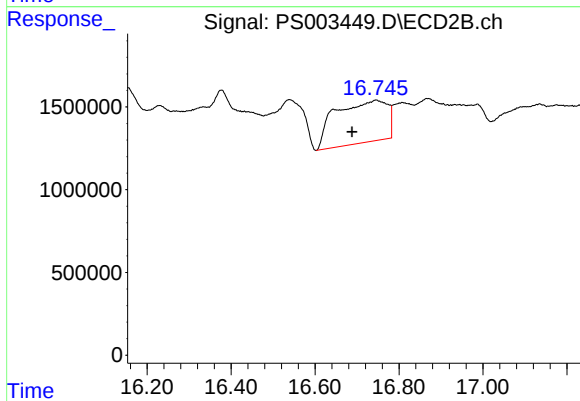

#15 Picloram

R.T.: 16.746 min
Delta R.T.: 0.057 min
Response: 21817553
Conc: 8.60 ng/ml