

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030619\
 Data File : PS003452.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Mar 2019 02:04
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 03:59:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.295	10.797	228.8E6	217.6E6	521.060	463.456
Target Compounds							
2) T	3,5-DICHL...	0.000	8.985	0	70461	N.D.	0.114 #
3) T	4-Nitroph...	0.000	9.866	0	30399	N.D.	0.135 #
7) T	MCPA	0.000	11.686	0	356938	N.D.	0.207 #
9) T	2,4-D	0.000	12.691	0	28042	N.D.	0.053 #
10) T	Pentachlo...	0.000	13.214	0	652542	N.D.	0.099 #
11) T	2,4,5-TP ...	0.000	13.846	0	145488	N.D.	0.057 #
12) T	2,4,5-T	0.000	14.361	0	44314	N.D.	0.022 #
13) T	2,4-DB	0.000	15.034	0	106883	N.D.	0.419 #
14) T	DINOSEB	0.000	15.512	0	251578	N.D.	0.141 #
15) T	Picloram	0.000	16.649	0	702326	N.D.	0.277 #
16) T	DCPA	0.000	16.649	0	702326	N.D.	0.226 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030619\
Data File : PS003452.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Mar 2019 02:04
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 03:59:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

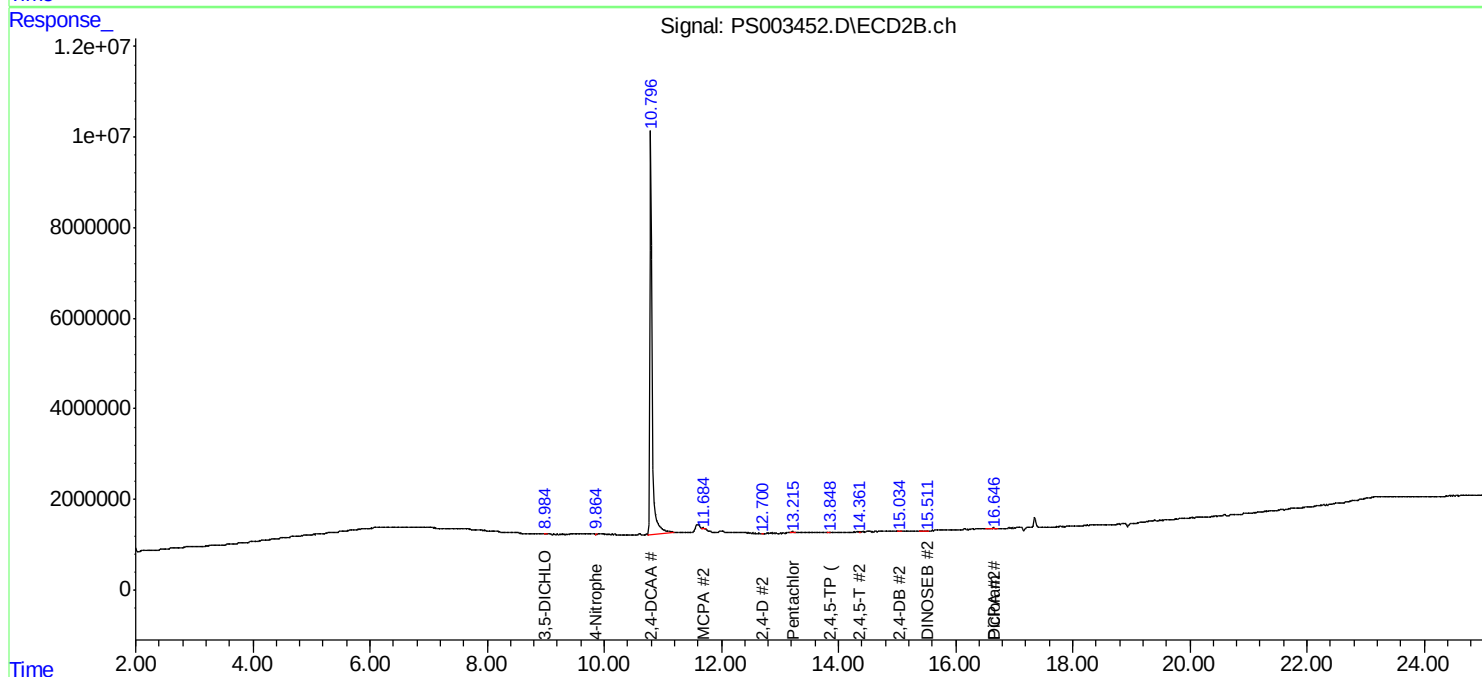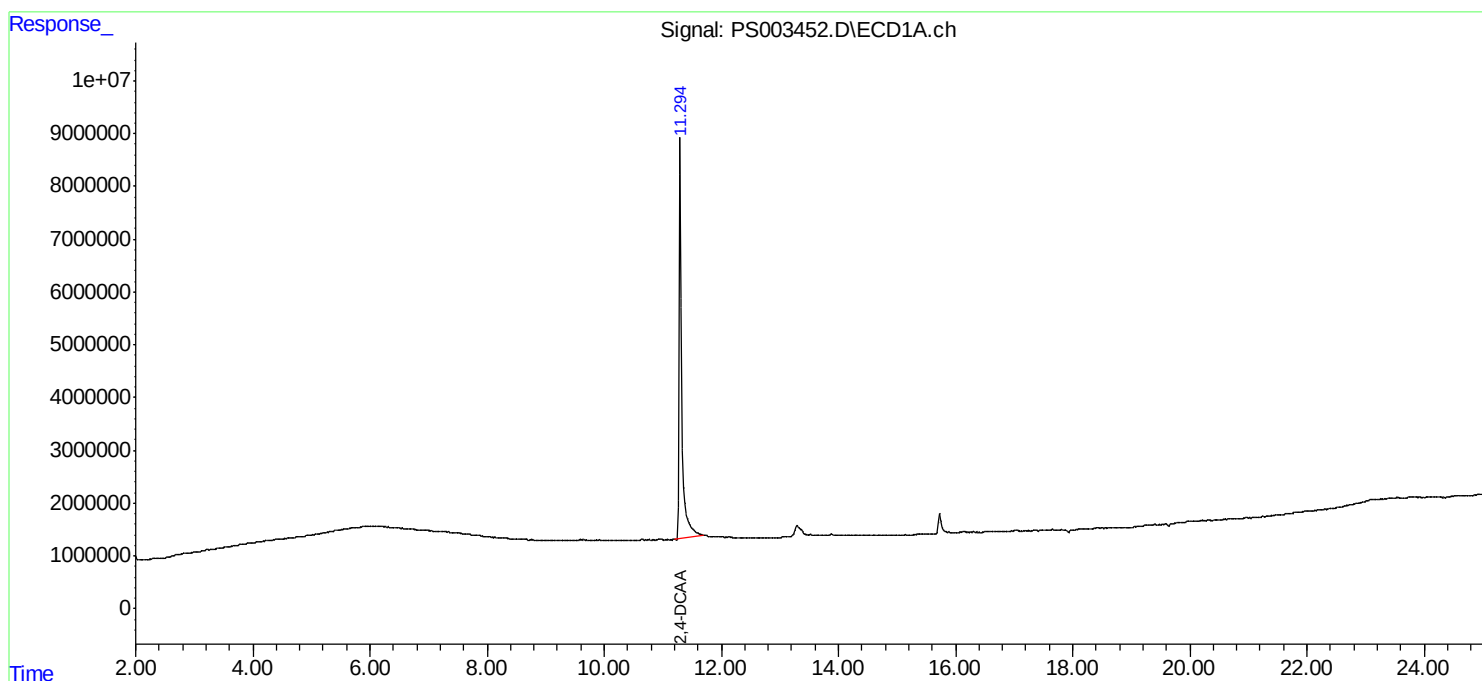


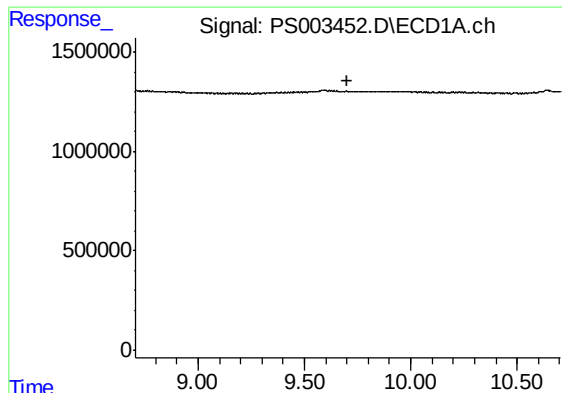

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.705 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

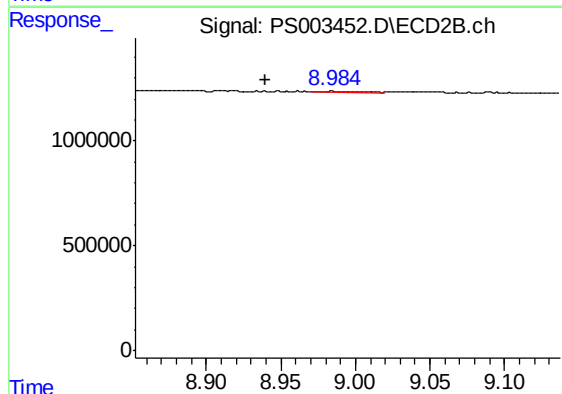


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 8.985 min
Delta R.T.: 0.045 min
Response: 70461
Conc: 0.11 ng/ml

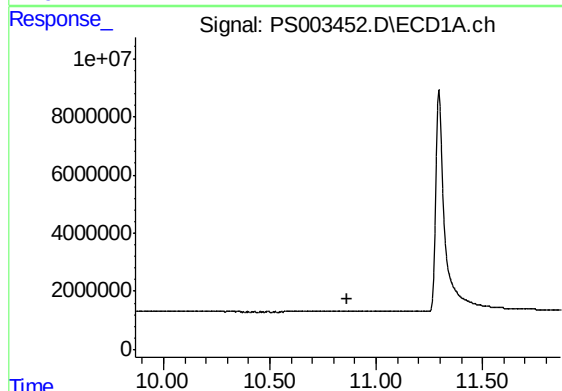


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

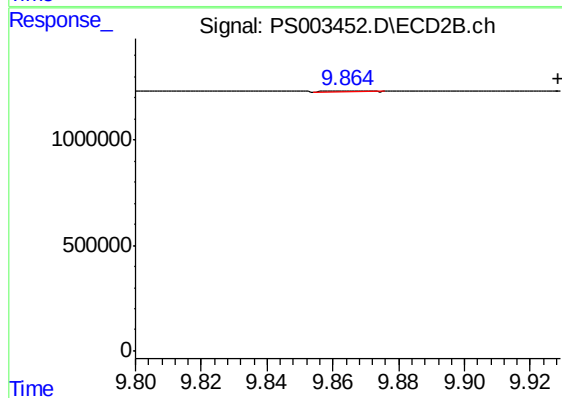

#3 4-Nitrophenol


R.T.: 9.866 min
Delta R.T.: -0.063 min
Response: 30399
Conc: 0.14 ng/ml

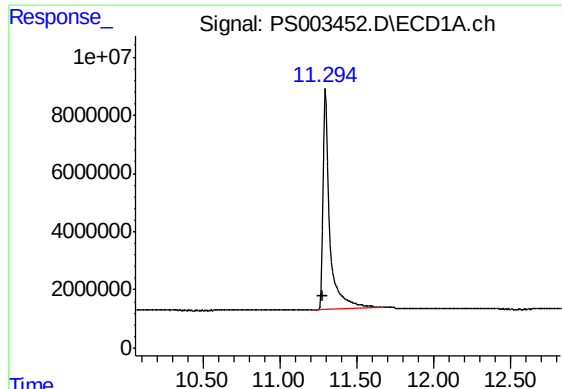

#4 2,4-DCAA


R.T.: 11.295 min
Delta R.T.: 0.017 min
Response: 228758192
Conc: 521.06 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

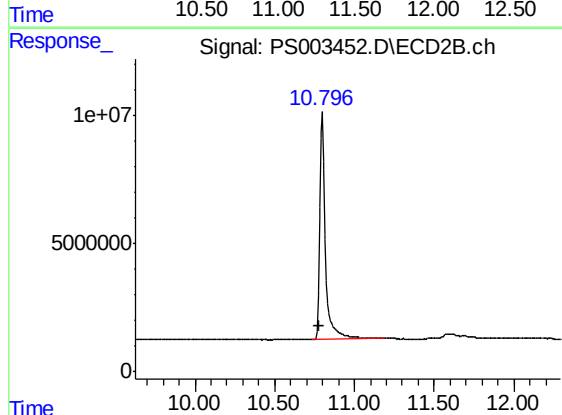


#4 2,4-DCAA

R.T.: 10.797 min
Delta R.T.: 0.017 min
Response: 217624667
Conc: 463.46 ng/ml

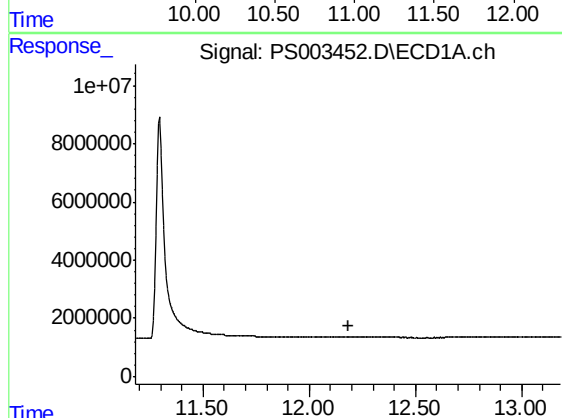


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.182 min
Response: 0
Conc: N.D.

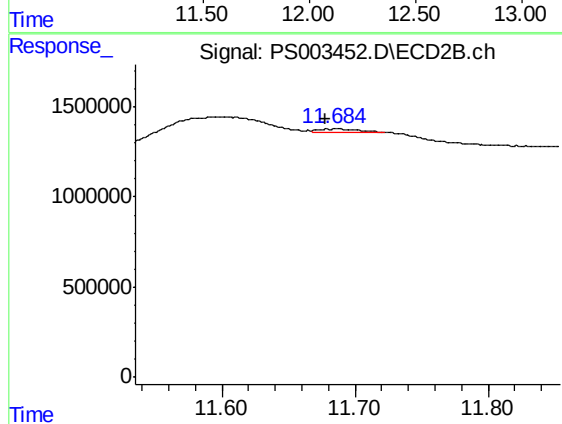

#7 MCPA


R.T.: 11.686 min
Delta R.T.: 0.008 min
Response: 356938
Conc: 0.21 ug/ml

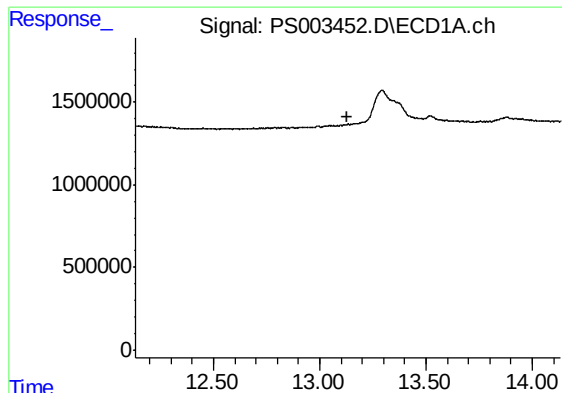

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 13.133 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

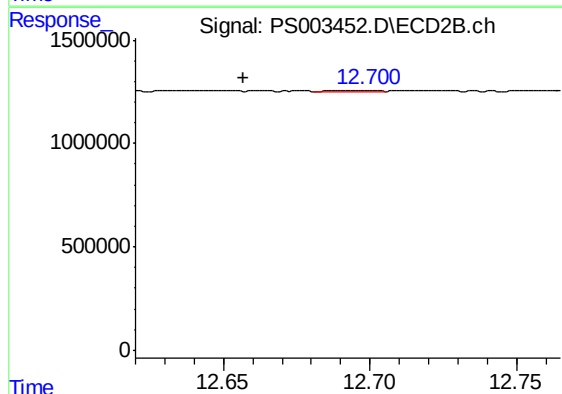


#9 2,4-D

R.T.: 12.691 min
Delta R.T.: 0.034 min
Response: 28042
Conc: 0.05 ng/ml

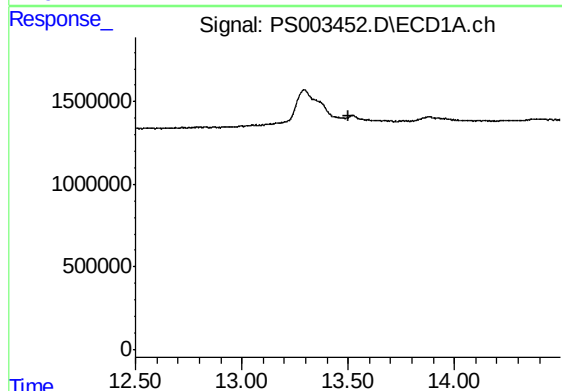


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.499 min
Response: 0
Conc: N.D.

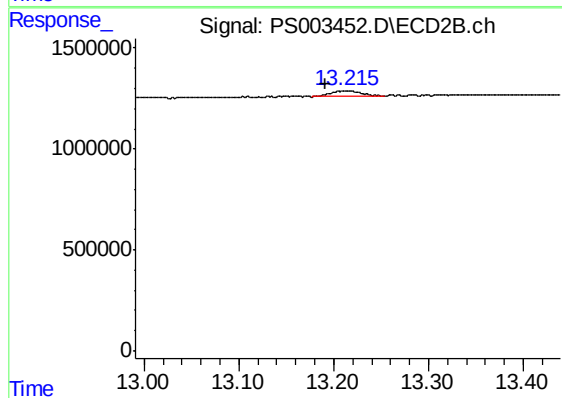

#10 Pentachlorophenol


R.T.: 13.214 min
Delta R.T.: 0.023 min
Response: 652542
Conc: 0.10 ng/ml

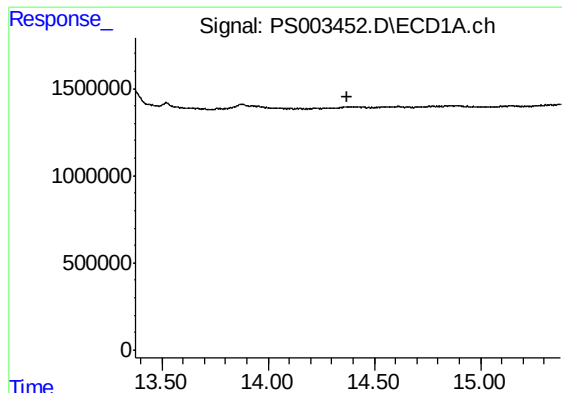

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 14.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

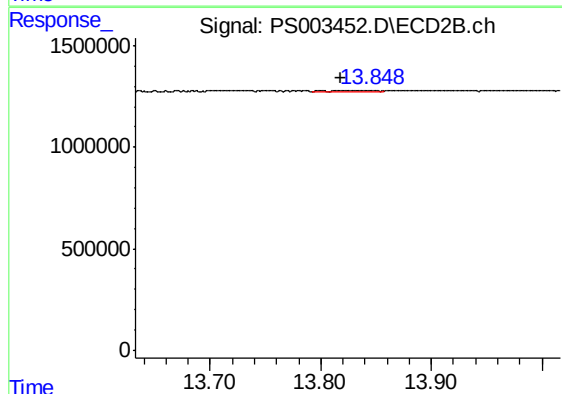


#11 2,4,5-TP (SILVEX)

R.T.: 13.846 min
Delta R.T.: 0.029 min
Response: 145488
Conc: 0.06 ng/ml

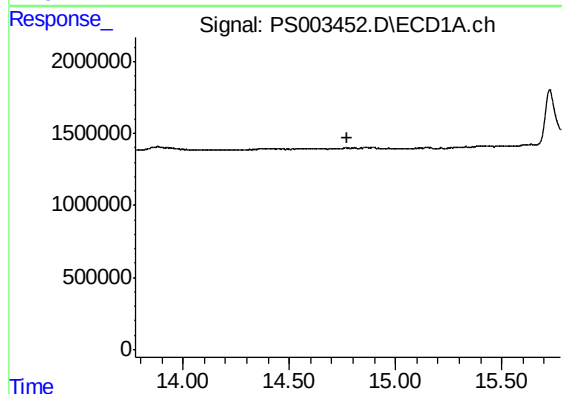


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 14.776 min
Response: 0
Conc: N.D.

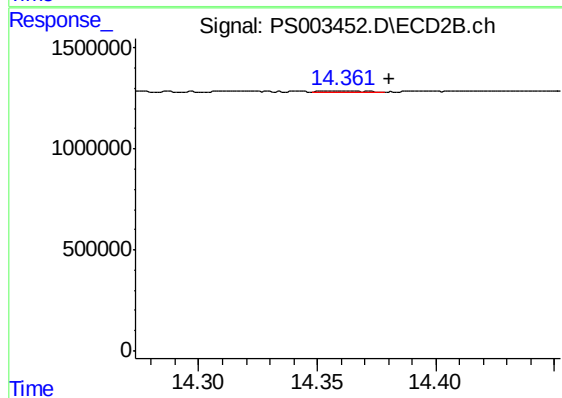

#12 2,4,5-T


R.T.: 14.361 min
Delta R.T.: -0.019 min
Response: 44314
Conc: 0.02 ng/ml

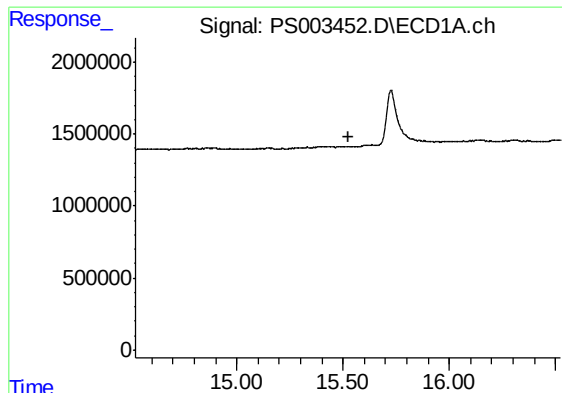

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 15.523 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

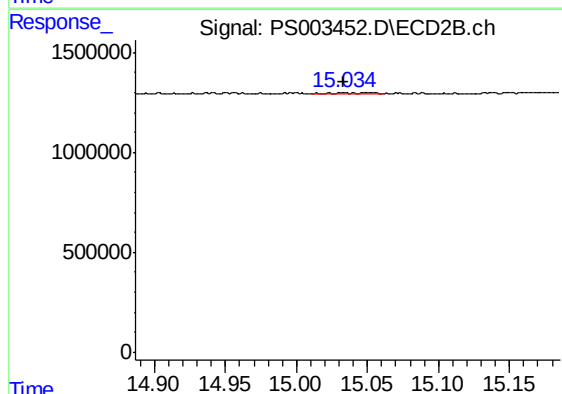


#13 2,4-DB

R.T.: 15.034 min
Delta R.T.: 0.000 min
Response: 106883
Conc: 0.42 ng/ml

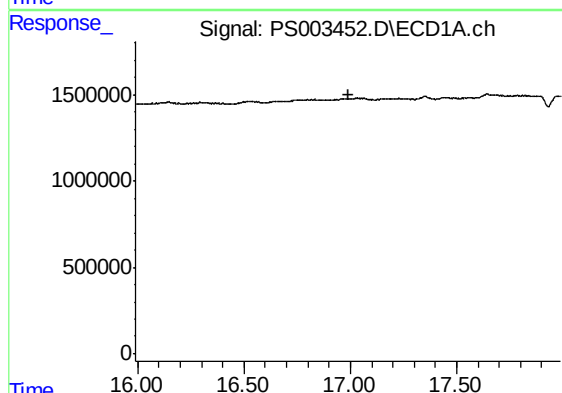


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 16.989 min
Response: 0
Conc: N.D.

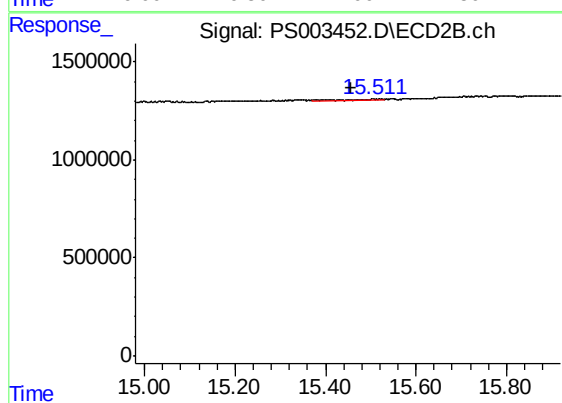

#14 DINOSEB


R.T.: 15.512 min
Delta R.T.: 0.055 min
Response: 251578
Conc: 0.14 ng/ml

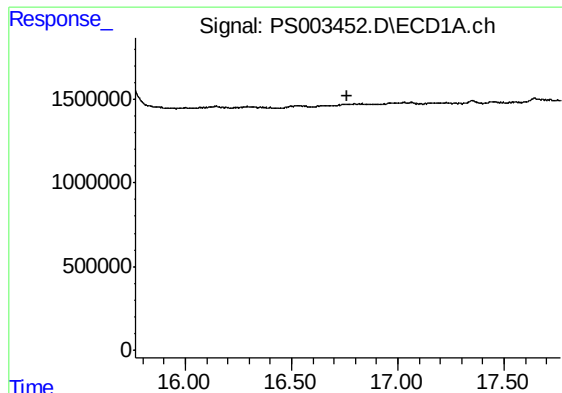

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 16.765 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

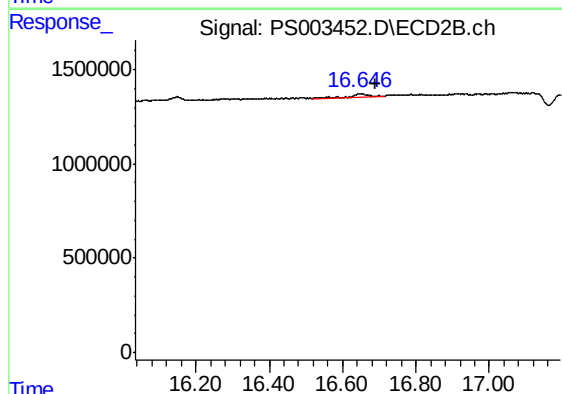


#15 Picloram

R.T.: 16.649 min
Delta R.T.: -0.040 min
Response: 702326
Conc: 0.28 ng/ml

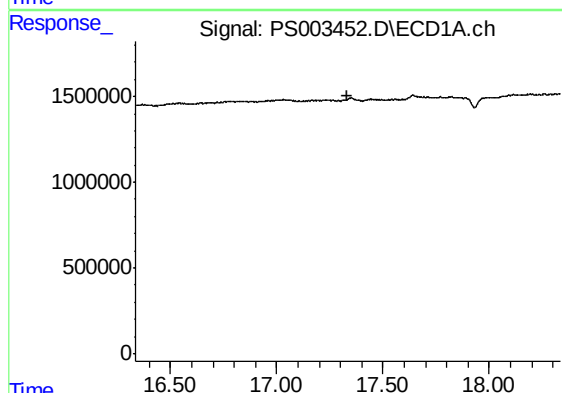

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.335 min
Response: 0
Conc: N.D.

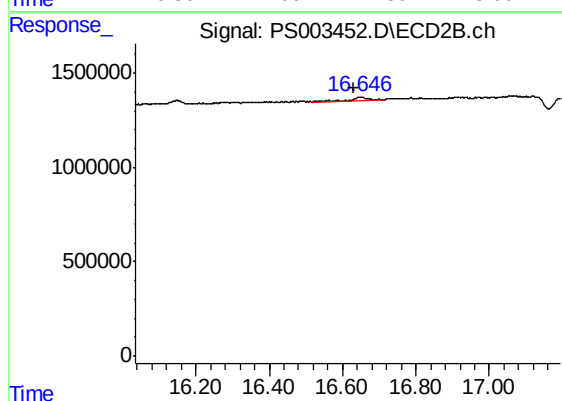

#16 DCPA

R.T.: 16.649 min
Delta R.T.: 0.017 min
Response: 702326
Conc: 0.23 ng/ml