

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030619\
 Data File : PS003456.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Mar 2019 04:08
 Operator : EI\SJ
 Sample : PB117670TB
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB117670TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 04:47:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.310	10.812	211.5E6	226.8E6	481.737	483.036
Target Compounds							
1) T	Dalapon	2.828	2.314	35888217	33194339	55.217	52.424
2) T	3,5-DICHL...	0.000	8.978	0	8587636	N.D.	13.908 #
5) T	DICAMBA	11.513	11.051	14004268	4900174	7.945	2.933 #
6) T	MCPD	0.000	11.306	0	161464	N.D.	0.137 #
7) T	MCPA	12.251	0.000	39720695	0	20.025	N.D. #
8) T	DICHLORPROP	0.000	12.117	0	25997883	N.D.	62.912 #
10) T	Pentachlo...	0.000	13.220	0	295015	N.D.	0.045 #
11) T	2,4,5-TP ...	0.000	13.823	0	1869495	N.D.	0.734 #
12) T	2,4,5-T	0.000	14.413	0	12282606	N.D.	6.090 #
15) T	Picloram	16.792	16.749	1670438	30462294	0.679	12.002 #
16) T	DCPA	0.000	16.583	0	9979070	N.D.	3.208 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030619\
Data File : PS003456.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Mar 2019 04:08
Operator : EI\SJ
Sample : PB117670TB
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB117670TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 04:47:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

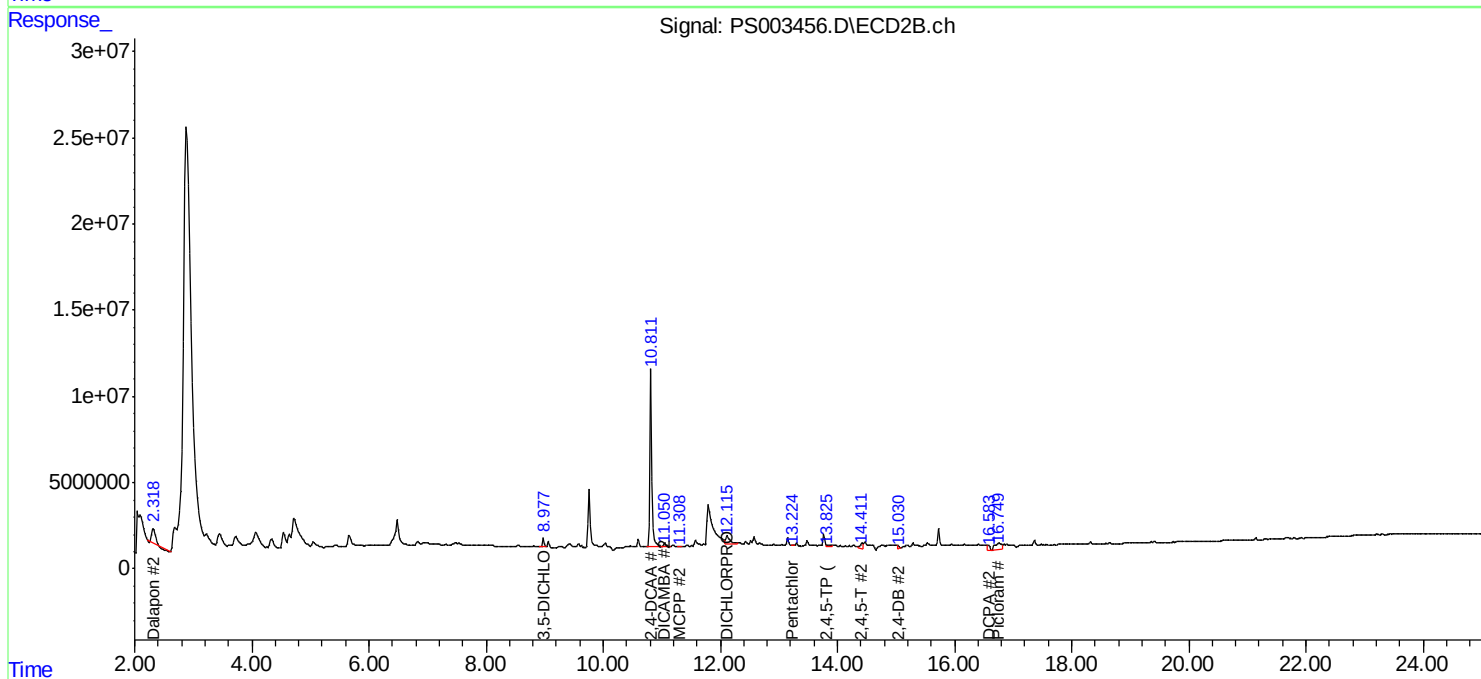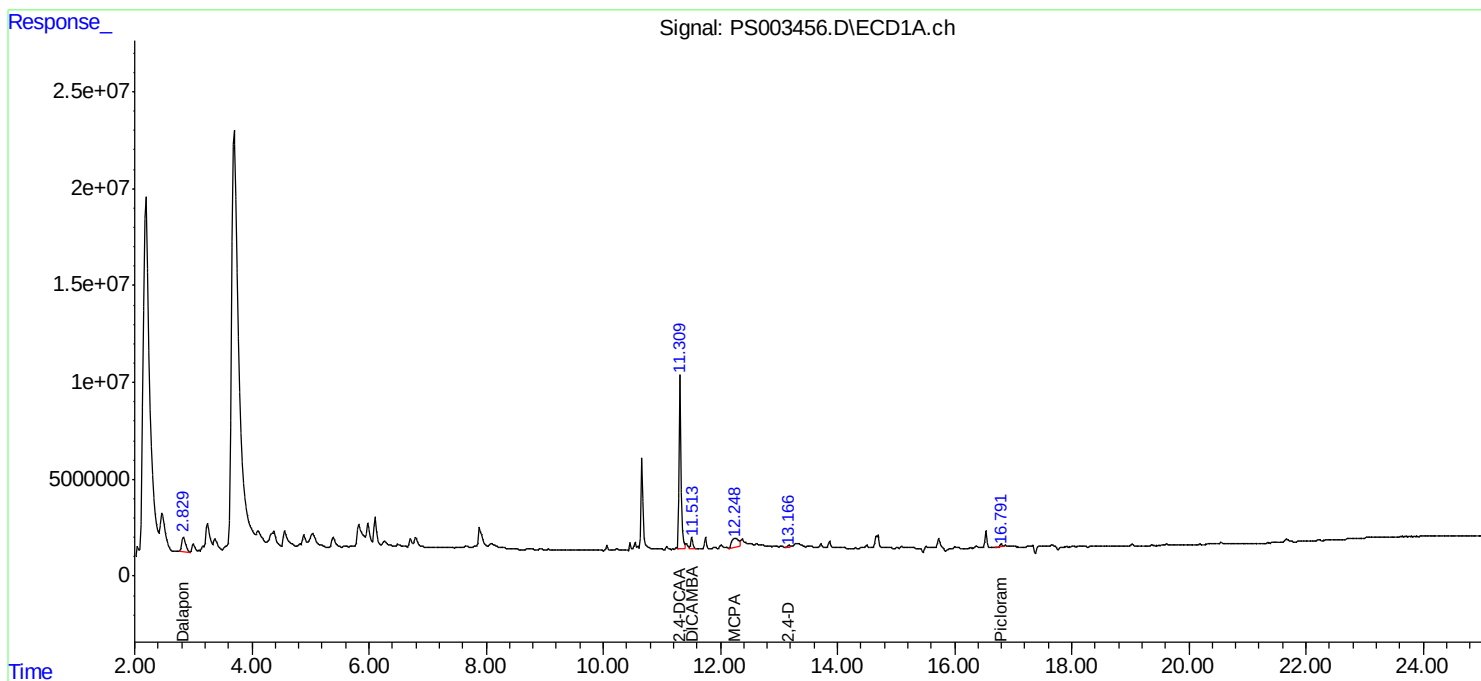


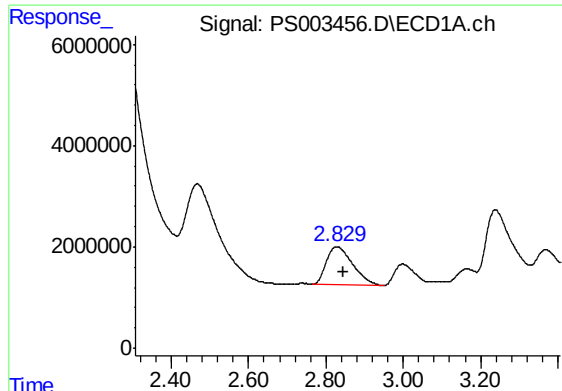

#1 Dalapon


R.T.: 2.828 min
Delta R.T.: -0.016 min
Response: 35888217
Conc: 55.22 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB117670TB

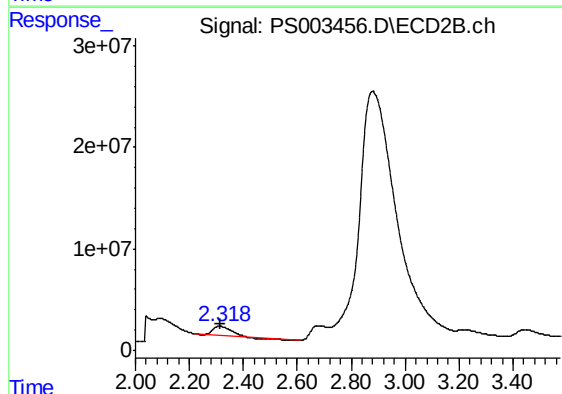


#1 Dalapon

R.T.: 2.314 min
Delta R.T.: -0.002 min
Response: 33194339
Conc: 52.42 ng/ml

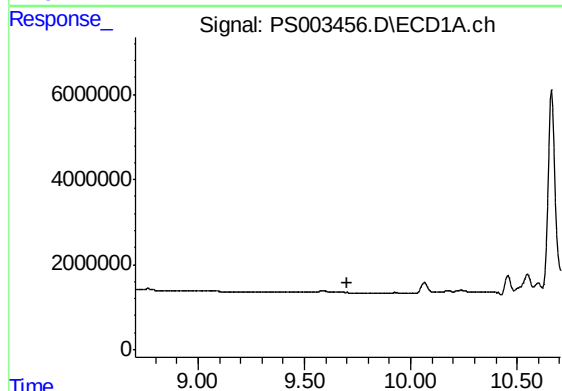


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.705 min
Response: 0
Conc: N.D.

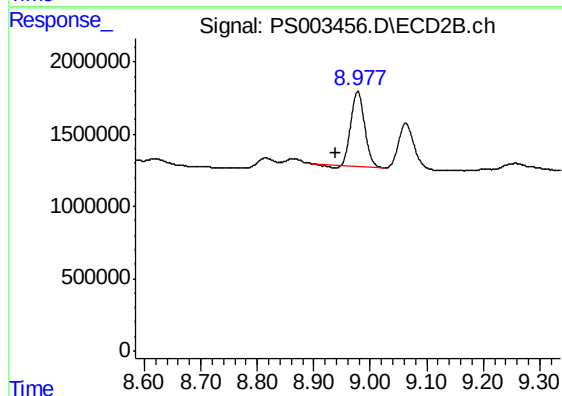

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.978 min
Delta R.T.: 0.038 min
Response: 8587636
Conc: 13.91 ng/ml

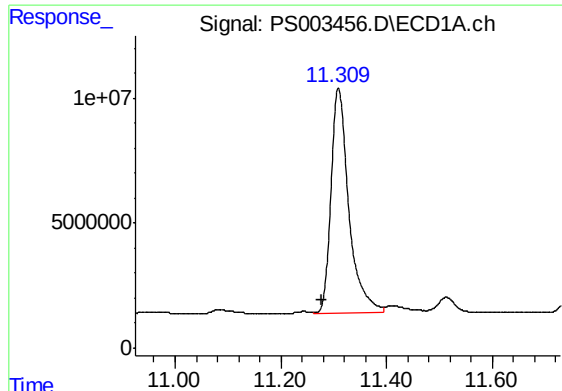

#4 2,4-DCAA


R.T.: 11.310 min
Delta R.T.: 0.032 min
Response: 211494383
Conc: 481.74 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB117670TB

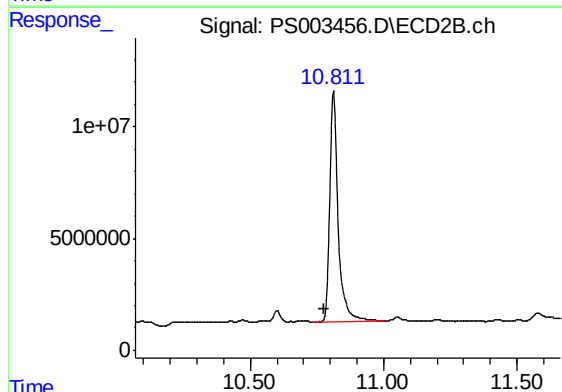


#4 2,4-DCAA

R.T.: 10.812 min
Delta R.T.: 0.032 min
Response: 226818707
Conc: 483.04 ng/ml

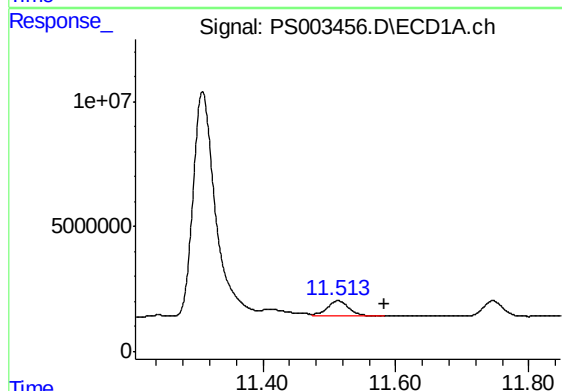


#5 DICAMBA

R.T.: 11.513 min
Delta R.T.: -0.069 min
Response: 14004268
Conc: 7.94 ng/ml

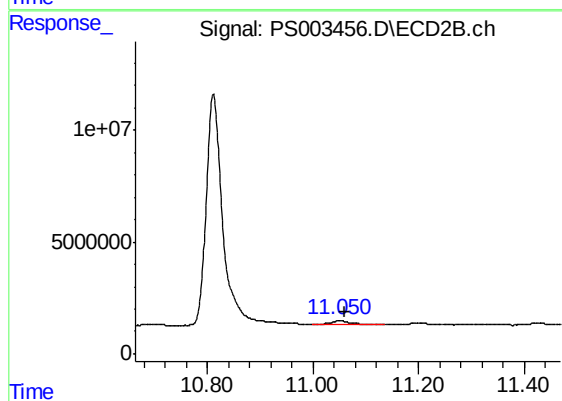

#5 DICAMBA


R.T.: 11.051 min
Delta R.T.: -0.008 min
Response: 4900174
Conc: 2.93 ng/ml

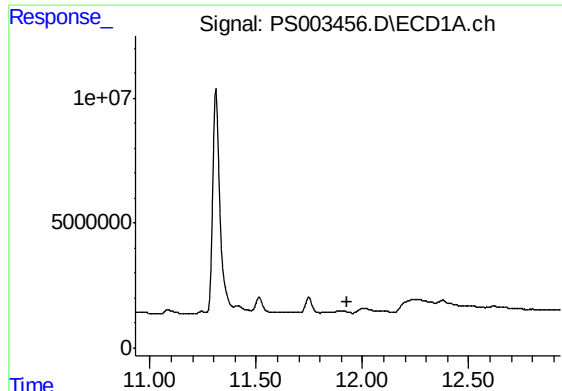

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 11.931 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB117670TB

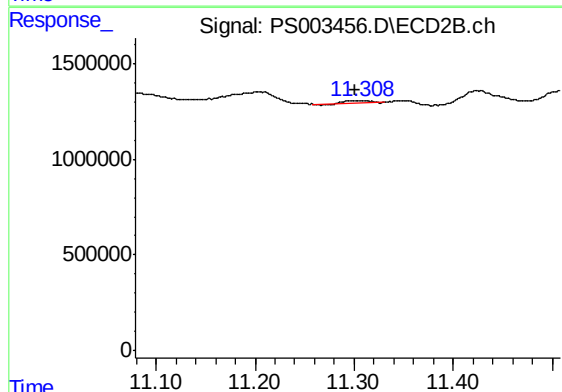


#6 MCPP

R.T.: 11.306 min
Delta R.T.: 0.005 min
Response: 161464
Conc: 0.14 ug/ml

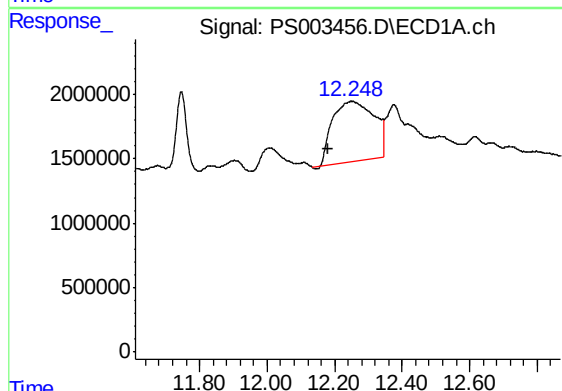


#7 MCPA

R.T.: 12.251 min
Delta R.T.: 0.068 min
Response: 39720695
Conc: 20.02 ug/ml

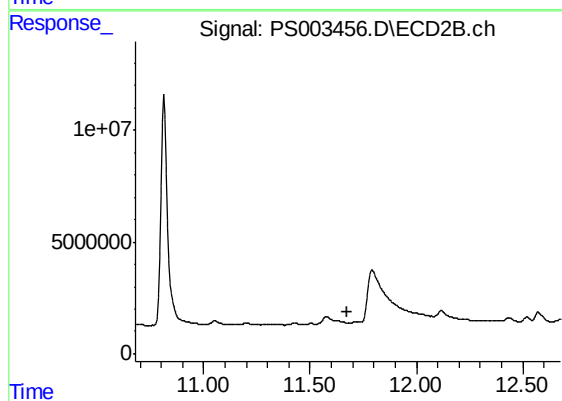

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 11.678 min
Response: 0
Conc: N.D.

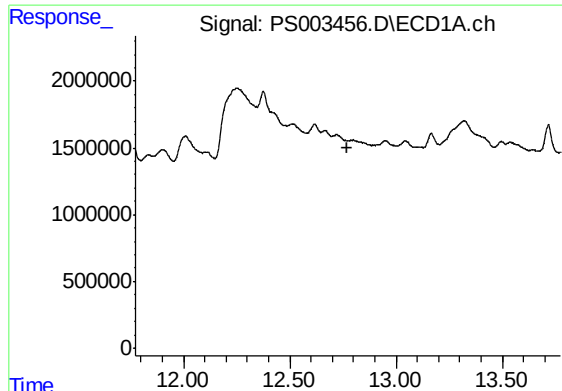

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.773 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB117670TB

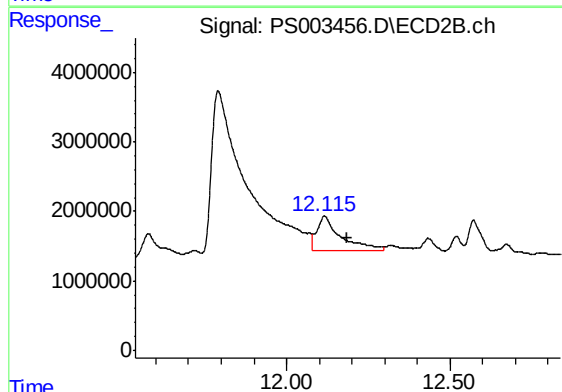


#8 DICHLORPROP

R.T.: 12.117 min
Delta R.T.: -0.068 min
Response: 25997883
Conc: 62.91 ng/ml

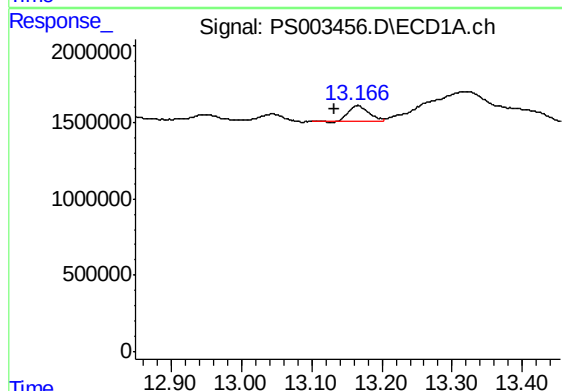


#9 2,4-D

R.T.: 13.166 min
Delta R.T.: 0.033 min
Response: 2042616
Conc: 4.40 ng/ml

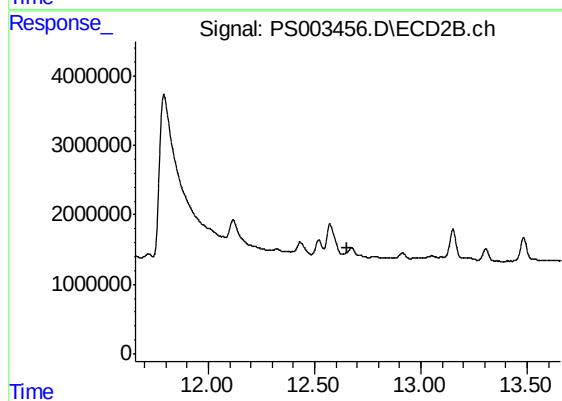

#9 2,4-D


R.T.: 12.672 min
Delta R.T.: 0.015 min
Response: -3990695
Conc: N.D.

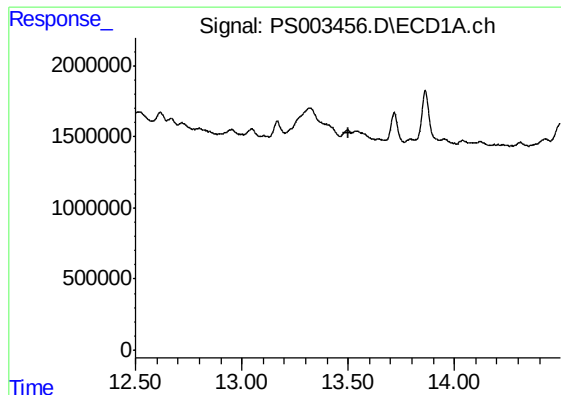

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.499 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB117670TB

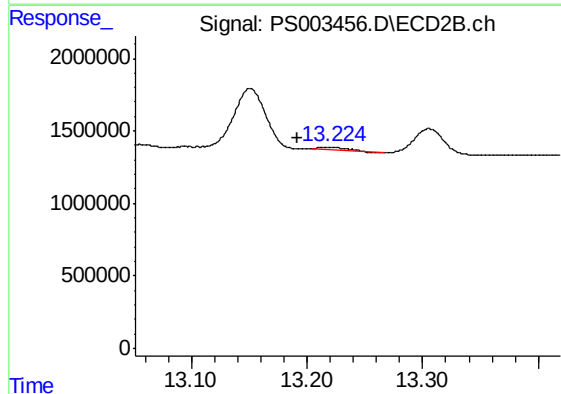


#10 Pentachlorophenol

R.T.: 13.220 min
Delta R.T.: 0.028 min
Response: 295015
Conc: 0.04 ng/ml

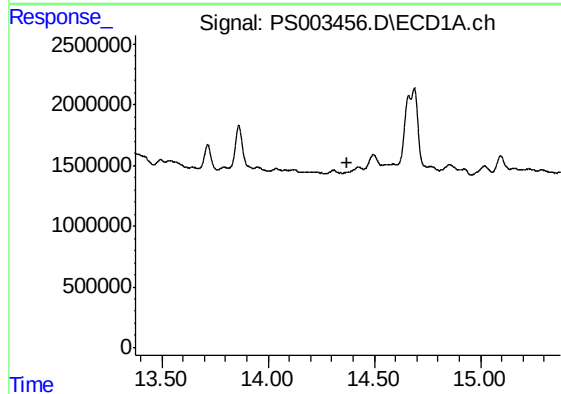


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

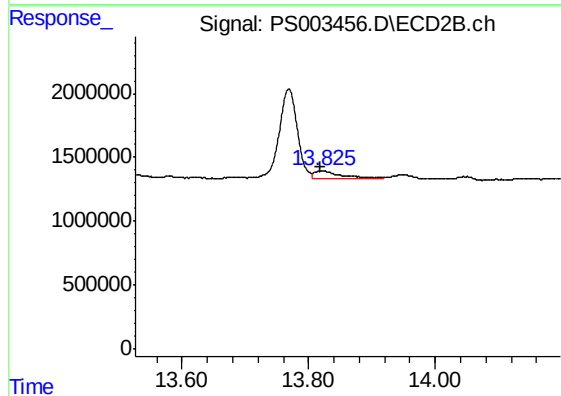

#11 2,4,5-TP (SILVEX)


R.T.: 13.823 min
Delta R.T.: 0.006 min
Response: 1869495
Conc: 0.73 ng/ml

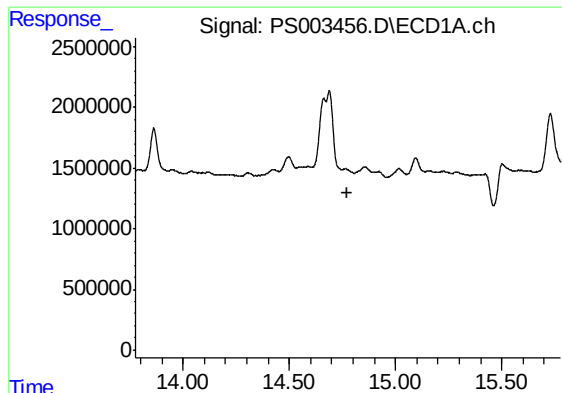

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB117670TB

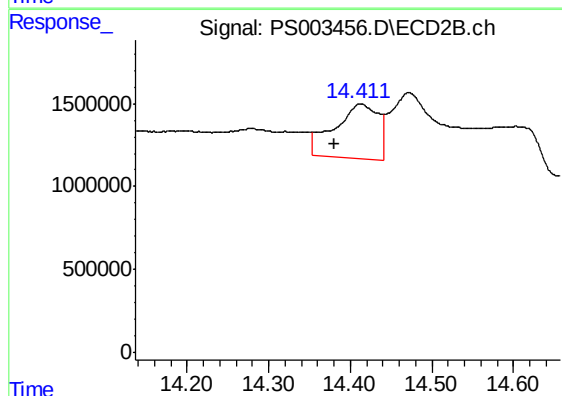


#12 2,4,5-T

R.T.: 14.413 min
Delta R.T.: 0.032 min
Response: 12282606
Conc: 6.09 ng/ml

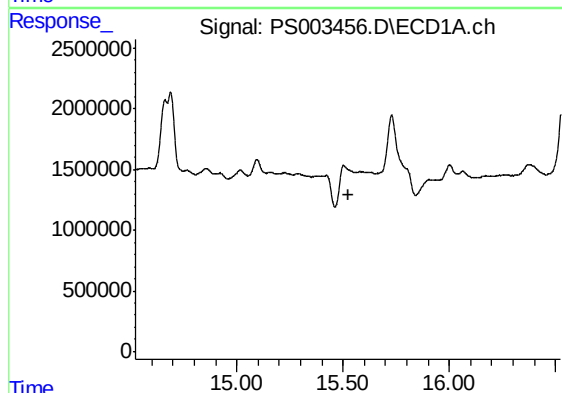


#13 2,4-DB

R.T.: 15.504 min
Delta R.T.: -0.019 min
Response: -4044422
Conc: N.D.

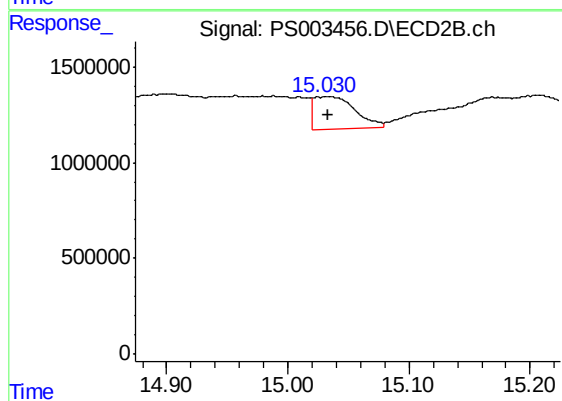

#13 2,4-DB


R.T.: 15.031 min
Delta R.T.: -0.002 min
Response: 3977523
Conc: 15.58 ng/ml

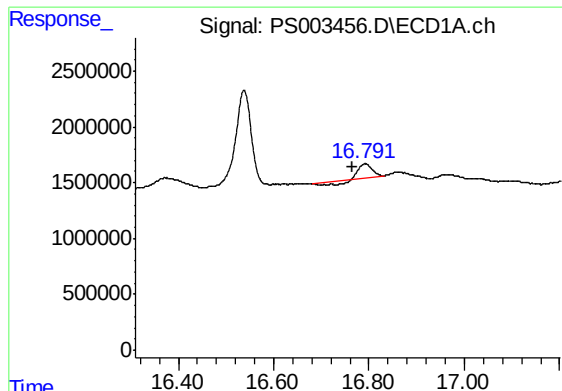

#15 Picloram


R.T.: 16.792 min
Delta R.T.: 0.027 min
Response: 1670438
Conc: 0.68 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB117670TB

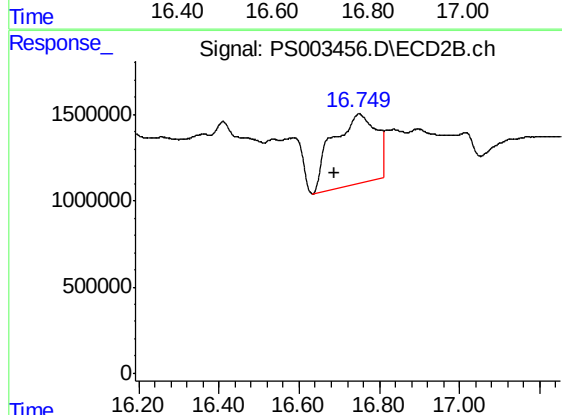


#15 Picloram

R.T.: 16.749 min
Delta R.T.: 0.061 min
Response: 30462294
Conc: 12.00 ng/ml

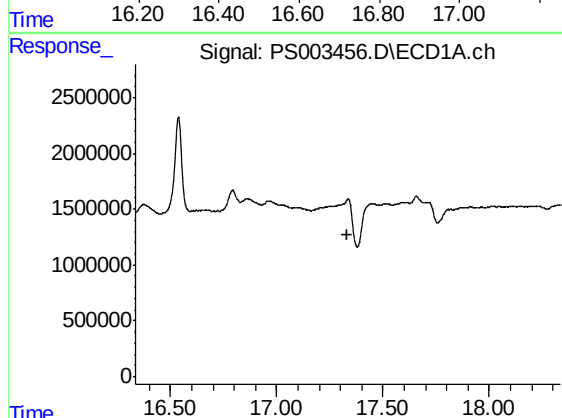

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.335 min
Response: 0
Conc: N.D.

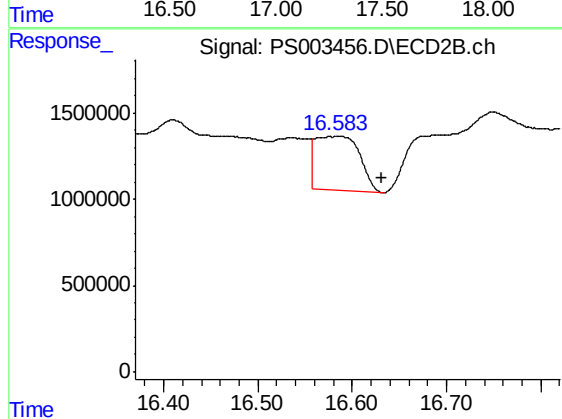

#16 DCPA

R.T.: 16.583 min
Delta R.T.: -0.049 min
Response: 9979070
Conc: 3.21 ng/ml