

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030619\
 Data File : PS003457.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Mar 2019 04:39
 Operator : EI\SJ
 Sample : K1707-02
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 S10

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 05:56:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.289	10.793	248.4E6	260.0E6	565.864	553.640
Target Compounds							
1) T	Dalapon	2.811	2.299	47894743	77893441	73.691	123.018 #
2) T	3,5-DICHL...	0.000	8.960	0	7765565	N.D.	12.577 #
5) T	DICAMBA	0.000	11.032	0	4906233	N.D.	2.937 #
6) T	MCP	11.978	11.279	633905	360059	0.483	0.305 #
7) T	MCPA	12.198	11.698	51695722	-445534	26.062	N.D. #
9) T	2,4-D	13.146	12.655	2926450	1958062	6.310	3.730 #
11) T	2,4,5-TP ...	0.000	13.804	0	1925698	N.D.	0.756 #
12) T	2,4,5-T	0.000	14.393	0	11344901	N.D.	5.625 #
13) T	2,4-DB	15.485	0.000	14966655	0	63.205	N.D. #
14) T	DINOSEB	0.000	15.513	0	10108383	N.D.	5.663 #
15) T	Picloram	16.770	16.731	3328382	28470258	1.352	11.217 #
16) T	DCPA	17.317	0.000	27171057	0	8.246	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030619\
Data File : PS003457.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Mar 2019 04:39
Operator : EI\SJ
Sample : K1707-02
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
S10

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 05:56:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

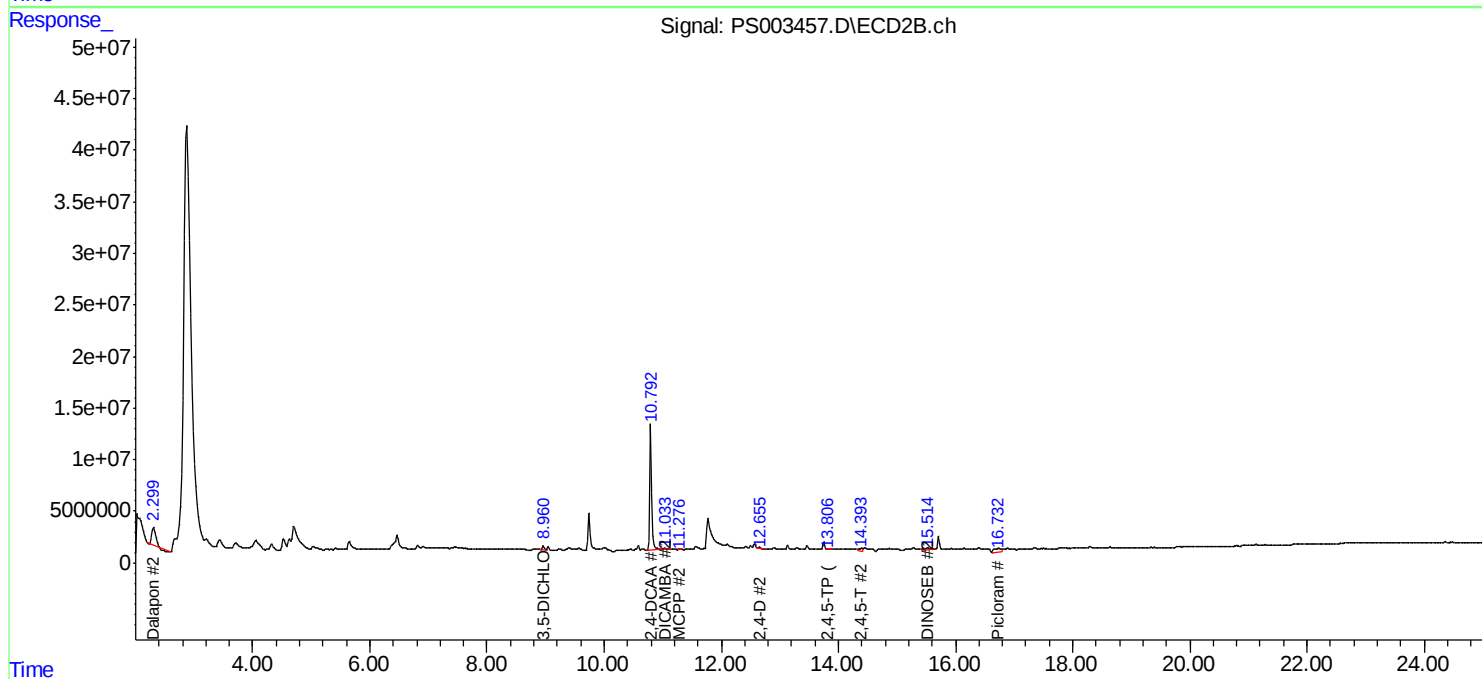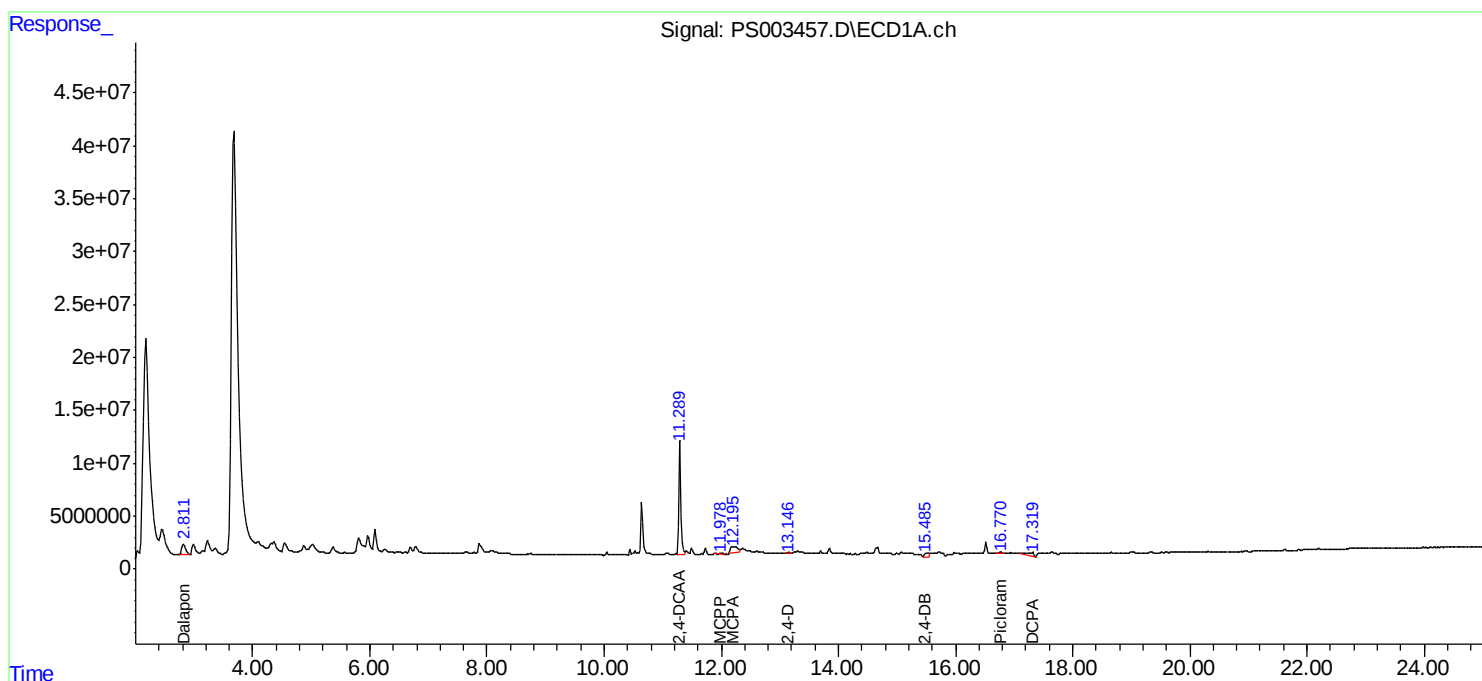


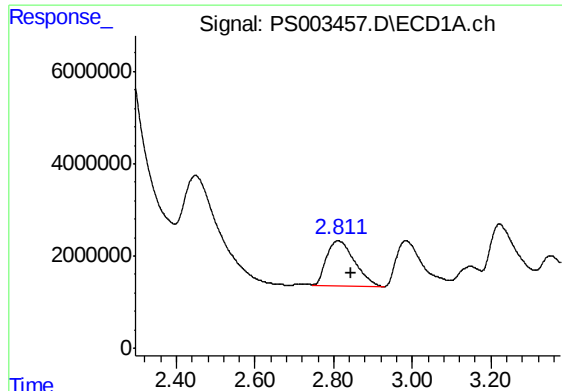

#1 Dalapon


R.T.: 2.811 min
Delta R.T.: -0.033 min
Response: 47894743
Conc: 73.69 ng/ml

Instrument :
ECD_S
ClientSampleId :
S10

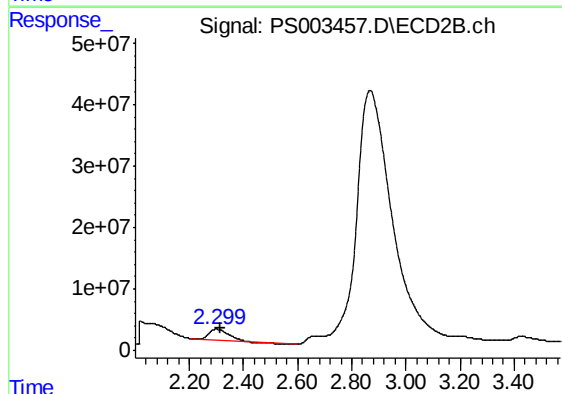


#1 Dalapon

R.T.: 2.299 min
Delta R.T.: -0.017 min
Response: 77893441
Conc: 123.02 ng/ml

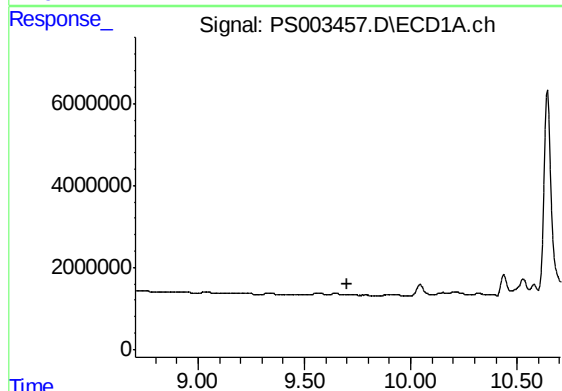


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.705 min
Response: 0
Conc: N.D.

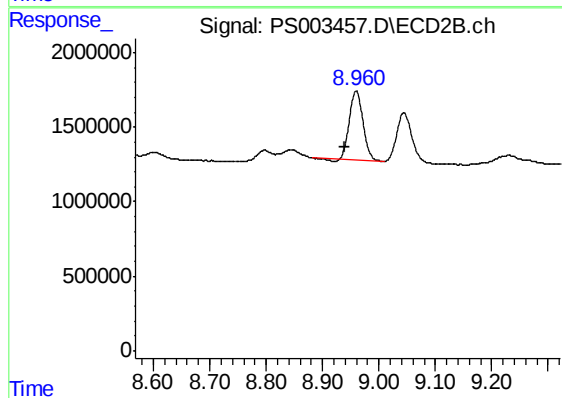

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.960 min
Delta R.T.: 0.020 min
Response: 7765565
Conc: 12.58 ng/ml

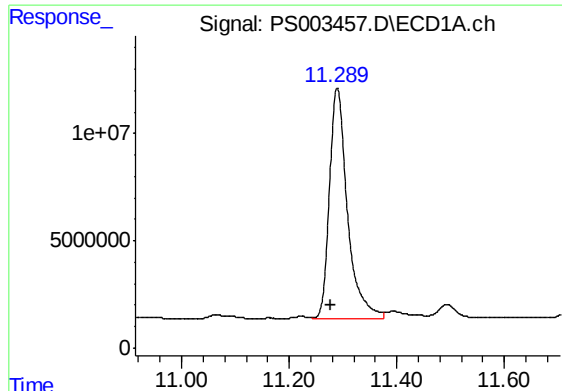

#4 2,4-DCAA


R.T.: 11.289 min
Delta R.T.: 0.012 min
Response: 248427935
Conc: 565.86 ng/ml

Instrument :
ECD_S
ClientSampleId :
S10

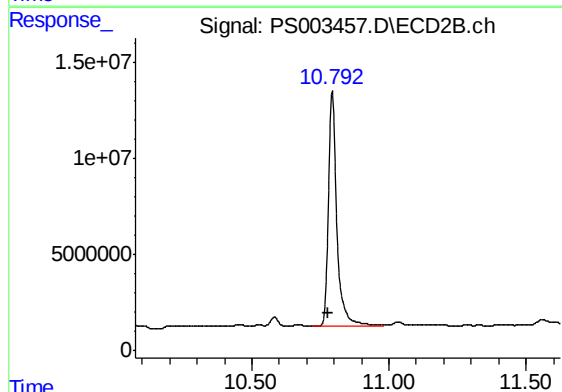


#4 2,4-DCAA

R.T.: 10.793 min
Delta R.T.: 0.013 min
Response: 259972487
Conc: 553.64 ng/ml

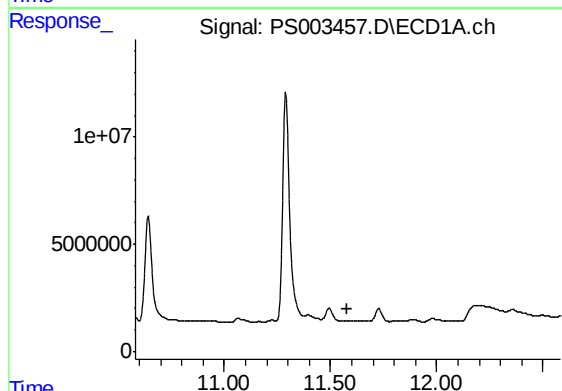


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.582 min
Response: 0
Conc: N.D.

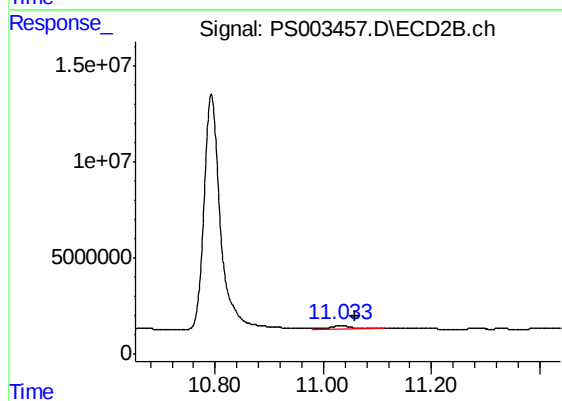

#5 DICAMBA


R.T.: 11.032 min
Delta R.T.: -0.027 min
Response: 4906233
Conc: 2.94 ng/ml

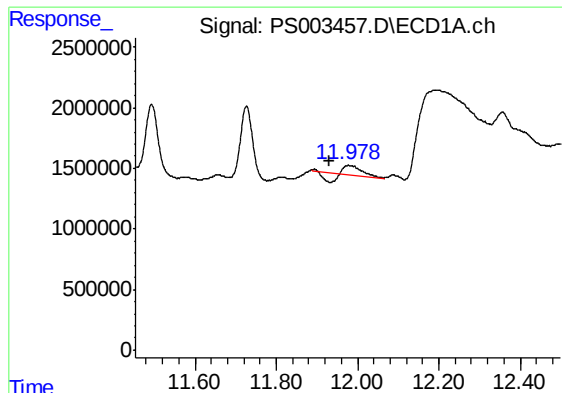

#6 MCPP


R.T.: 11.978 min
Delta R.T.: 0.047 min
Response: 633905
Conc: 0.48 ug/ml

Instrument :
ECD_S
ClientSampleId :
S10

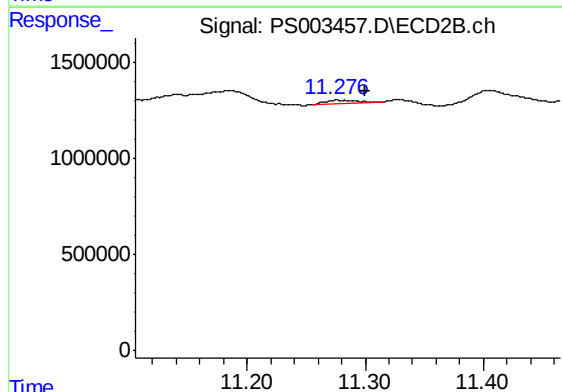


#6 MCPP

R.T.: 11.279 min
Delta R.T.: -0.021 min
Response: 360059
Conc: 0.31 ug/ml

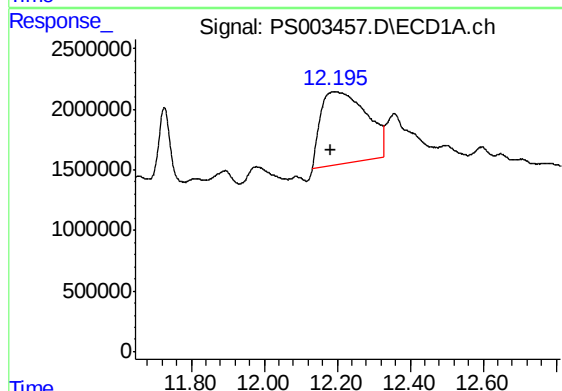


#7 MCPA

R.T.: 12.198 min
Delta R.T.: 0.015 min
Response: 51695722
Conc: 26.06 ug/ml

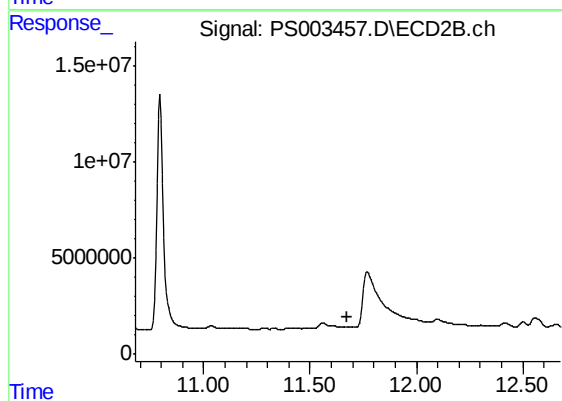

#7 MCPA


R.T.: 11.698 min
Delta R.T.: 0.021 min
Response: -445534
Conc: N.D.

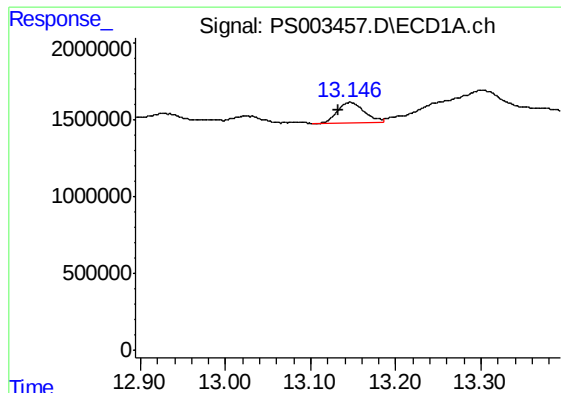

#9 2,4-D


R.T.: 13.146 min
Delta R.T.: 0.014 min
Response: 2926450
Conc: 6.31 ng/ml

Instrument :
ECD_S
ClientSampleId :
S10

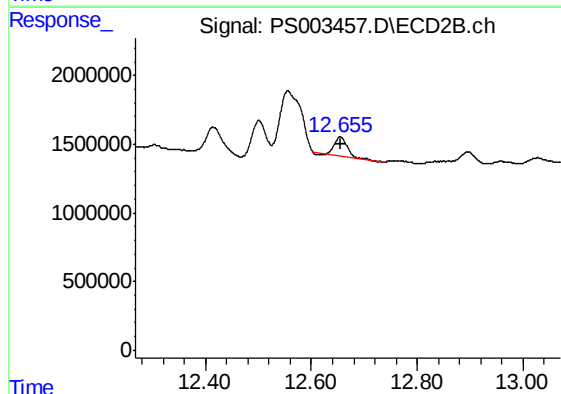


#9 2,4-D

R.T.: 12.655 min
Delta R.T.: -0.002 min
Response: 1958062
Conc: 3.73 ng/ml

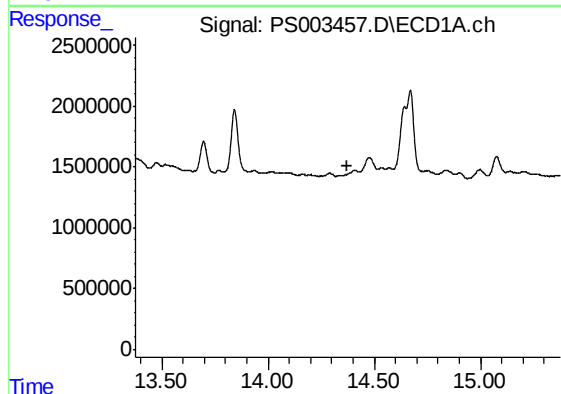


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.376 min
Response: 0
Conc: N.D.

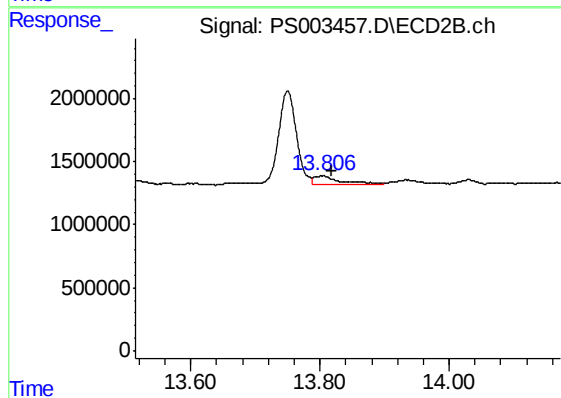

#11 2,4,5-TP (SILVEX)


R.T.: 13.804 min
Delta R.T.: -0.014 min
Response: 1925698
Conc: 0.76 ng/ml

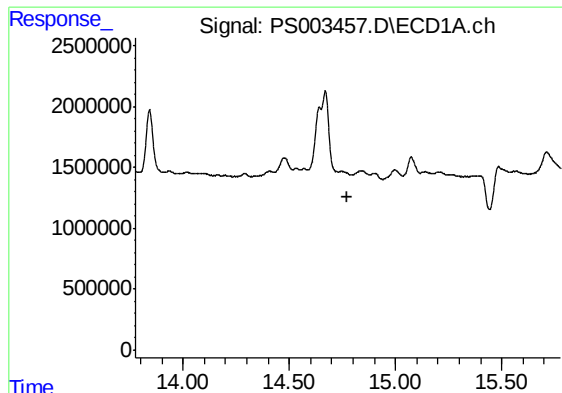

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 14.776 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
S10

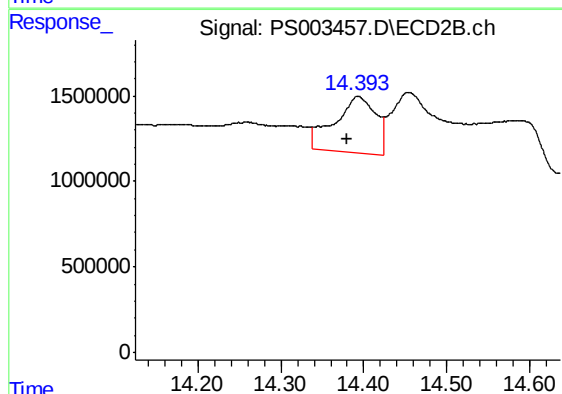


#12 2,4,5-T

R.T.: 14.393 min
Delta R.T.: 0.013 min
Response: 11344901
Conc: 5.63 ng/ml

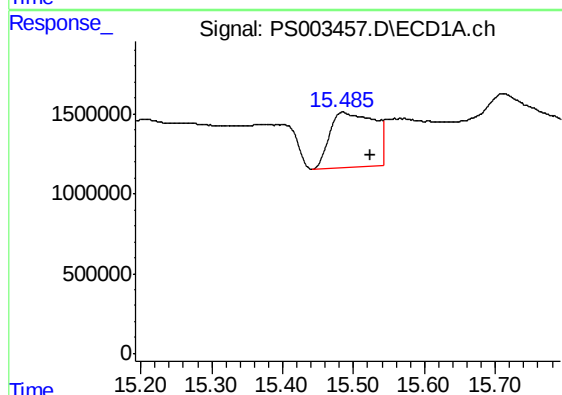


#13 2,4-DB

R.T.: 15.485 min
Delta R.T.: -0.038 min
Response: 14966655
Conc: 63.20 ng/ml

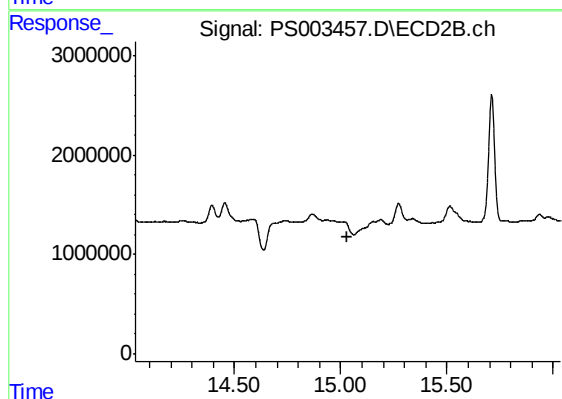

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 15.033 min
Response: 0
Conc: N.D.

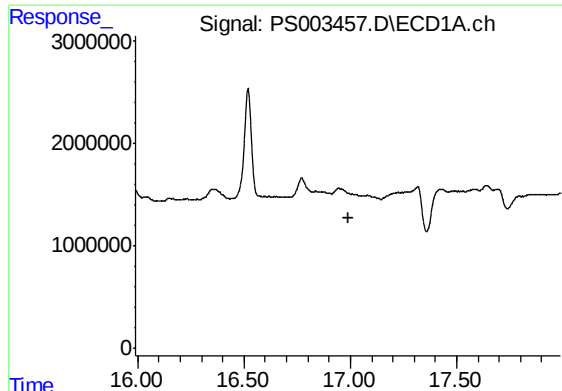

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
S10

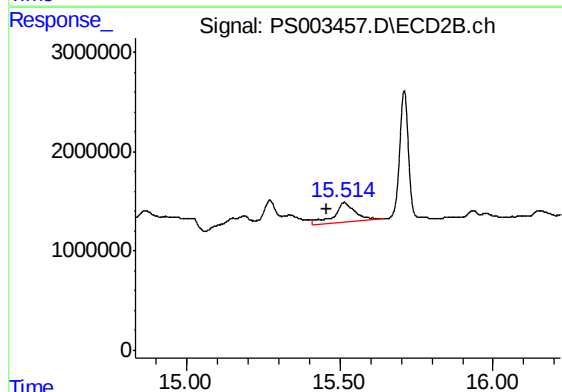


#14 DINOSEB

R.T.: 15.513 min
Delta R.T.: 0.056 min
Response: 10108383
Conc: 5.66 ng/ml

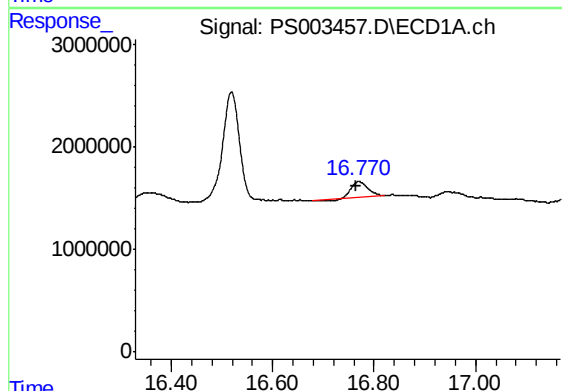


#15 Picloram

R.T.: 16.770 min
Delta R.T.: 0.005 min
Response: 3328382
Conc: 1.35 ng/ml

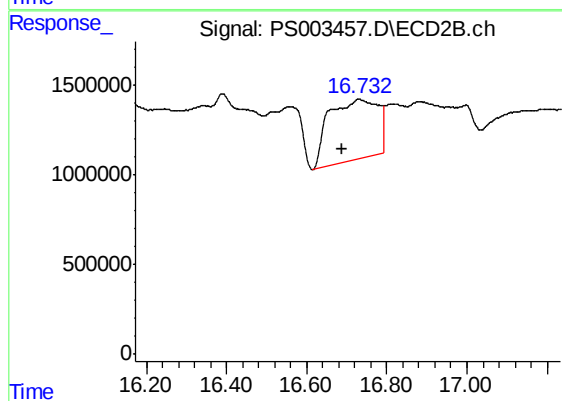

#15 Picloram


R.T.: 16.731 min
Delta R.T.: 0.043 min
Response: 28470258
Conc: 11.22 ng/ml

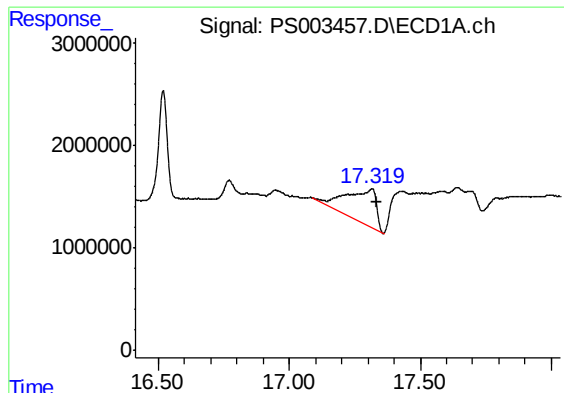

#16 DCPA

R.T.: 17.317 min
Delta R.T.: -0.018 min
Response: 27171057
Conc: 8.25 ng/ml

Instrument :
ECD_S
ClientSampleId :
S10

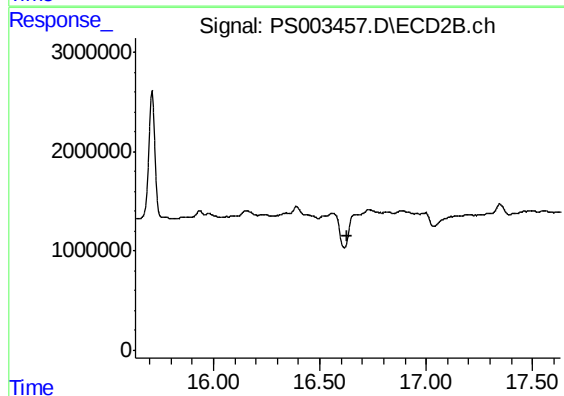

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 16.632 min
Response: 0
Conc: N.D.