

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030619\
 Data File : PS003461.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Mar 2019 06:43
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 07:29:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.295	10.795	226.1E6	215.8E6	515.087	459.675
Target Compounds							
1) T	Dalapon	0.000	2.348	0	490	N.D.	0.001 #
7) T	MCPA	0.000	11.683	0	284138	N.D.	0.165 #
8) T	DICHLORPROP	0.000	12.178	0	167518	N.D.	0.405 #
10) T	Pentachlo...	0.000	13.210	0	1052365	N.D.	0.160 #
11) T	2,4,5-TP ...	0.000	13.811	0	57299	N.D.	0.023 #
12) T	2,4,5-T	0.000	14.357	0	27090	N.D.	0.013 #
14) T	DINOSEB	0.000	15.486	0	299827	N.D.	0.168 #
15) T	Picloram	0.000	16.716	0	17319	N.D.	0.007 #
16) T	DCPA	0.000	16.647	0	563599	N.D.	0.181 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030619\
Data File : PS003461.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Mar 2019 06:43
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 07:29:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

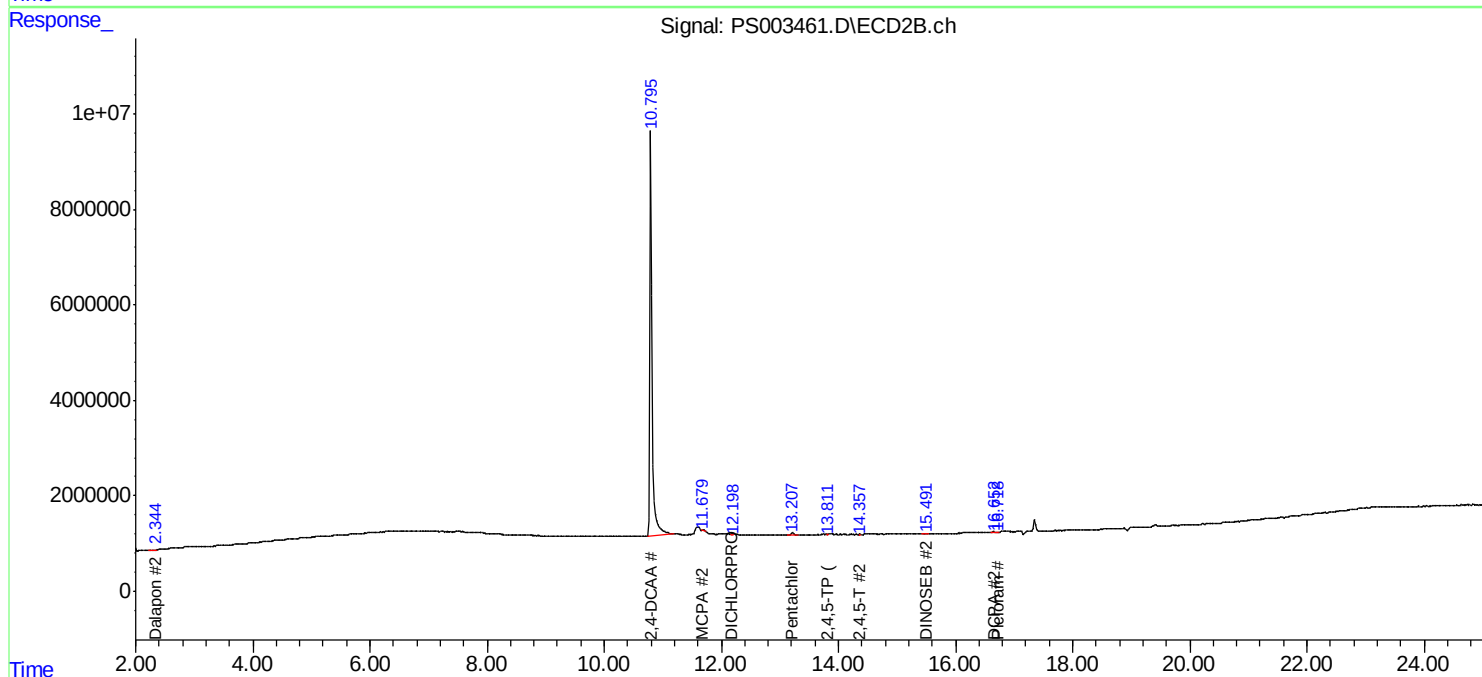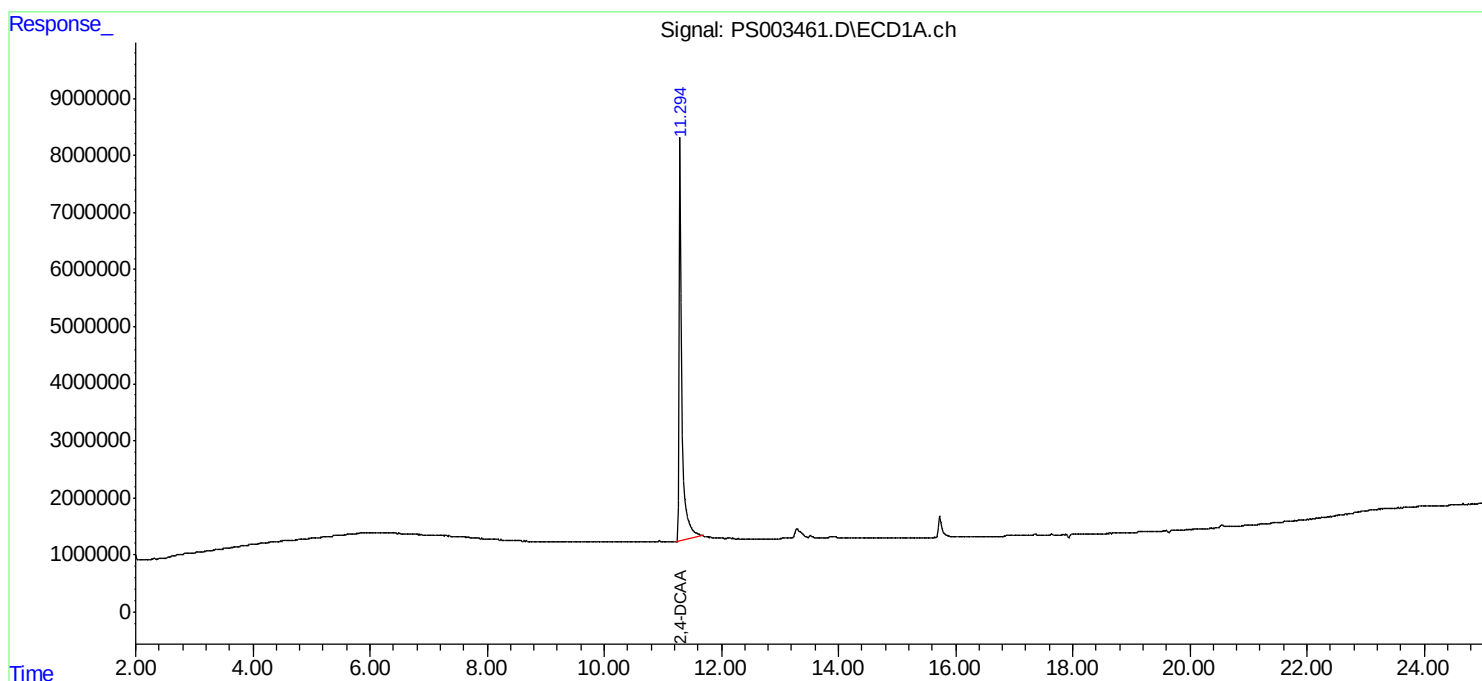


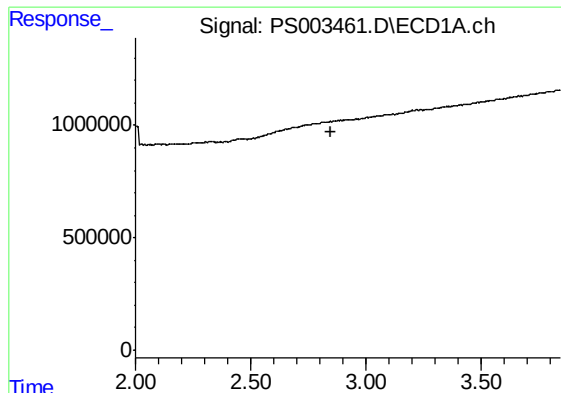

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.844 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

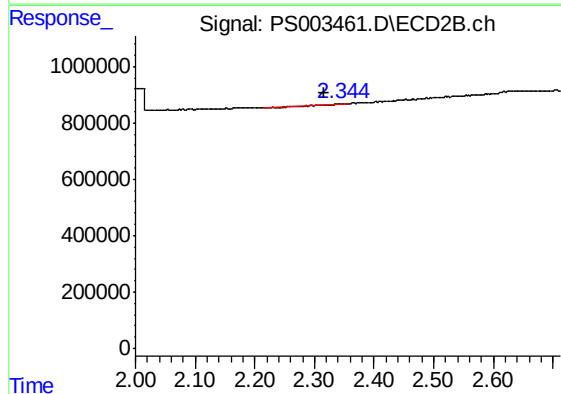


#1 Dalapon

R.T.: 2.348 min
Delta R.T.: 0.031 min
Response: 490
Conc: 0.00 ng/ml

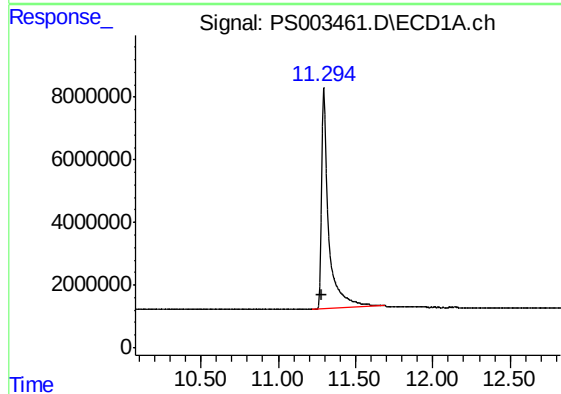


#4 2,4-DCAA

R.T.: 11.295 min
Delta R.T.: 0.017 min
Response: 226135941
Conc: 515.09 ng/ml

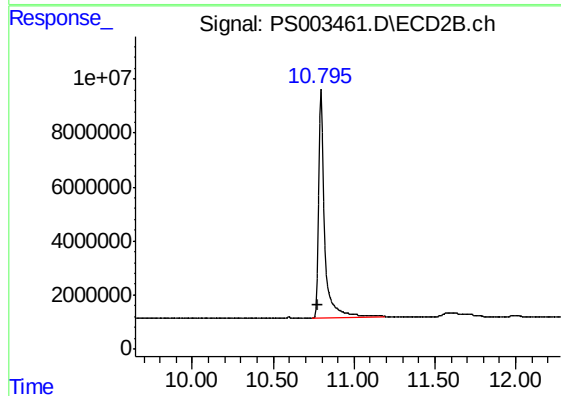

#4 2,4-DCAA


R.T.: 10.795 min
Delta R.T.: 0.015 min
Response: 215848993
Conc: 459.67 ng/ml

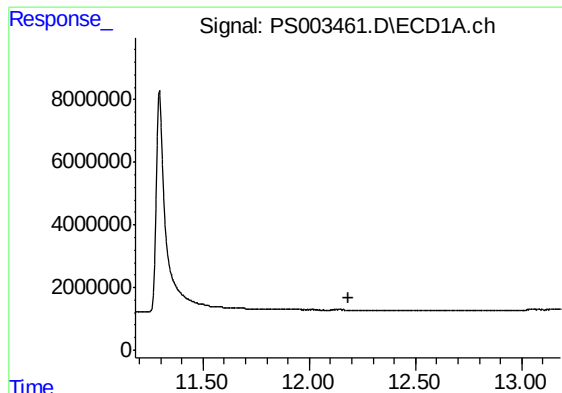

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 12.182 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

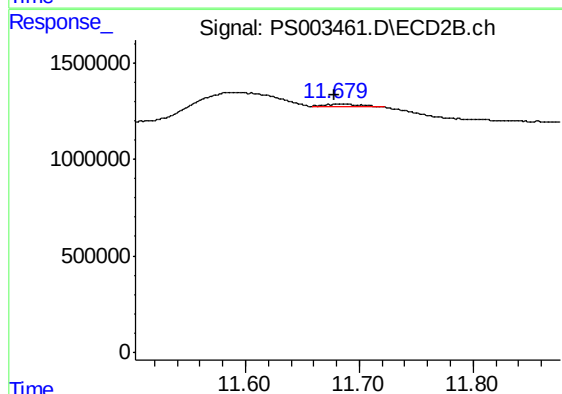


#7 MCPA

R.T.: 11.683 min
Delta R.T.: 0.005 min
Response: 284138
Conc: 0.16 ug/ml

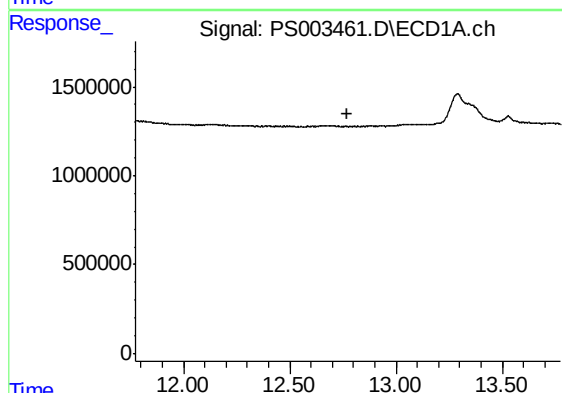


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.773 min
Response: 0
Conc: N.D.

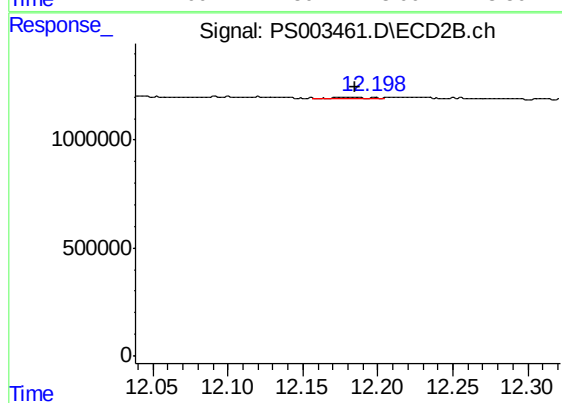

#8 DICHLORPROP


R.T.: 12.178 min
Delta R.T.: -0.007 min
Response: 167518
Conc: 0.41 ng/ml

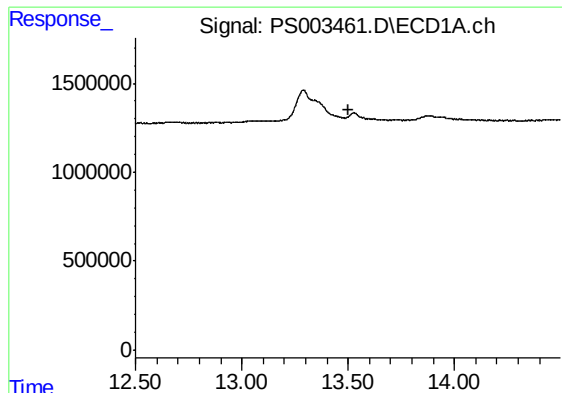

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 13.499 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

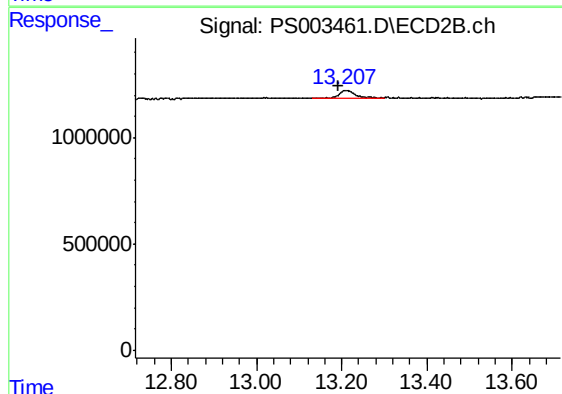


#10 Pentachlorophenol

R.T.: 13.210 min
Delta R.T.: 0.019 min
Response: 1052365
Conc: 0.16 ng/ml

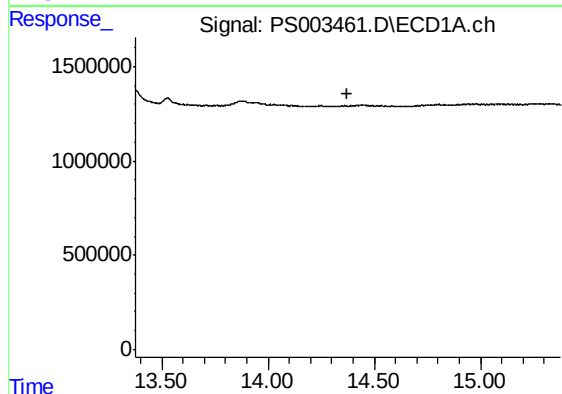


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.376 min
Response: 0
Conc: N.D.

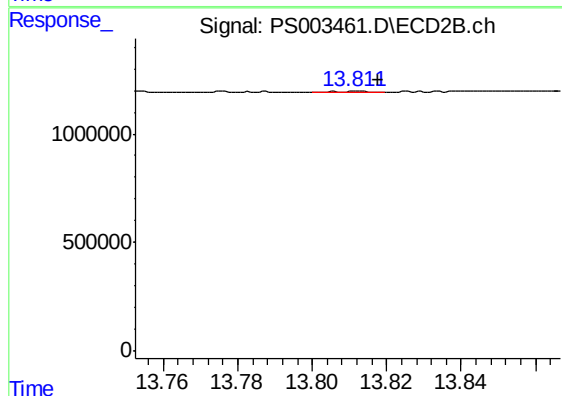

#11 2,4,5-TP (SILVEX)


R.T.: 13.811 min
Delta R.T.: -0.007 min
Response: 57299
Conc: 0.02 ng/ml

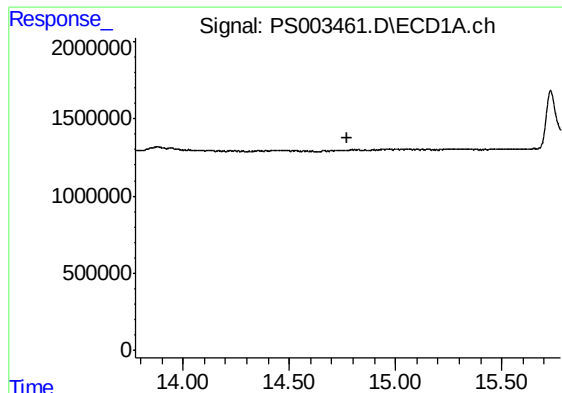

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 14.776 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

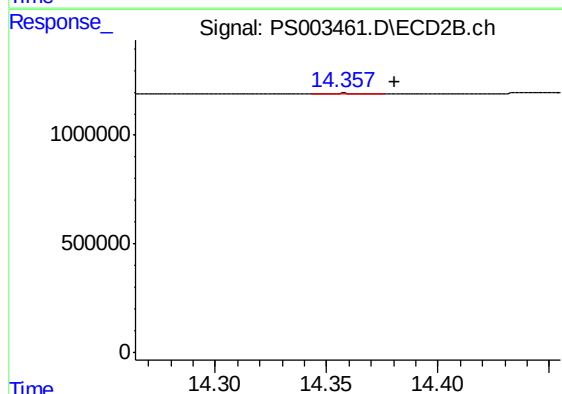


#12 2,4,5-T

R.T.: 14.357 min
Delta R.T.: -0.023 min
Response: 27090
Conc: 0.01 ng/ml

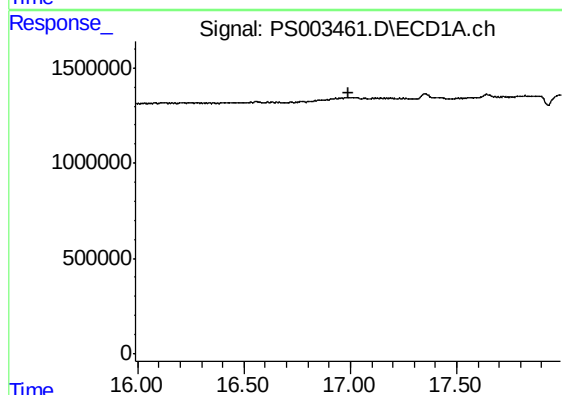


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 16.989 min
Response: 0
Conc: N.D.

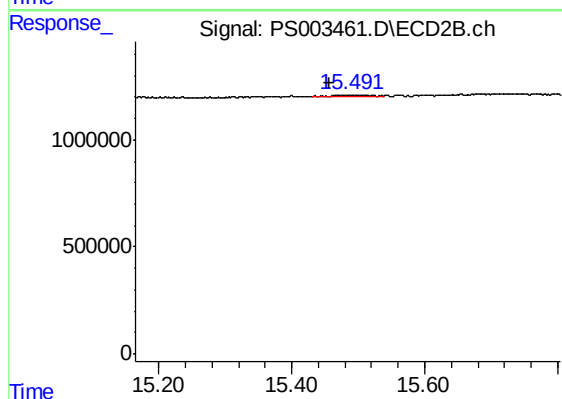

#14 DINOSEB


R.T.: 15.486 min
Delta R.T.: 0.029 min
Response: 299827
Conc: 0.17 ng/ml

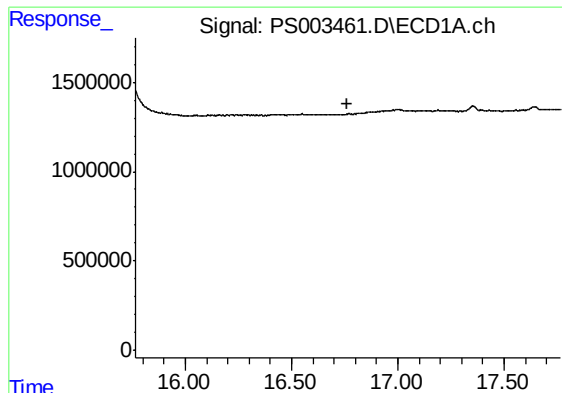

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 16.765 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

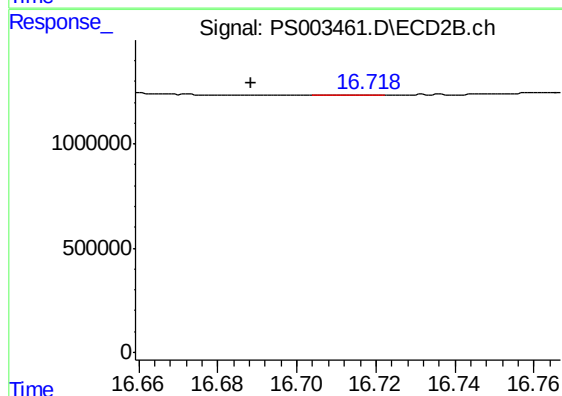


#15 Picloram

R.T.: 16.716 min
Delta R.T.: 0.027 min
Response: 17319
Conc: 0.01 ng/ml

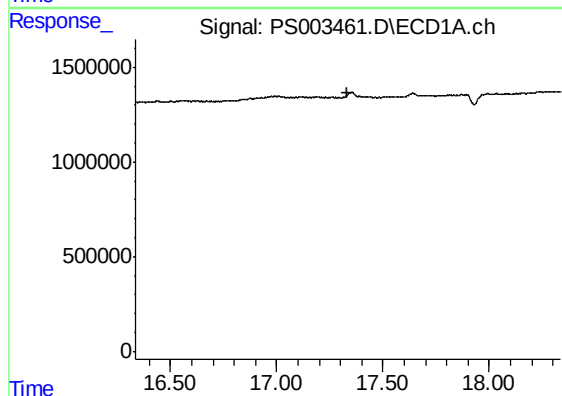

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.335 min
Response: 0
Conc: N.D.

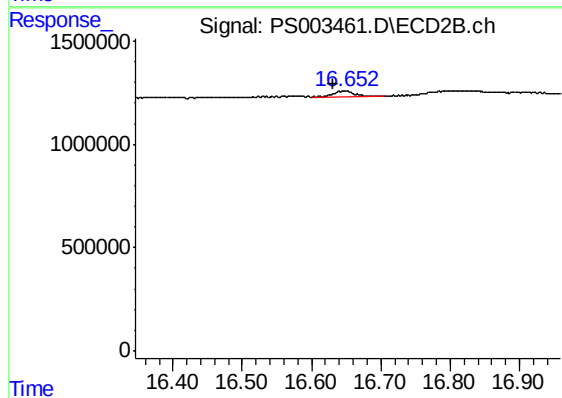

#16 DCPA

R.T.: 16.647 min
Delta R.T.: 0.015 min
Response: 563599
Conc: 0.18 ng/ml