

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030620\
 Data File : PS009137.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Mar 2020 10:45
 Operator : DD\AJ
 Sample : PB127286BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB127286BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 06 15:17:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.249	6.936	1020.8E6	512.0E6	466.841	531.405
Target Compounds							
1) T	Dalapon	0.000	2.585	0	235.3E6	N.D.	160.895
2) T	3,5-DICHL...	0.000	6.111	0	148.7E6	N.D.	101.898
7) T	MCPA	7.801	7.404	226.6E6	143.0E6	28.176	32.328
8) T	DICHLORPROP	0.000	7.757	0	72880922	N.D.	72.740
11) T	2,4,5-TP ...	0.000	8.792	0	71584690	N.D.	13.215
12) T	2,4,5-T	0.000	9.257	0	65968696	N.D.	12.187
14) T	DINOSEB	0.000	10.058	0	16096470	N.D.	4.071
15) T	Picloram	11.047	11.028	185.6E6	172.0E6	13.554	23.671 #
16) T	DCPA	0.000	11.028	0	172.0E6	N.D.	24.859



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030620\
Data File : PS009137.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2020 10:45
Operator : DD\AJ
Sample : PB127286BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB127286BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 06 15:17:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

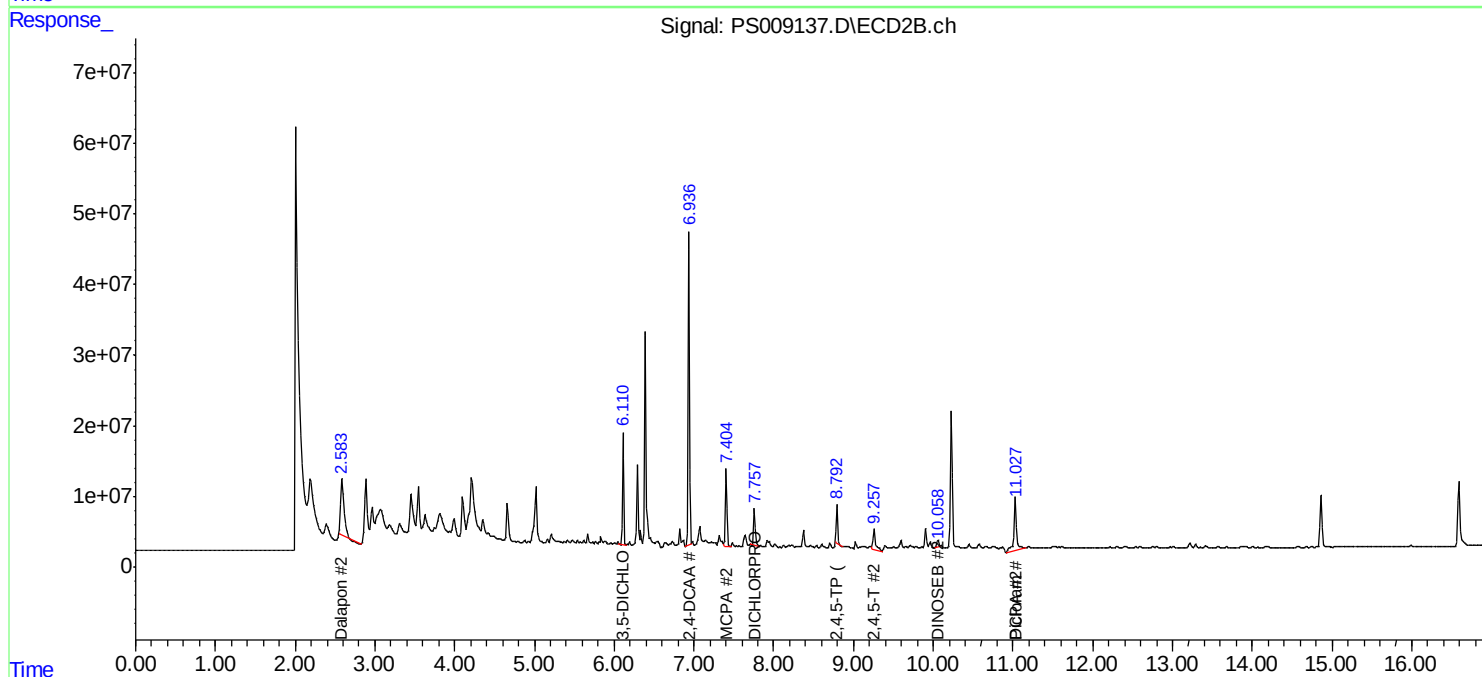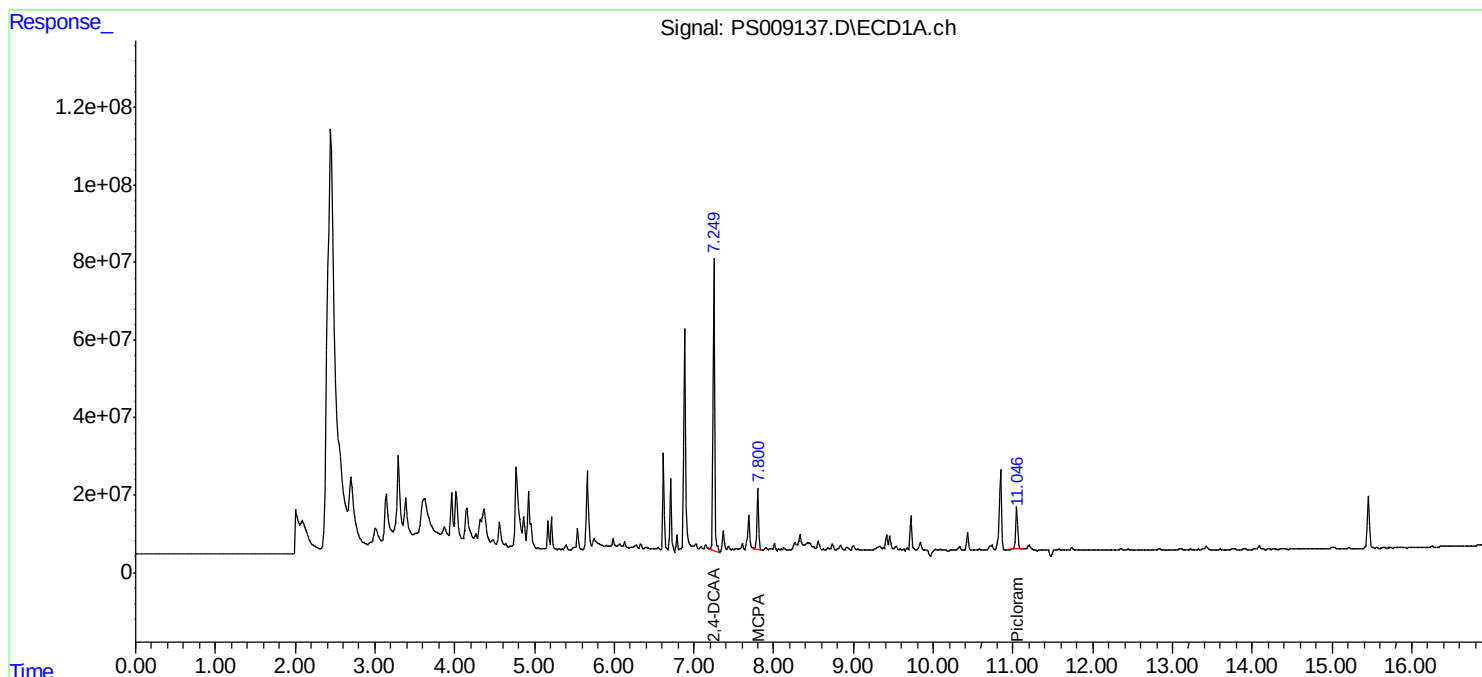


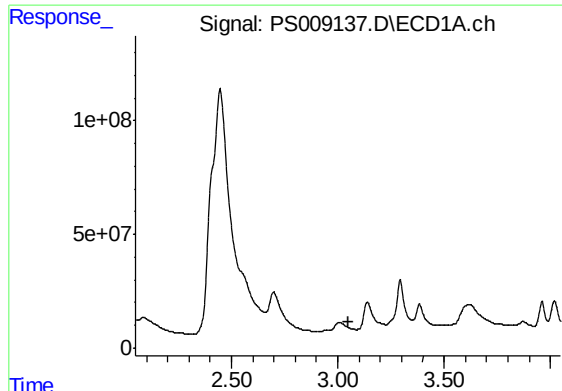

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 3.048 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB127286BL

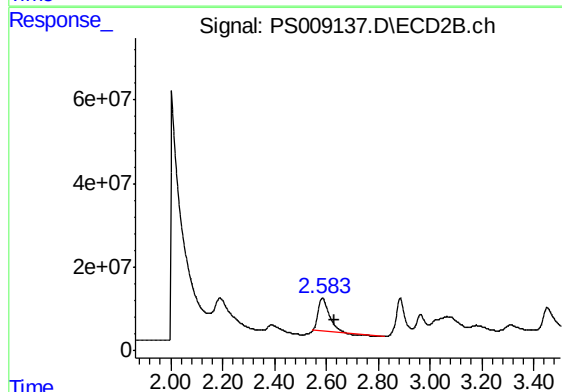


#1 Dalapon

R.T.: 2.585 min
Delta R.T.: -0.045 min
Response: 235264104
Conc: 160.90 ng/ml

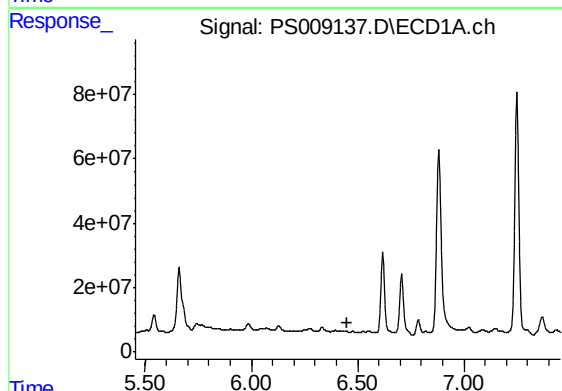


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.455 min
Response: 0
Conc: N.D.

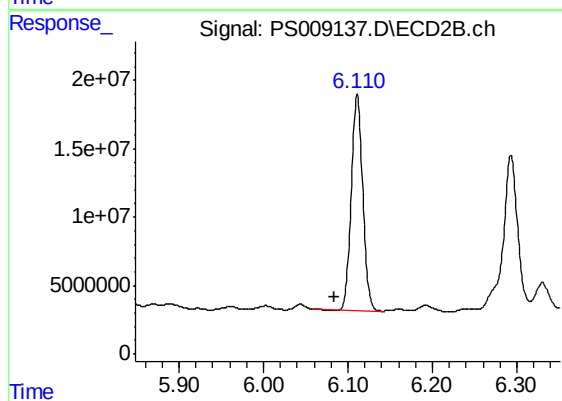

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.111 min
Delta R.T.: 0.028 min
Response: 148697370
Conc: 101.90 ng/ml

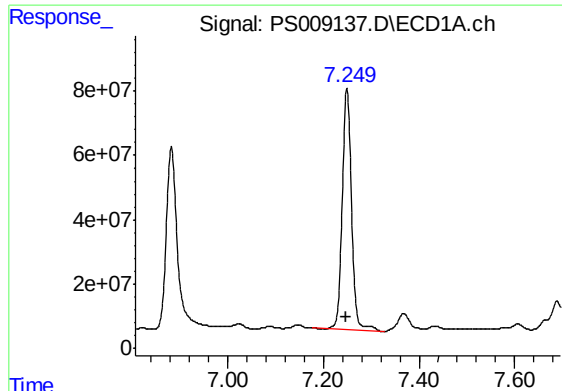

#4 2,4-DCAA


R.T.: 7.249 min
Delta R.T.: 0.002 min
Response: 1020791791
Conc: 466.84 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB127286BL

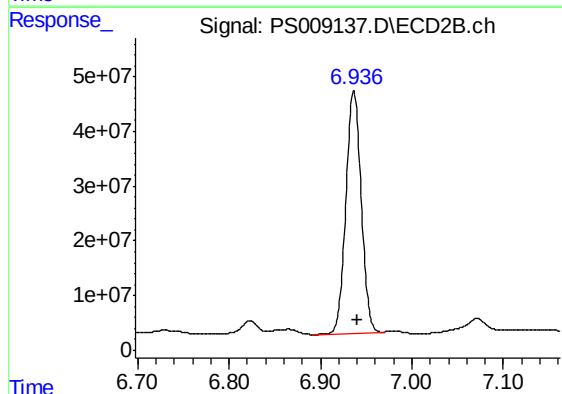


#4 2,4-DCAA

R.T.: 6.936 min
Delta R.T.: -0.004 min
Response: 512038260
Conc: 531.41 ng/ml

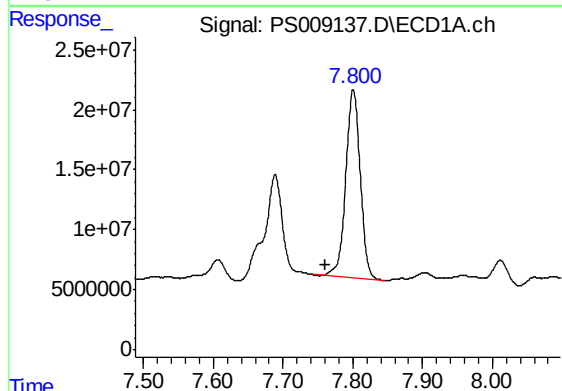


#7 MCPA

R.T.: 7.801 min
Delta R.T.: 0.040 min
Response: 226649107
Conc: 28.18 ug/ml

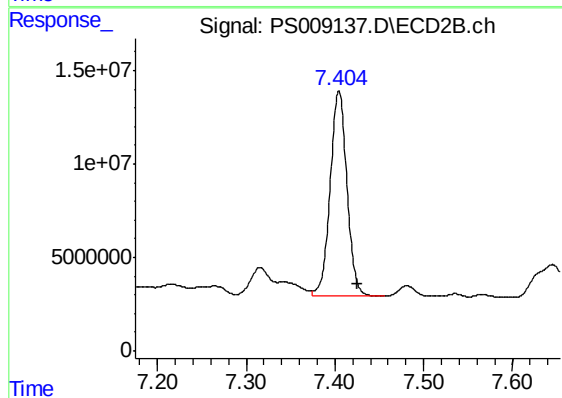

#7 MCPA


R.T.: 7.404 min
Delta R.T.: -0.021 min
Response: 143027421
Conc: 32.33 ug/ml

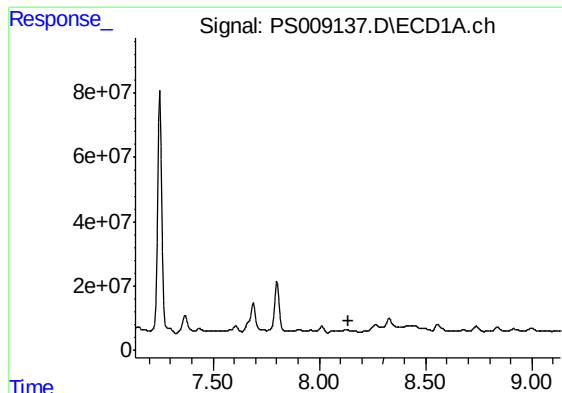

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 8.135 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB127286BL

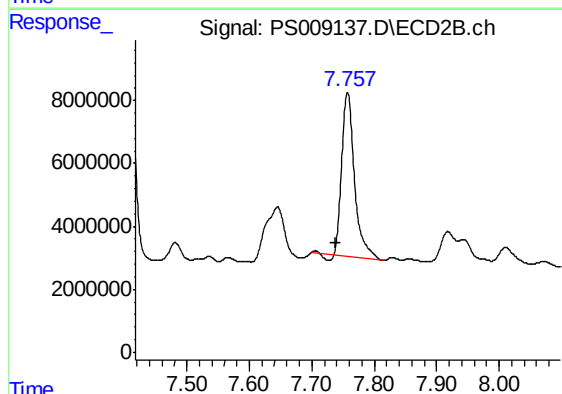


#8 DICHLORPROP

R.T.: 7.757 min
Delta R.T.: 0.018 min
Response: 72880922
Conc: 72.74 ng/ml

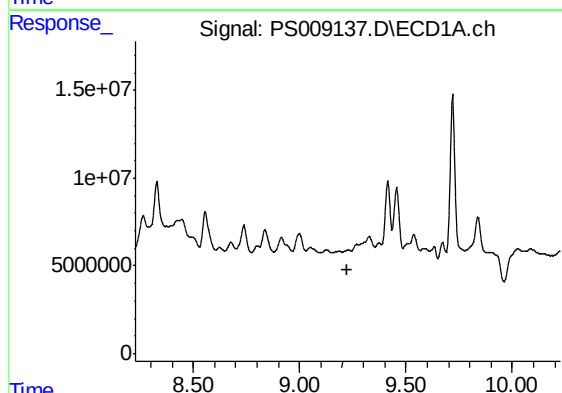


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.227 min
Response: 0
Conc: N.D.

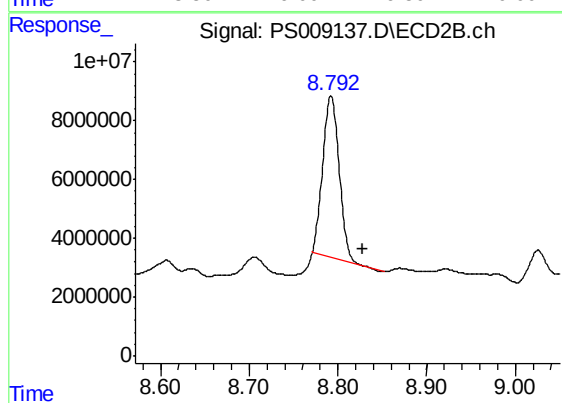

#11 2,4,5-TP (SILVEX)


R.T.: 8.792 min
Delta R.T.: -0.036 min
Response: 71584690
Conc: 13.22 ng/ml

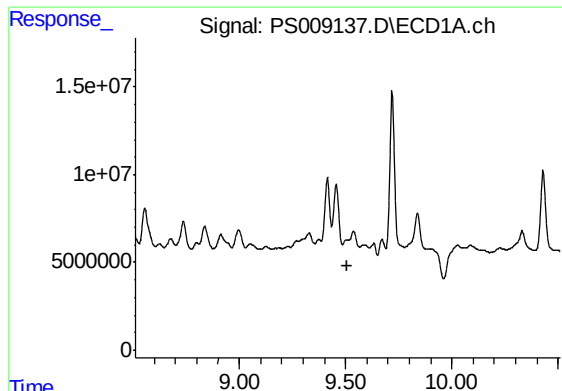

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 9.511 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB127286BL

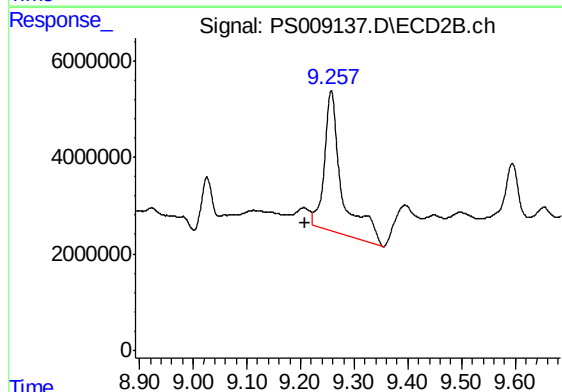


#12 2,4,5-T

R.T.: 9.257 min
Delta R.T.: 0.050 min
Response: 65968696
Conc: 12.19 ng/ml

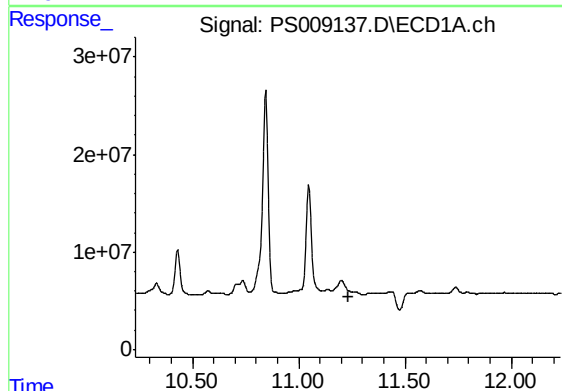


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.231 min
Response: 0
Conc: N.D.

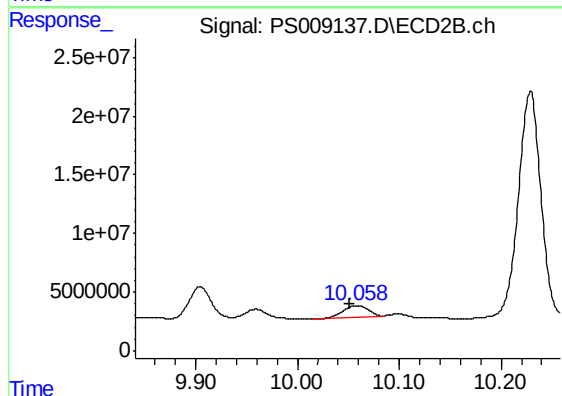

#14 DINOSEB


R.T.: 10.058 min
Delta R.T.: 0.007 min
Response: 16096470
Conc: 4.07 ng/ml

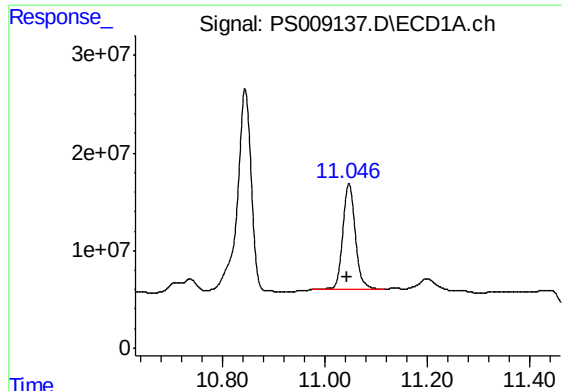

#15 Picloram


R.T.: 11.047 min
Delta R.T.: 0.003 min
Response: 185566459
Conc: 13.55 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB127286BL

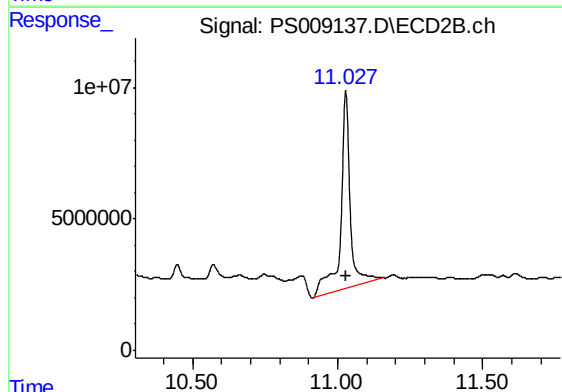


#15 Picloram

R.T.: 11.028 min
Delta R.T.: -0.003 min
Response: 172006454
Conc: 23.67 ng/ml

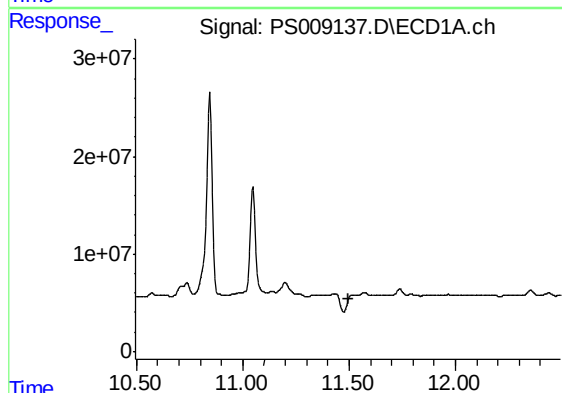

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.495 min
Response: 0
Conc: N.D.

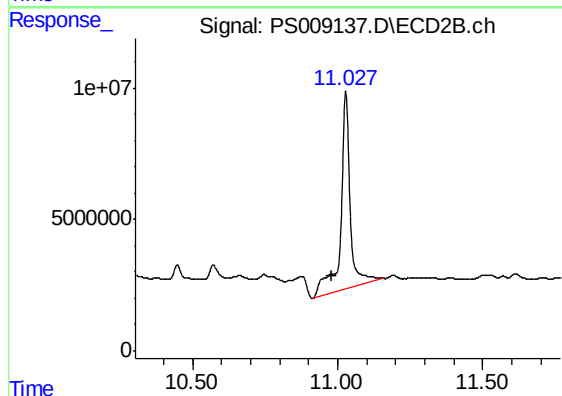

#16 DCPA

R.T.: 11.028 min
Delta R.T.: 0.046 min
Response: 172006454
Conc: 24.86 ng/ml