

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030620\
 Data File : PS009139.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Mar 2020 11:30
 Operator : DD\AJ
 Sample : L1774-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 VNJ-223

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 06 15:18:02 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.246	6.938	665.1E6	295.2E6	304.174	306.340
Target Compounds							
1) T	Dalapon	0.000	2.590	0	103.4E6	N.D.	70.741
2) T	3,5-DICHL...	0.000	6.113	0	163.8E6	N.D.	112.256
7) T	MCPA	7.798	7.405	194.5E6	156.9E6	24.182	35.473 #
8) T	DICHLORPROP	0.000	7.758	0	80872954	N.D.	80.717
10) T	Pentachlo...	8.674	8.463	60569962	40246758	2.087	2.833 #
11) T	2,4,5-TP ...	0.000	8.792	0	77628664	N.D.	14.331
12) T	2,4,5-T	9.453	9.197	96134768	18350872	8.991	3.390 #
14) T	DINOSEB	0.000	10.061	0	35444073	N.D.	8.964
15) T	Picloram	0.000	11.028	0	72150638	N.D.	9.929
16) T	DCPA	0.000	11.028	0	72150638	N.D.	10.427



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030620\
Data File : PS009139.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2020 11:30
Operator : DD\AJ
Sample : L1774-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
VNJ-223

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 06 15:18:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

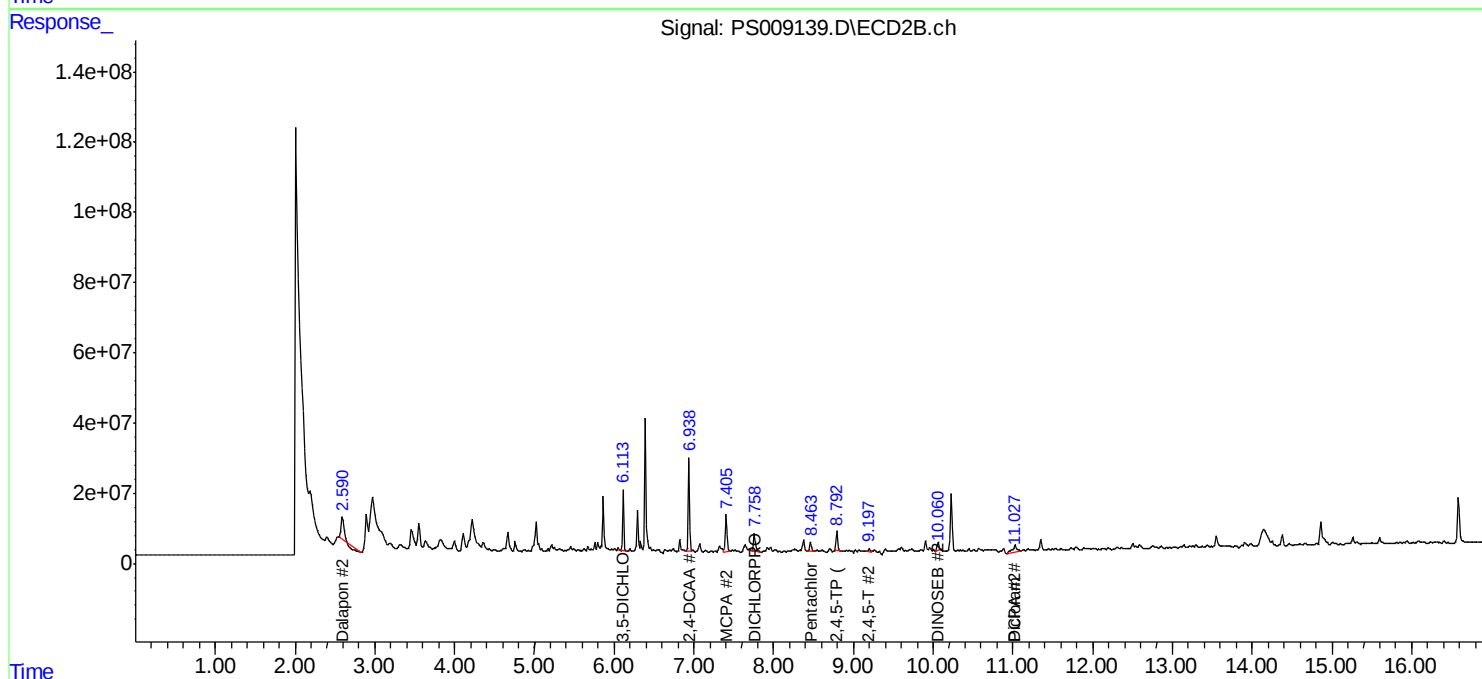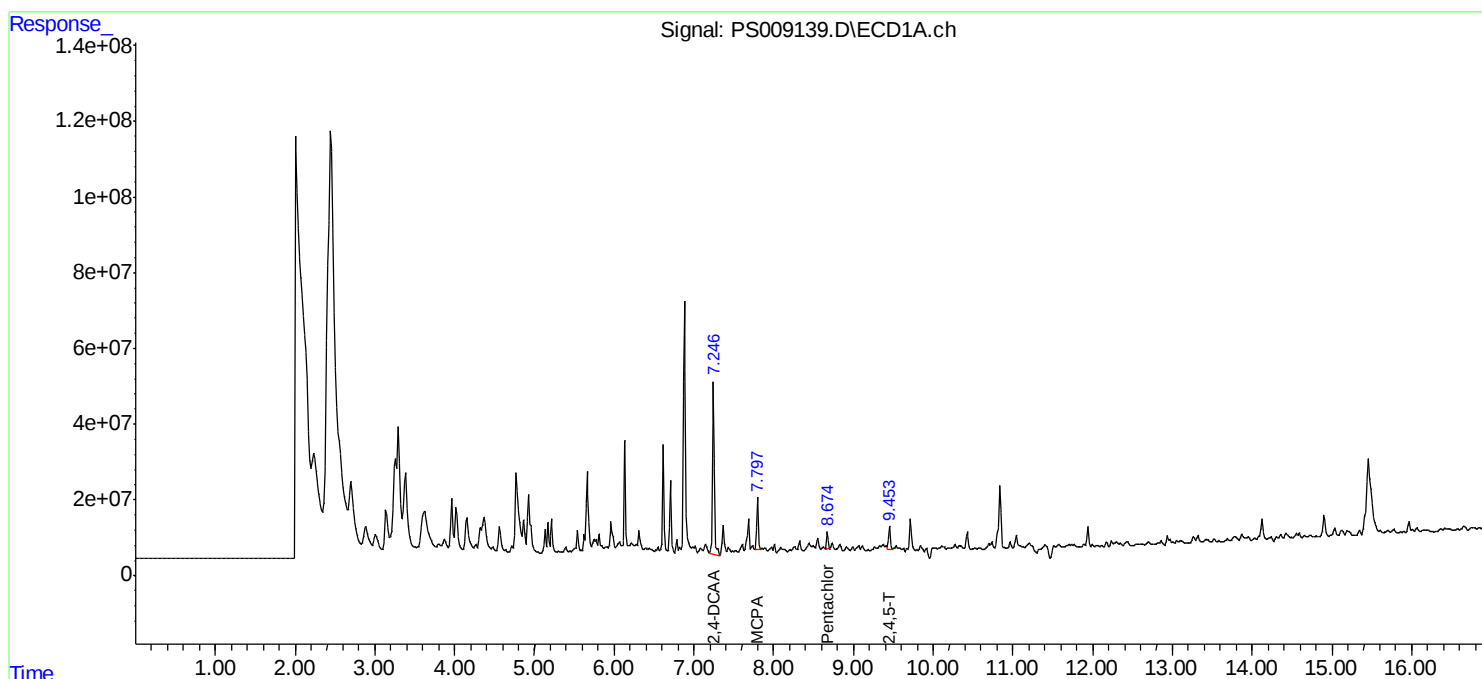


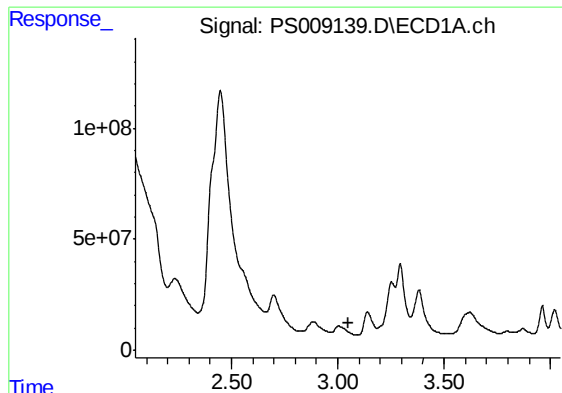

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 3.048 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
VNJ-223

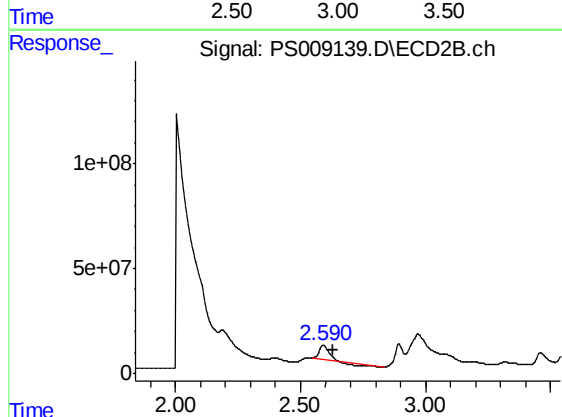


#1 Dalapon

R.T.: 2.590 min
Delta R.T.: -0.040 min
Response: 103438931
Conc: 70.74 ng/ml

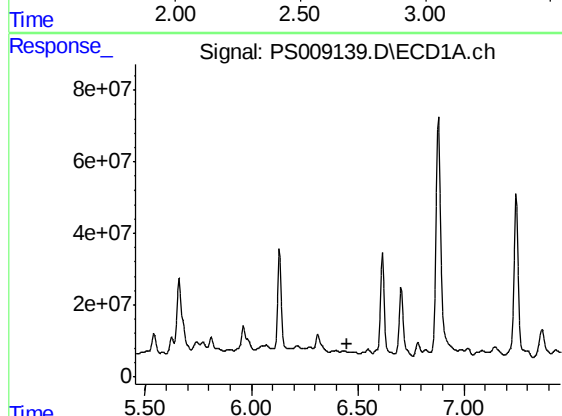


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.455 min
Response: 0
Conc: N.D.

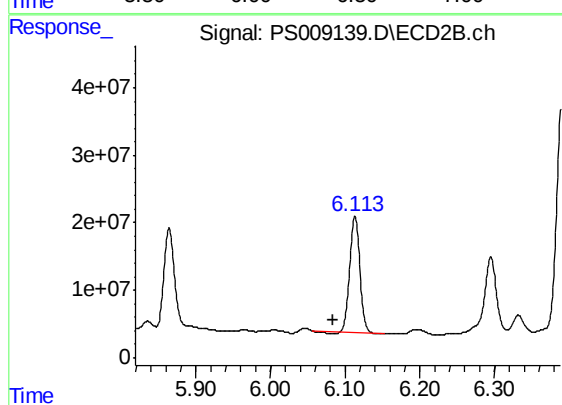

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.113 min
Delta R.T.: 0.030 min
Response: 163811283
Conc: 112.26 ng/ml

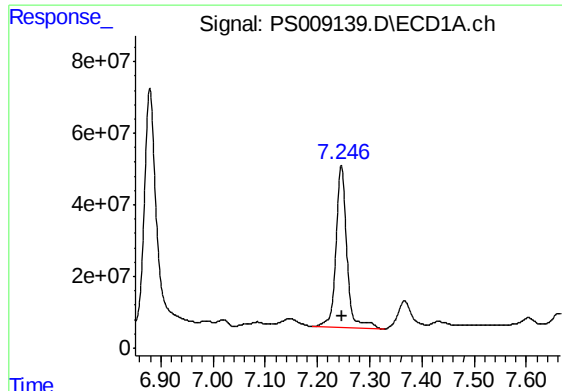

#4 2,4-DCAA


R.T.: 7.246 min
Delta R.T.: 0.000 min
Response: 665103898
Conc: 304.17 ng/ml

Instrument :
ECD_S
ClientSampleId :
VNJ-223

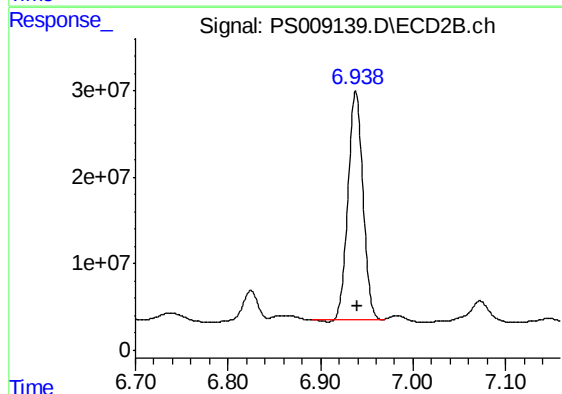


#4 2,4-DCAA

R.T.: 6.938 min
Delta R.T.: -0.002 min
Response: 295175745
Conc: 306.34 ng/ml

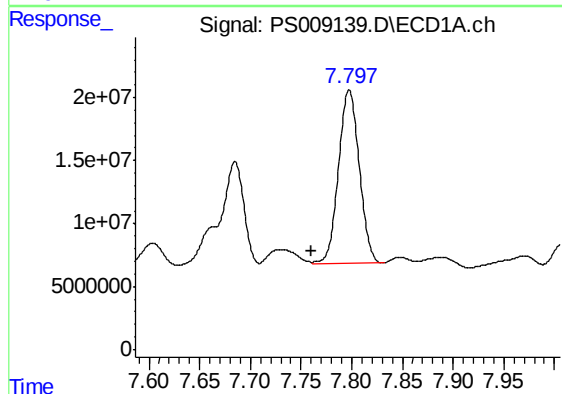


#7 MCPA

R.T.: 7.798 min
Delta R.T.: 0.037 min
Response: 194520064
Conc: 24.18 ug/ml

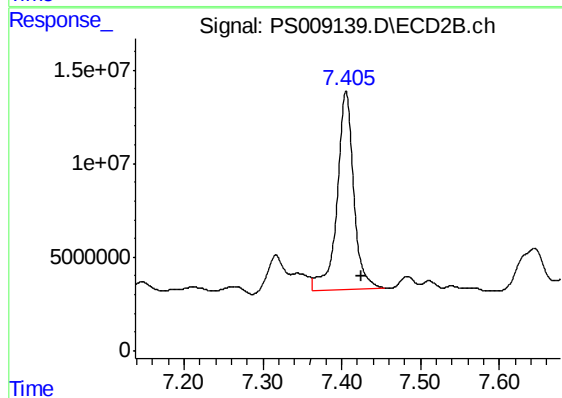

#7 MCPA


R.T.: 7.405 min
Delta R.T.: -0.020 min
Response: 156942572
Conc: 35.47 ug/ml

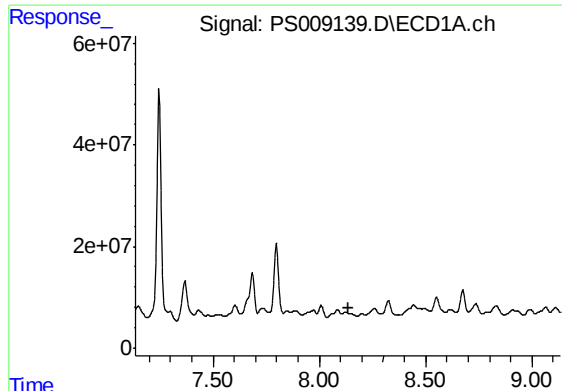

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.135 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
VNJ-223

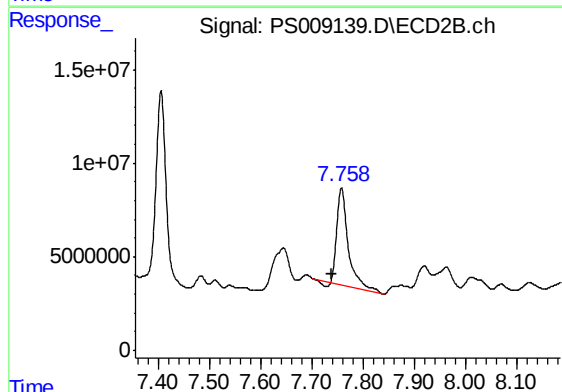


#8 DICHLORPROP

R.T.: 7.758 min
Delta R.T.: 0.019 min
Response: 80872954
Conc: 80.72 ng/ml

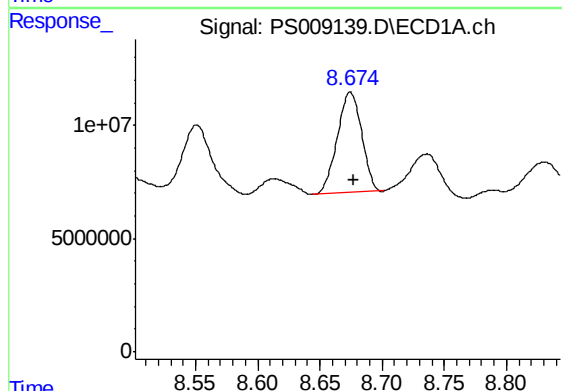


#10 Pentachlorophenol

R.T.: 8.674 min
Delta R.T.: -0.002 min
Response: 60569962
Conc: 2.09 ng/ml

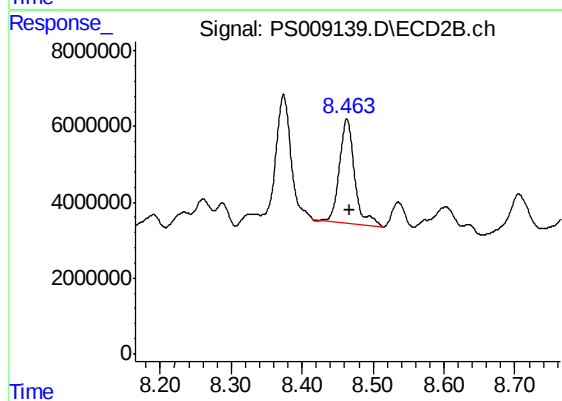

#10 Pentachlorophenol


R.T.: 8.463 min
Delta R.T.: -0.004 min
Response: 40246758
Conc: 2.83 ng/ml

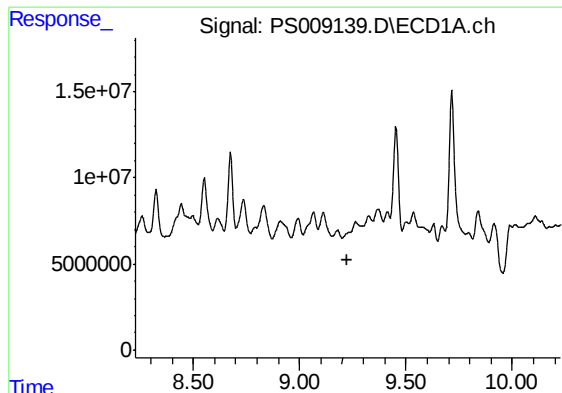

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.227 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
VNJ-223

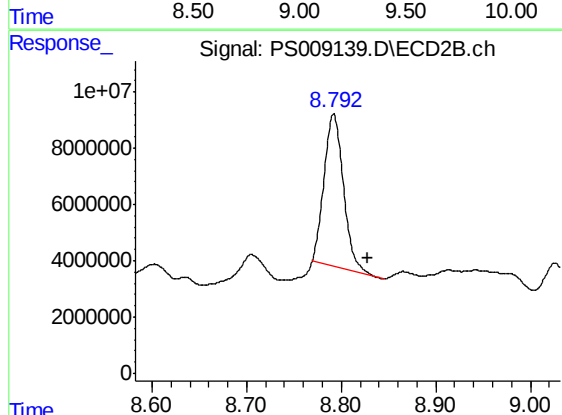


#11 2,4,5-TP (SILVEX)

R.T.: 8.792 min
Delta R.T.: -0.036 min
Response: 77628664
Conc: 14.33 ng/ml

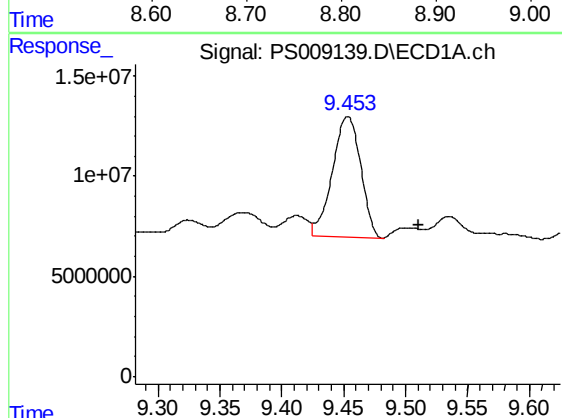


#12 2,4,5-T

R.T.: 9.453 min
Delta R.T.: -0.058 min
Response: 96134768
Conc: 8.99 ng/ml

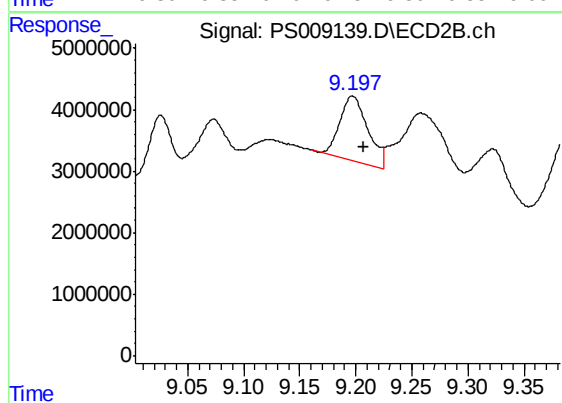

#12 2,4,5-T


R.T.: 9.197 min
Delta R.T.: -0.011 min
Response: 18350872
Conc: 3.39 ng/ml

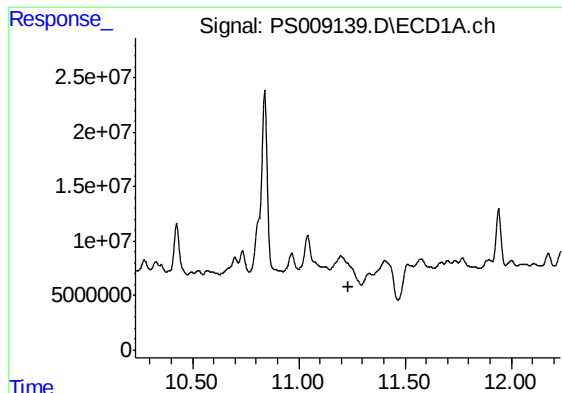

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 11.231 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
VNJ-223

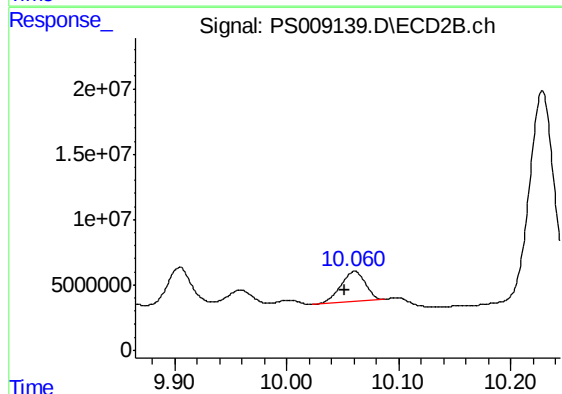


#14 DINOSEB

R.T.: 10.061 min
Delta R.T.: 0.009 min
Response: 35444073
Conc: 8.96 ng/ml

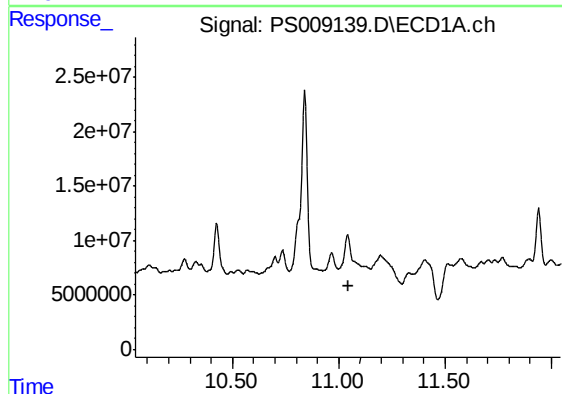


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.043 min
Response: 0
Conc: N.D.

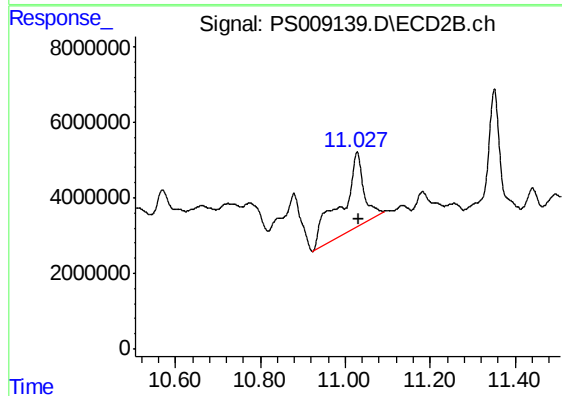

#15 Picloram


R.T.: 11.028 min
Delta R.T.: -0.003 min
Response: 72150638
Conc: 9.93 ng/ml

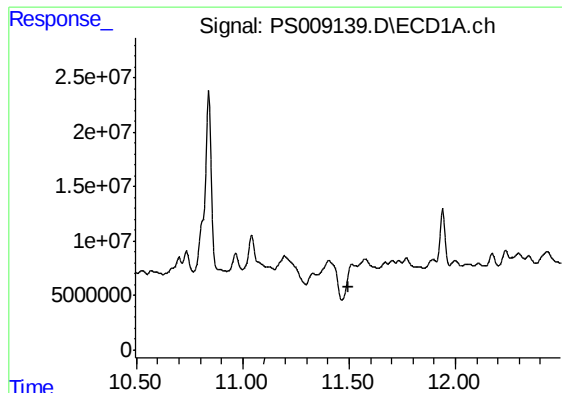

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.495 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
VNJ-223

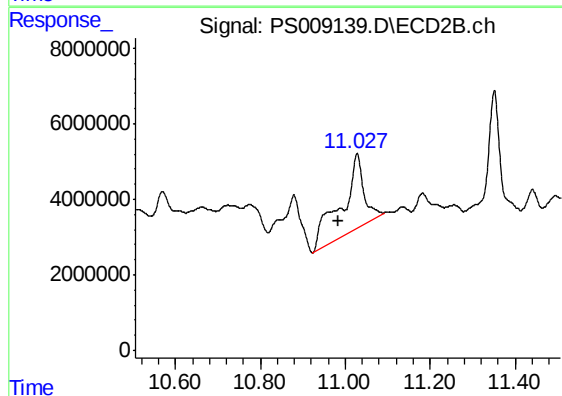

#16 DCPA

R.T.: 11.028 min
Delta R.T.: 0.046 min
Response: 72150638
Conc: 10.43 ng/ml