

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030620\
 Data File : PS009140.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Mar 2020 11:53
 Operator : DD\AJ
 Sample : L1774-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 VNJ-236

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 06 15:18:18 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.246	6.938	456.4E6	186.6E6	208.733	193.617
Target Compounds							
1) T	Dalapon	0.000	2.589	0	8498655	N.D.	5.812
2) T	3,5-DICHL...	0.000	6.113	0	195.3E6	N.D.	133.855
7) T	MCPA	7.797	7.405	222.7E6	163.0E6	27.681	36.837 #
8) T	DICHLORPROP	0.000	7.757	0	76058238	N.D.	75.912
10) T	Pentachlo...	0.000	8.463	0	25727839	N.D.	1.811
11) T	2,4,5-TP ...	0.000	8.792	0	64035654	N.D.	11.821
12) T	2,4,5-T	9.452	9.196	132.4E6	17494162	12.380	3.232 #
13) T	2,4-DB	0.000	9.731	0	51073469	N.D.	72.709
14) T	DINOSEB	0.000	10.061	0	61054144	N.D.	15.441
15) T	Picloram	0.000	11.028	0	62537148	N.D.	8.606
16) T	DCPA	11.508	11.028	42715643	62537148	3.109	9.038 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030620\
Data File : PS009140.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2020 11:53
Operator : DD\AJ
Sample : L1774-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
VNJ-236

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 06 15:18:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

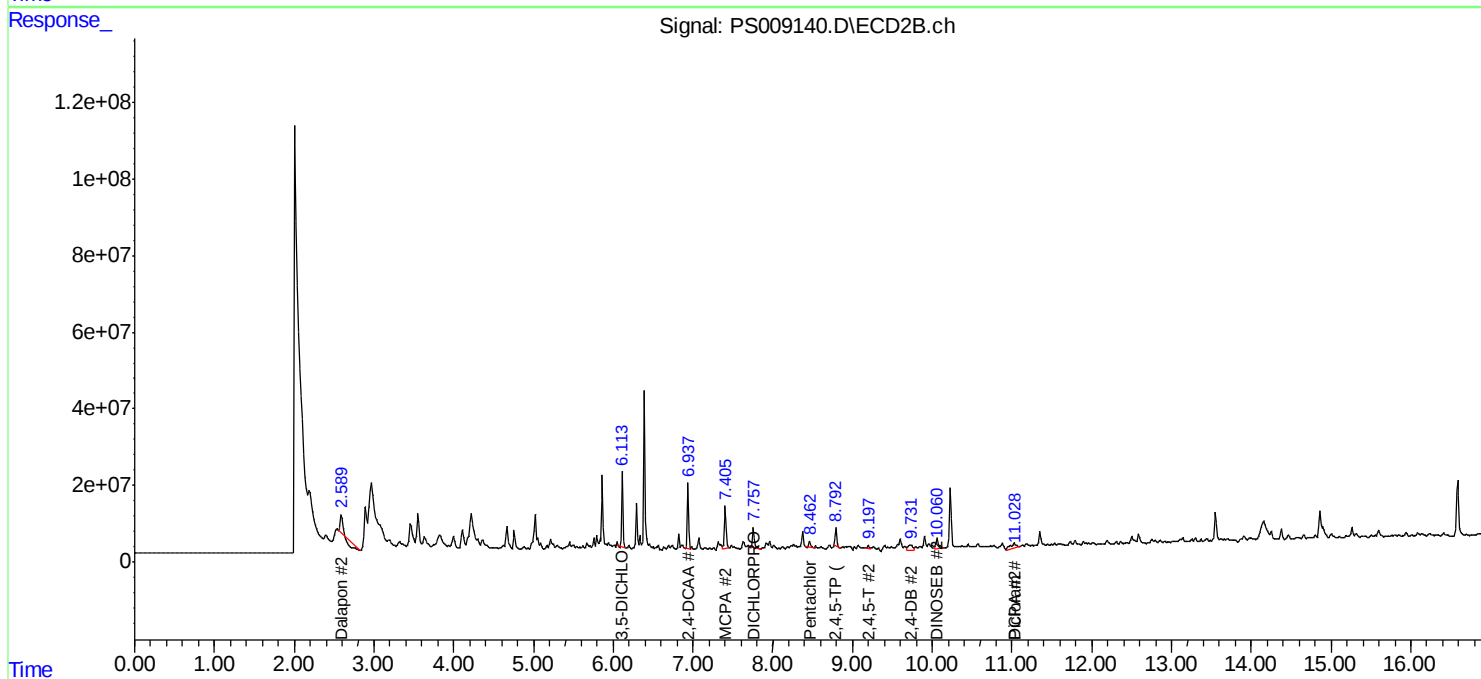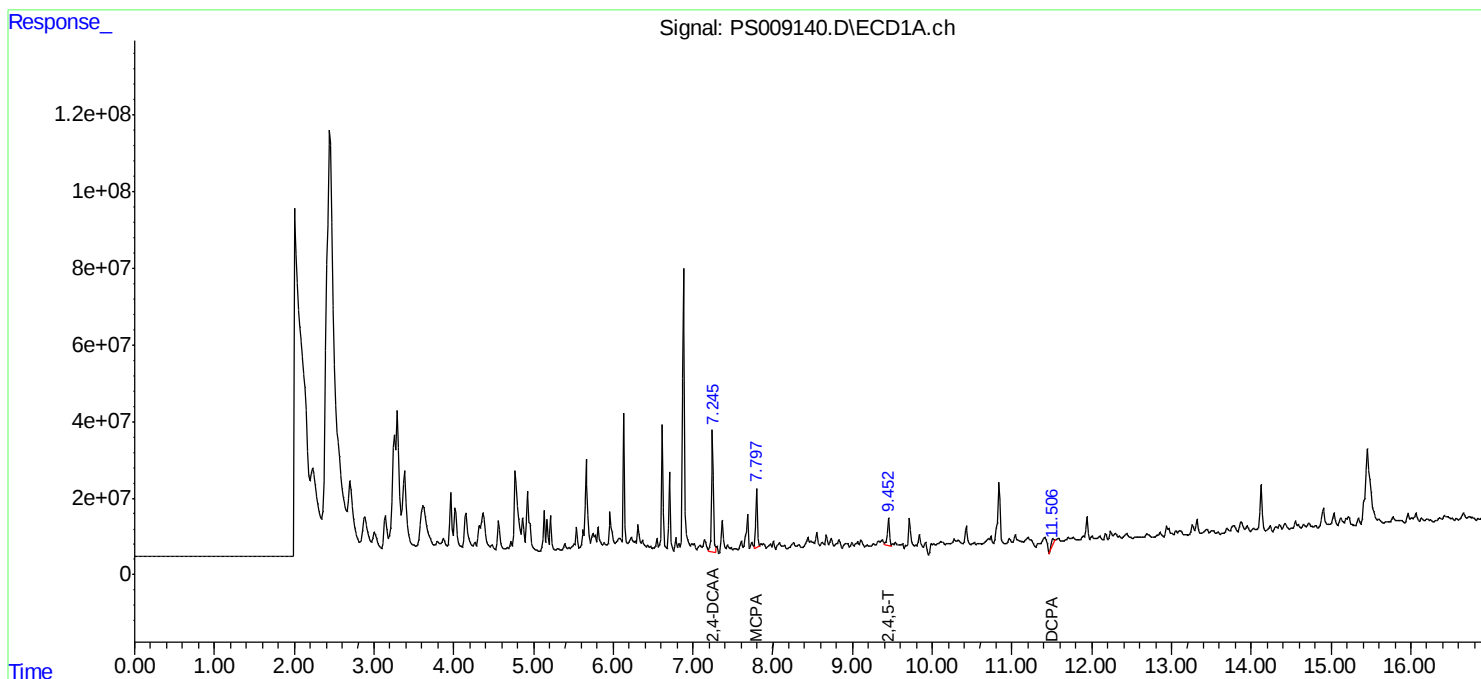


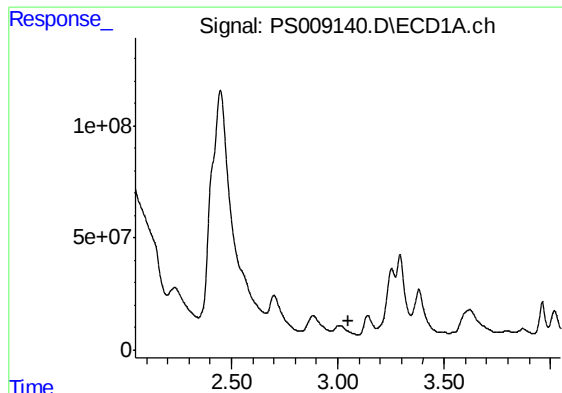

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 3.048 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
VNJ-236

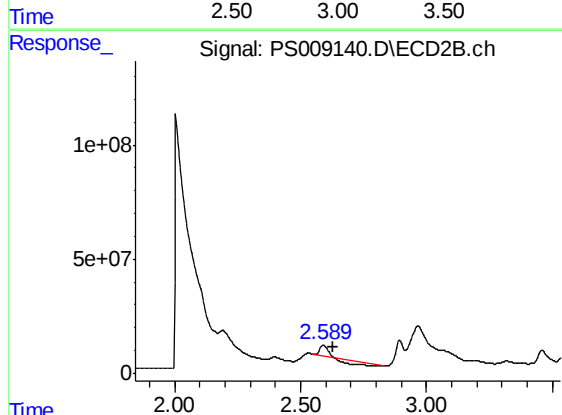


#1 Dalapon

R.T.: 2.589 min
Delta R.T.: -0.041 min
Response: 8498655
Conc: 5.81 ng/ml

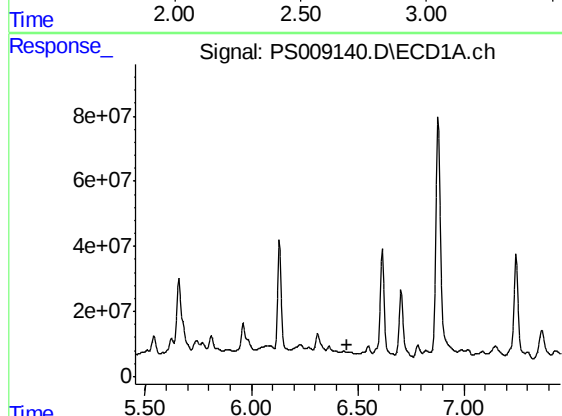


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.455 min
Response: 0
Conc: N.D.

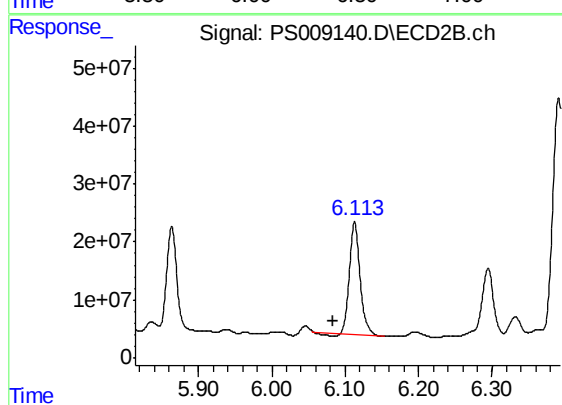

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.113 min
Delta R.T.: 0.030 min
Response: 195331204
Conc: 133.86 ng/ml

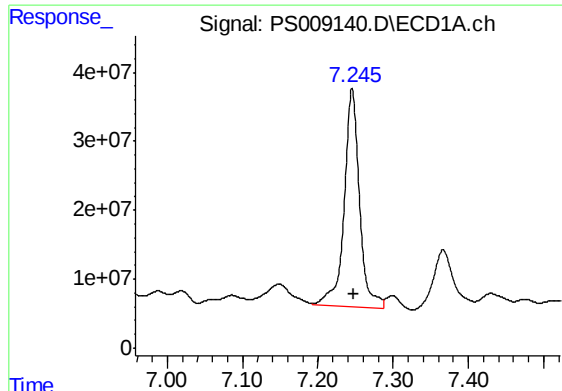

#4 2,4-DCAA


R.T.: 7.246 min
Delta R.T.: -0.001 min
Response: 456414333
Conc: 208.73 ng/ml

Instrument :
ECD_S
ClientSampleId :
VNJ-236

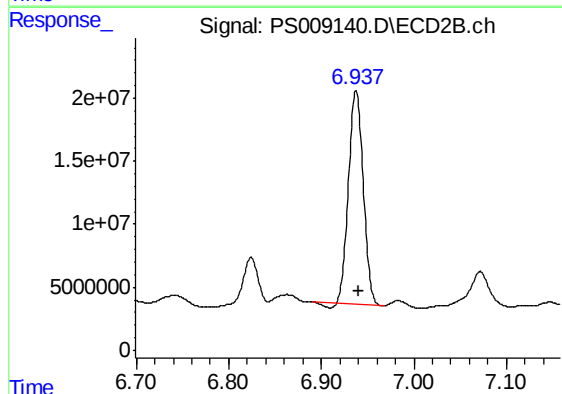


#4 2,4-DCAA

R.T.: 6.938 min
Delta R.T.: -0.003 min
Response: 186561141
Conc: 193.62 ng/ml

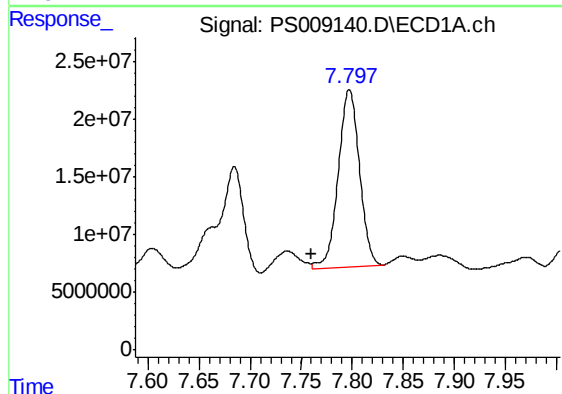


#7 MCPA

R.T.: 7.797 min
Delta R.T.: 0.037 min
Response: 222663706
Conc: 27.68 ug/ml

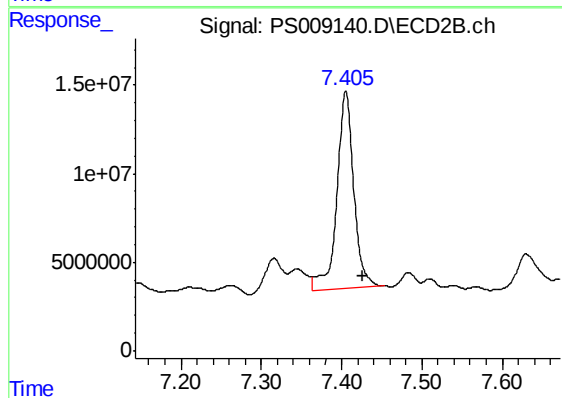

#7 MCPA


R.T.: 7.405 min
Delta R.T.: -0.020 min
Response: 162974598
Conc: 36.84 ug/ml

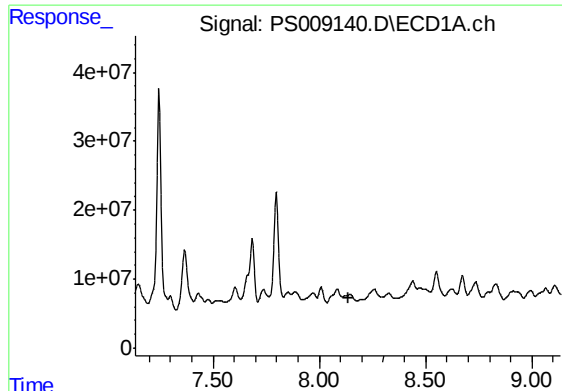

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 8.135 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
VNJ-236

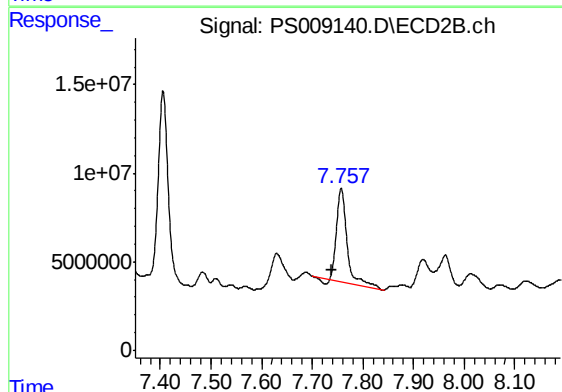


#8 DICHLORPROP

R.T.: 7.757 min
Delta R.T.: 0.018 min
Response: 76058238
Conc: 75.91 ng/ml

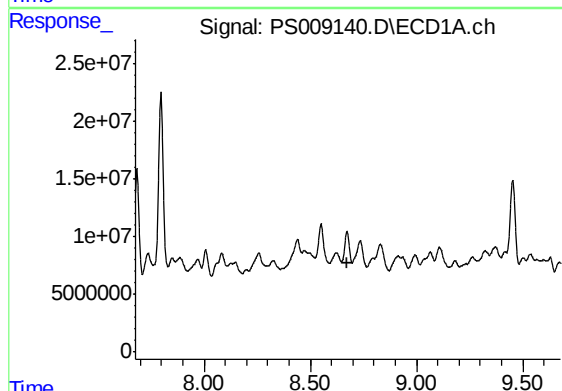


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 8.677 min
Response: 0
Conc: N.D.

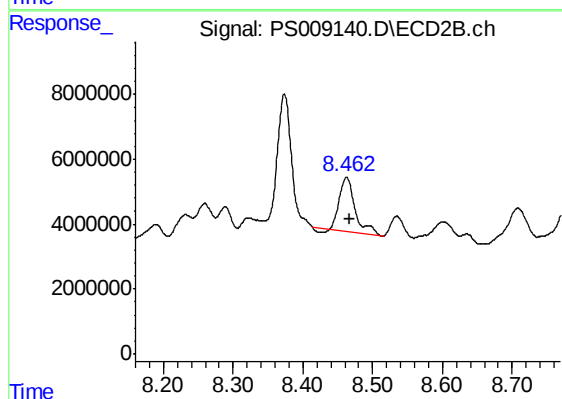

#10 Pentachlorophenol


R.T.: 8.463 min
Delta R.T.: -0.004 min
Response: 25727839
Conc: 1.81 ng/ml

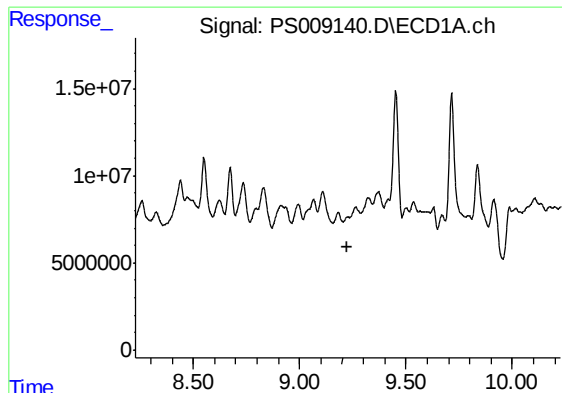

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.227 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
VNJ-236

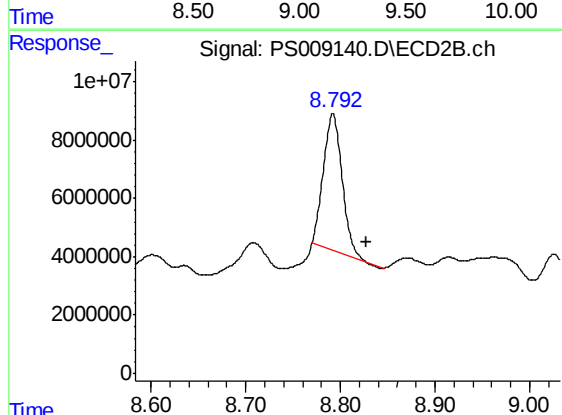


#11 2,4,5-TP (SILVEX)

R.T.: 8.792 min
Delta R.T.: -0.036 min
Response: 64035654
Conc: 11.82 ng/ml

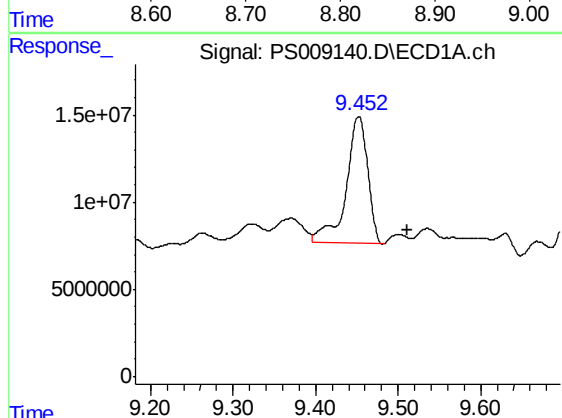


#12 2,4,5-T

R.T.: 9.452 min
Delta R.T.: -0.059 min
Response: 132364190
Conc: 12.38 ng/ml

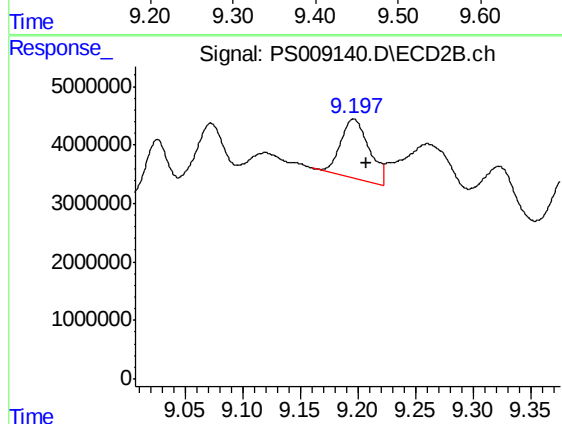

#12 2,4,5-T


R.T.: 9.196 min
Delta R.T.: -0.011 min
Response: 17494162
Conc: 3.23 ng/ml

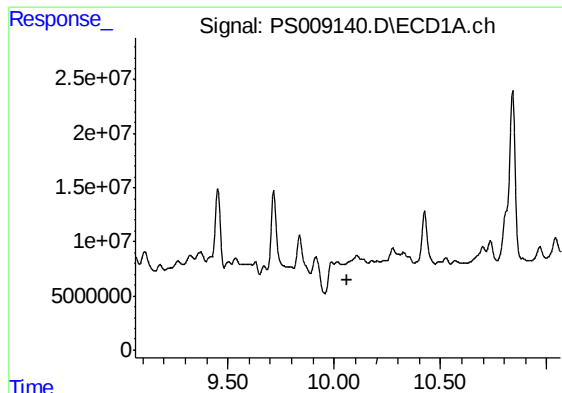

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 10.064 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
VNJ-236

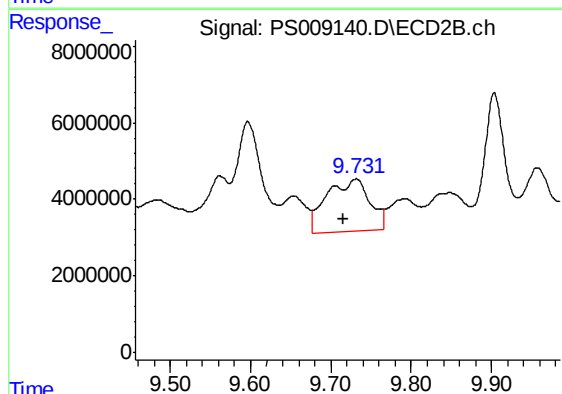


#13 2,4-DB

R.T.: 9.731 min
Delta R.T.: 0.016 min
Response: 51073469
Conc: 72.71 ng/ml

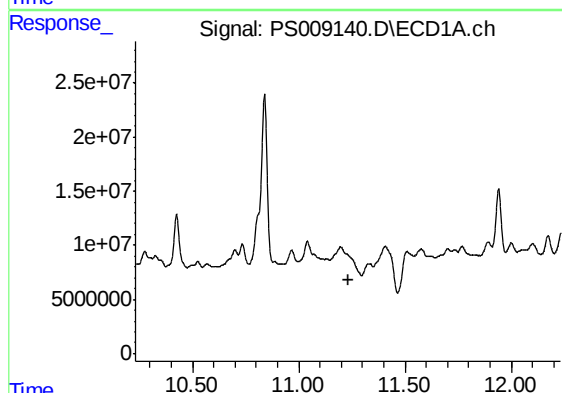


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.231 min
Response: 0
Conc: N.D.

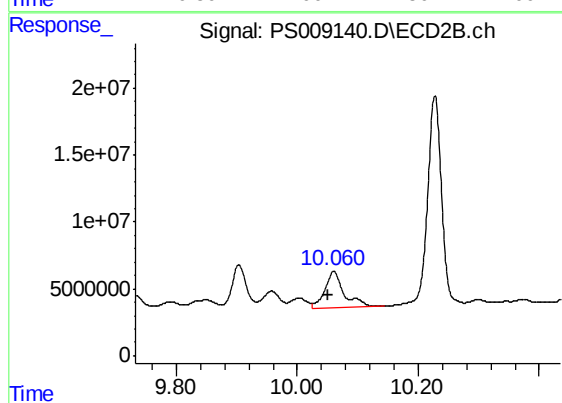

#14 DINOSEB


R.T.: 10.061 min
Delta R.T.: 0.009 min
Response: 61054144
Conc: 15.44 ng/ml

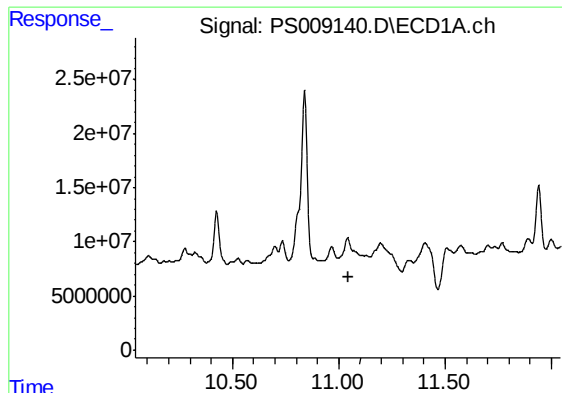

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 11.043 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
VNJ-236

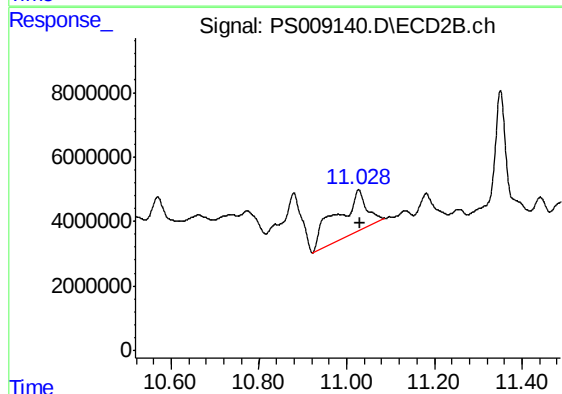


#15 Picloram

R.T.: 11.028 min
Delta R.T.: -0.003 min
Response: 62537148
Conc: 8.61 ng/ml

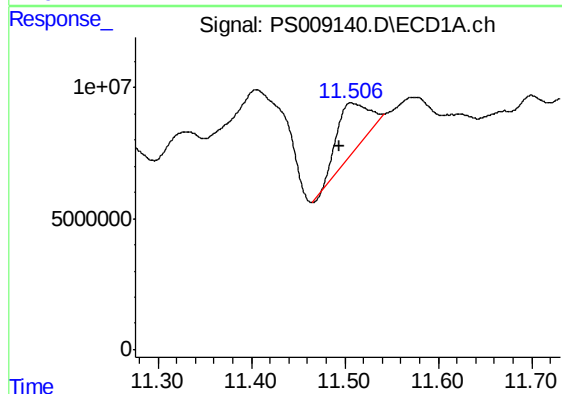

#16 DCPA

R.T.: 11.508 min
Delta R.T.: 0.013 min
Response: 42715643
Conc: 3.11 ng/ml

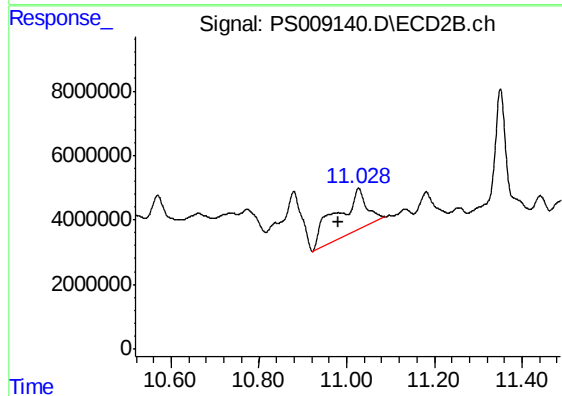

#16 DCPA

R.T.: 11.028 min
Delta R.T.: 0.045 min
Response: 62537148
Conc: 9.04 ng/ml