

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030620\
 Data File : PS009141.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Mar 2020 12:16
 Operator : DD\AJ
 Sample : L1775-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CR-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 06 15:18:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.246	6.938	622.7E6	231.6E6	284.766	240.373
Target Compounds							
2) T	3,5-DICHL...	0.000	6.113	0	182.9E6	N.D.	125.306
7) T	MCPA	7.798	7.406	205.2E6	190.1E6	25.512	42.970 #
8) T	DICHLORPROP	0.000	7.758	0	59828749	N.D.	59.713
11) T	2,4,5-TP ...	0.000	8.792	0	76297891	N.D.	14.085
12) T	2,4,5-T	9.453	9.195	111.2E6	23883468	10.401	4.412 #
13) T	2,4-DB	0.000	9.731	0	78596768	N.D.	111.891
14) T	DINOSEB	0.000	10.061	0	72620461	N.D.	18.366
15) T	Picloram	0.000	11.028	0	38007731	N.D.	5.231
16) T	DCPA	11.512	10.977	56199359	44206900	4.090	6.389 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030620\
Data File : PS009141.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2020 12:16
Operator : DD\AJ
Sample : L1775-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
CR-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 06 15:18:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

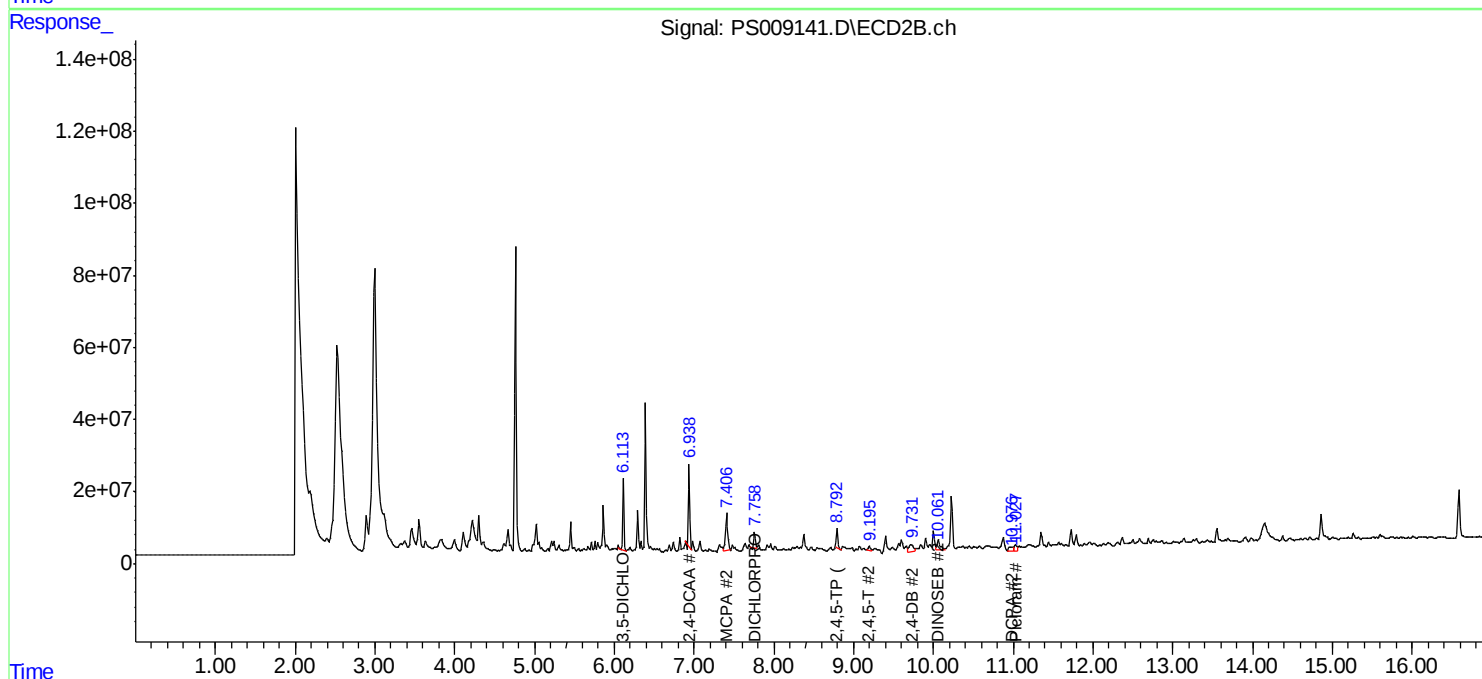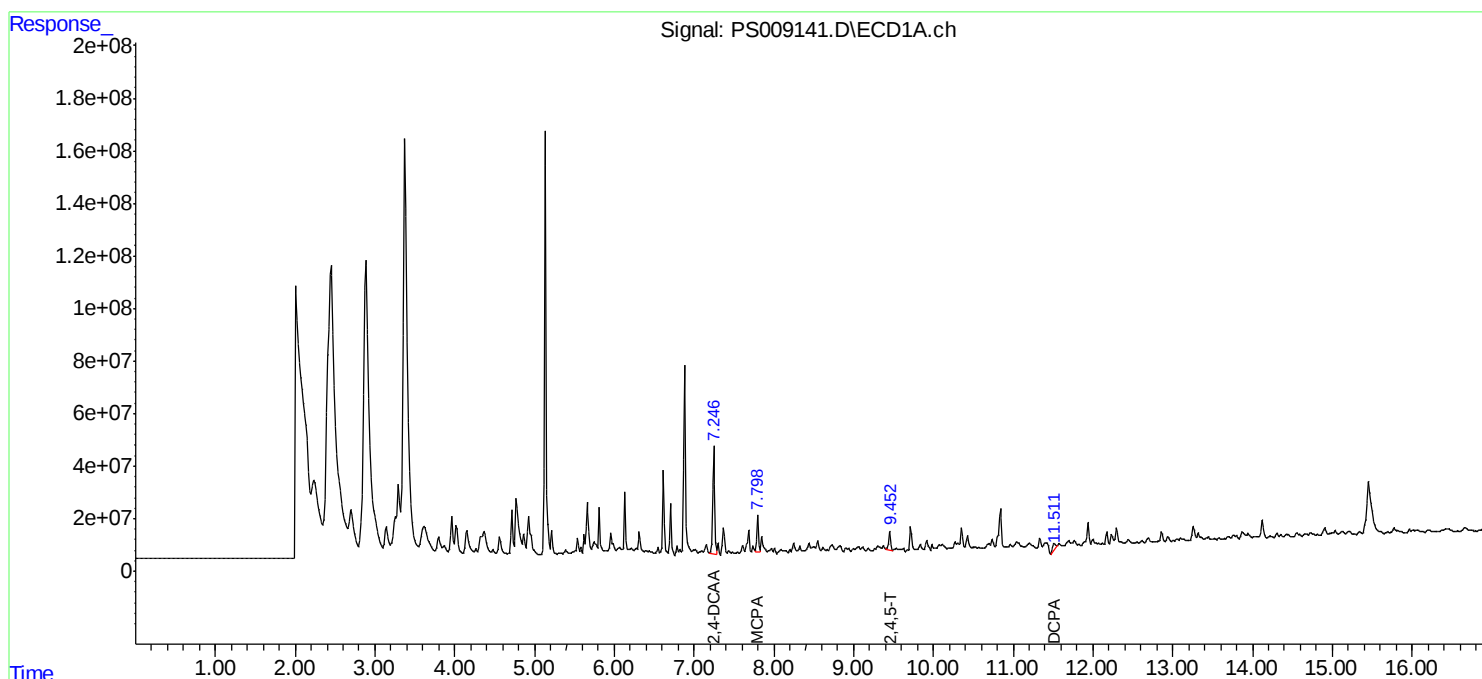


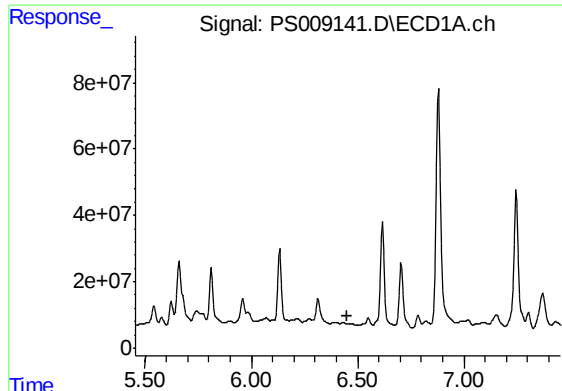

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CR-1

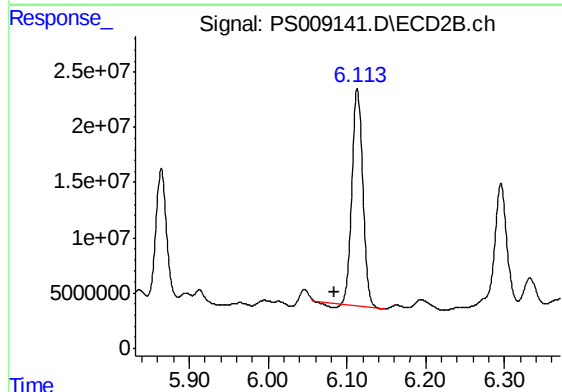


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.113 min
Delta R.T.: 0.030 min
Response: 182855349
Conc: 125.31 ng/ml

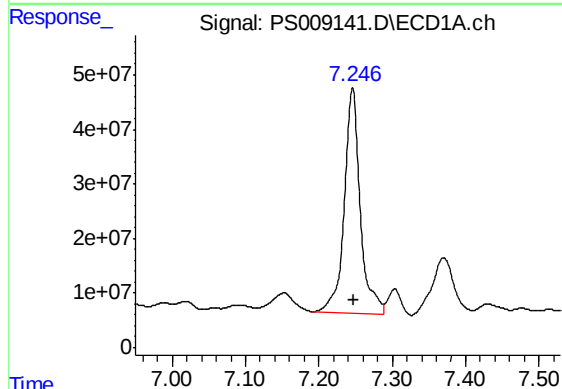


#4 2,4-DCAA

R.T.: 7.246 min
Delta R.T.: 0.000 min
Response: 622666341
Conc: 284.77 ng/ml

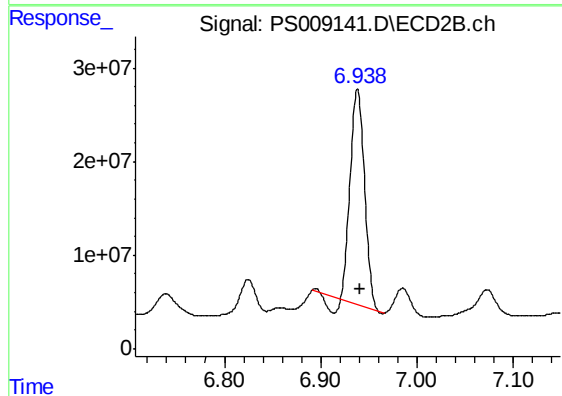

#4 2,4-DCAA


R.T.: 6.938 min
Delta R.T.: -0.002 min
Response: 231612495
Conc: 240.37 ng/ml

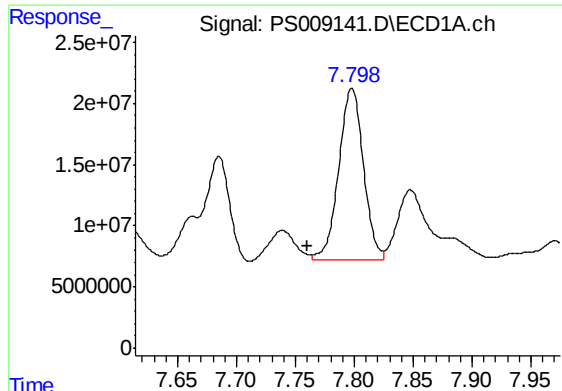

#7 MCPA


R.T.: 7.798 min
Delta R.T.: 0.037 min
Response: 205219046
Conc: 25.51 ug/ml

Instrument :
ECD_S
ClientSampleId :
CR-1

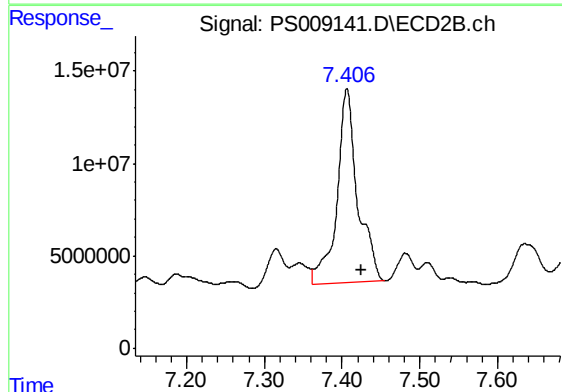


#7 MCPA

R.T.: 7.406 min
Delta R.T.: -0.019 min
Response: 190110427
Conc: 42.97 ug/ml

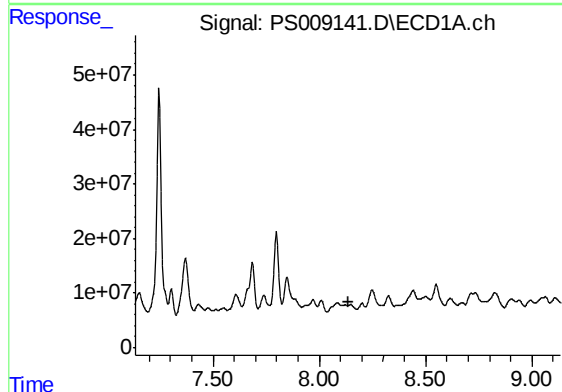


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.135 min
Response: 0
Conc: N.D.

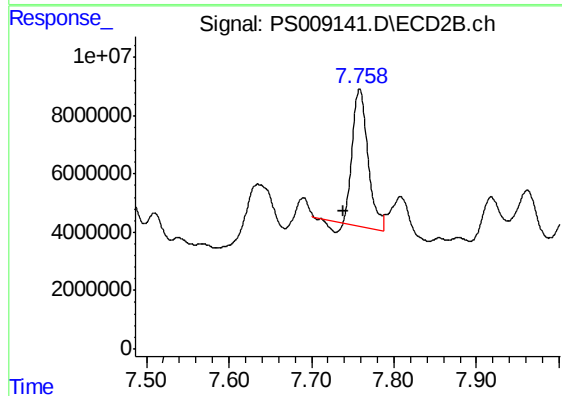

#8 DICHLORPROP


R.T.: 7.758 min
Delta R.T.: 0.019 min
Response: 59828749
Conc: 59.71 ng/ml

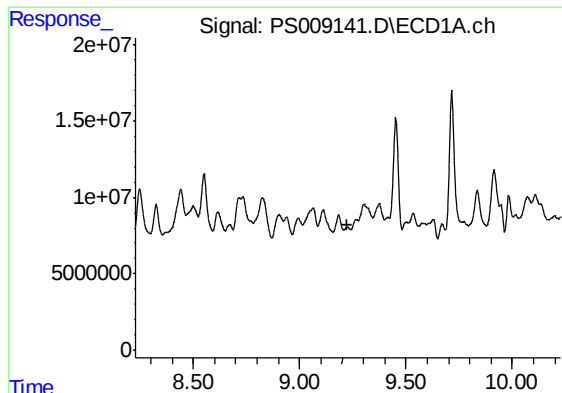

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.227 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CR-1

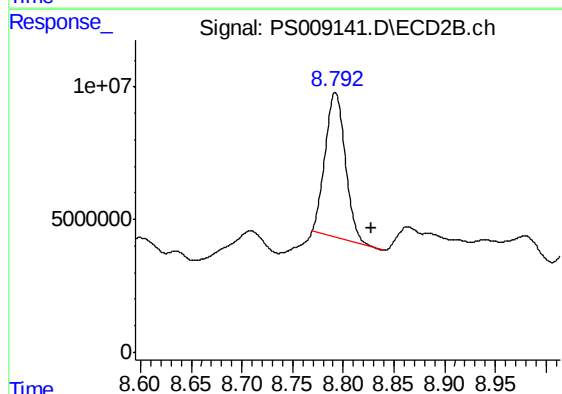


#11 2,4,5-TP (SILVEX)

R.T.: 8.792 min
Delta R.T.: -0.036 min
Response: 76297891
Conc: 14.09 ng/ml

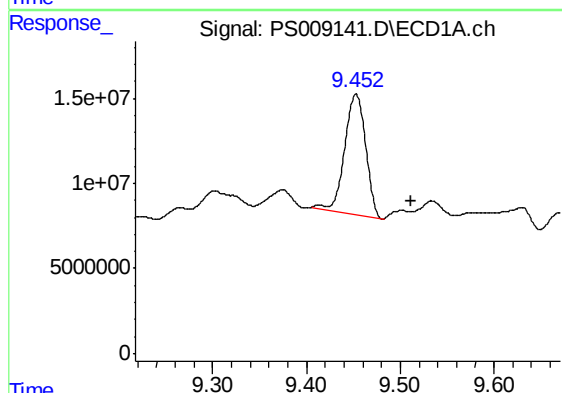


#12 2,4,5-T

R.T.: 9.453 min
Delta R.T.: -0.058 min
Response: 111210830
Conc: 10.40 ng/ml

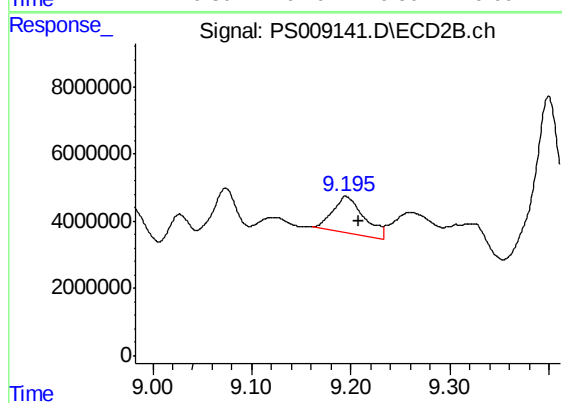

#12 2,4,5-T


R.T.: 9.195 min
Delta R.T.: -0.012 min
Response: 23883468
Conc: 4.41 ng/ml

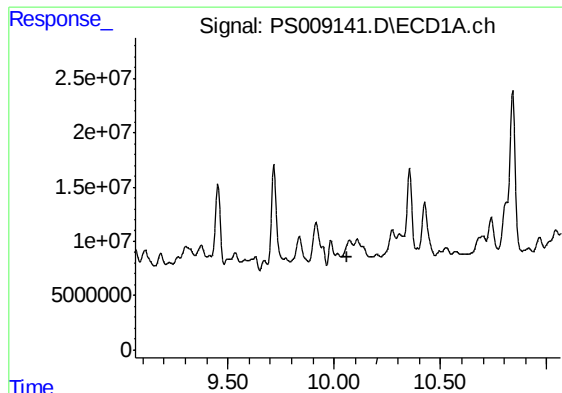

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 10.064 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CR-1

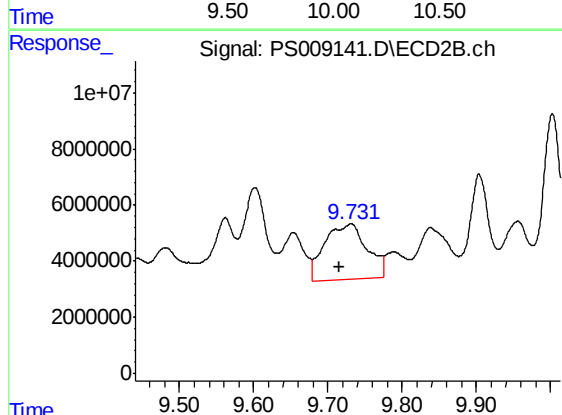


#13 2,4-DB

R.T.: 9.731 min
Delta R.T.: 0.016 min
Response: 78596768
Conc: 111.89 ng/ml

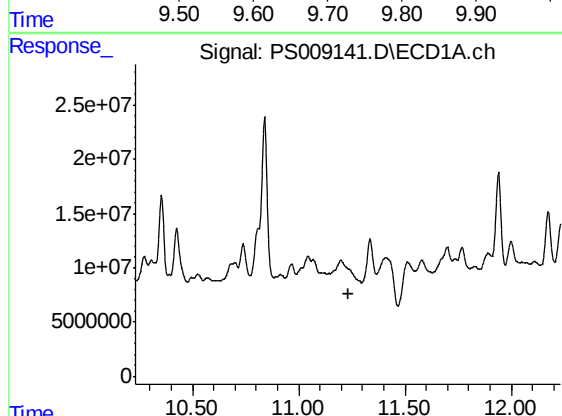


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.231 min
Response: 0
Conc: N.D.

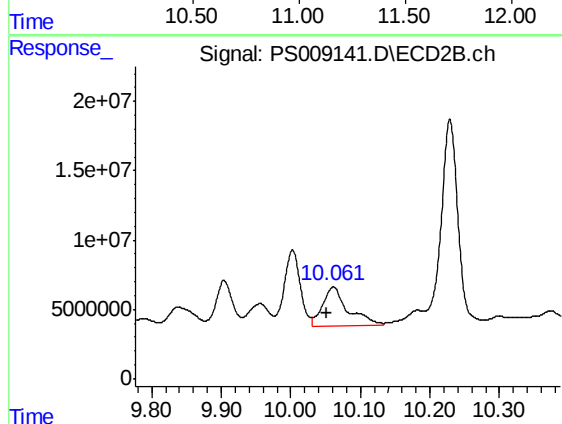

#14 DINOSEB


R.T.: 10.061 min
Delta R.T.: 0.010 min
Response: 72620461
Conc: 18.37 ng/ml

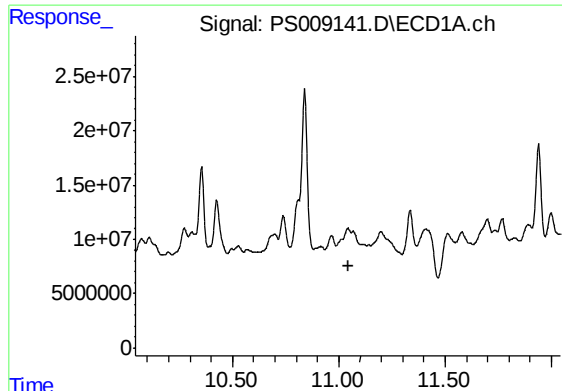

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 11.043 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CR-1

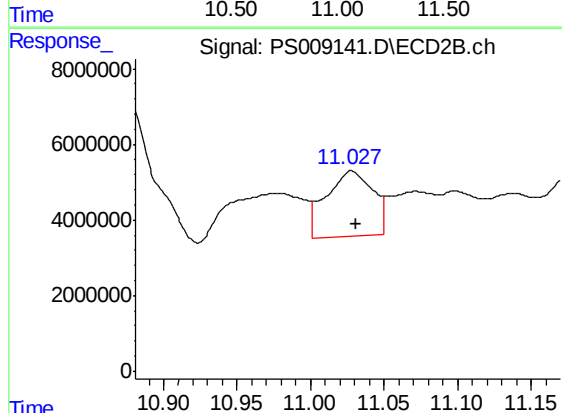


#15 Picloram

R.T.: 11.028 min
Delta R.T.: -0.003 min
Response: 38007731
Conc: 5.23 ng/ml

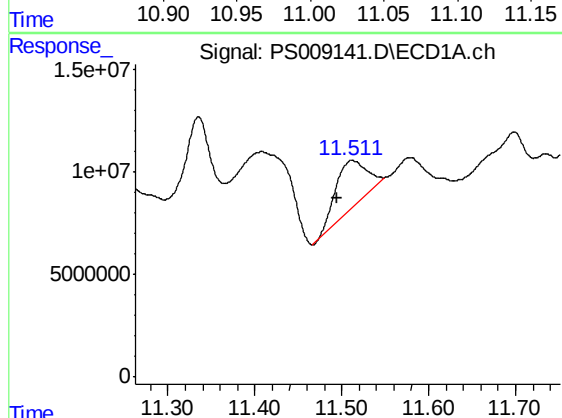

#16 DCPA

R.T.: 11.512 min
Delta R.T.: 0.018 min
Response: 56199359
Conc: 4.09 ng/ml

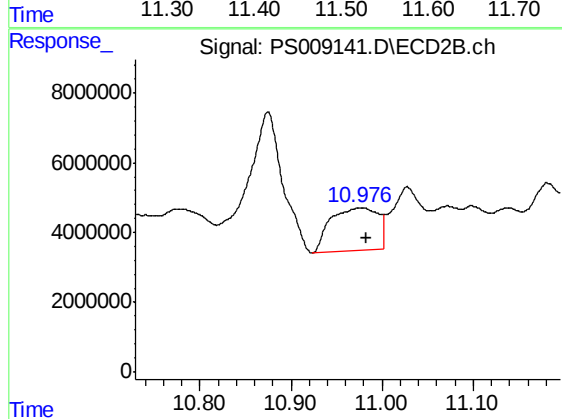

#16 DCPA

R.T.: 10.977 min
Delta R.T.: -0.006 min
Response: 44206900
Conc: 6.39 ng/ml