

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030620\
 Data File : PS009143.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Mar 2020 13:02
 Operator : DD\AJ
 Sample : L1775-13
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CR-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 06 15:19:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.246	6.939	640.5E6	255.3E6	292.903	265.004
Target Compounds							
2) T	3,5-DICHL...	0.000	6.114	0	164.5E6	N.D.	112.725
7) T	MCPA	7.798	7.406	209.2E6	181.3E6	26.004	40.983 #
8) T	DICHLORPROP	0.000	7.758	0	58314909	N.D.	58.202
11) T	2,4,5-TP ...	0.000	8.792	0	71769139	N.D.	13.249
12) T	2,4,5-T	9.452	9.196	142.3E6	14078464	13.307	2.601 #
13) T	2,4-DB	0.000	9.731	0	34189617	N.D.	48.673
14) T	DINOSEB	0.000	10.061	0	46417445	N.D.	11.739
15) T	Picloram	0.000	11.028	0	21206066	N.D.	2.918
16) T	DCPA	11.509	10.983	32129713	32709675	2.338	4.727 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030620\
Data File : PS009143.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2020 13:02
Operator : DD\AJ
Sample : L1775-13
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
CR-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 06 15:19:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

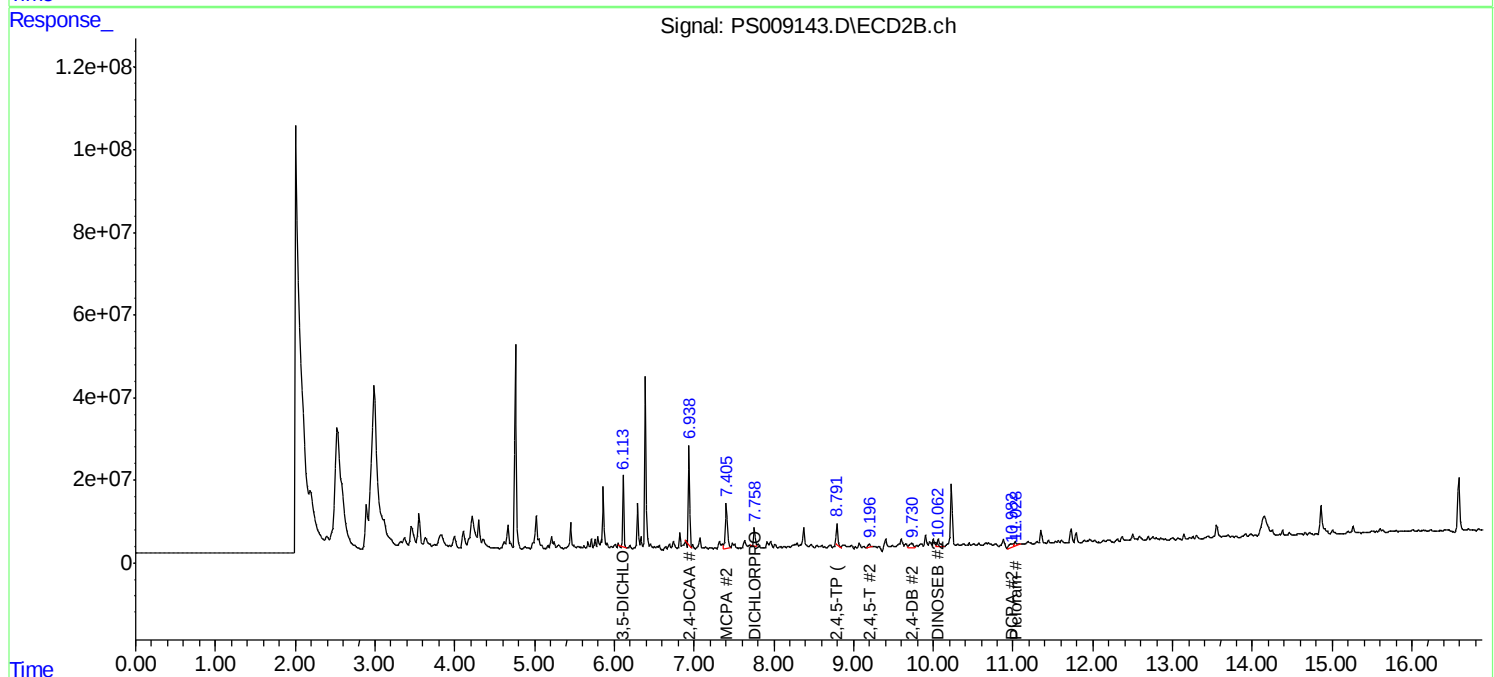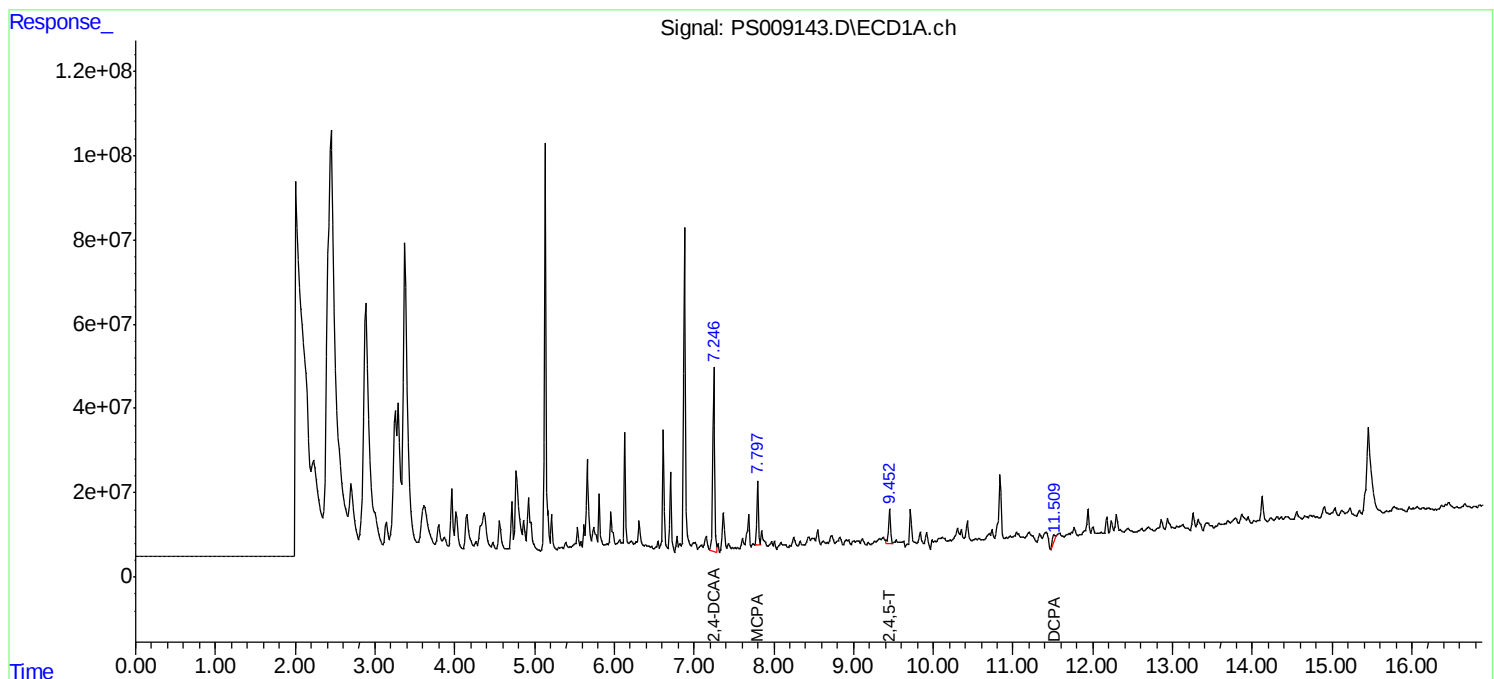


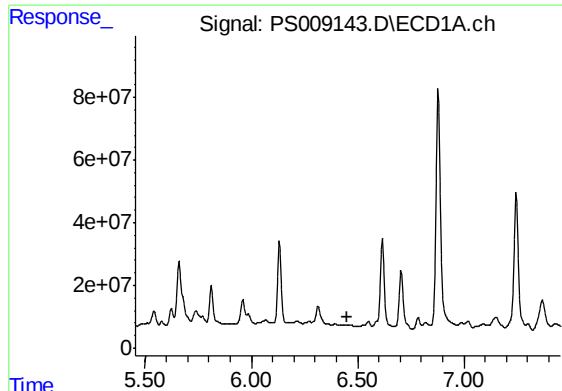

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CR-3

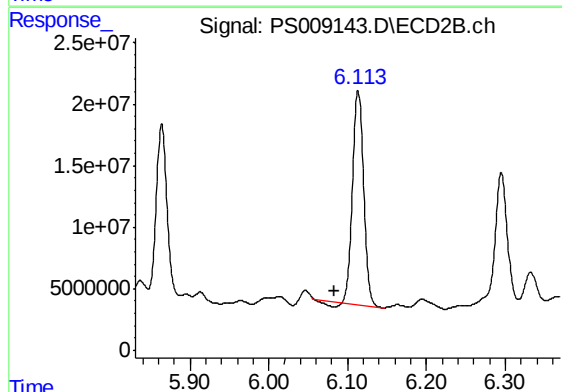


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.114 min
Delta R.T.: 0.030 min
Response: 164495654
Conc: 112.72 ng/ml

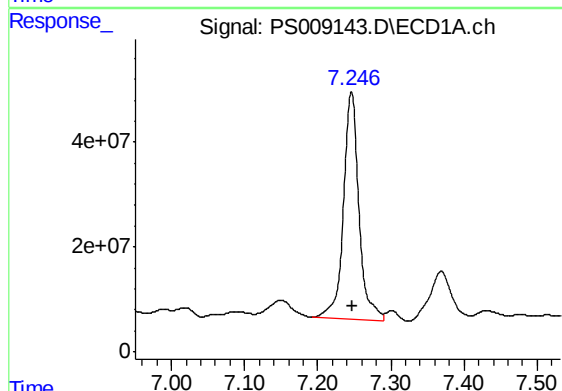


#4 2,4-DCAA

R.T.: 7.246 min
Delta R.T.: 0.000 min
Response: 640459122
Conc: 292.90 ng/ml

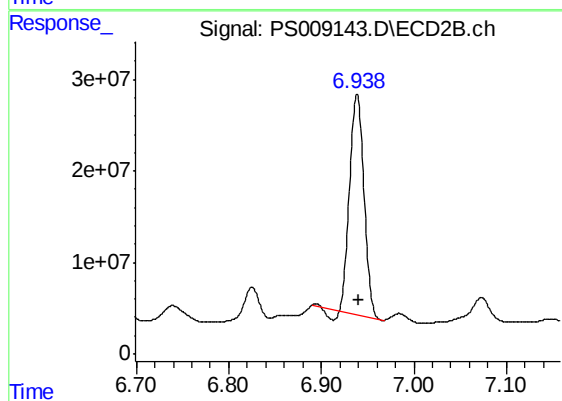

#4 2,4-DCAA


R.T.: 6.939 min
Delta R.T.: -0.002 min
Response: 255346350
Conc: 265.00 ng/ml

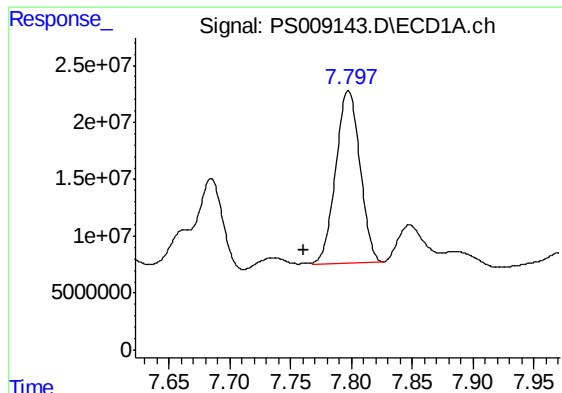

#7 MCPA


R.T.: 7.798 min
Delta R.T.: 0.037 min
Response: 209175852
Conc: 26.00 ug/ml

Instrument :
ECD_S
ClientSampleId :
CR-3

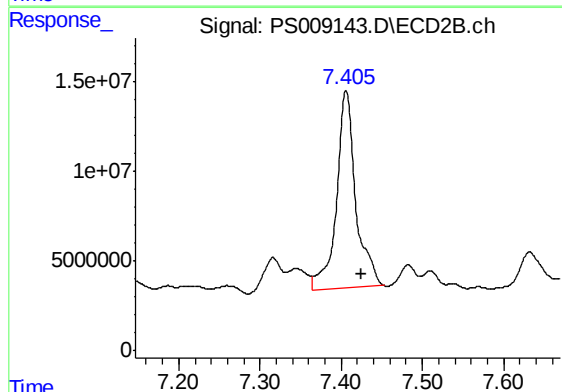


#7 MCPA

R.T.: 7.406 min
Delta R.T.: -0.019 min
Response: 181317926
Conc: 40.98 ug/ml

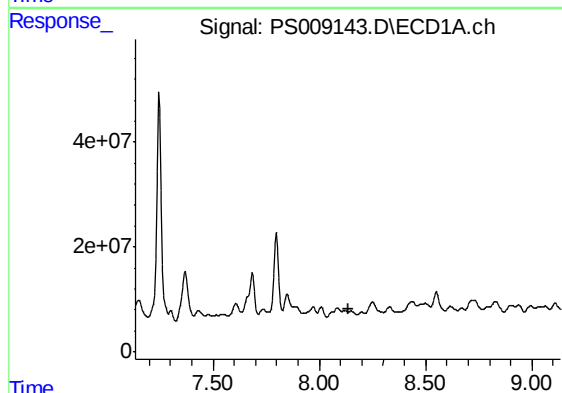


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.135 min
Response: 0
Conc: N.D.

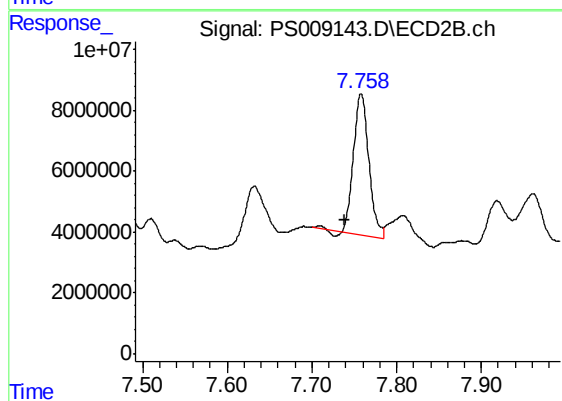

#8 DICHLORPROP


R.T.: 7.758 min
Delta R.T.: 0.019 min
Response: 58314909
Conc: 58.20 ng/ml

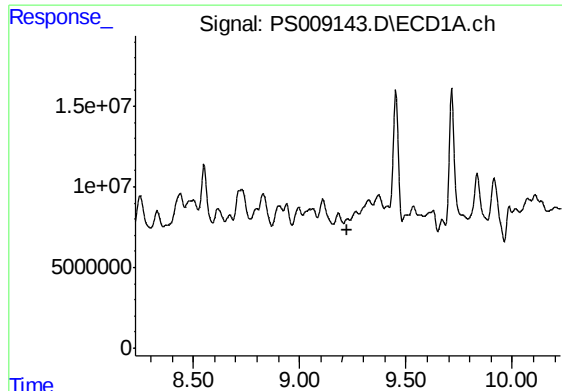

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.227 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CR-3

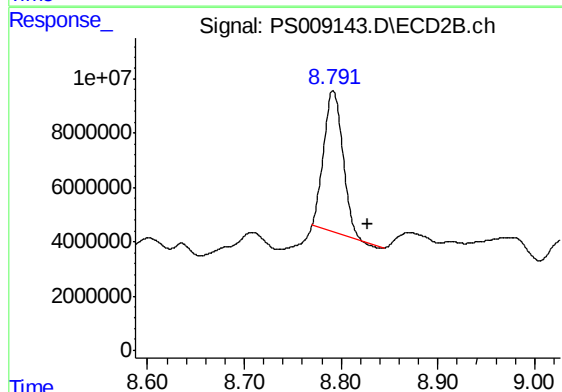


#11 2,4,5-TP (SILVEX)

R.T.: 8.792 min
Delta R.T.: -0.036 min
Response: 71769139
Conc: 13.25 ng/ml

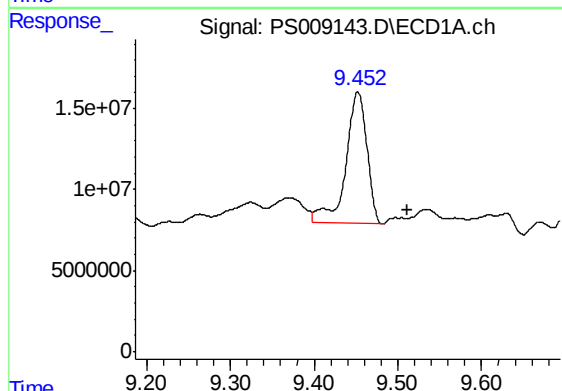


#12 2,4,5-T

R.T.: 9.452 min
Delta R.T.: -0.059 min
Response: 142280835
Conc: 13.31 ng/ml

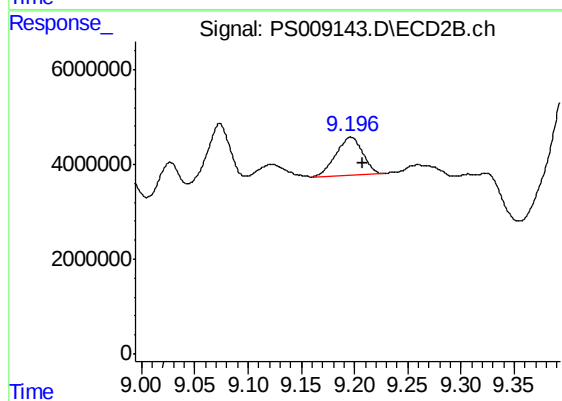

#12 2,4,5-T


R.T.: 9.196 min
Delta R.T.: -0.011 min
Response: 14078464
Conc: 2.60 ng/ml

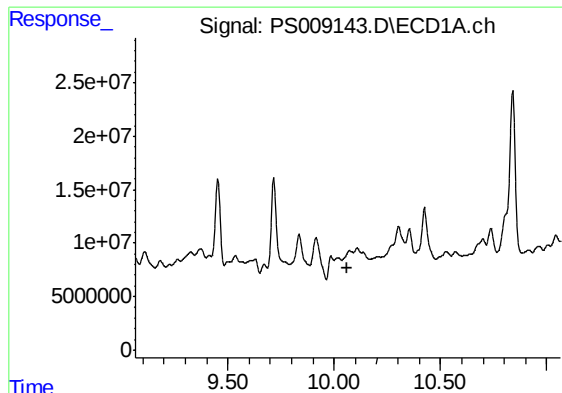

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 10.064 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CR-3

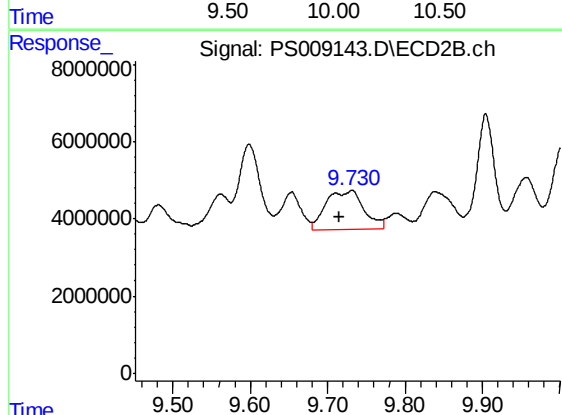


#13 2,4-DB

R.T.: 9.731 min
Delta R.T.: 0.016 min
Response: 34189617
Conc: 48.67 ng/ml

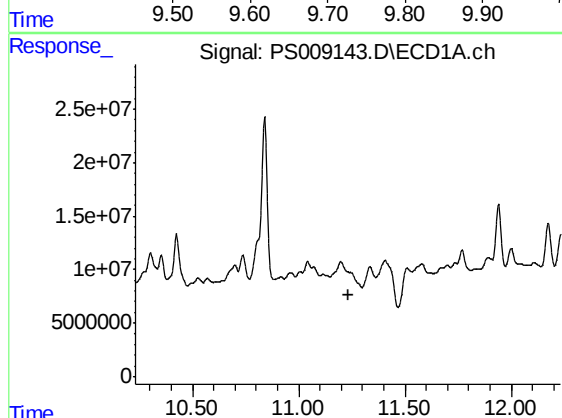


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.231 min
Response: 0
Conc: N.D.

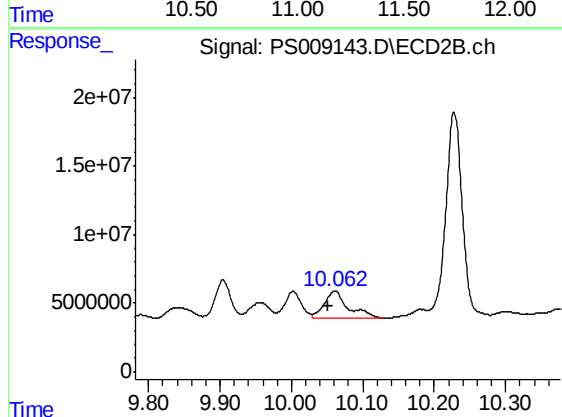

#14 DINOSEB


R.T.: 10.061 min
Delta R.T.: 0.009 min
Response: 46417445
Conc: 11.74 ng/ml

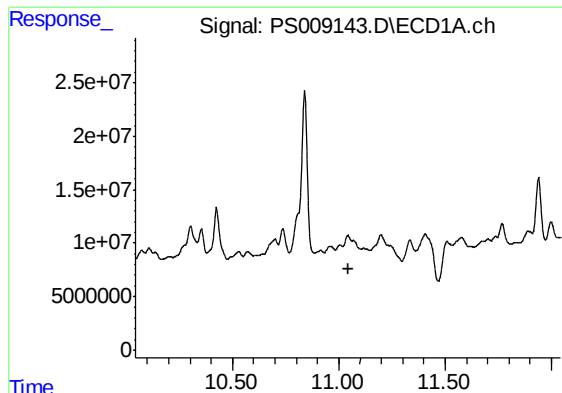

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 11.043 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CR-3

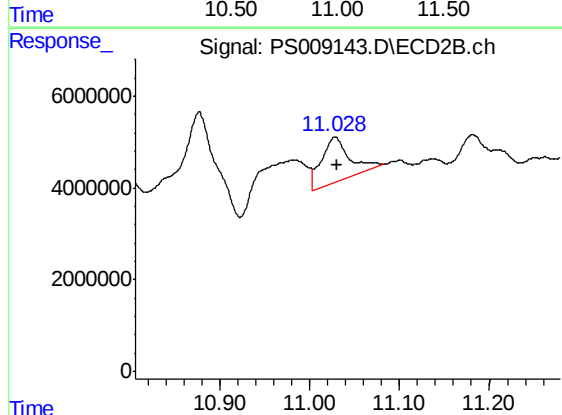


#15 Picloram

R.T.: 11.028 min
Delta R.T.: -0.003 min
Response: 21206066
Conc: 2.92 ng/ml

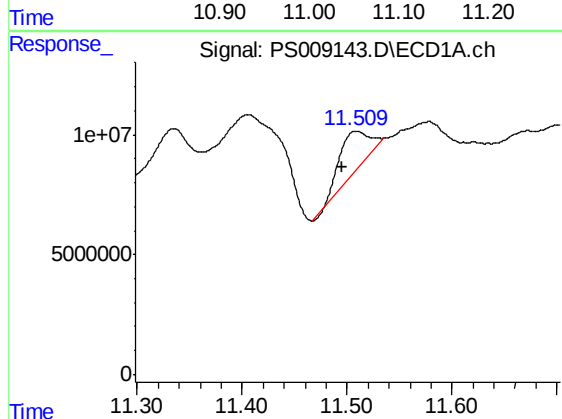

#16 DCPA

R.T.: 11.509 min
Delta R.T.: 0.015 min
Response: 32129713
Conc: 2.34 ng/ml

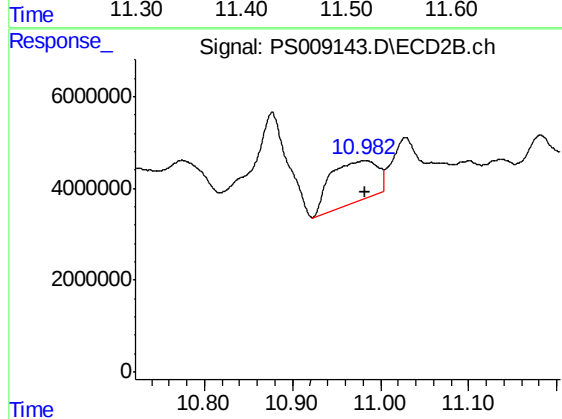

#16 DCPA

R.T.: 10.983 min
Delta R.T.: 0.000 min
Response: 32709675
Conc: 4.73 ng/ml