

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030620\
 Data File : PS009150.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Mar 2020 15:43
 Operator : DD\AJ
 Sample : L1778-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 DN1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 06 17:08:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.218	0.000	53226799	0	24.342	N.D. #
Target Compounds							
2) T	3,5-DICHL...	0.000	6.113	0 99047176		N.D.	67.874
3) T	4-Nitroph...	0.000	6.568	0 47362554		N.D.	81.937
7) T	MCPA	7.798	7.406	463.9E6 229.7E6		57.671	51.907
8) T	DICHLORPROP	0.000	7.758	0 71122089		N.D.	70.985
11) T	2,4,5-TP ...	0.000	8.792	0 68582982		N.D.	12.661
12) T	2,4,5-T	9.451	0.000	77134401 0		7.214	N.D. #
14) T	DINOSEB	0.000	10.061	0 20725161		N.D.	5.241
15) T	Picloram	0.000	11.028	0 59682224		N.D.	8.213
16) T	DCPA	0.000	11.028	0 59682224		N.D.	8.625



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030620\
Data File : PS009150.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2020 15:43
Operator : DD\AJ
Sample : L1778-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
DN1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 06 17:08:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

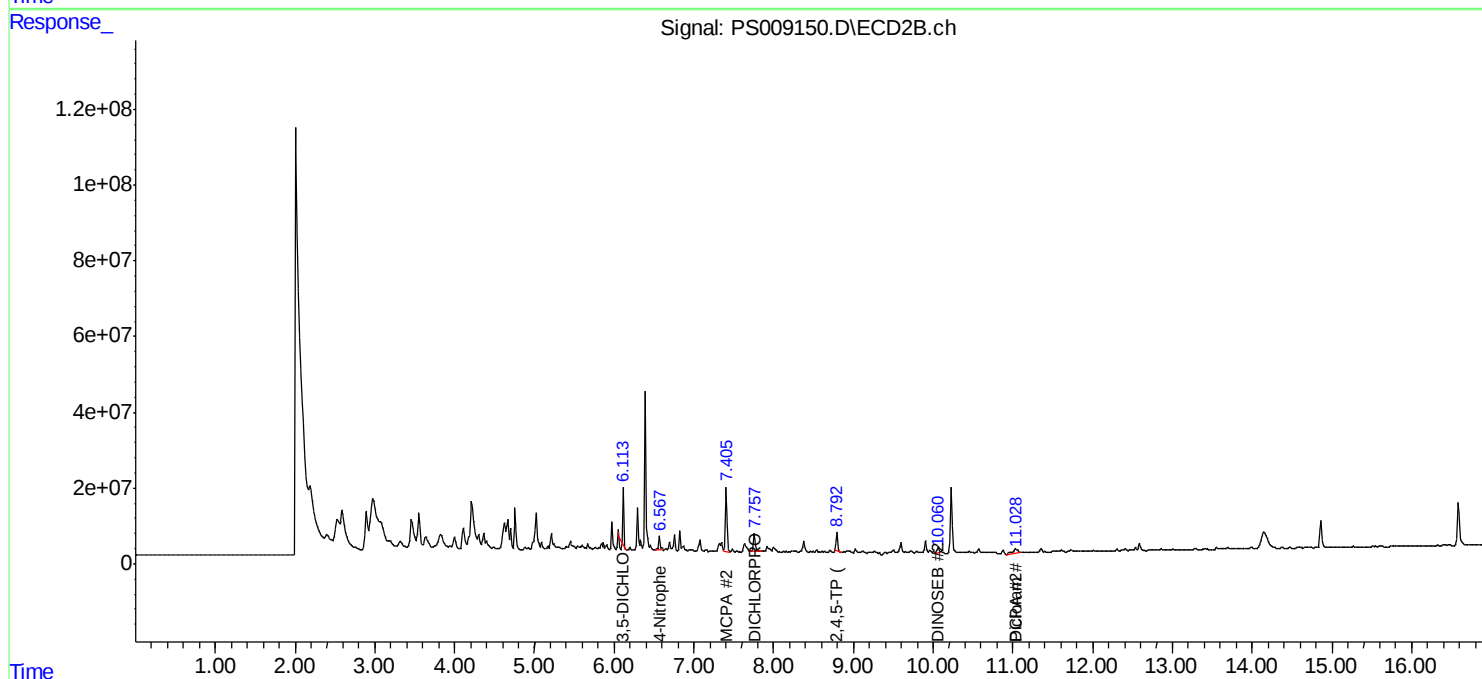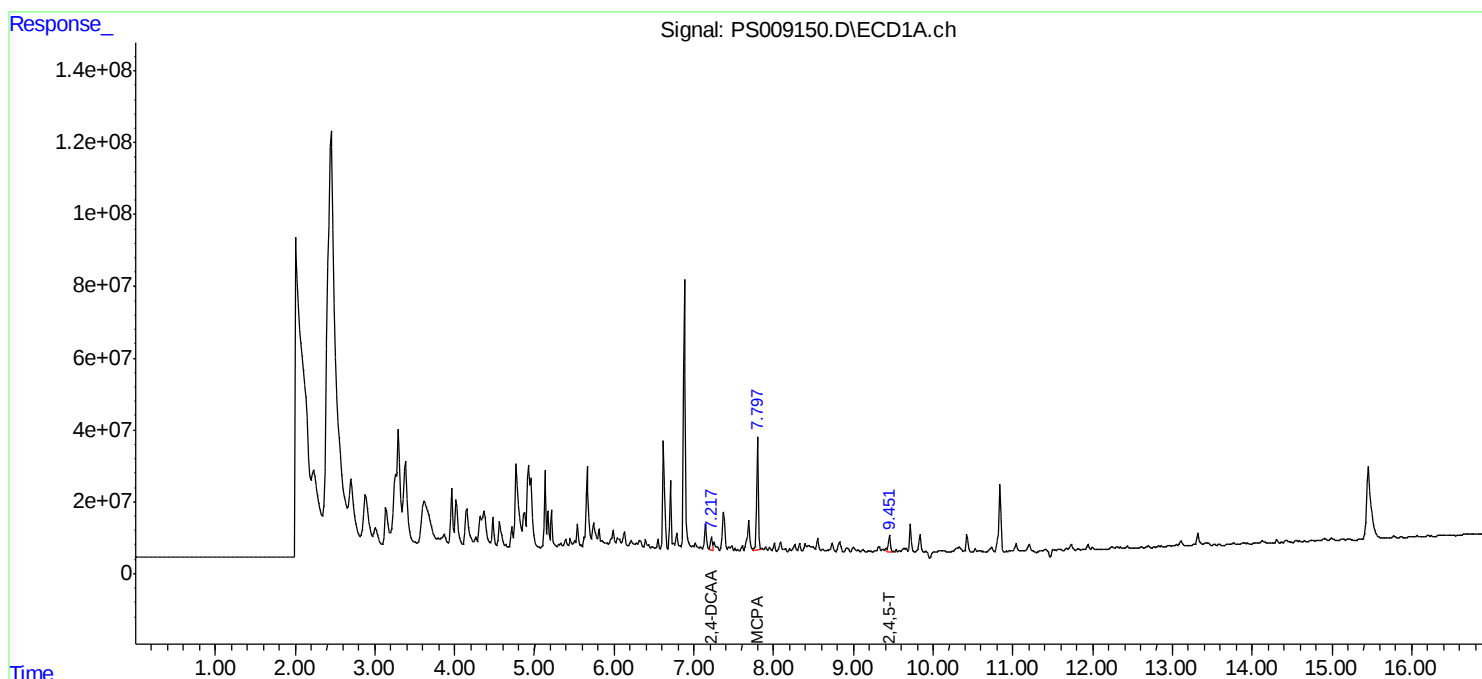


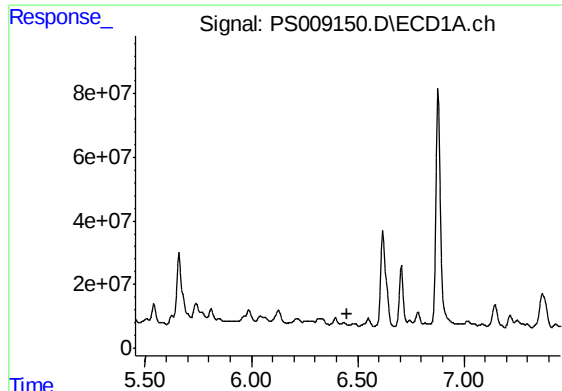

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
DN1

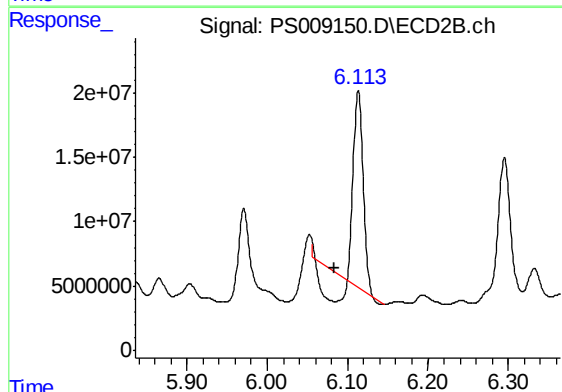


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.113 min
Delta R.T.: 0.030 min
Response: 99047176
Conc: 67.87 ng/ml

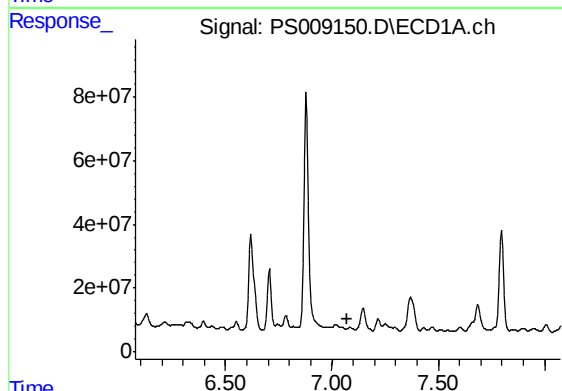


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 7.075 min
Response: 0
Conc: N.D.

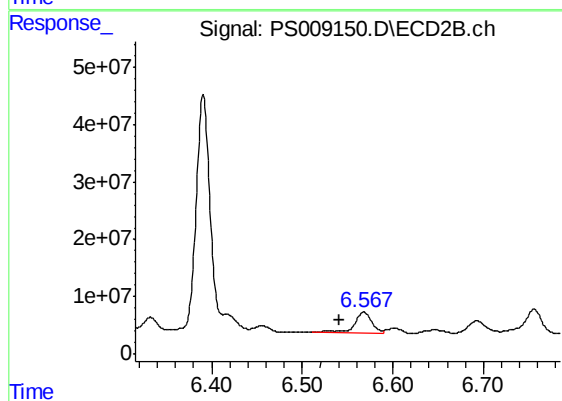

#3 4-Nitrophenol


R.T.: 6.568 min
Delta R.T.: 0.027 min
Response: 47362554
Conc: 81.94 ng/ml

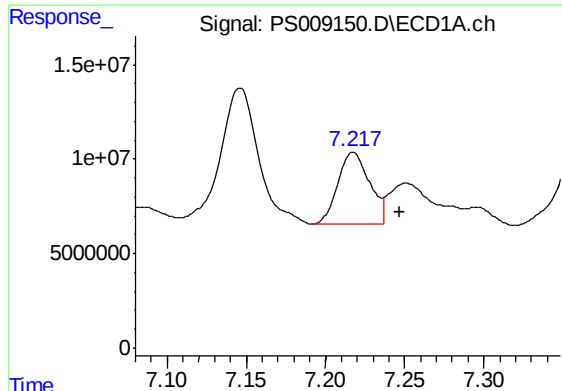

#4 2,4-DCAA


R.T.: 7.218 min
Delta R.T.: -0.029 min
Response: 53226799
Conc: 24.34 ng/ml

Instrument :
ECD_S
ClientSampleId :
DN1

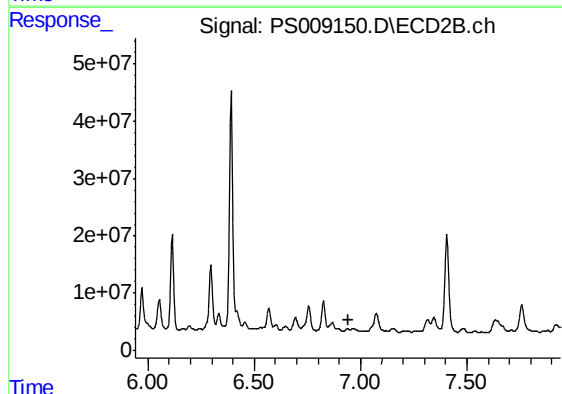


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.940 min
Response: 0
Conc: N.D.

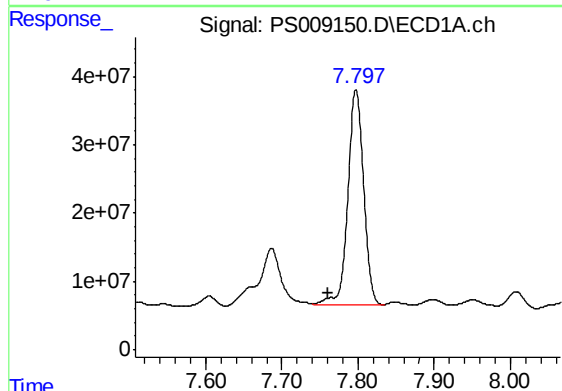


#7 MCPA

R.T.: 7.798 min
Delta R.T.: 0.037 min
Response: 463898978
Conc: 57.67 ug/ml

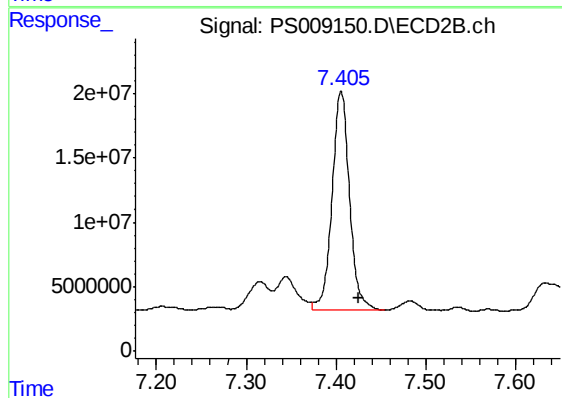

#7 MCPA


R.T.: 7.406 min
Delta R.T.: -0.020 min
Response: 229650171
Conc: 51.91 ug/ml

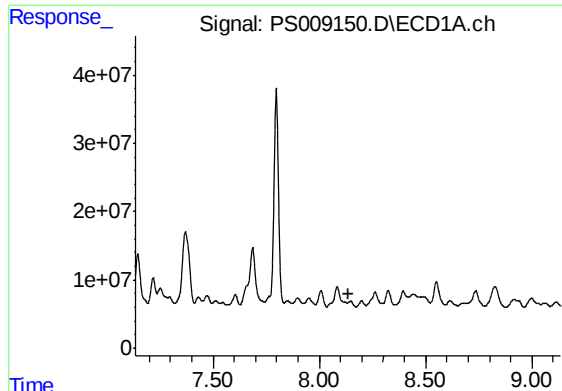

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 8.135 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
DN1

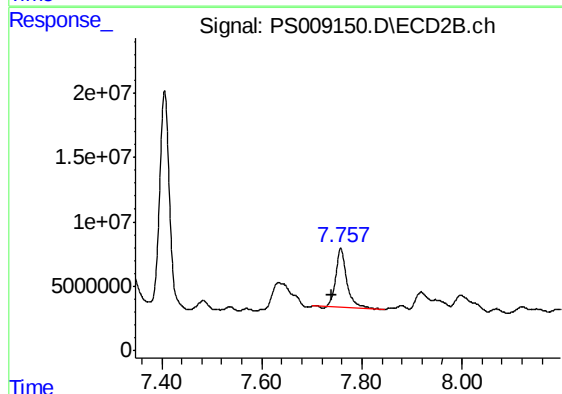


#8 DICHLORPROP

R.T.: 7.758 min
Delta R.T.: 0.019 min
Response: 71122089
Conc: 70.98 ng/ml

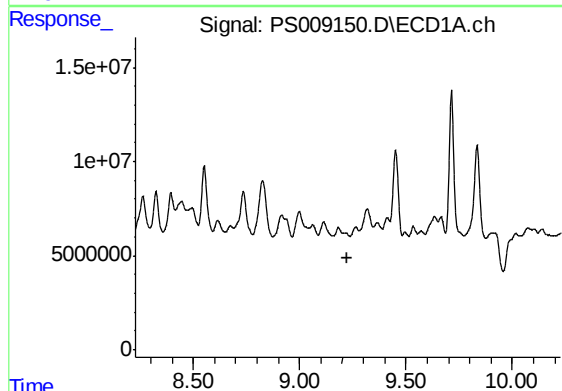


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.227 min
Response: 0
Conc: N.D.

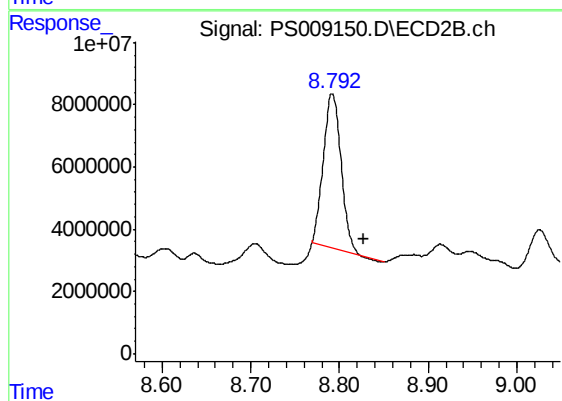

#11 2,4,5-TP (SILVEX)


R.T.: 8.792 min
Delta R.T.: -0.036 min
Response: 68582982
Conc: 12.66 ng/ml

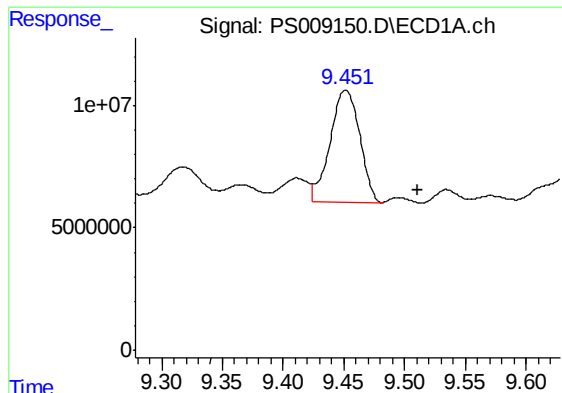

#12 2,4,5-T


R.T.: 9.451 min
Delta R.T.: -0.060 min
Response: 77134401
Conc: 7.21 ng/ml

Instrument :
ECD_S
ClientSampleId :
DN1

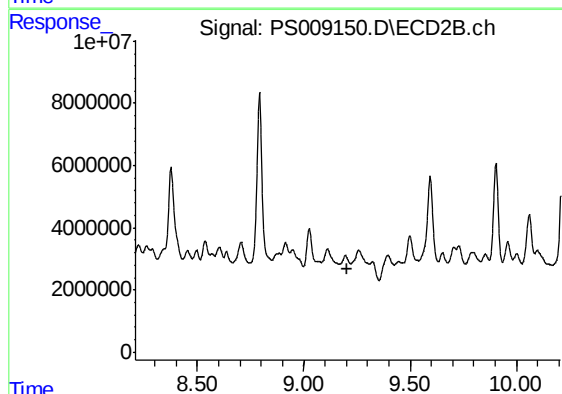


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.208 min
Response: 0
Conc: N.D.

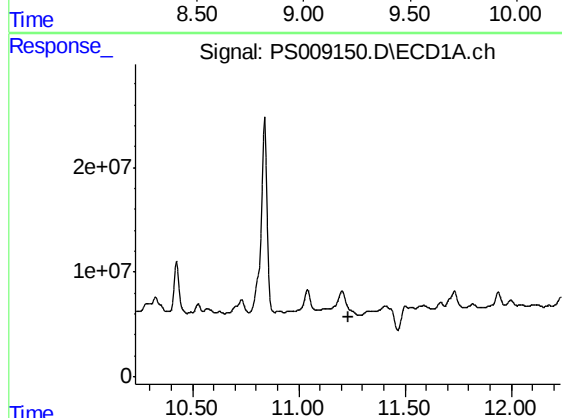


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.231 min
Response: 0
Conc: N.D.

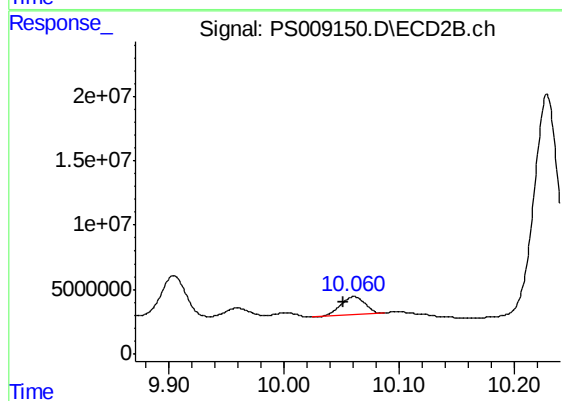

#14 DINOSEB


R.T.: 10.061 min
Delta R.T.: 0.009 min
Response: 20725161
Conc: 5.24 ng/ml

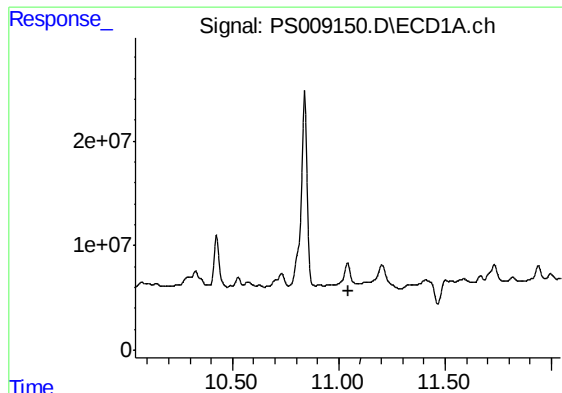

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 11.043 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
DN1

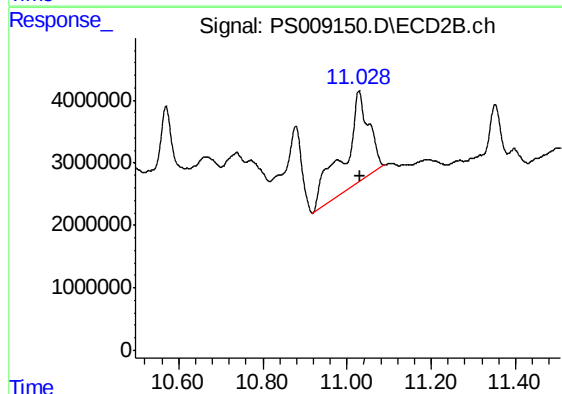


#15 Picloram

R.T.: 11.028 min
Delta R.T.: -0.003 min
Response: 59682224
Conc: 8.21 ng/ml

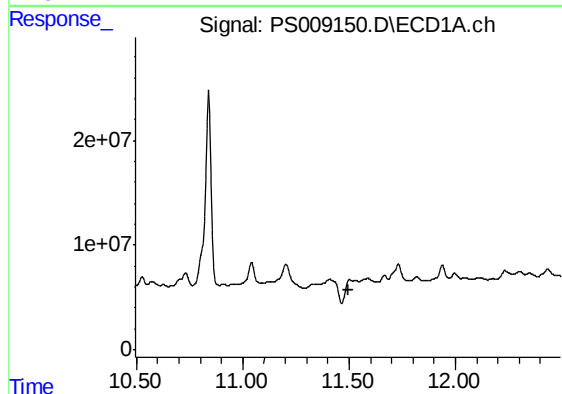

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.495 min
Response: 0
Conc: N.D.

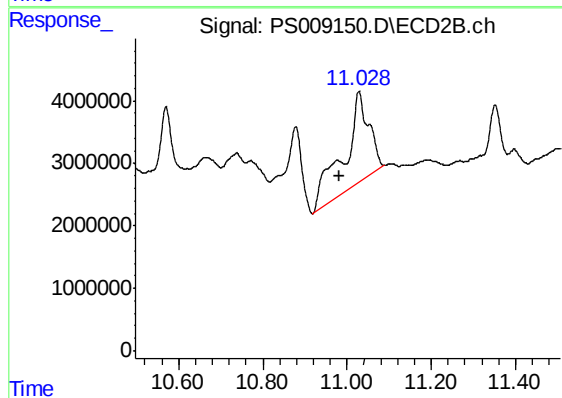

#16 DCPA

R.T.: 11.028 min
Delta R.T.: 0.046 min
Response: 59682224
Conc: 8.63 ng/ml