

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030620\
 Data File : PS009151.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Mar 2020 16:08
 Operator : DD\AJ
 Sample : L1778-07
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 DN2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 06 17:08:48 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.247	6.938	405.3E6	173.9E6	185.375	180.474
Target Compounds							
1) T	Dalapon	0.000	2.588	0 49624111		N.D.	33.938
2) T	3,5-DICHL...	0.000	6.113	0 157.0E6		N.D.	107.558
7) T	MCPA	7.799	7.405	248.6E6	155.0E6	30.909	35.043
8) T	DICHLORPROP	0.000	7.758	0 64069829		N.D.	63.946
10) T	Pentachlo...	0.000	8.462	0 20536741		N.D.	1.445
11) T	2,4,5-TP ...	0.000	8.791	0 49934479		N.D.	9.218
12) T	2,4,5-T	9.453	0.000	103.6E6	0	9.690	N.D. #
13) T	2,4-DB	0.000	9.732	0 20816079		N.D.	29.634
14) T	DINOSEB	0.000	10.061	0 28710574		N.D.	7.261
15) T	Picloram	0.000	11.028	0 5554153		N.D.	<MDL
16) T	DCPA	0.000	11.028	0 5554153		N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030620\
Data File : PS009151.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2020 16:08
Operator : DD\AJ
Sample : L1778-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
DN2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 06 17:08:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

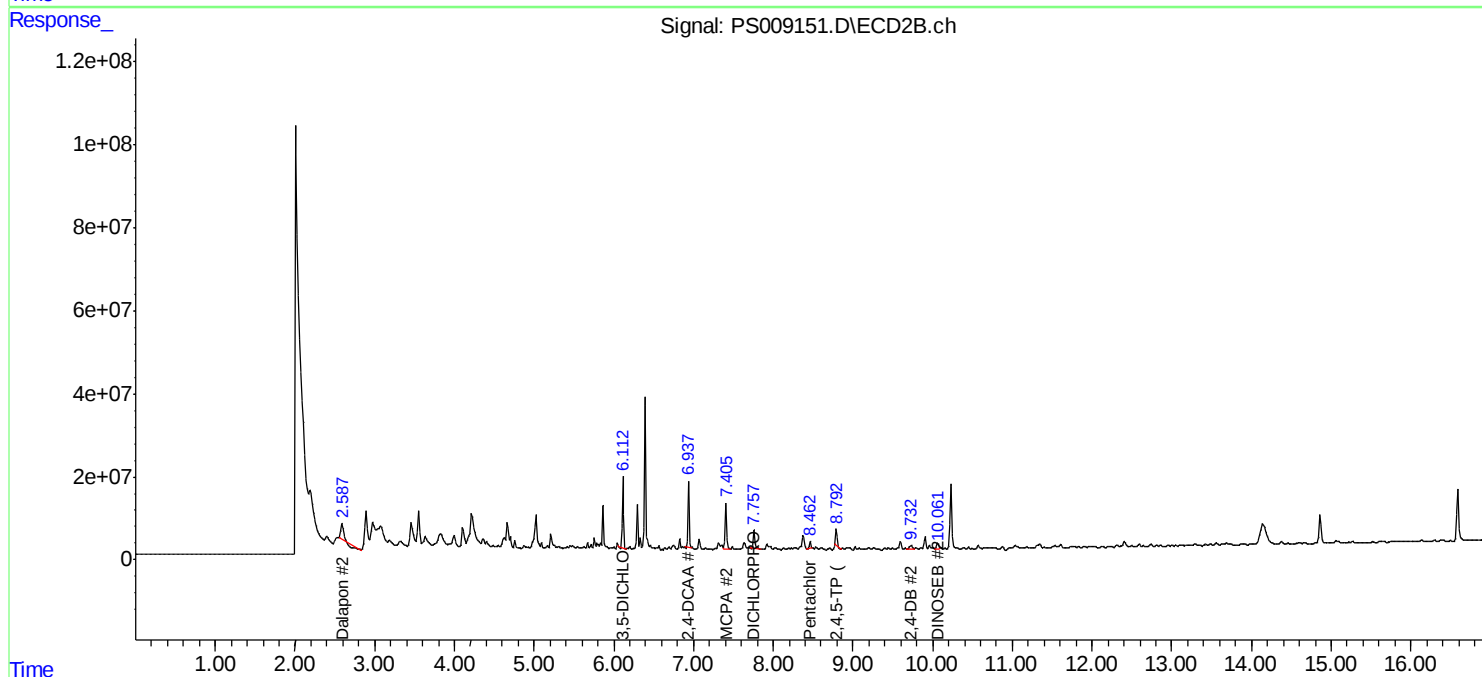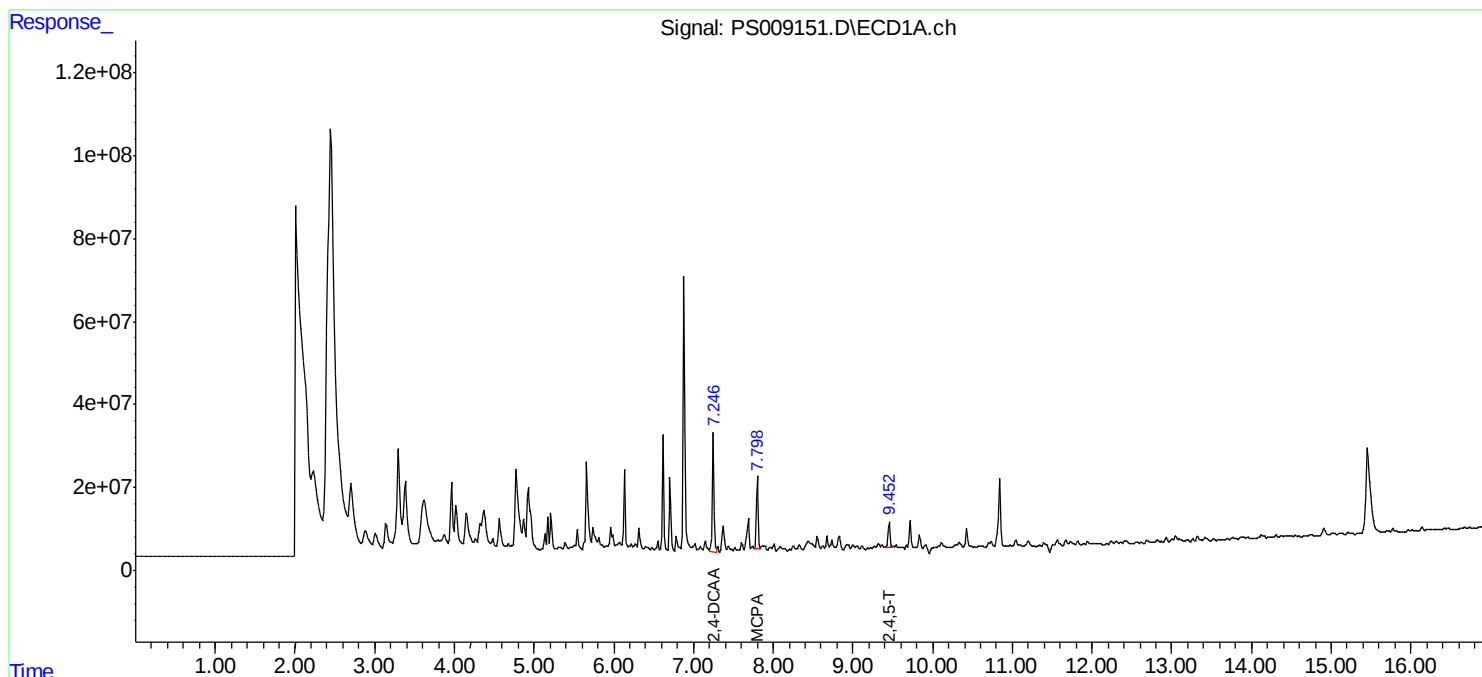


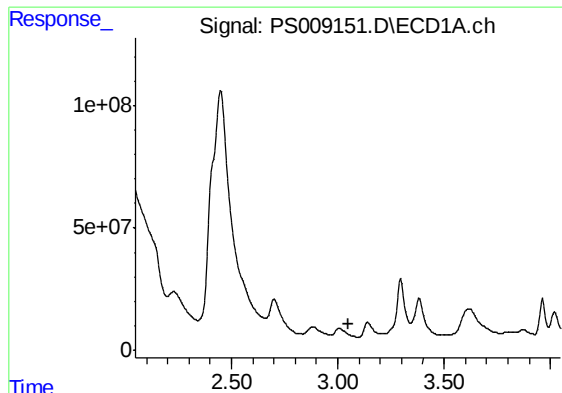

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 3.048 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
DN2

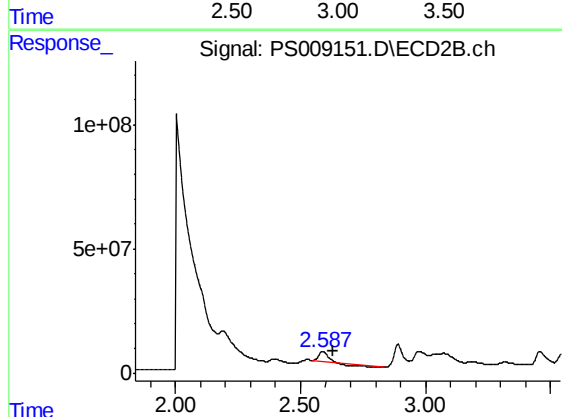


#1 Dalapon

R.T.: 2.588 min
Delta R.T.: -0.042 min
Response: 49624111
Conc: 33.94 ng/ml

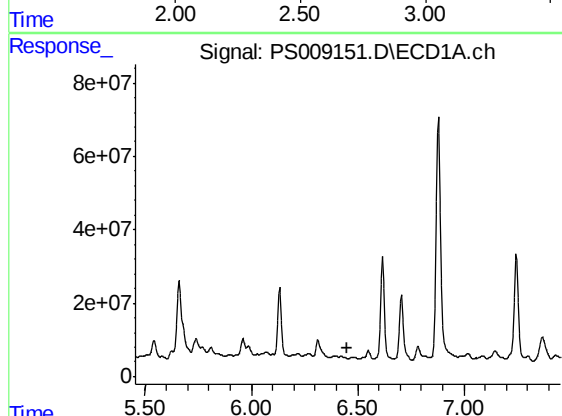


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.455 min
Response: 0
Conc: N.D.

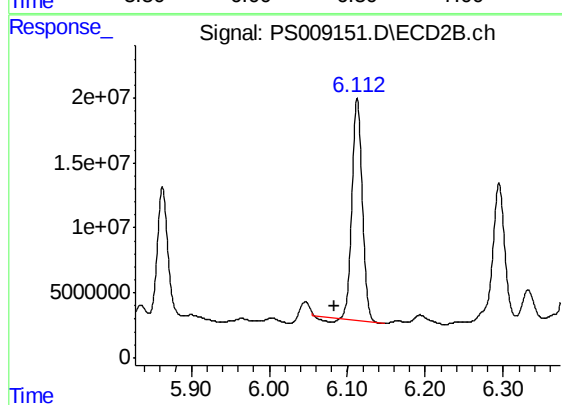

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.113 min
Delta R.T.: 0.029 min
Response: 156956645
Conc: 107.56 ng/ml

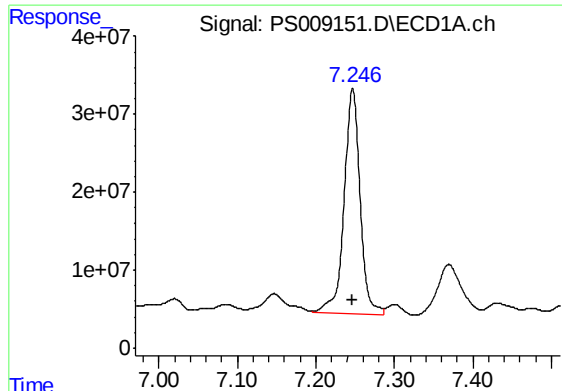

#4 2,4-DCAA


R.T.: 7.247 min
Delta R.T.: 0.000 min
Response: 405339922
Conc: 185.38 ng/ml

Instrument :
ECD_S
ClientSampleId :
DN2

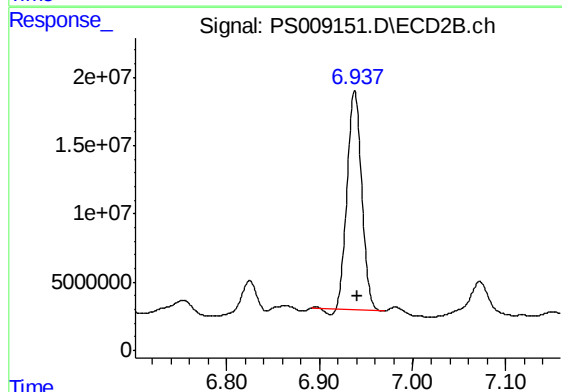


#4 2,4-DCAA

R.T.: 6.938 min
Delta R.T.: -0.003 min
Response: 173896554
Conc: 180.47 ng/ml

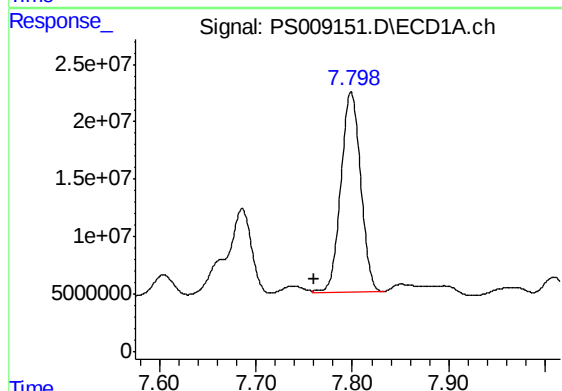


#7 MCPA

R.T.: 7.799 min
Delta R.T.: 0.038 min
Response: 248632031
Conc: 30.91 ug/ml

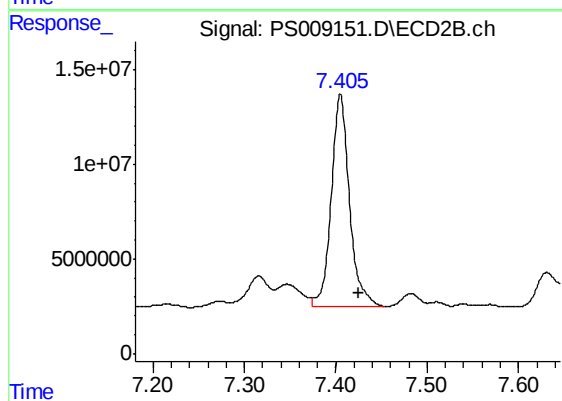

#7 MCPA


R.T.: 7.405 min
Delta R.T.: -0.020 min
Response: 155038049
Conc: 35.04 ug/ml

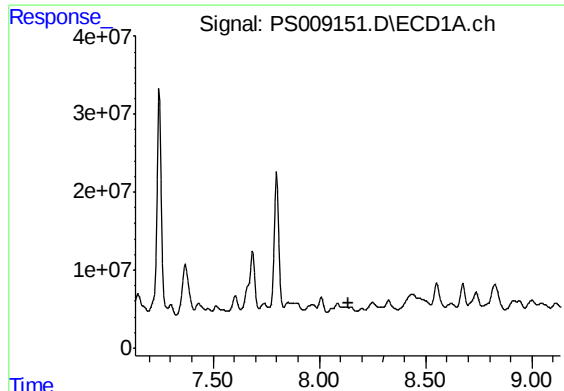

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.135 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
DN2

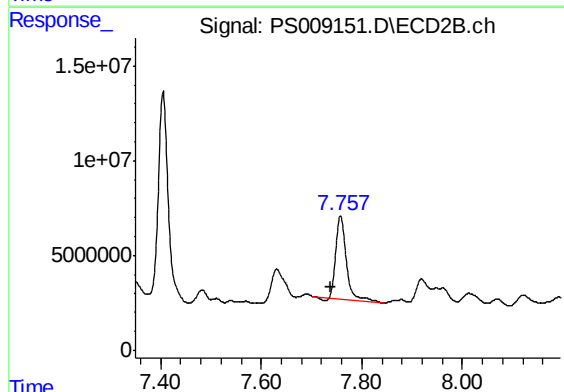


#8 DICHLORPROP

R.T.: 7.758 min
Delta R.T.: 0.019 min
Response: 64069829
Conc: 63.95 ng/ml

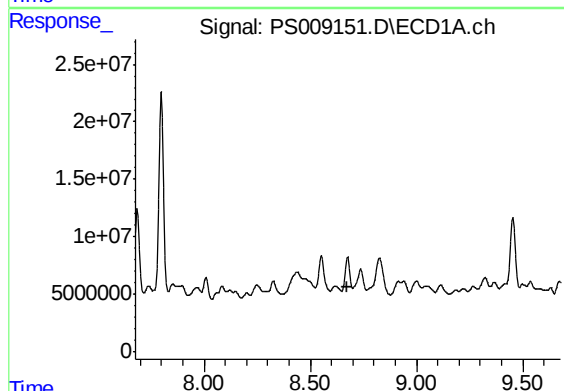


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 8.677 min
Response: 0
Conc: N.D.

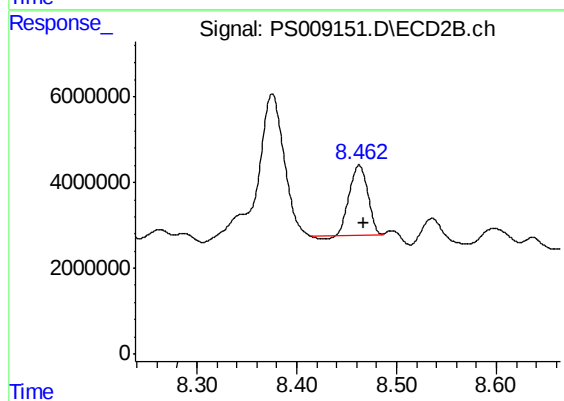

#10 Pentachlorophenol


R.T.: 8.462 min
Delta R.T.: -0.004 min
Response: 20536741
Conc: 1.45 ng/ml

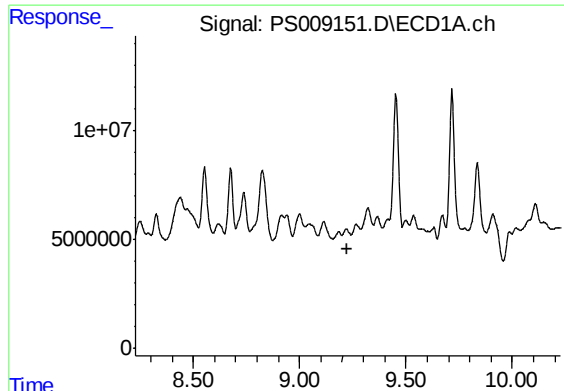

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 9.227 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
DN2

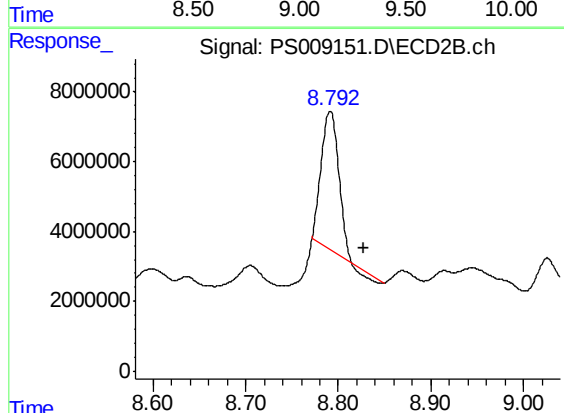


#11 2,4,5-TP (SILVEX)

R.T.: 8.791 min
Delta R.T.: -0.037 min
Response: 49934479
Conc: 9.22 ng/ml

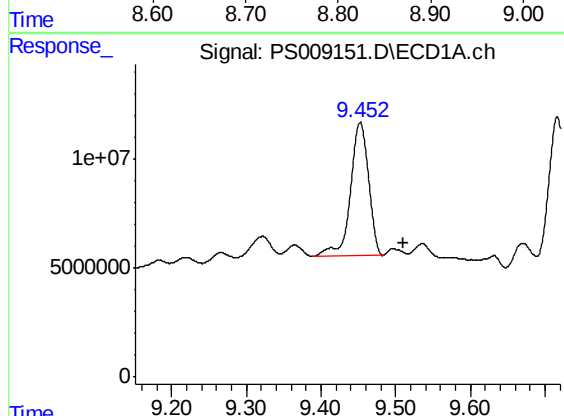


#12 2,4,5-T

R.T.: 9.453 min
Delta R.T.: -0.058 min
Response: 103606290
Conc: 9.69 ng/ml

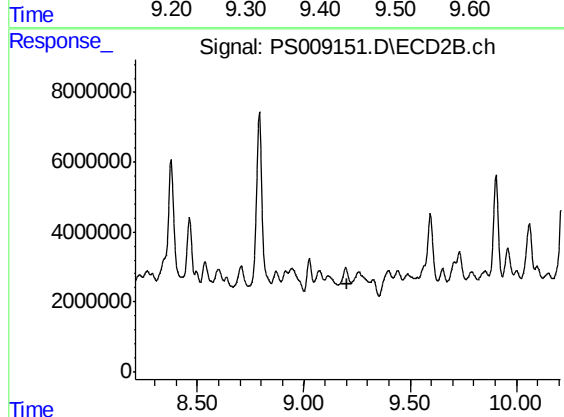

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 9.208 min
Response: 0
Conc: N.D.

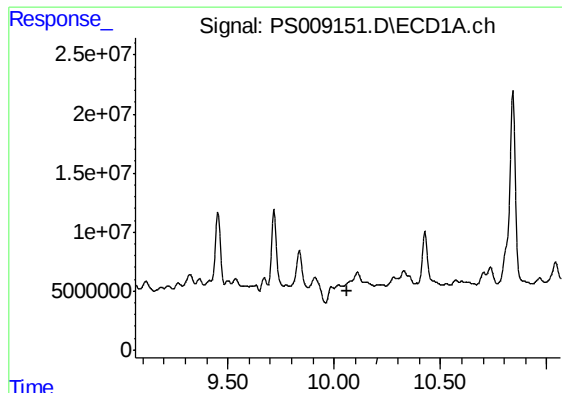

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 10.064 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
DN2

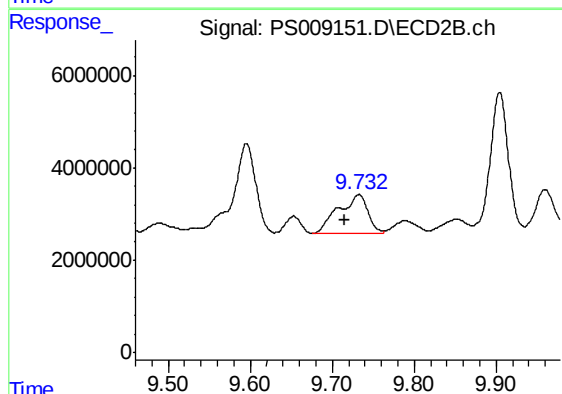


#13 2,4-DB

R.T.: 9.732 min
Delta R.T.: 0.017 min
Response: 20816079
Conc: 29.63 ng/ml

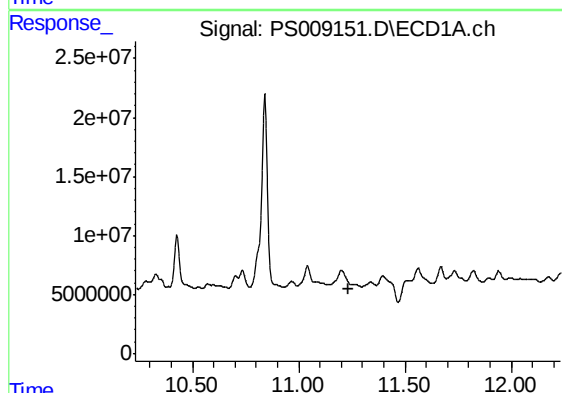

#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.231 min
Response: 0
Conc: N.D.

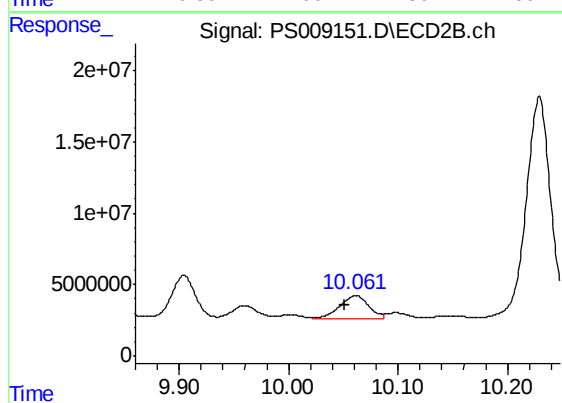

#14 DINOSEB

R.T.: 10.061 min
Delta R.T.: 0.010 min
Response: 28710574
Conc: 7.26 ng/ml