

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030620\
 Data File : PS009152.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Mar 2020 16:31
 Operator : DD\AJ
 Sample : L1778-09
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 S3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 06 17:09:02 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	6.937	0	12425441	N.D.	12.895
Target Compounds							
1) T	Dalapon	0.000	2.589	0	226.3E6	N.D.	154.785
2) T	3,5-DICHL...	0.000	6.113	0	160.1E6	N.D.	109.708
3) T	4-Nitroph...	0.000	6.568	0	21354796	N.D.	36.944
7) T	MCPA	7.798	7.406	238.6E6	135.4E6	29.668	30.612
8) T	DICHLORPROP	0.000	7.758	0	72717474	N.D.	72.577
10) T	Pentachlo...	8.740	8.497	73504191	42241805	2.533	2.973
11) T	2,4,5-TP ...	0.000	8.791	0	32891637	N.D.	6.072
12) T	2,4,5-T	9.452	0.000	82569991	0	7.723	N.D. #
14) T	DINOSEB	0.000	10.060	0	15284969	N.D.	3.866
15) T	Picloram	0.000	11.056	0	30229912	N.D.	4.160



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030620\
Data File : PS009152.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2020 16:31
Operator : DD\AJ
Sample : L1778-09
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
S3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 06 17:09:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

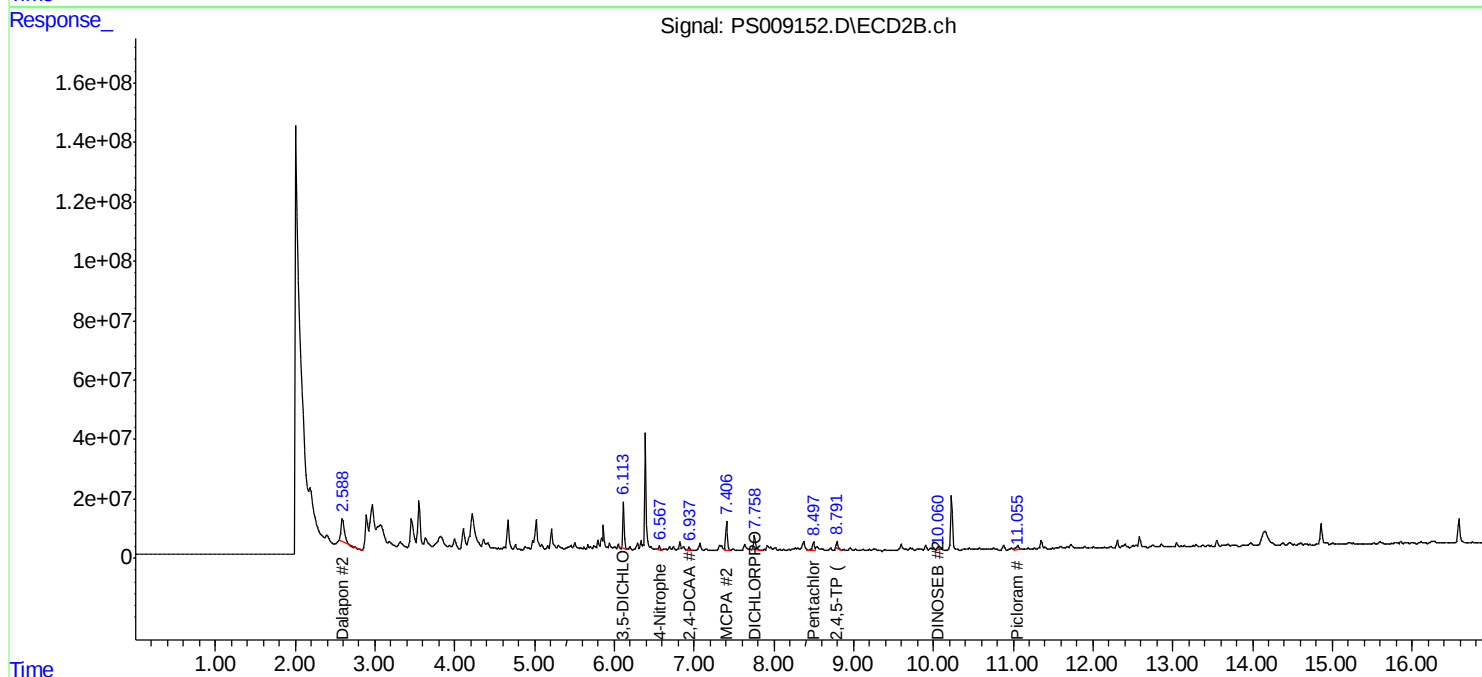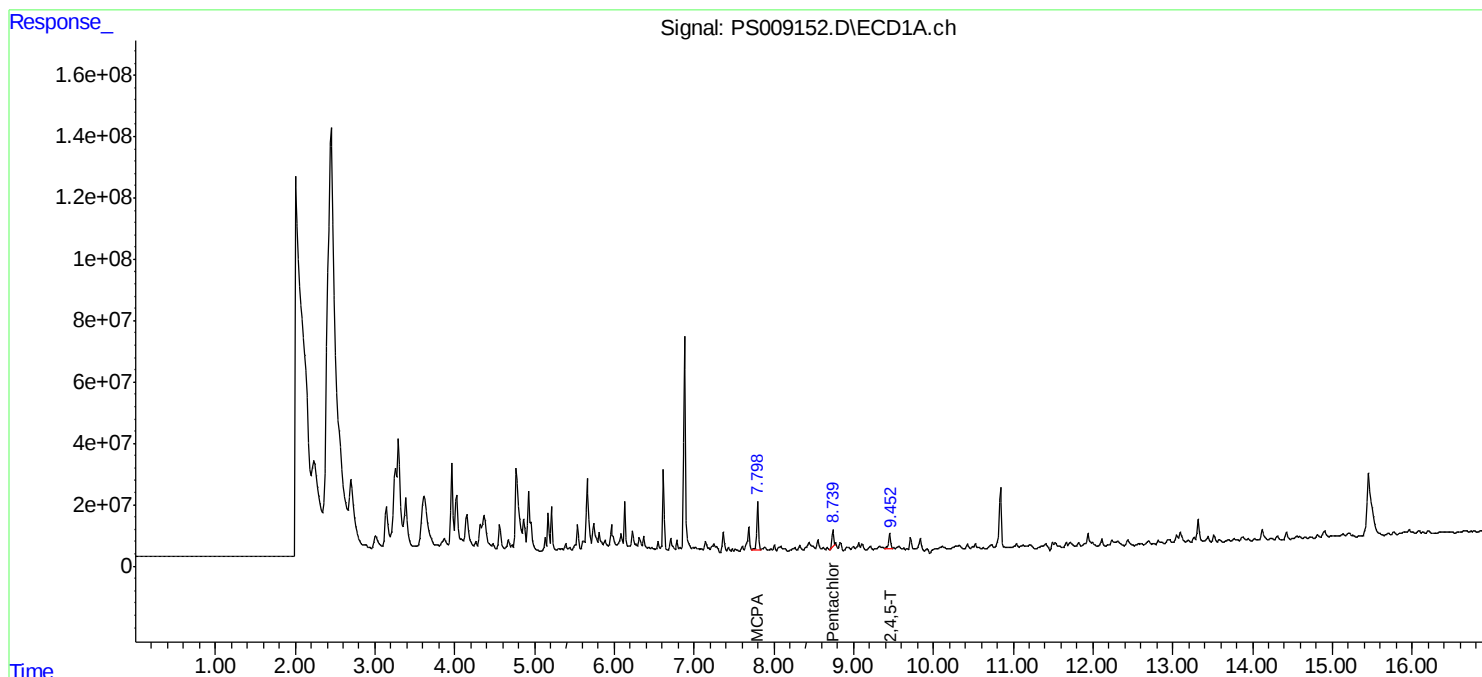


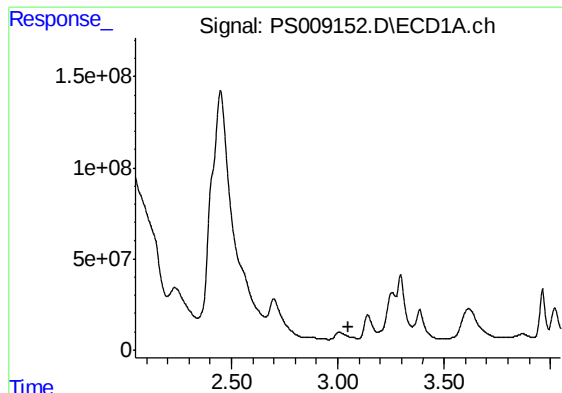

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 3.048 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
S3

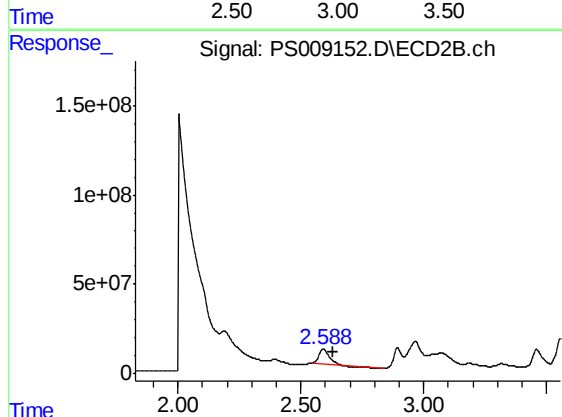


#1 Dalapon

R.T.: 2.589 min
Delta R.T.: -0.040 min
Response: 226329802
Conc: 154.79 ng/ml

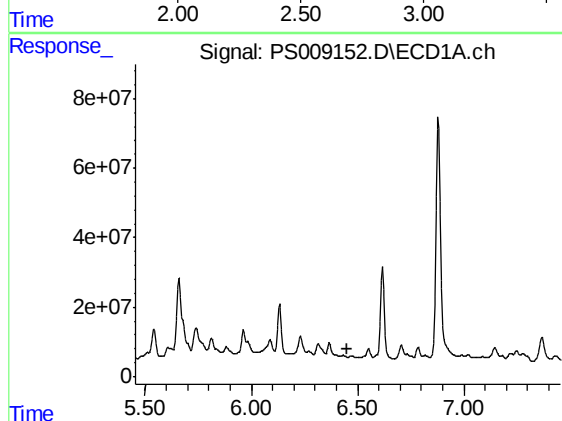


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.455 min
Response: 0
Conc: N.D.

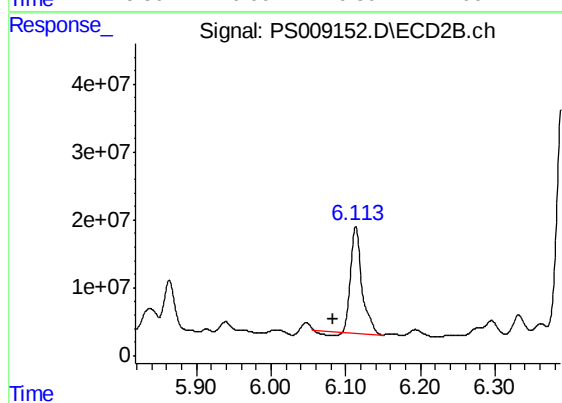

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.113 min
Delta R.T.: 0.030 min
Response: 160094314
Conc: 109.71 ng/ml

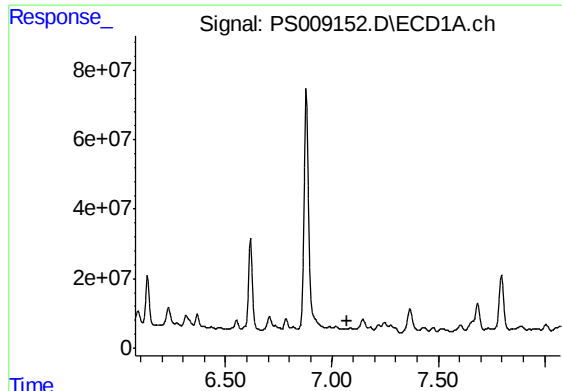

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.075 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
S3

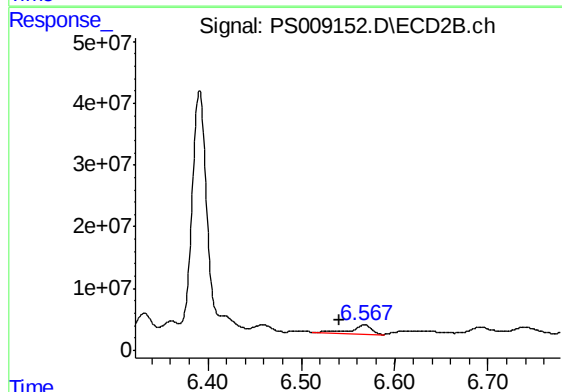


#3 4-Nitrophenol

R.T.: 6.568 min
Delta R.T.: 0.027 min
Response: 21354796
Conc: 36.94 ng/ml

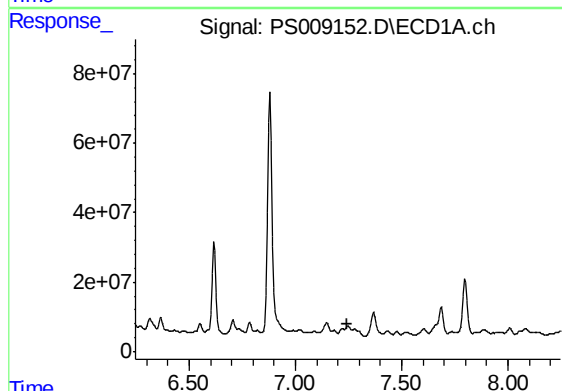


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 7.247 min
Response: 0
Conc: N.D.

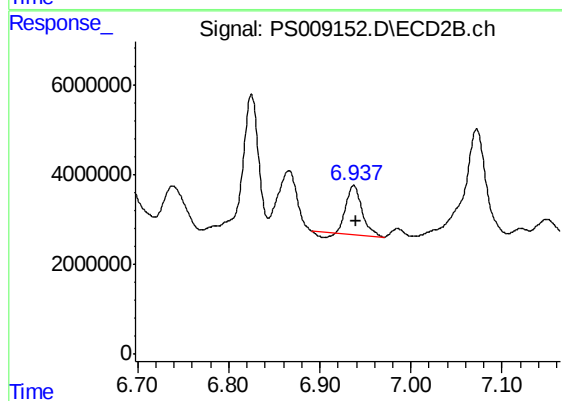

#4 2,4-DCAA


R.T.: 6.937 min
Delta R.T.: -0.003 min
Response: 12425441
Conc: 12.90 ng/ml

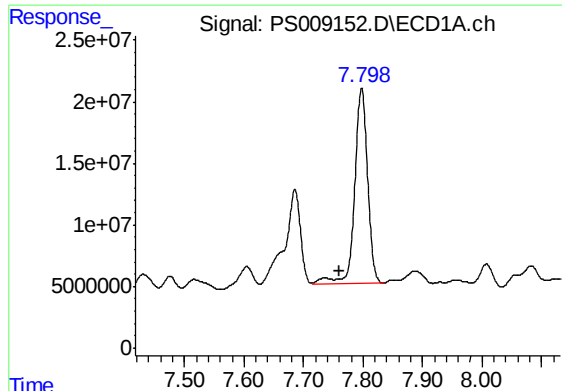

#7 MCPA


R.T.: 7.798 min
Delta R.T.: 0.037 min
Response: 238646542
Conc: 29.67 ug/ml

Instrument :
ECD_S
ClientSampleId :
S3

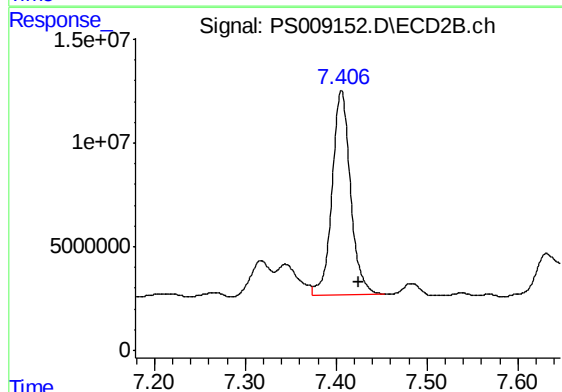


#7 MCPA

R.T.: 7.406 min
Delta R.T.: -0.020 min
Response: 135436853
Conc: 30.61 ug/ml

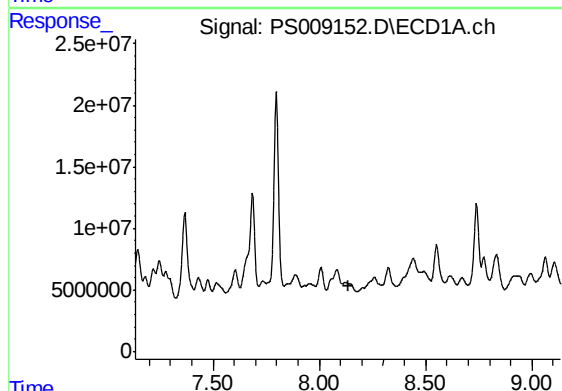


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.135 min
Response: 0
Conc: N.D.

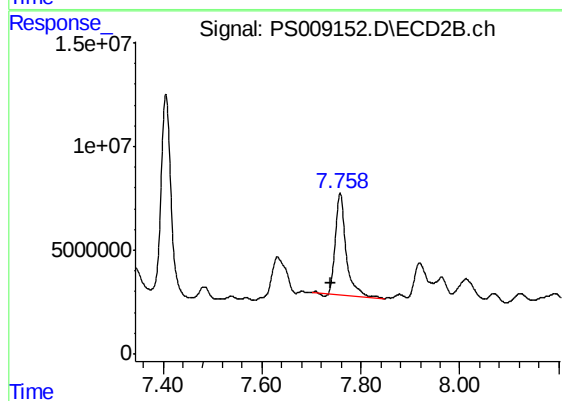

#8 DICHLORPROP


R.T.: 7.758 min
Delta R.T.: 0.019 min
Response: 72717474
Conc: 72.58 ng/ml

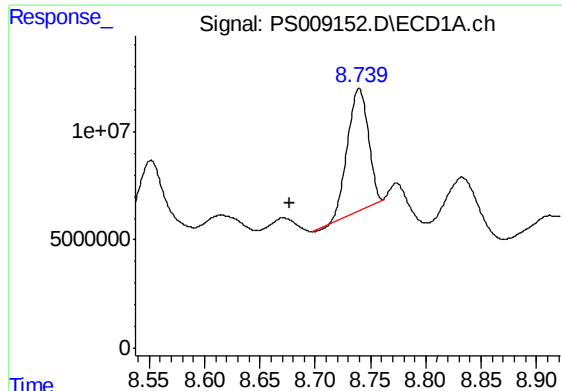

#10 Pentachlorophenol


R.T.: 8.740 min
Delta R.T.: 0.063 min
Response: 73504191
Conc: 2.53 ng/ml

Instrument :
ECD_S
ClientSampleId :
S3

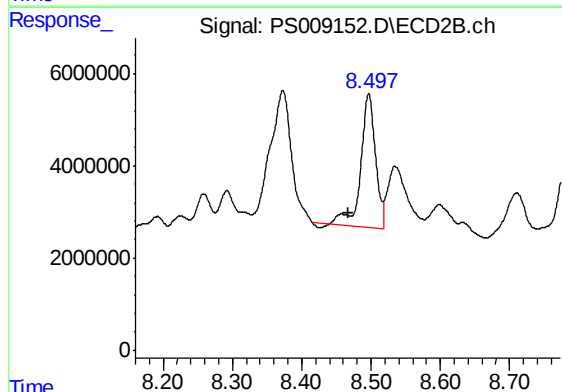


#10 Pentachlorophenol

R.T.: 8.497 min
Delta R.T.: 0.030 min
Response: 42241805
Conc: 2.97 ng/ml

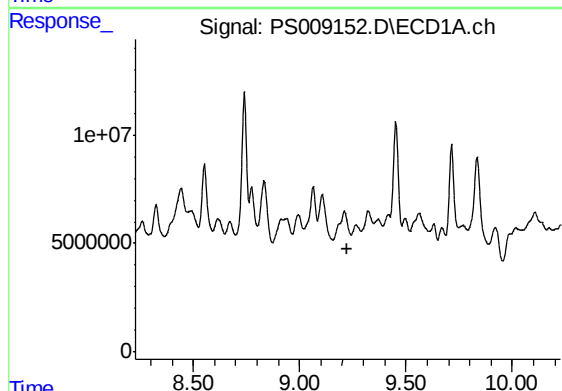


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.227 min
Response: 0
Conc: N.D.

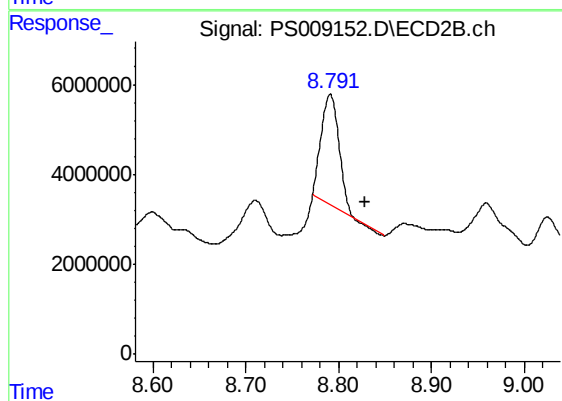

#11 2,4,5-TP (SILVEX)


R.T.: 8.791 min
Delta R.T.: -0.037 min
Response: 32891637
Conc: 6.07 ng/ml

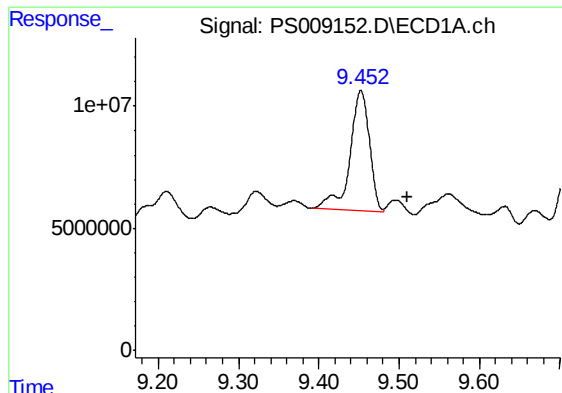

#12 2,4,5-T


R.T.: 9.452 min
Delta R.T.: -0.059 min
Response: 82569991
Conc: 7.72 ng/ml

Instrument :
ECD_S
ClientSampleId :
S3

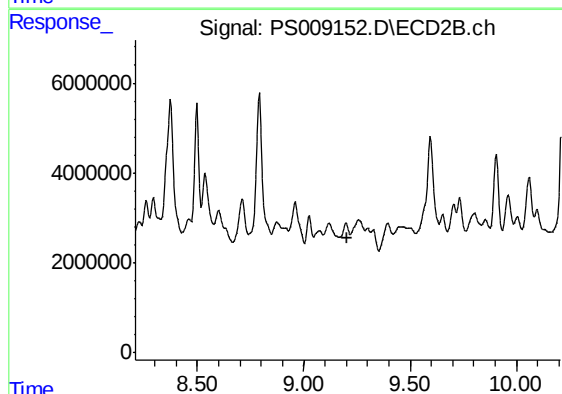


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.208 min
Response: 0
Conc: N.D.

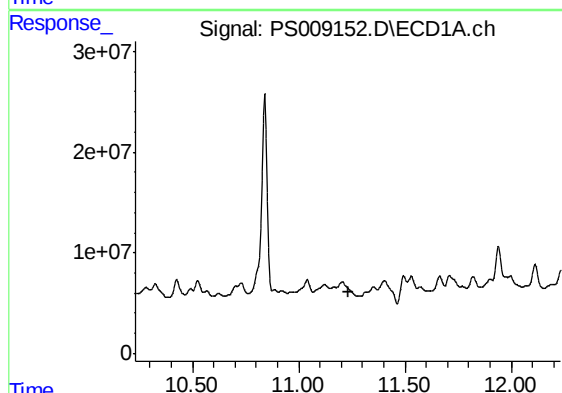


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.231 min
Response: 0
Conc: N.D.

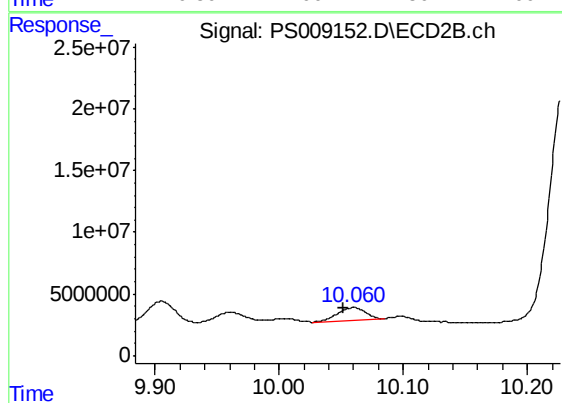

#14 DINOSEB


R.T.: 10.060 min
Delta R.T.: 0.008 min
Response: 15284969
Conc: 3.87 ng/ml

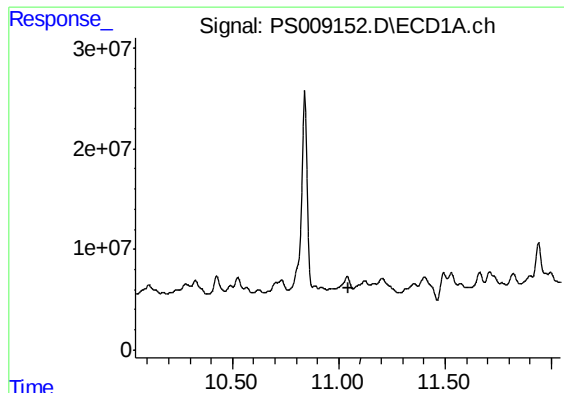

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.043 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
S3

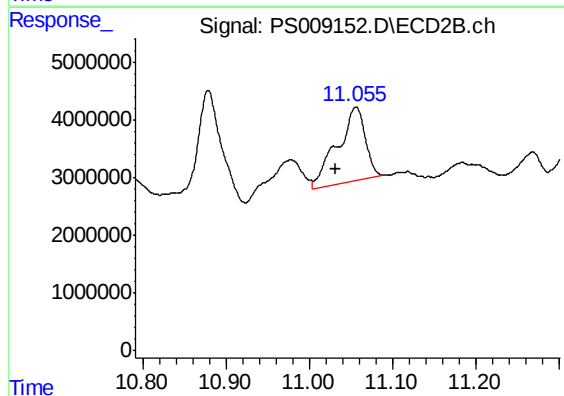

#15 Picloram

R.T.: 11.056 min
Delta R.T.: 0.025 min
Response: 30229912
Conc: 4.16 ng/ml