

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030620\
 Data File : PS009154.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Mar 2020 17:17
 Operator : DD\AJ
 Sample : L1778-13
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 06 23:23:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.245	6.938	223.8E6	84312555	102.362	87.502
Target Compounds							
1) T	Dalapon	0.000	2.589	0	194.9E6	N.D.	133.325
2) T	3,5-DICHL...	0.000	6.113	0	141.6E6	N.D.	97.027
3) T	4-Nitroph...	0.000	6.567	0	24836724	N.D.	42.967
7) T	MCPA	7.797	7.405	167.5E6	113.9E6	20.823	25.745
8) T	DICHLORPROP	0.000	7.758	0	61851788	N.D.	61.733
10) T	Pentachlo...	8.738	8.496	73413521	19466065	2.530	1.370 #
11) T	2,4,5-TP ...	0.000	8.789	0	35971512	N.D.	6.641
12) T	2,4,5-T	9.451	0.000	107.1E6	0	10.018	N.D. #
13) T	2,4-DB	10.107	9.733	172.7E6	33374793	119.698	47.513 #
14) T	DINOSEB	0.000	10.058	0	25180117	N.D.	6.368
15) T	Picloram	0.000	11.055	0	38234376	N.D.	5.262
16) T	DCPA	0.000	10.976	0	28457574	N.D.	4.113



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030620\
Data File : PS009154.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2020 17:17
Operator : DD\AJ
Sample : L1778-13
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 06 23:23:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

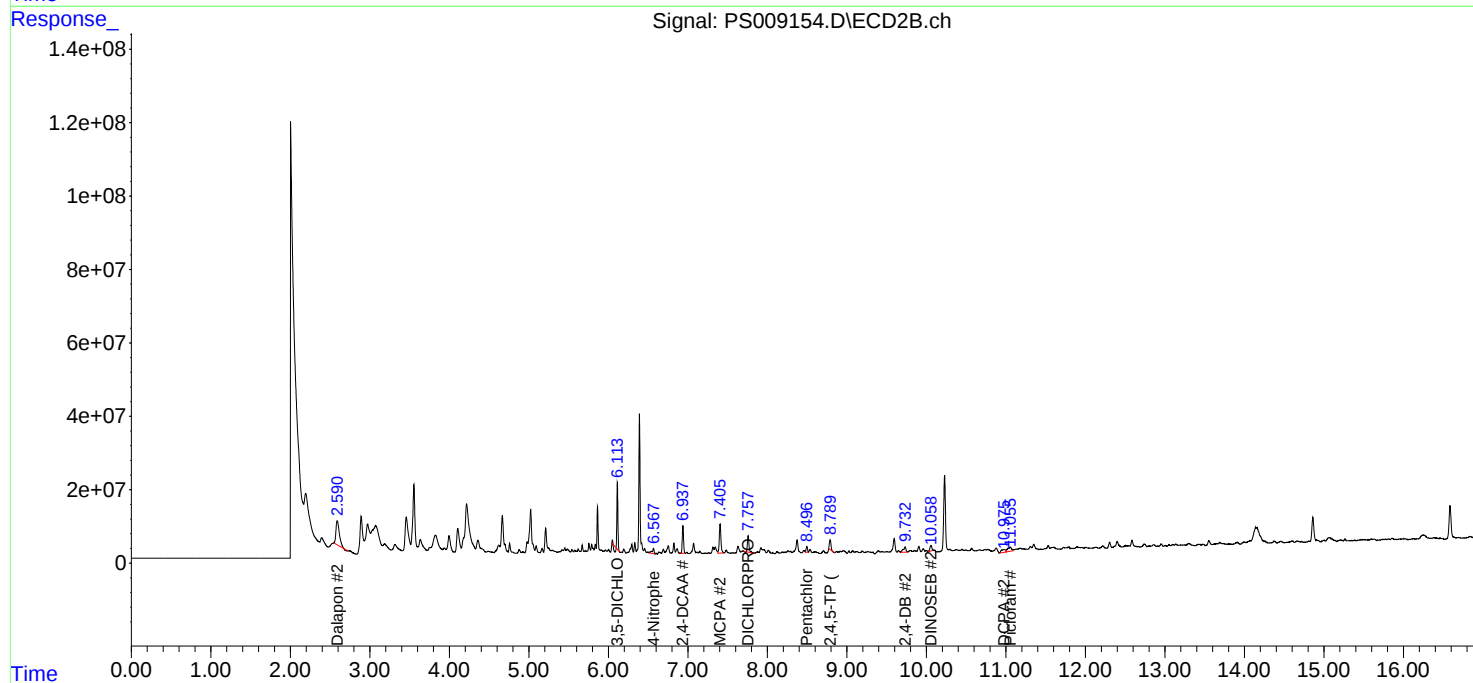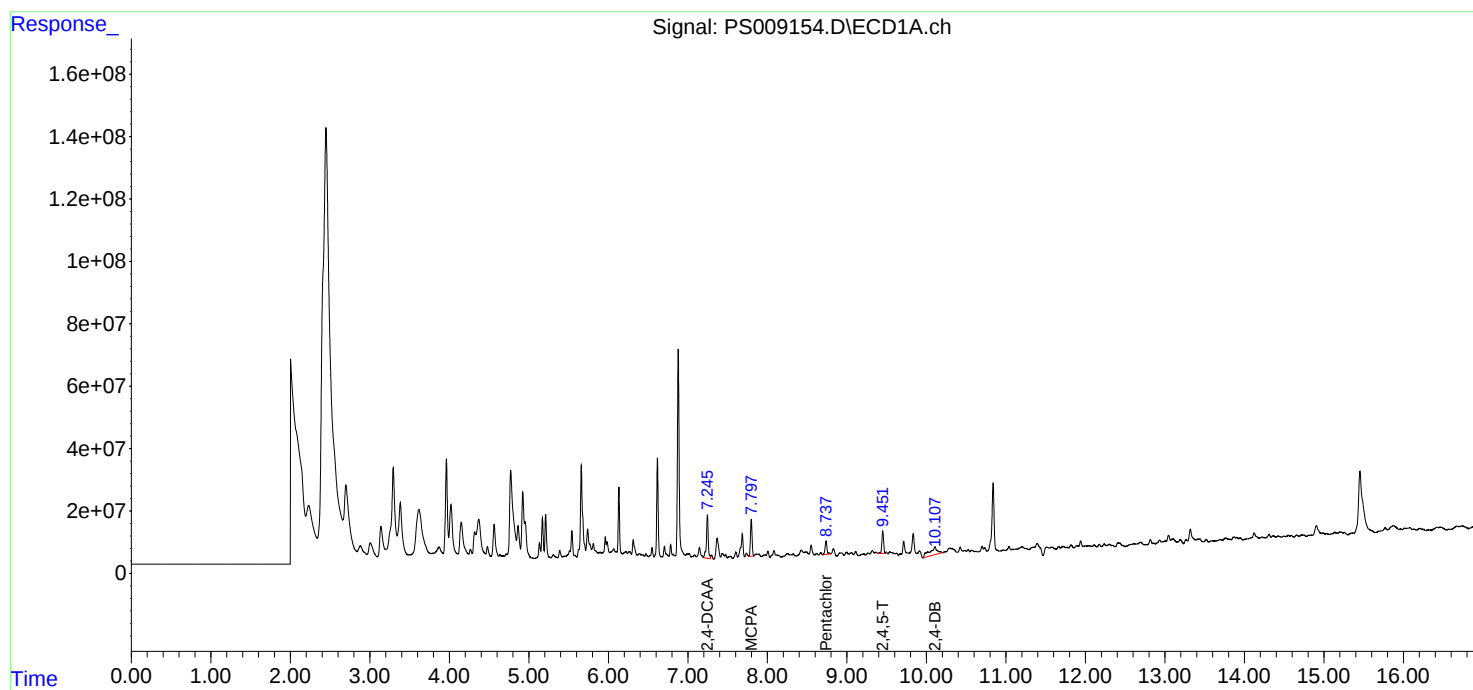


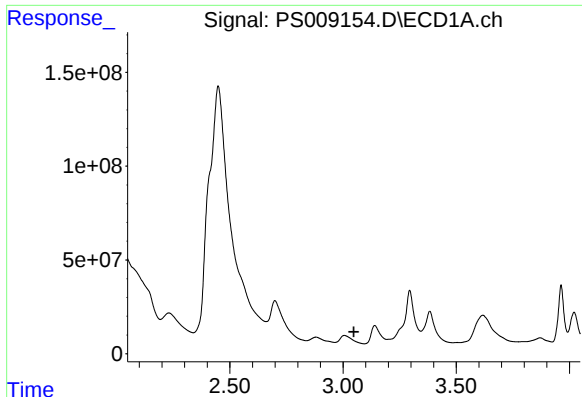

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.048 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

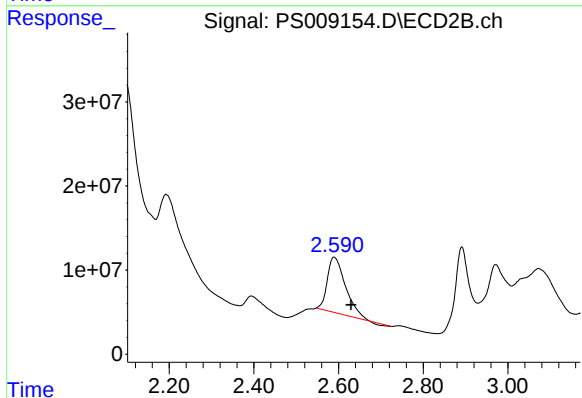


#1 Dalapon

R.T.: 2.589 min
Delta R.T.: -0.040 min
Response: 194949910
Conc: 133.32 ng/ml

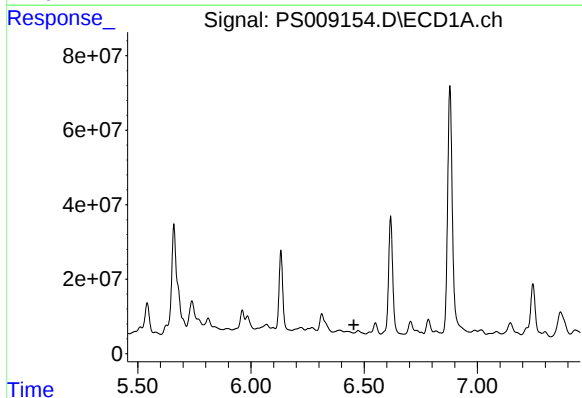


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

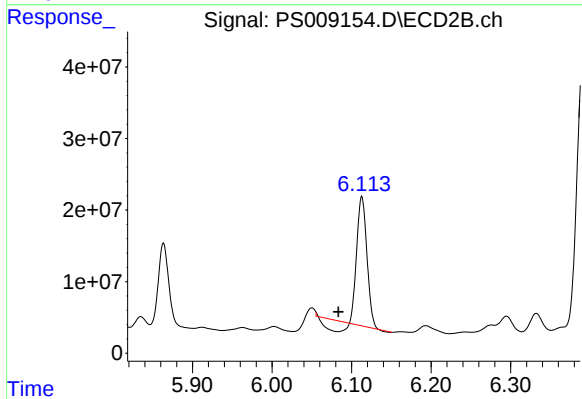

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.113 min
Delta R.T.: 0.030 min
Response: 141588969
Conc: 97.03 ng/ml

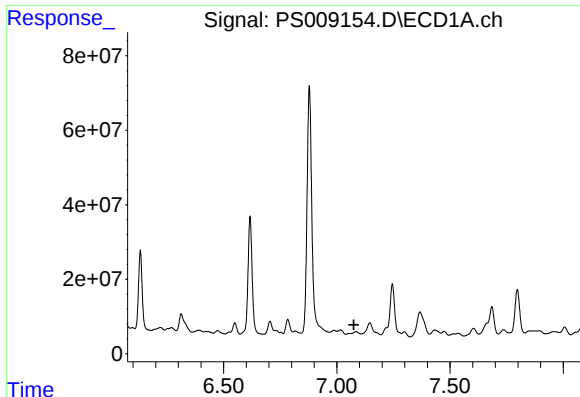

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.075 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

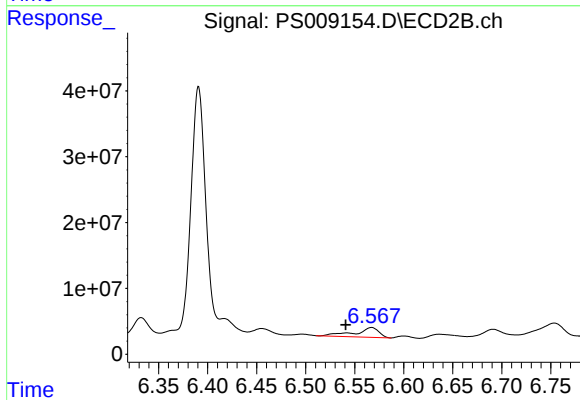


#3 4-Nitrophenol

R.T.: 6.567 min
Delta R.T.: 0.026 min
Response: 24836724
Conc: 42.97 ng/ml

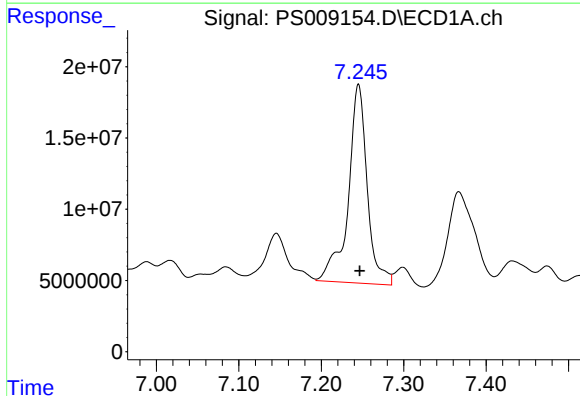


#4 2,4-DCAA

R.T.: 7.245 min
Delta R.T.: -0.002 min
Response: 223824006
Conc: 102.36 ng/ml

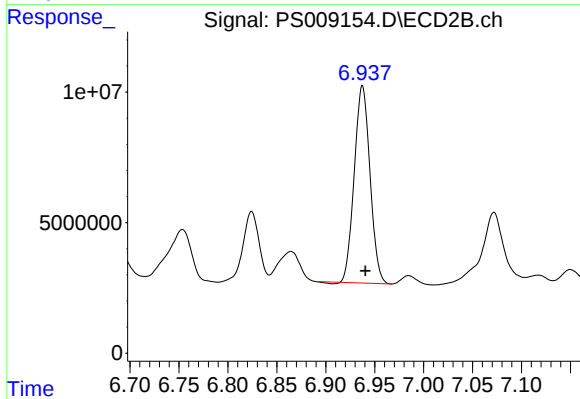

#4 2,4-DCAA


R.T.: 6.938 min
Delta R.T.: -0.003 min
Response: 84312555
Conc: 87.50 ng/ml

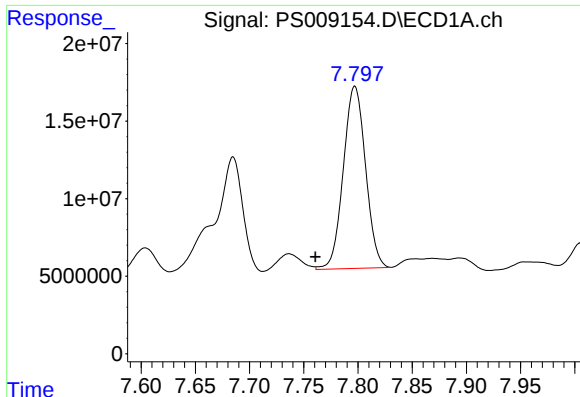

#7 MCPA


R.T.: 7.797 min
Delta R.T.: 0.037 min
Response: 167496610
Conc: 20.82 ug/ml

Instrument :
ECD_S
ClientSampleId :

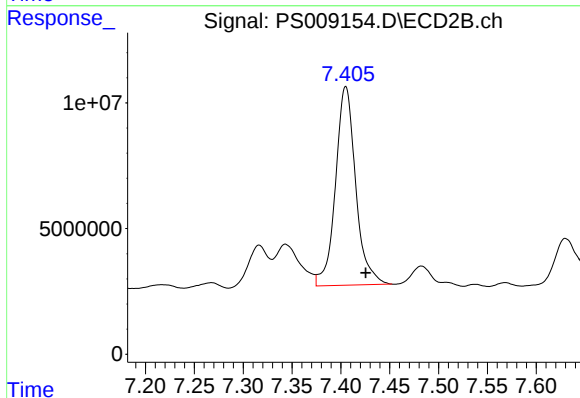


#7 MCPA

R.T.: 7.405 min
Delta R.T.: -0.020 min
Response: 113900064
Conc: 25.74 ug/ml

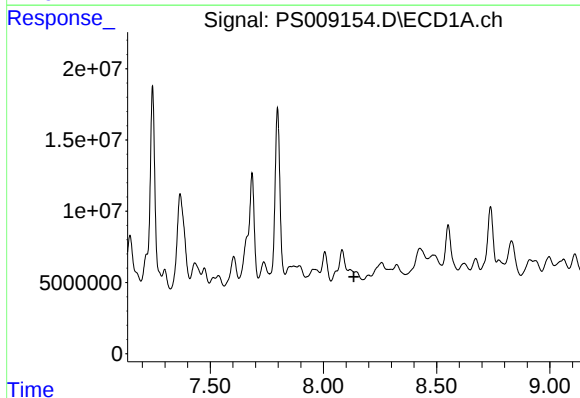


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.135 min
Response: 0
Conc: N.D.

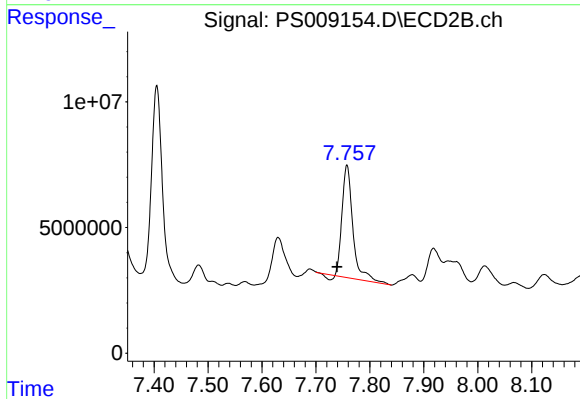

#8 DICHLORPROP


R.T.: 7.758 min
Delta R.T.: 0.019 min
Response: 61851788
Conc: 61.73 ng/ml

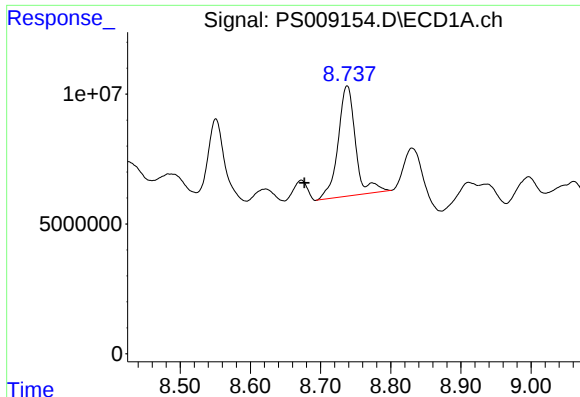

#10 Pentachlorophenol


R.T.: 8.738 min
Delta R.T.: 0.061 min
Response: 73413521
Conc: 2.53 ng/ml

Instrument :
ECD_S
ClientSampleId :

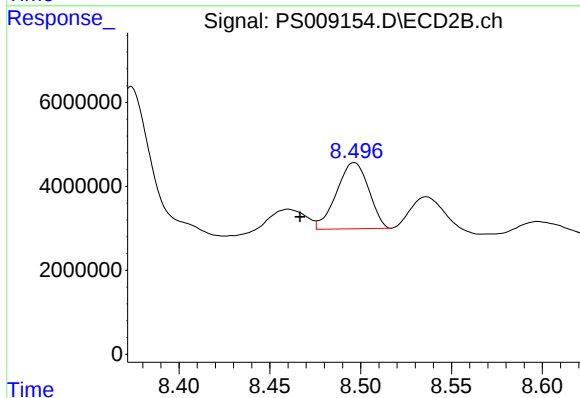


#10 Pentachlorophenol

R.T.: 8.496 min
Delta R.T.: 0.030 min
Response: 19466065
Conc: 1.37 ng/ml

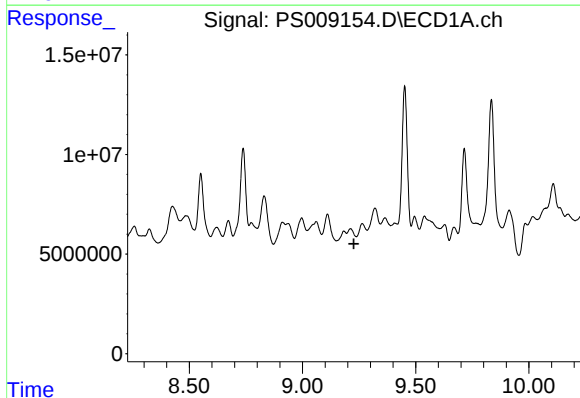


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.227 min
Response: 0
Conc: N.D.

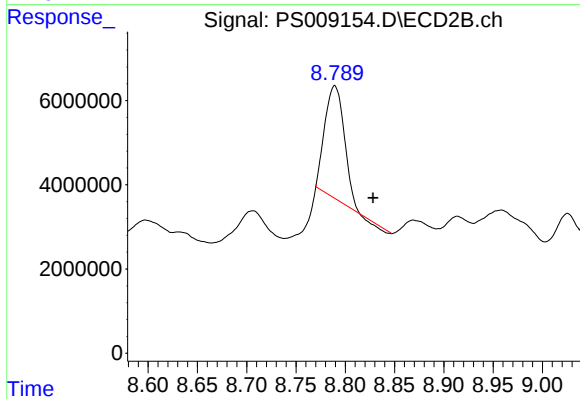

#11 2,4,5-TP (SILVEX)


R.T.: 8.789 min
Delta R.T.: -0.039 min
Response: 35971512
Conc: 6.64 ng/ml

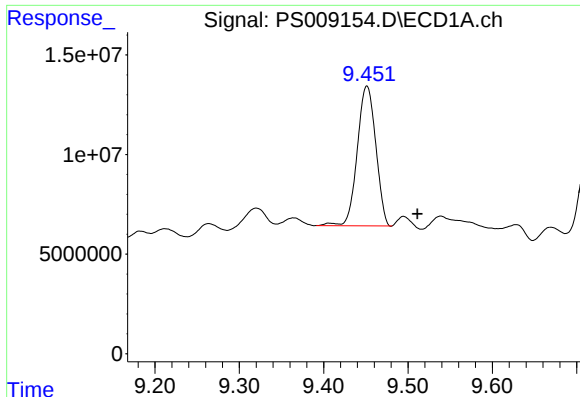

#12 2,4,5-T


R.T.: 9.451 min
Delta R.T.: -0.060 min
Response: 107108740
Conc: 10.02 ng/ml

Instrument :
ECD_S
ClientSampleId :

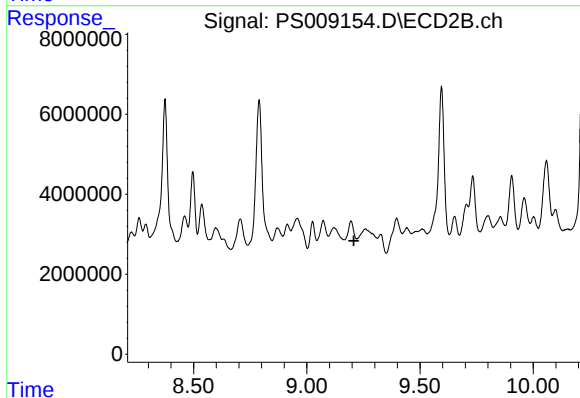


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.208 min
Response: 0
Conc: N.D.

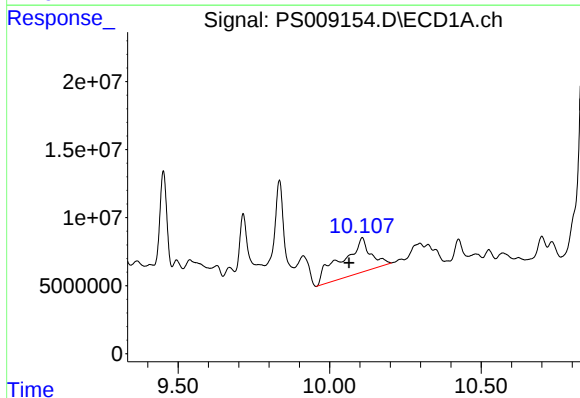


#13 2,4-DB

R.T.: 10.107 min
Delta R.T.: 0.043 min
Response: 172728759
Conc: 119.70 ng/ml

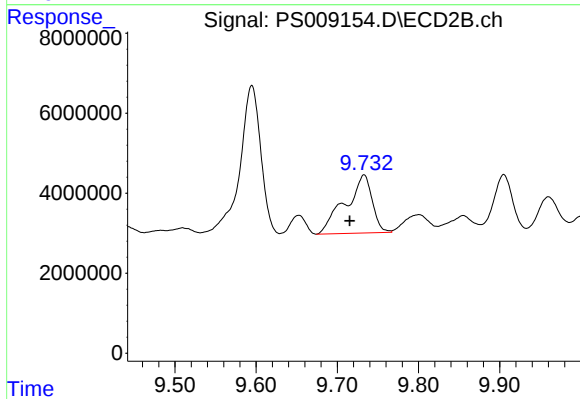

#13 2,4-DB


R.T.: 9.733 min
Delta R.T.: 0.018 min
Response: 33374793
Conc: 47.51 ng/ml

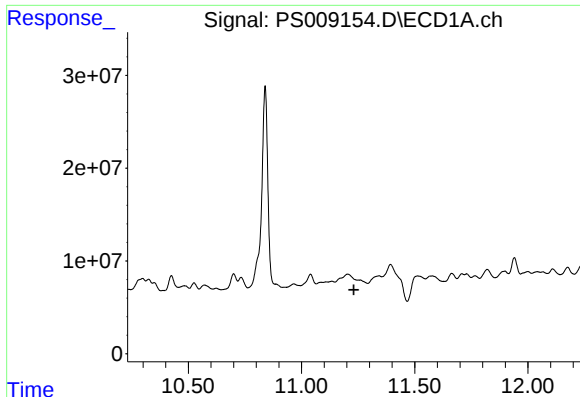

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 11.231 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

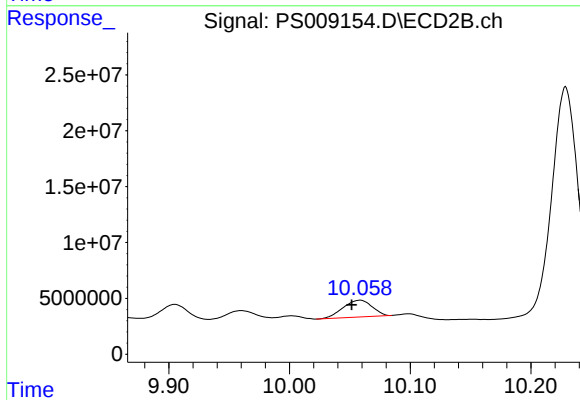


#14 DINOSEB

R.T.: 10.058 min
Delta R.T.: 0.007 min
Response: 25180117
Conc: 6.37 ng/ml

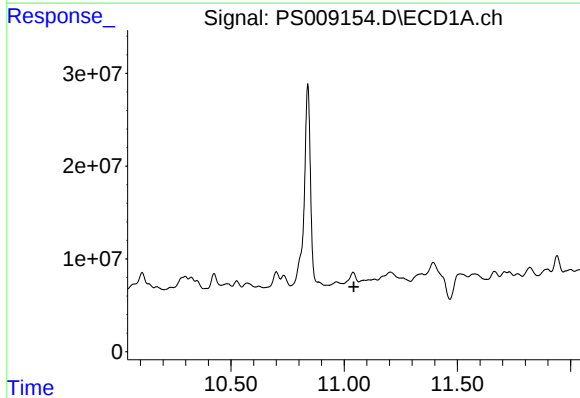


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.043 min
Response: 0
Conc: N.D.

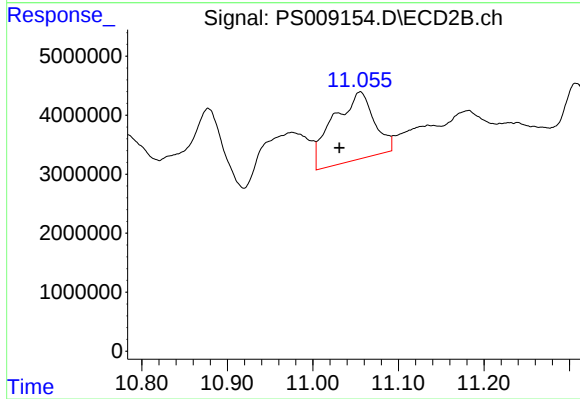

#15 Picloram


R.T.: 11.055 min
Delta R.T.: 0.024 min
Response: 38234376
Conc: 5.26 ng/ml

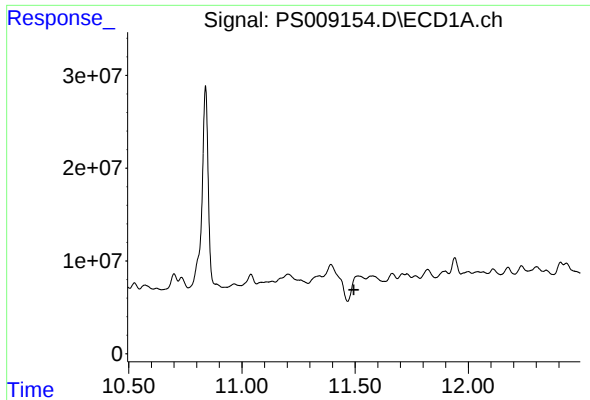

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.495 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

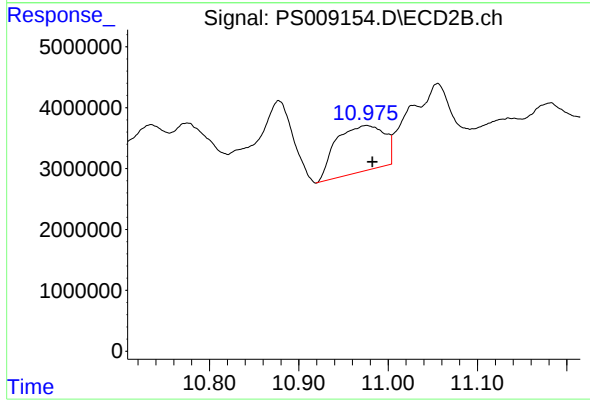

#16 DCPA

R.T.: 10.976 min
Delta R.T.: -0.007 min
Response: 28457574
Conc: 4.11 ng/ml