

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030620\
 Data File : PS009161.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Mar 2020 19:57
 Operator : DD\AJ
 Sample : L1778-23
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 06 23:24:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.245	6.938	271.5E6	118.6E6	124.157	123.133
Target Compounds							
1) T	Dalapon	0.000	2.590	0	218.7E6	N.D.	149.587
2) T	3,5-DICHL...	0.000	6.113	0	189.1E6	N.D.	129.590
3) T	4-Nitroph...	0.000	6.573	0	26975971	N.D.	46.668
7) T	MCPA	7.797	7.405	243.1E6	138.4E6	30.224	31.274
8) T	DICHLORPROP	0.000	7.757	0	87796229	N.D.	87.627
10) T	Pentachlo...	8.739	8.495	55841643	17668294	1.924	1.244 #
11) T	2,4,5-TP ...	0.000	8.788	0	38501355	N.D.	7.108
12) T	2,4,5-T	9.451	9.194	122.7E6	19536689	11.477	3.609 #
13) T	2,4-DB	10.109	9.731	60236103	64705013	41.743	92.115 #
14) T	DINOSEB	0.000	10.060	0	68587626	N.D.	17.346
15) T	Picloram	11.041	11.026	278.8E6	211.7E6	20.365	29.133 #
16) T	DCPA	0.000	11.026	0	211.7E6	N.D.	30.595



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030620\
Data File : PS009161.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2020 19:57
Operator : DD\AJ
Sample : L1778-23
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 06 23:24:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

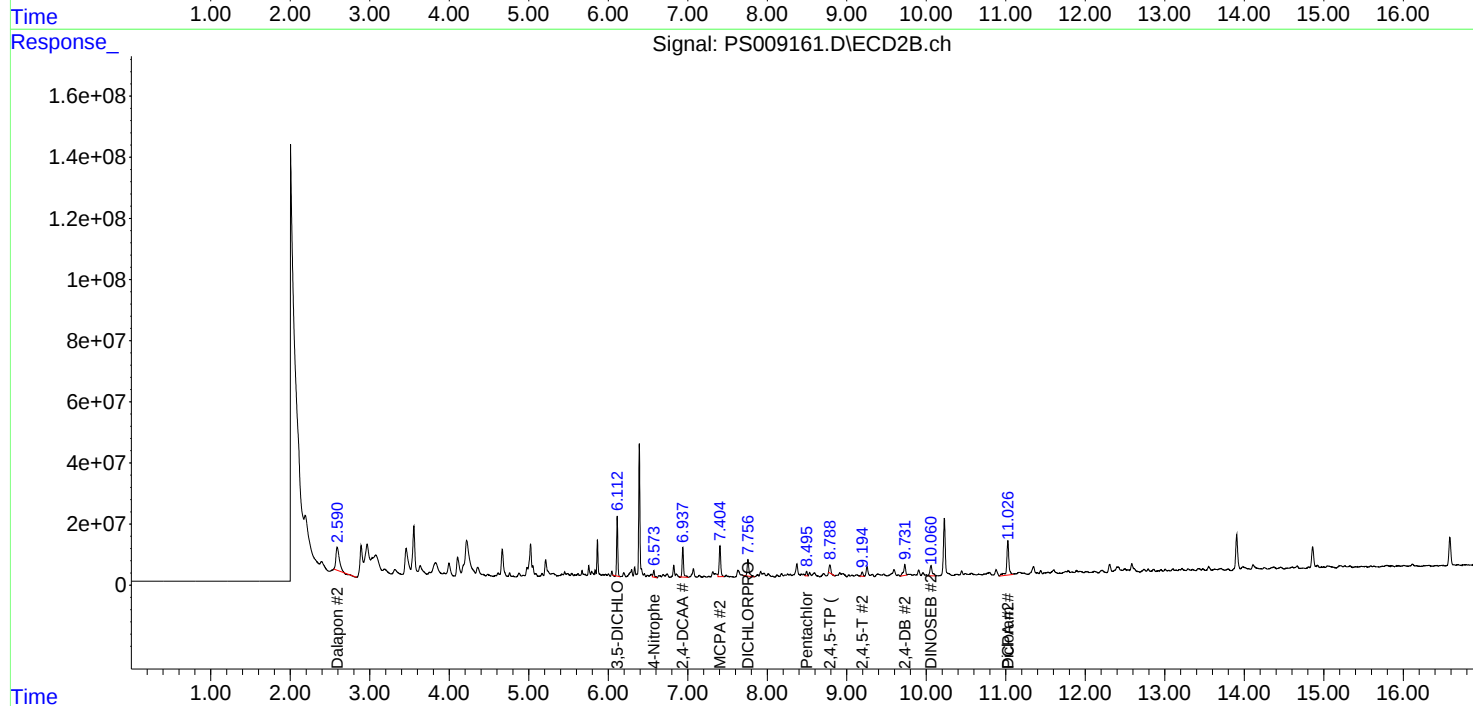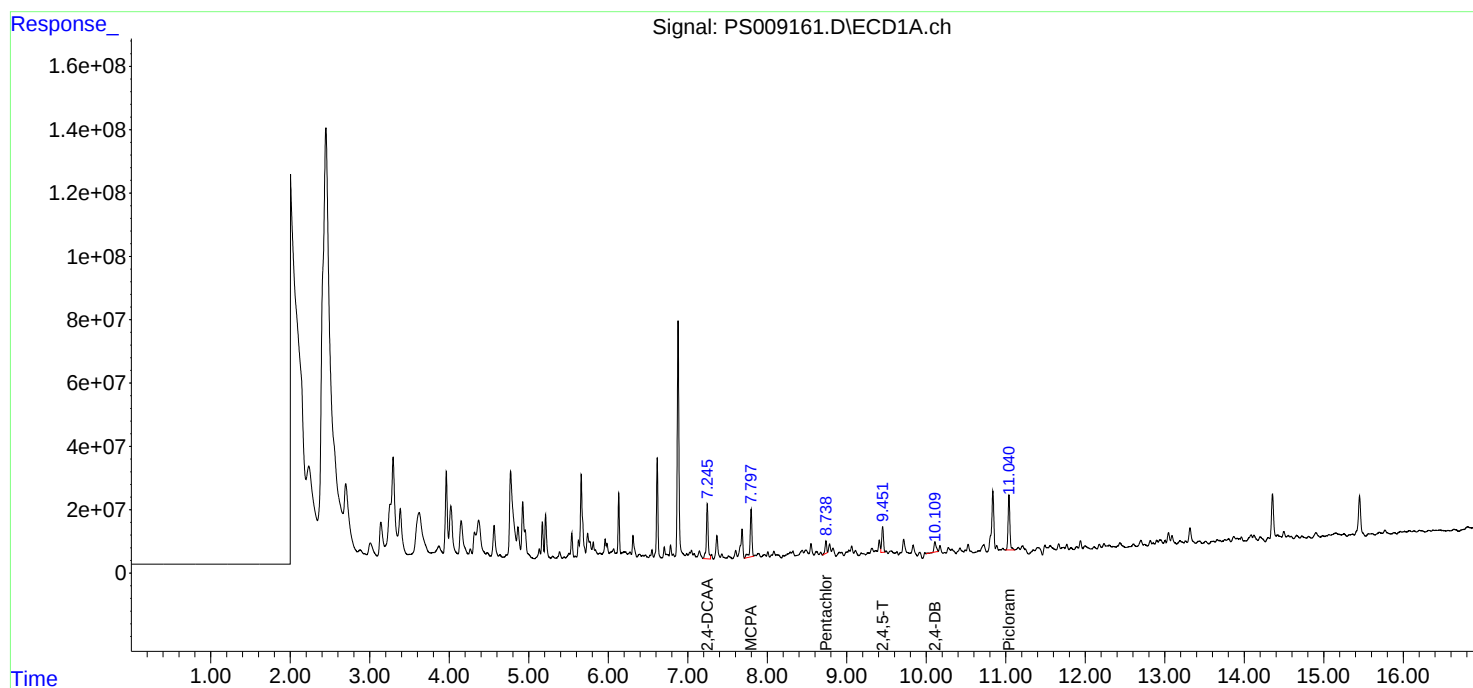


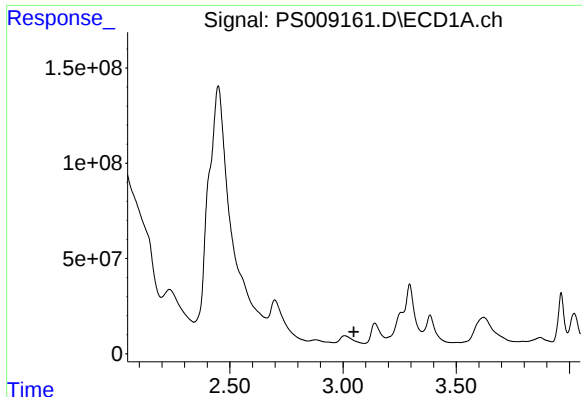

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.048 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

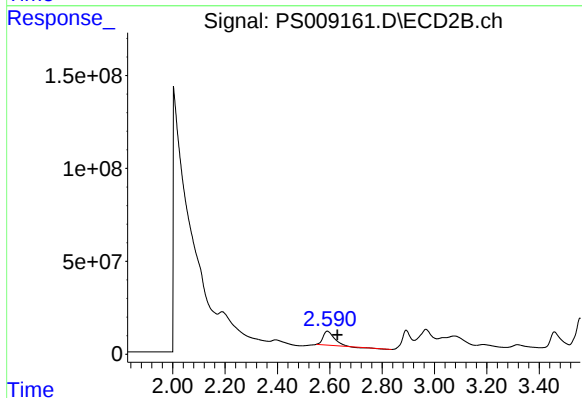


#1 Dalapon

R.T.: 2.590 min
Delta R.T.: -0.039 min
Response: 218729553
Conc: 149.59 ng/ml

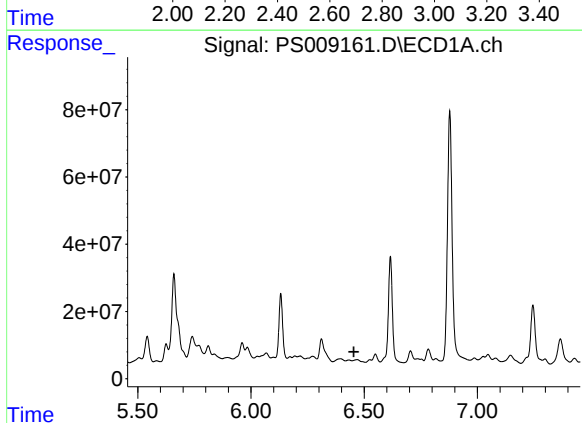


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

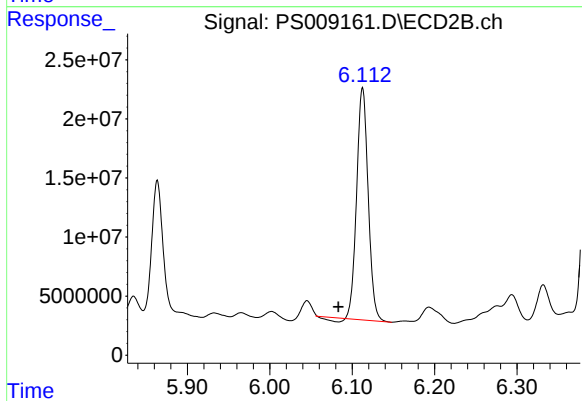

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.113 min
Delta R.T.: 0.029 min
Response: 189107117
Conc: 129.59 ng/ml

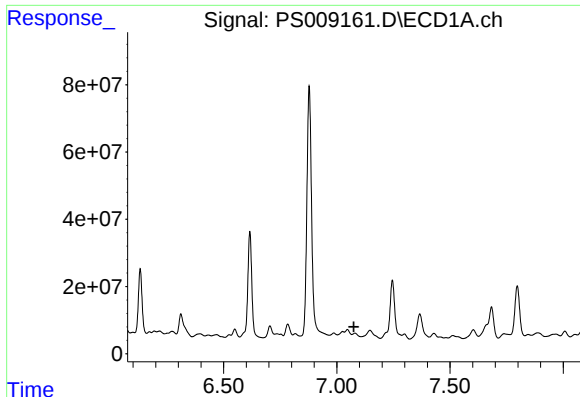

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.075 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

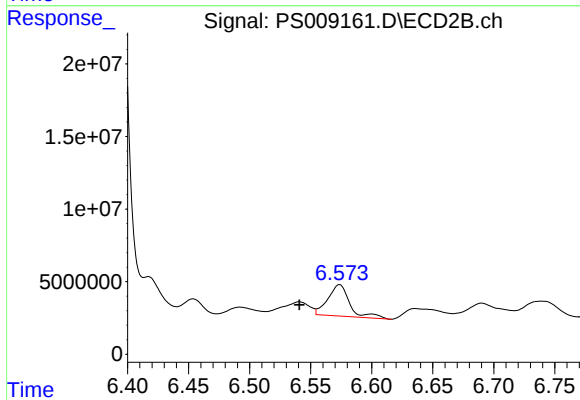


#3 4-Nitrophenol

R.T.: 6.573 min
Delta R.T.: 0.033 min
Response: 26975971
Conc: 46.67 ng/ml

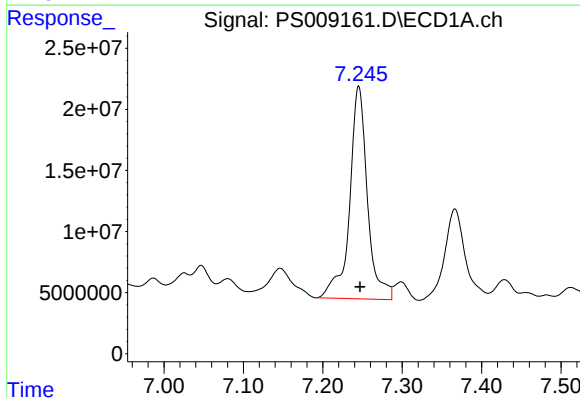


#4 2,4-DCAA

R.T.: 7.245 min
Delta R.T.: -0.002 min
Response: 271481720
Conc: 124.16 ng/ml

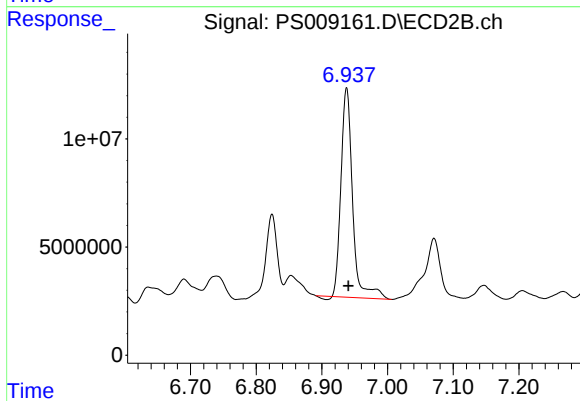

#4 2,4-DCAA


R.T.: 6.938 min
Delta R.T.: -0.003 min
Response: 118644994
Conc: 123.13 ng/ml

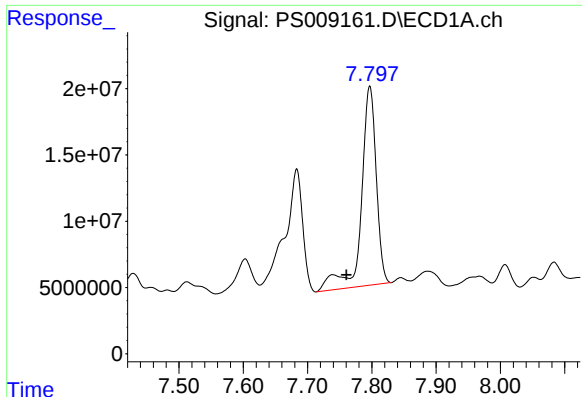

#7 MCPA


R.T.: 7.797 min
Delta R.T.: 0.036 min
Response: 243121177
Conc: 30.22 ug/ml

Instrument :
ECD_S
ClientSampleId :

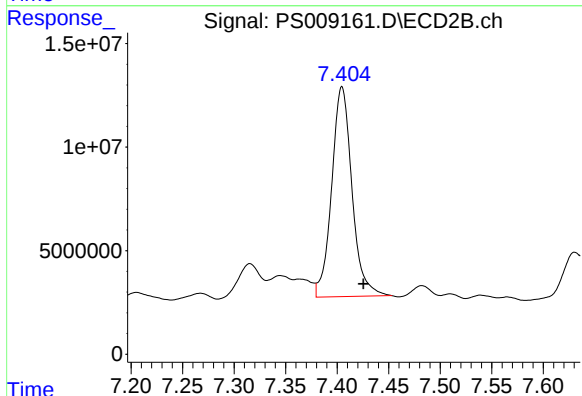


#7 MCPA

R.T.: 7.405 min
Delta R.T.: -0.021 min
Response: 138361974
Conc: 31.27 ug/ml

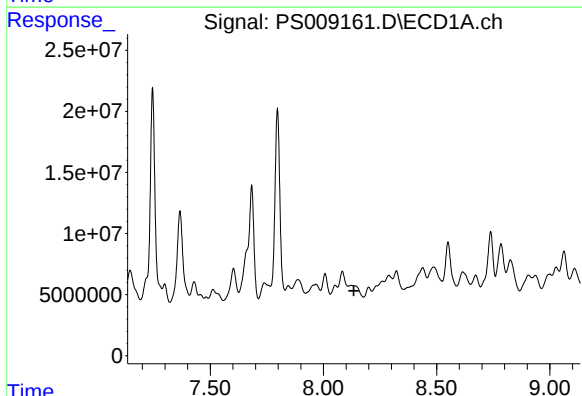


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.135 min
Response: 0
Conc: N.D.

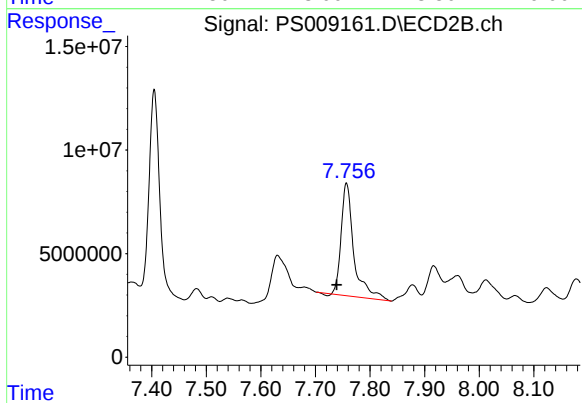

#8 DICHLORPROP


R.T.: 7.757 min
Delta R.T.: 0.018 min
Response: 87796229
Conc: 87.63 ng/ml

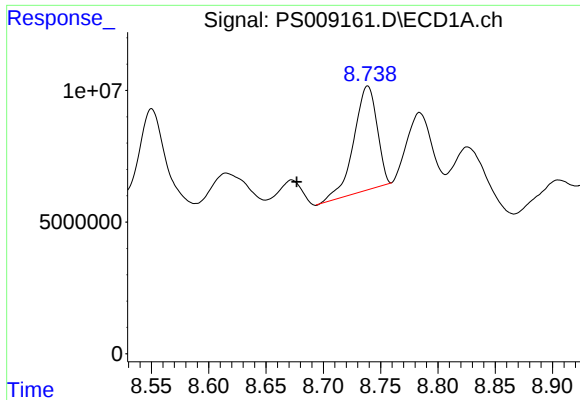

#10 Pentachlorophenol


R.T.: 8.739 min
Delta R.T.: 0.062 min
Response: 55841643
Conc: 1.92 ng/ml

Instrument :
ECD_S
ClientSampleId :

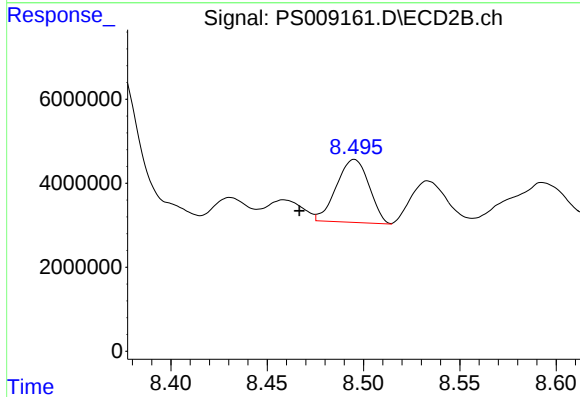


#10 Pentachlorophenol

R.T.: 8.495 min
Delta R.T.: 0.028 min
Response: 17668294
Conc: 1.24 ng/ml

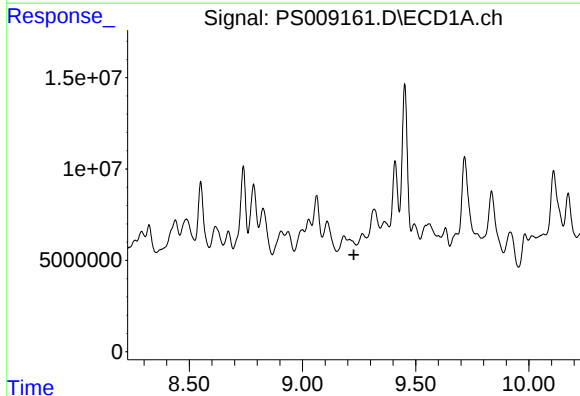


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.227 min
Response: 0
Conc: N.D.

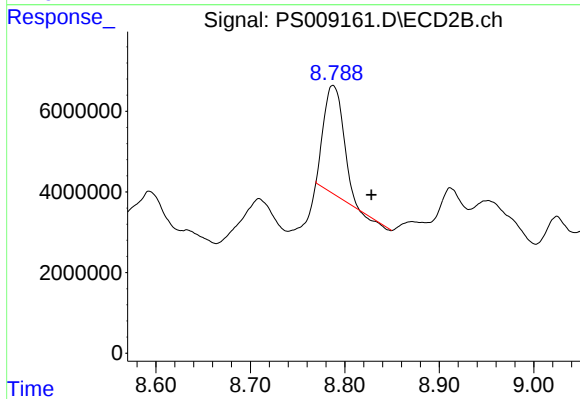

#11 2,4,5-TP (SILVEX)


R.T.: 8.788 min
Delta R.T.: -0.040 min
Response: 38501355
Conc: 7.11 ng/ml

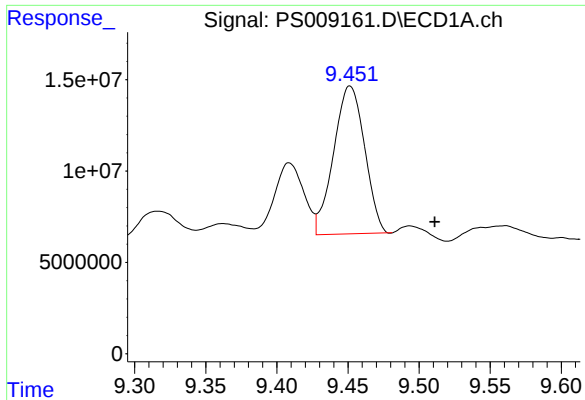

#12 2,4,5-T


R.T.: 9.451 min
Delta R.T.: -0.060 min
Response: 122713534
Conc: 11.48 ng/ml

Instrument :
ECD_S
ClientSampleId :

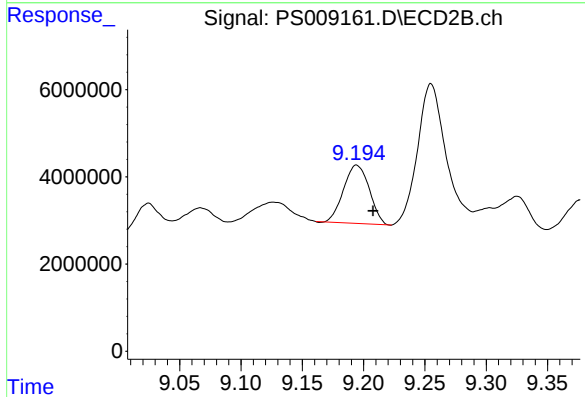


#12 2,4,5-T

R.T.: 9.194 min
Delta R.T.: -0.013 min
Response: 19536689
Conc: 3.61 ng/ml

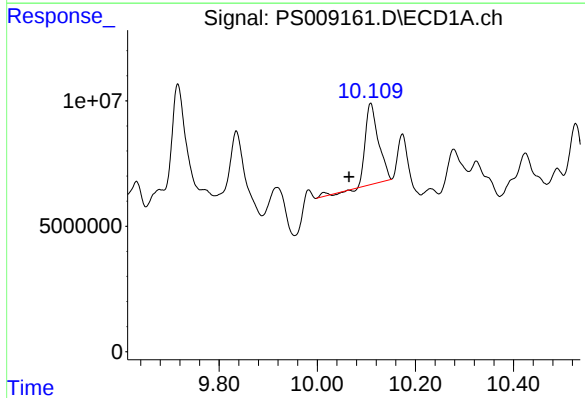


#13 2,4-DB

R.T.: 10.109 min
Delta R.T.: 0.044 min
Response: 60236103
Conc: 41.74 ng/ml

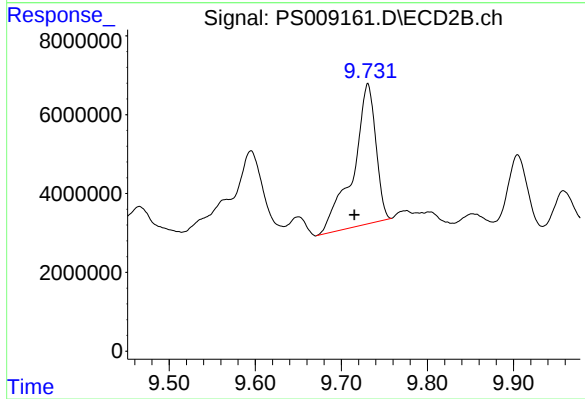

#13 2,4-DB


R.T.: 9.731 min
Delta R.T.: 0.016 min
Response: 64705013
Conc: 92.11 ng/ml

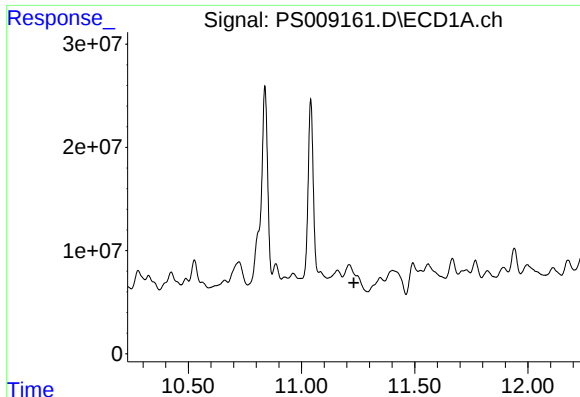

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 11.231 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

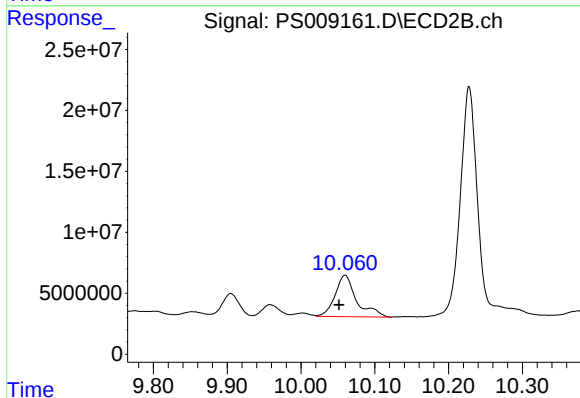


#14 DINOSEB

R.T.: 10.060 min
Delta R.T.: 0.008 min
Response: 68587626
Conc: 17.35 ng/ml

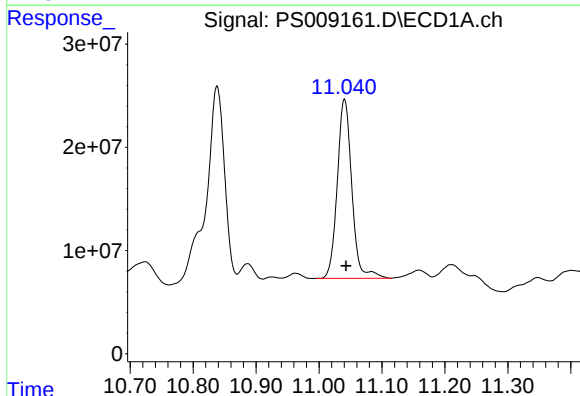


#15 Picloram

R.T.: 11.041 min
Delta R.T.: -0.003 min
Response: 278811018
Conc: 20.36 ng/ml

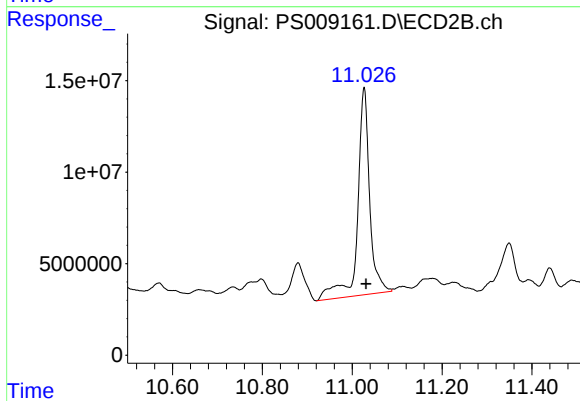

#15 Picloram


R.T.: 11.026 min
Delta R.T.: -0.005 min
Response: 211697238
Conc: 29.13 ng/ml

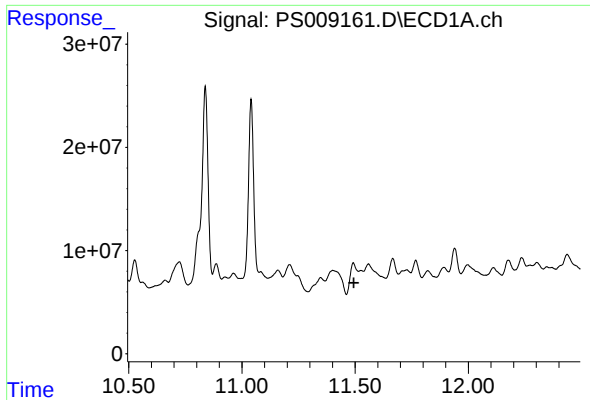

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.495 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

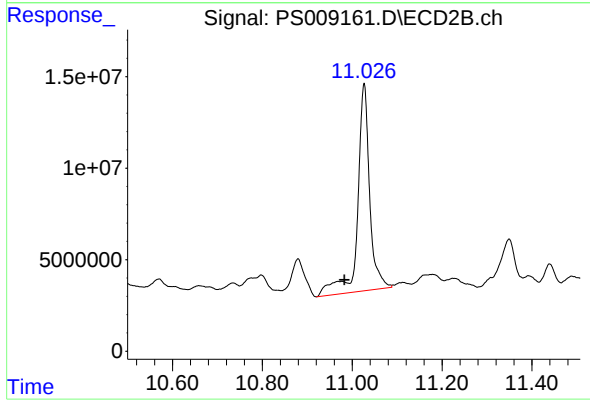

#16 DCPA

R.T.: 11.026 min
Delta R.T.: 0.044 min
Response: 211697238
Conc: 30.59 ng/ml