

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030620\
 Data File : PS009162.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Mar 2020 20:20
 Operator : DD\AJ
 Sample : L1778-25
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 06 23:24:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.245	6.937	531.3E6	276.7E6	242.971	287.183
Target Compounds							
1) T	Dalapon	0.000	2.591	0	269.1E6	N.D.	184.067
2) T	3,5-DICHL...	0.000	6.113	0	169.9E6	N.D.	116.443
7) T	MCPA	7.797	7.405	106.1E6	77909184	13.186	17.610 #
8) T	DICHLORPROP	0.000	7.757	0	68508706	N.D.	68.377
11) T	2,4,5-TP ...	0.000	8.788	0	30057596	N.D.	5.549
12) T	2,4,5-T	9.451	0.000	150.8E6	0	14.102	N.D. #
13) T	2,4-DB	0.000	9.732	0	14283487	N.D.	20.334
14) T	DINOSEB	0.000	10.057	0	36219778	N.D.	9.160
15) T	Picloram	0.000	11.023	0	84861093	N.D.	11.678
16) T	DCPA	0.000	11.023	0	84861093	N.D.	12.264



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030620\
Data File : PS009162.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2020 20:20
Operator : DD\AJ
Sample : L1778-25
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 06 23:24:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

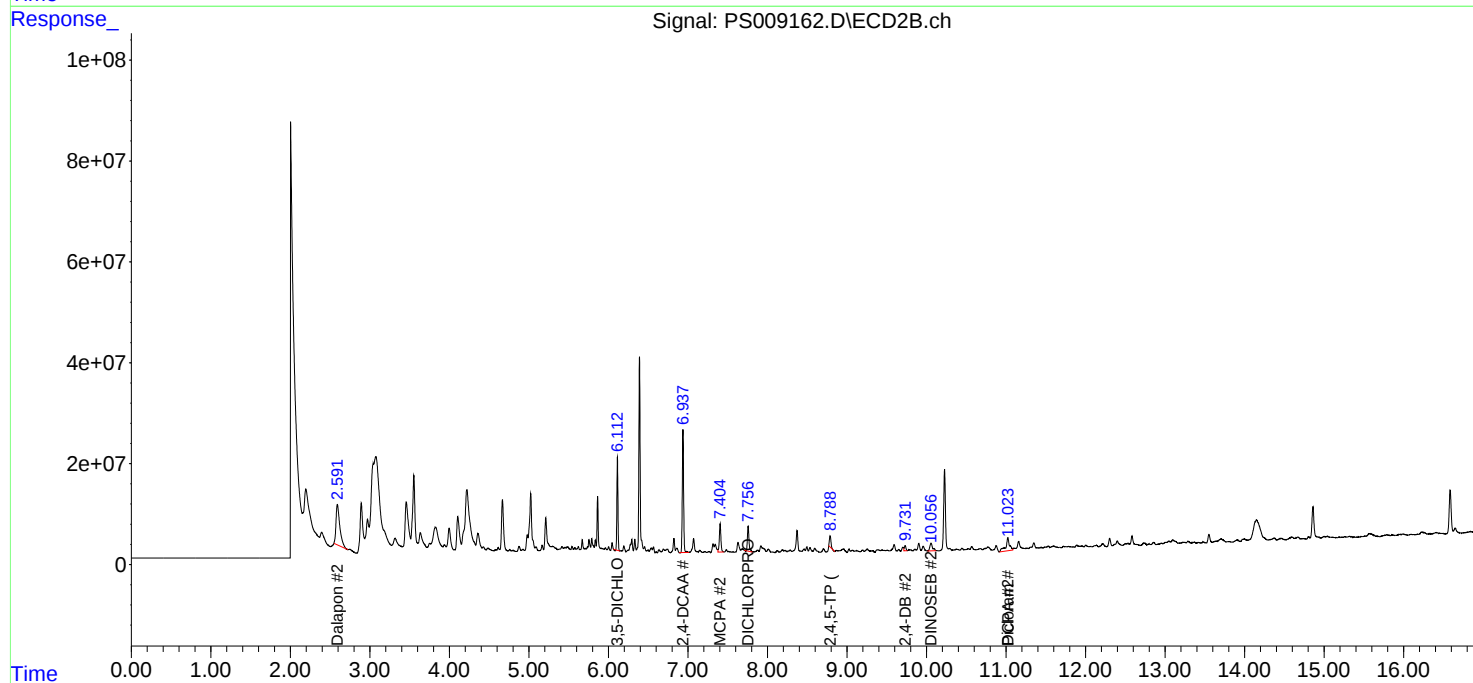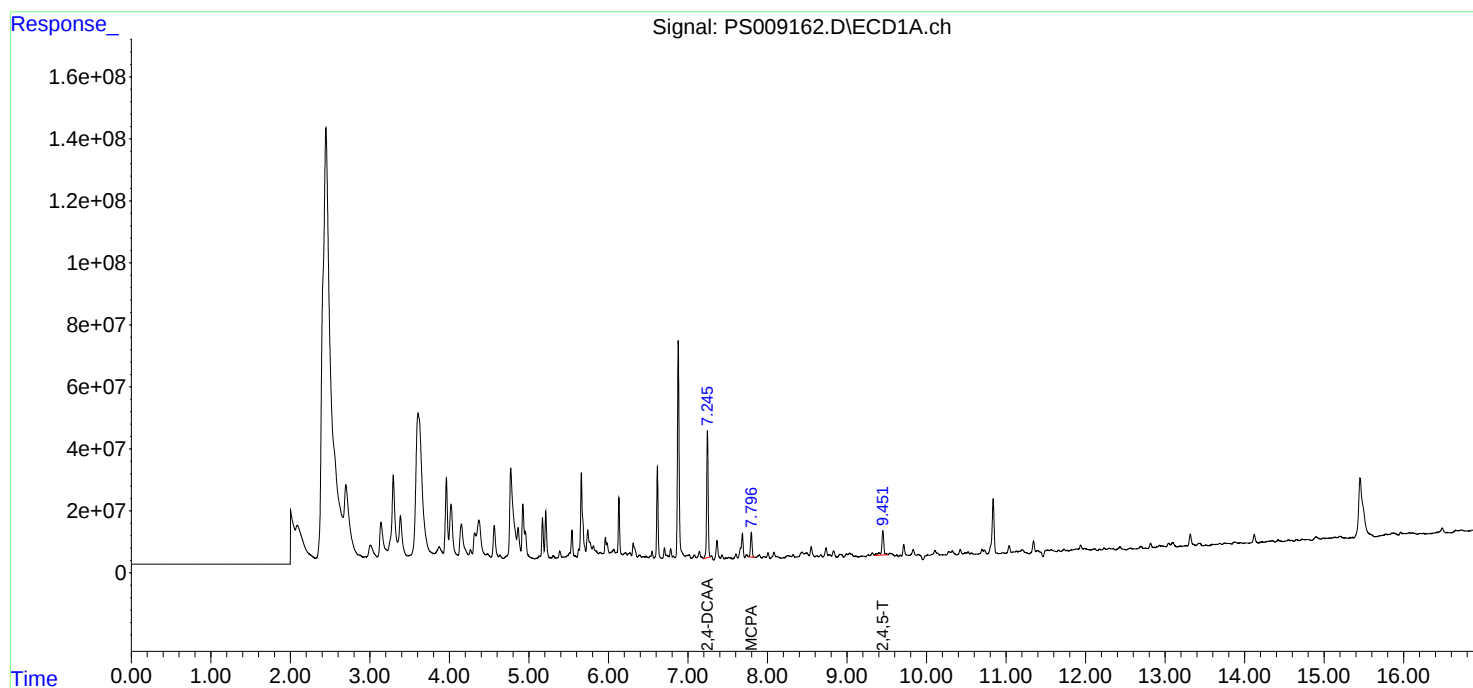


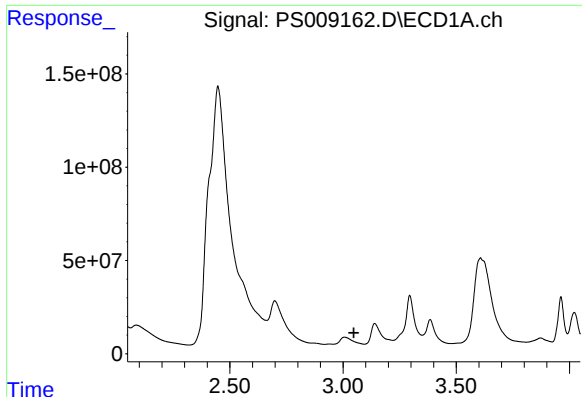

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 3.048 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

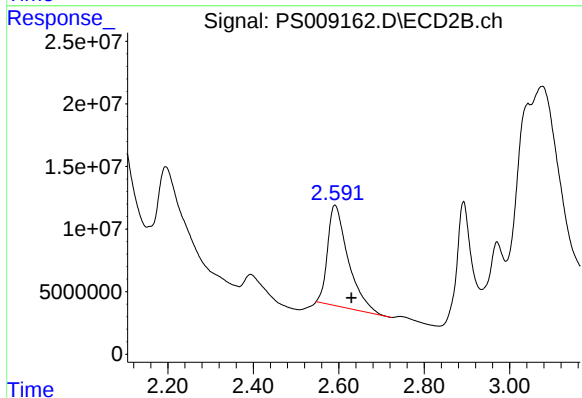


#1 Dalapon

R.T.: 2.591 min
Delta R.T.: -0.039 min
Response: 269146389
Conc: 184.07 ng/ml

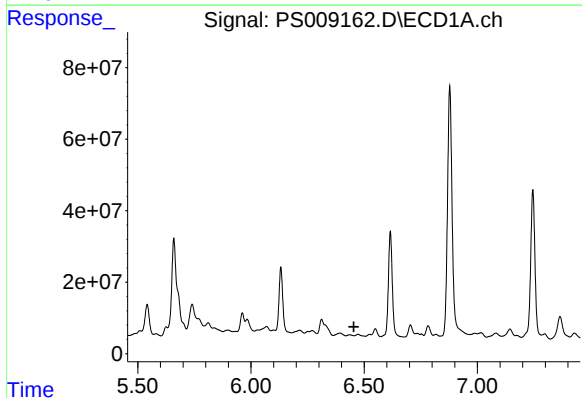


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.455 min
Response: 0
Conc: N.D.

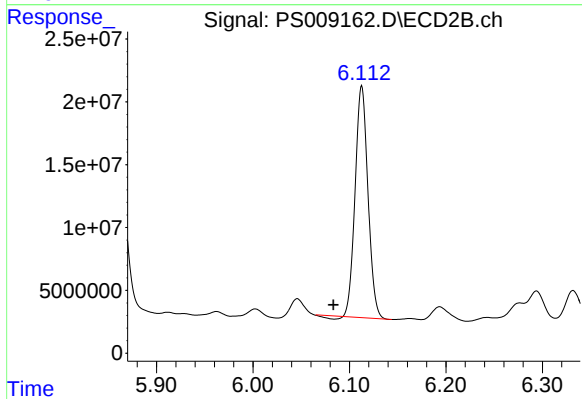

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.113 min
Delta R.T.: 0.029 min
Response: 169921718
Conc: 116.44 ng/ml

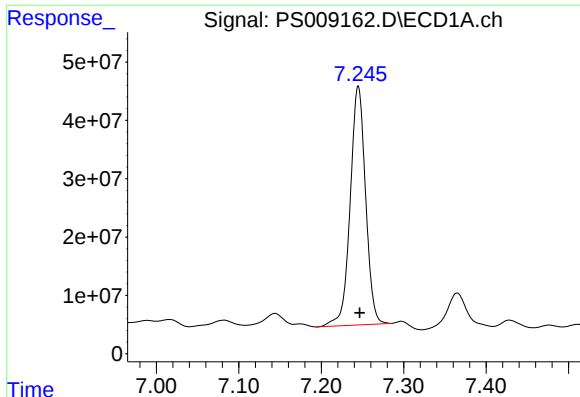

#4 2,4-DCAA


R.T.: 7.245 min
Delta R.T.: -0.002 min
Response: 531279080
Conc: 242.97 ng/ml

Instrument :
ECD_S
ClientSampleId :

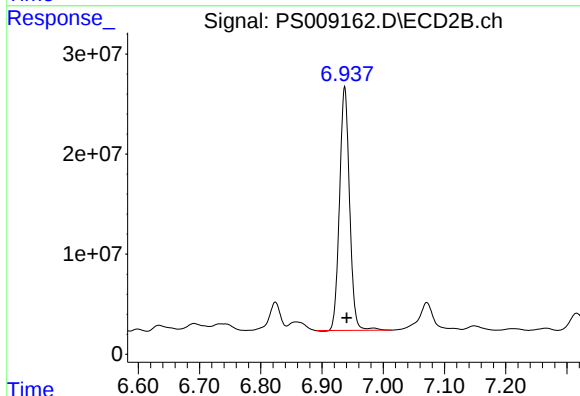


#4 2,4-DCAA

R.T.: 6.937 min
Delta R.T.: -0.003 min
Response: 276717161
Conc: 287.18 ng/ml

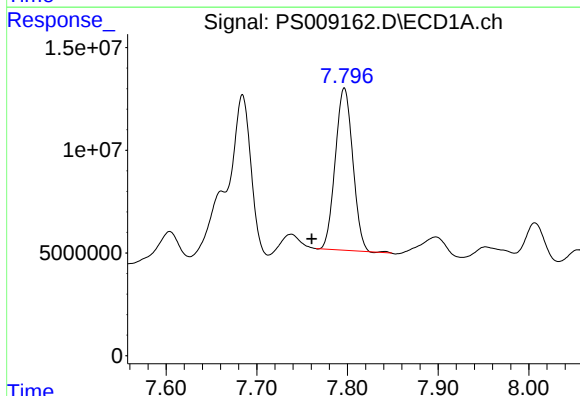


#7 MCPA

R.T.: 7.797 min
Delta R.T.: 0.036 min
Response: 106069463
Conc: 13.19 ug/ml

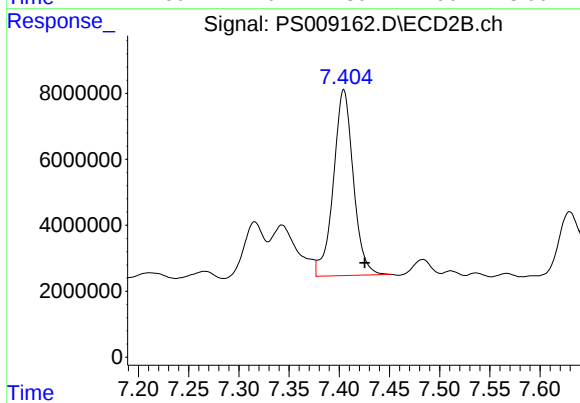

#7 MCPA


R.T.: 7.405 min
Delta R.T.: -0.021 min
Response: 77909184
Conc: 17.61 ug/ml

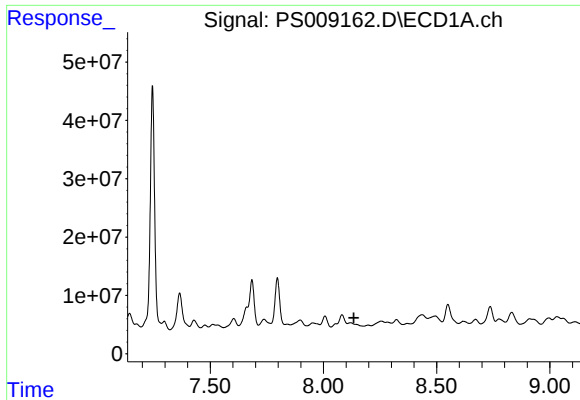

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.135 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

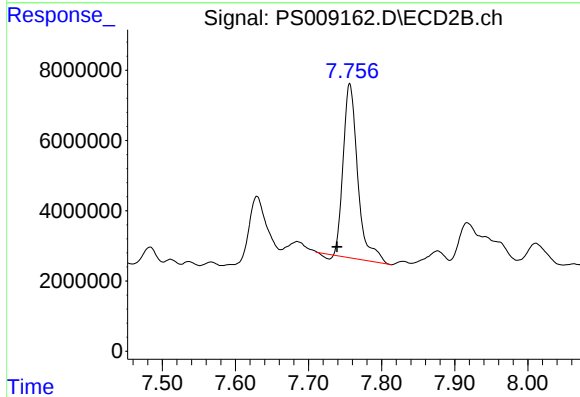


#8 DICHLORPROP

R.T.: 7.757 min
Delta R.T.: 0.018 min
Response: 68508706
Conc: 68.38 ng/ml

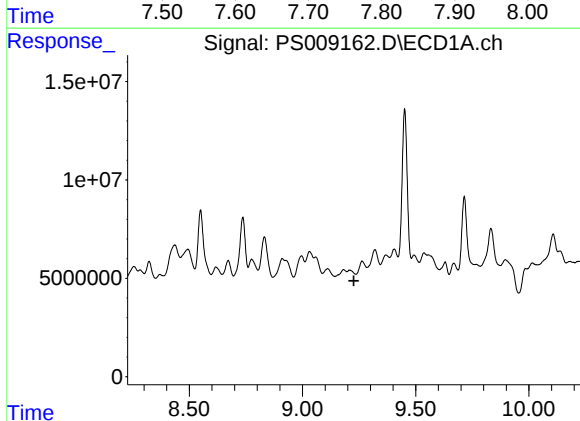


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 9.227 min
Response: 0
Conc: N.D.

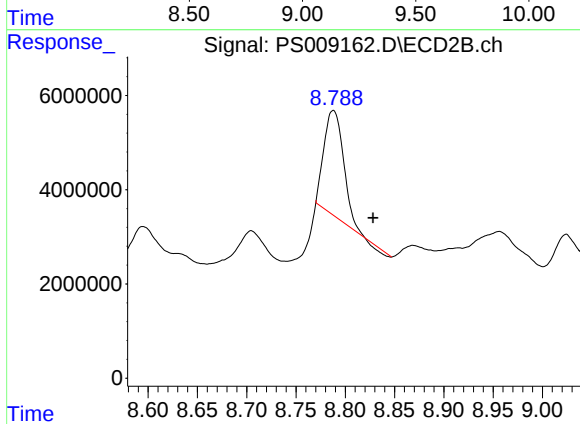

#11 2,4,5-TP (SILVEX)


R.T.: 8.788 min
Delta R.T.: -0.040 min
Response: 30057596
Conc: 5.55 ng/ml

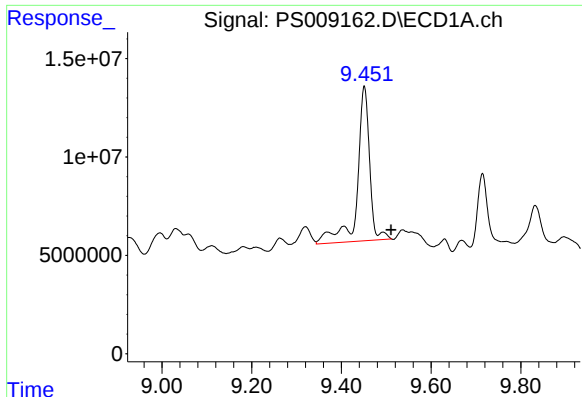

#12 2,4,5-T


R.T.: 9.451 min
Delta R.T.: -0.060 min
Response: 150777743
Conc: 14.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

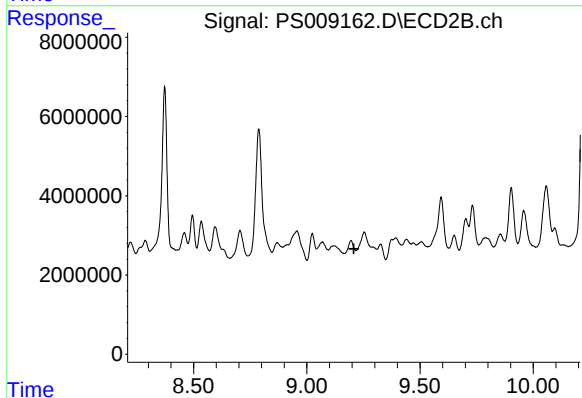


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.208 min
Response: 0
Conc: N.D.

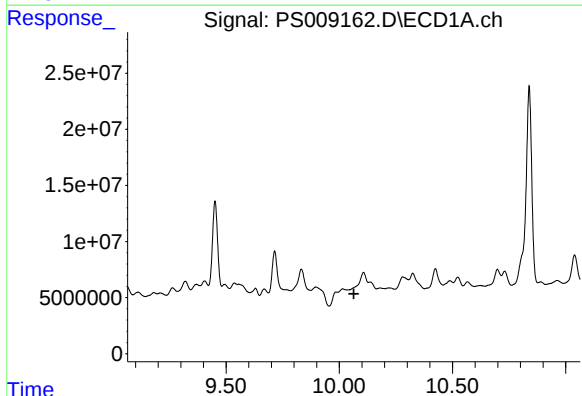


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.064 min
Response: 0
Conc: N.D.

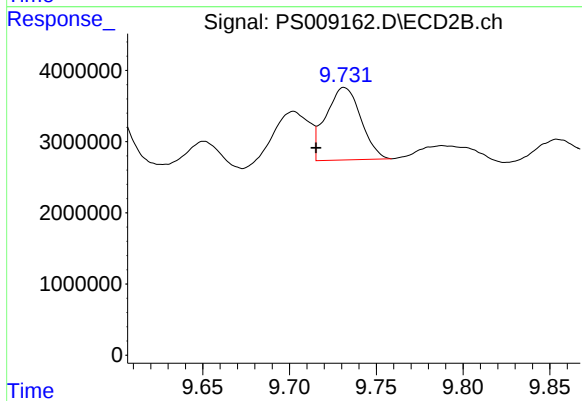

#13 2,4-DB


R.T.: 9.732 min
Delta R.T.: 0.016 min
Response: 14283487
Conc: 20.33 ng/ml

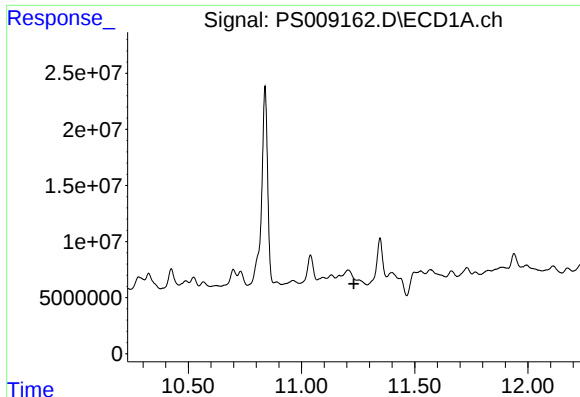

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 11.231 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

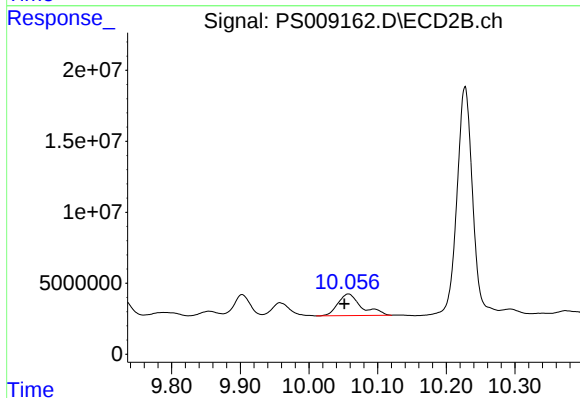


#14 DINOSEB

R.T.: 10.057 min
Delta R.T.: 0.006 min
Response: 36219778
Conc: 9.16 ng/ml

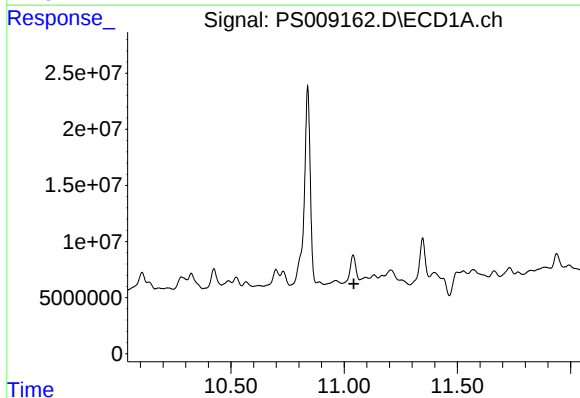


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.043 min
Response: 0
Conc: N.D.

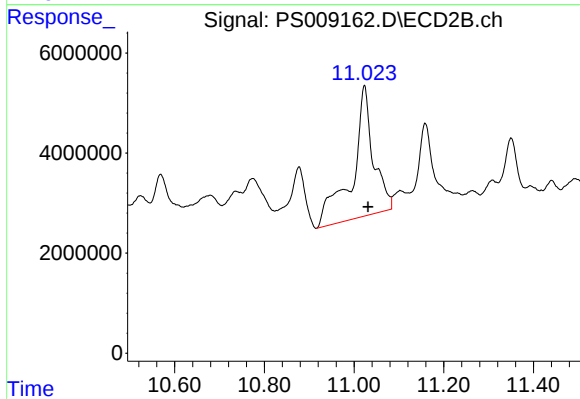

#15 Picloram


R.T.: 11.023 min
Delta R.T.: -0.008 min
Response: 84861093
Conc: 11.68 ng/ml

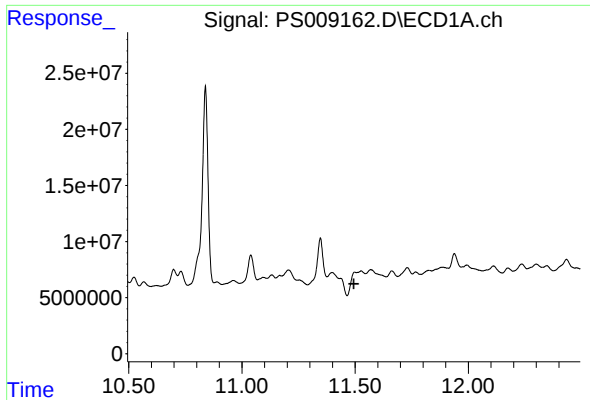

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.495 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

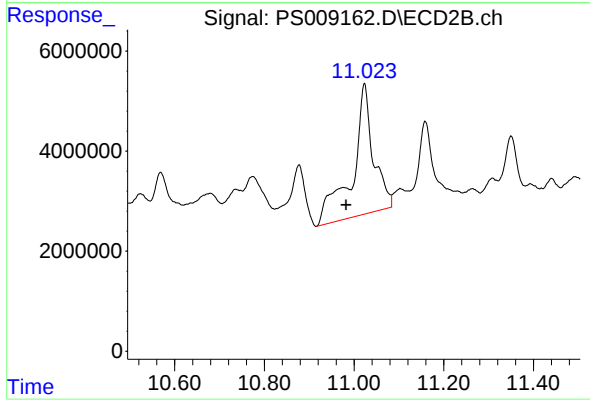

#16 DCPA

R.T.: 11.023 min
Delta R.T.: 0.041 min
Response: 84861093
Conc: 12.26 ng/ml