

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030620\
 Data File : PS009163.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Mar 2020 20:43
 Operator : DD\AJ
 Sample : PB127311BL
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 06 23:24:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.245	6.937	933.7E6	473.7E6	426.989	491.662
Target Compounds							
1) T	Dalapon	3.010	2.593	221.1E6	184.8E6	73.895	126.377 #
2) T	3,5-DICHL...	0.000	6.113	0	123.1E6	N.D.	84.390
7) T	MCPA	7.796	7.405	173.0E6	101.0E6	21.503	22.818
8) T	DICHLORPROP	0.000	7.757	0	59703821	N.D.	59.589
11) T	2,4,5-TP ...	0.000	8.791	0	32340222	N.D.	5.970
12) T	2,4,5-T	9.451	0.000	88317877	0	8.260	N.D. #
14) T	DINOSEB	0.000	10.057	0	20186746	N.D.	5.105
15) T	Picloram	0.000	11.027	0	42228875	N.D.	5.811
16) T	DCPA	0.000	11.027	0	42228875	N.D.	6.103



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030620\
Data File : PS009163.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2020 20:43
Operator : DD\AJ
Sample : PB127311BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 06 23:24:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

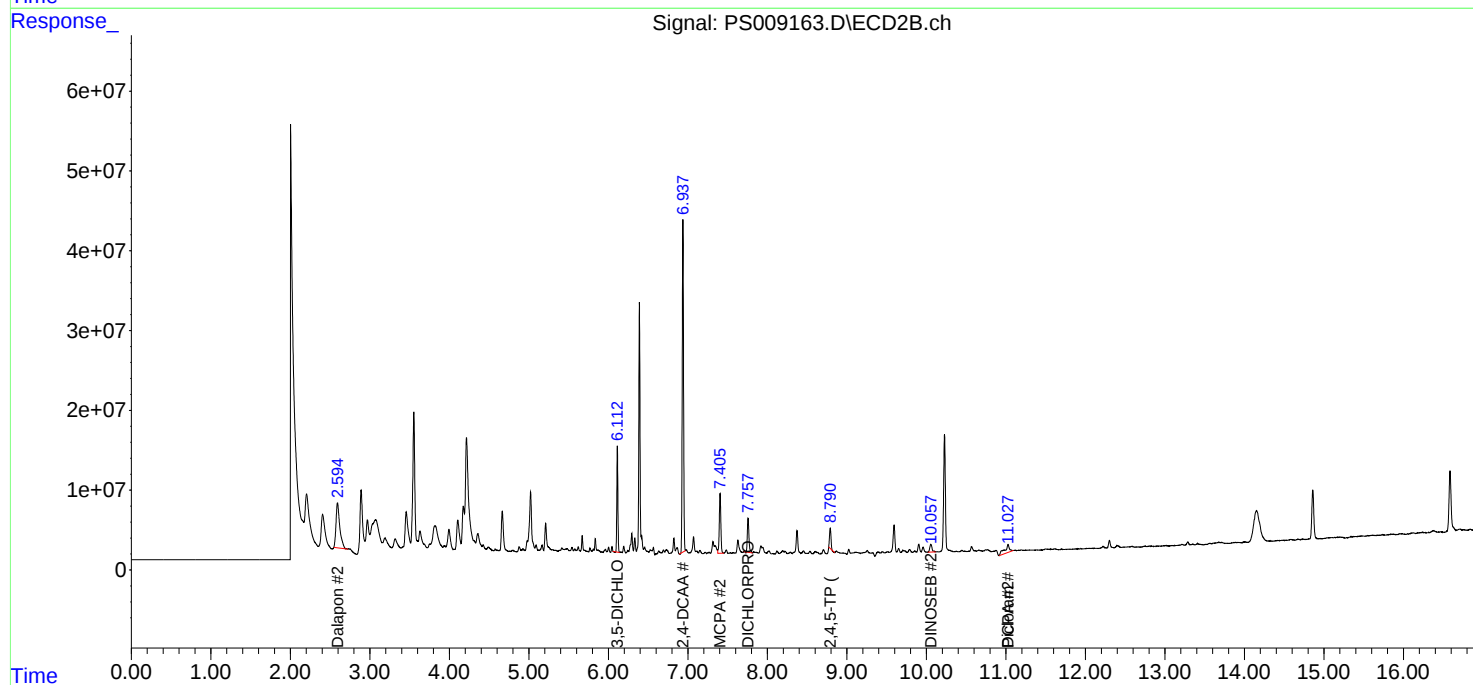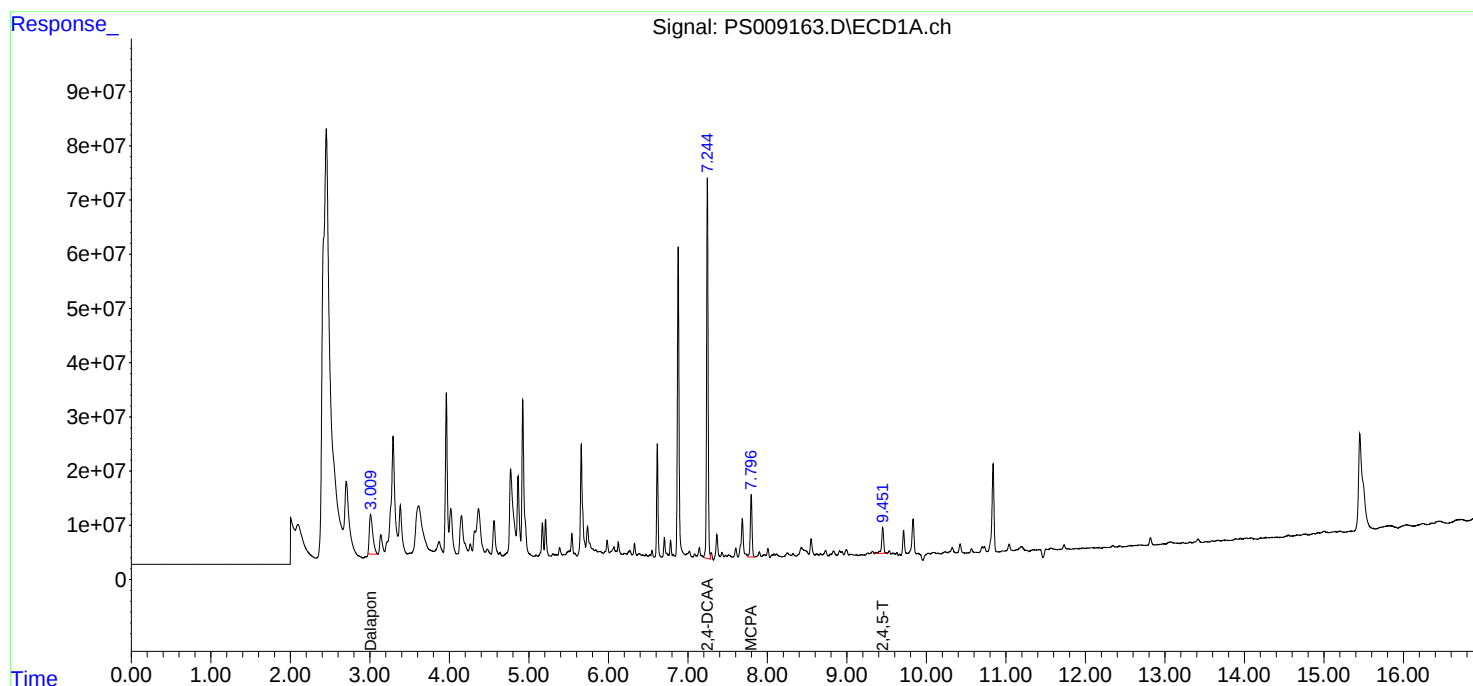


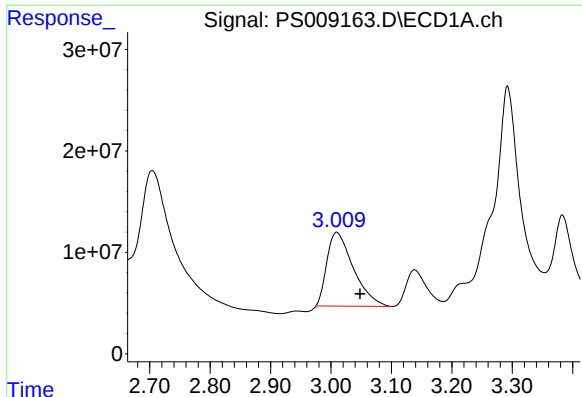

#1 Dalapon


R.T.: 3.010 min
Delta R.T.: -0.038 min
Response: 221077931
Conc: 73.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

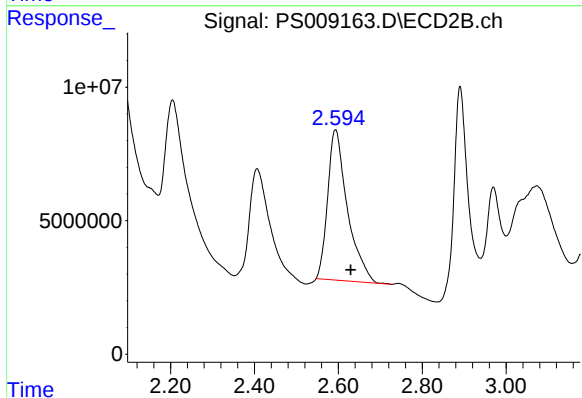


#1 Dalapon

R.T.: 2.593 min
Delta R.T.: -0.037 min
Response: 184790936
Conc: 126.38 ng/ml

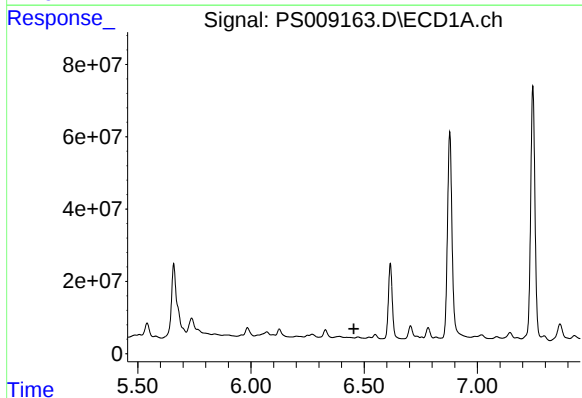


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.455 min
Response: 0
Conc: N.D.

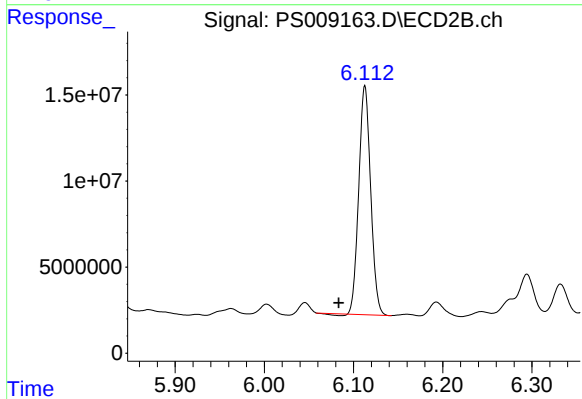

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.113 min
Delta R.T.: 0.029 min
Response: 123148456
Conc: 84.39 ng/ml

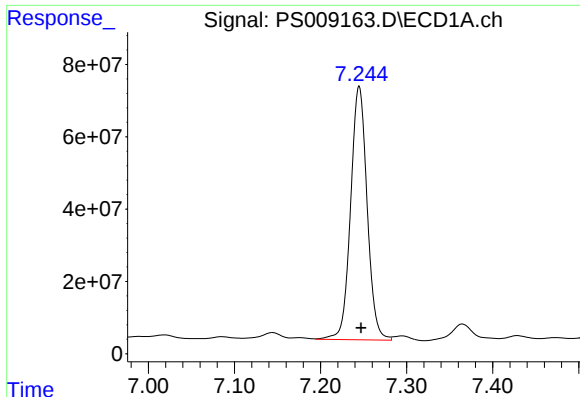

#4 2,4-DCAA


R.T.: 7.245 min
Delta R.T.: -0.002 min
Response: 933651669
Conc: 426.99 ng/ml

Instrument :
ECD_S
ClientSampleId :

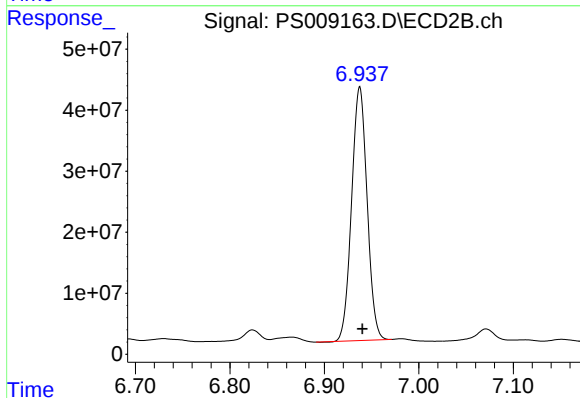


#4 2,4-DCAA

R.T.: 6.937 min
Delta R.T.: -0.003 min
Response: 473743377
Conc: 491.66 ng/ml

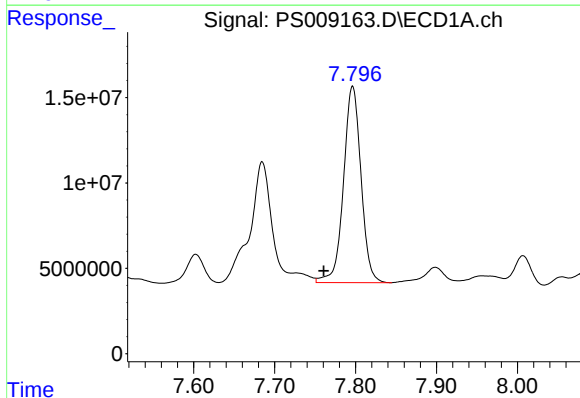


#7 MCPA

R.T.: 7.796 min
Delta R.T.: 0.036 min
Response: 172971493
Conc: 21.50 ug/ml

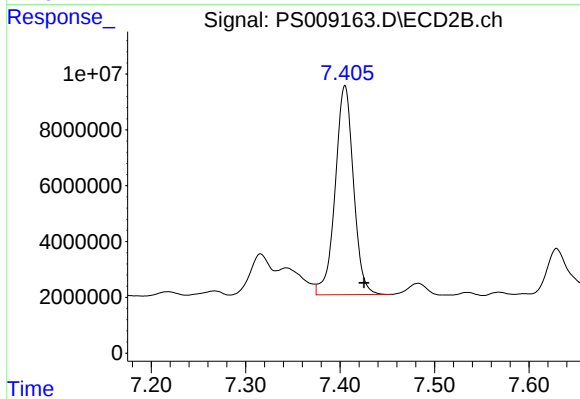

#7 MCPA


R.T.: 7.405 min
Delta R.T.: -0.020 min
Response: 100951949
Conc: 22.82 ug/ml

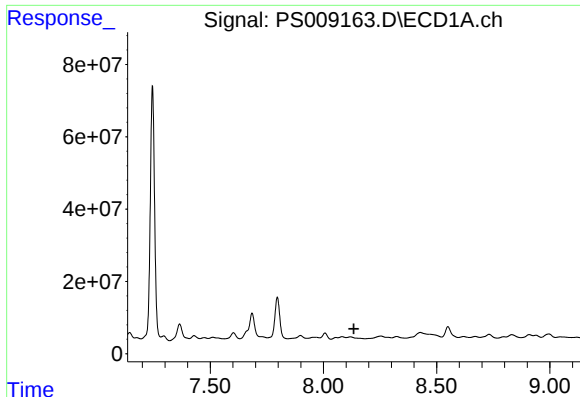

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.135 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

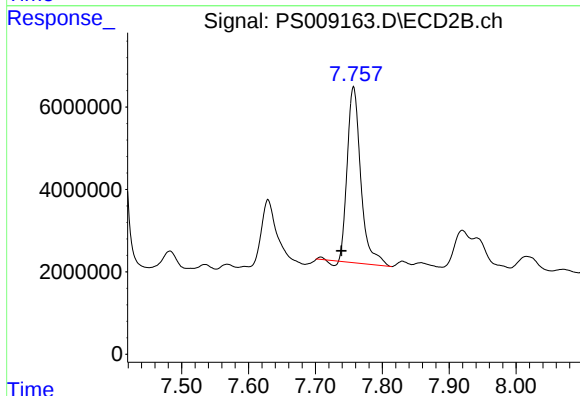


#8 DICHLORPROP

R.T.: 7.757 min
Delta R.T.: 0.018 min
Response: 59703821
Conc: 59.59 ng/ml

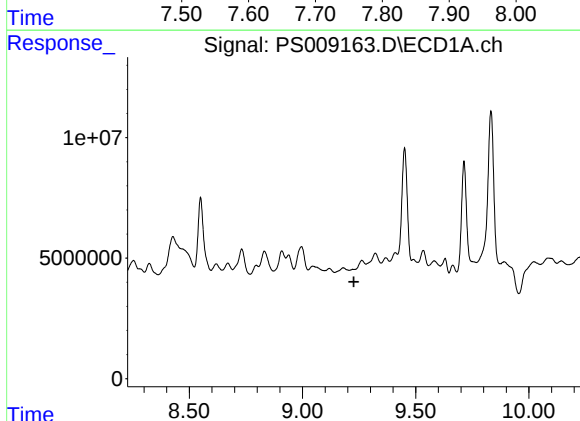


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 9.227 min
Response: 0
Conc: N.D.

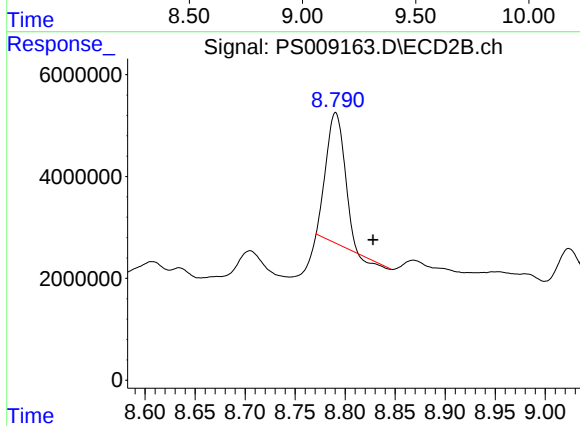

#11 2,4,5-TP (SILVEX)


R.T.: 8.791 min
Delta R.T.: -0.037 min
Response: 32340222
Conc: 5.97 ng/ml

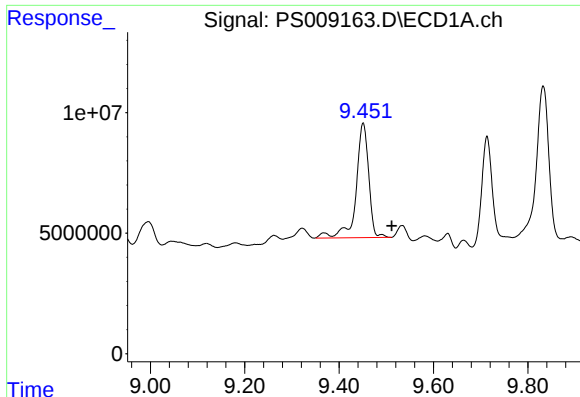

#12 2,4,5-T


R.T.: 9.451 min
Delta R.T.: -0.060 min
Response: 88317877
Conc: 8.26 ng/ml

Instrument :
ECD_S
ClientSampleId :

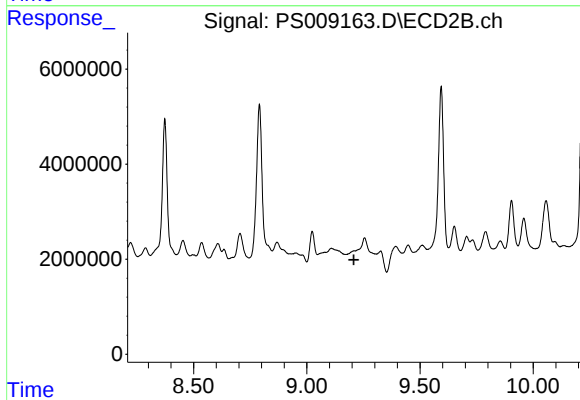


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.208 min
Response: 0
Conc: N.D.

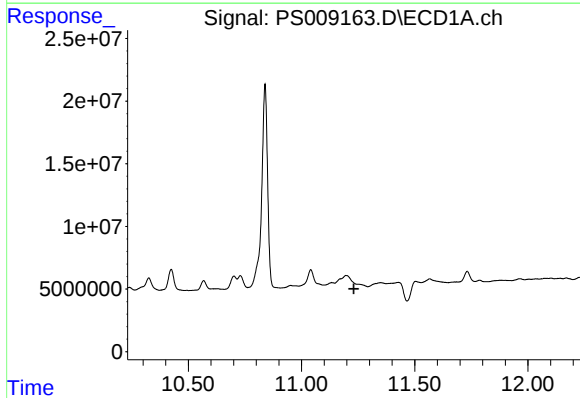


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.231 min
Response: 0
Conc: N.D.

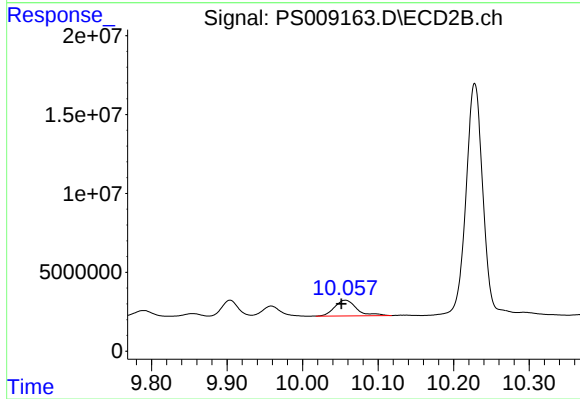

#14 DINOSEB


R.T.: 10.057 min
Delta R.T.: 0.005 min
Response: 20186746
Conc: 5.11 ng/ml

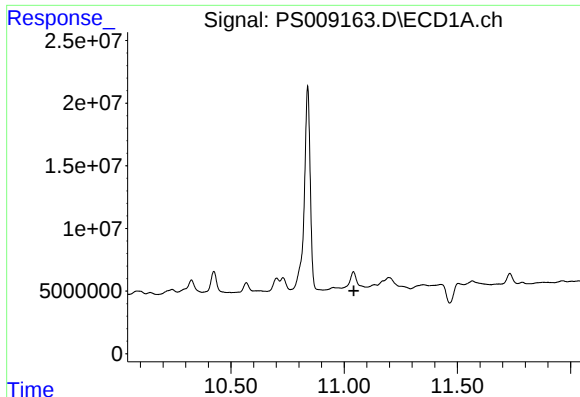

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 11.043 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

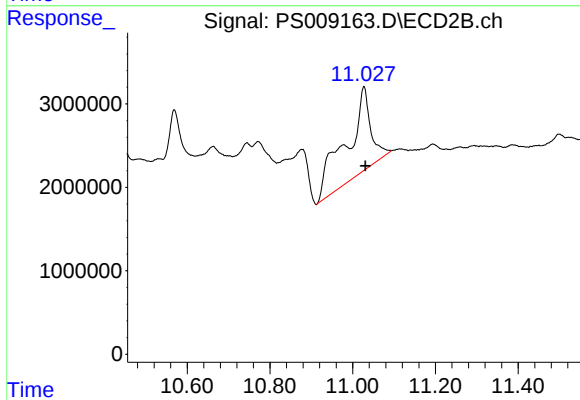


#15 Picloram

R.T.: 11.027 min
Delta R.T.: -0.004 min
Response: 42228875
Conc: 5.81 ng/ml

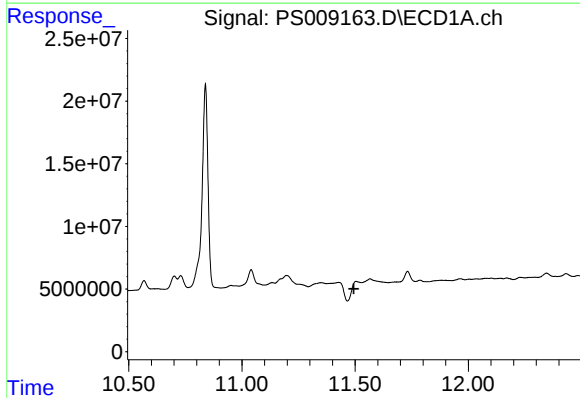

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.495 min
Response: 0
Conc: N.D.

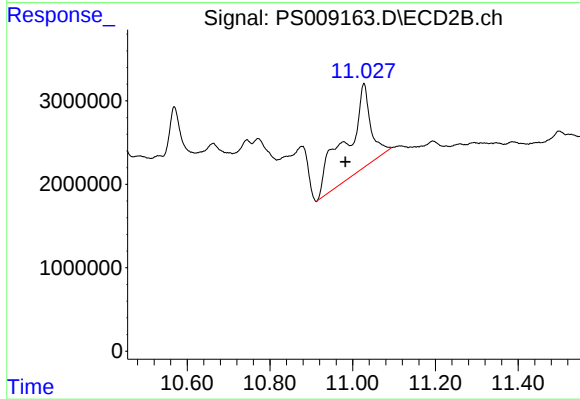

#16 DCPA

R.T.: 11.027 min
Delta R.T.: 0.045 min
Response: 42228875
Conc: 6.10 ng/ml