

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030620\
 Data File : PS009166.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Mar 2020 21:52
 Operator : DD\AJ
 Sample : L1792-03
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 06 23:25:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.246	6.937	395.7E6	174.7E6	180.971	181.280
Target Compounds							
1) T	Dalapon	0.000	2.589	0 30608547		N.D.	20.933
2) T	3,5-DICHL...	0.000	6.113	0 191.6E6		N.D.	131.323
7) T	MCPA	7.797	7.405	234.8E6	143.6E6	29.189	32.461
8) T	DICHLORPROP	0.000	7.757	0 64099898		N.D.	63.976
9) T	2,4-D	0.000	8.012	0 12513128		N.D.	10.561
11) T	2,4,5-TP ...	0.000	8.789	0 40401045		N.D.	7.458
12) T	2,4,5-T	9.451	0.000	140.2E6	0	13.113	N.D. #
13) T	2,4-DB	0.000	9.732	0 27757430		N.D.	39.516
14) T	DINOSEB	0.000	10.058	0 42880202		N.D.	10.845
15) T	Picloram	0.000	11.028	0 41380212		N.D.	5.695
16) T	DCPA	0.000	11.028	0 41380212		N.D.	5.980



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030620\
Data File : PS009166.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2020 21:52
Operator : DD\AJ
Sample : L1792-03
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 06 23:25:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

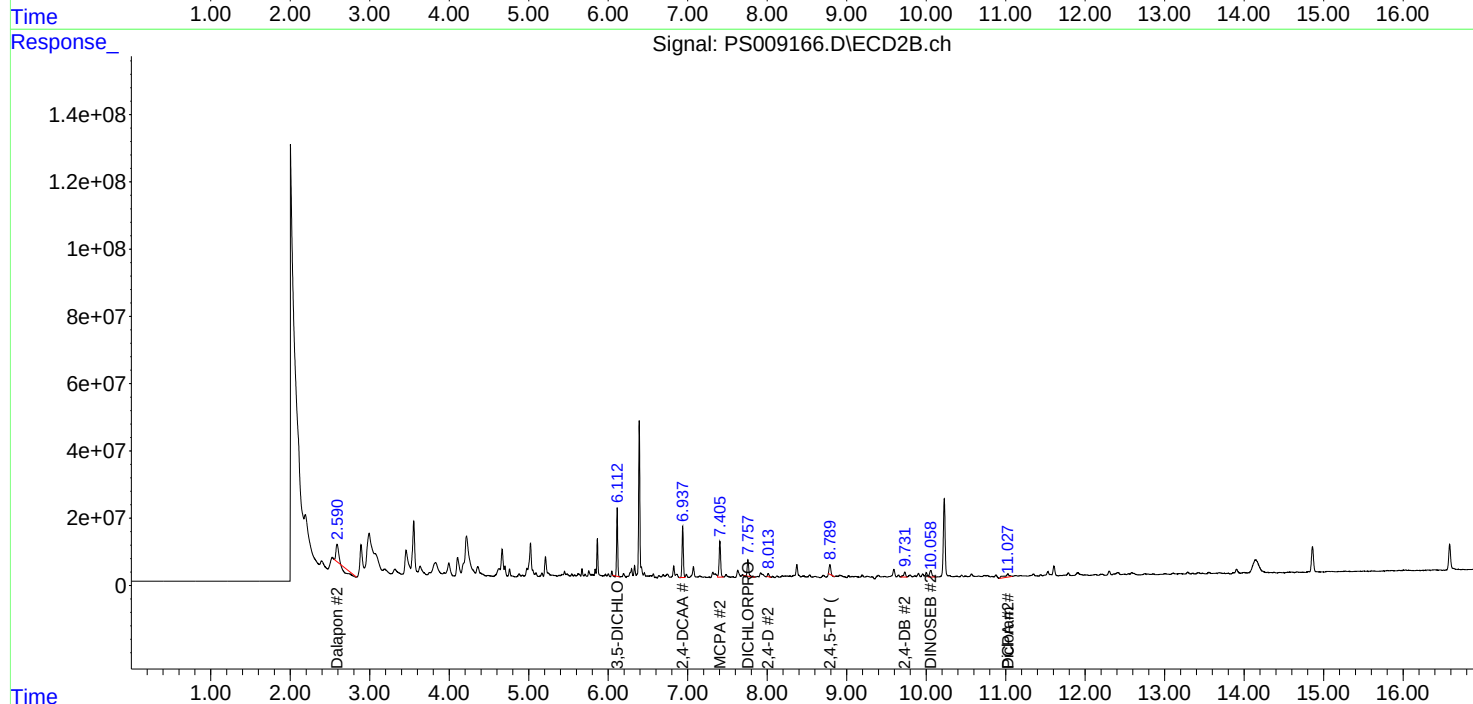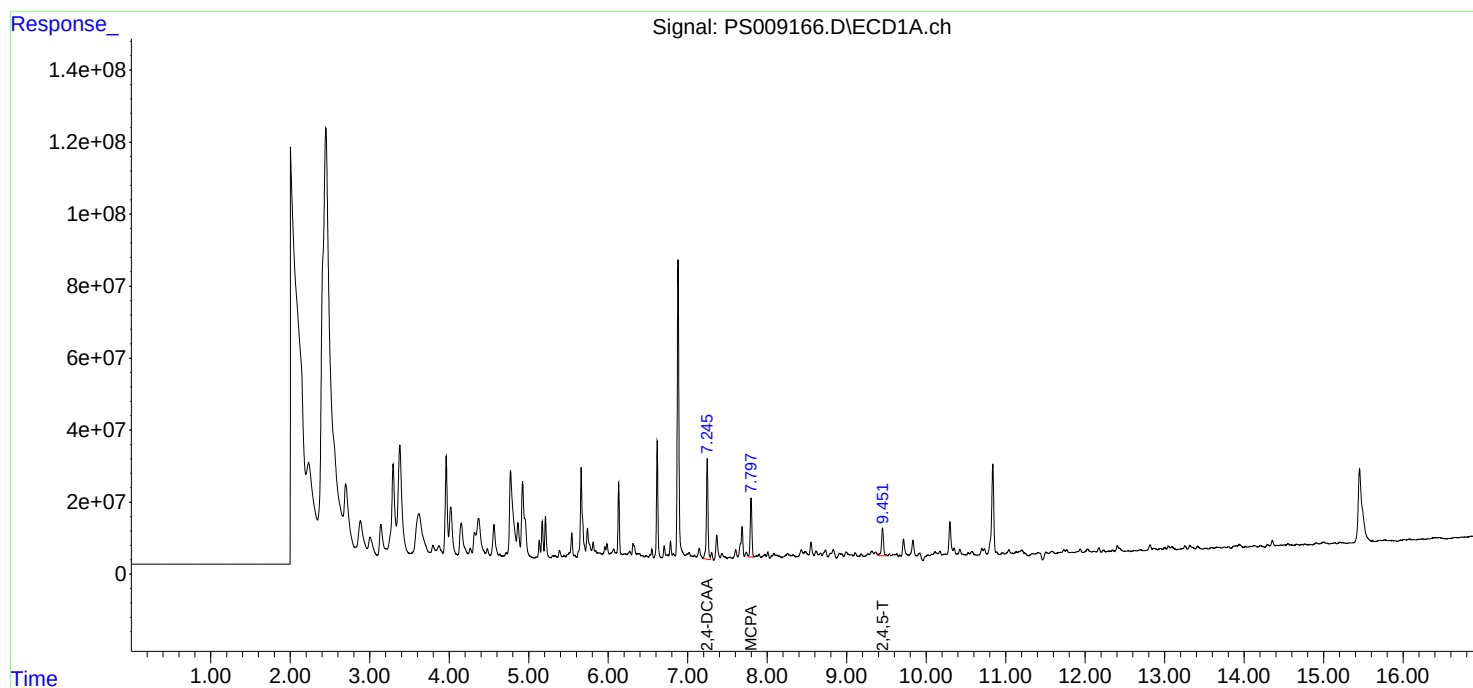


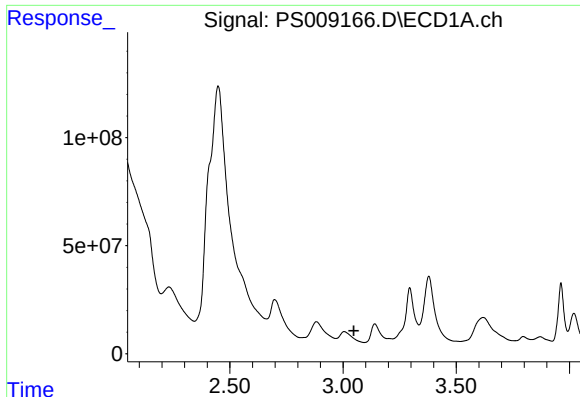

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.048 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

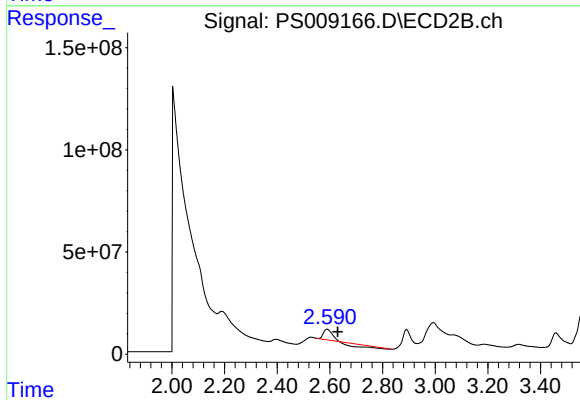


#1 Dalapon

R.T.: 2.589 min
Delta R.T.: -0.041 min
Response: 30608547
Conc: 20.93 ng/ml

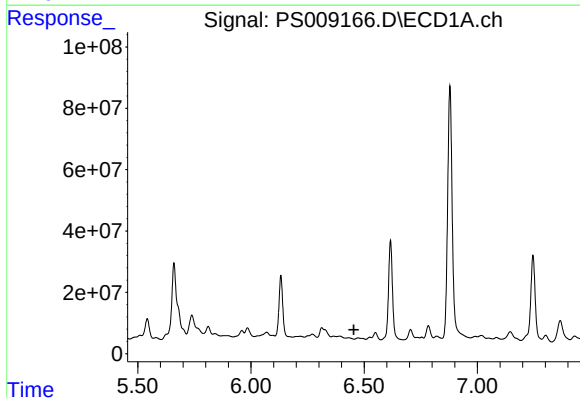


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

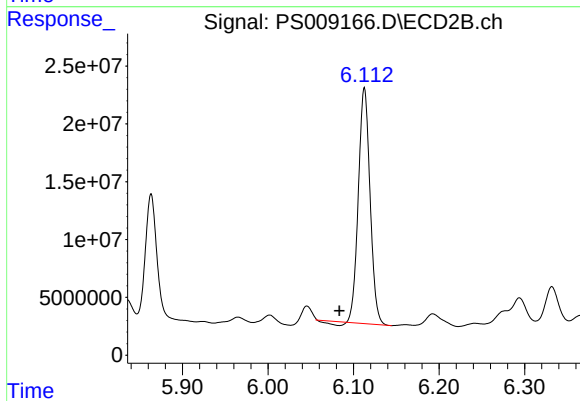

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.113 min
Delta R.T.: 0.029 min
Response: 191635183
Conc: 131.32 ng/ml

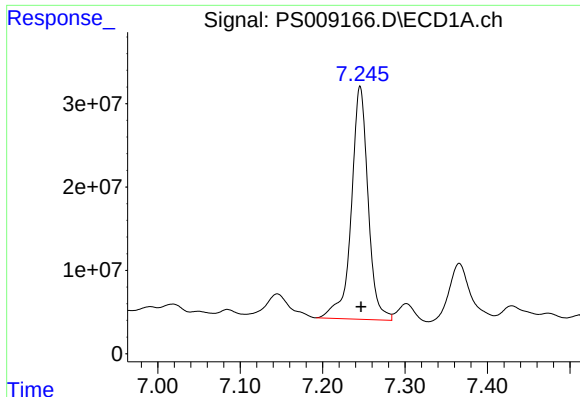

#4 2,4-DCAA


R.T.: 7.246 min
Delta R.T.: -0.001 min
Response: 395710016
Conc: 180.97 ng/ml

Instrument :
ECD_S
ClientSampleId :

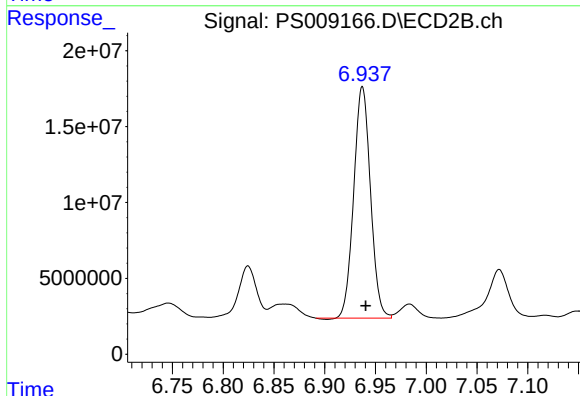


#4 2,4-DCAA

R.T.: 6.937 min
Delta R.T.: -0.003 min
Response: 174673338
Conc: 181.28 ng/ml

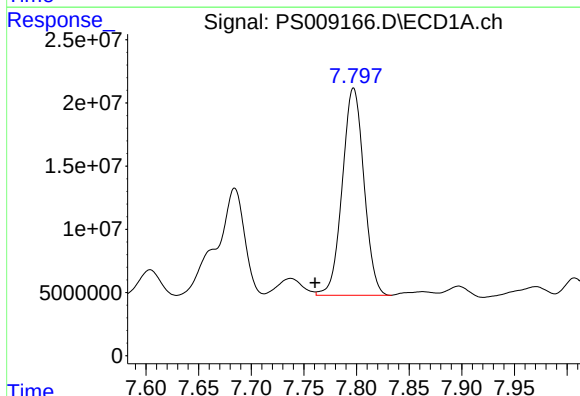


#7 MCPA

R.T.: 7.797 min
Delta R.T.: 0.037 min
Response: 234795511
Conc: 29.19 ug/ml

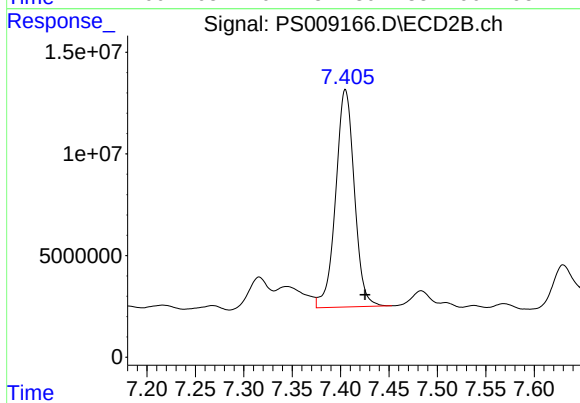

#7 MCPA


R.T.: 7.405 min
Delta R.T.: -0.020 min
Response: 143616648
Conc: 32.46 ug/ml

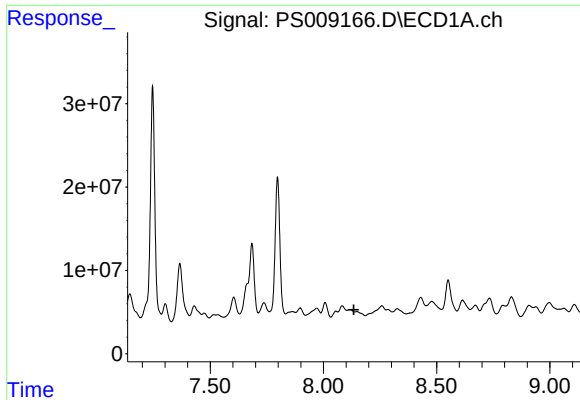

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.135 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

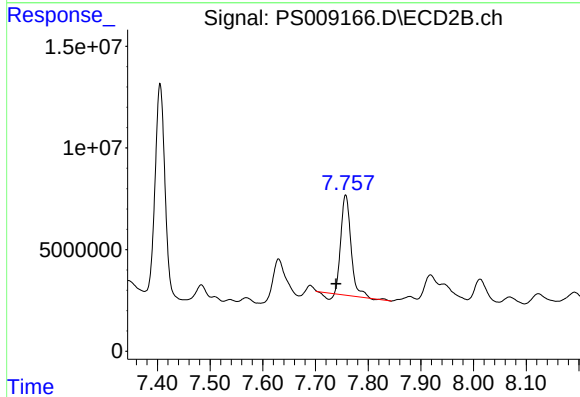


#8 DICHLORPROP

R.T.: 7.757 min
Delta R.T.: 0.018 min
Response: 64099898
Conc: 63.98 ng/ml

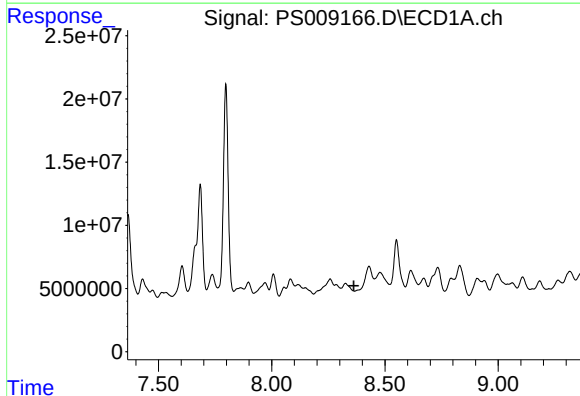


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 8.363 min
Response: 0
Conc: N.D.

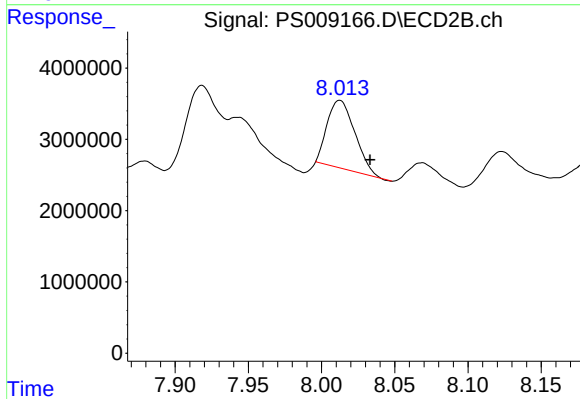

#9 2,4-D


R.T.: 8.012 min
Delta R.T.: -0.021 min
Response: 12513128
Conc: 10.56 ng/ml

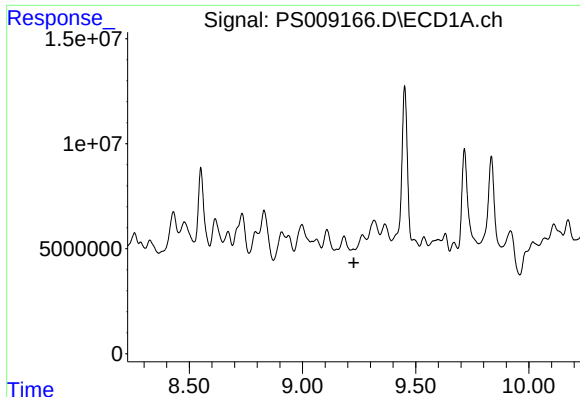

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.227 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

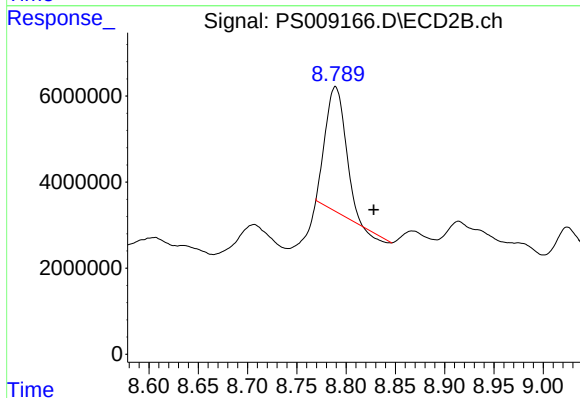


#11 2,4,5-TP (SILVEX)

R.T.: 8.789 min
Delta R.T.: -0.039 min
Response: 40401045
Conc: 7.46 ng/ml

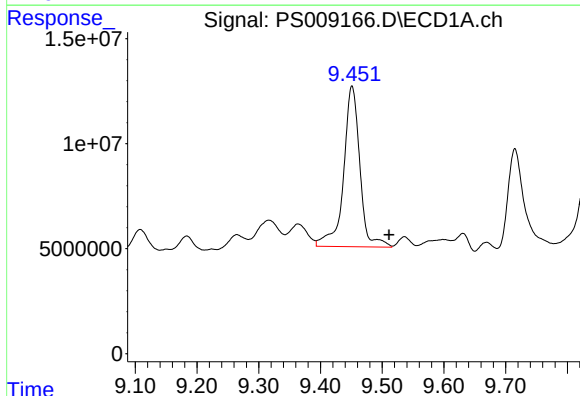


#12 2,4,5-T

R.T.: 9.451 min
Delta R.T.: -0.060 min
Response: 140209374
Conc: 13.11 ng/ml

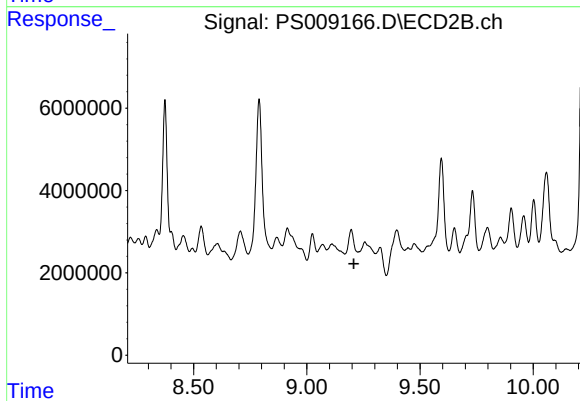

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.208 min
Response: 0
Conc: N.D.

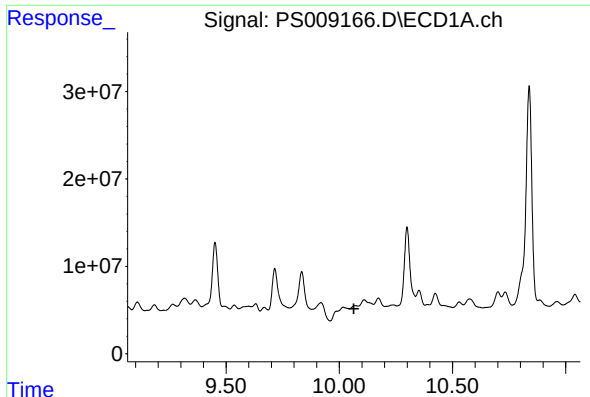

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.064 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

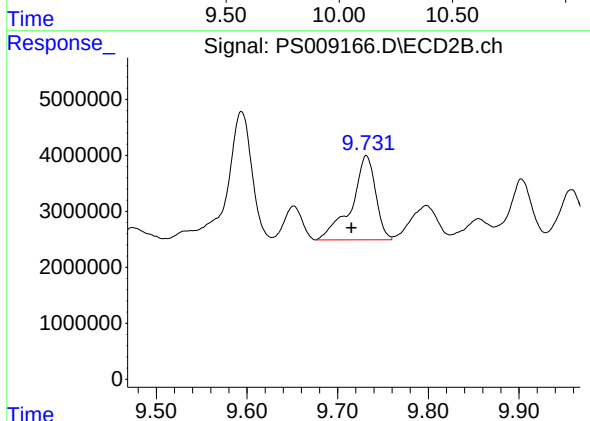


#13 2,4-DB

R.T.: 9.732 min
Delta R.T.: 0.017 min
Response: 27757430
Conc: 39.52 ng/ml

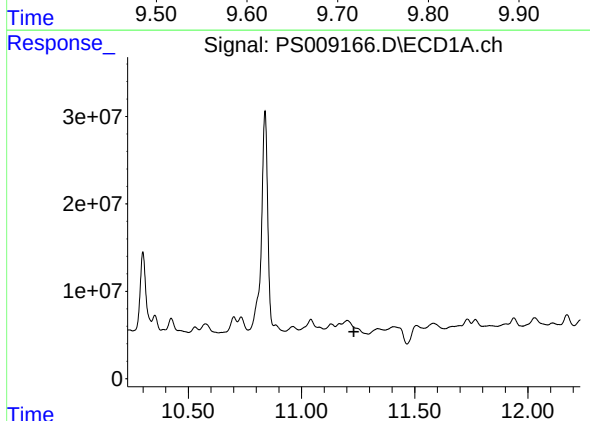


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 11.231 min
Response: 0
Conc: N.D.

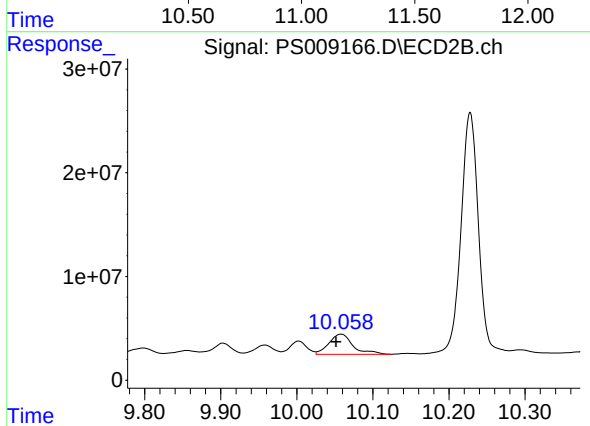

#14 DINOSEB


R.T.: 10.058 min
Delta R.T.: 0.006 min
Response: 42880202
Conc: 10.84 ng/ml

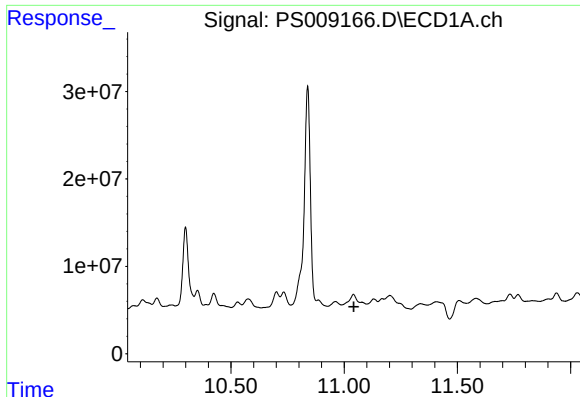

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 11.043 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

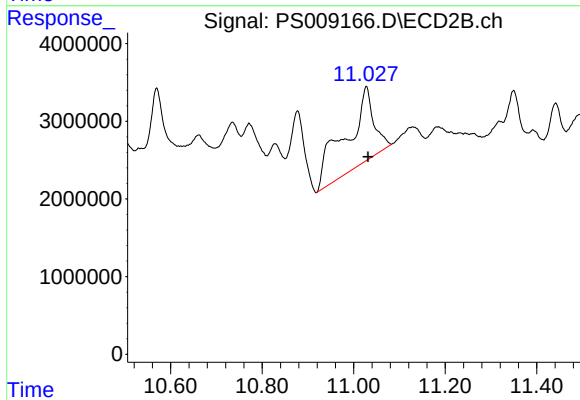


#15 Picloram

R.T.: 11.028 min
Delta R.T.: -0.003 min
Response: 41380212
Conc: 5.69 ng/ml

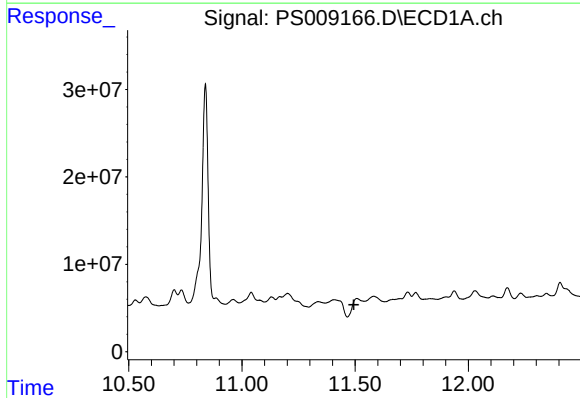

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.495 min
Response: 0
Conc: N.D.

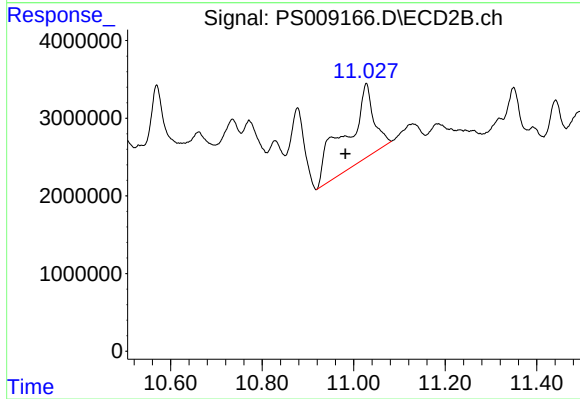

#16 DCPA

R.T.: 11.028 min
Delta R.T.: 0.045 min
Response: 41380212
Conc: 5.98 ng/ml