

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030620\
 Data File : PS009167.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Mar 2020 22:15
 Operator : DD\AJ
 Sample : L1792-05
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 06 23:25:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.245	6.937	579.1E6	267.3E6	264.824	277.444
Target Compounds							
1) T	Dalapon	0.000	2.590	0 17312268		N.D.	11.840
2) T	3,5-DICHL...	0.000	6.113	0 202.6E6		N.D.	138.814
7) T	MCPA	7.797	7.405	174.4E6	123.3E6	21.676	27.864 #
8) T	DICHLORPROP	0.000	7.757	0 58101637		N.D.	57.990
9) T	2,4-D	0.000	7.964	0 45898376		N.D.	38.739
10) T	Pentachlo...	0.000	8.464	0 19462187		N.D.	1.370
11) T	2,4,5-TP ...	0.000	8.788	0 29963580		N.D.	5.531
12) T	2,4,5-T	9.451	9.192	128.9E6	24163462	12.053	4.464 #
13) T	2,4-DB	0.000	9.731	0 66069468		N.D.	94.057
14) T	DINOSEB	0.000	10.060	0 71274650		N.D.	18.026
15) T	Picloram	0.000	11.026	0 29163885		N.D.	4.013
16) T	DCPA	0.000	10.969	0 41318862		N.D.	5.971



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030620\
Data File : PS009167.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2020 22:15
Operator : DD\AJ
Sample : L1792-05
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 06 23:25:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

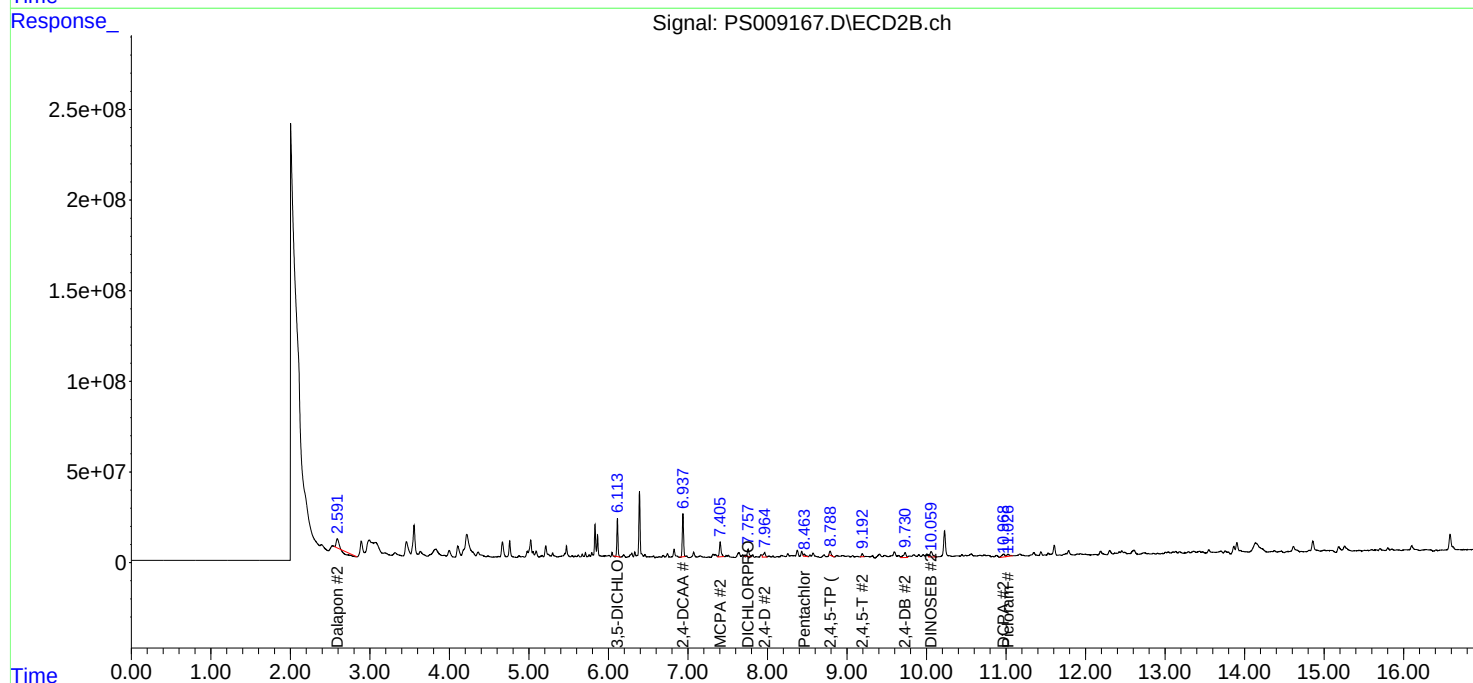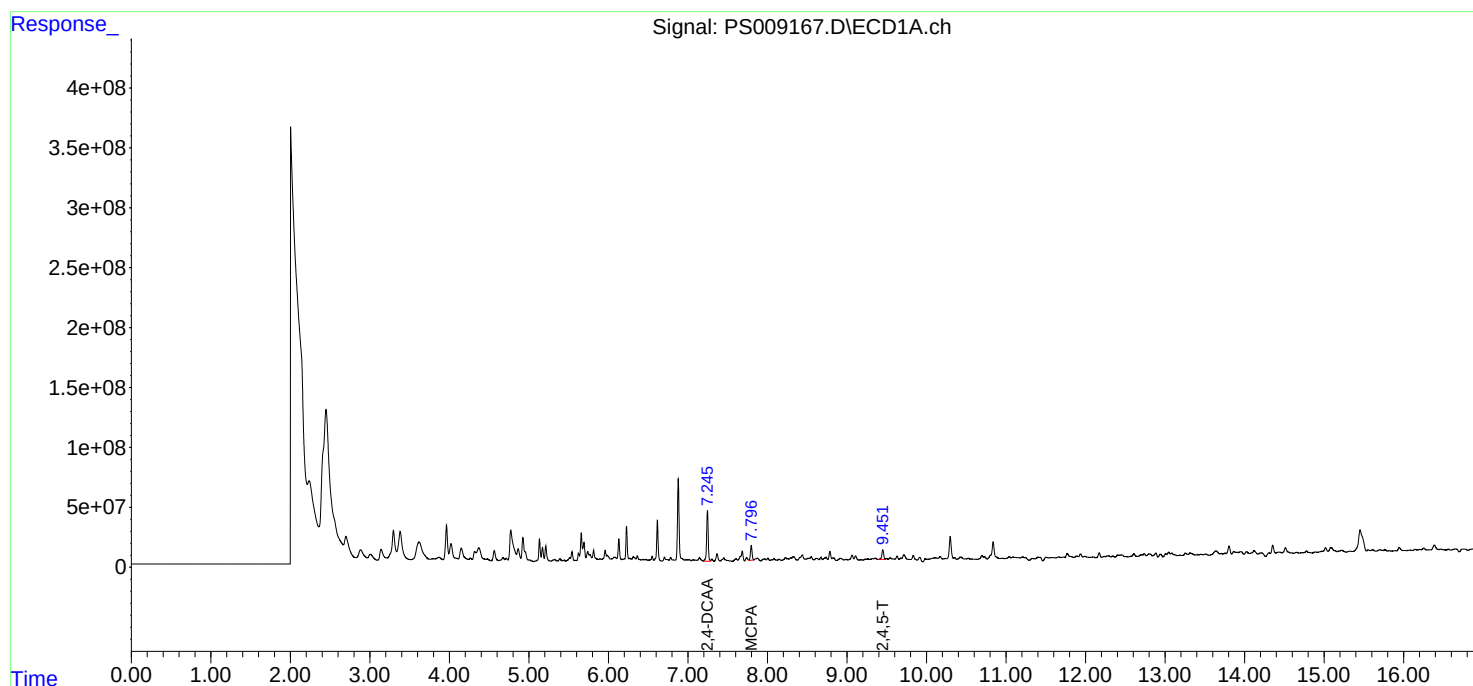


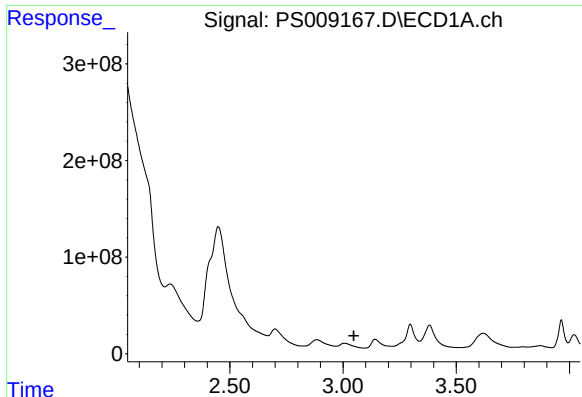

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.048 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

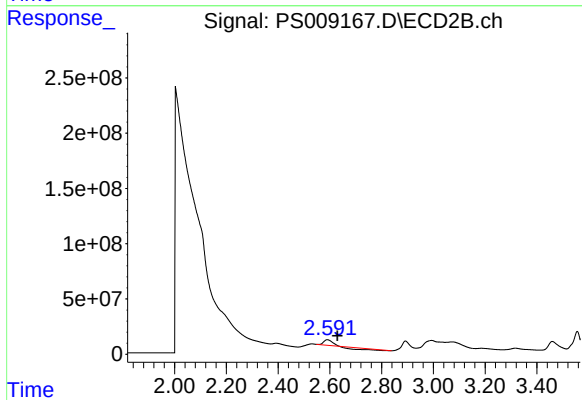


#1 Dalapon

R.T.: 2.590 min
Delta R.T.: -0.040 min
Response: 17312268
Conc: 11.84 ng/ml

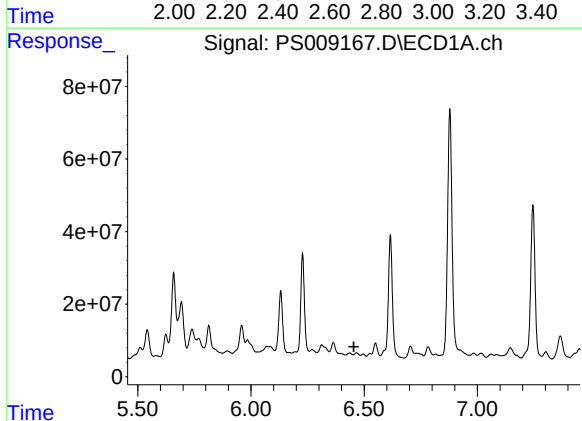


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

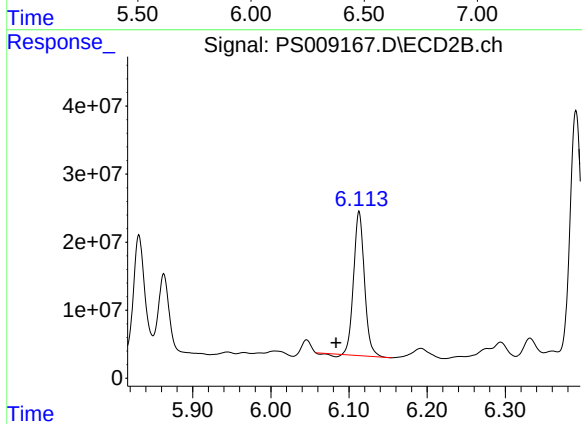

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.113 min
Delta R.T.: 0.030 min
Response: 202566555
Conc: 138.81 ng/ml

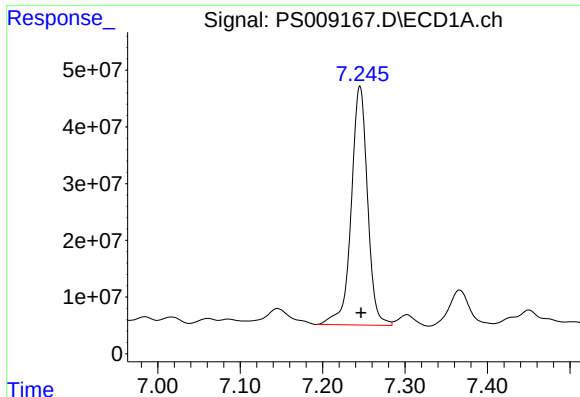

#4 2,4-DCAA


R.T.: 7.245 min
Delta R.T.: -0.002 min
Response: 579062788
Conc: 264.82 ng/ml

Instrument :
ECD_S
ClientSampleId :

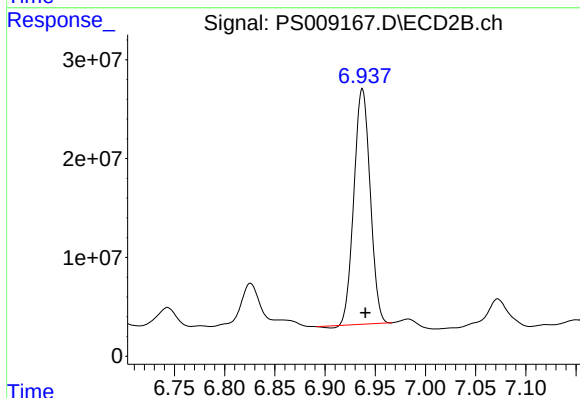


#4 2,4-DCAA

R.T.: 6.937 min
Delta R.T.: -0.003 min
Response: 267332229
Conc: 277.44 ng/ml

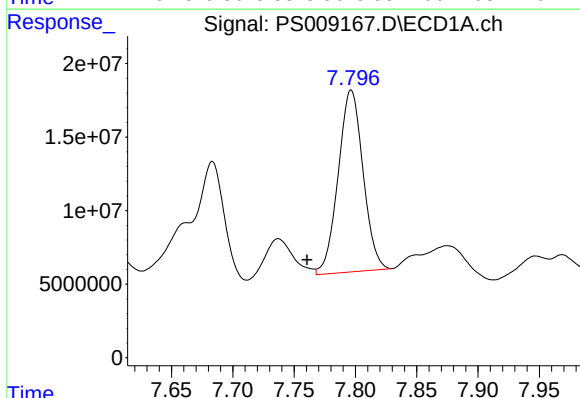


#7 MCPA

R.T.: 7.797 min
Delta R.T.: 0.036 min
Response: 174362222
Conc: 21.68 ug/ml

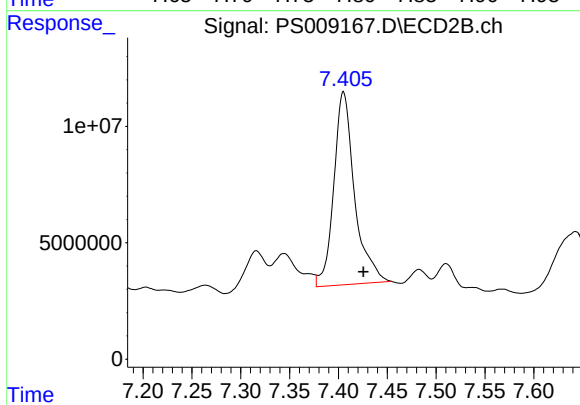

#7 MCPA


R.T.: 7.405 min
Delta R.T.: -0.020 min
Response: 123275080
Conc: 27.86 ug/ml

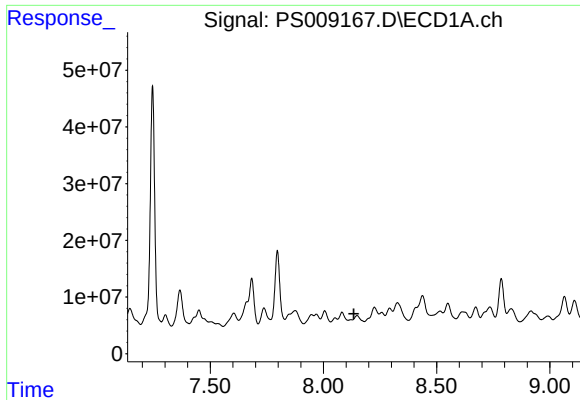

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.135 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

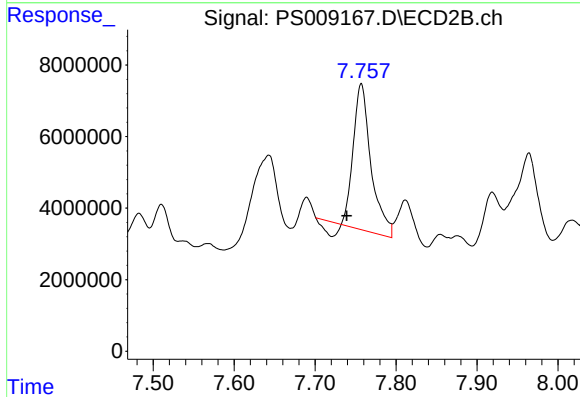


#8 DICHLORPROP

R.T.: 7.757 min
Delta R.T.: 0.018 min
Response: 58101637
Conc: 57.99 ng/ml

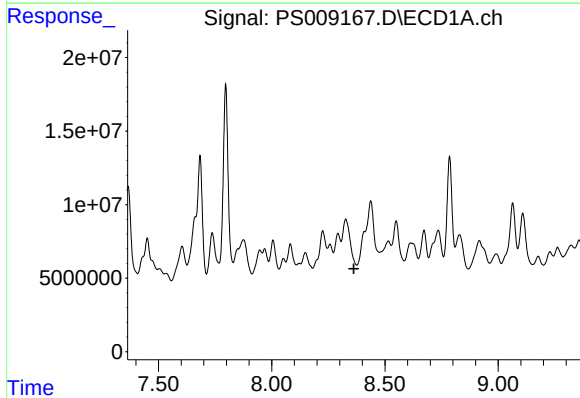


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 8.363 min
Response: 0
Conc: N.D.

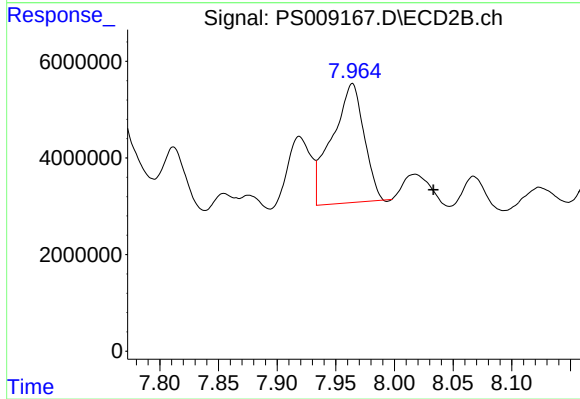

#9 2,4-D


R.T.: 7.964 min
Delta R.T.: -0.069 min
Response: 45898376
Conc: 38.74 ng/ml

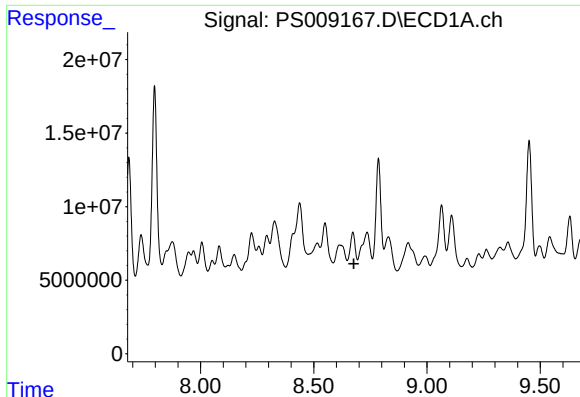

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 8.677 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

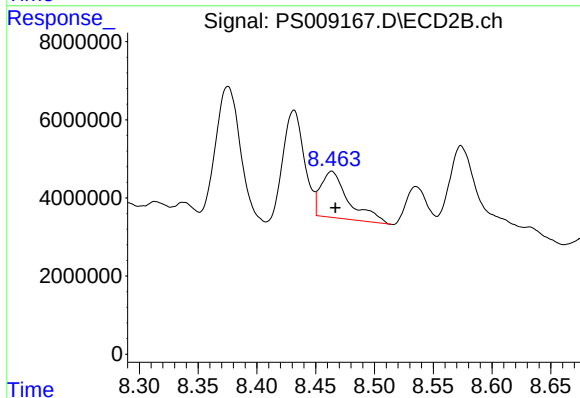


#10 Pentachlorophenol

R.T.: 8.464 min
Delta R.T.: -0.003 min
Response: 19462187
Conc: 1.37 ng/ml

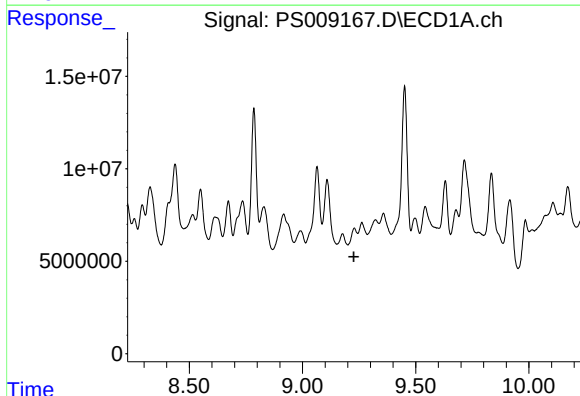


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 9.227 min
Response: 0
Conc: N.D.

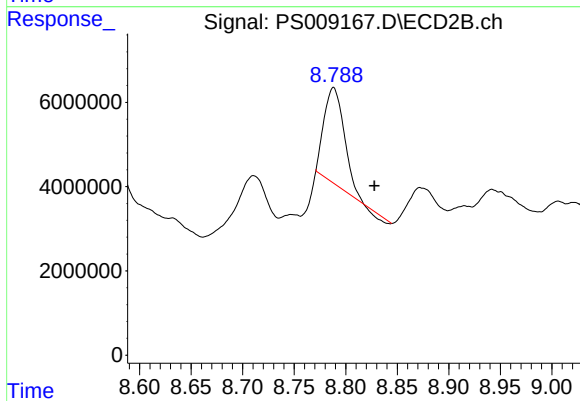

#11 2,4,5-TP (SILVEX)


R.T.: 8.788 min
Delta R.T.: -0.040 min
Response: 29963580
Conc: 5.53 ng/ml

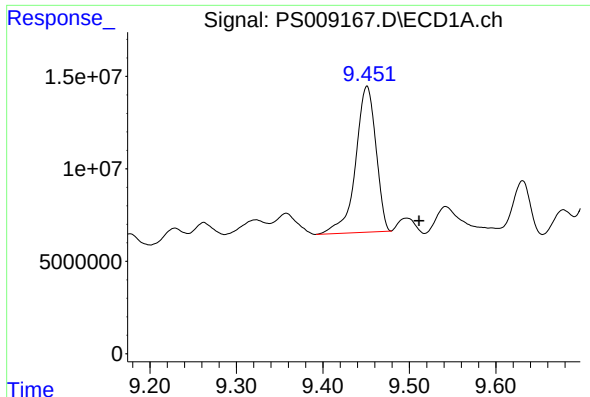

#12 2,4,5-T


R.T.: 9.451 min
Delta R.T.: -0.060 min
Response: 128875514
Conc: 12.05 ng/ml

Instrument :
ECD_S
ClientSampleId :

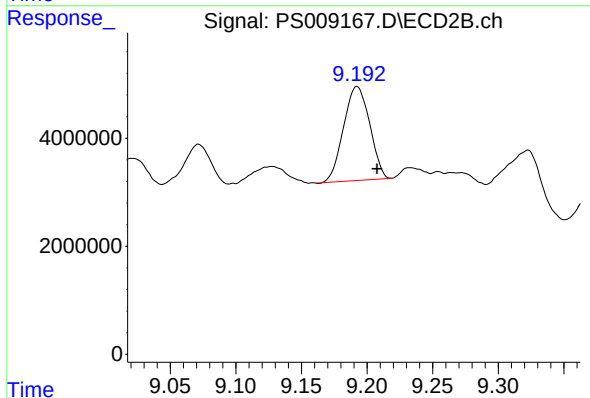


#12 2,4,5-T

R.T.: 9.192 min
Delta R.T.: -0.015 min
Response: 24163462
Conc: 4.46 ng/ml

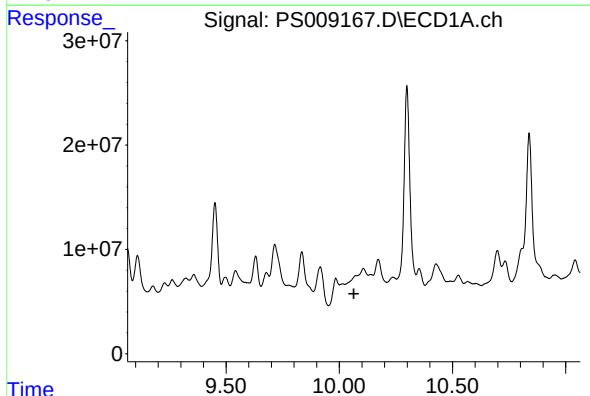


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.064 min
Response: 0
Conc: N.D.

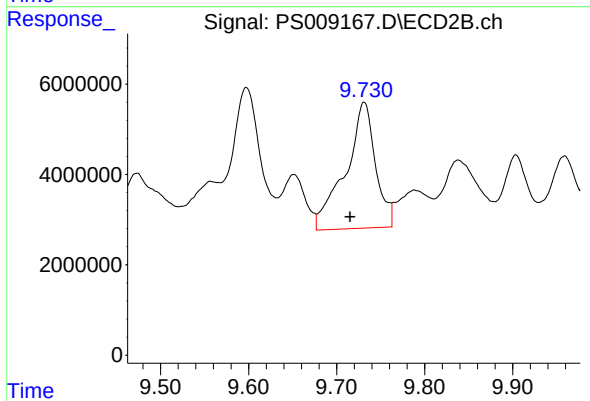

#13 2,4-DB


R.T.: 9.731 min
Delta R.T.: 0.016 min
Response: 66069468
Conc: 94.06 ng/ml

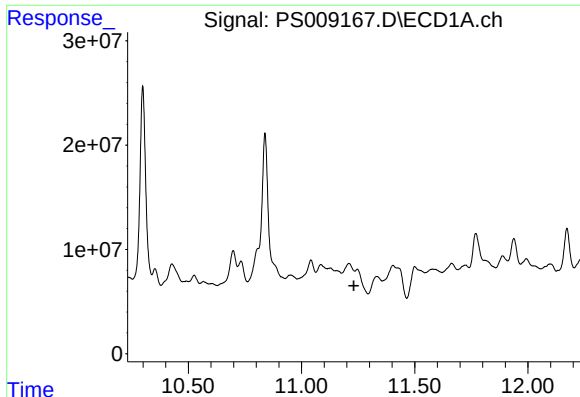

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 11.231 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

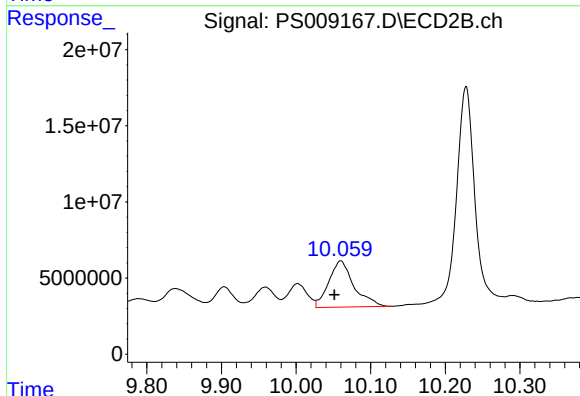


#14 DINOSEB

R.T.: 10.060 min
Delta R.T.: 0.008 min
Response: 71274650
Conc: 18.03 ng/ml

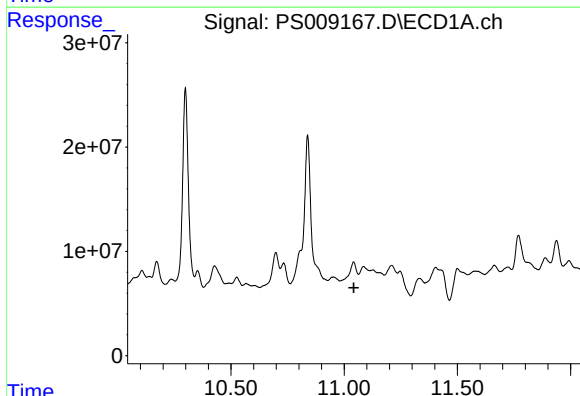


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.043 min
Response: 0
Conc: N.D.

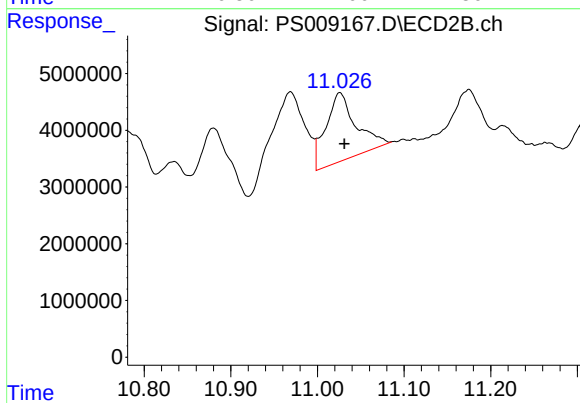

#15 Picloram


R.T.: 11.026 min
Delta R.T.: -0.005 min
Response: 29163885
Conc: 4.01 ng/ml

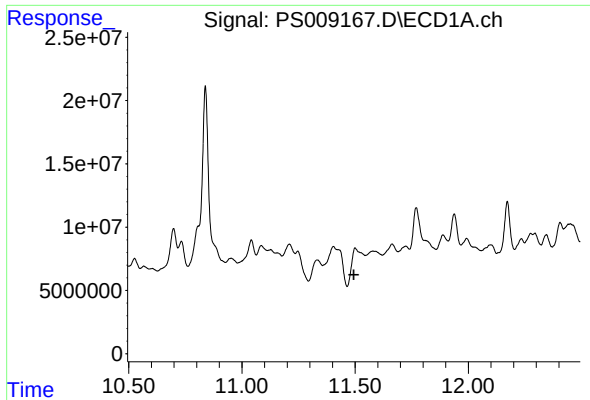

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.495 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

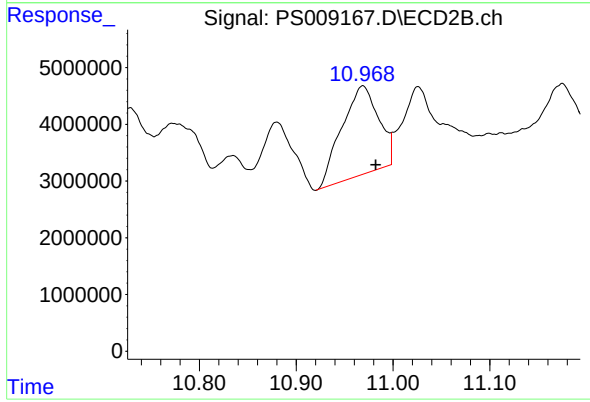

#16 DCPA

R.T.: 10.969 min
Delta R.T.: -0.014 min
Response: 41318862
Conc: 5.97 ng/ml