

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030620\
 Data File : PS009177.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Mar 2020 02:04
 Operator : DD\AJ
 Sample : PB127333BL
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 04:01:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.245	6.937	1160.3E6	588.2E6	530.657	610.470
Target Compounds							
1) T	Dalapon	3.009	2.594	187.3E6	123.7E6	62.598	84.631 #
2) T	3,5-DICHL...	0.000	6.113	0	149.0E6	N.D.	102.139
7) T	MCPA	7.796	7.405	260.1E6	147.7E6	32.332	33.395
8) T	DICHLORPROP	0.000	7.757	0	69385337	N.D.	69.252
11) T	2,4,5-TP ...	0.000	8.790	0	27859058	N.D.	5.143
12) T	2,4,5-T	9.451	0.000	105.4E6	0	9.860	N.D. #
14) T	DINOSEB	0.000	10.058	0	25048391	N.D.	6.335
15) T	Picloram	0.000	11.027	0	43690667	N.D.	6.013
16) T	DCPA	0.000	11.027	0	43690667	N.D.	6.314



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030620\
Data File : PS009177.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Mar 2020 02:04
Operator : DD\AJ
Sample : PB127333BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 04:01:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

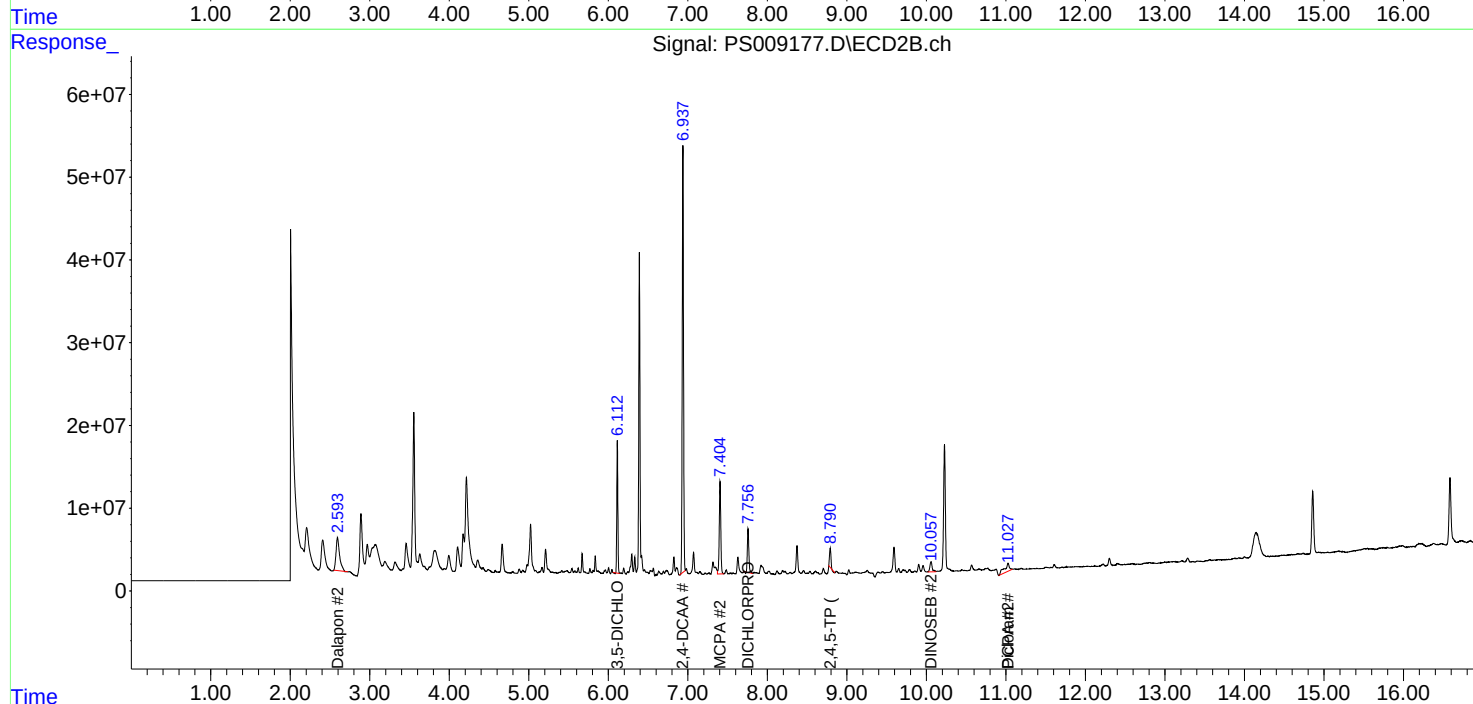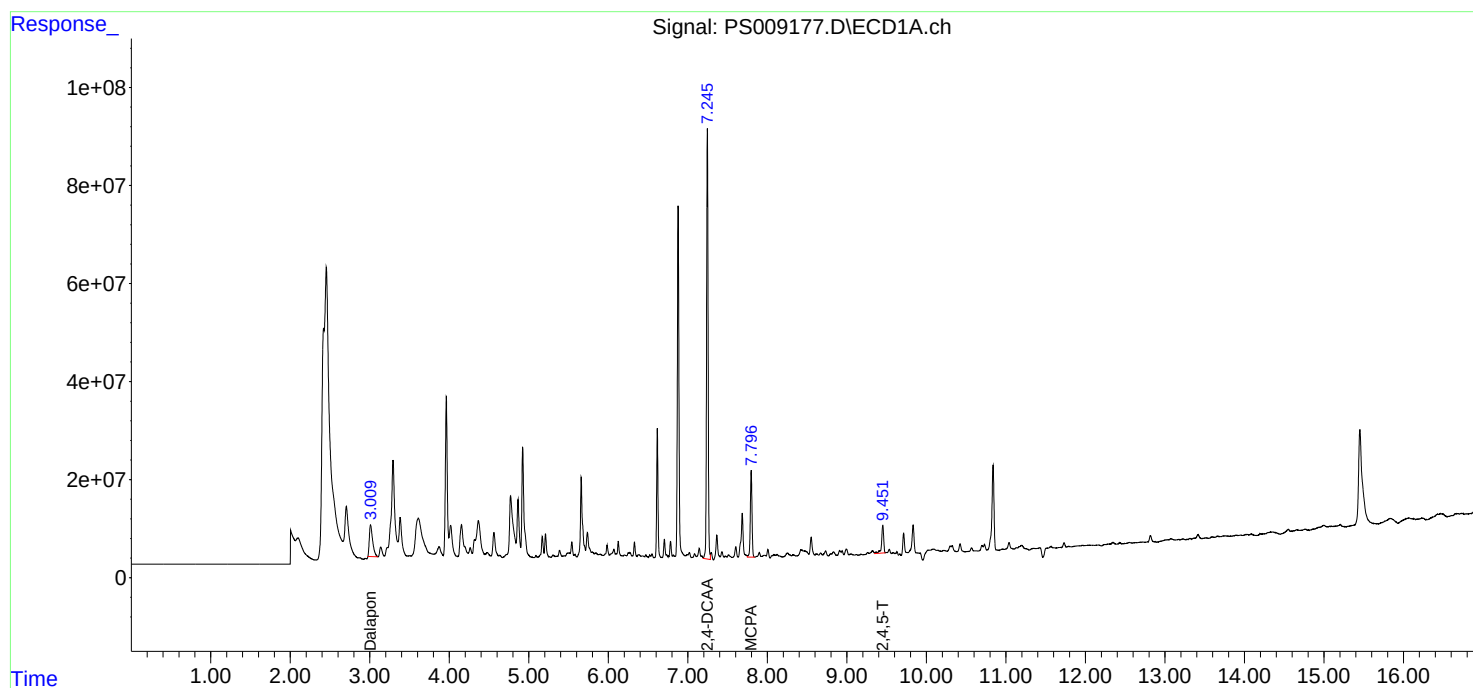


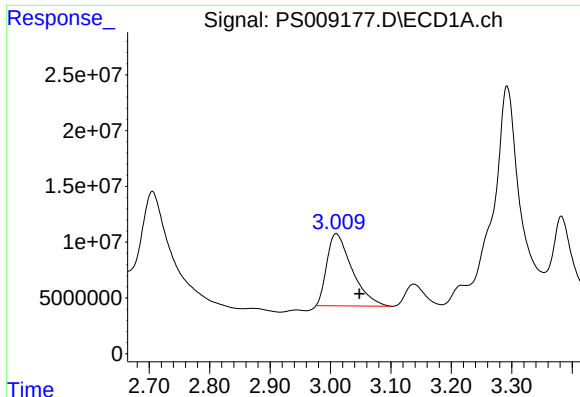

#1 Dalapon


R.T.: 3.009 min
Delta R.T.: -0.039 min
Response: 187278448
Conc: 62.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

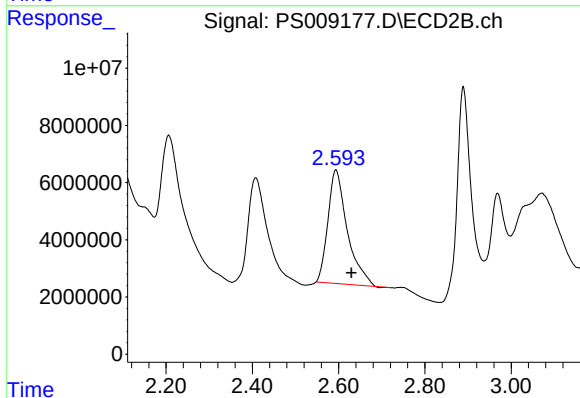


#1 Dalapon

R.T.: 2.594 min
Delta R.T.: -0.036 min
Response: 123749233
Conc: 84.63 ng/ml

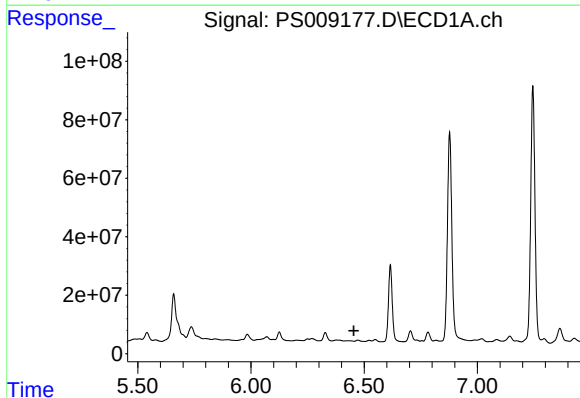


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.455 min
Response: 0
Conc: N.D.

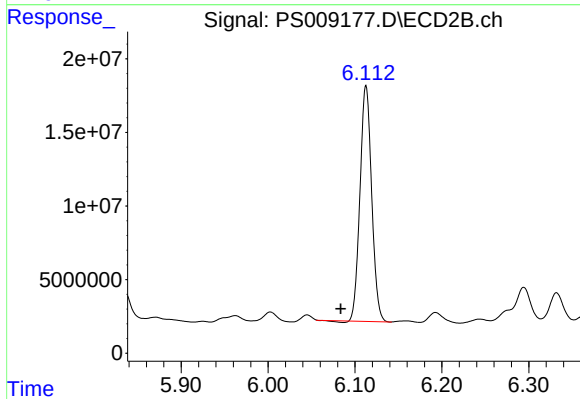

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.113 min
Delta R.T.: 0.029 min
Response: 149048869
Conc: 102.14 ng/ml

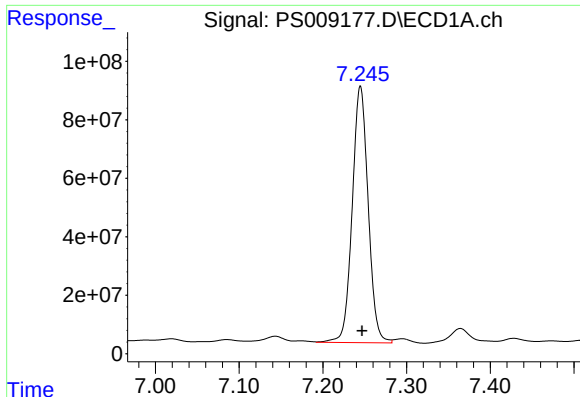

#4 2,4-DCAA


R.T.: 7.245 min
Delta R.T.: -0.002 min
Response: 1160331434
Conc: 530.66 ng/ml

Instrument :
ECD_S
ClientSampleId :

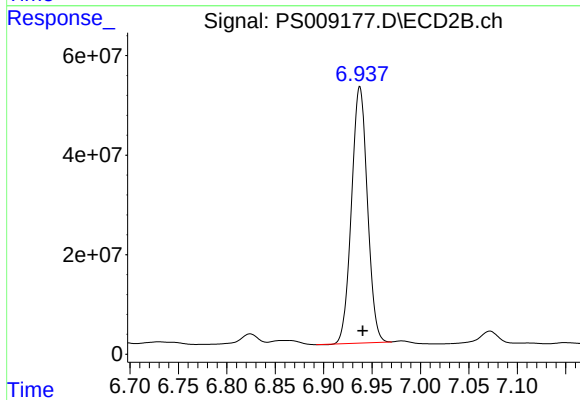


#4 2,4-DCAA

R.T.: 6.937 min
Delta R.T.: -0.003 min
Response: 588221995
Conc: 610.47 ng/ml

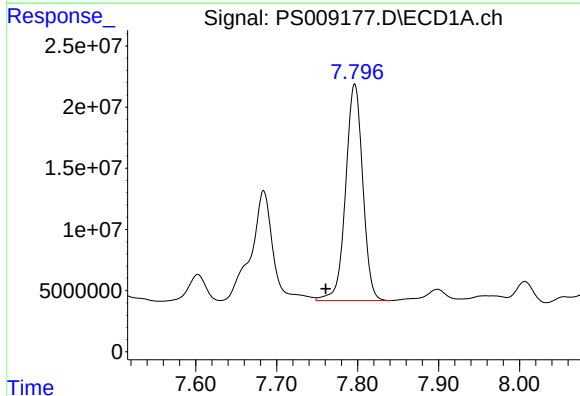


#7 MCPA

R.T.: 7.796 min
Delta R.T.: 0.036 min
Response: 260076821
Conc: 32.33 ug/ml

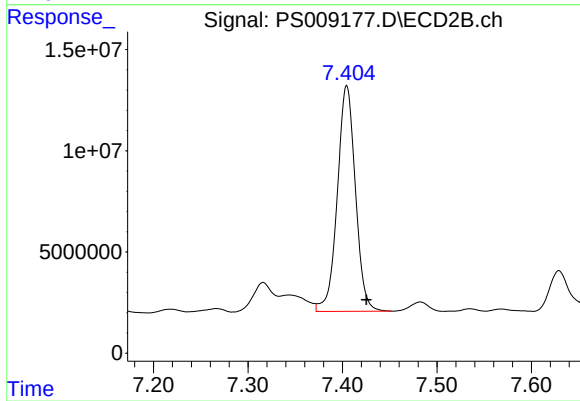

#7 MCPA


R.T.: 7.405 min
Delta R.T.: -0.021 min
Response: 147749252
Conc: 33.40 ug/ml

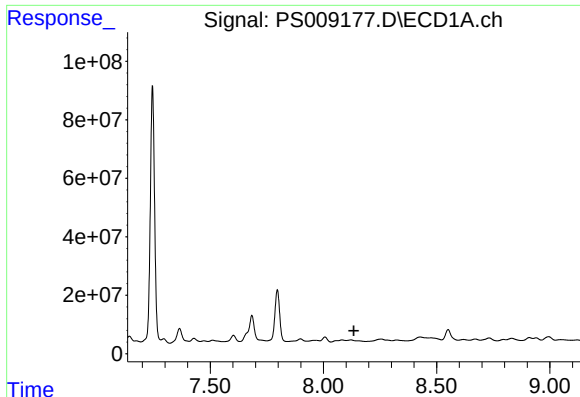

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.135 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

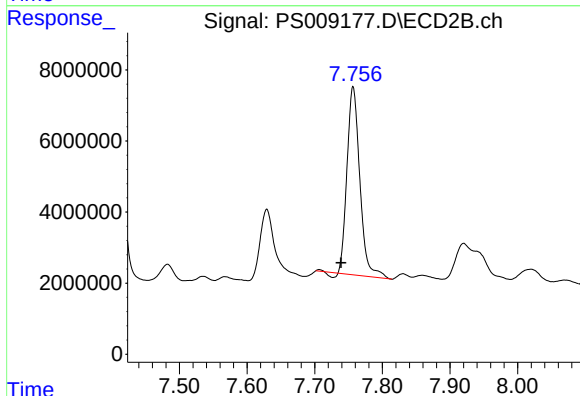


#8 DICHLORPROP

R.T.: 7.757 min
Delta R.T.: 0.018 min
Response: 69385337
Conc: 69.25 ng/ml

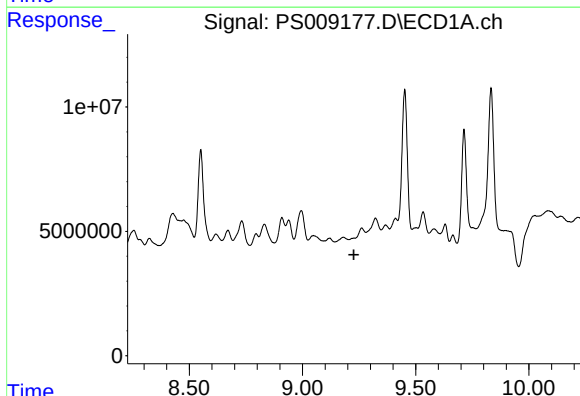


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 9.227 min
Response: 0
Conc: N.D.

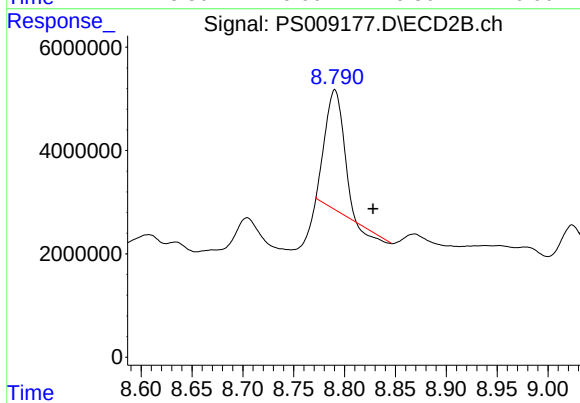

#11 2,4,5-TP (SILVEX)


R.T.: 8.790 min
Delta R.T.: -0.038 min
Response: 27859058
Conc: 5.14 ng/ml

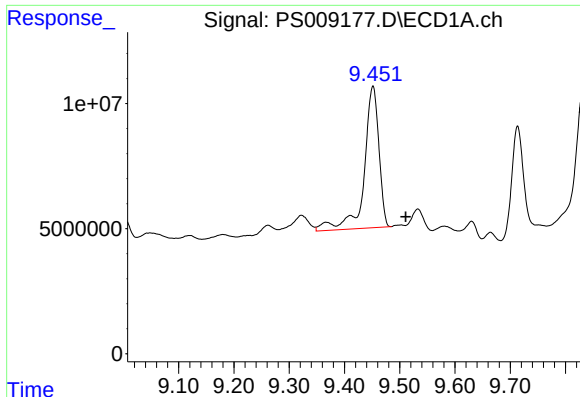

#12 2,4,5-T


R.T.: 9.451 min
Delta R.T.: -0.060 min
Response: 105420098
Conc: 9.86 ng/ml

Instrument :
ECD_S
ClientSampleId :

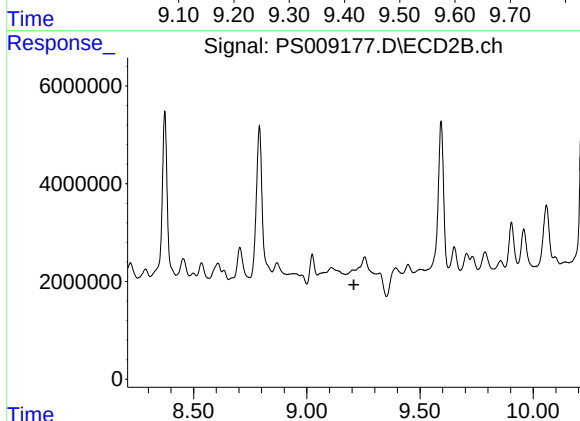


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.208 min
Response: 0
Conc: N.D.

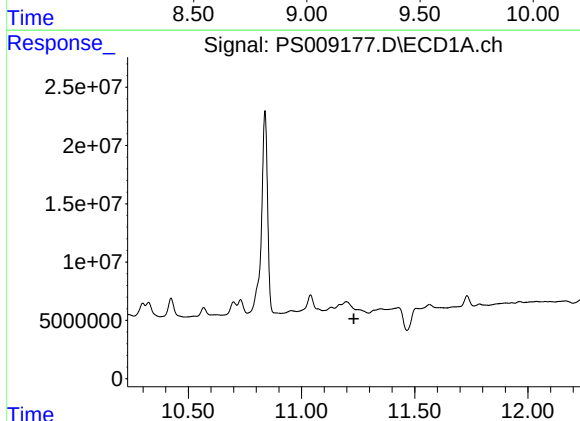


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.231 min
Response: 0
Conc: N.D.

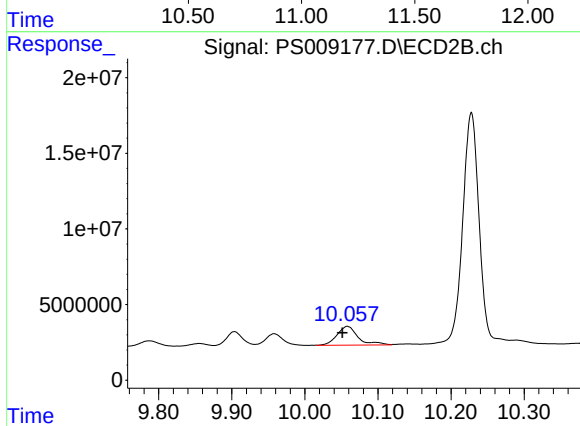

#14 DINOSEB


R.T.: 10.058 min
Delta R.T.: 0.007 min
Response: 25048391
Conc: 6.33 ng/ml

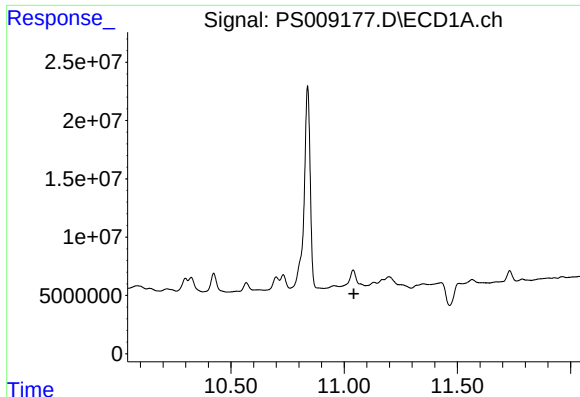

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 11.043 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

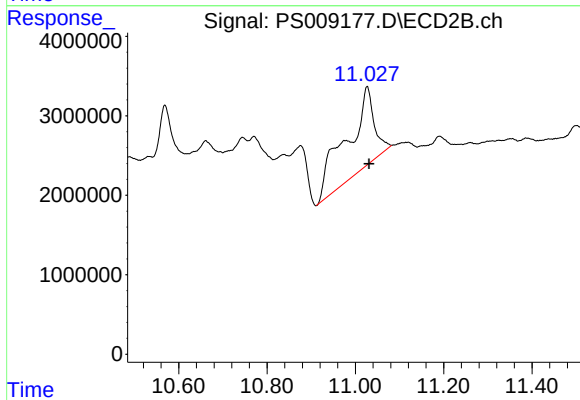


#15 Picloram

R.T.: 11.027 min
Delta R.T.: -0.004 min
Response: 43690667
Conc: 6.01 ng/ml

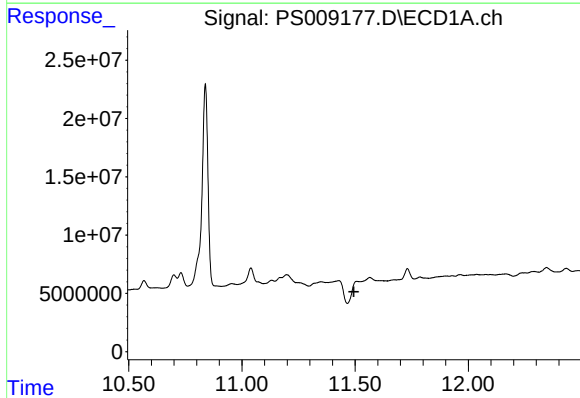

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.495 min
Response: 0
Conc: N.D.

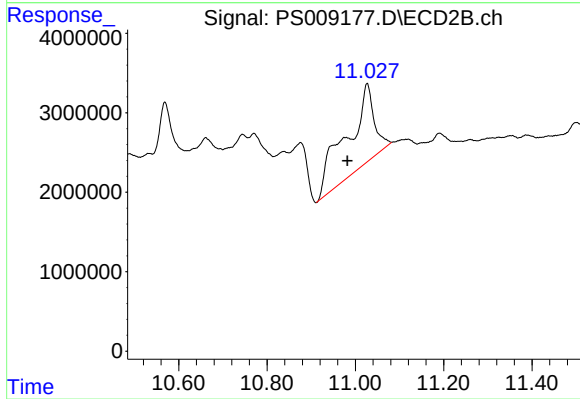

#16 DCPA

R.T.: 11.027 min
Delta R.T.: 0.044 min
Response: 43690667
Conc: 6.31 ng/ml