

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030620\
 Data File : PS009179.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Mar 2020 02:49
 Operator : DD\AJ
 Sample : PB127333TB
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 04:01:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.245	6.937	1025.4E6	561.1E6	468.936	582.275
Target Compounds							
1) T	Dalapon	3.009	2.593	162.4E6	99552858	54.285	68.083 #
2) T	3,5-DICHL...	0.000	6.112	0	167.2E6	N.D.	114.549
8) T	DICHLORPROP	0.000	7.757	0	73275972	N.D.	73.135
12) T	2,4,5-T	9.450	0.000	151.0E6	0	14.122	N.D. #
15) T	Picloram	0.000	11.026	0	33091178	N.D.	4.554
16) T	DCPA	0.000	11.026	0	33091178	N.D.	4.782



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030620\
Data File : PS009179.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Mar 2020 02:49
Operator : DD\AJ
Sample : PB127333TB
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 04:01:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

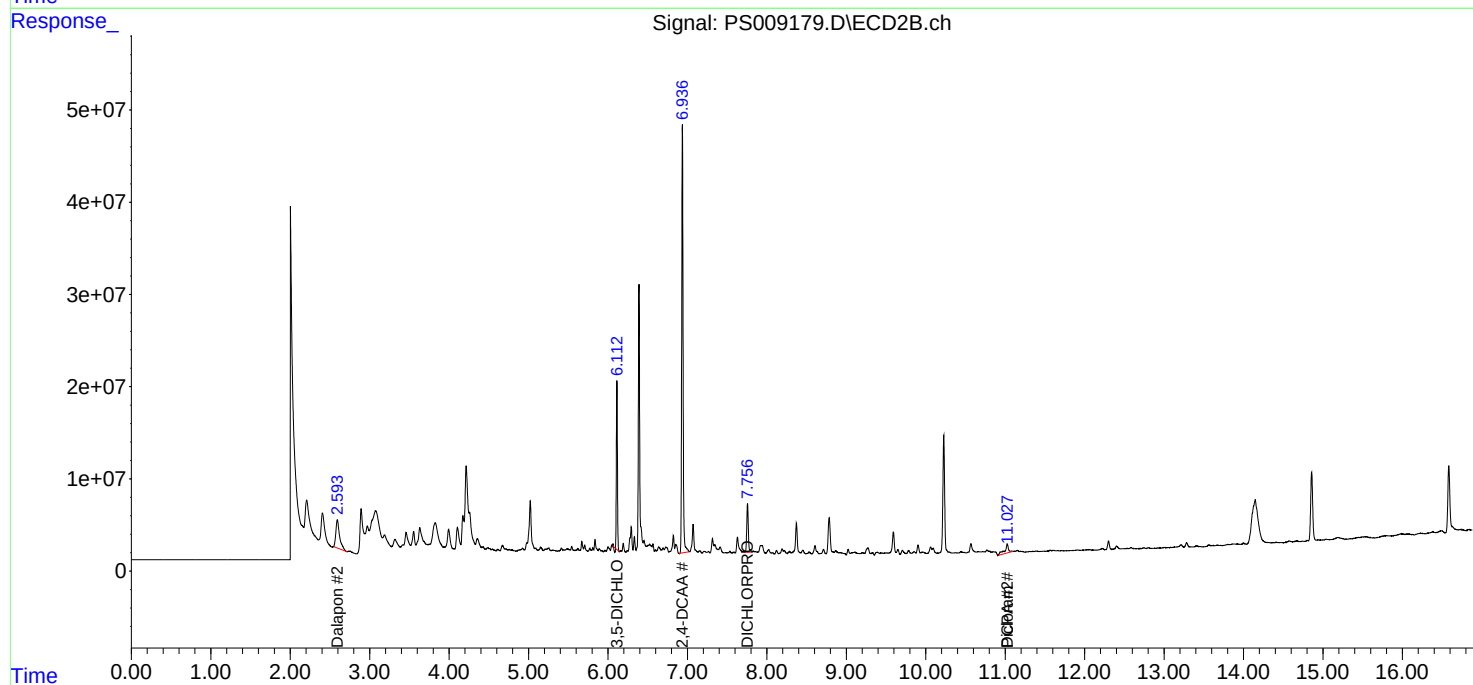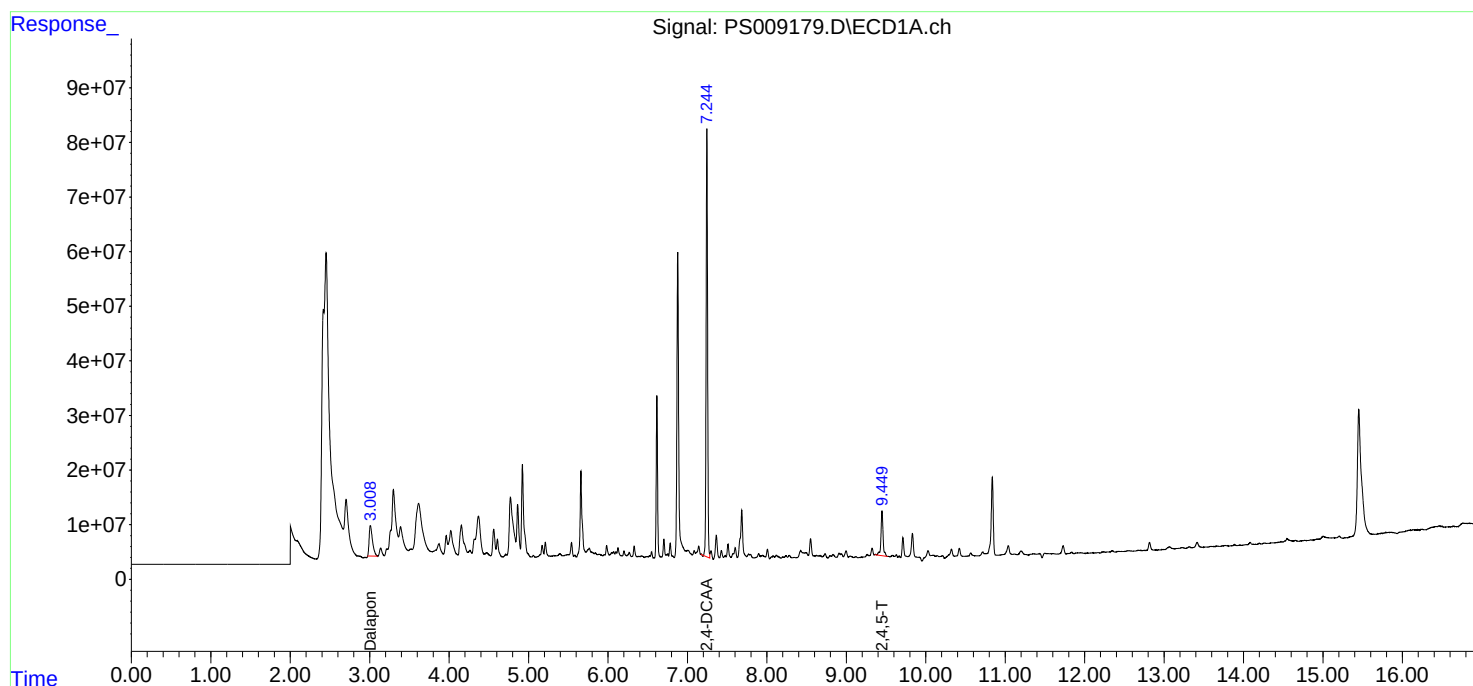


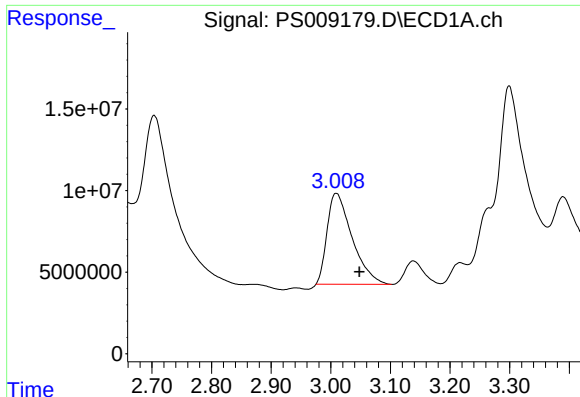

#1 Dalapon


R.T.: 3.009 min
Delta R.T.: -0.039 min
Response: 162408001
Conc: 54.28 ng/ml

Instrument :
ECD_S
ClientSampleId :

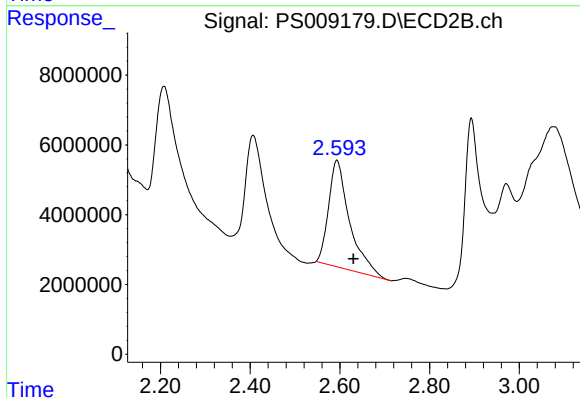


#1 Dalapon

R.T.: 2.593 min
Delta R.T.: -0.037 min
Response: 99552858
Conc: 68.08 ng/ml

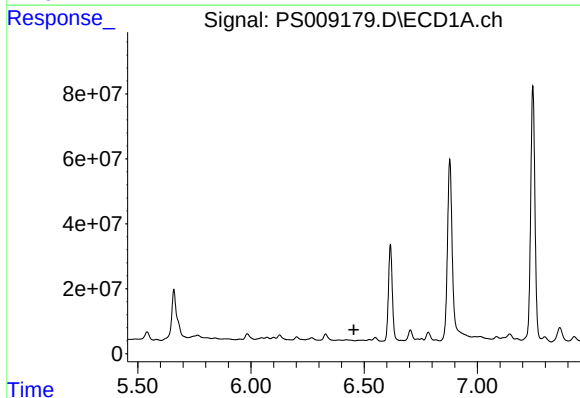


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.455 min
Response: 0
Conc: N.D.

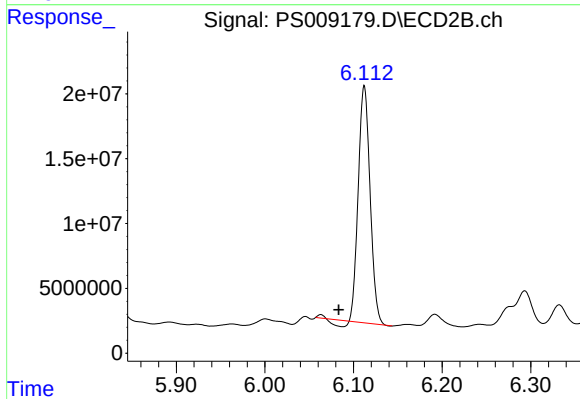

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.112 min
Delta R.T.: 0.029 min
Response: 167157299
Conc: 114.55 ng/ml

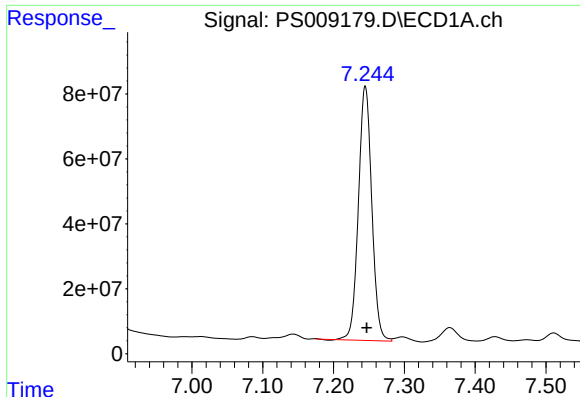

#4 2,4-DCAA


R.T.: 7.245 min
Delta R.T.: -0.002 min
Response: 1025371247
Conc: 468.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

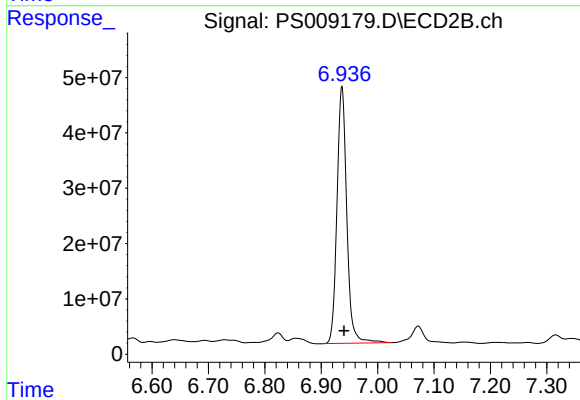


#4 2,4-DCAA

R.T.: 6.937 min
Delta R.T.: -0.004 min
Response: 561054098
Conc: 582.27 ng/ml

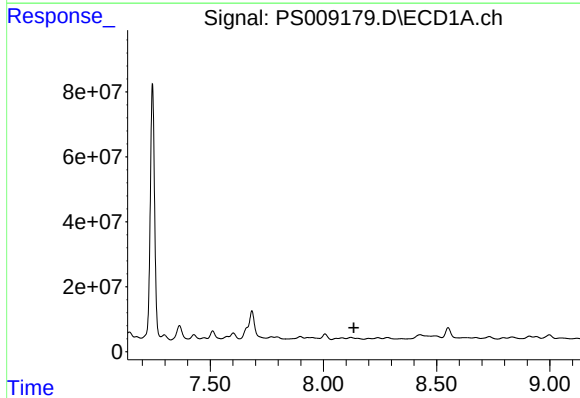


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.135 min
Response: 0
Conc: N.D.

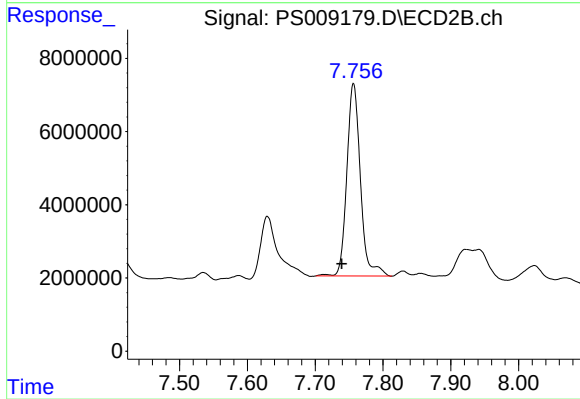

#8 DICHLORPROP


R.T.: 7.757 min
Delta R.T.: 0.018 min
Response: 73275972
Conc: 73.13 ng/ml

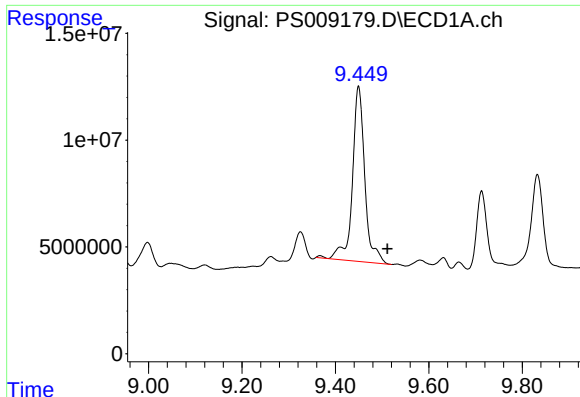

#12 2,4,5-T


R.T.: 9.450 min
Delta R.T.: -0.062 min
Response: 150994370
Conc: 14.12 ng/ml

Instrument :
ECD_S
ClientSampleId :

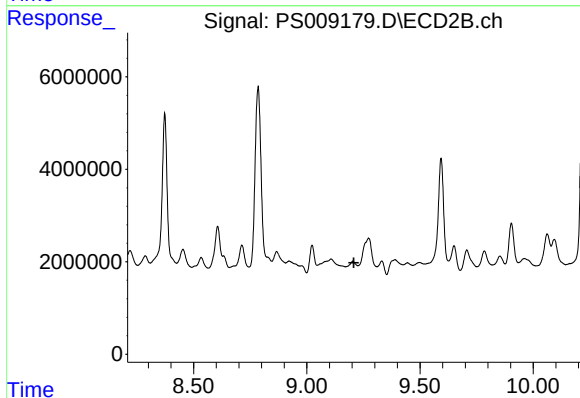


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.208 min
Response: 0
Conc: N.D.

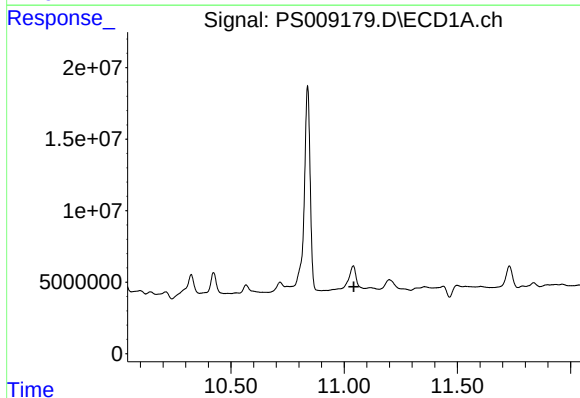


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.043 min
Response: 0
Conc: N.D.

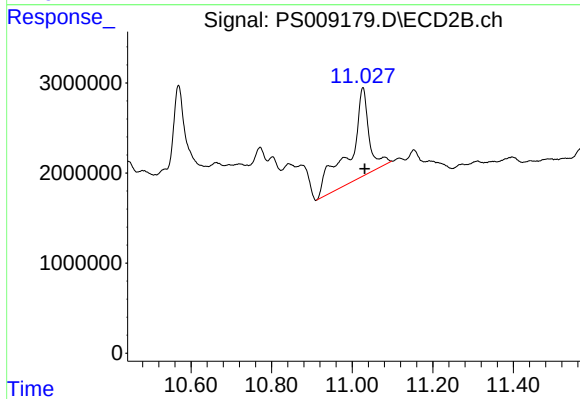

#15 Picloram


R.T.: 11.026 min
Delta R.T.: -0.005 min
Response: 33091178
Conc: 4.55 ng/ml

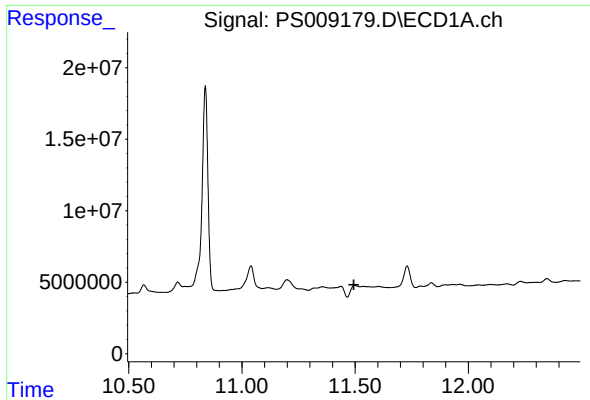

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.495 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

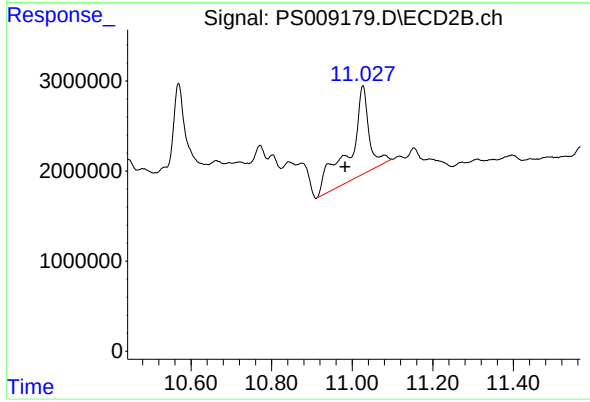

#16 DCPA

R.T.: 11.026 min
Delta R.T.: 0.044 min
Response: 33091178
Conc: 4.78 ng/ml