

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030723\
 Data File : PS022317.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Mar 2023 08:40
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 11:08:47 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022023.M
 Quant Title : 8080.M
 QLast Update : Mon Feb 20 13:26:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.304	0.000	479406	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	2.416	0.000	1837671	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.714	0.000	697087	0	<MDL	N.D. #
3) T	4-Nitroph...	6.145	0.000	2314608	0	1.819	N.D. #
5) T	DICAMBA	6.453	0.000	174585	0	<MDL	N.D. #
8) T	DICHLORPROP	7.047	0.000	294407	0	<MDL	N.D. #
9) T	2,4-D	7.229	0.000	2359369	0	<MDL	N.D. #
10) T	Pentachlo...	7.449	0.000	372074	0	<MDL	N.D. #
11) T	2,4,5-TP ...	7.929	8.575	163806	7800301	<MDL	<MDL #
12) T	2,4,5-T	8.223	8.940	4003476	7191479	<MDL	<MDL #
13) T	2,4-DB	8.752	0.000	2707761	0	<MDL	N.D. #
14) T	DINOSEB	9.827f	0.000	1359593	0	<MDL	N.D. #
15) T	Picloram	9.571f	10.703f	6289214	27389324	<MDL	1.397 #
16) T	DCPA	10.055	10.703	21660	27389324	<MDL	1.751 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030723\
Data File : PS022317.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Mar 2023 08:40
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 11:08:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022023.M
Quant Title : 8080.M
QLast Update : Mon Feb 20 13:26:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

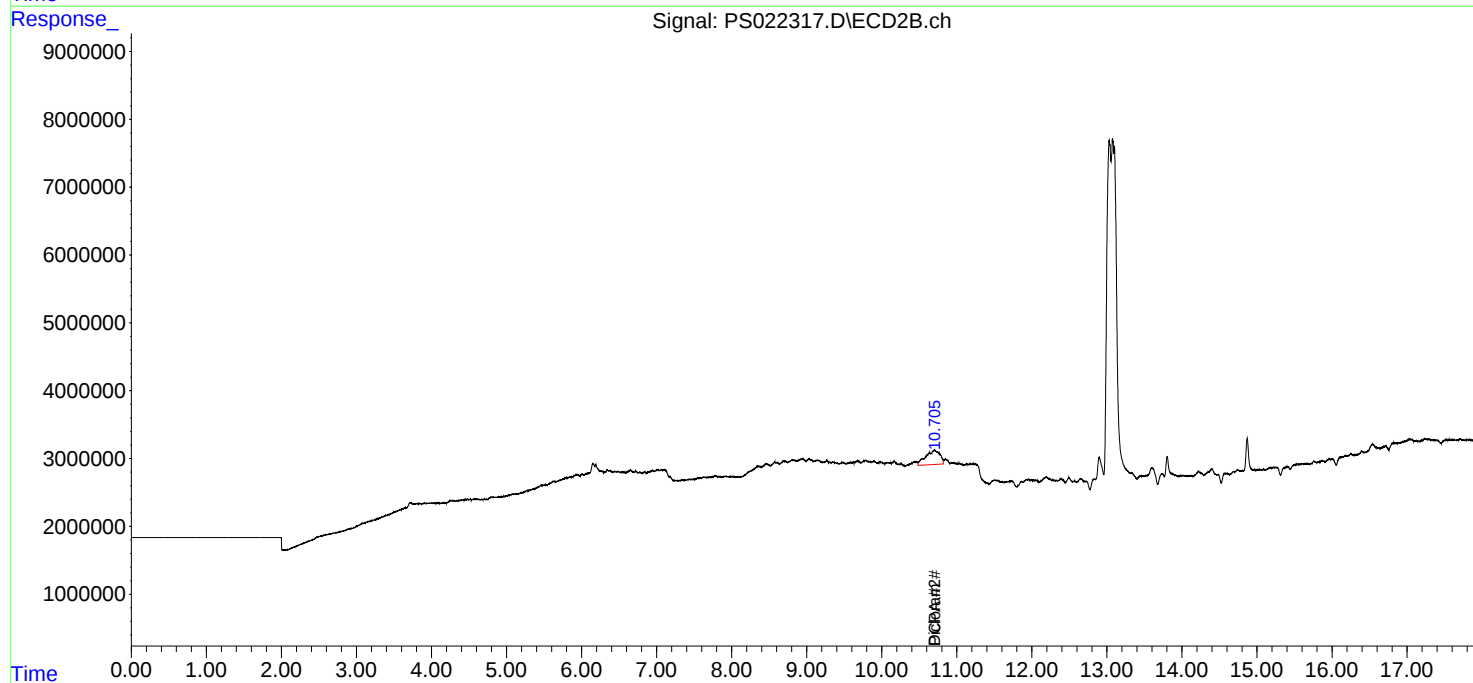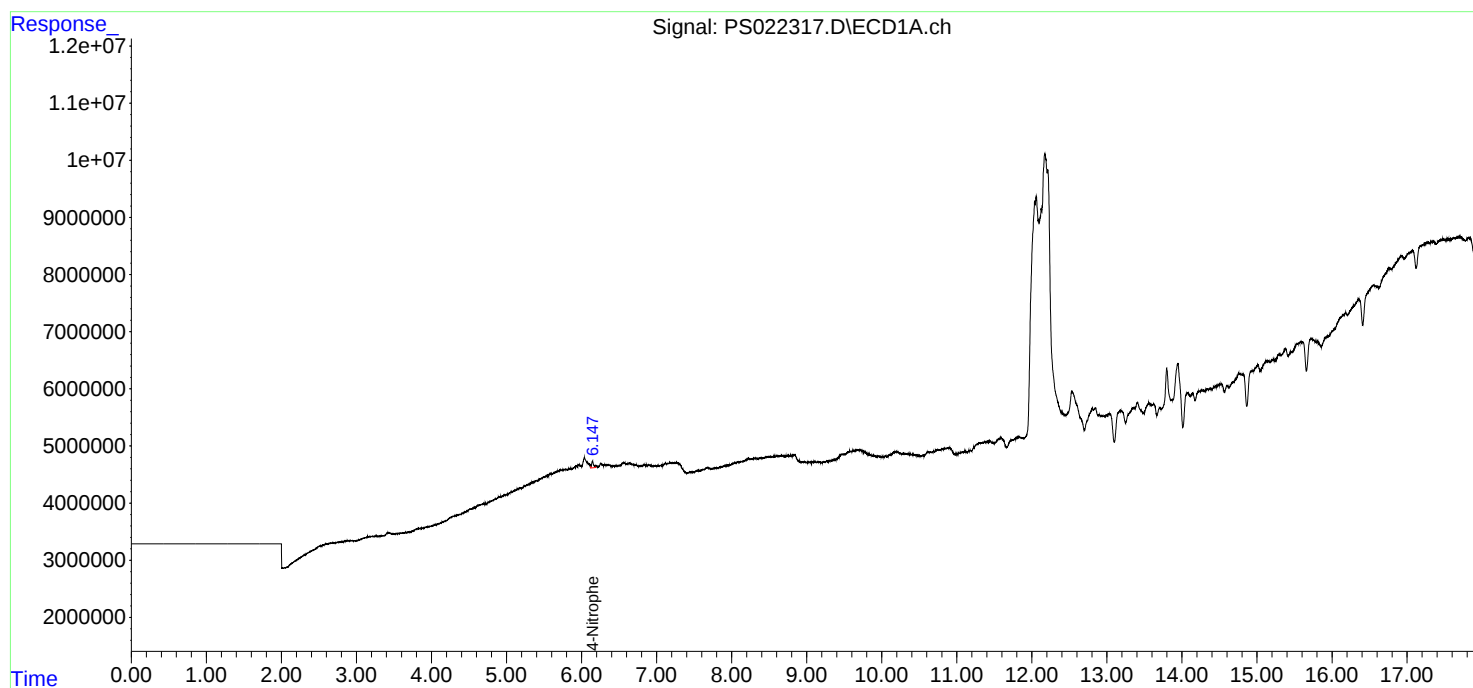


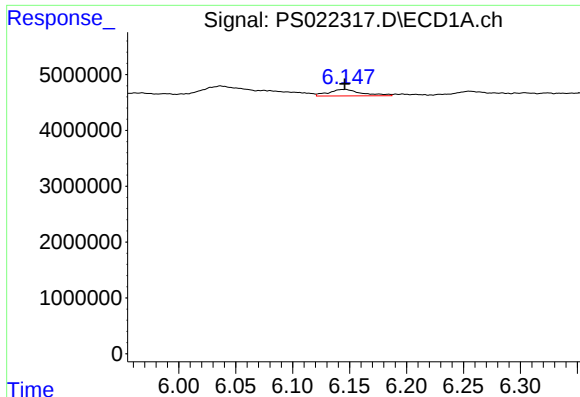

#3 4-Nitrophenol


R.T.: 6.145 min
Delta R.T.: -0.001 min
Response: 2314608
Conc: 1.82 ng/ml

Instrument :
ECD_S
ClientSampleId :

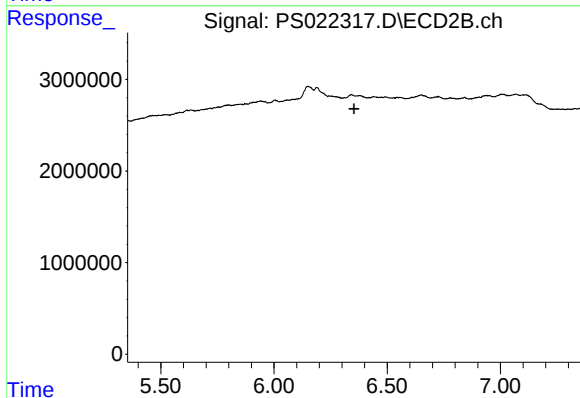


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.353 min
Response: 0
Conc: N.D.

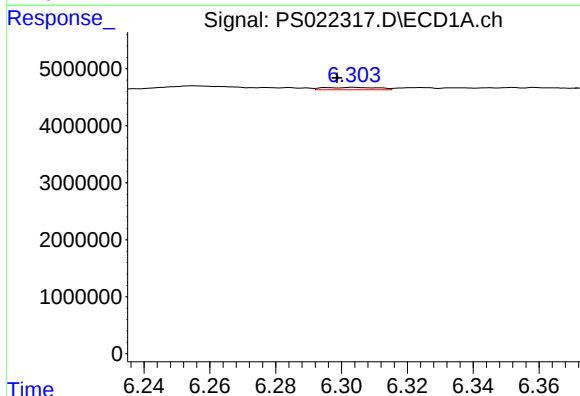


#4 2,4-DCAA

R.T.: 6.304 min
Delta R.T.: 0.005 min
Response: 479406
Conc: N.D.

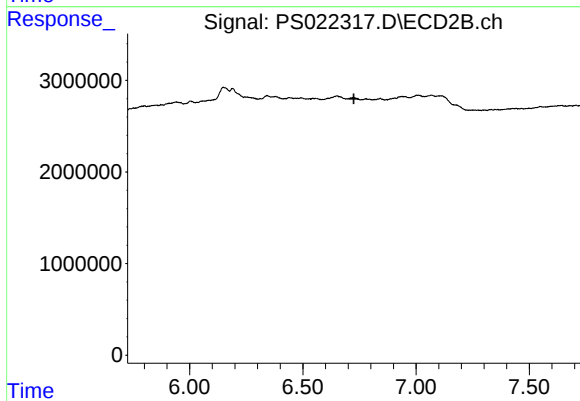

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.726 min
Response: 0
Conc: N.D.

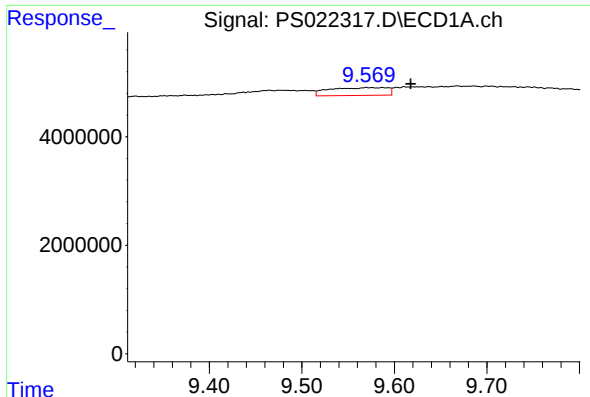

#15 Picloram


R.T.: 9.571 min
Delta R.T.: -0.046 min
Response: 6289214
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

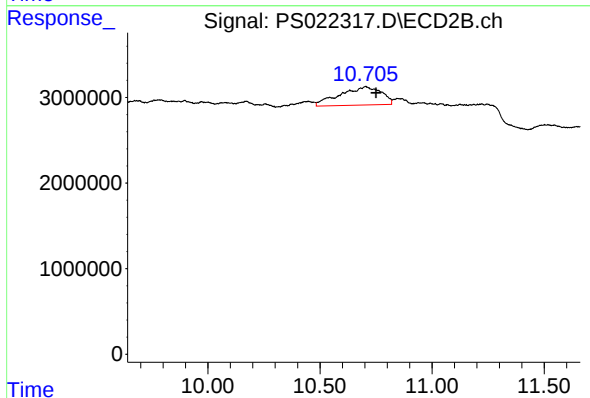


#15 Picloram

R.T.: 10.703 min
Delta R.T.: -0.047 min
Response: 27389324
Conc: 1.40 ng/ml

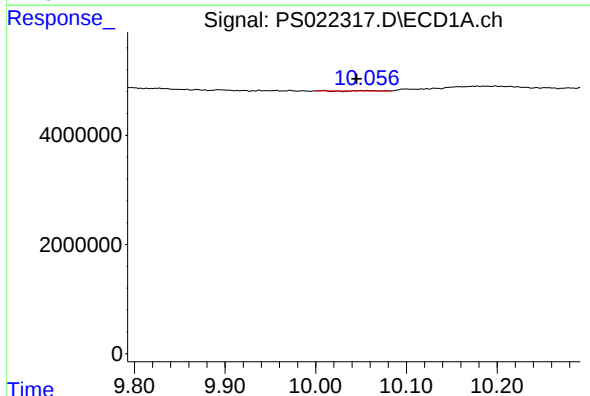

#16 DCPA

R.T.: 10.055 min
Delta R.T.: 0.010 min
Response: 21660
Conc: N.D.

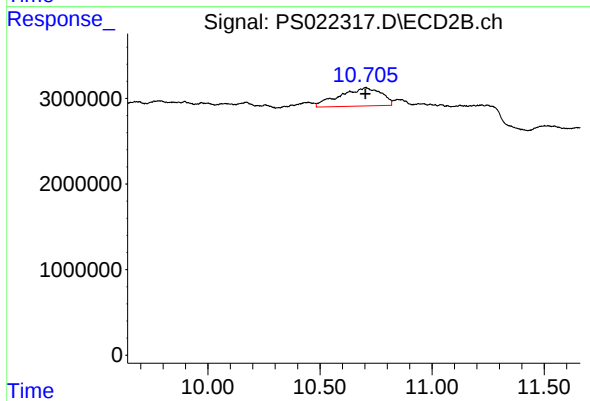

#16 DCPA

R.T.: 10.703 min
Delta R.T.: 0.000 min
Response: 27389324
Conc: 1.75 ng/ml