

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030723\
 Data File : PS022318.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Mar 2023 09:04
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 11:09:02 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022023.M
 Quant Title : 8080.M
 QLast Update : Mon Feb 20 13:26:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.303	6.724	1233.4E6	1150.2E6	497.606	547.985
Target Compounds							
1) T	Dalapon	2.389	0.000	568858	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.675	0.000	1044372	0	<MDL	N.D. #
3) T	4-Nitroph...	6.165	6.364	5430145	1250384	4.267	<MDL #
6) T	MCP	0.000	7.005	0	1658726	N.D.	<MDL
7) T	MCPA	0.000	7.133f	0	4930280	N.D.	<MDL
8) T	DICHLORPROP	7.075f	0.000	683048	0	<MDL	N.D. #
9) T	2,4-D	7.276f	0.000	8541817	0	2.605	N.D. #
10) T	Pentachlo...	7.456	8.216	9211361	6752278	<MDL	<MDL #
11) T	2,4,5-TP ...	7.941	8.596	539824	2363371	<MDL	<MDL #
13) T	2,4-DB	8.747	0.000	185466	0	<MDL	N.D. #
14) T	DINOSEB	9.784	9.784	4571497	2514323	<MDL	<MDL #
15) T	Picloram	9.643	10.703f	8676979	4943546	<MDL	<MDL #
16) T	DCPA	10.050	10.703	6120375	4943546	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030723\
Data File : PS022318.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Mar 2023 09:04
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 11:09:02 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022023.M
Quant Title : 8080.M
QLast Update : Mon Feb 20 13:26:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

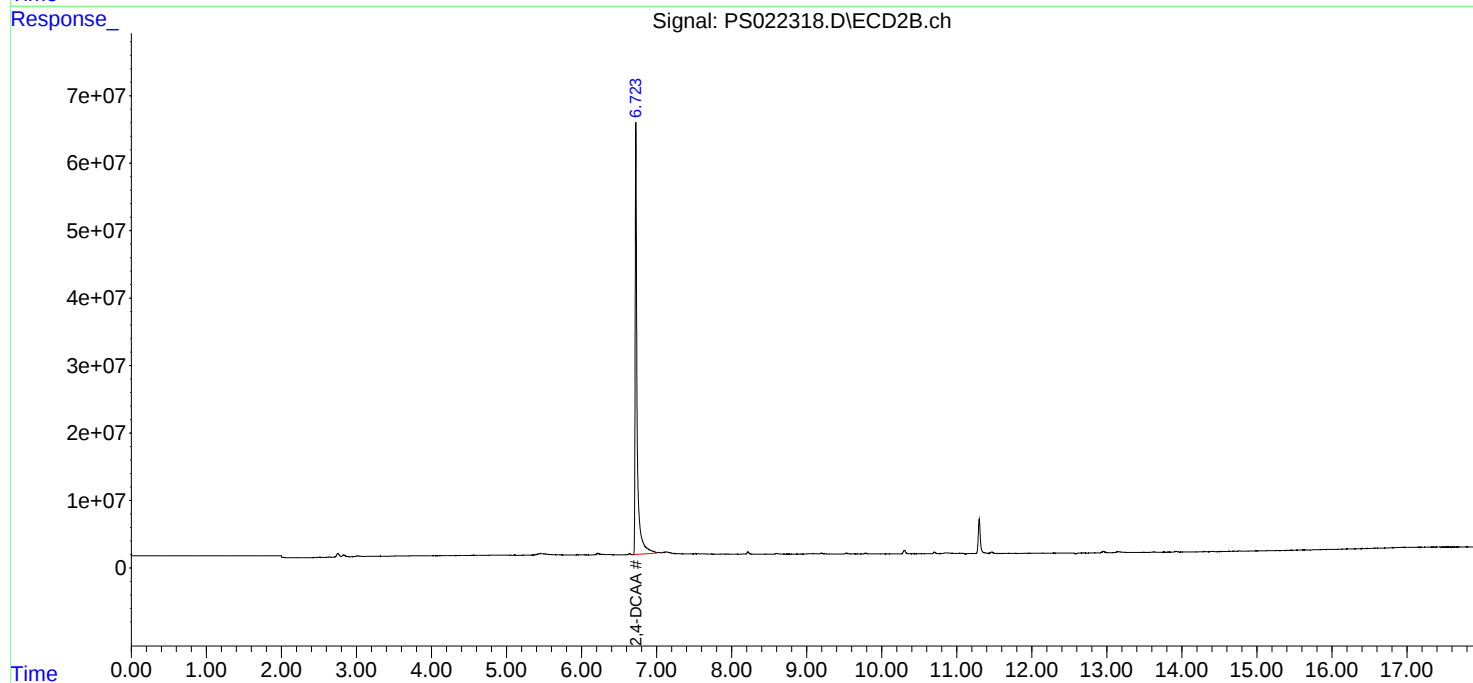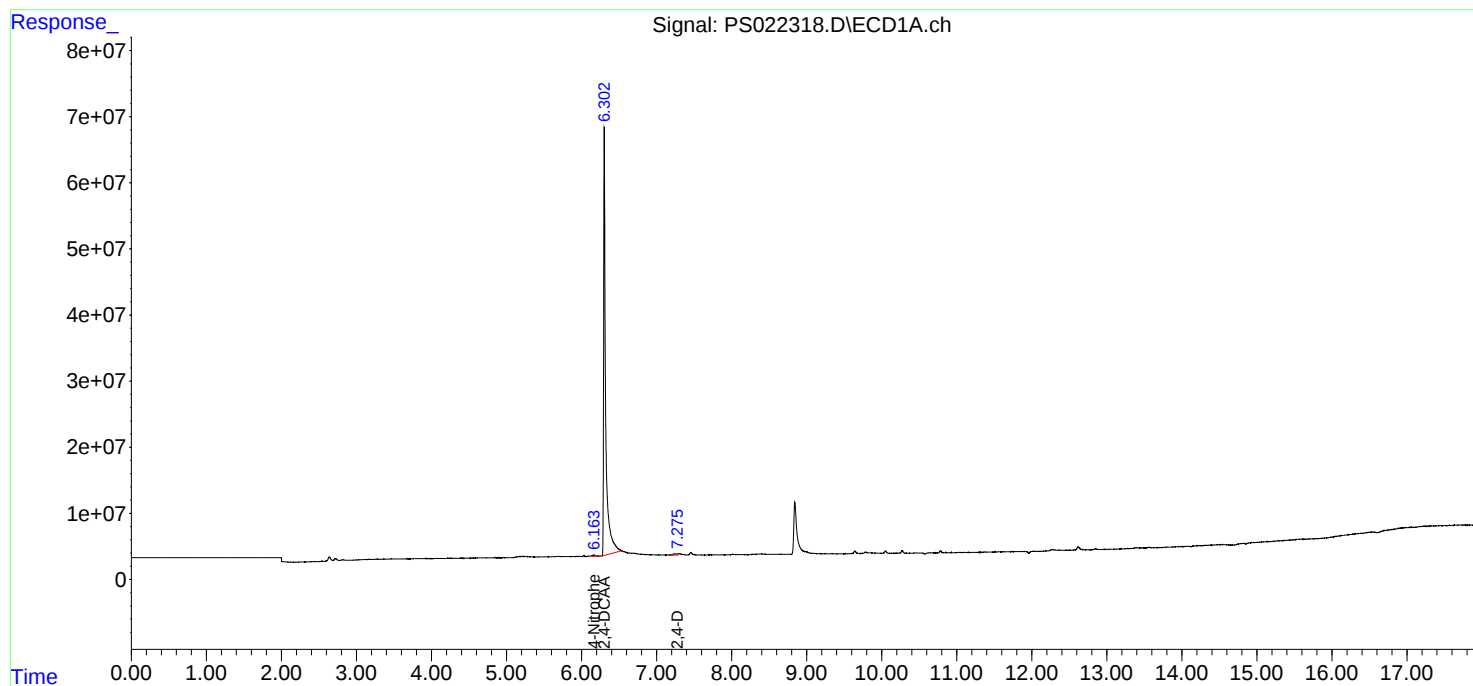


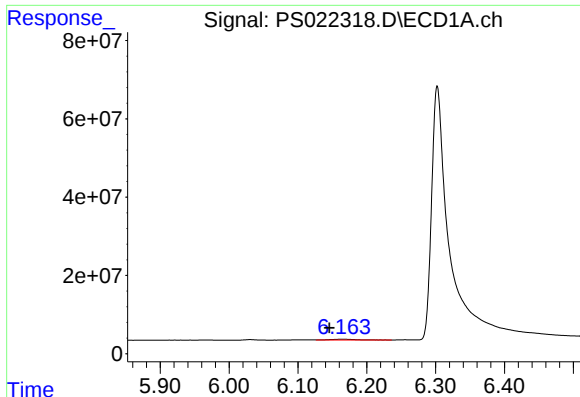

#3 4-Nitrophenol


R.T.: 6.165 min
Delta R.T.: 0.019 min
Response: 5430145
Conc: 4.27 ng/ml

Instrument :
ECD_S
ClientSampleId :

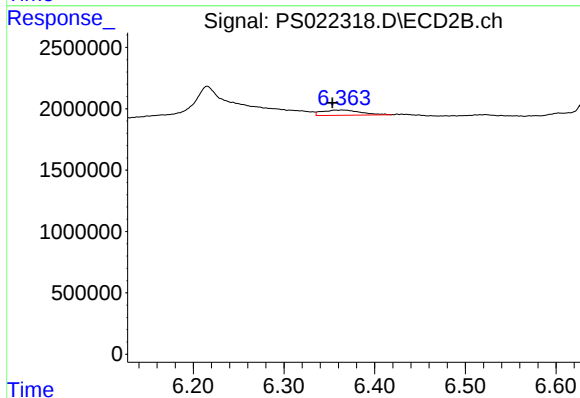


#3 4-Nitrophenol

R.T.: 6.364 min
Delta R.T.: 0.011 min
Response: 1250384
Conc: N.D.

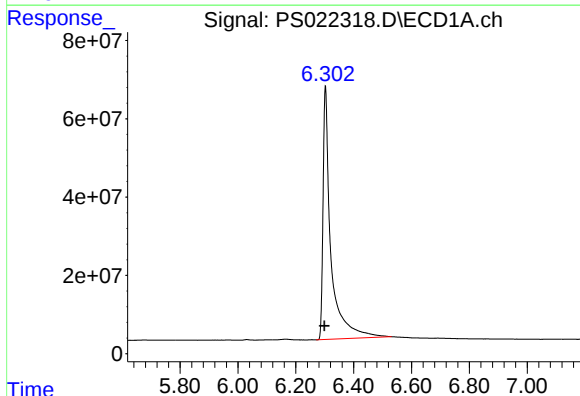


#4 2,4-DCAA

R.T.: 6.303 min
Delta R.T.: 0.004 min
Response: 1233411768
Conc: 497.61 ng/ml

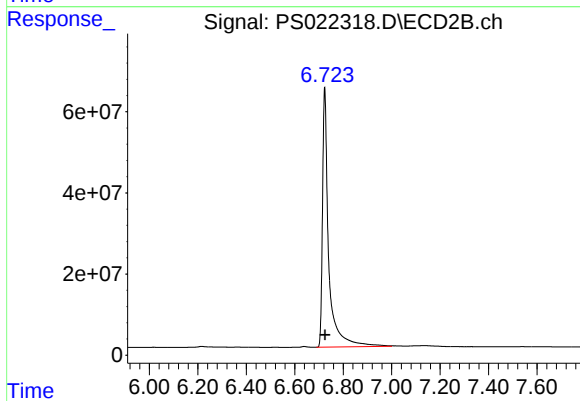

#4 2,4-DCAA


R.T.: 6.724 min
Delta R.T.: -0.002 min
Response: 1150201112
Conc: 547.99 ng/ml

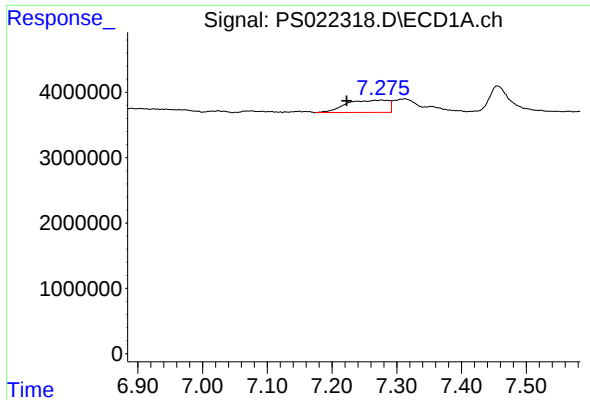

#9 2,4-D

R.T.: 7.276 min
Delta R.T.: 0.053 min
Response: 8541817
Conc: 2.61 ng/ml

Instrument :
ECD_S
ClientSampleId :

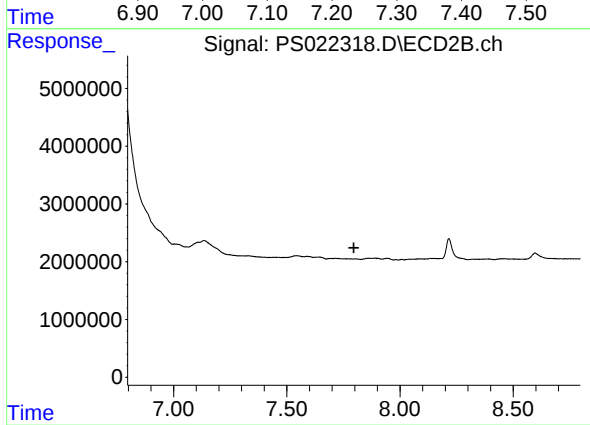

#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.796 min
Response: 0
Conc: N.D.