

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030723\
 Data File : PS022328.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Mar 2023 13:52
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 19:35:55 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022023.M
 Quant Title : 8080.M
 QLast Update : Mon Feb 20 13:26:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.299	6.722	1288.1E6	1191.2E6	519.675	567.538
Target Compounds							
1) T	Dalapon	2.445	0.000	1149187	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.670	0.000	814273	0	<MDL	N.D. #
3) T	4-Nitroph...	6.155	6.352	5667716	1321457	4.454	<MDL #
6) T	MCP	0.000	7.021	0	5682638	N.D.	<MDL
7) T	MCPA	0.000	7.126f	0	31688962	N.D.	3.109
9) T	2,4-D	7.220	0.000	4595354	0	1.402	N.D. #
10) T	Pentachlo...	7.448	8.212	9598563	7250241	<MDL	<MDL #
11) T	2,4,5-TP ...	7.987	8.583	2638747	3443655	<MDL	<MDL #
12) T	2,4,5-T	8.239	8.996f	3330137	2492174	<MDL	<MDL #
13) T	2,4-DB	8.740	0.000	353997	0	<MDL	N.D. #
14) T	DINOSEB	9.778	9.780	15345661	2261690	1.117	<MDL #
15) T	Picloram	9.640	10.701f	4635875	37674717	<MDL	1.922 #
16) T	DCPA	10.044	10.701	7423862	37674717	<MDL	2.408 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030723\
Data File : PS022328.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Mar 2023 13:52
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 19:35:55 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022023.M
Quant Title : 8080.M
QLast Update : Mon Feb 20 13:26:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

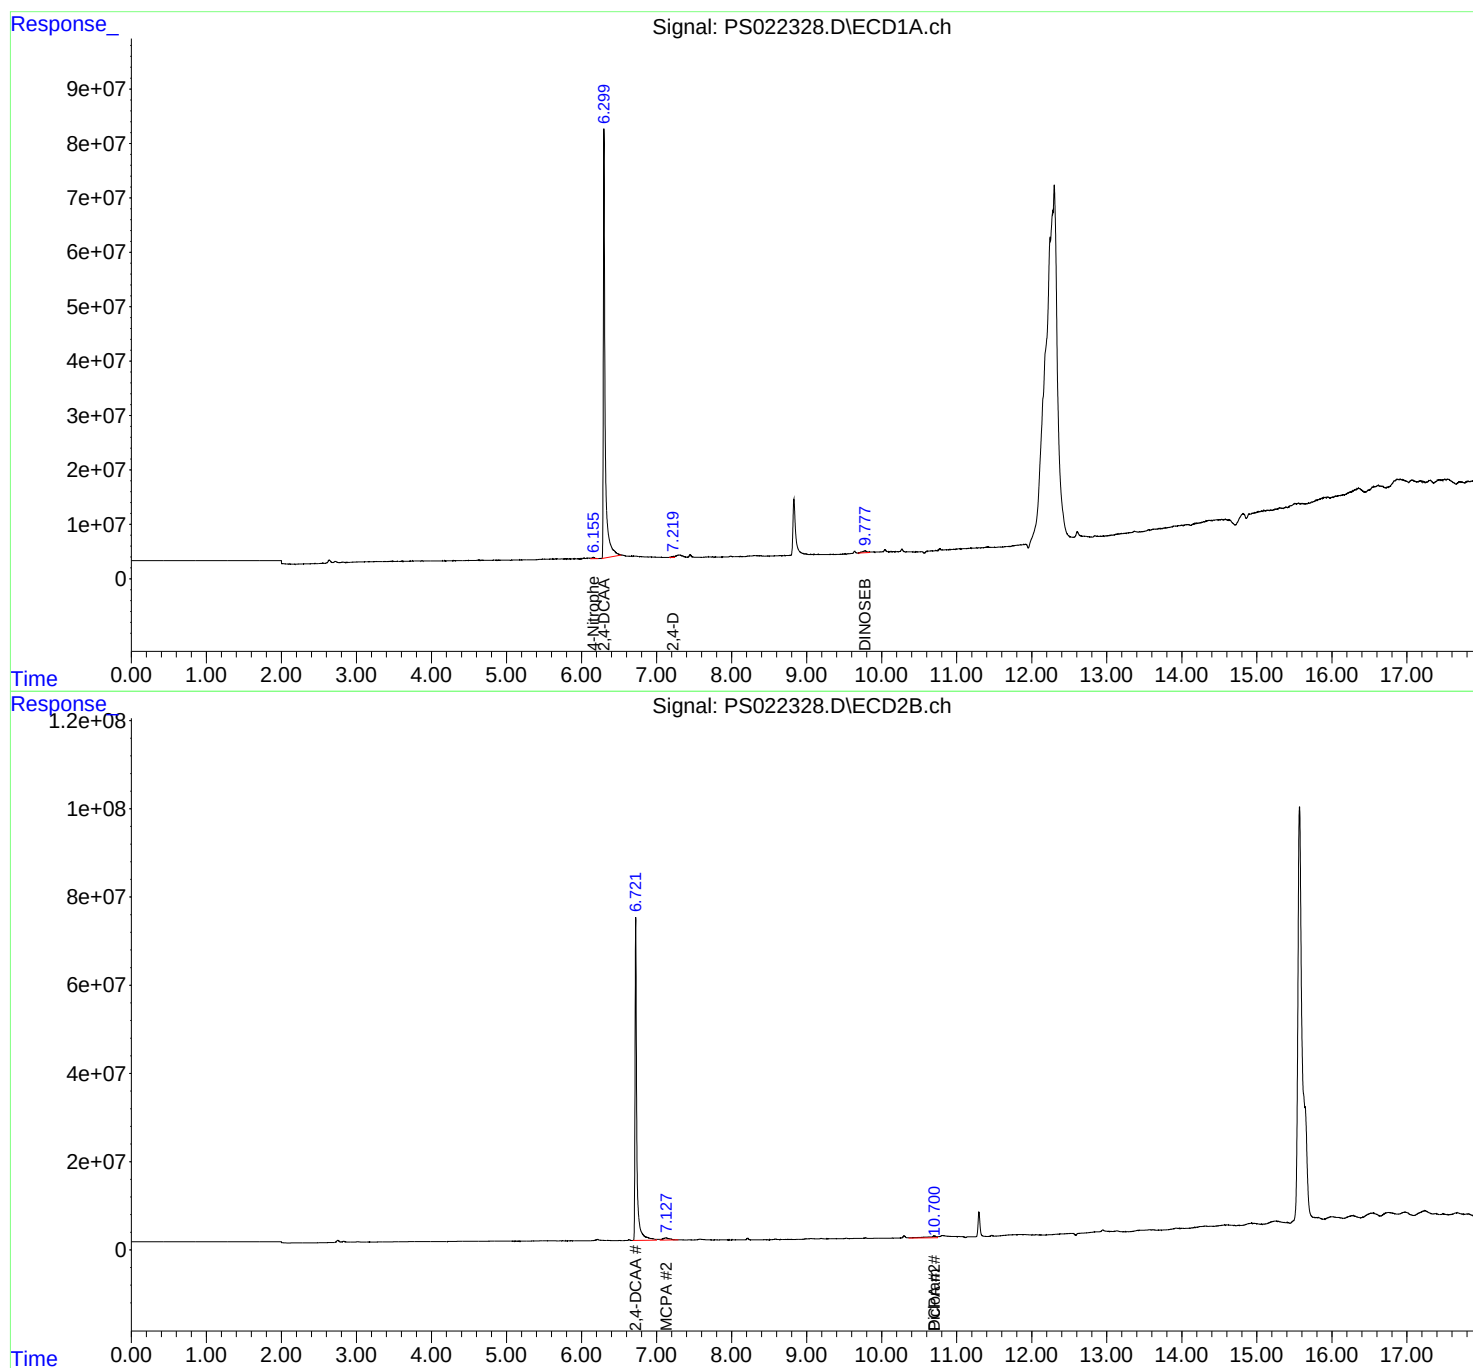


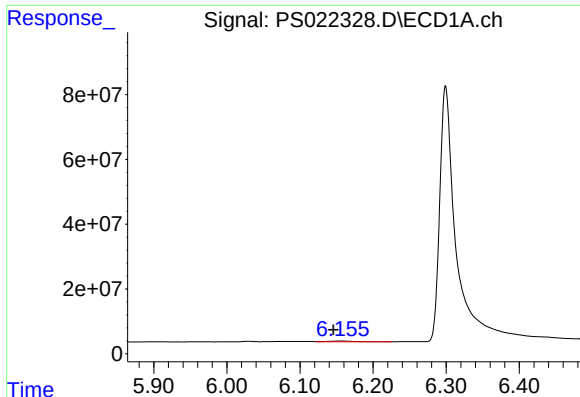

#3 4-Nitrophenol


R.T.: 6.155 min
Delta R.T.: 0.009 min
Response: 5667716
Conc: 4.45 ng/ml

Instrument :
ECD_S
ClientSampleId :

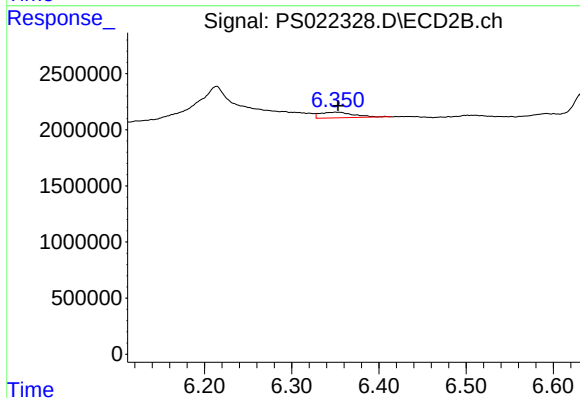


#3 4-Nitrophenol

R.T.: 6.352 min
Delta R.T.: -0.001 min
Response: 1321457
Conc: N.D.

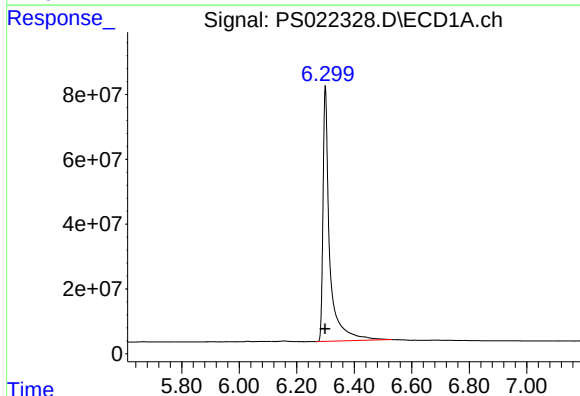


#4 2,4-DCAA

R.T.: 6.299 min
Delta R.T.: 0.000 min
Response: 1288114235
Conc: 519.68 ng/ml

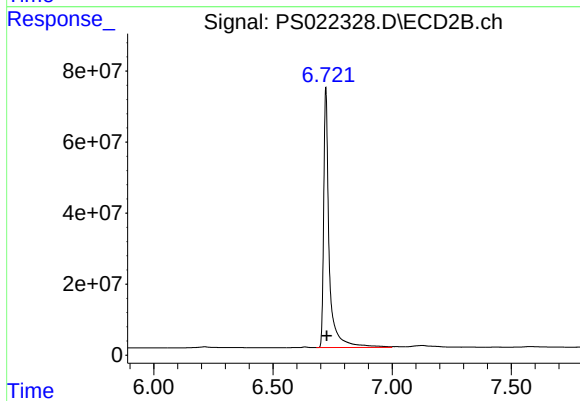

#4 2,4-DCAA


R.T.: 6.722 min
Delta R.T.: -0.004 min
Response: 1191240454
Conc: 567.54 ng/ml

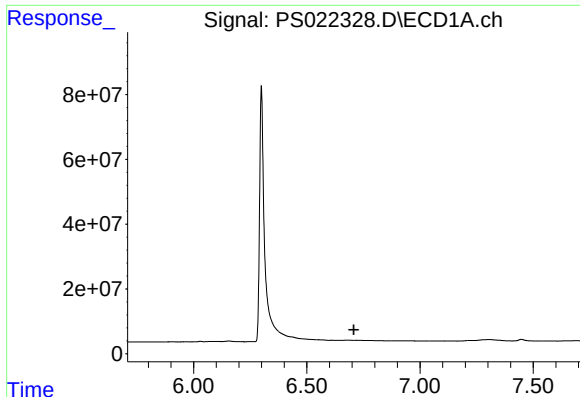

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.708 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

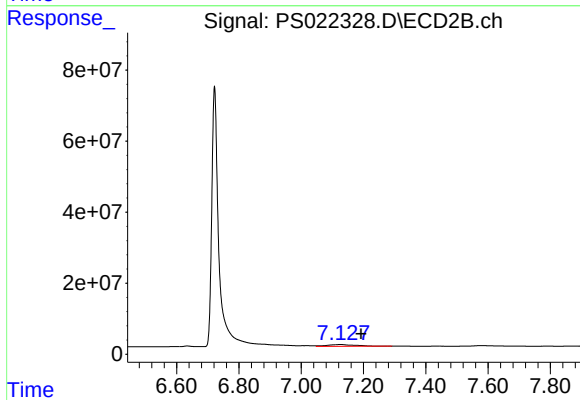


#7 MCPA

R.T.: 7.126 min
Delta R.T.: -0.066 min
Response: 31688962
Conc: 3.11 ug/ml

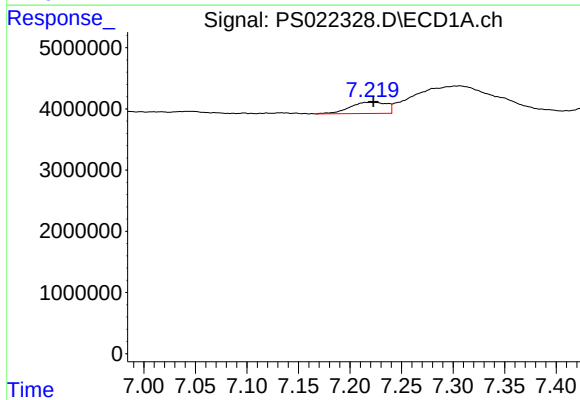


#9 2,4-D

R.T.: 7.220 min
Delta R.T.: -0.003 min
Response: 4595354
Conc: 1.40 ng/ml

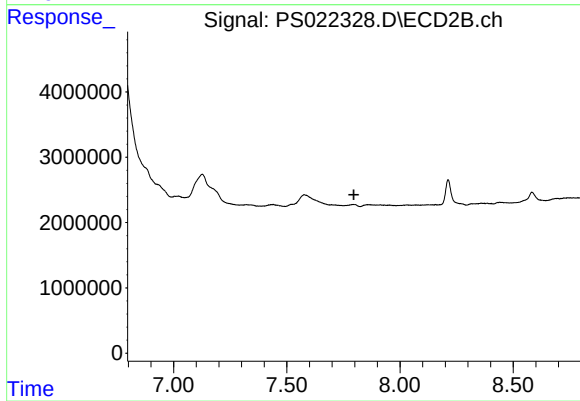

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.796 min
Response: 0
Conc: N.D.

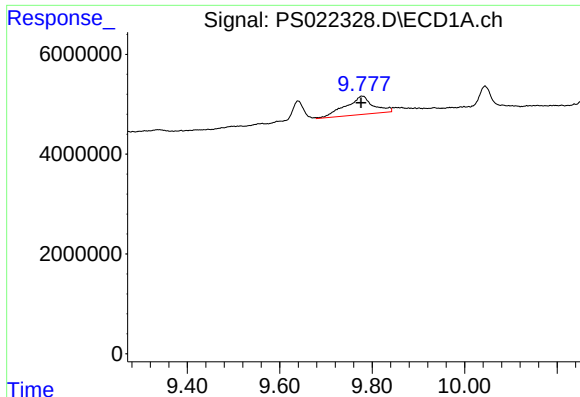

#14 DINoseb


R.T.: 9.778 min
Delta R.T.: 0.002 min
Response: 15345661
Conc: 1.12 ng/ml

Instrument :
ECD_S
ClientSampleId :

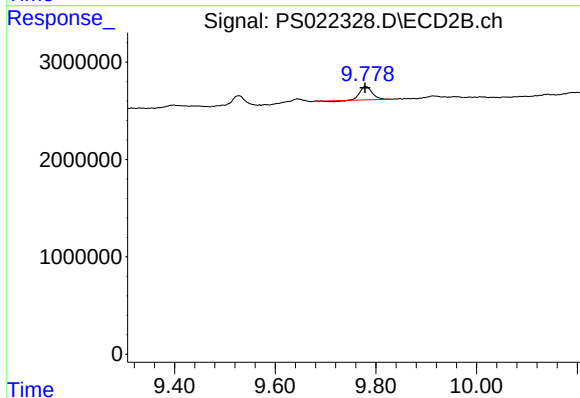


#14 DINoseb

R.T.: 9.780 min
Delta R.T.: 0.000 min
Response: 2261690
Conc: N.D.

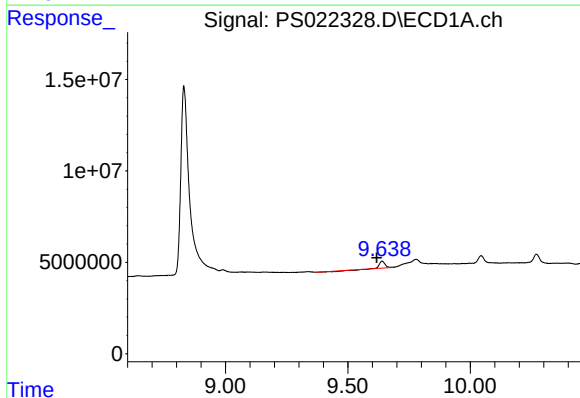


#15 Picloram

R.T.: 9.640 min
Delta R.T.: 0.022 min
Response: 4635875
Conc: N.D.

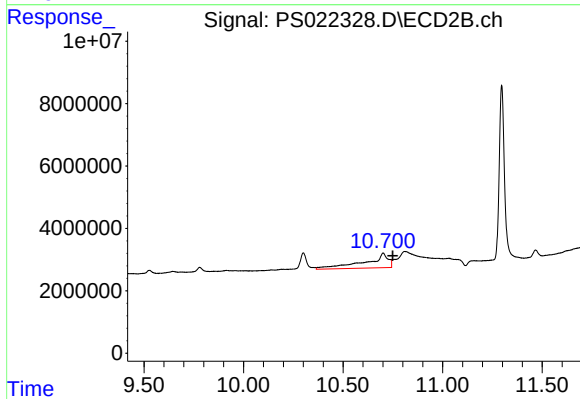

#15 Picloram


R.T.: 10.701 min
Delta R.T.: -0.049 min
Response: 37674717
Conc: 1.92 ng/ml

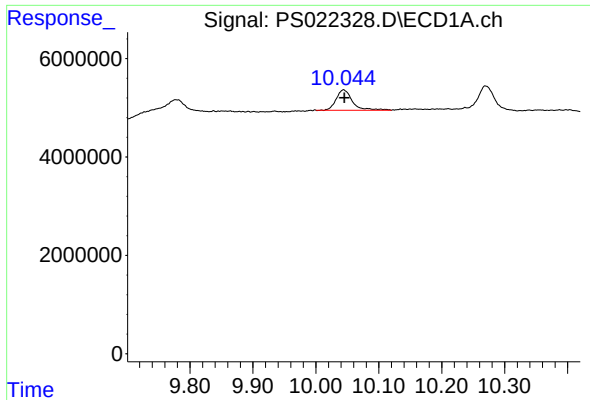

#16 DCPA

R.T.: 10.044 min
Delta R.T.: -0.001 min
Response: 7423862
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

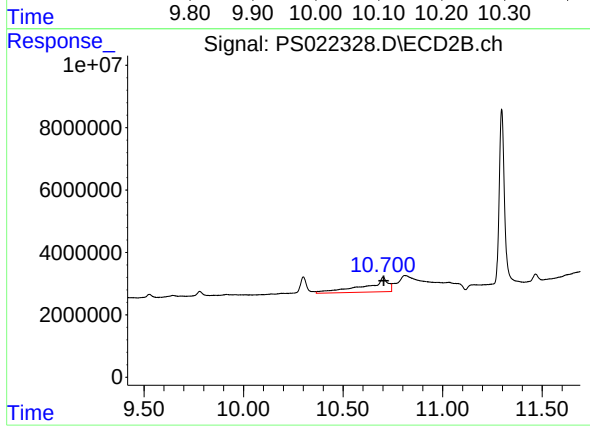

#16 DCPA

R.T.: 10.701 min
Delta R.T.: -0.002 min
Response: 37674717
Conc: 2.41 ng/ml