

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030819\
 Data File : PS003464.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Mar 2019 11:45
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 08 21:59:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.287	10.786	214.0E6	203.4E6	487.391	433.233
Target Compounds							
3) T	4-Nitroph...	0.000	9.957	0	176024	N.D.	0.783 #
8) T	DICHLORPROP	0.000	12.202	0	75787	N.D.	0.183 #
9) T	2,4-D	0.000	12.687	0	190210	N.D.	0.362 #
10) T	Pentachlo...	0.000	13.203	0	570561	N.D.	0.087 #
11) T	2,4,5-TP ...	0.000	13.871	0	256899	N.D.	0.101 #
12) T	2,4,5-T	0.000	14.399	0	70468	N.D.	0.035 #
14) T	DINOSEB	0.000	15.478	0	215537	N.D.	0.121 #
15) T	Picloram	0.000	16.641	0	730451	N.D.	0.288 #
16) T	DCPA	0.000	16.641	0	730451	N.D.	0.235 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030819\
Data File : PS003464.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Mar 2019 11:45
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 08 21:59:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

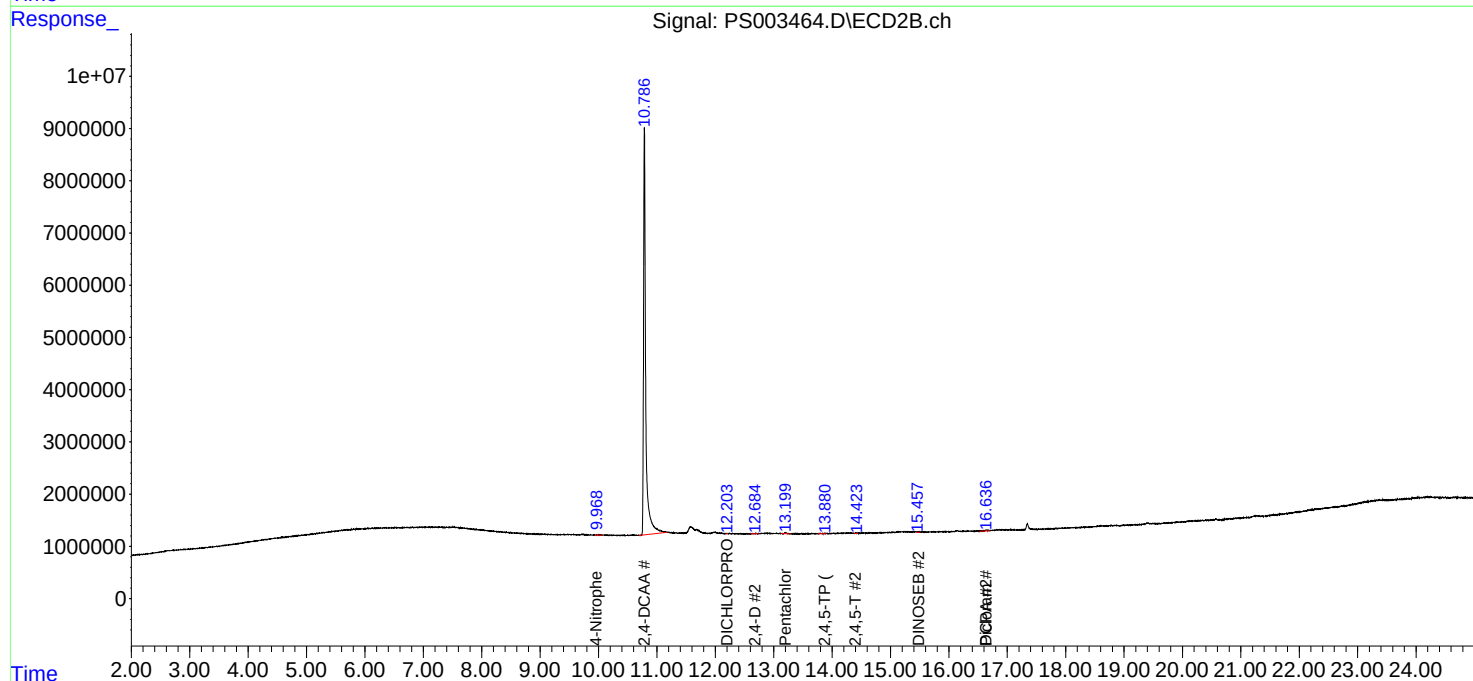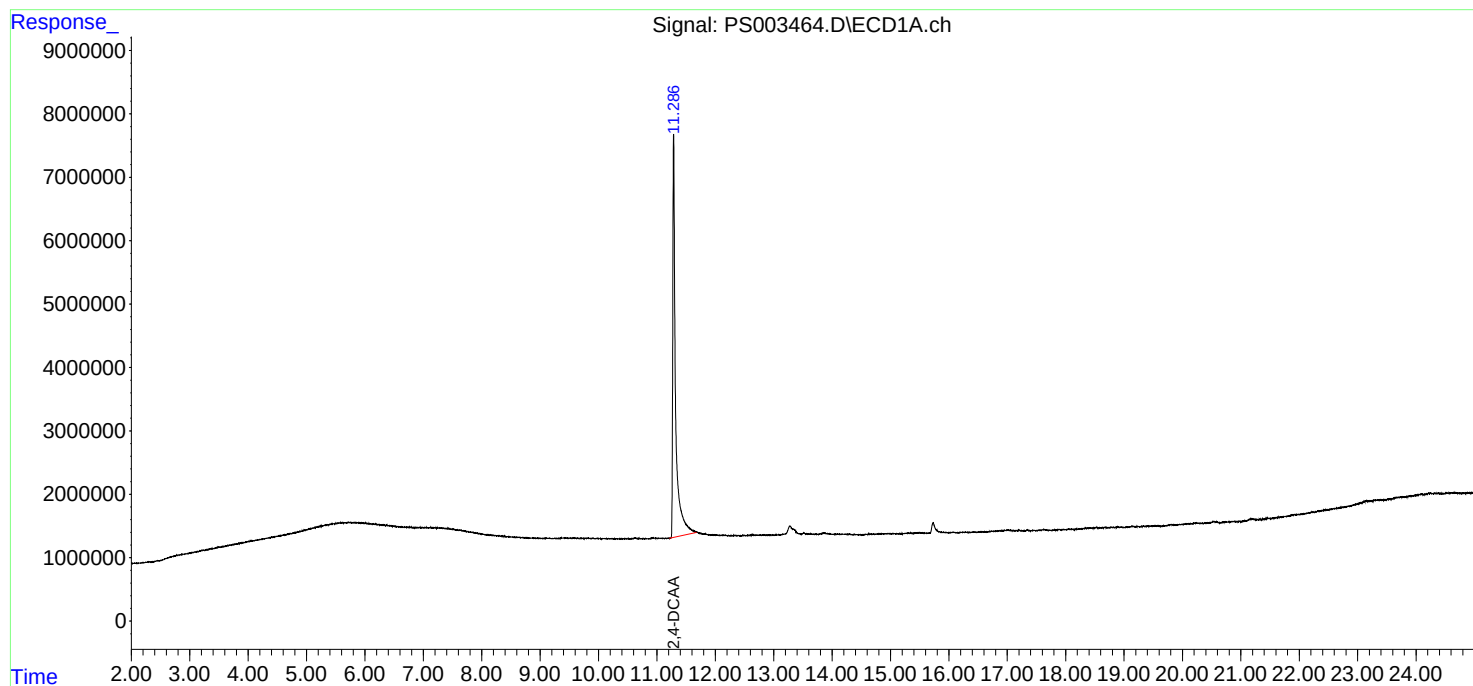


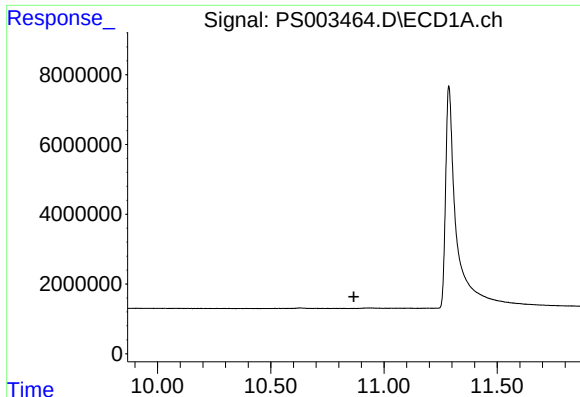

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

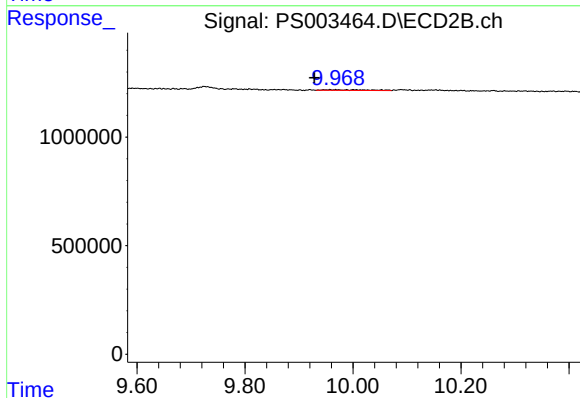


#3 4-Nitrophenol

R.T.: 9.957 min
Delta R.T.: 0.029 min
Response: 176024
Conc: 0.78 ng/ml

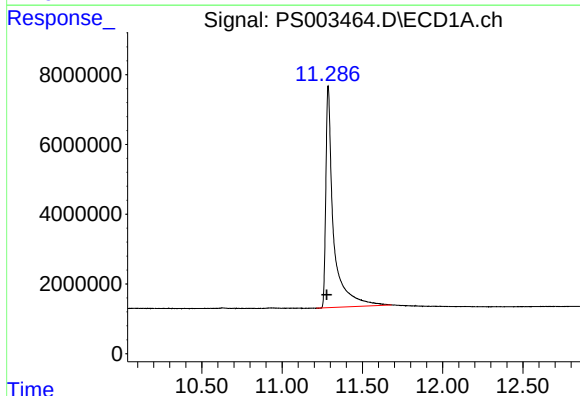


#4 2,4-DCAA

R.T.: 11.287 min
Delta R.T.: 0.009 min
Response: 213976386
Conc: 487.39 ng/ml

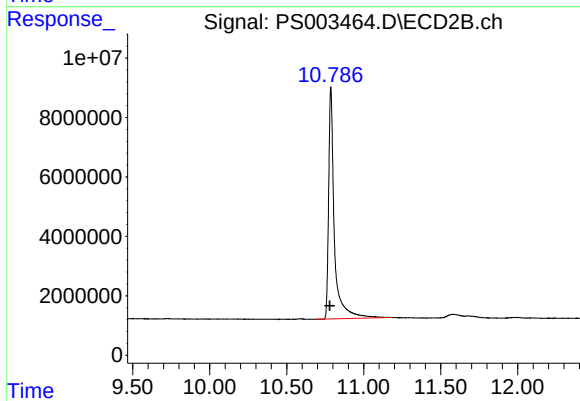

#4 2,4-DCAA


R.T.: 10.786 min
Delta R.T.: 0.007 min
Response: 203432786
Conc: 433.23 ng/ml

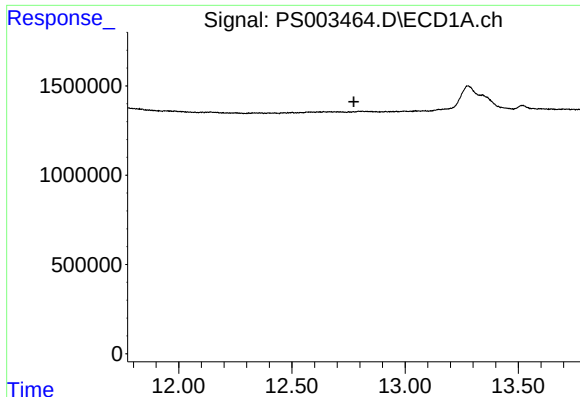

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 12.773 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

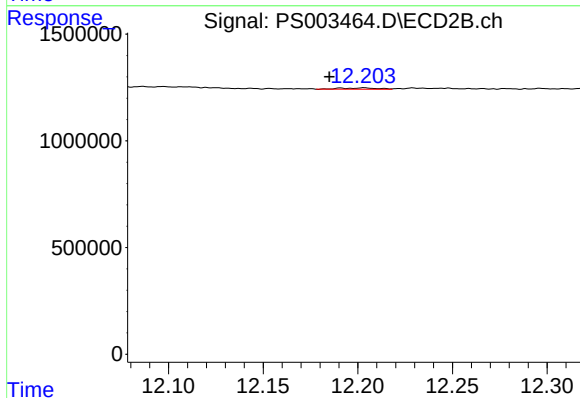


#8 DICHLORPROP

R.T.: 12.202 min
Delta R.T.: 0.017 min
Response: 75787
Conc: 0.18 ng/ml

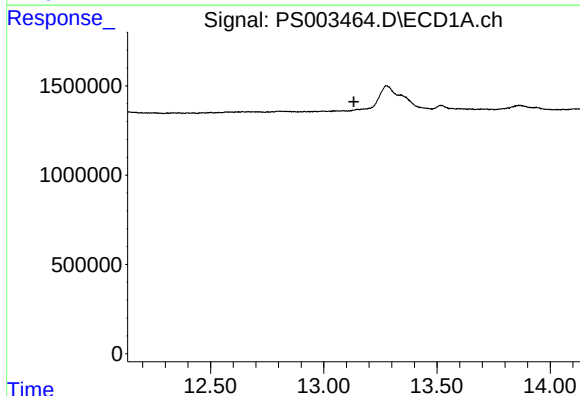


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.133 min
Response: 0
Conc: N.D.

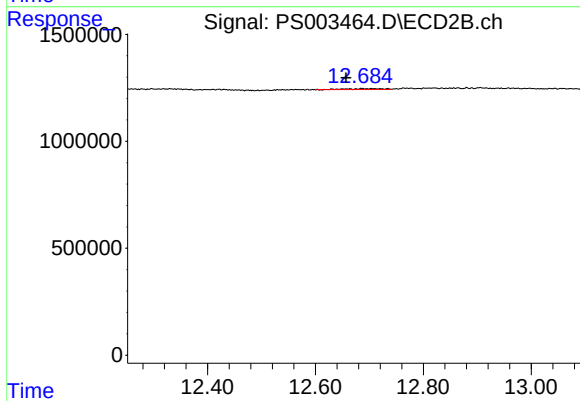

#9 2,4-D


R.T.: 12.687 min
Delta R.T.: 0.030 min
Response: 190210
Conc: 0.36 ng/ml

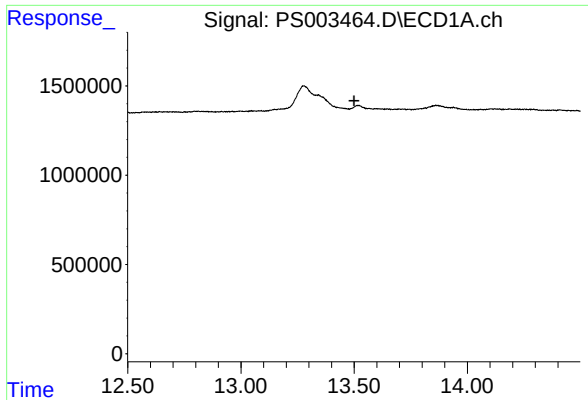

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.499 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

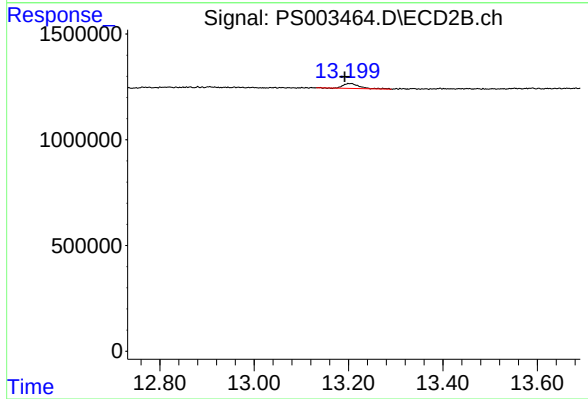


#10 Pentachlorophenol

R.T.: 13.203 min
Delta R.T.: 0.011 min
Response: 570561
Conc: 0.09 ng/ml

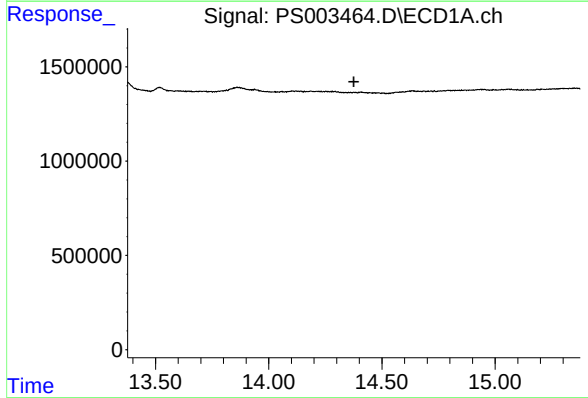


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

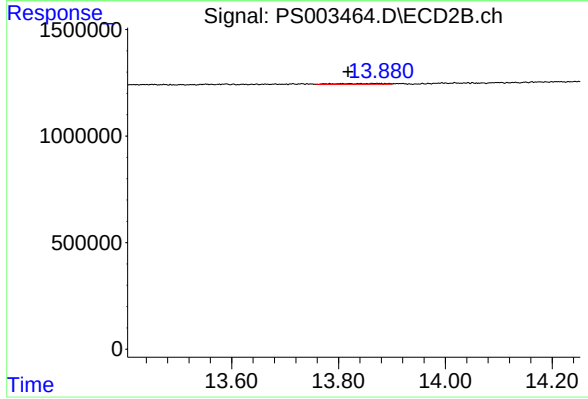

#11 2,4,5-TP (SILVEX)


R.T.: 13.871 min
Delta R.T.: 0.054 min
Response: 256899
Conc: 0.10 ng/ml

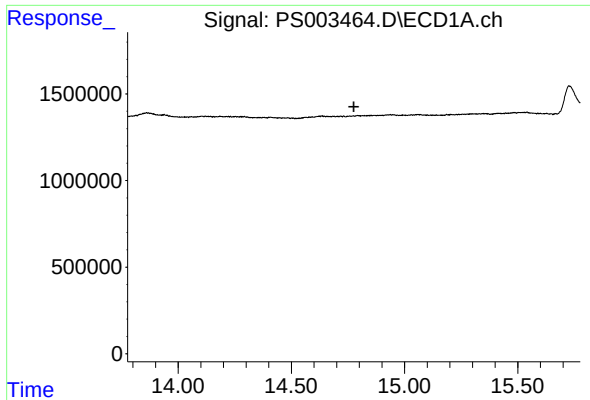

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 14.776 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

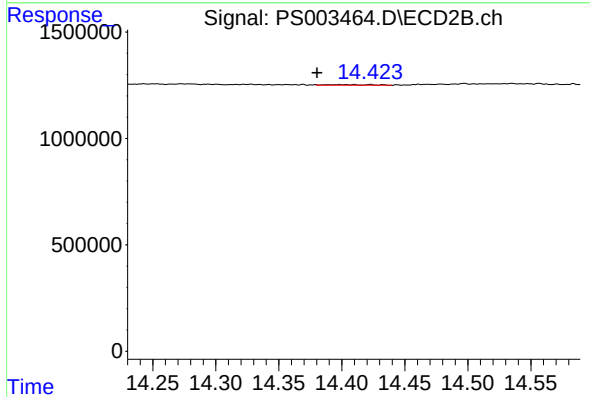


#12 2,4,5-T

R.T.: 14.399 min
Delta R.T.: 0.019 min
Response: 70468
Conc: 0.03 ng/ml

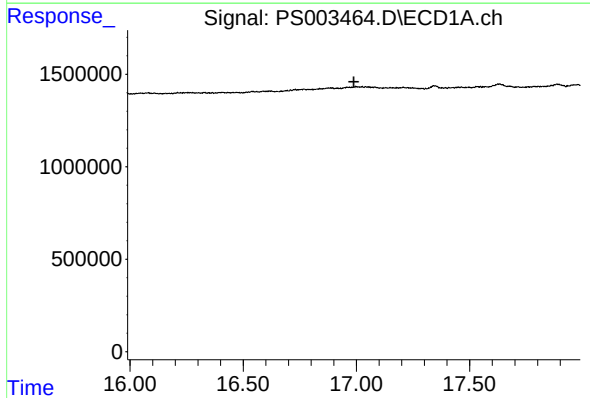


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 16.989 min
Response: 0
Conc: N.D.

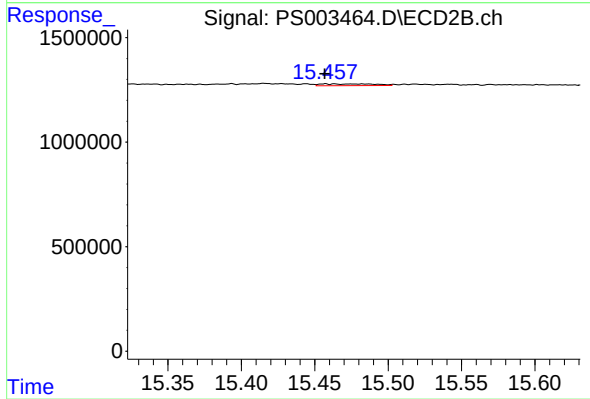

#14 DINOSEB


R.T.: 15.478 min
Delta R.T.: 0.022 min
Response: 215537
Conc: 0.12 ng/ml

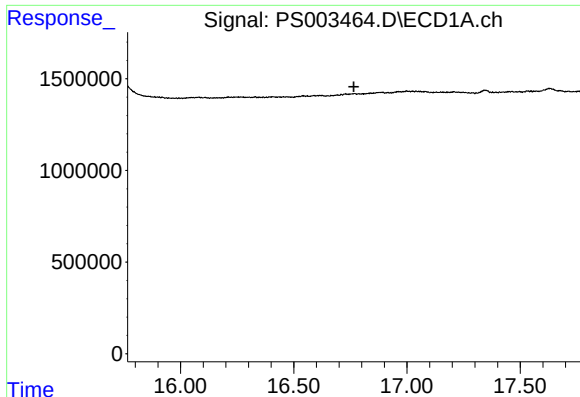

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.765 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

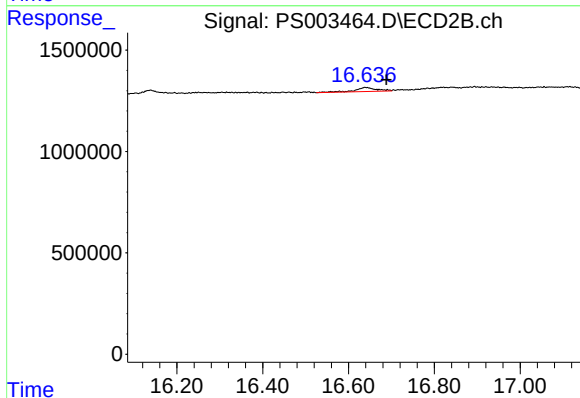


#15 Picloram

R.T.: 16.641 min
Delta R.T.: -0.048 min
Response: 730451
Conc: 0.29 ng/ml

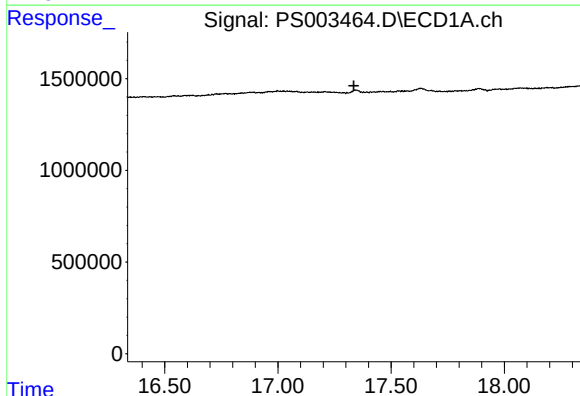

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.335 min
Response: 0
Conc: N.D.

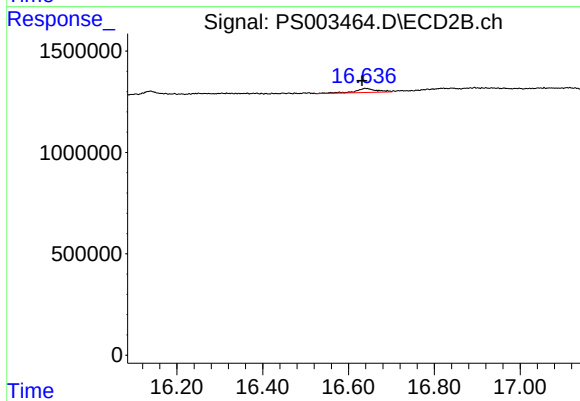

#16 DCPA

R.T.: 16.641 min
Delta R.T.: 0.009 min
Response: 730451
Conc: 0.23 ng/ml