

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030819\
 Data File : PS003470.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Mar 2019 15:41
 Operator : EI\SJ
 Sample : K1760-08
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 Z2-9

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 08 22:01:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.304	10.808	253.3E6	265.1E6	576.948	564.573
Target Compounds							
1) T	Dalapon	2.823	2.313	45412507	47278446	69.872	74.668
2) T	3,5-DICHL...	0.000	8.974	0	10042768	N.D.	16.265 #
5) T	DICAMBA	0.000	11.048	0	5747895	N.D.	3.440 #
6) T	MCP	0.000	11.304	0	392651	N.D.	0.333 #
8) T	DICHLORPROP	0.000	12.116	0	23122731	N.D.	55.954 #
11) T	2,4,5-TP ...	0.000	13.765	0	19437599	N.D.	7.633 #
12) T	2,4,5-T	0.000	14.410	0	8612937	N.D.	4.271 #
13) T	2,4-DB	15.492	14.973	8491870	8685955	35.862	34.015
15) T	Picloram	16.788	16.673	4409528	6207954	1.792	2.446 #
16) T	DCPA	0.000	16.673	0	6207954	N.D.	1.996 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030819\
Data File : PS003470.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Mar 2019 15:41
Operator : EI\SJ
Sample : K1760-08
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
Z2-9

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 08 22:01:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

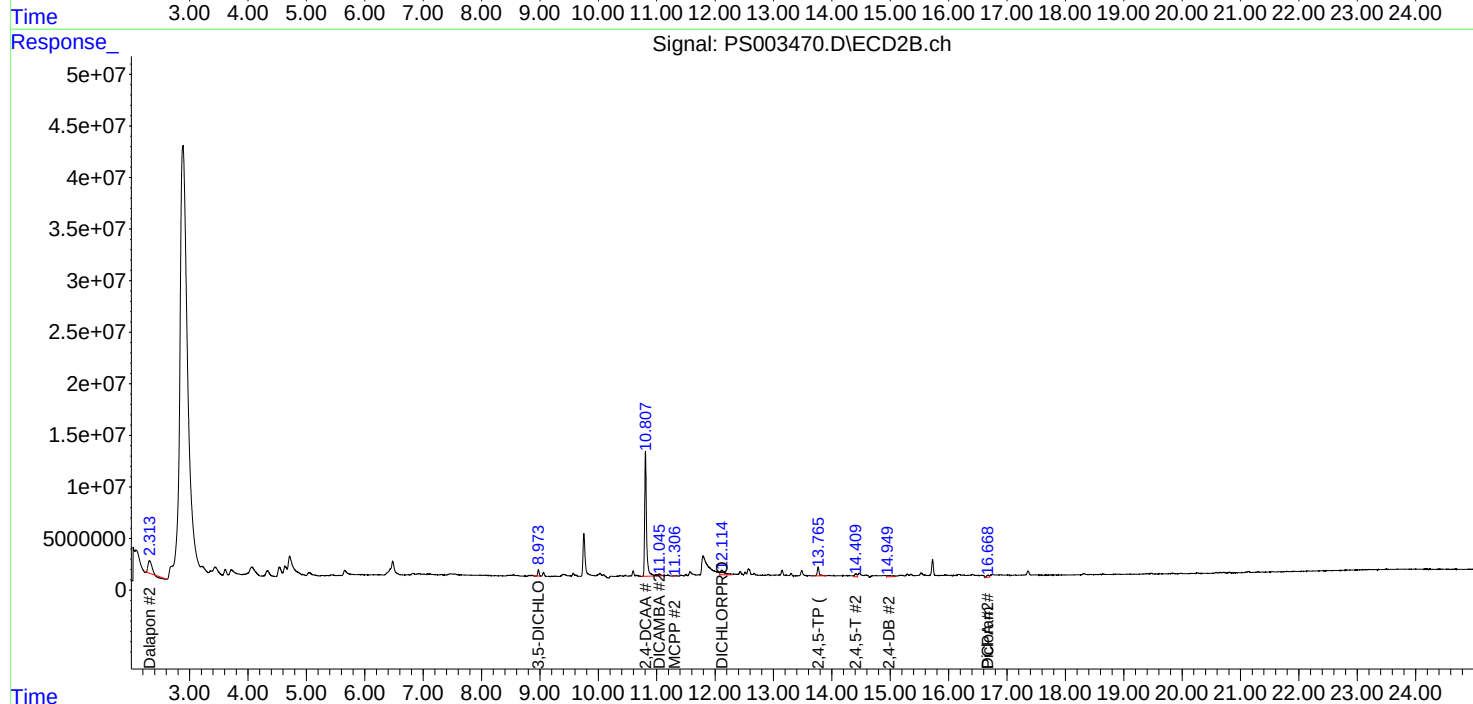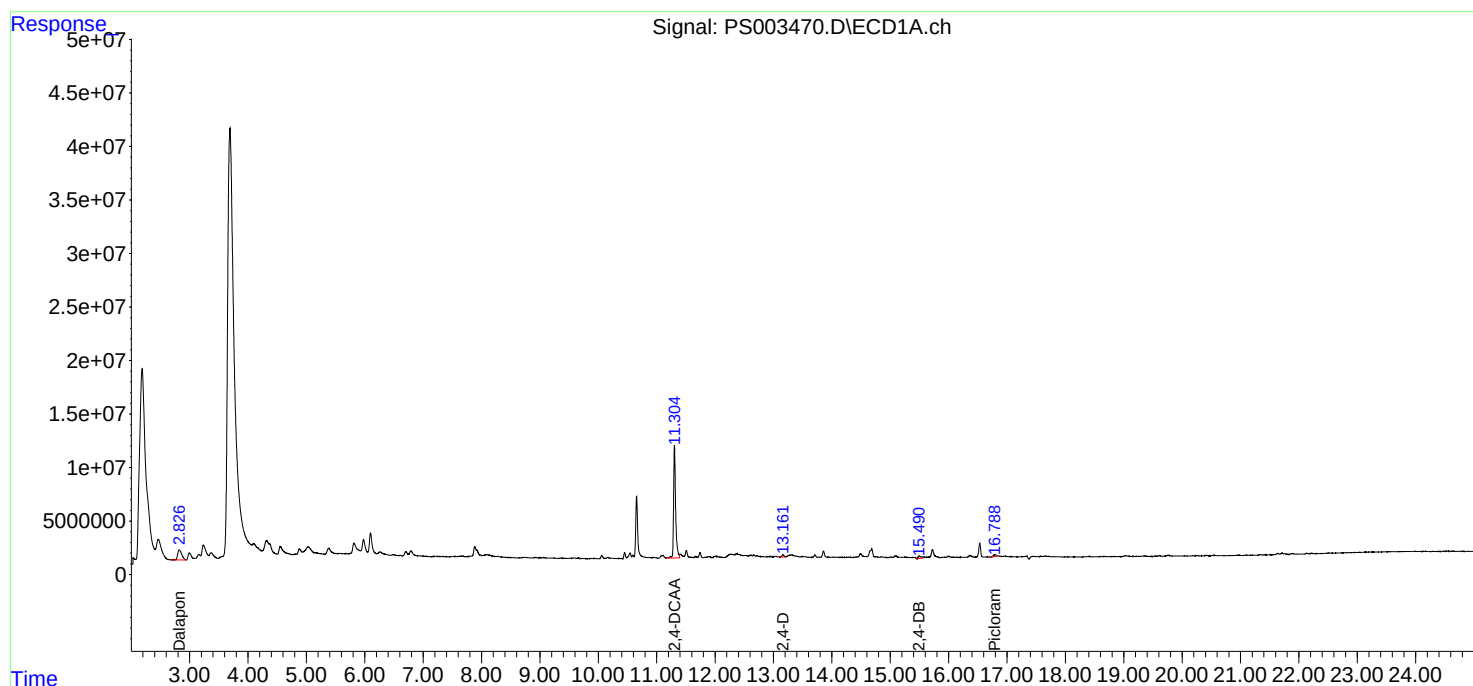


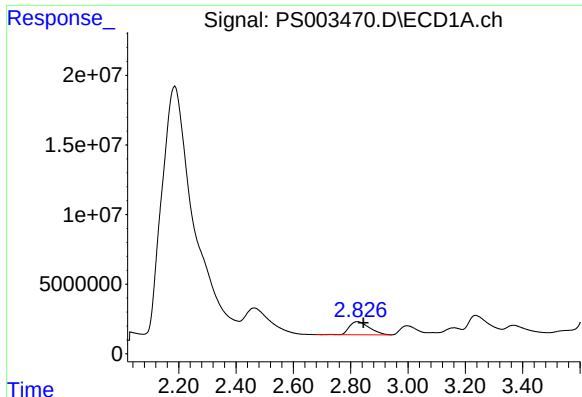

#1 Dalapon


R.T.: 2.823 min
Delta R.T.: -0.021 min
Response: 45412507
Conc: 69.87 ng/ml

Instrument :
ECD_S
ClientSampleId :
Z2-9

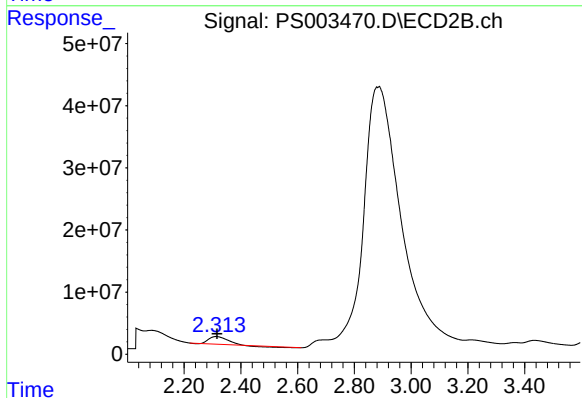


#1 Dalapon

R.T.: 2.313 min
Delta R.T.: -0.004 min
Response: 47278446
Conc: 74.67 ng/ml

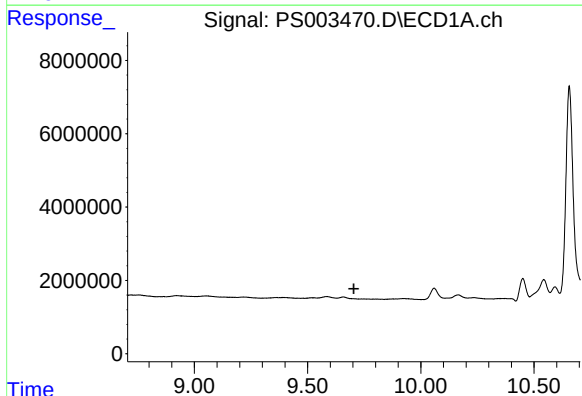


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.705 min
Response: 0
Conc: N.D.

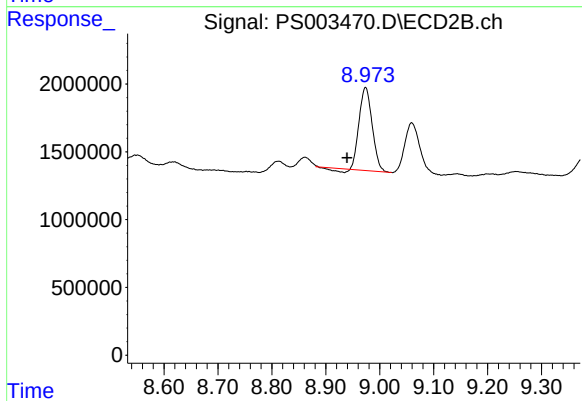

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.974 min
Delta R.T.: 0.034 min
Response: 10042768
Conc: 16.26 ng/ml

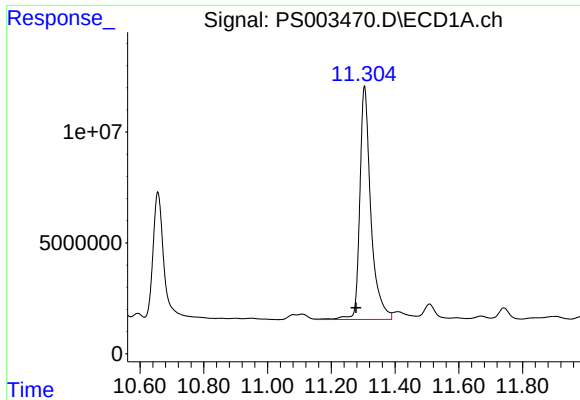

#4 2,4-DCAA


R.T.: 11.304 min
Delta R.T.: 0.026 min
Response: 253294197
Conc: 576.95 ng/ml

Instrument :
ECD_S
ClientSampleId :
Z2-9

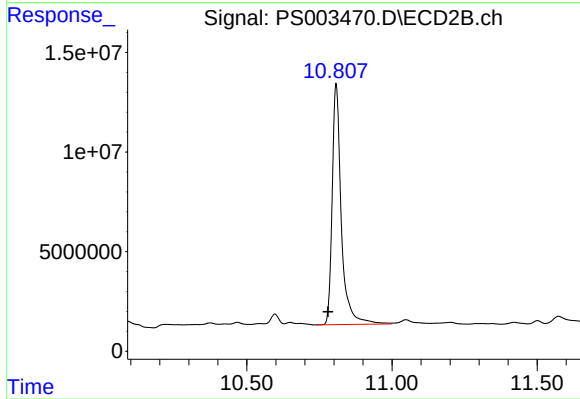


#4 2,4-DCAA

R.T.: 10.808 min
Delta R.T.: 0.028 min
Response: 265106128
Conc: 564.57 ng/ml

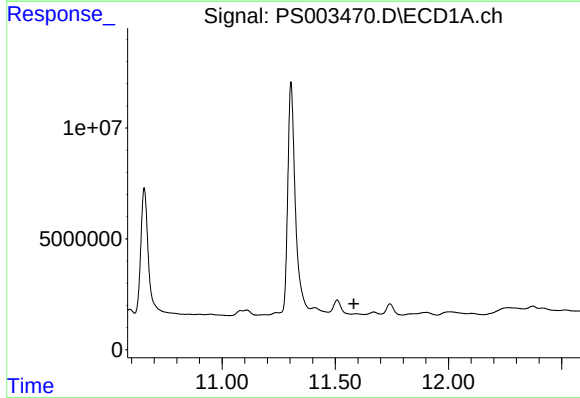


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.582 min
Response: 0
Conc: N.D.

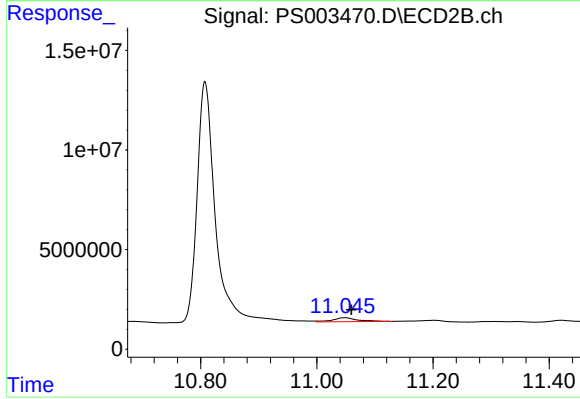

#5 DICAMBA


R.T.: 11.048 min
Delta R.T.: -0.012 min
Response: 5747895
Conc: 3.44 ng/ml

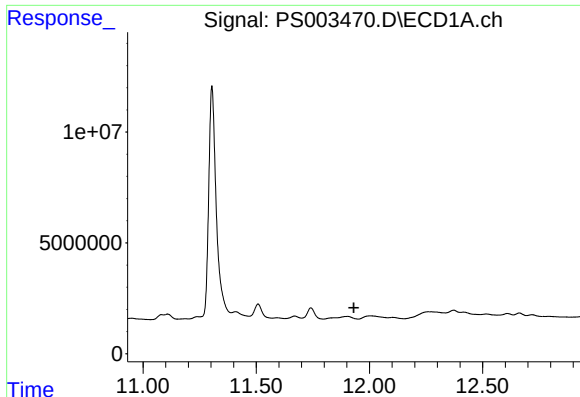

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.931 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
Z2-9

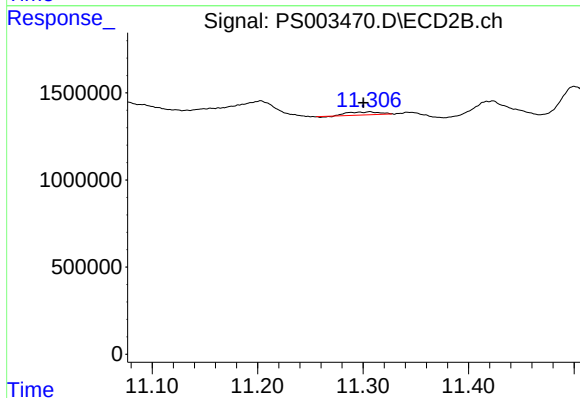


#6 MCP

R.T.: 11.304 min
Delta R.T.: 0.004 min
Response: 392651
Conc: 0.33 ug/ml

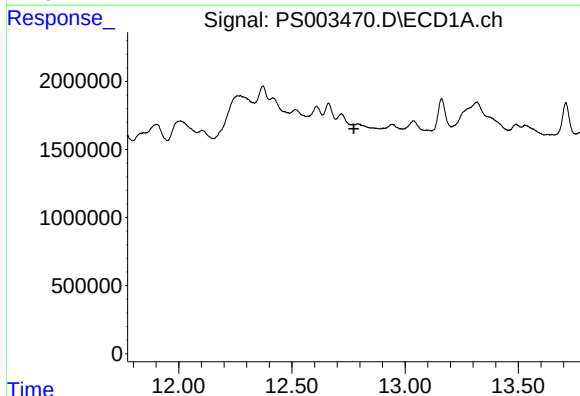


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 12.773 min
Response: 0
Conc: N.D.

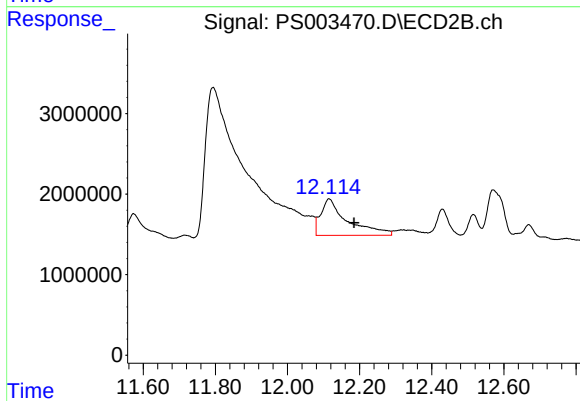

#8 DICHLORPROP


R.T.: 12.116 min
Delta R.T.: -0.069 min
Response: 23122731
Conc: 55.95 ng/ml

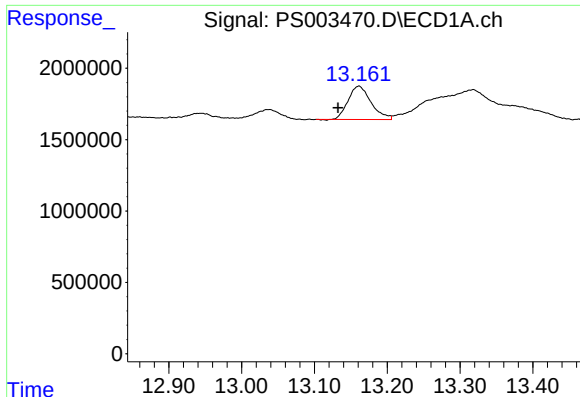

#9 2,4-D


R.T.: 13.161 min
Delta R.T.: 0.028 min
Response: 5107614
Conc: 11.01 ng/ml

Instrument :
ECD_S
ClientSampleId :
Z2-9

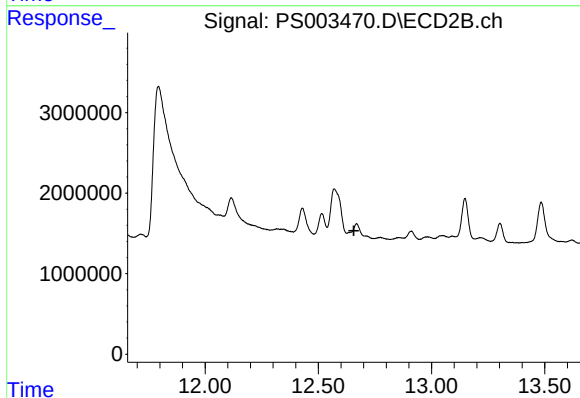


#9 2,4-D

R.T.: 12.669 min
Delta R.T.: 0.012 min
Response: -7221310
Conc: N.D.

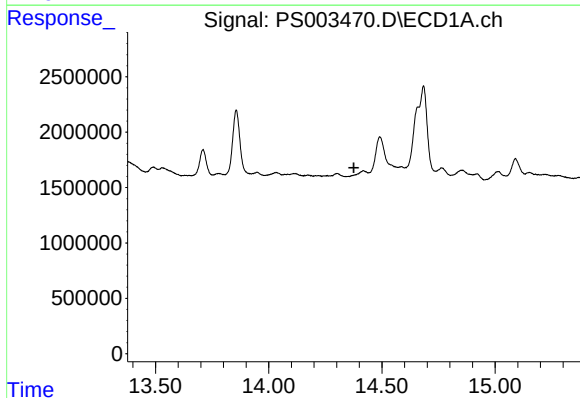


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.376 min
Response: 0
Conc: N.D.

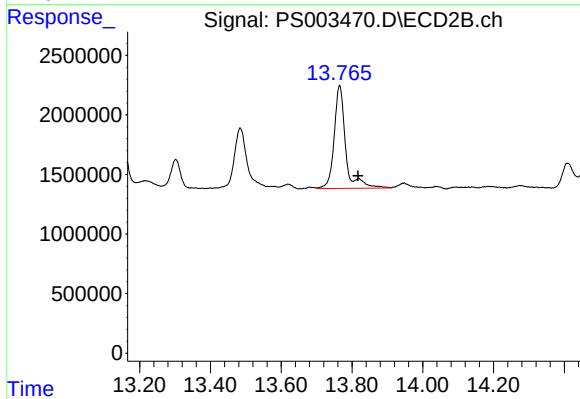

#11 2,4,5-TP (SILVEX)


R.T.: 13.765 min
Delta R.T.: -0.053 min
Response: 19437599
Conc: 7.63 ng/ml

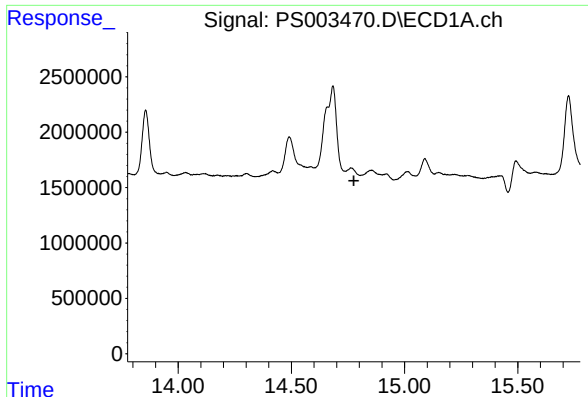

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
Z2-9

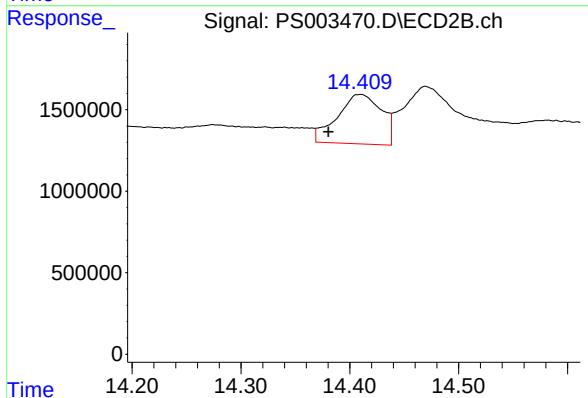


#12 2,4,5-T

R.T.: 14.410 min
Delta R.T.: 0.030 min
Response: 8612937
Conc: 4.27 ng/ml

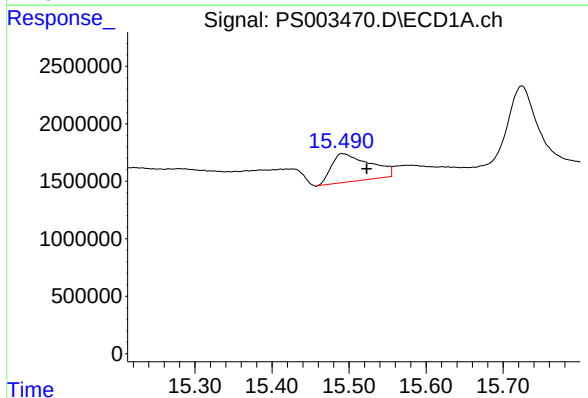


#13 2,4-DB

R.T.: 15.492 min
Delta R.T.: -0.031 min
Response: 8491870
Conc: 35.86 ng/ml

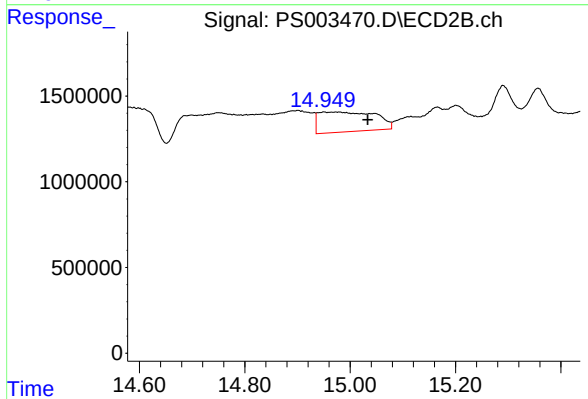

#13 2,4-DB


R.T.: 14.973 min
Delta R.T.: -0.060 min
Response: 8685955
Conc: 34.01 ng/ml

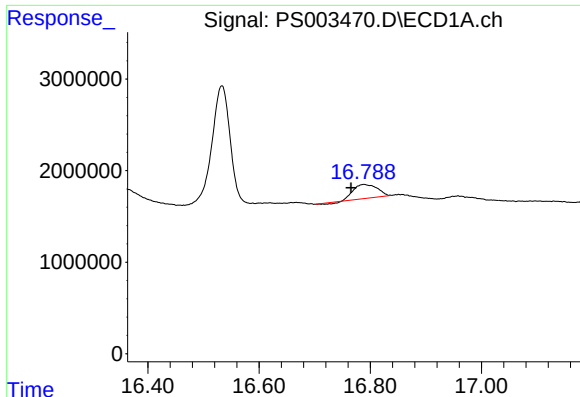

#15 Picloram


R.T.: 16.788 min
Delta R.T.: 0.023 min
Response: 4409528
Conc: 1.79 ng/ml

Instrument :
ECD_S
ClientSampleId :
Z2-9

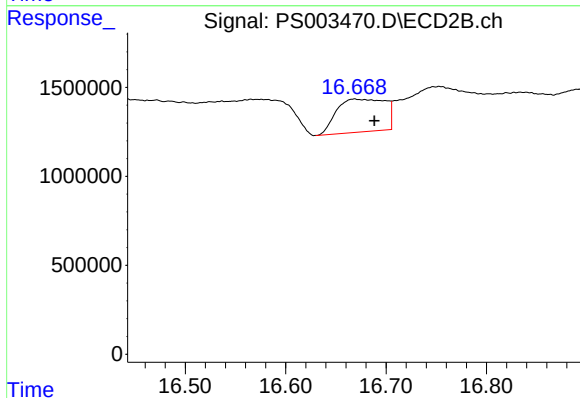


#15 Picloram

R.T.: 16.673 min
Delta R.T.: -0.016 min
Response: 6207954
Conc: 2.45 ng/ml

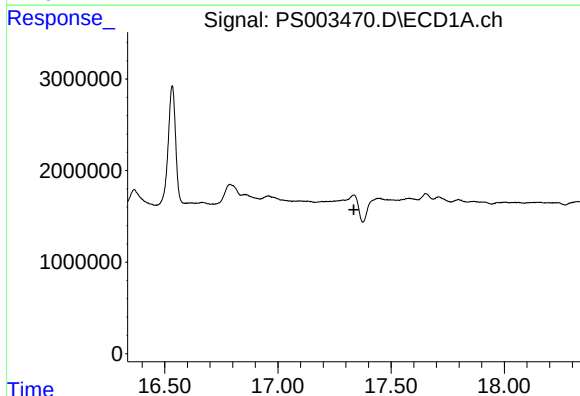

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.335 min
Response: 0
Conc: N.D.

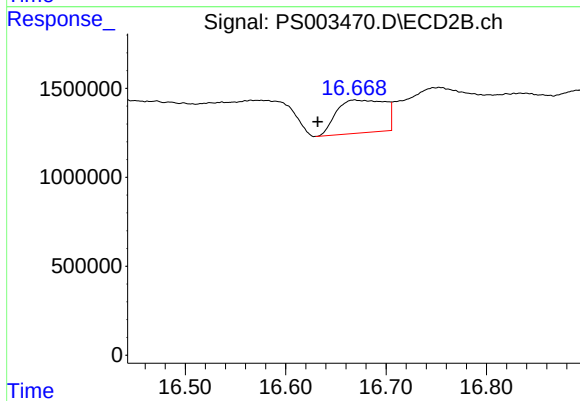

#16 DCPA

R.T.: 16.673 min
Delta R.T.: 0.041 min
Response: 6207954
Conc: 2.00 ng/ml