

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030819\
 Data File : PS003476.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Mar 2019 18:47
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 08 22:03:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.309	10.809	222.4E6	209.9E6	506.596	447.040
Target Compounds							
2) T	3,5-DICHL...	0.000	8.933	0	28572	N.D.	0.046 #
3) T	4-Nitroph...	0.000	9.975	0	13970	N.D.	0.062 #
7) T	MCPA	0.000	11.695	0	366629	N.D.	0.213 #
10) T	Pentachlo...	0.000	13.227	0	923222	N.D.	0.140 #
11) T	2,4,5-TP ...	0.000	13.751	0	67942	N.D.	0.027 #
12) T	2,4,5-T	0.000	14.411	0	93095	N.D.	0.046 #
13) T	2,4-DB	0.000	14.990	0	174097	N.D.	0.682 #
14) T	DINOSEB	0.000	15.464	0	63012	N.D.	0.035 #
15) T	Picloram	0.000	16.661	0	763900	N.D.	0.301 #
16) T	DCPA	0.000	16.661	0	763900	N.D.	0.246 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030819\
Data File : PS003476.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Mar 2019 18:47
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 08 22:03:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

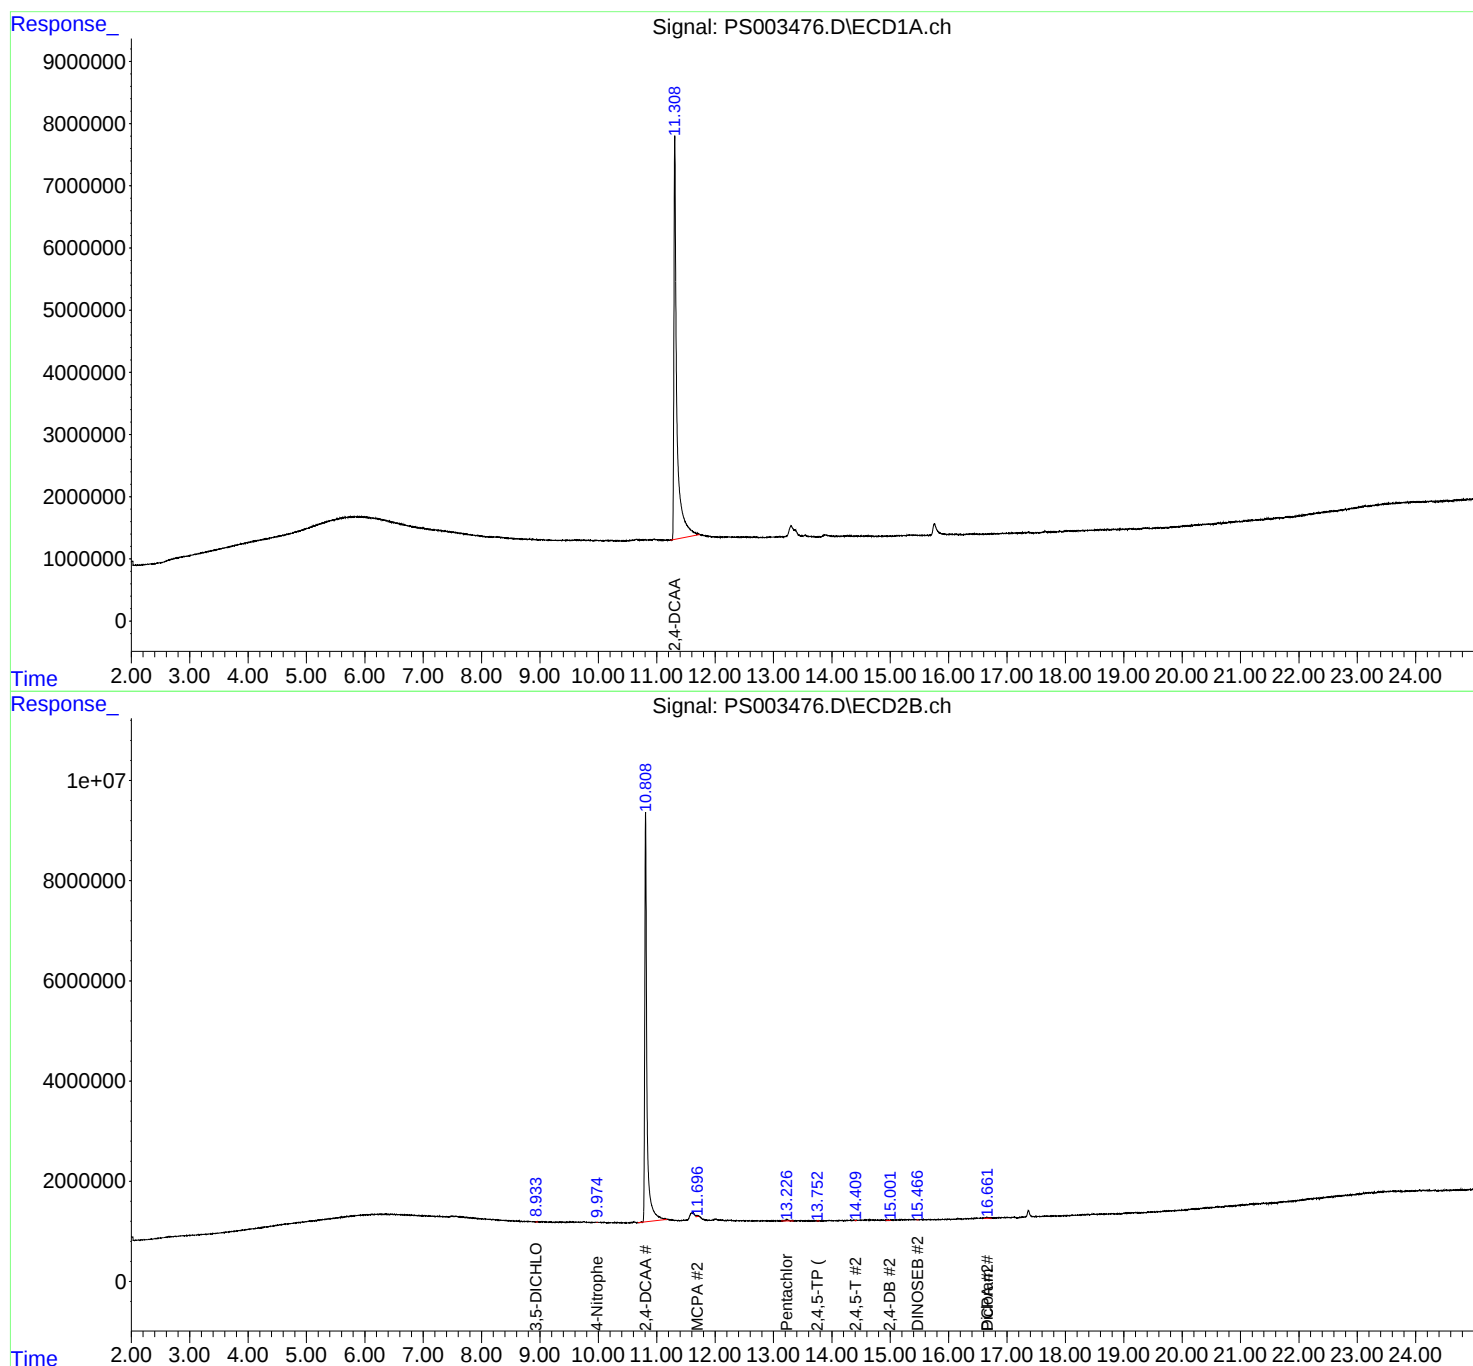


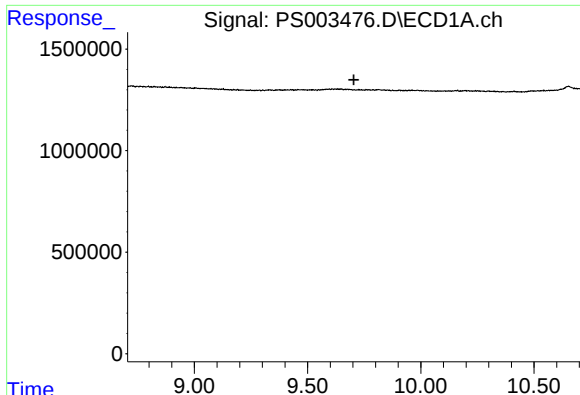

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.705 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

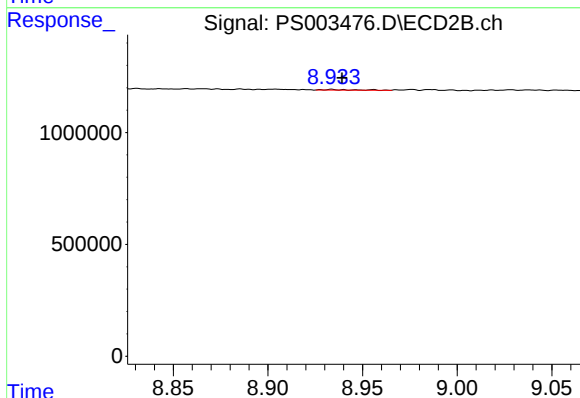


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 8.933 min
Delta R.T.: -0.006 min
Response: 28572
Conc: 0.05 ng/ml

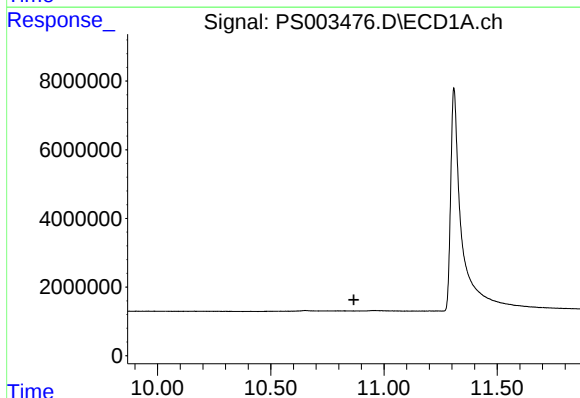


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

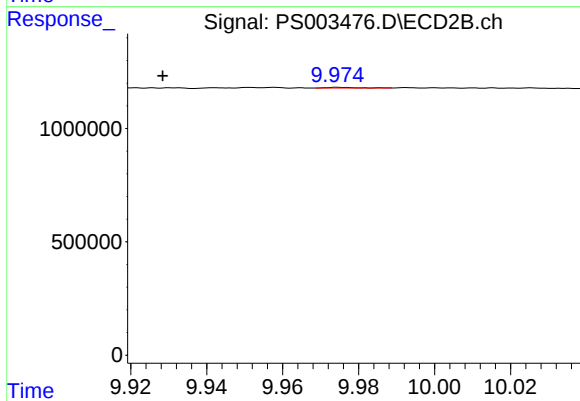

#3 4-Nitrophenol


R.T.: 9.975 min
Delta R.T.: 0.047 min
Response: 13970
Conc: 0.06 ng/ml

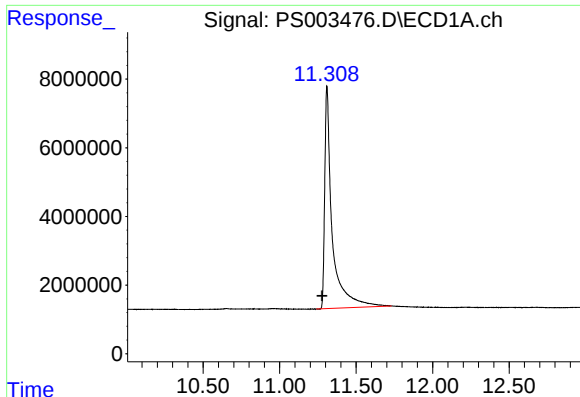

#4 2,4-DCAA


R.T.: 11.309 min
Delta R.T.: 0.031 min
Response: 222407976
Conc: 506.60 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

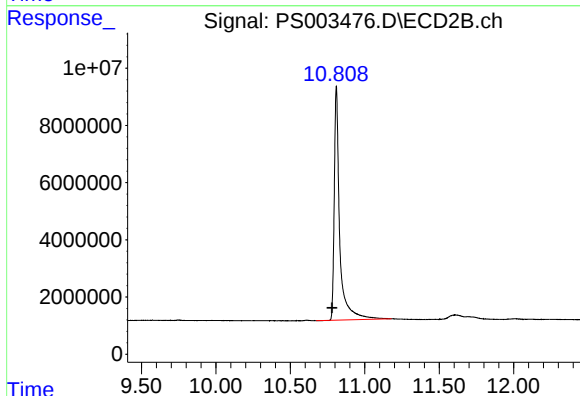


#4 2,4-DCAA

R.T.: 10.809 min
Delta R.T.: 0.029 min
Response: 209916345
Conc: 447.04 ng/ml

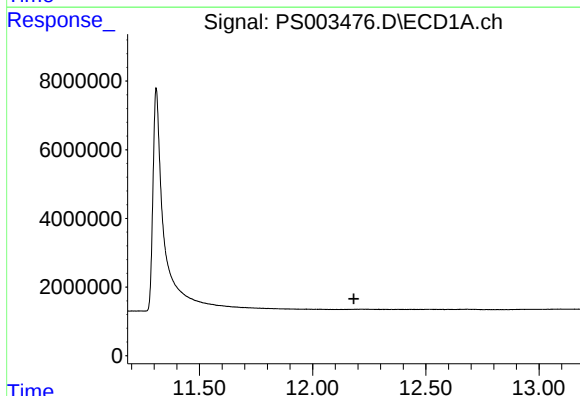


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.182 min
Response: 0
Conc: N.D.

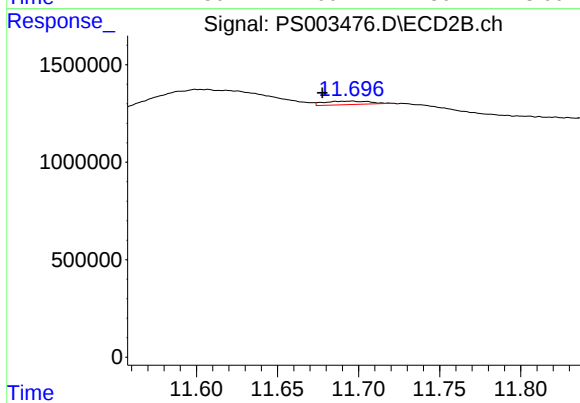

#7 MCPA


R.T.: 11.695 min
Delta R.T.: 0.017 min
Response: 366629
Conc: 0.21 ug/ml

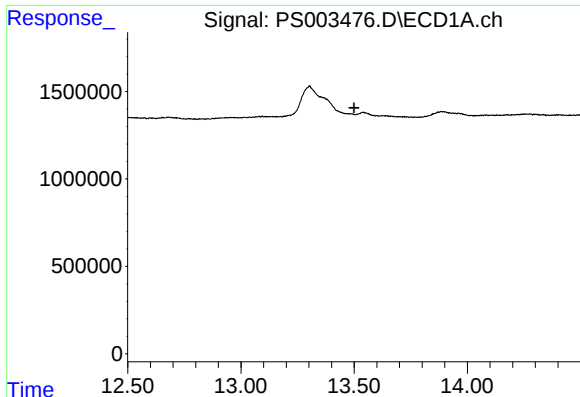

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.499 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

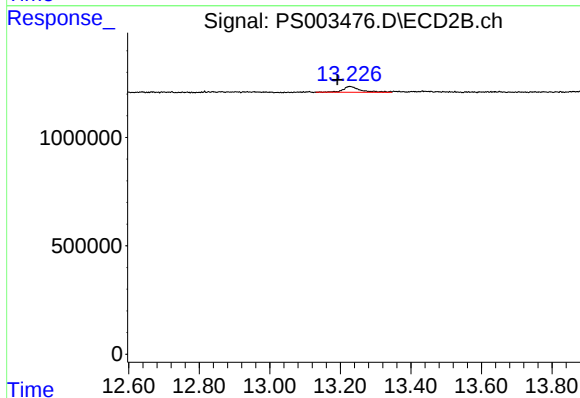


#10 Pentachlorophenol

R.T.: 13.227 min
Delta R.T.: 0.036 min
Response: 923222
Conc: 0.14 ng/ml

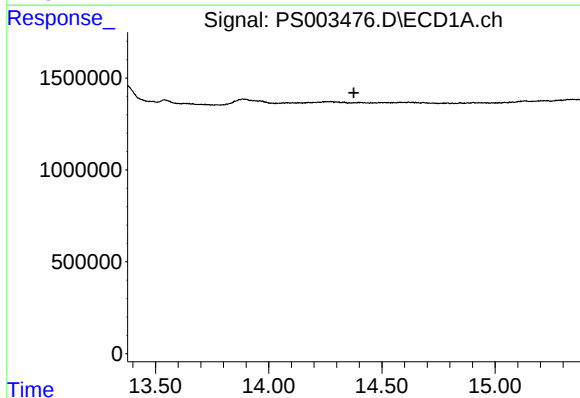


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

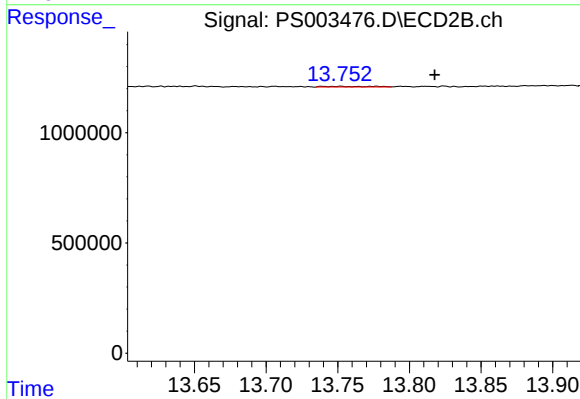

#11 2,4,5-TP (SILVEX)


R.T.: 13.751 min
Delta R.T.: -0.066 min
Response: 67942
Conc: 0.03 ng/ml

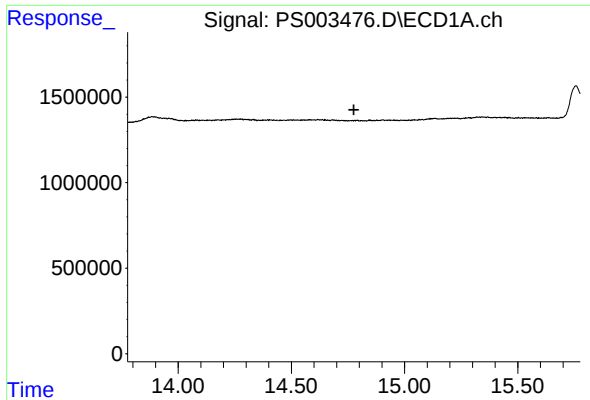

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

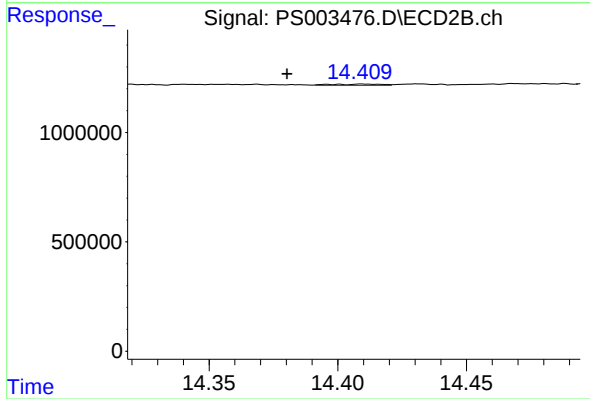


#12 2,4,5-T

R.T.: 14.411 min
Delta R.T.: 0.031 min
Response: 93095
Conc: 0.05 ng/ml

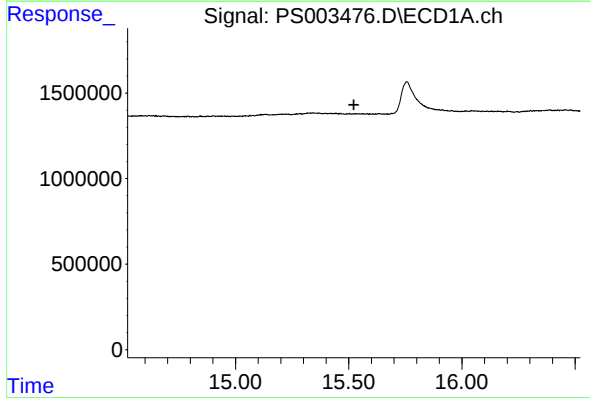


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.523 min
Response: 0
Conc: N.D.

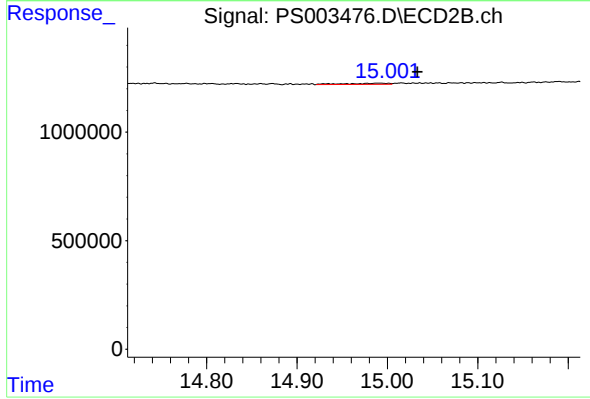

#13 2,4-DB


R.T.: 14.990 min
Delta R.T.: -0.043 min
Response: 174097
Conc: 0.68 ng/ml

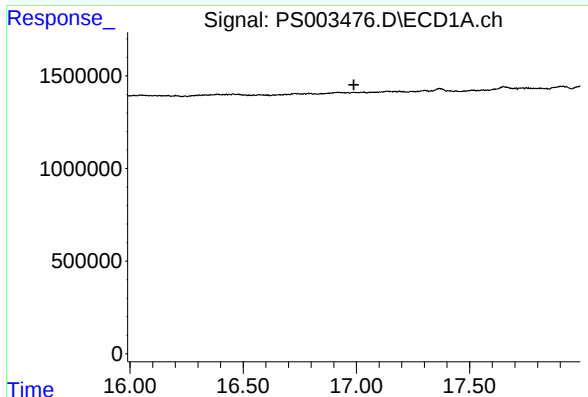

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

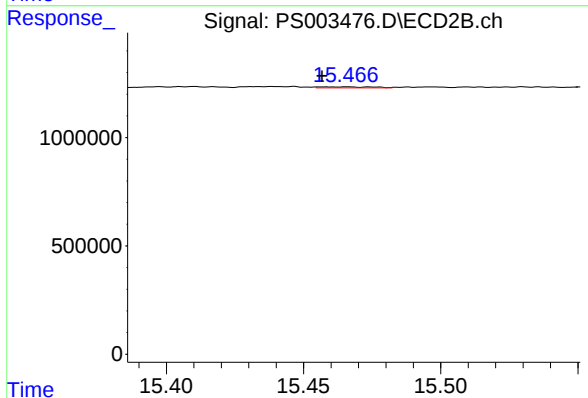


#14 DINOSEB

R.T.: 15.464 min
Delta R.T.: 0.007 min
Response: 63012
Conc: 0.04 ng/ml

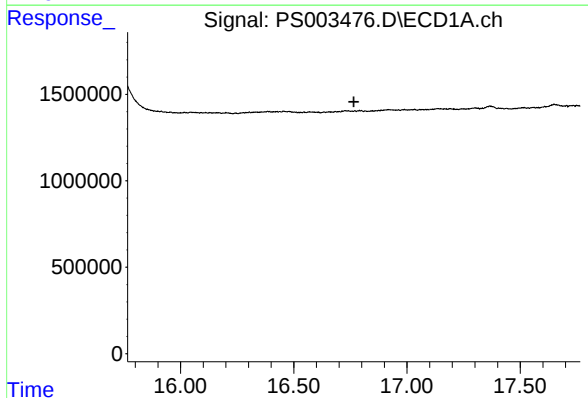


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.765 min
Response: 0
Conc: N.D.

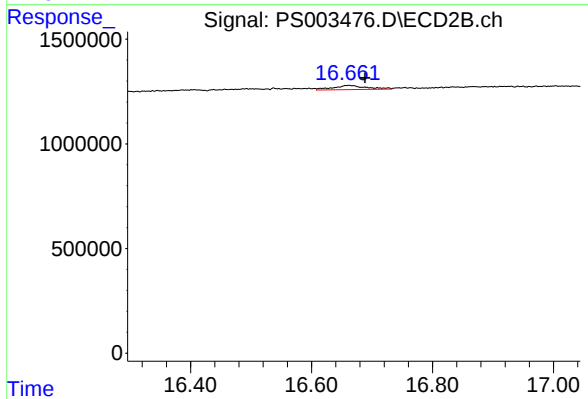

#15 Picloram


R.T.: 16.661 min
Delta R.T.: -0.027 min
Response: 763900
Conc: 0.30 ng/ml

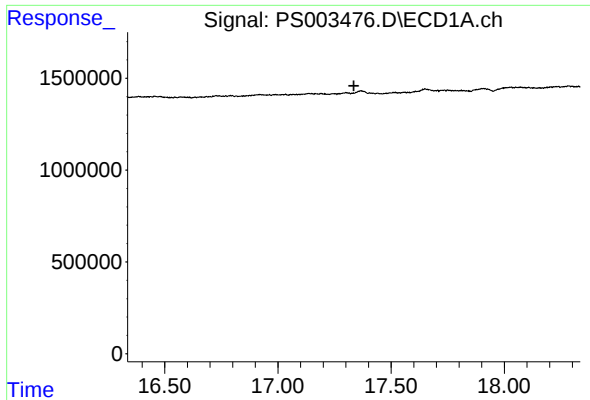

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.335 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

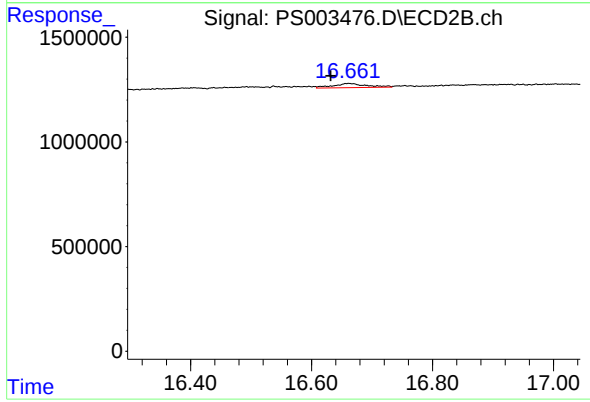

#16 DCPA

R.T.: 16.661 min
Delta R.T.: 0.029 min
Response: 763900
Conc: 0.25 ng/ml