

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030819\
 Data File : PS003481.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Mar 2019 21:22
 Operator : EI\SJ
 Sample : K1757-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-6CD-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 08 22:04:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.271	10.773	234.3E6	239.9E6	533.772	510.979
Target Compounds							
1) T	Dalapon	2.790	2.279	31159393	41400009	47.942	65.384 #
2) T	3,5-DICHL...	0.000	8.939	0	8592904	N.D.	13.917 #
3) T	4-Nitroph...	0.000	9.992	0	10193180	N.D.	45.338 #
5) T	DICAMBA	11.634	11.013	3284118	5134751	1.863	3.073 #
6) T	MCP	11.980	11.308	12590655	235305	9.590	0.199 #
7) T	MCPA	12.214	11.685	31716232	-871467	15.990	N.D. #
9) T	2,4-D	13.126	12.634	5718912	1818726	12.330	3.465 #
11) T	2,4,5-TP ...	0.000	13.783	0	1722043	N.D.	0.676 #
12) T	2,4,5-T	0.000	14.374	0	8827252	N.D.	4.377 #
13) T	2,4-DB	15.460	15.002	925811	2666016	3.910	10.440 #
14) T	DINOSEB	0.000	15.497	0	2858895	N.D.	1.602 #
15) T	Picloram	16.761	16.720	7439462	11843300	3.023	4.666 #
16) T	DCPA	0.000	16.637	0	5484726	N.D.	1.763 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030819\
Data File : PS003481.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Mar 2019 21:22
Operator : EI\SJ
Sample : K1757-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-6CD-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 08 22:04:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

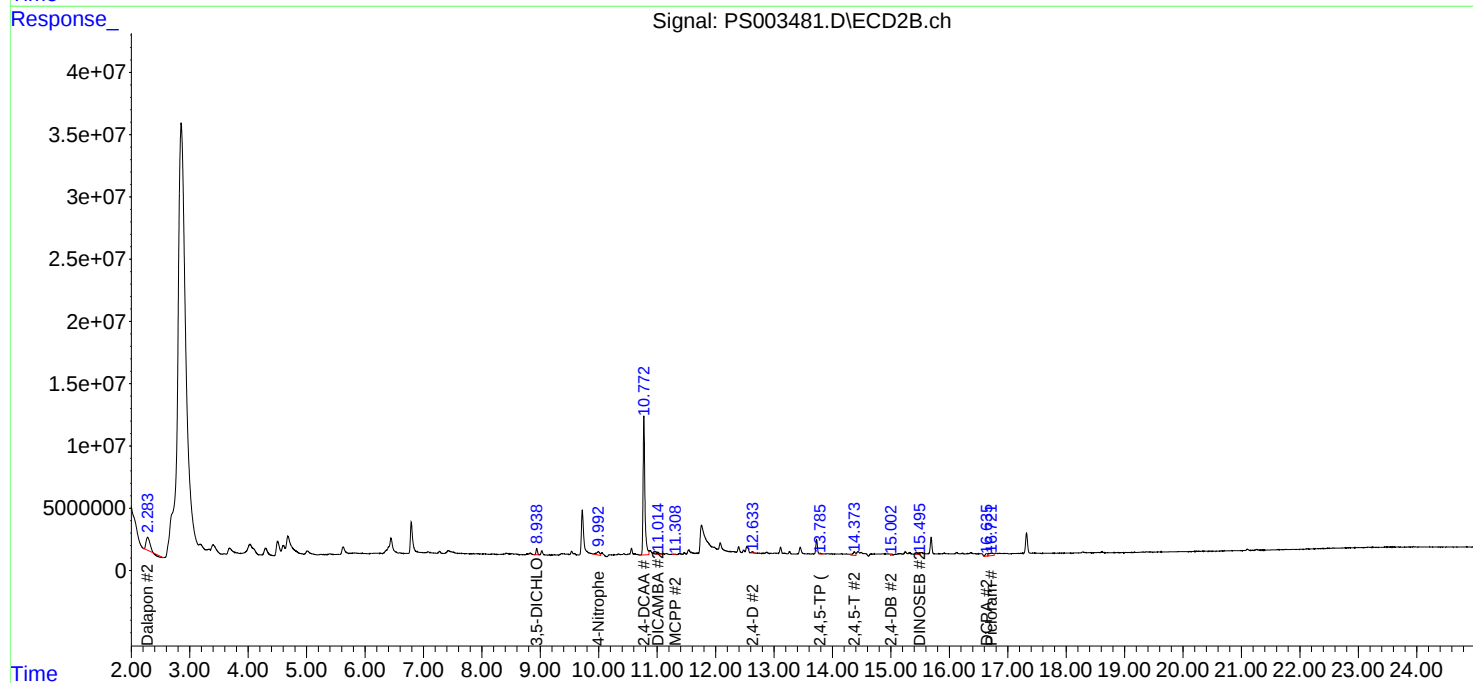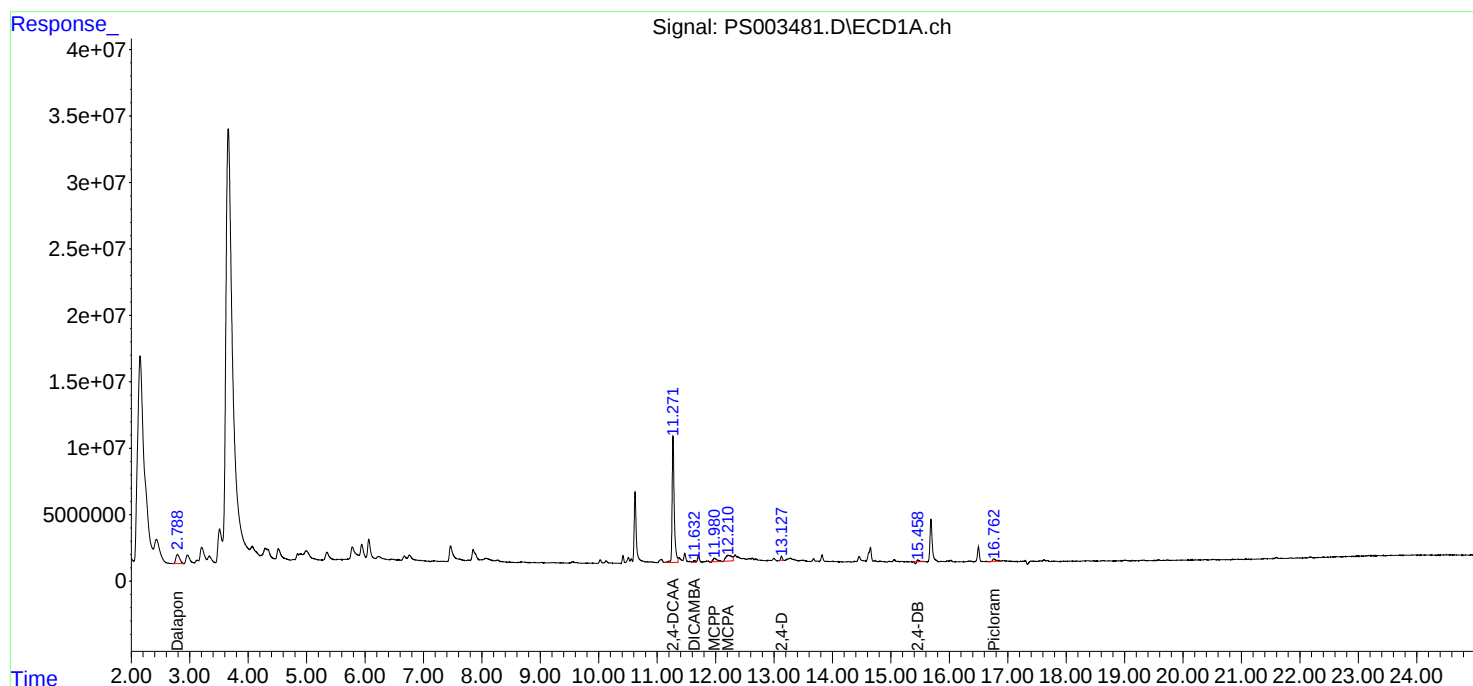


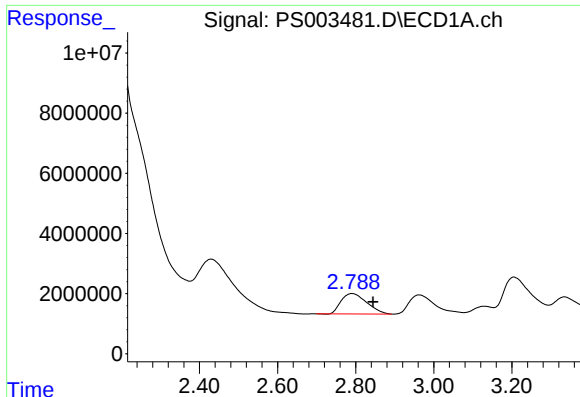

#1 Dalapon


R.T.: 2.790 min
Delta R.T.: -0.054 min
Response: 31159393
Conc: 47.94 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-6CD-S

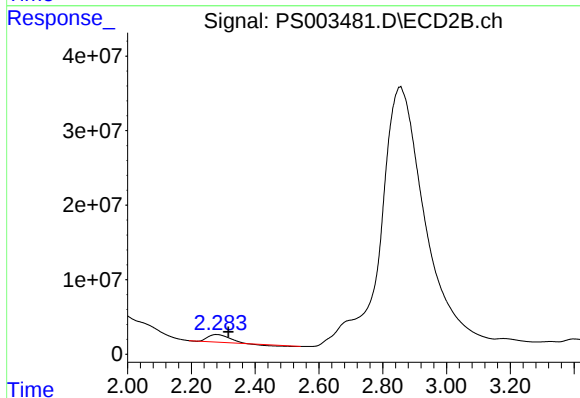


#1 Dalapon

R.T.: 2.279 min
Delta R.T.: -0.038 min
Response: 41400009
Conc: 65.38 ng/ml

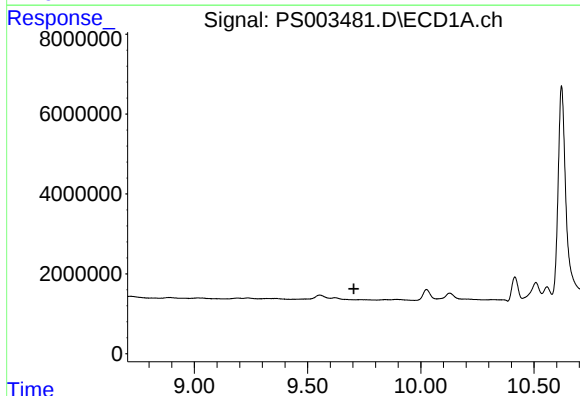


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.705 min
Response: 0
Conc: N.D.

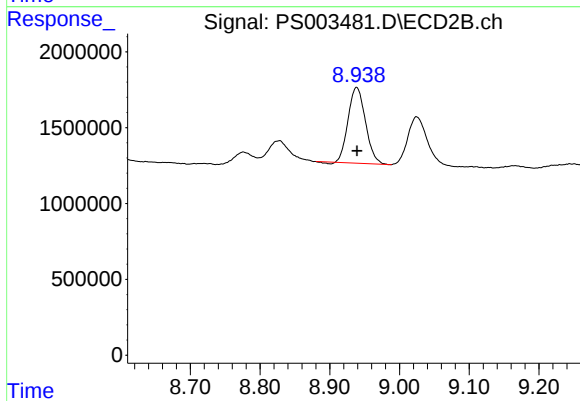

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.939 min
Delta R.T.: 0.000 min
Response: 8592904
Conc: 13.92 ng/ml

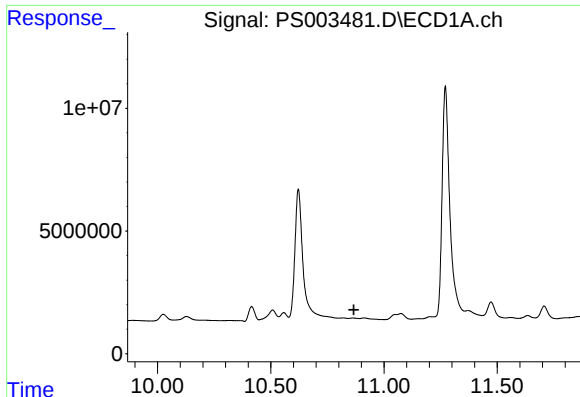

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-6CD-S

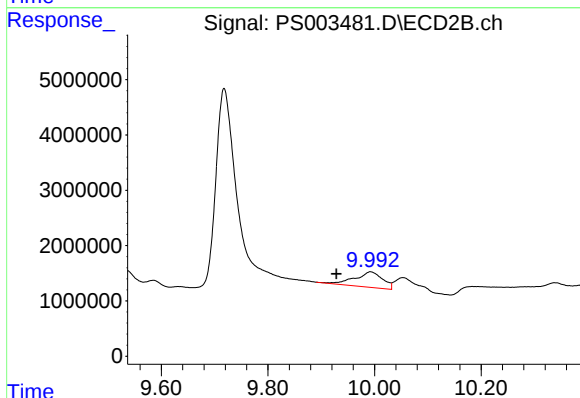


#3 4-Nitrophenol

R.T.: 9.992 min
Delta R.T.: 0.064 min
Response: 10193180
Conc: 45.34 ng/ml

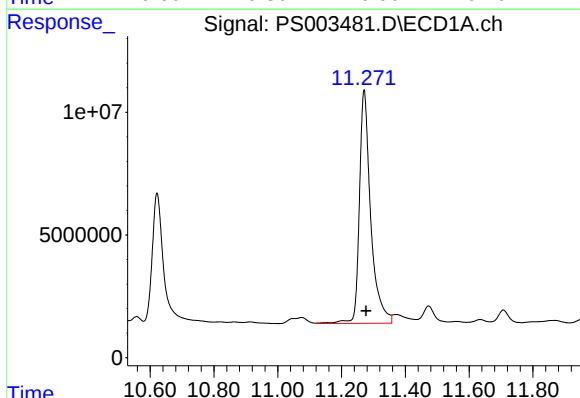


#4 2,4-DCAA

R.T.: 11.271 min
Delta R.T.: -0.007 min
Response: 234338780
Conc: 533.77 ng/ml

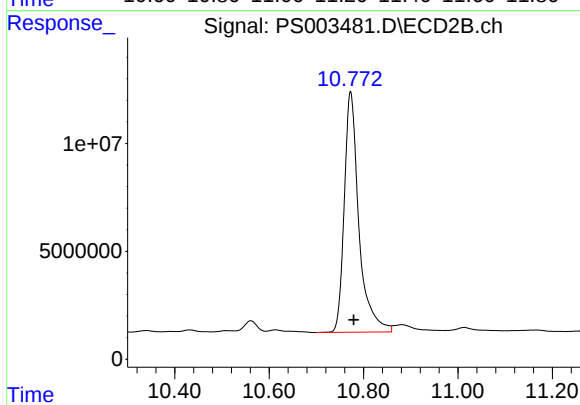

#4 2,4-DCAA


R.T.: 10.773 min
Delta R.T.: -0.007 min
Response: 239939844
Conc: 510.98 ng/ml

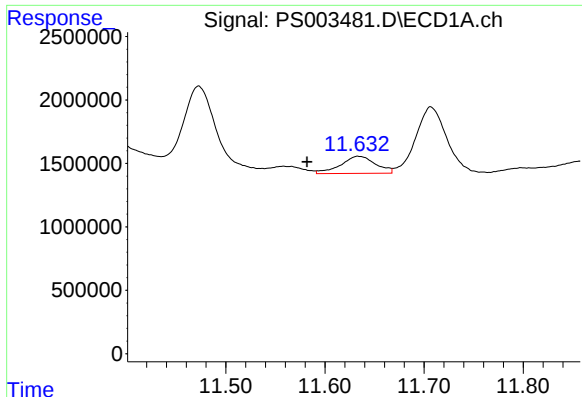

#5 DICAMBA


R.T.: 11.634 min
Delta R.T.: 0.052 min
Response: 3284118
Conc: 1.86 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-6CD-S

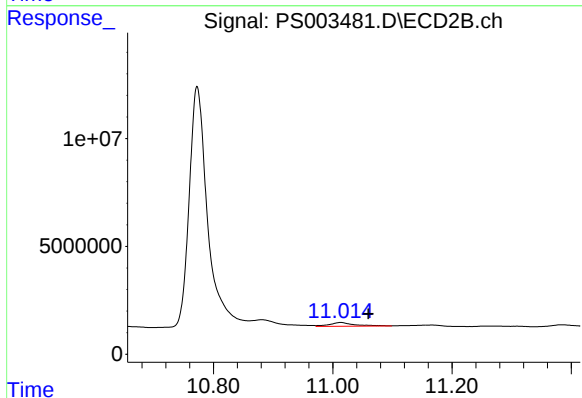


#5 DICAMBA

R.T.: 11.013 min
Delta R.T.: -0.046 min
Response: 5134751
Conc: 3.07 ng/ml

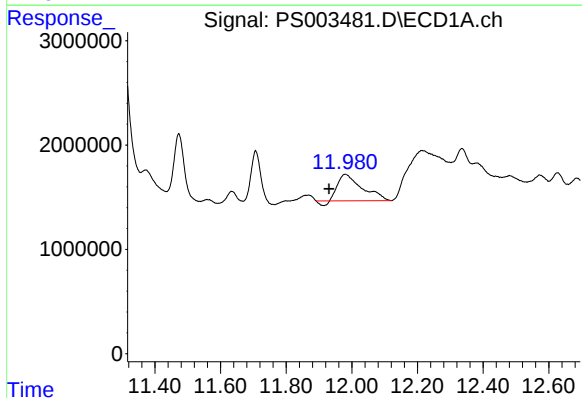


#6 MCP

R.T.: 11.980 min
Delta R.T.: 0.049 min
Response: 12590655
Conc: 9.59 ug/ml

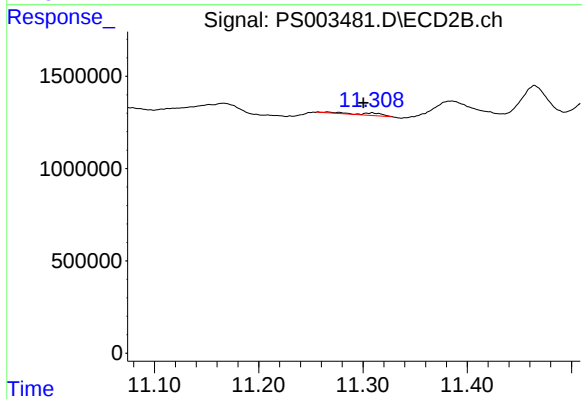

#6 MCP


R.T.: 11.308 min
Delta R.T.: 0.008 min
Response: 235305
Conc: 0.20 ug/ml

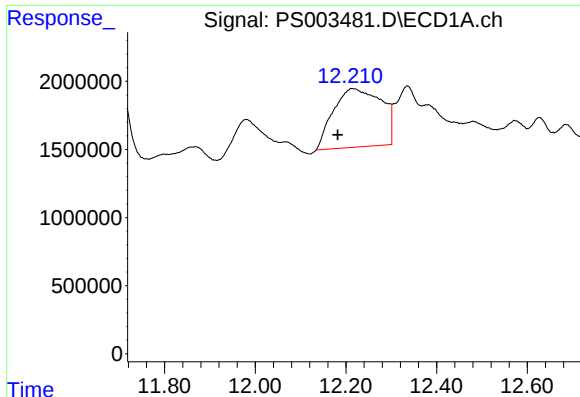

#7 MCPA


R.T.: 12.214 min
Delta R.T.: 0.032 min
Response: 31716232
Conc: 15.99 ug/ml

Instrument :
ECD_S
ClientSampleId :
TP-6CD-S

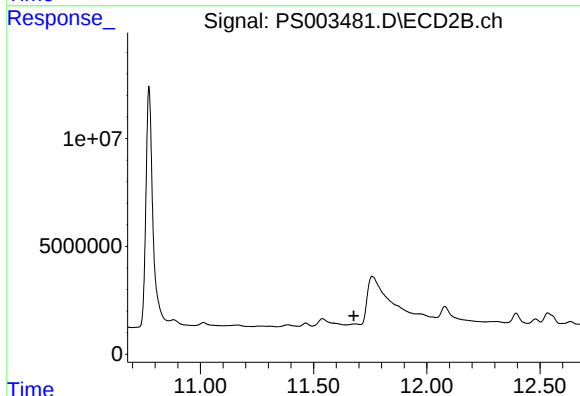


#7 MCPA

R.T.: 11.685 min
Delta R.T.: 0.007 min
Response: -871467
Conc: N.D.

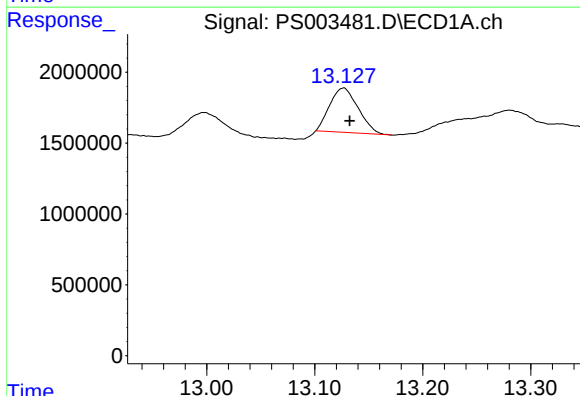


#9 2,4-D

R.T.: 13.126 min
Delta R.T.: -0.006 min
Response: 5718912
Conc: 12.33 ng/ml

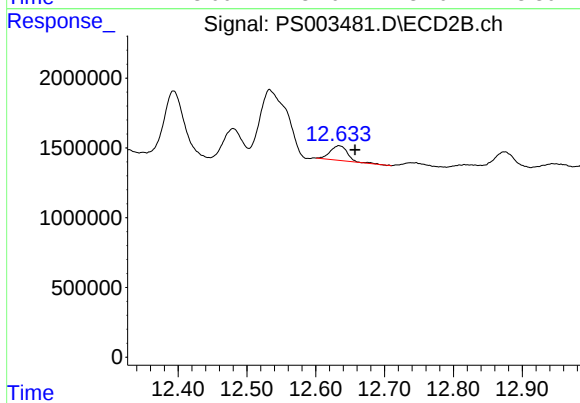

#9 2,4-D


R.T.: 12.634 min
Delta R.T.: -0.023 min
Response: 1818726
Conc: 3.46 ng/ml

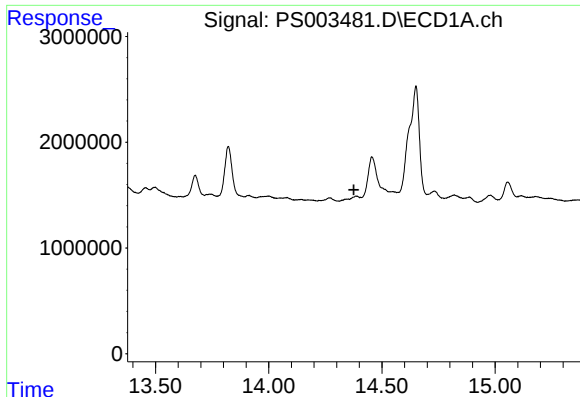

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-6CD-S

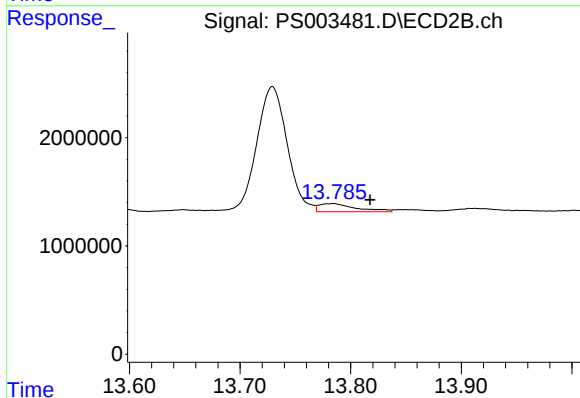


#11 2,4,5-TP (SILVEX)

R.T.: 13.783 min
Delta R.T.: -0.035 min
Response: 1722043
Conc: 0.68 ng/ml

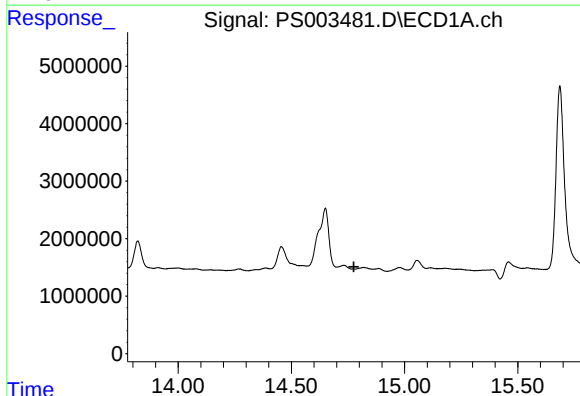


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

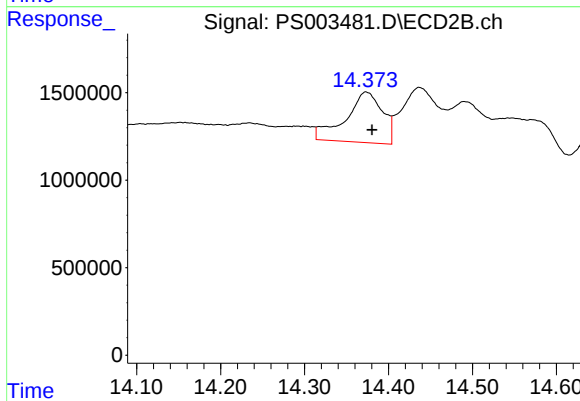

#12 2,4,5-T


R.T.: 14.374 min
Delta R.T.: -0.007 min
Response: 8827252
Conc: 4.38 ng/ml

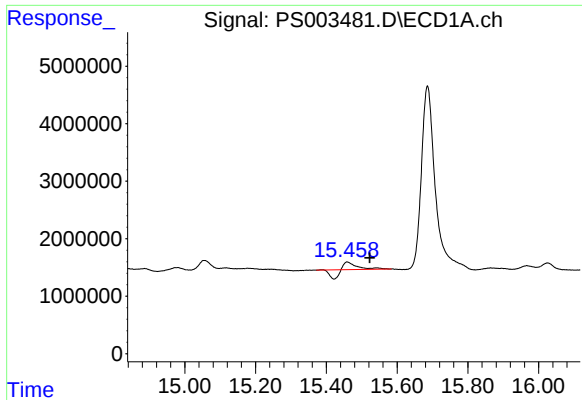

#13 2,4-DB


R.T.: 15.460 min
Delta R.T.: -0.063 min
Response: 925811
Conc: 3.91 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-6CD-S

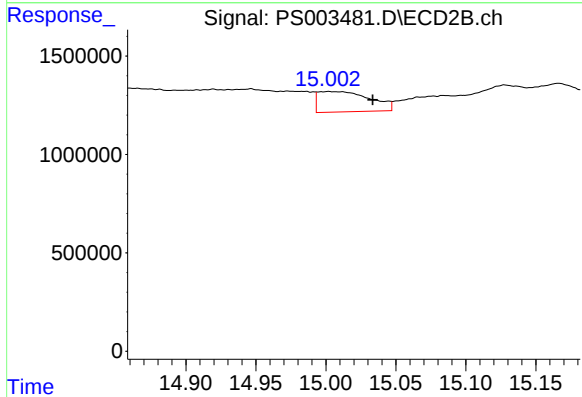


#13 2,4-DB

R.T.: 15.002 min
Delta R.T.: -0.031 min
Response: 2666016
Conc: 10.44 ng/ml

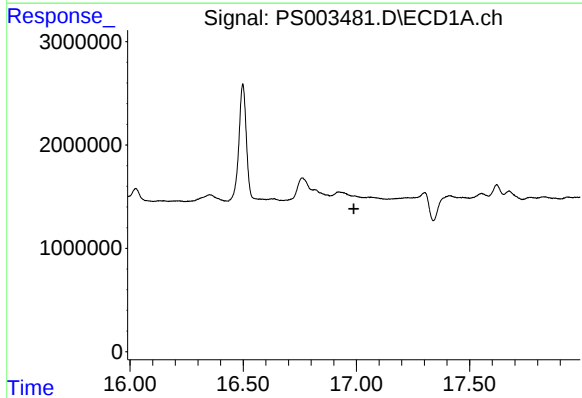


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 16.989 min
Response: 0
Conc: N.D.

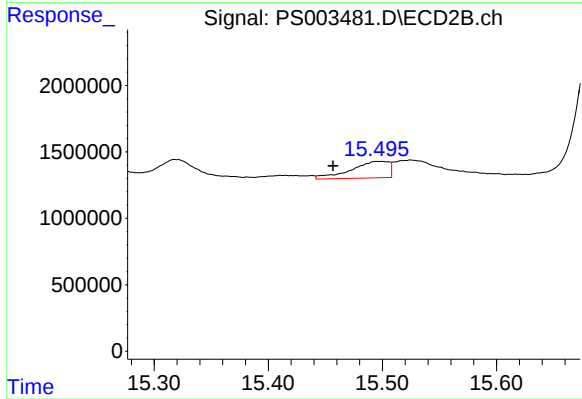

#14 DINOSEB


R.T.: 15.497 min
Delta R.T.: 0.041 min
Response: 2858895
Conc: 1.60 ng/ml

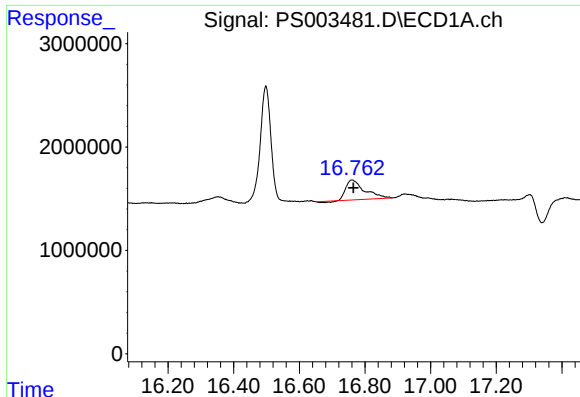

#15 Picloram


R.T.: 16.761 min
Delta R.T.: -0.004 min
Response: 7439462
Conc: 3.02 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-6CD-S

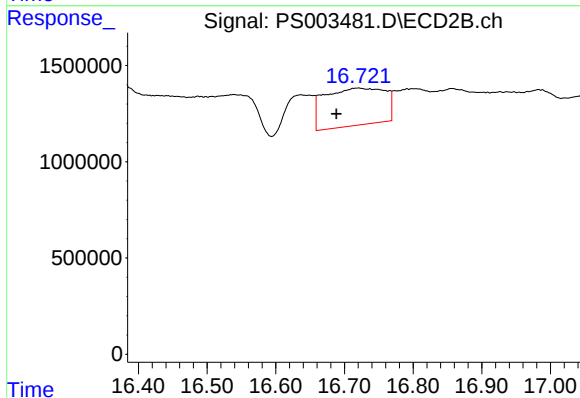


#15 Picloram

R.T.: 16.720 min
Delta R.T.: 0.032 min
Response: 11843300
Conc: 4.67 ng/ml

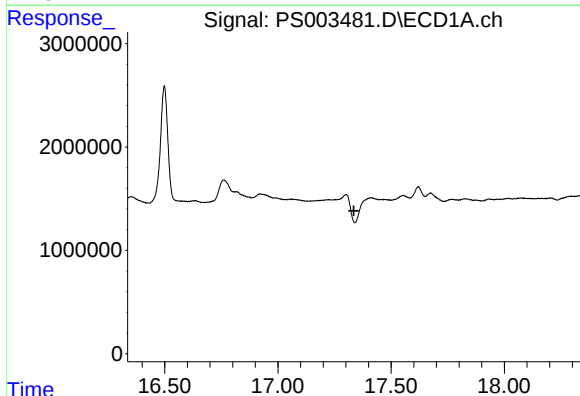

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.335 min
Response: 0
Conc: N.D.

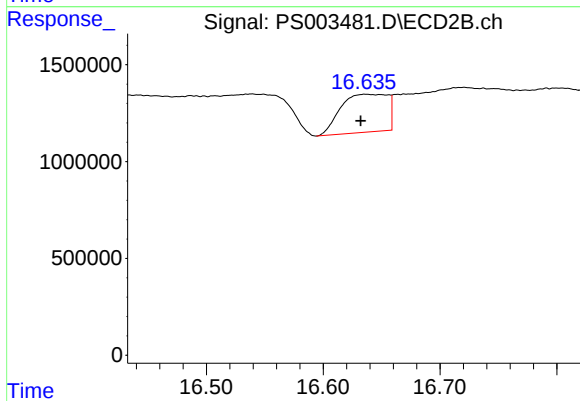

#16 DCPA

R.T.: 16.637 min
Delta R.T.: 0.005 min
Response: 5484726
Conc: 1.76 ng/ml