

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030819\
 Data File : PS003484.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Mar 2019 22:56
 Operator : EI\SJ
 Sample : K1757-08
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-6CD-D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 00:33:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.303	10.806	273.2E6	263.9E6	622.178	561.974
Target Compounds							
1) T	Dalapon	2.822	2.313	36459946	35411641	56.097	55.926
2) T	3,5-DICHL...	0.000	8.973	0	9513733	N.D.	15.408 #
5) T	DICAMBA	0.000	11.047	0	3485648	N.D.	2.086 #
6) T	MCP	0.000	11.287	0	398888	N.D.	0.338 #
7) T	MCPA	12.245	0.000	33981535	0	17.132	N.D. #
9) T	2,4-D	13.159	12.668	5378860	-5493419	11.597	N.D. #
10) T	Pentachlo...	13.528	13.217	12921488	2645421	1.829	0.402 #
11) T	2,4,5-TP ...	14.414	13.846	4326072	5368860	1.610	2.108 #
12) T	2,4,5-T	0.000	14.408	0	16222043	N.D.	8.044 #
13) T	2,4-DB	15.493	0.000	247742	0	1.046	N.D. #
14) T	DINOSEB	17.015	0.000	9420974	0	4.196	N.D. #
15) T	Picloram	16.793	16.662	8146878	7763419	3.310	3.059
16) T	DCPA	0.000	16.662	0	7763419	N.D.	2.496 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030819\
Data File : PS003484.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Mar 2019 22:56
Operator : EI\SJ
Sample : K1757-08
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-6CD-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 00:33:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

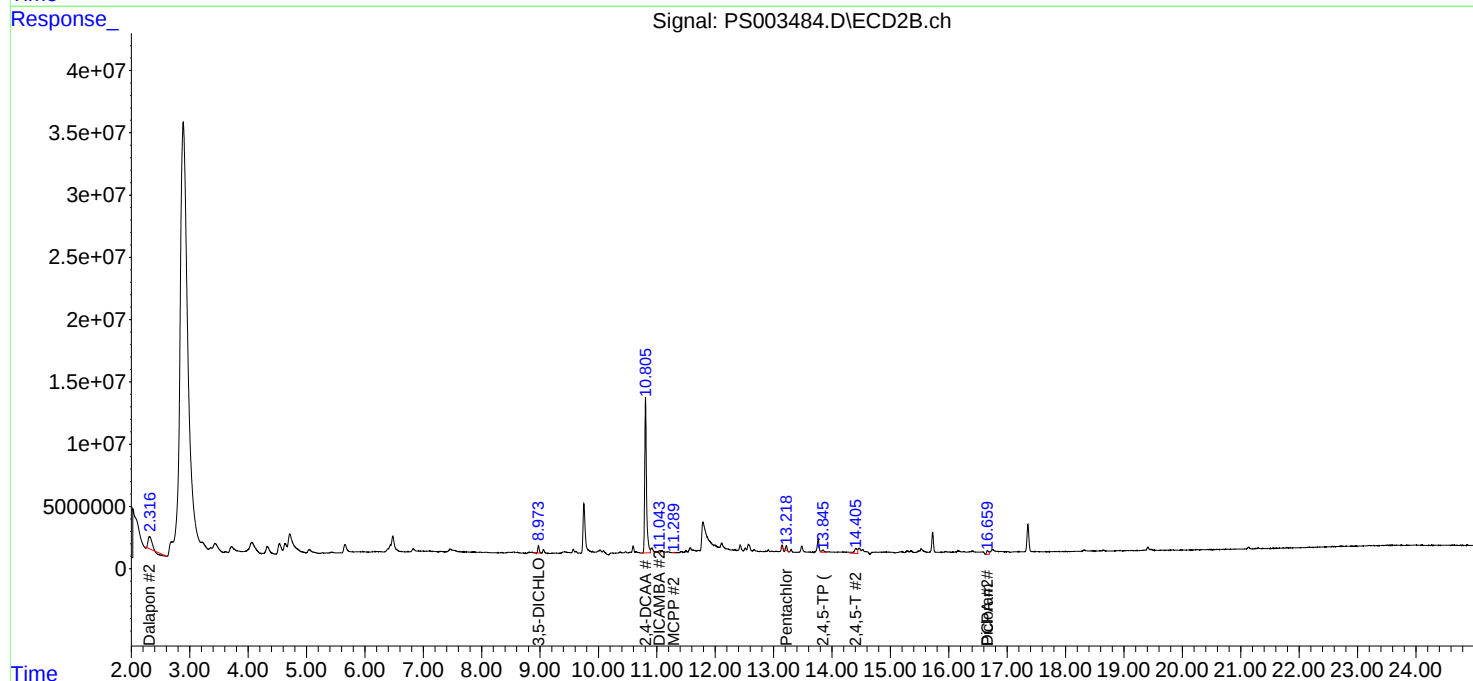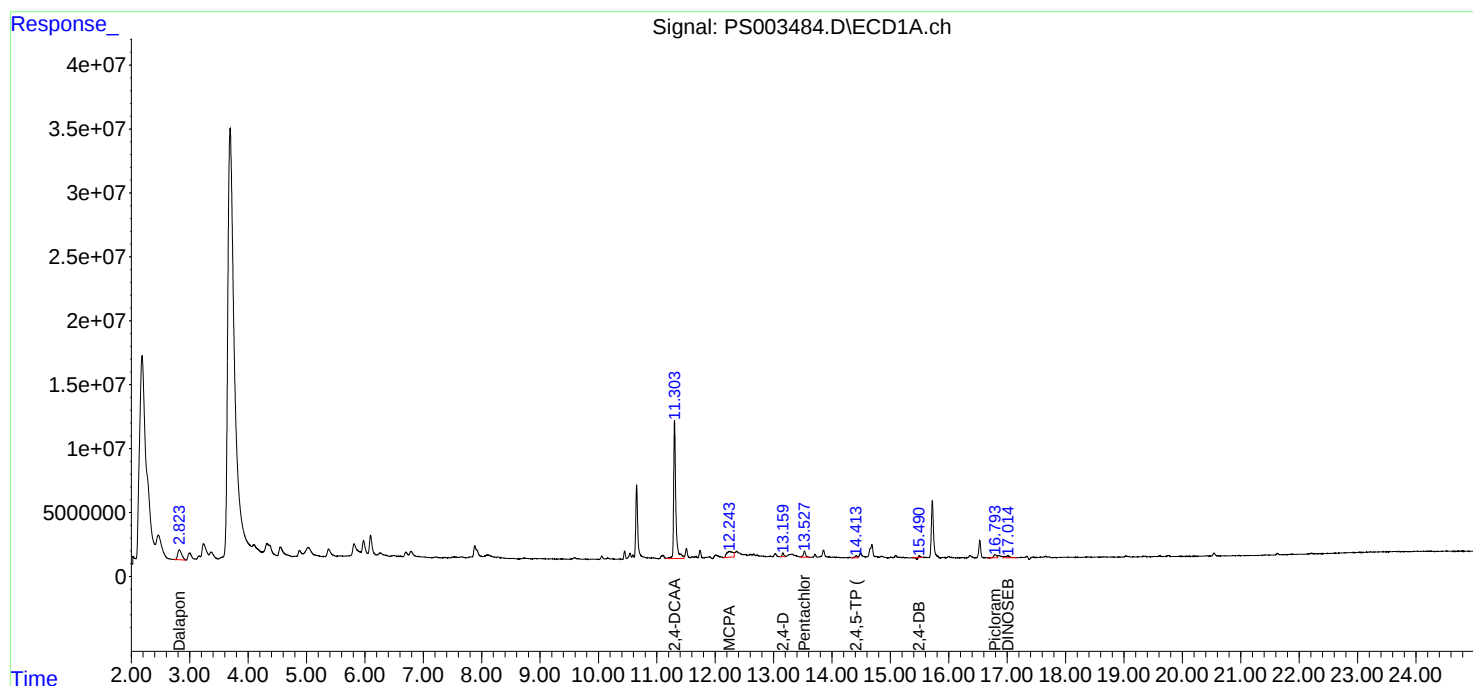


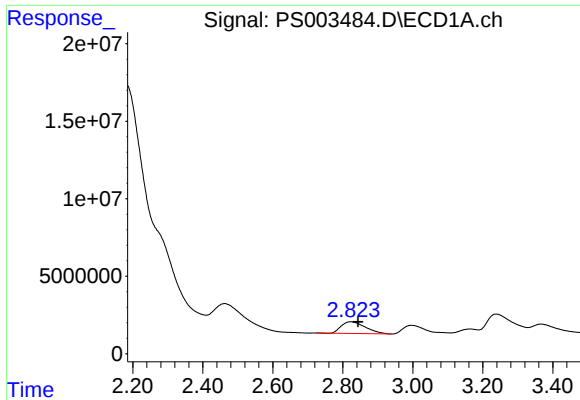

#1 Dalapon


R.T.: 2.822 min
Delta R.T.: -0.022 min
Response: 36459946
Conc: 56.10 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-6CD-D

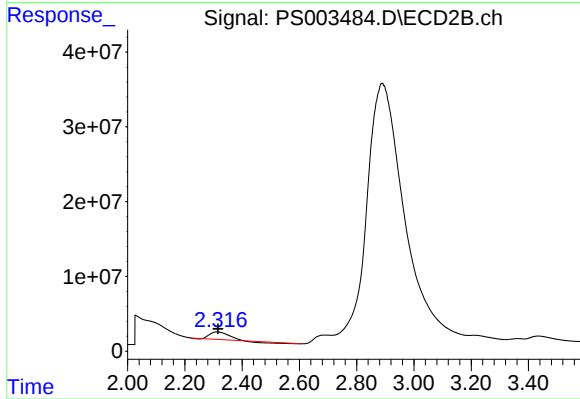


#1 Dalapon

R.T.: 2.313 min
Delta R.T.: -0.004 min
Response: 35411641
Conc: 55.93 ng/ml

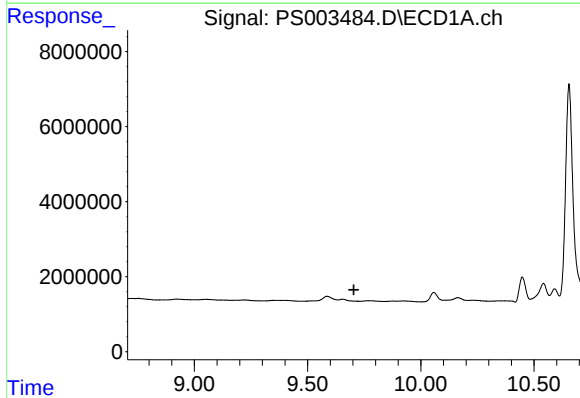


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.705 min
Response: 0
Conc: N.D.

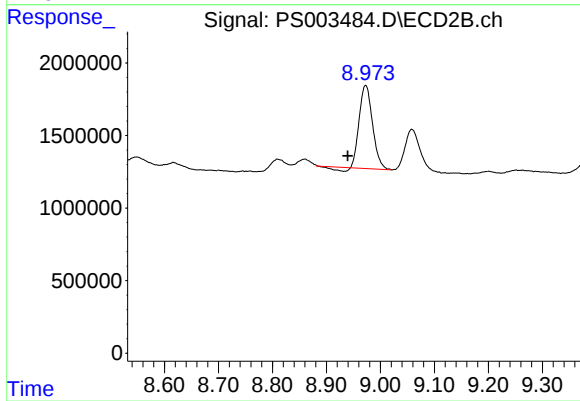

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.973 min
Delta R.T.: 0.033 min
Response: 9513733
Conc: 15.41 ng/ml

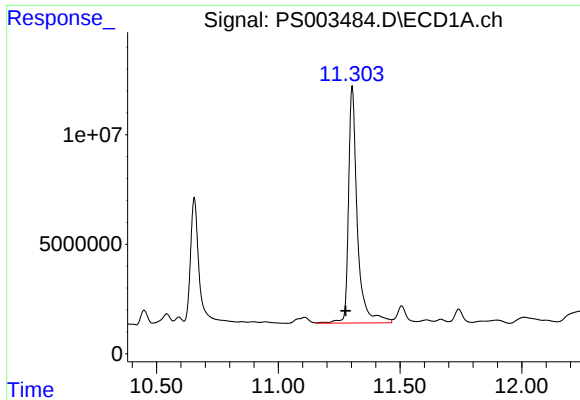

#4 2,4-DCAA


R.T.: 11.303 min
Delta R.T.: 0.026 min
Response: 273151504
Conc: 622.18 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-6CD-D

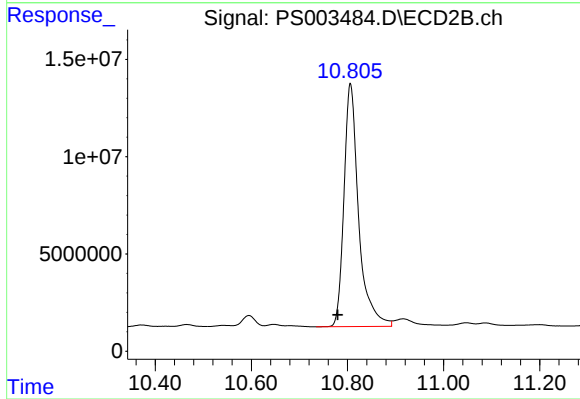


#4 2,4-DCAA

R.T.: 10.806 min
Delta R.T.: 0.027 min
Response: 263885549
Conc: 561.97 ng/ml

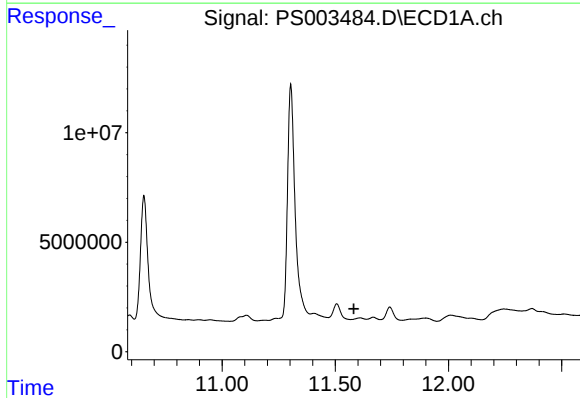


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.582 min
Response: 0
Conc: N.D.

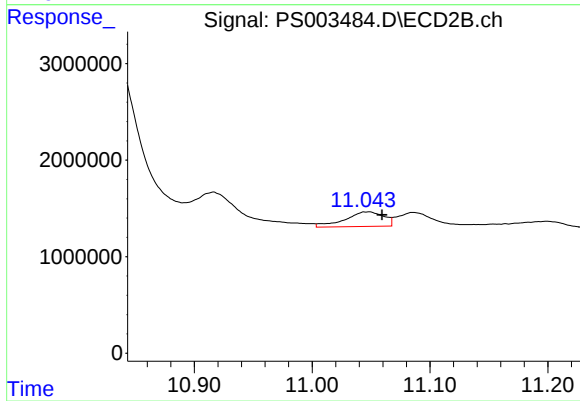

#5 DICAMBA


R.T.: 11.047 min
Delta R.T.: -0.012 min
Response: 3485648
Conc: 2.09 ng/ml

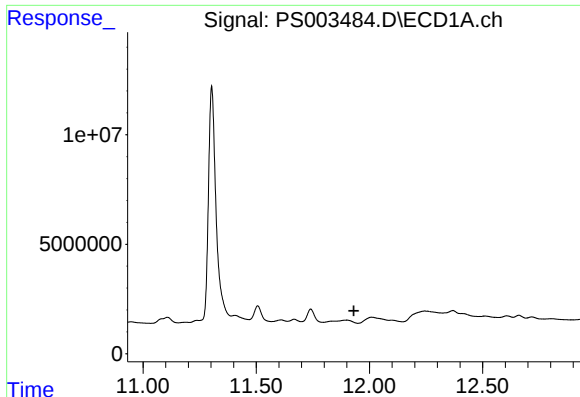

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 11.931 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-6CD-D

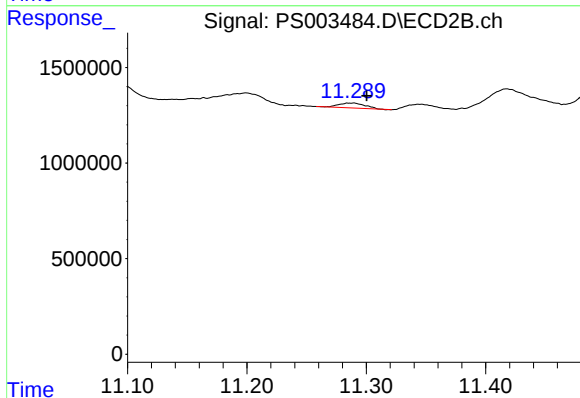


#6 MCPP

R.T.: 11.287 min
Delta R.T.: -0.014 min
Response: 398888
Conc: 0.34 ug/ml

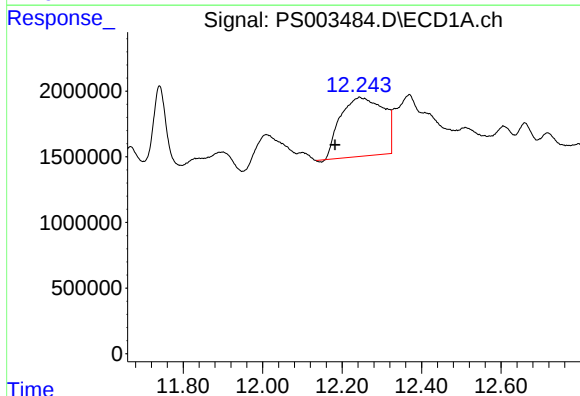


#7 MCPA

R.T.: 12.245 min
Delta R.T.: 0.062 min
Response: 33981535
Conc: 17.13 ug/ml

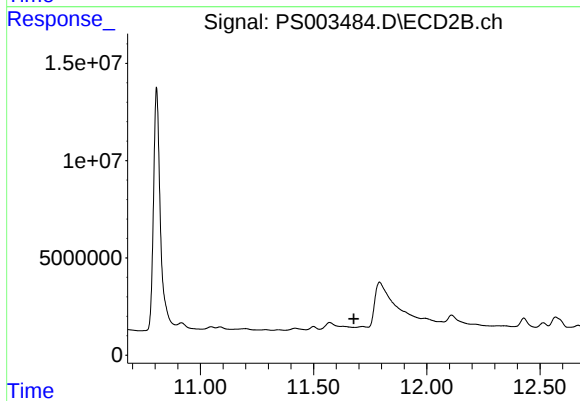

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 11.678 min
Response: 0
Conc: N.D.

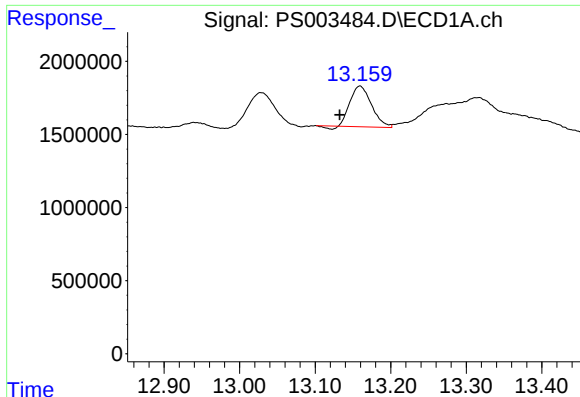

#9 2,4-D


R.T.: 13.159 min
Delta R.T.: 0.027 min
Response: 5378860
Conc: 11.60 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-6CD-D

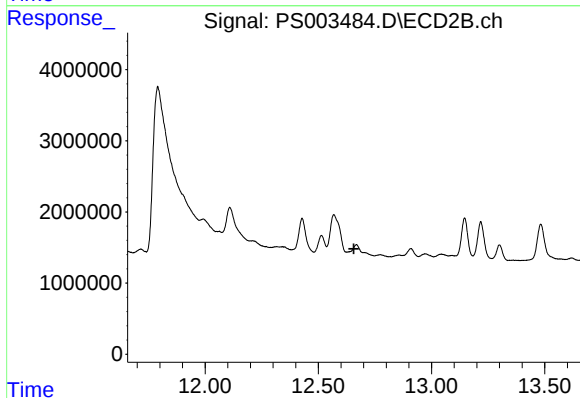


#9 2,4-D

R.T.: 12.668 min
Delta R.T.: 0.011 min
Response: -5493419
Conc: N.D.

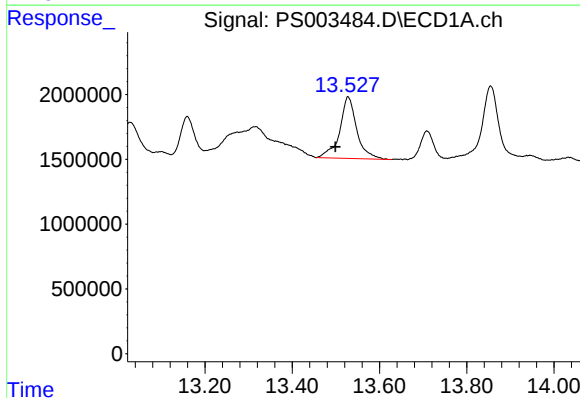


#10 Pentachlorophenol

R.T.: 13.528 min
Delta R.T.: 0.029 min
Response: 12921488
Conc: 1.83 ng/ml

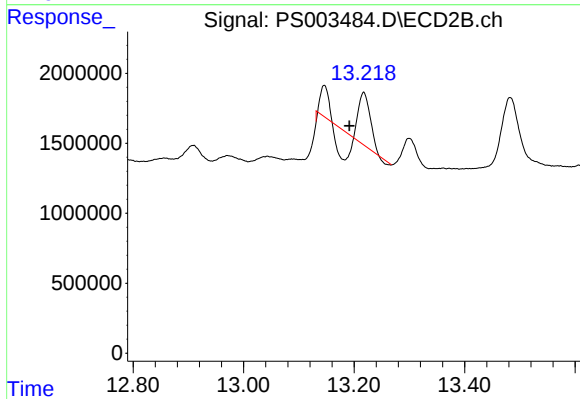

#10 Pentachlorophenol


R.T.: 13.217 min
Delta R.T.: 0.026 min
Response: 2645421
Conc: 0.40 ng/ml

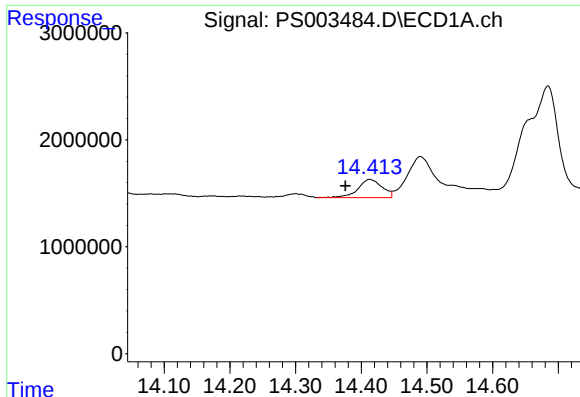

#11 2,4,5-TP (SILVEX)


R.T.: 14.414 min
Delta R.T.: 0.037 min
Response: 4326072
Conc: 1.61 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-6CD-D

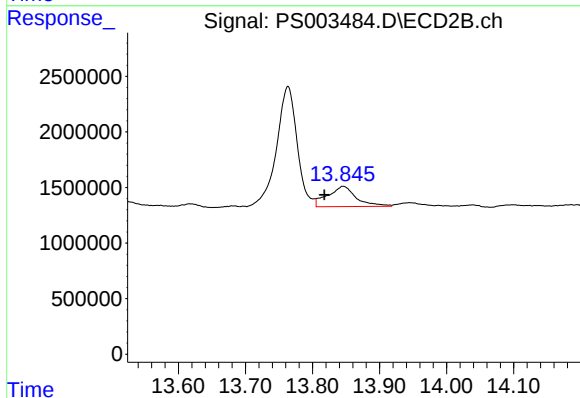


#11 2,4,5-TP (SILVEX)

R.T.: 13.846 min
Delta R.T.: 0.028 min
Response: 5368860
Conc: 2.11 ng/ml

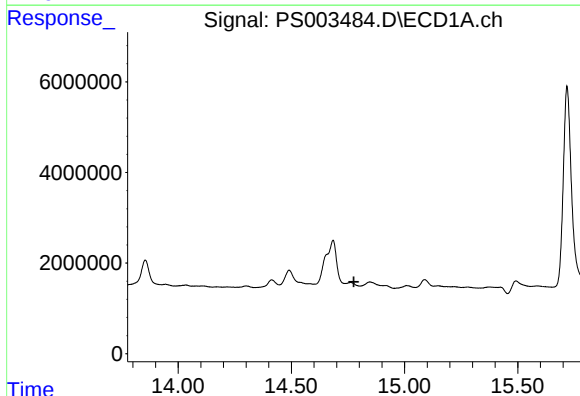


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 14.776 min
Response: 0
Conc: N.D.

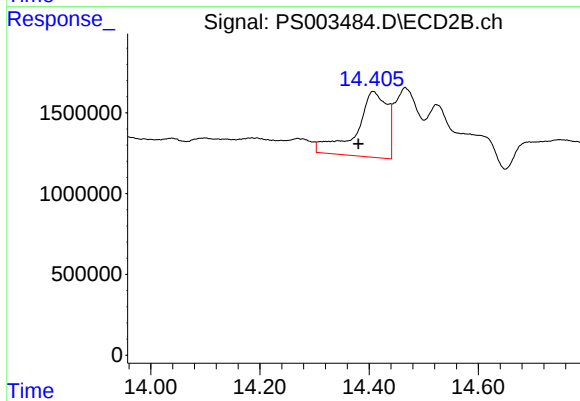

#12 2,4,5-T


R.T.: 14.408 min
Delta R.T.: 0.028 min
Response: 16222043
Conc: 8.04 ng/ml

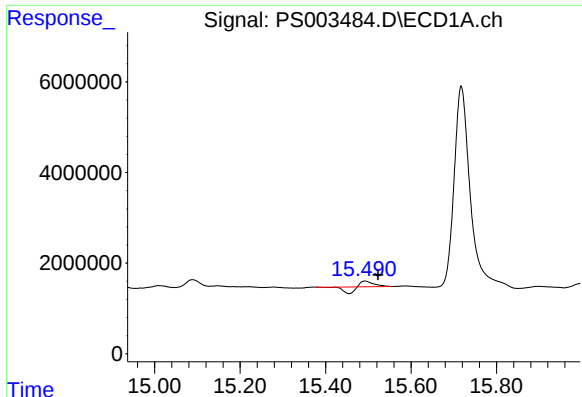

#13 2,4-DB


R.T.: 15.493 min
Delta R.T.: -0.030 min
Response: 247742
Conc: 1.05 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-6CD-D

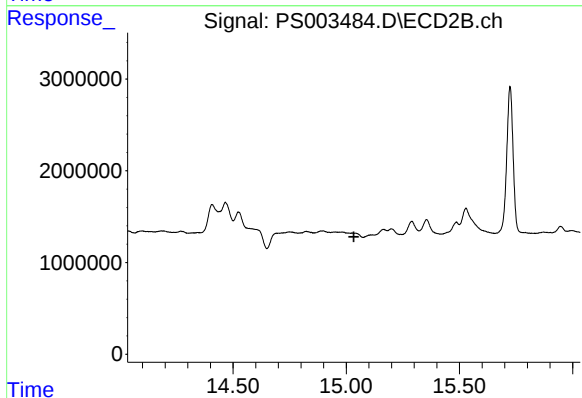


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 15.033 min
Response: 0
Conc: N.D.

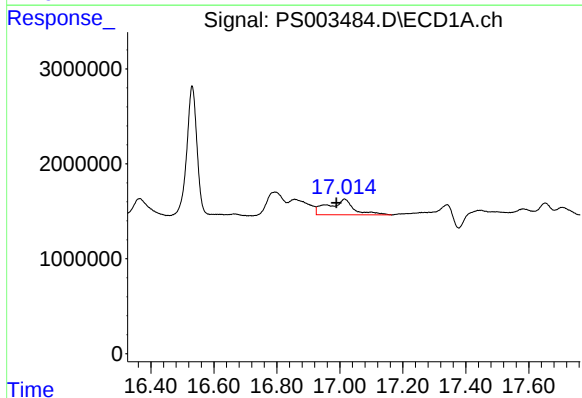


#14 DINOSEB

R.T.: 17.015 min
Delta R.T.: 0.026 min
Response: 9420974
Conc: 4.20 ng/ml

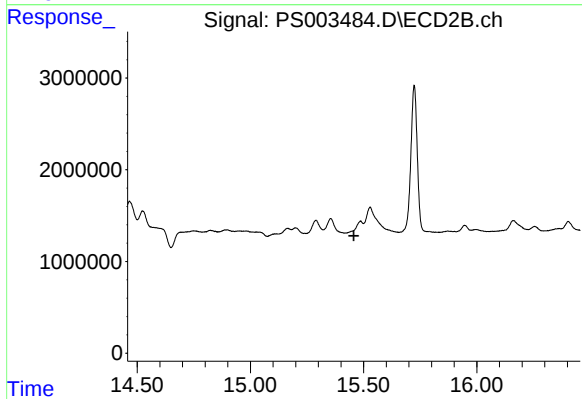

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 15.457 min
Response: 0
Conc: N.D.

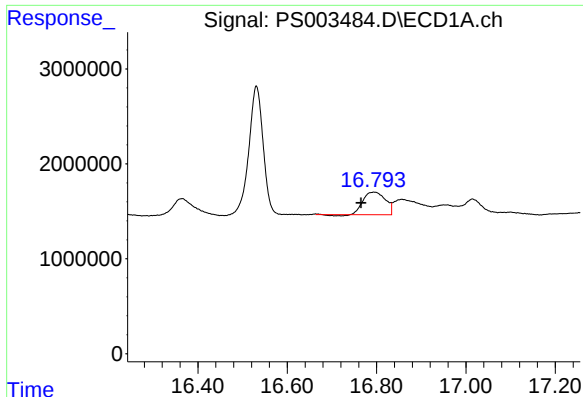

#15 Picloram


R.T.: 16.793 min
Delta R.T.: 0.028 min
Response: 8146878
Conc: 3.31 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-6CD-D

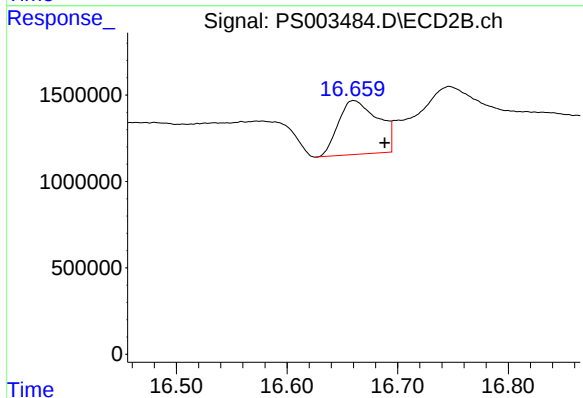


#15 Picloram

R.T.: 16.662 min
Delta R.T.: -0.027 min
Response: 7763419
Conc: 3.06 ng/ml

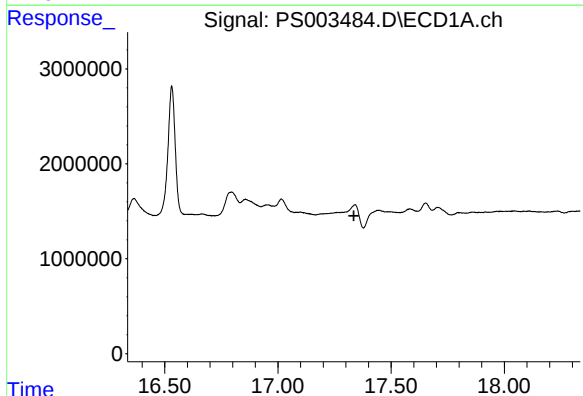

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.335 min
Response: 0
Conc: N.D.

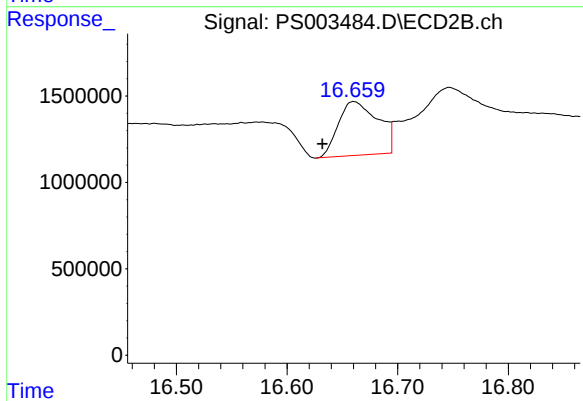

#16 DCPA

R.T.: 16.662 min
Delta R.T.: 0.030 min
Response: 7763419
Conc: 2.50 ng/ml