

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030819\
 Data File : PS003486.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Mar 2019 23:58
 Operator : EI\SJ
 Sample : K1757-16
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-6AB-D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 00:34:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.313	10.815	264.8E6	254.3E6	603.195	541.625
Target Compounds							
1) T	Dalapon	2.833	2.324	44212568	82227869	68.025	129.864 #
2) T	3,5-DICHL...	0.000	8.981	0	6503604	N.D.	10.533 #
5) T	DICAMBA	11.516	11.055	16773167	3852609	9.515	2.306 #
6) T	MCP	0.000	11.298	0	320392	N.D.	0.271 #
8) T	DICHLORPROP	0.000	12.123	0	25614340	N.D.	61.984 #
10) T	Pentachlo...	0.000	13.155	0	5782510	N.D.	0.878 #
11) T	2,4,5-TP ...	0.000	13.825	0	1531145	N.D.	0.601 #
12) T	2,4,5-T	0.000	14.416	0	10036159	N.D.	4.976 #
13) T	2,4-DB	15.503	15.024	11082569	1267736	46.802	4.965 #
15) T	Picloram	16.803	16.680	9323655	6446598	3.788	2.540 #
16) T	DCPA	0.000	16.680	0	6446598	N.D.	2.073 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030819\
Data File : PS003486.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Mar 2019 23:58
Operator : EI\SJ
Sample : K1757-16
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-6AB-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 00:34:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

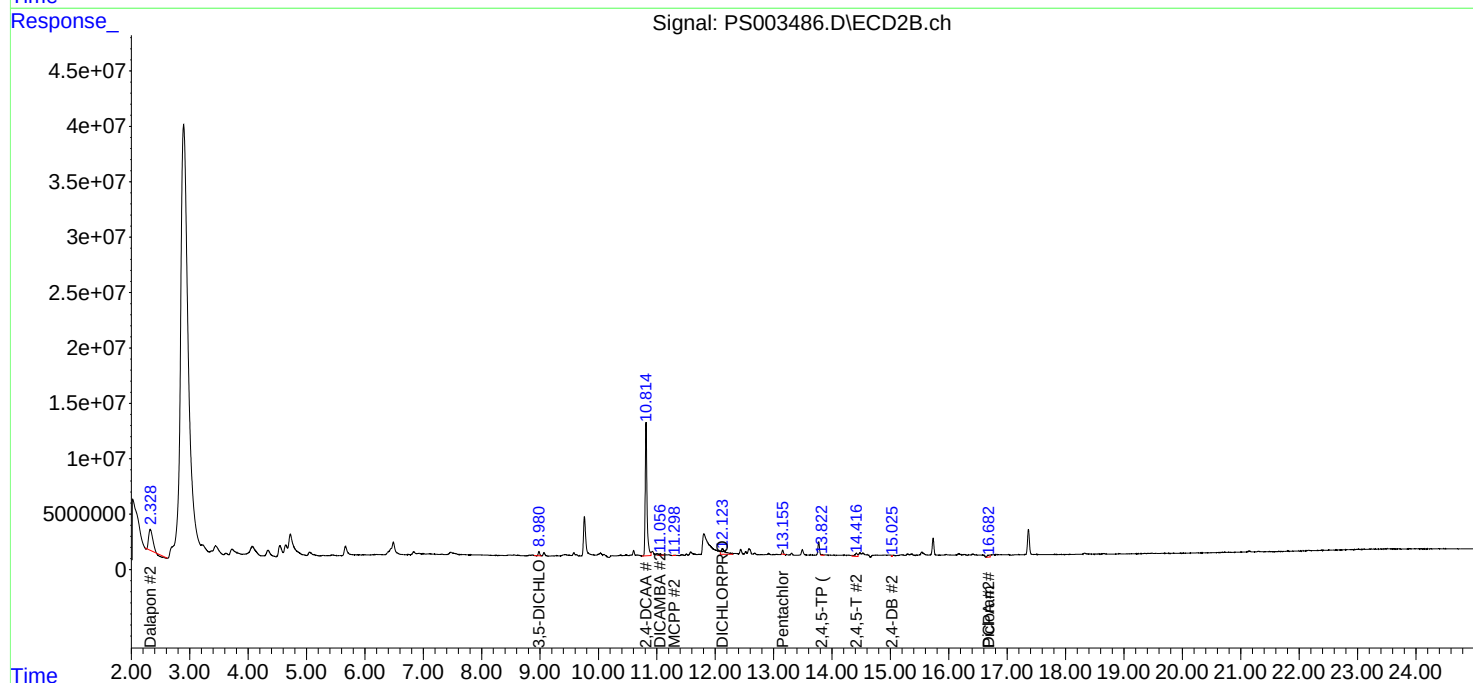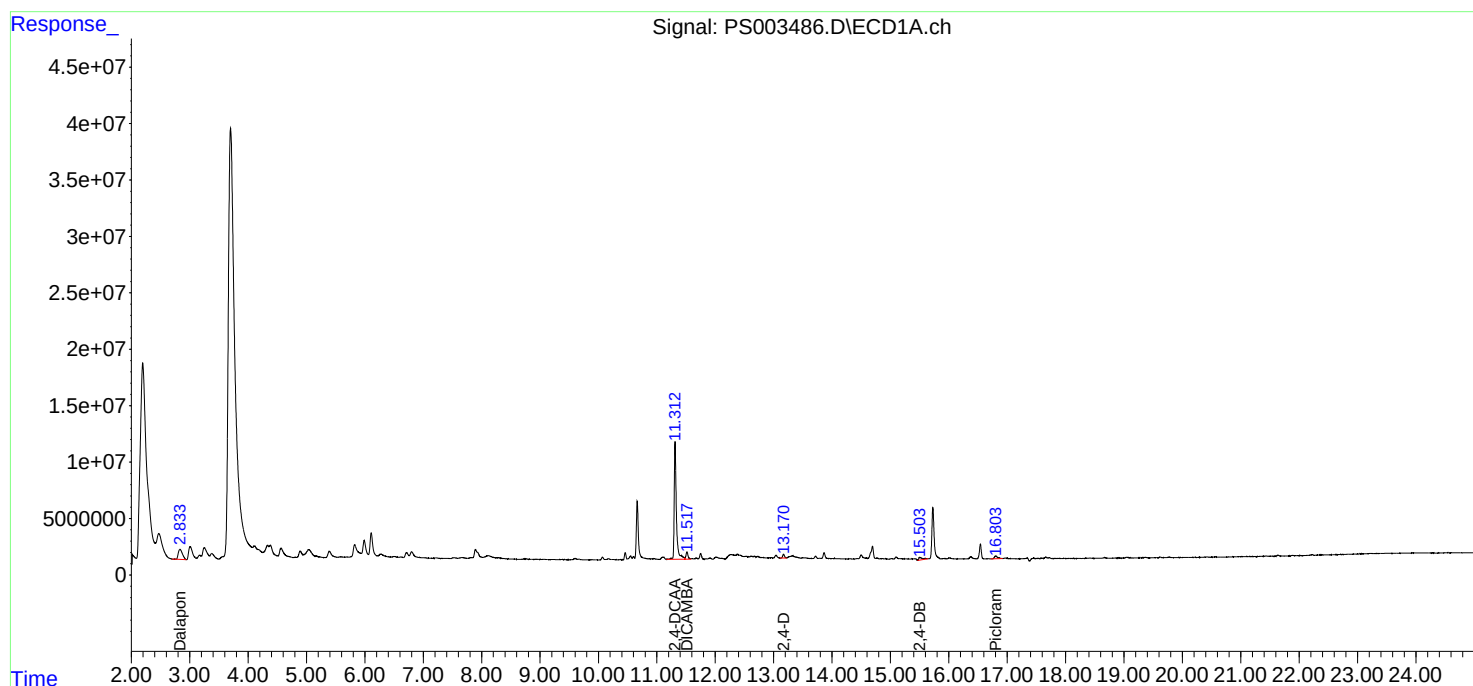


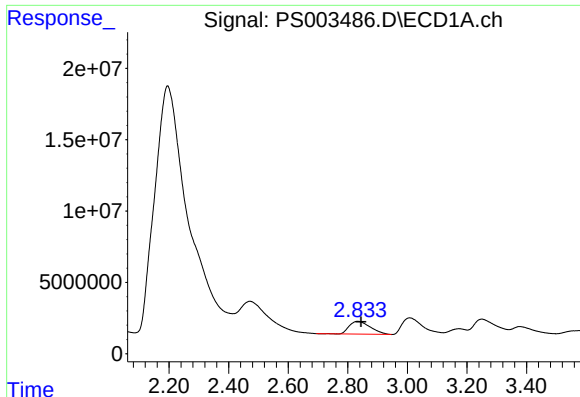

#1 Dalapon


R.T.: 2.833 min
Delta R.T.: -0.011 min
Response: 44212568
Conc: 68.03 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-6AB-D

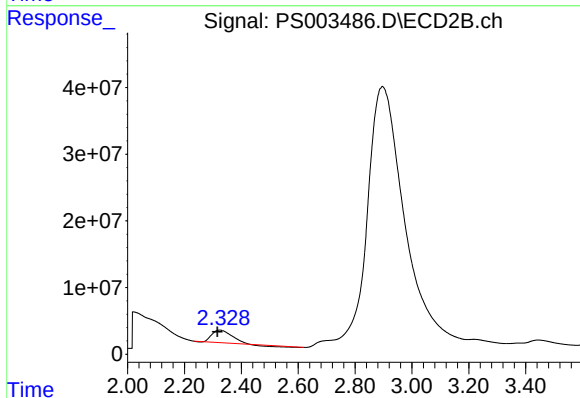


#1 Dalapon

R.T.: 2.324 min
Delta R.T.: 0.008 min
Response: 82227869
Conc: 129.86 ng/ml

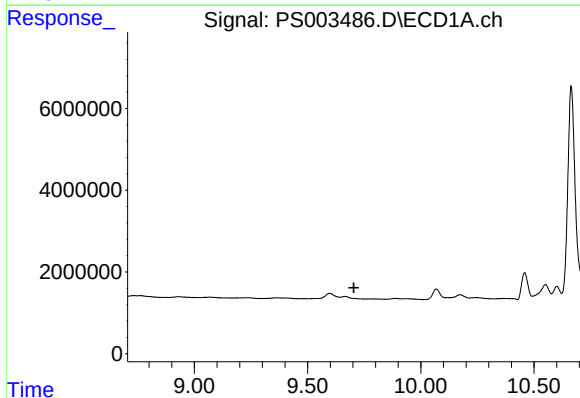


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.705 min
Response: 0
Conc: N.D.

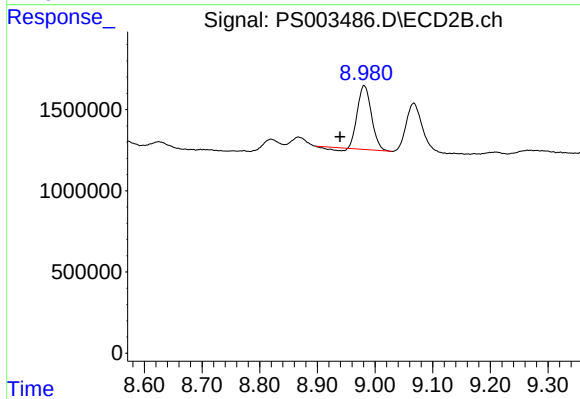

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.981 min
Delta R.T.: 0.042 min
Response: 6503604
Conc: 10.53 ng/ml

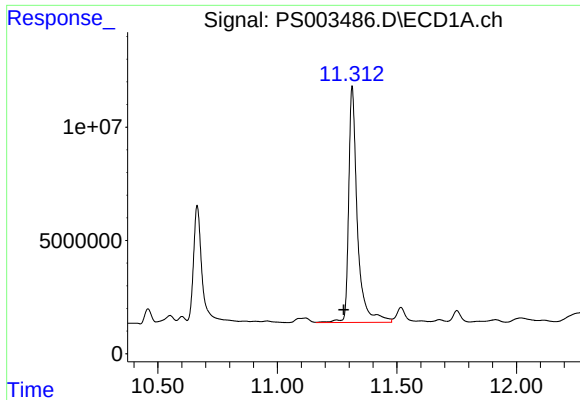

#4 2,4-DCAA


R.T.: 11.313 min
Delta R.T.: 0.035 min
Response: 264817492
Conc: 603.20 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-6AB-D

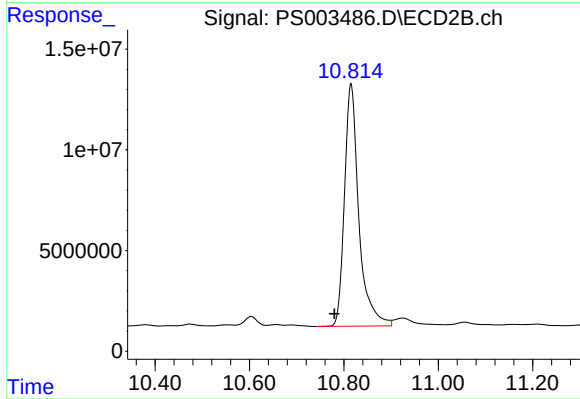


#4 2,4-DCAA

R.T.: 10.815 min
Delta R.T.: 0.035 min
Response: 254330488
Conc: 541.63 ng/ml

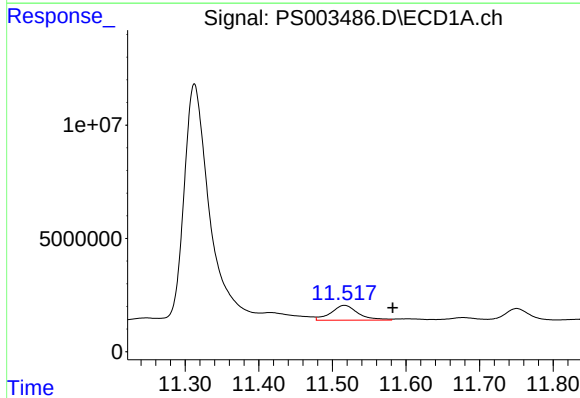


#5 DICAMBA

R.T.: 11.516 min
Delta R.T.: -0.066 min
Response: 16773167
Conc: 9.52 ng/ml

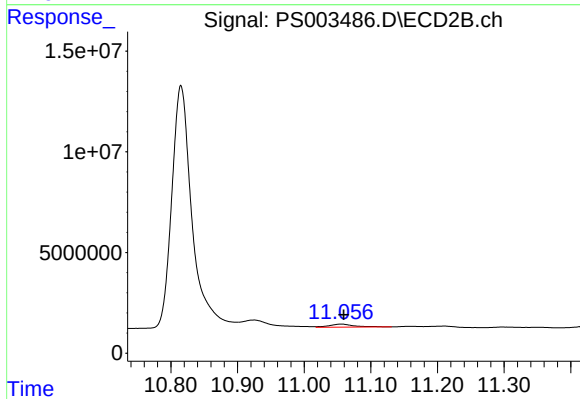

#5 DICAMBA


R.T.: 11.055 min
Delta R.T.: -0.004 min
Response: 3852609
Conc: 2.31 ng/ml

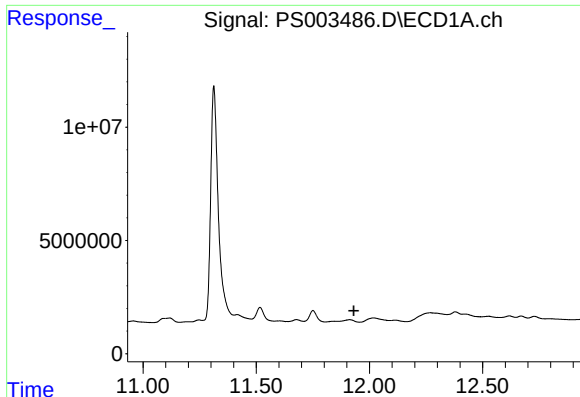

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.931 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-6AB-D

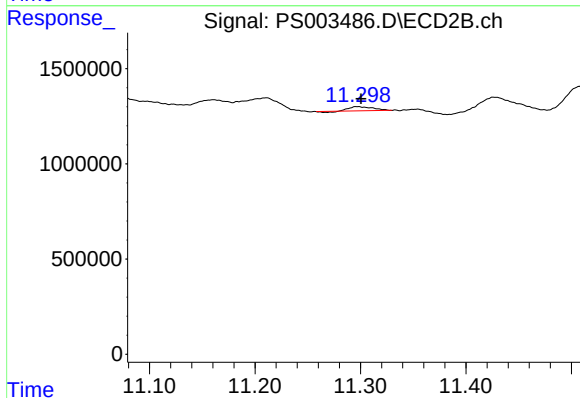


#6 MCP

R.T.: 11.298 min
Delta R.T.: -0.003 min
Response: 320392
Conc: 0.27 ug/ml

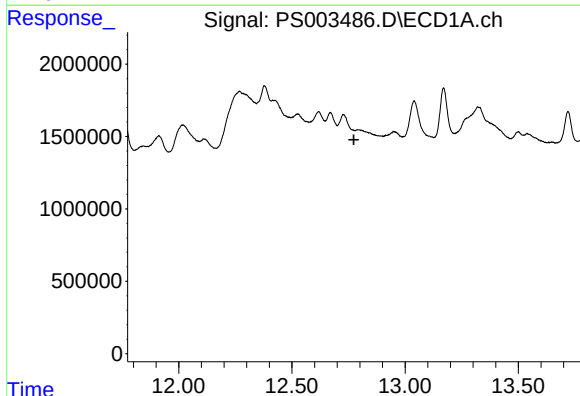


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 12.773 min
Response: 0
Conc: N.D.

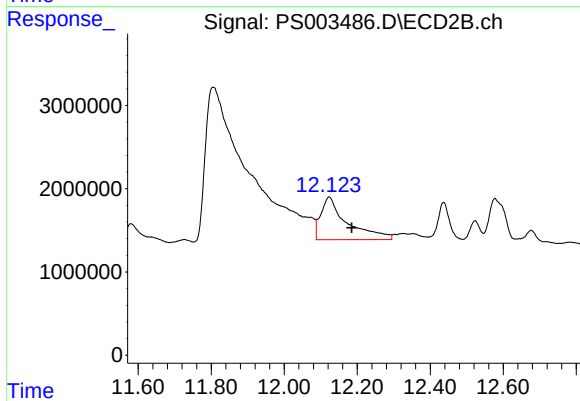

#8 DICHLORPROP


R.T.: 12.123 min
Delta R.T.: -0.062 min
Response: 25614340
Conc: 61.98 ng/ml

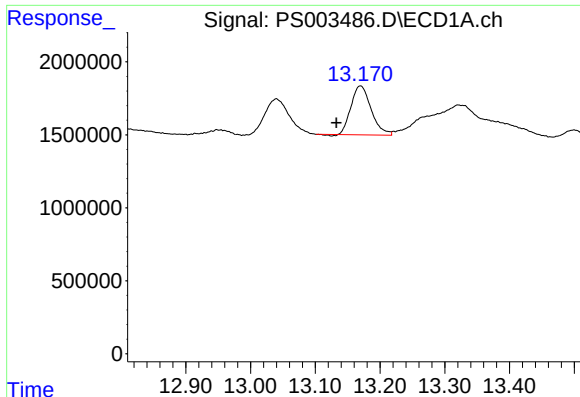

#9 2,4-D


R.T.: 13.170 min
Delta R.T.: 0.037 min
Response: 7205935
Conc: 15.54 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-6AB-D

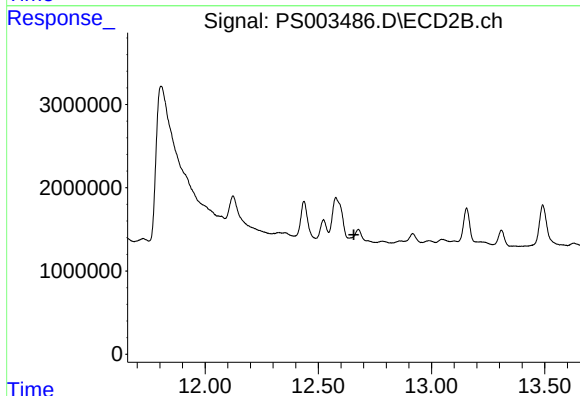


#9 2,4-D

R.T.: 12.676 min
Delta R.T.: 0.019 min
Response: -11842802
Conc: N.D.

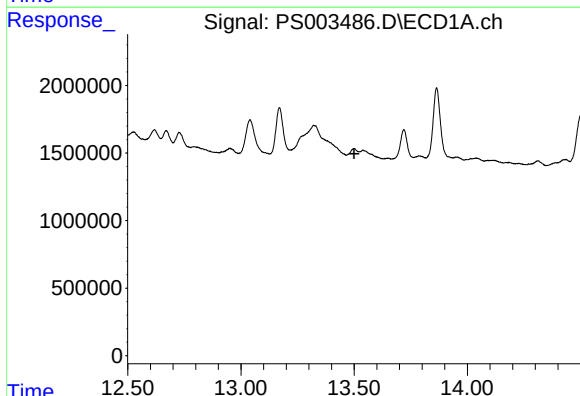


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.499 min
Response: 0
Conc: N.D.

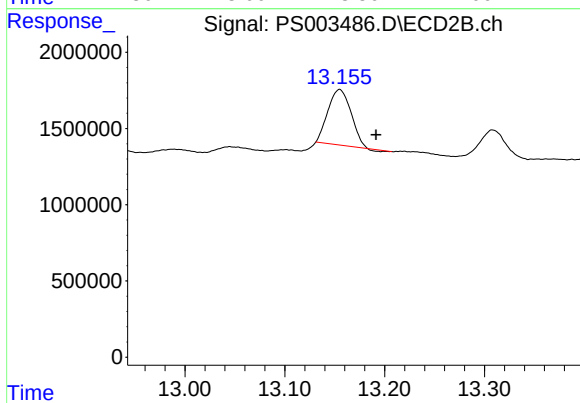

#10 Pentachlorophenol


R.T.: 13.155 min
Delta R.T.: -0.037 min
Response: 5782510
Conc: 0.88 ng/ml

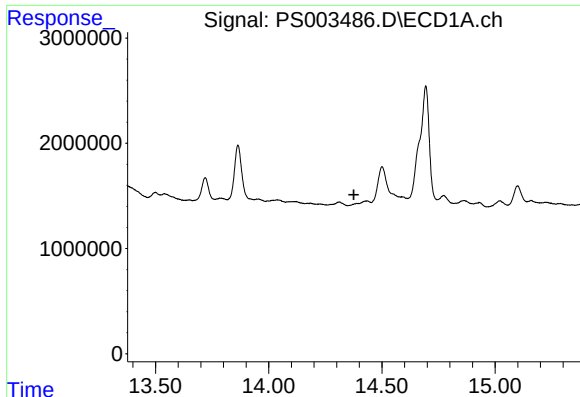

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-6AB-D

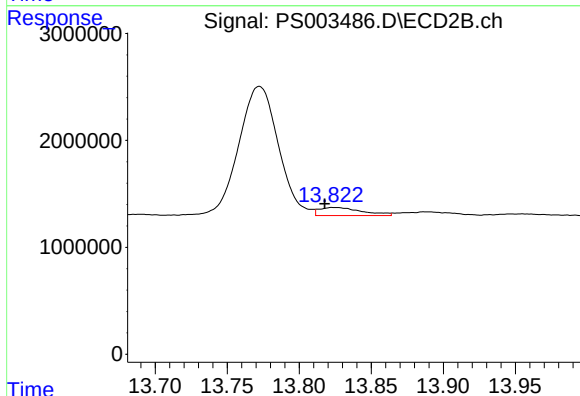


#11 2,4,5-TP (SILVEX)

R.T.: 13.825 min
Delta R.T.: 0.007 min
Response: 1531145
Conc: 0.60 ng/ml

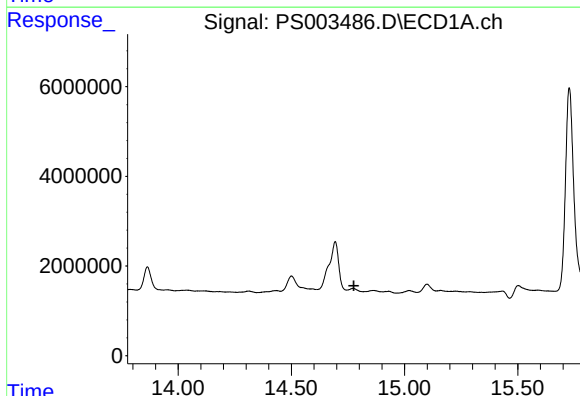


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

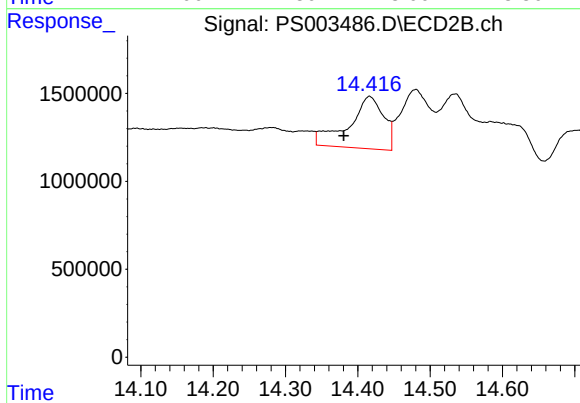

#12 2,4,5-T


R.T.: 14.416 min
Delta R.T.: 0.036 min
Response: 10036159
Conc: 4.98 ng/ml

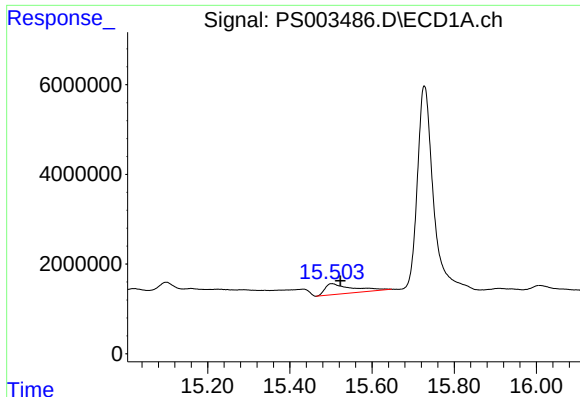

#13 2,4-DB


R.T.: 15.503 min
Delta R.T.: -0.020 min
Response: 11082569
Conc: 46.80 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-6AB-D

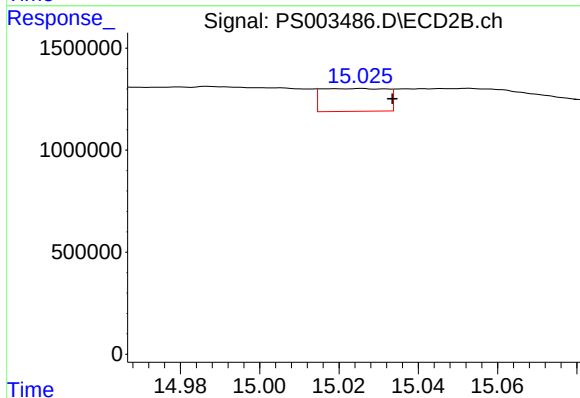


#13 2,4-DB

R.T.: 15.024 min
Delta R.T.: -0.009 min
Response: 1267736
Conc: 4.96 ng/ml

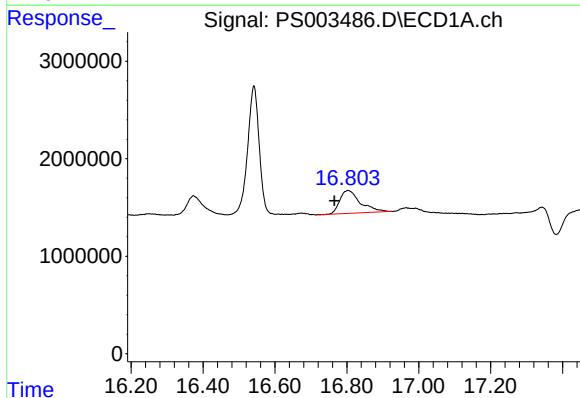


#15 Picloram

R.T.: 16.803 min
Delta R.T.: 0.038 min
Response: 9323655
Conc: 3.79 ng/ml

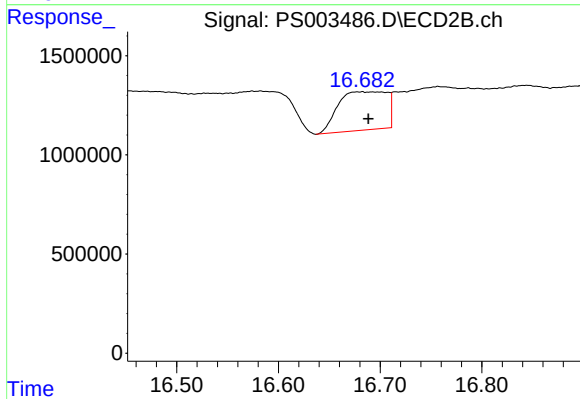

#15 Picloram


R.T.: 16.680 min
Delta R.T.: -0.009 min
Response: 6446598
Conc: 2.54 ng/ml

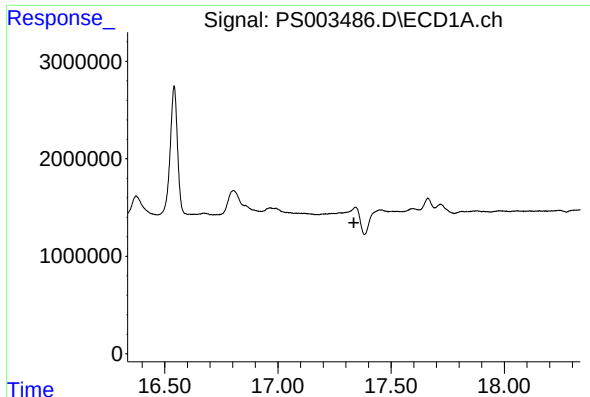

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.335 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-6AB-D

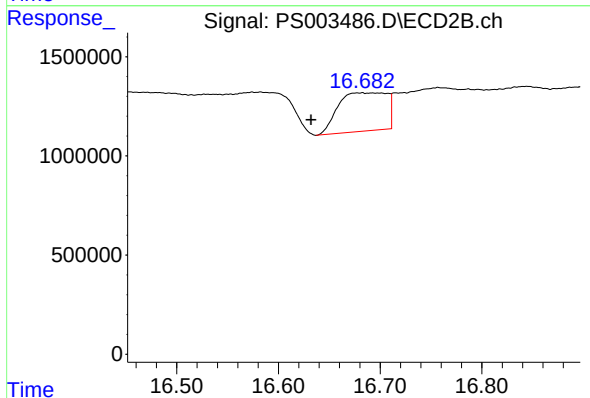

#16 DCPA

R.T.: 16.680 min
Delta R.T.: 0.048 min
Response: 6446598
Conc: 2.07 ng/ml