

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030819\
 Data File : PS003488.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Mar 2019 01:00
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 02:41:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.310	10.810	224.4E6	211.0E6	511.134	449.417
Target Compounds							
3) T	4-Nitroph...	0.000	9.989	0	147363	N.D.	0.655 #
7) T	MCPA	0.000	11.701	0	296784	N.D.	0.172 #
10) T	Pentachlo...	0.000	13.228	0	937743	N.D.	0.142 #
11) T	2,4,5-TP ...	0.000	13.833	0	484033	N.D.	0.190 #
13) T	2,4-DB	0.000	14.989	0	127737	N.D.	0.500 #
14) T	DINOSEB	0.000	15.443	0	38688	N.D.	0.022 #
15) T	Picloram	0.000	16.663	0	608271	N.D.	0.240 #
16) T	DCPA	0.000	16.663	0	608271	N.D.	0.196 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030819\
Data File : PS003488.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Mar 2019 01:00
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 02:41:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

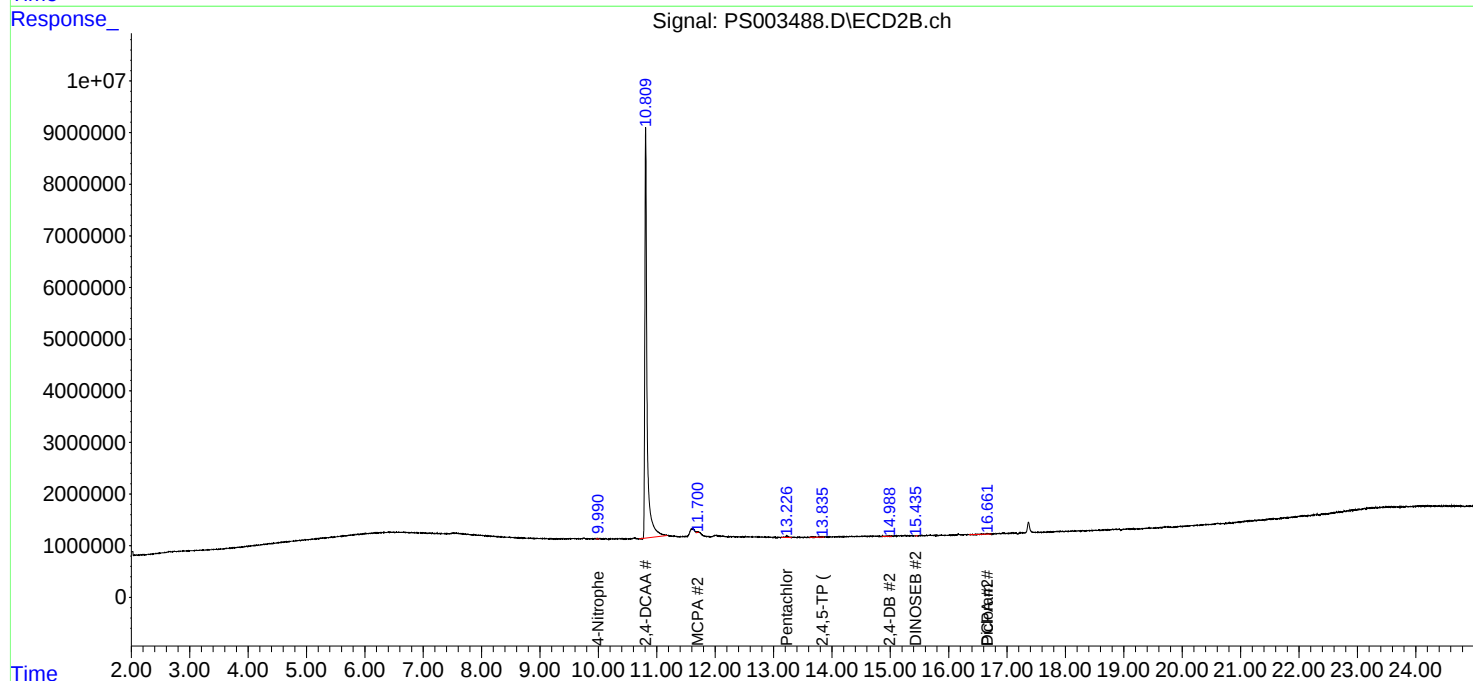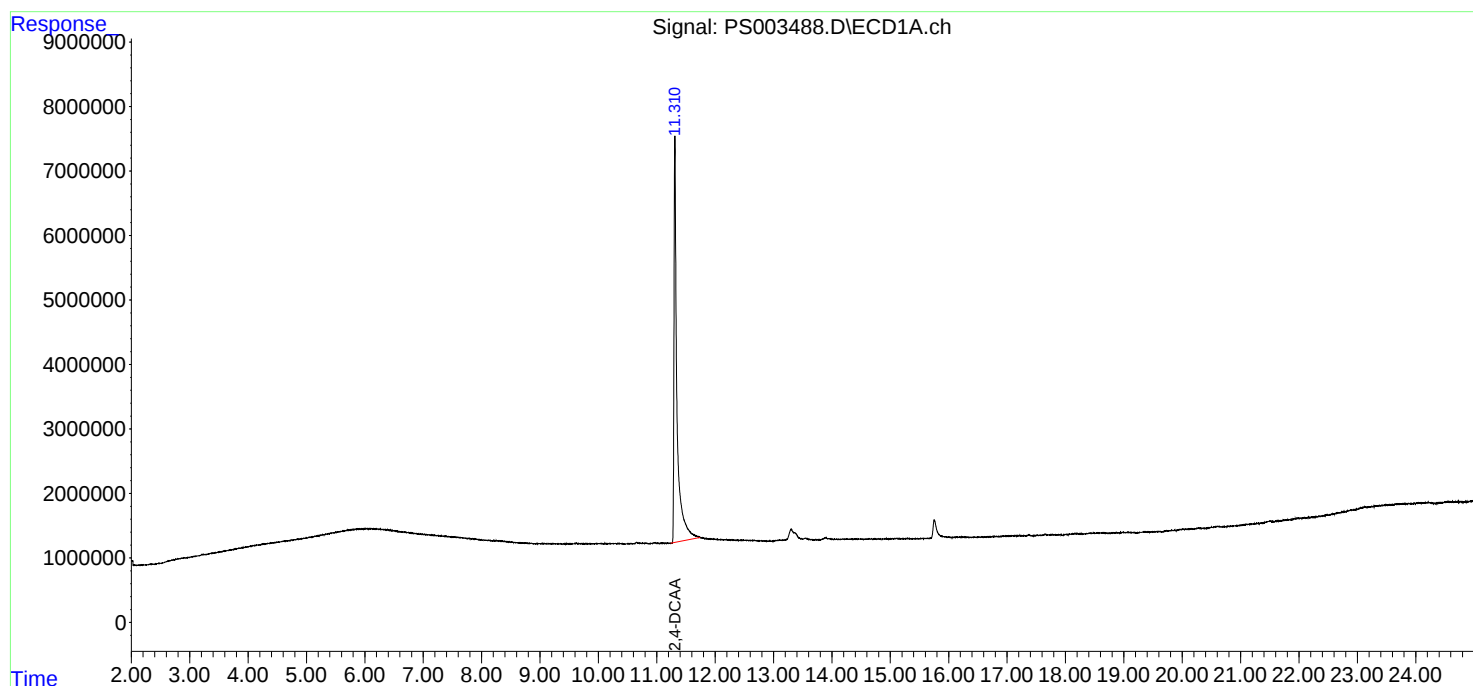


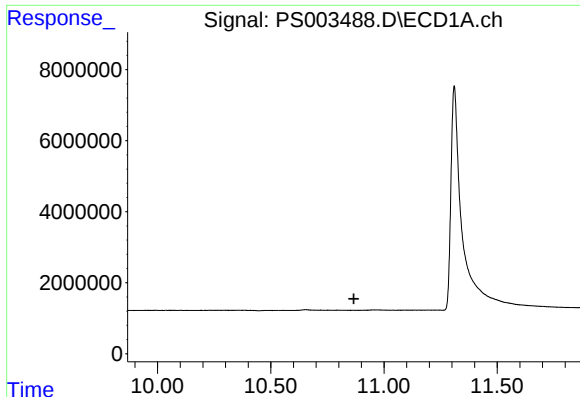

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

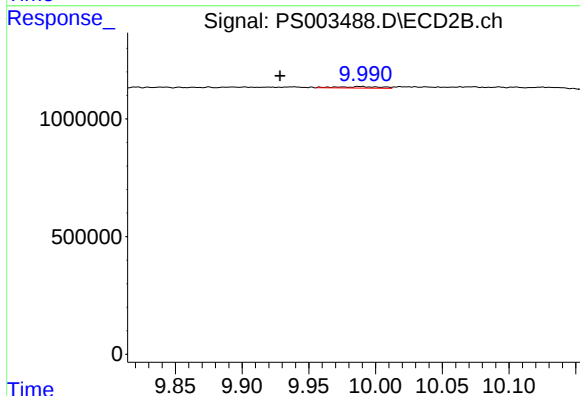


#3 4-Nitrophenol

R.T.: 9.989 min
Delta R.T.: 0.060 min
Response: 147363
Conc: 0.66 ng/ml

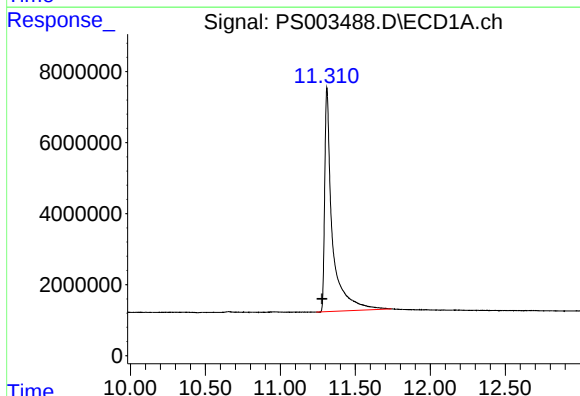


#4 2,4-DCAA

R.T.: 11.310 min
Delta R.T.: 0.033 min
Response: 224400274
Conc: 511.13 ng/ml

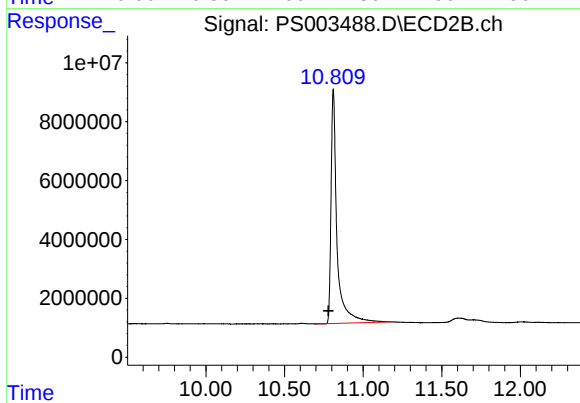

#4 2,4-DCAA


R.T.: 10.810 min
Delta R.T.: 0.030 min
Response: 211032582
Conc: 449.42 ng/ml

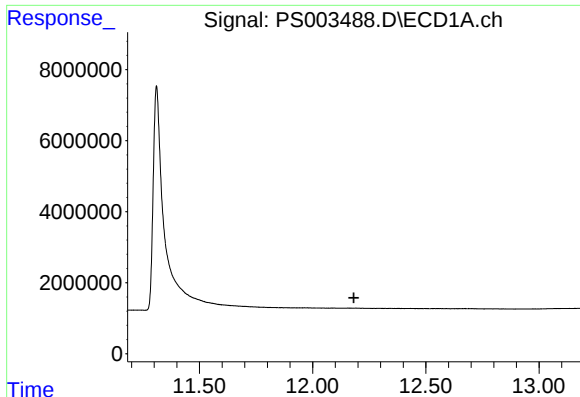

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.182 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

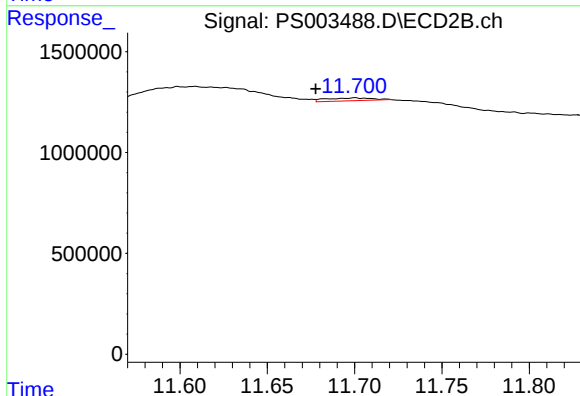


#7 MCPA

R.T.: 11.701 min
Delta R.T.: 0.023 min
Response: 296784
Conc: 0.17 ug/ml

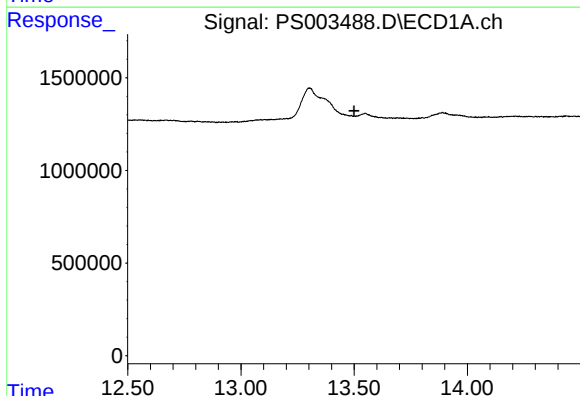


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 13.499 min
Response: 0
Conc: N.D.

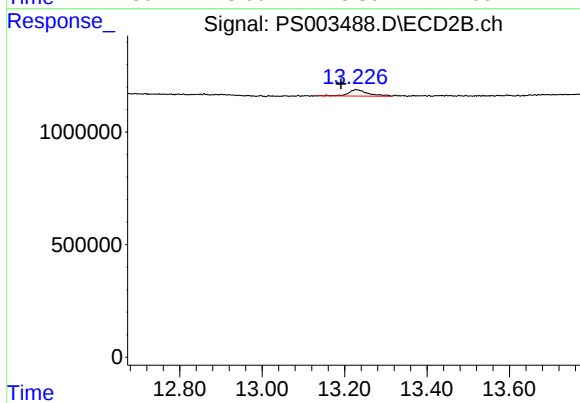

#10 Pentachlorophenol


R.T.: 13.228 min
Delta R.T.: 0.037 min
Response: 937743
Conc: 0.14 ng/ml

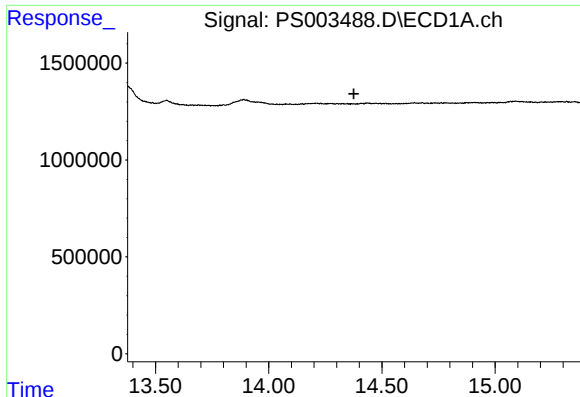

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

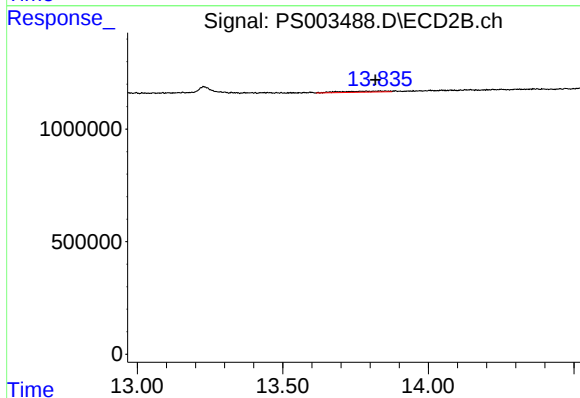


#11 2,4,5-TP (SILVEX)

R.T.: 13.833 min
Delta R.T.: 0.015 min
Response: 484033
Conc: 0.19 ng/ml

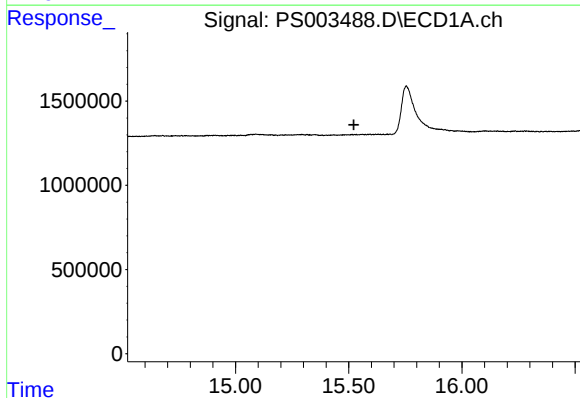


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.523 min
Response: 0
Conc: N.D.

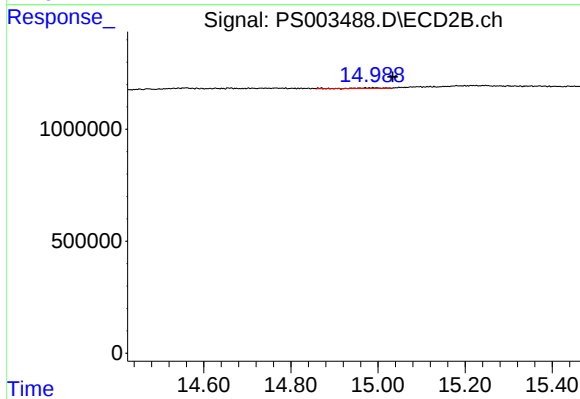

#13 2,4-DB


R.T.: 14.989 min
Delta R.T.: -0.044 min
Response: 127737
Conc: 0.50 ng/ml

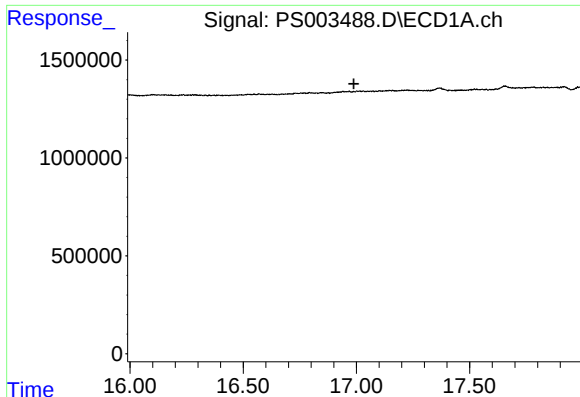

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 16.989 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

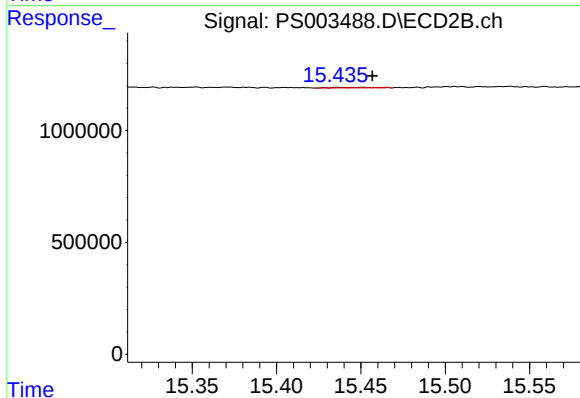


#14 DINOSEB

R.T.: 15.443 min
Delta R.T.: -0.013 min
Response: 38688
Conc: 0.02 ng/ml

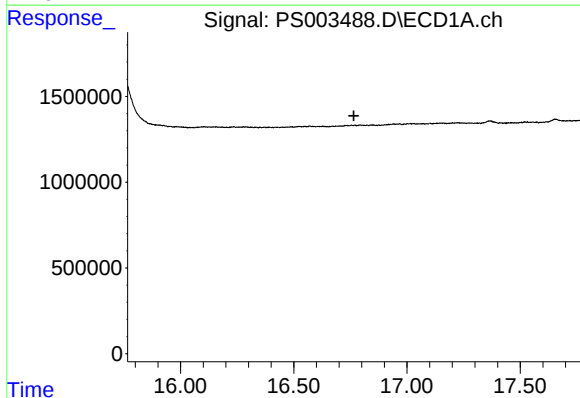


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.765 min
Response: 0
Conc: N.D.

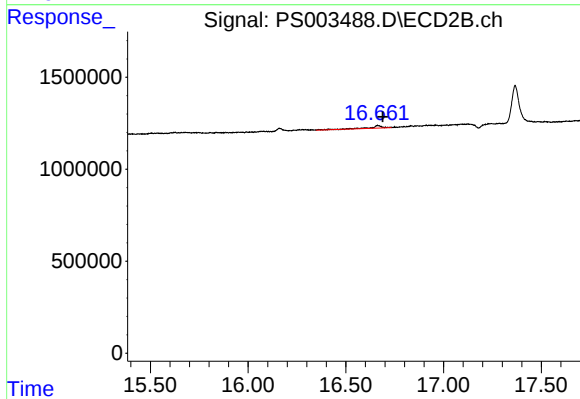

#15 Picloram


R.T.: 16.663 min
Delta R.T.: -0.025 min
Response: 608271
Conc: 0.24 ng/ml

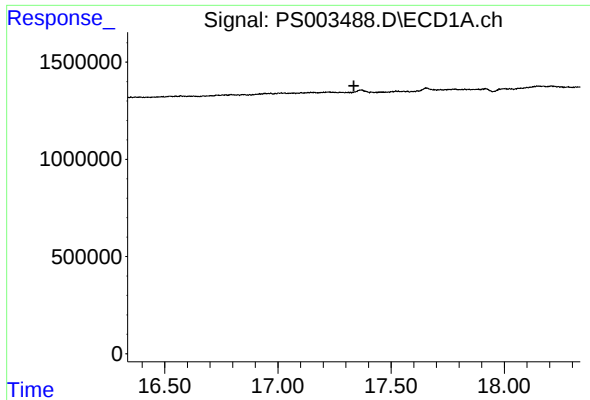

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.335 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

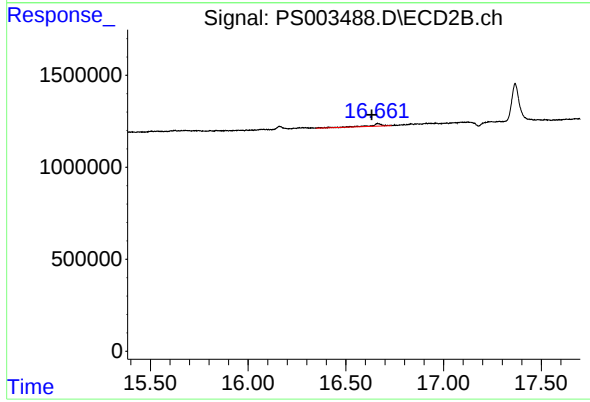

#16 DCPA

R.T.: 16.663 min
Delta R.T.: 0.032 min
Response: 608271
Conc: 0.20 ng/ml