

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS030821\  
 Data File : PS014175.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 08 Mar 2021 08:16  
 Operator : DD\AJ  
 Sample : HEXANE  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 09 03:34:53 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS030521.M  
 Quant Title : 8080.M  
 QLast Update : Sat Mar 06 03:17:26 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

#### System Monitoring Compounds

| Target Compounds |          |       |        |   |        |      |
|------------------|----------|-------|--------|---|--------|------|
| 15) T            | Picloram | 0.000 | 11.010 | 0 | 39411  | <MDL |
| 16) T            | DCPA     | 0.000 | 10.919 | 0 | 137062 | <MDL |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS030821\  
Data File : PS014175.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 08 Mar 2021 08:16  
Operator : DD\AJ  
Sample : HEXANE  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Mar 09 03:34:53 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS030521.M  
Quant Title : 8080.M  
QLast Update : Sat Mar 06 03:17:26 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

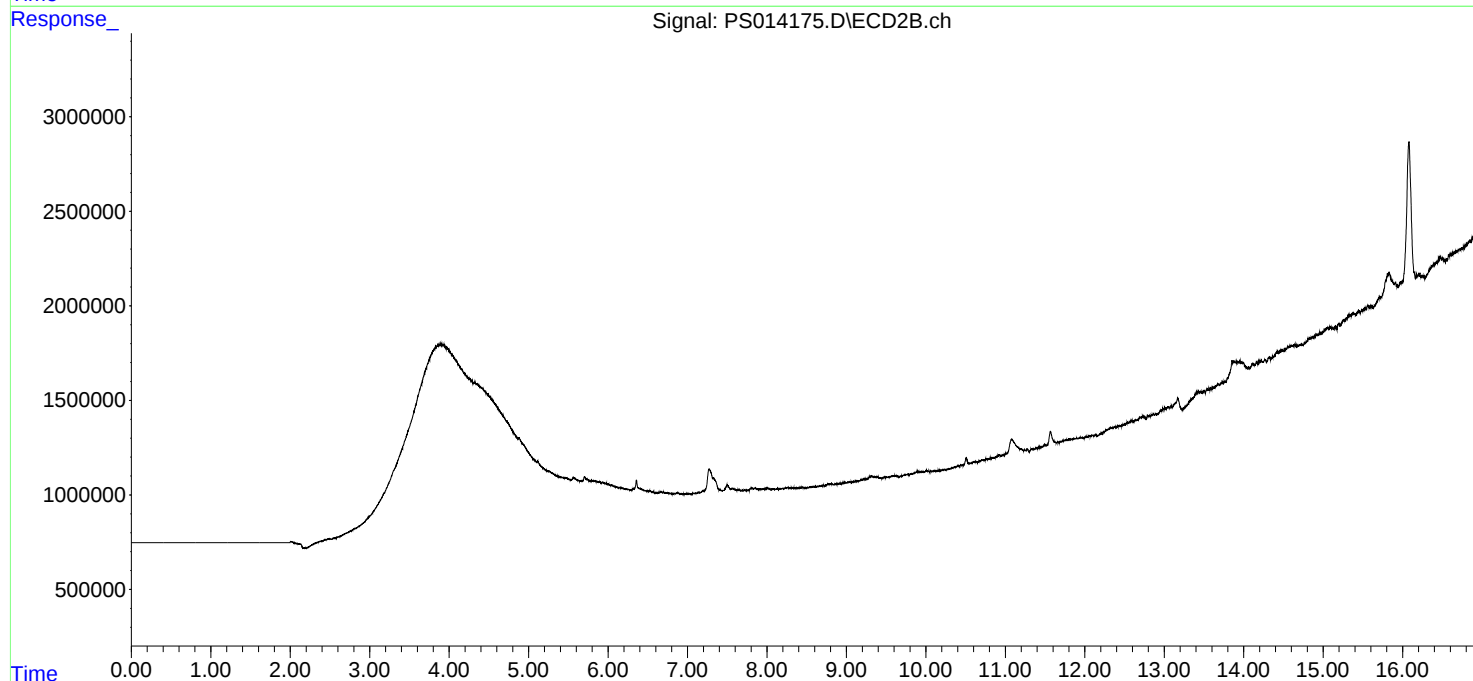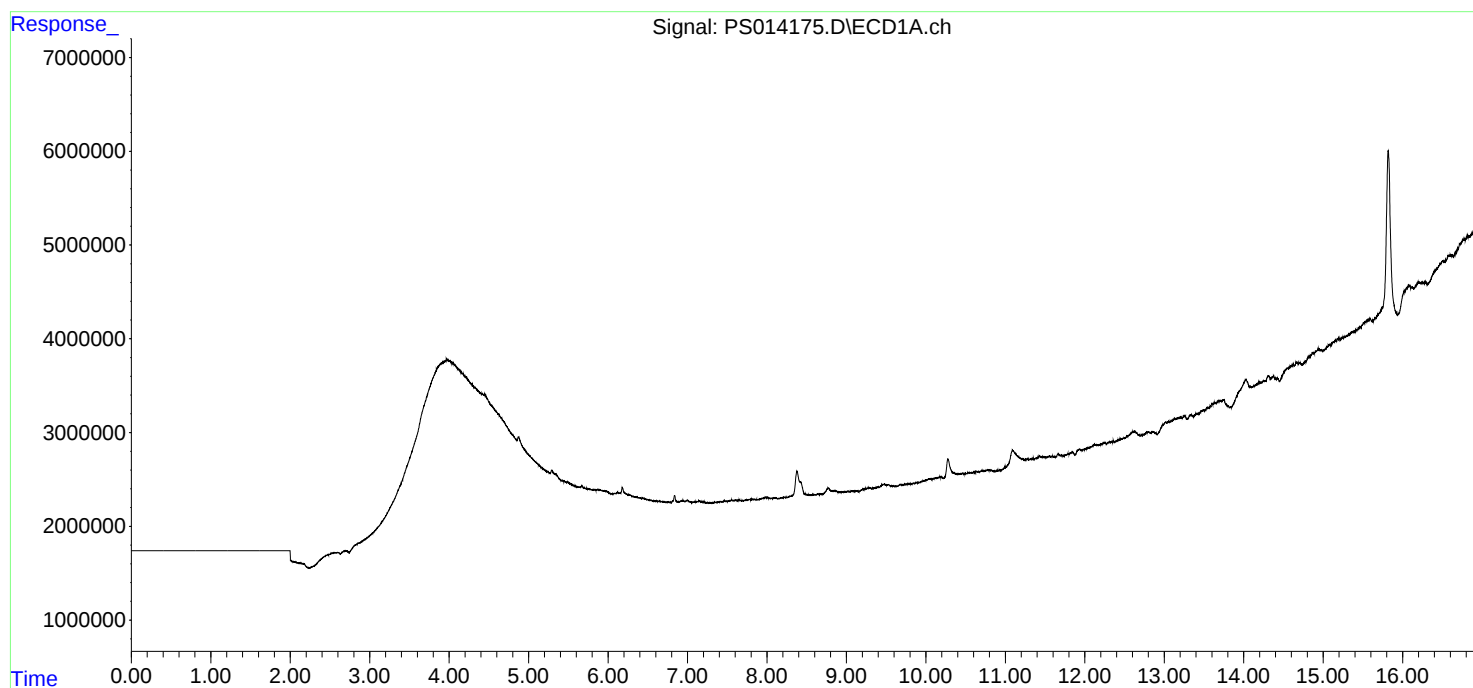


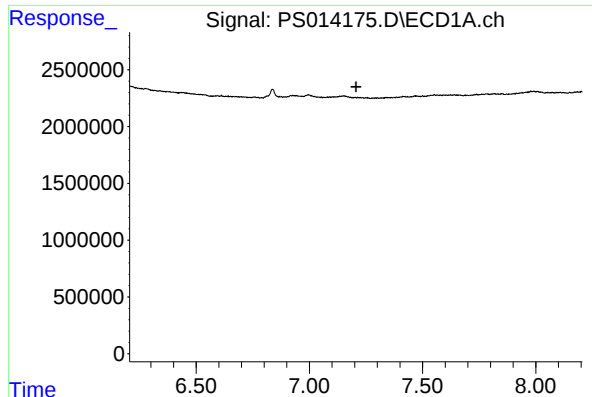

#4 2,4-DCAA

R.T.: 0.000 min  
Exp R.T. : 7.206 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :

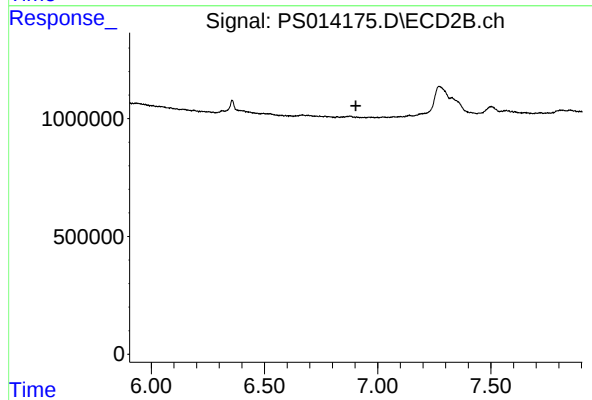

#4 2,4-DCAA

R.T.: 0.000 min  
Exp R.T. : 6.904 min  
Response: 0  
Conc: N.D.