

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030822\
 Data File : PS018513.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Mar 2022 09:34
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 08 23:55:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 22 00:27:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
9) T	2,4-D	8.189f	0.000	5343895	0	2.620	N.D. #
10) T	Pentachlo...	8.423	8.106	2987210	2850216	<MDL	<MDL #
11) T	2,4,5-TP ...	8.972	8.428	3512690	60711133	<MDL	14.705 #
12) T	2,4,5-T	9.277	8.874	18062286	6548701	1.796	1.664
14) T	DINOSEB	10.920	9.669	60647486	4294360	7.806	1.477 #
15) T	Picloram	10.747	10.681	59431903	131.2E6	4.677	22.691 #
16) T	DCPA	11.204	10.583	2851841	6747087	<MDL	1.359 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030822\
Data File : PS018513.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Mar 2022 09:34
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 08 23:55:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
Quant Title : 8080.M
QLast Update : Tue Feb 22 00:27:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

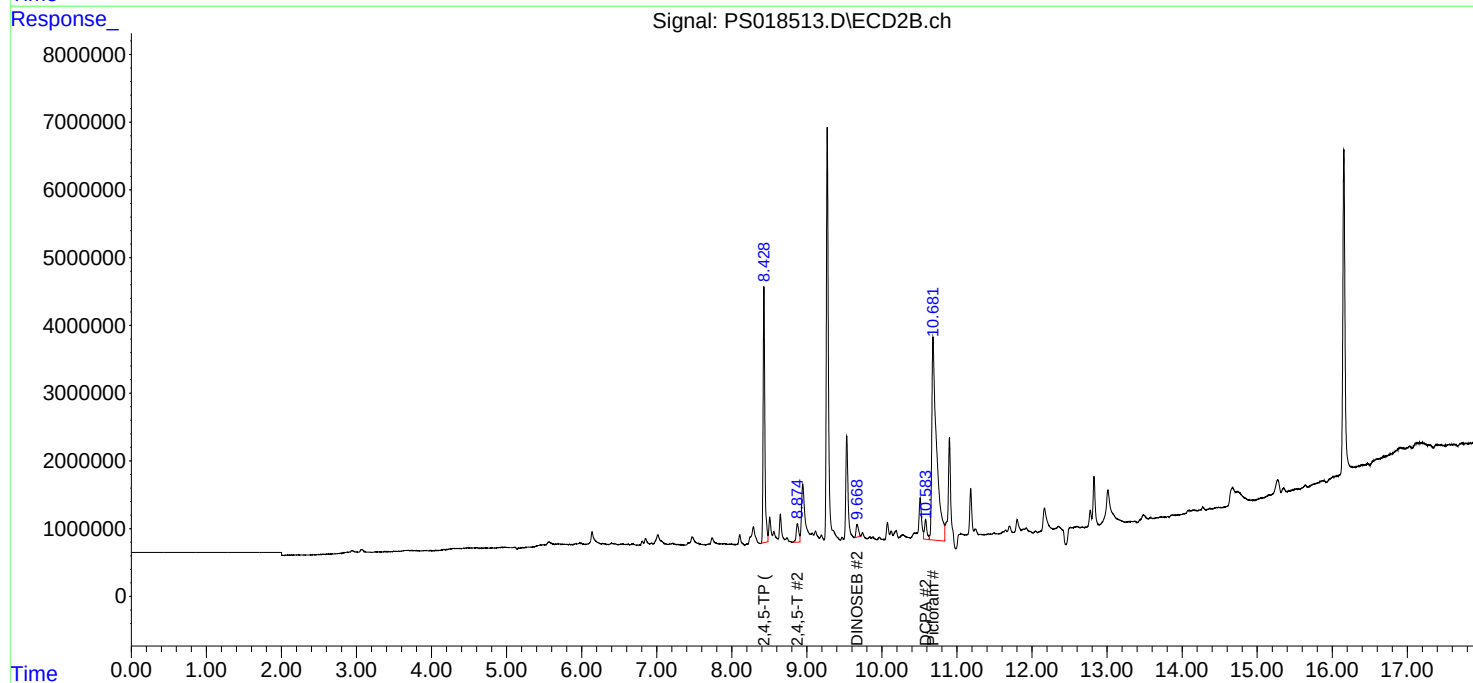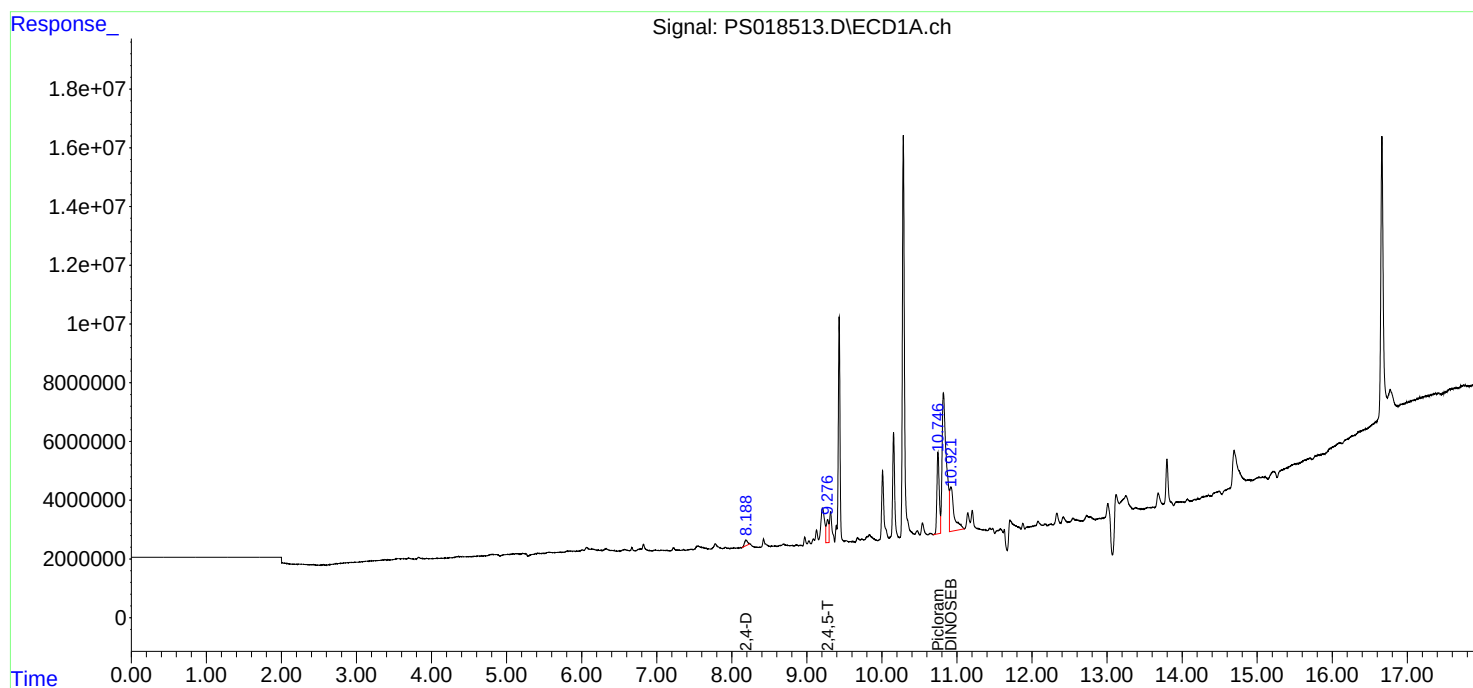


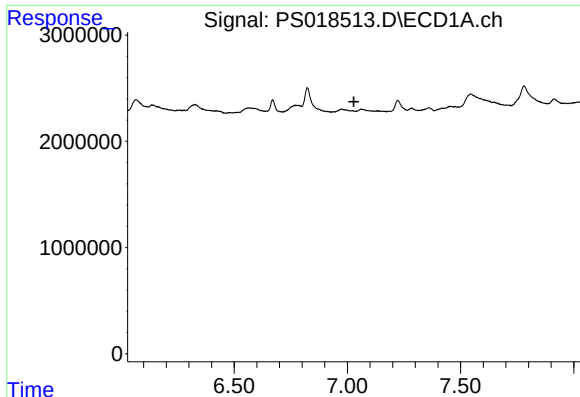

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.029 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

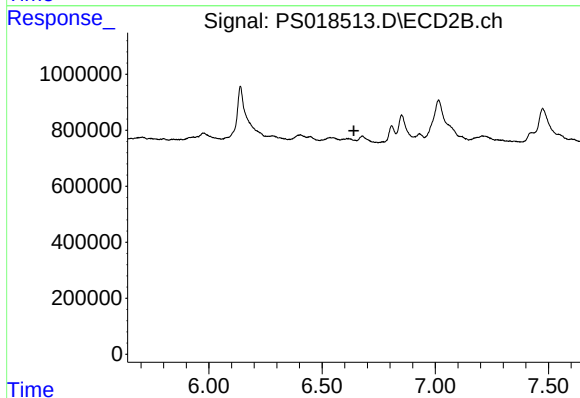


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.640 min
Response: 0
Conc: N.D.

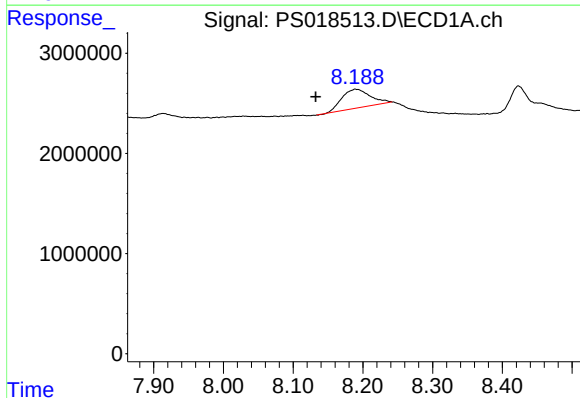


#9 2,4-D

R.T.: 8.189 min
Delta R.T.: 0.057 min
Response: 5343895
Conc: 2.62 ng/ml

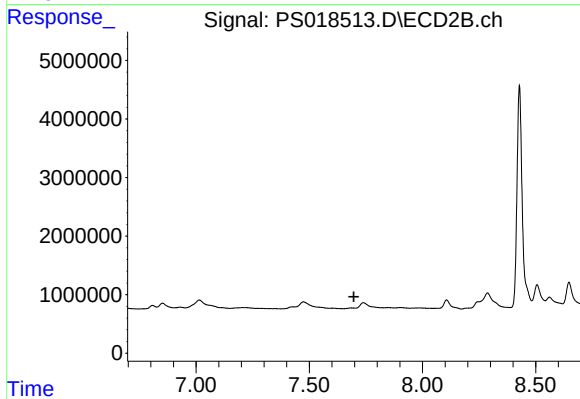

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.697 min
Response: 0
Conc: N.D.

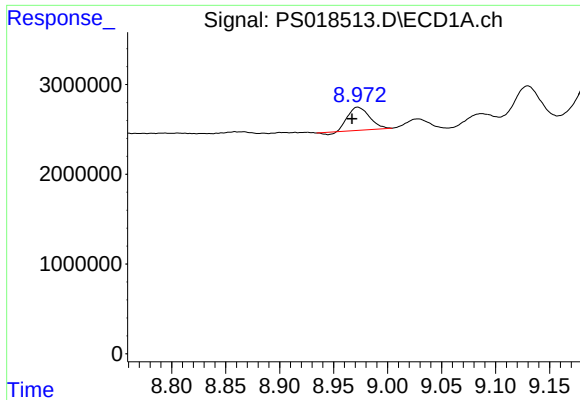

#11 2,4,5-TP (SILVEX)


R.T.: 8.972 min
Delta R.T.: 0.005 min
Response: 3512690
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

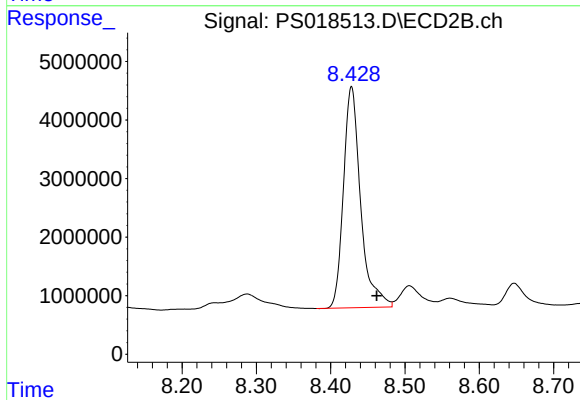


#11 2,4,5-TP (SILVEX)

R.T.: 8.428 min
Delta R.T.: -0.034 min
Response: 60711133
Conc: 14.71 ng/ml

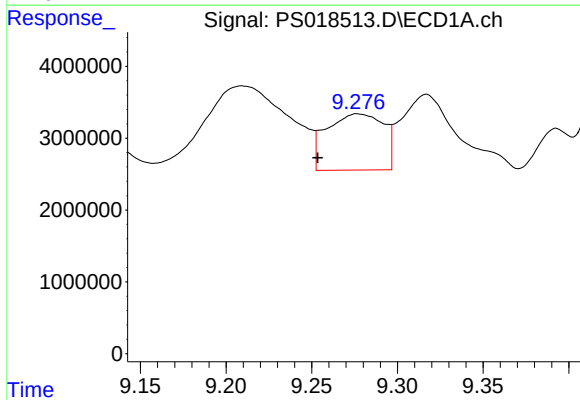


#12 2,4,5-T

R.T.: 9.277 min
Delta R.T.: 0.023 min
Response: 18062286
Conc: 1.80 ng/ml

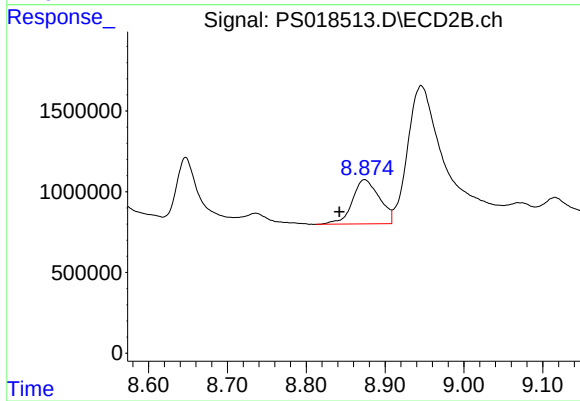

#12 2,4,5-T


R.T.: 8.874 min
Delta R.T.: 0.032 min
Response: 6548701
Conc: 1.66 ng/ml

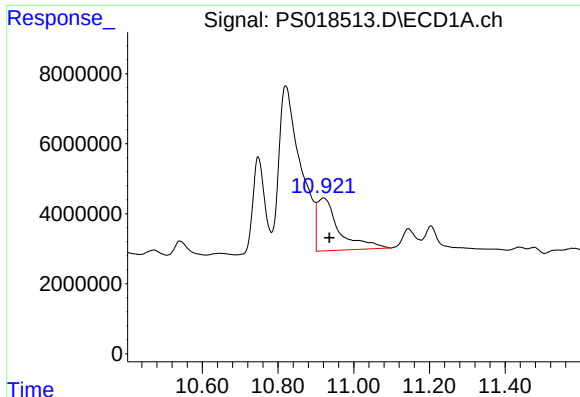

#14 DINOSEB


R.T.: 10.920 min
Delta R.T.: -0.016 min
Response: 60647486
Conc: 7.81 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

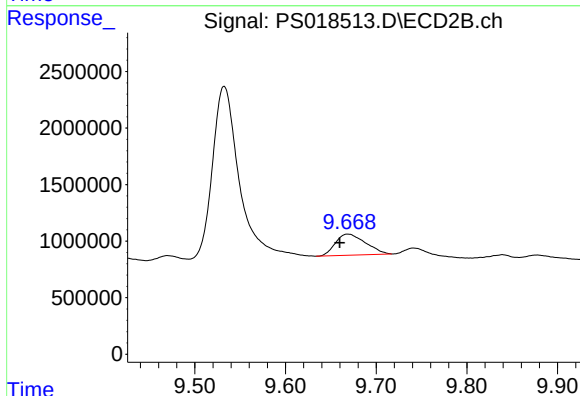


#14 DINOSEB

R.T.: 9.669 min
Delta R.T.: 0.009 min
Response: 4294360
Conc: 1.48 ng/ml

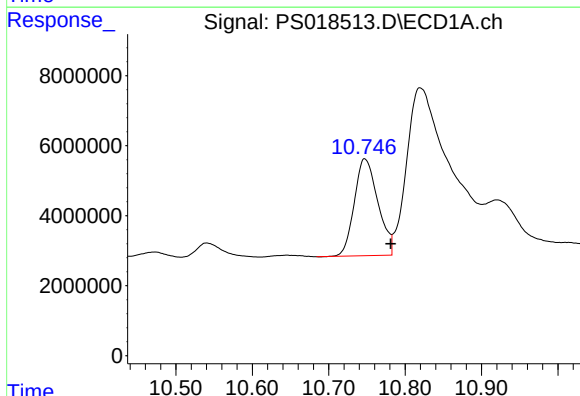


#15 Picloram

R.T.: 10.747 min
Delta R.T.: -0.034 min
Response: 59431903
Conc: 4.68 ng/ml

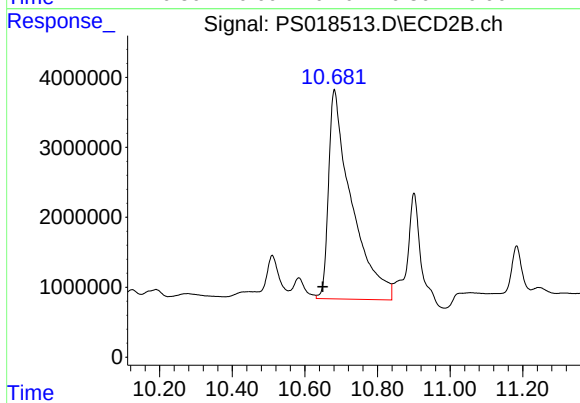

#15 Picloram


R.T.: 10.681 min
Delta R.T.: 0.032 min
Response: 131222196
Conc: 22.69 ng/ml

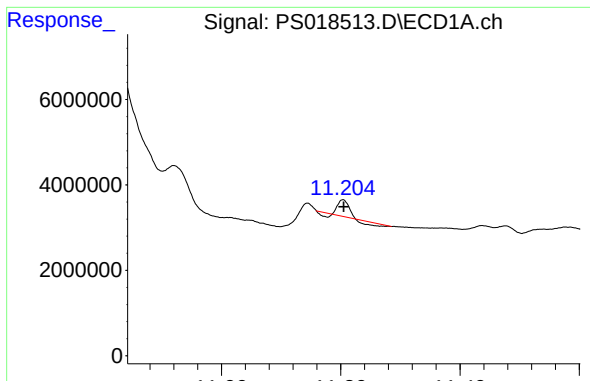

#16 DCPA

R.T.: 11.204 min
Delta R.T.: -0.001 min
Response: 2851841
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

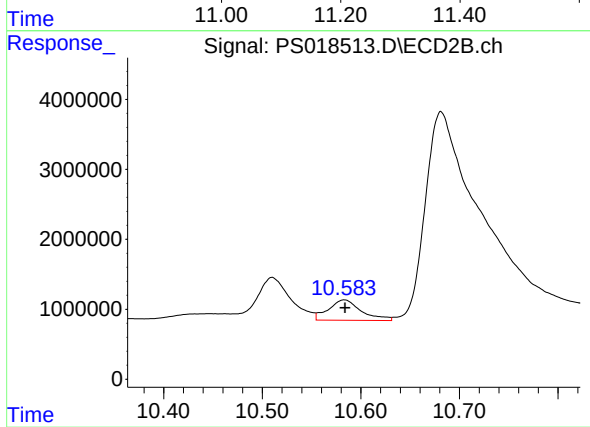

#16 DCPA

R.T.: 10.583 min
Delta R.T.: 0.000 min
Response: 6747087
Conc: 1.36 ng/ml