

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030822\
 Data File : PS018514.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Mar 2022 09:58
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 08 23:55:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 22 00:27:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.028	6.641	630.3E6	358.2E6	378.800	537.580 #
Target Compounds							
7) T	MCPA	0.000	7.018f	0	7242782	N.D.	2.162
9) T	2,4-D	8.190f	0.000	3646494	0	1.788	N.D. #
11) T	2,4,5-TP ...	0.000	8.431	0	37292575	N.D.	9.033
12) T	2,4,5-T	9.228	8.890f	12225152	1768300	1.215	<MDL #
14) T	DINOSEB	10.922	9.685	49066202	2536895	6.316	<MDL #
15) T	Picloram	10.763	10.699f	6946171	90120459	<MDL	15.584 #
16) T	DCPA	0.000	10.585	0	2980785	N.D.	<MDL


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030822\
Data File : PS018514.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Mar 2022 09:58
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 08 23:55:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
Quant Title : 8080.M
QLast Update : Tue Feb 22 00:27:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

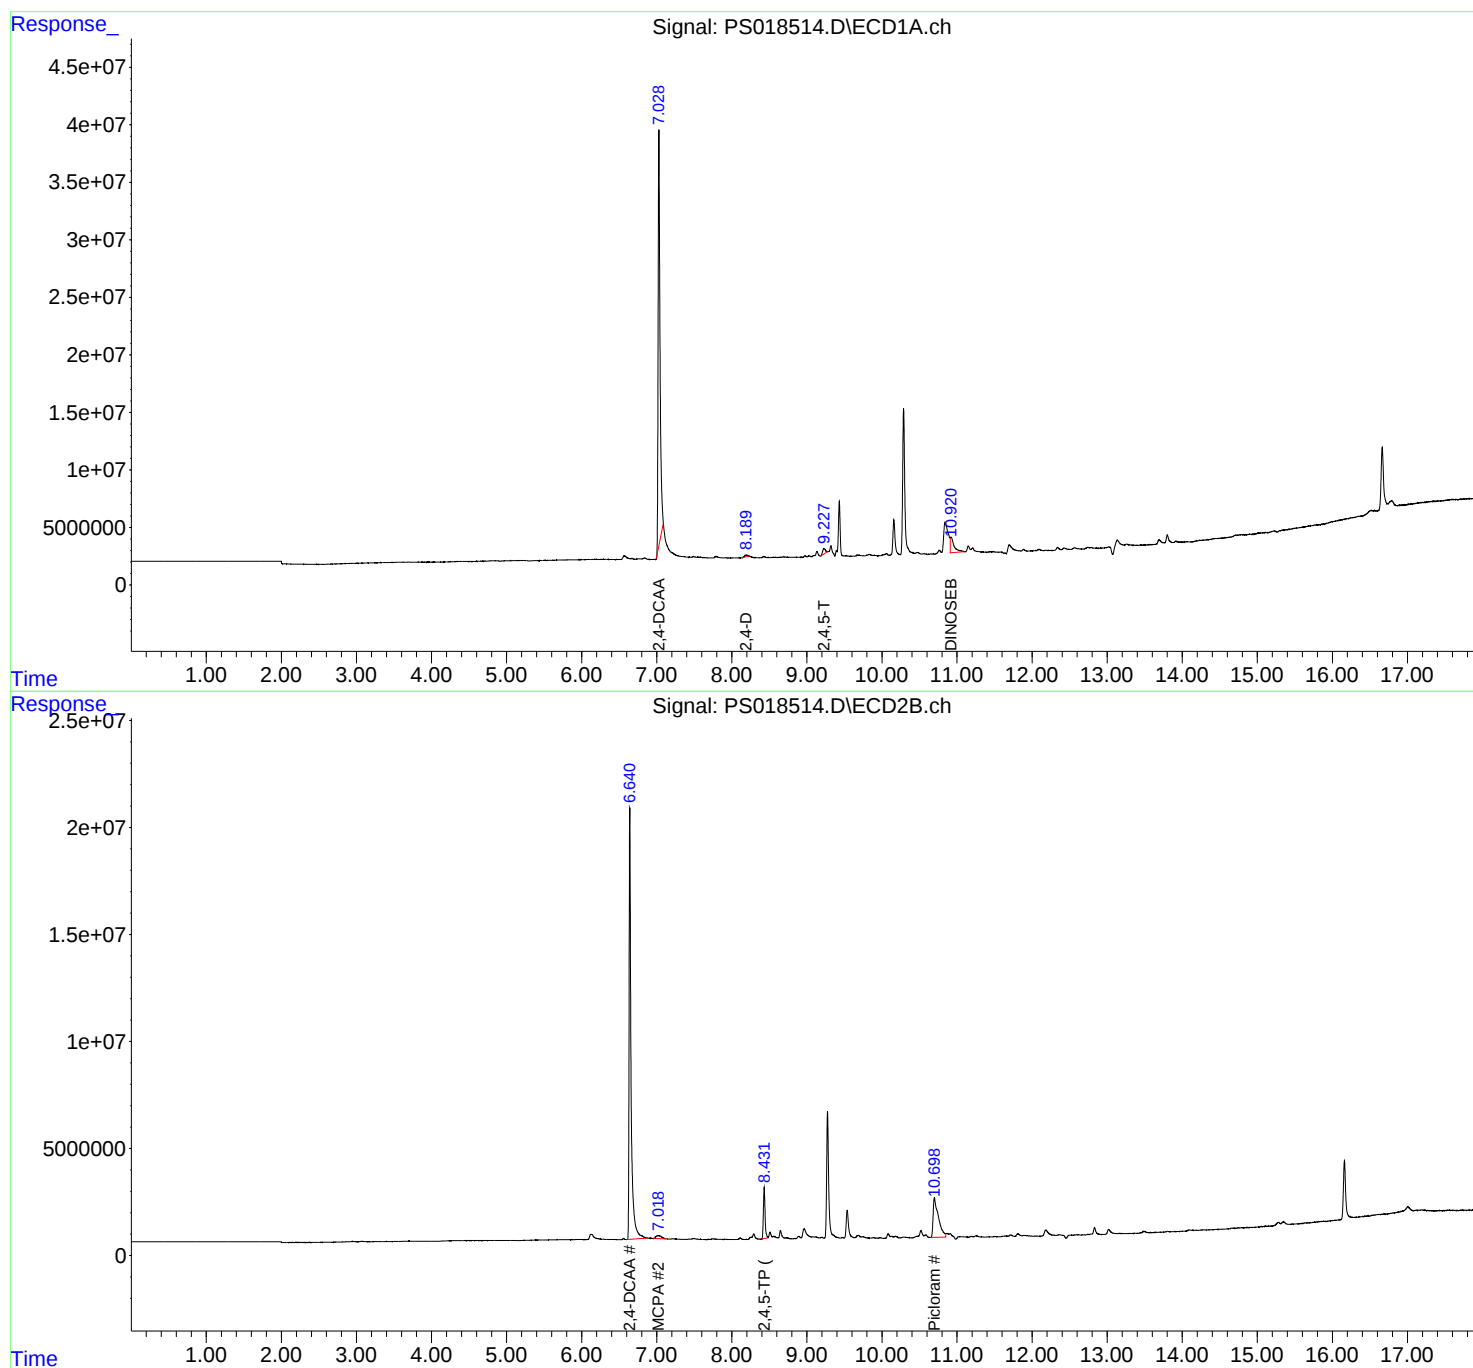


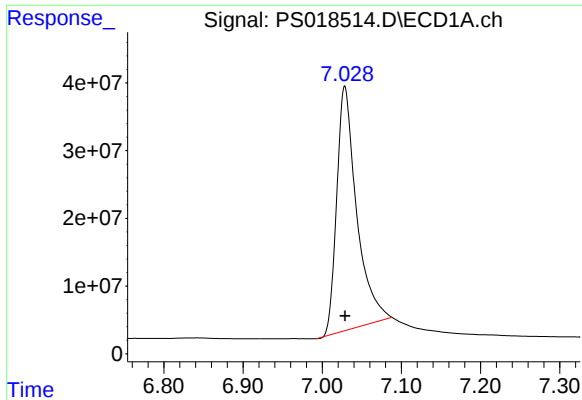

#4 2,4-DCAA


R.T.: 7.028 min
Delta R.T.: 0.000 min
Response: 630342193
Conc: 378.80 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

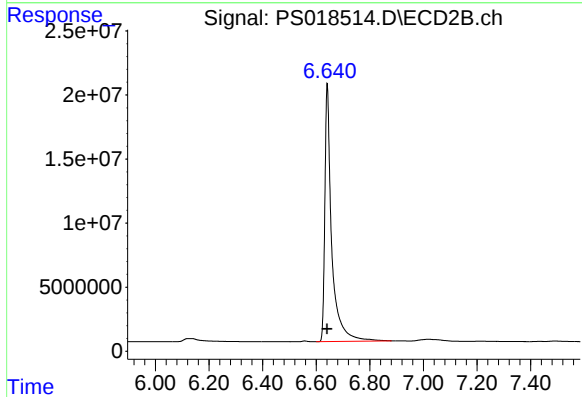


#4 2,4-DCAA

R.T.: 6.641 min
Delta R.T.: 0.000 min
Response: 358212040
Conc: 537.58 ng/ml

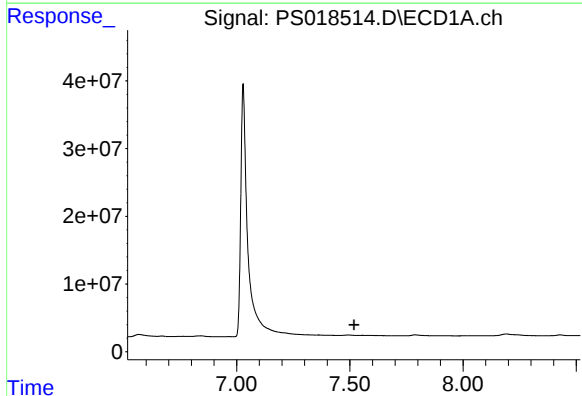


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.518 min
Response: 0
Conc: N.D.

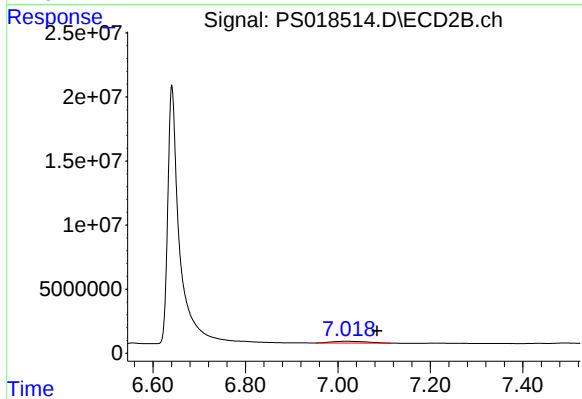

#7 MCPA


R.T.: 7.018 min
Delta R.T.: -0.067 min
Response: 7242782
Conc: 2.16 ug/ml

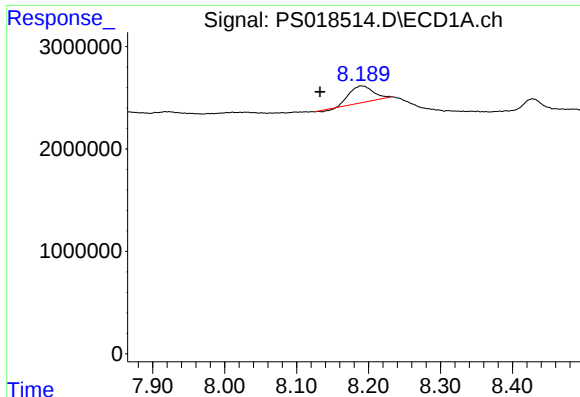

#9 2,4-D


R.T.: 8.190 min
Delta R.T.: 0.057 min
Response: 3646494
Conc: 1.79 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

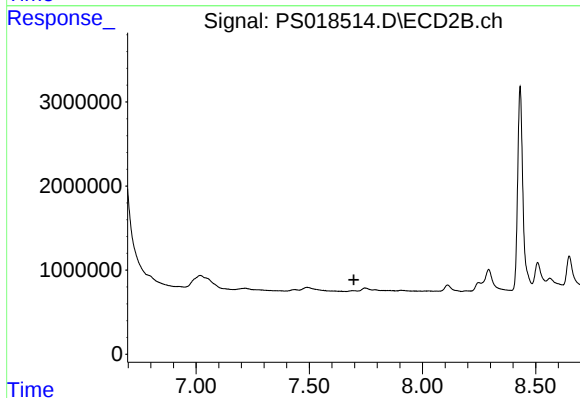


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.697 min
Response: 0
Conc: N.D.

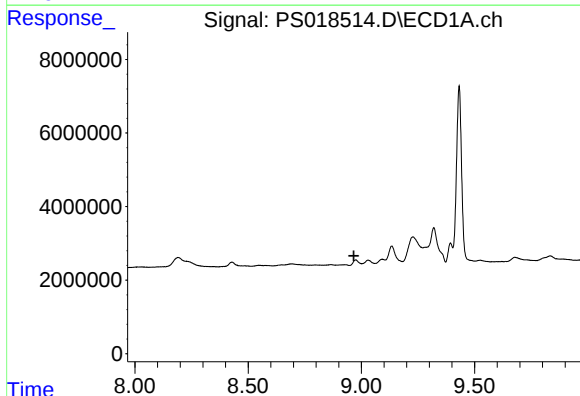


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 8.967 min
Response: 0
Conc: N.D.

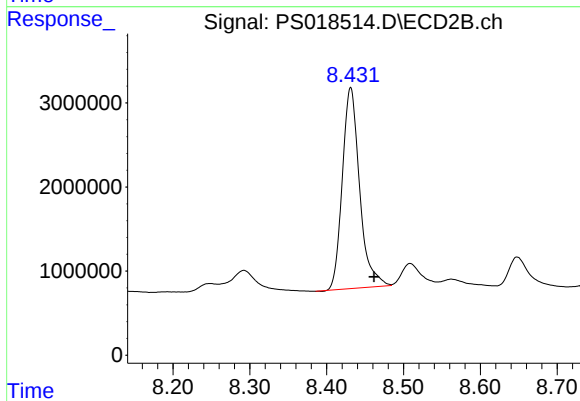

#11 2,4,5-TP (SILVEX)


R.T.: 8.431 min
Delta R.T.: -0.031 min
Response: 37292575
Conc: 9.03 ng/ml

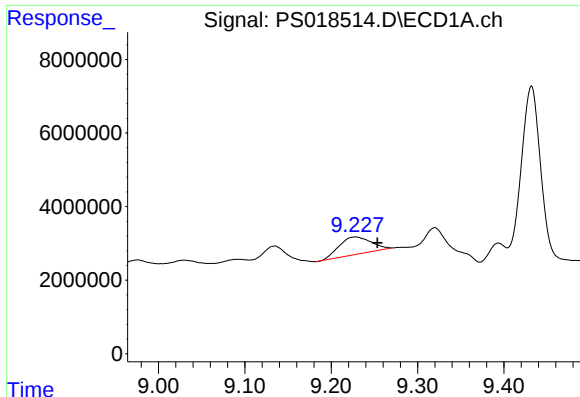

#12 2,4,5-T


R.T.: 9.228 min
Delta R.T.: -0.026 min
Response: 12225152
Conc: 1.22 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

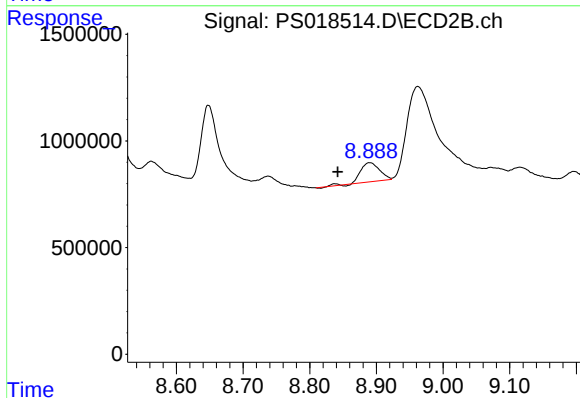


#12 2,4,5-T

R.T.: 8.890 min
Delta R.T.: 0.047 min
Response: 1768300
Conc: N.D.

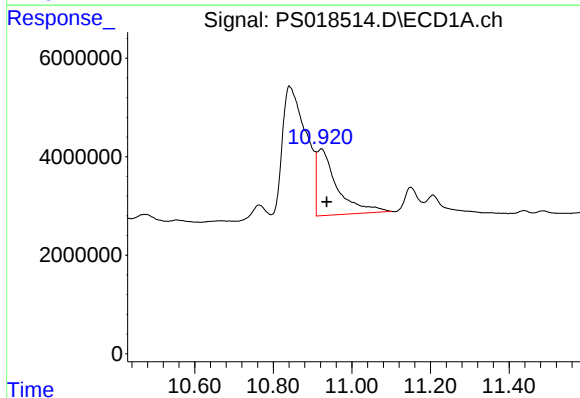


#14 DINOSEB

R.T.: 10.922 min
Delta R.T.: -0.014 min
Response: 49066202
Conc: 6.32 ng/ml

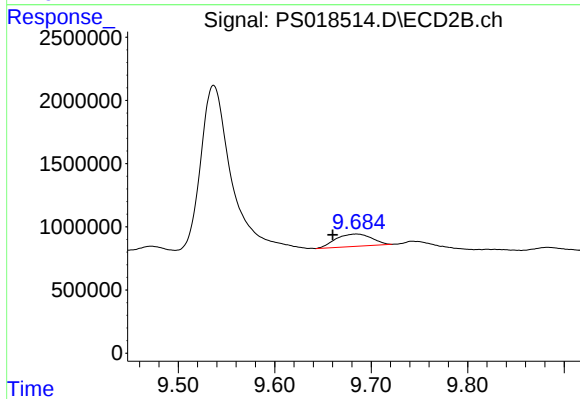

#14 DINOSEB


R.T.: 9.685 min
Delta R.T.: 0.025 min
Response: 2536895
Conc: N.D.

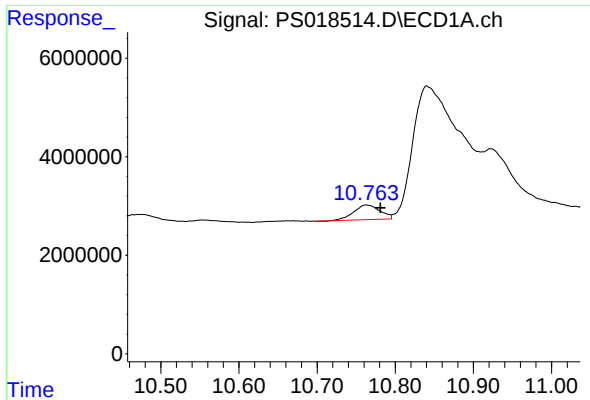

#15 Picloram

R.T.: 10.763 min
Delta R.T.: -0.018 min
Response: 6946171
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

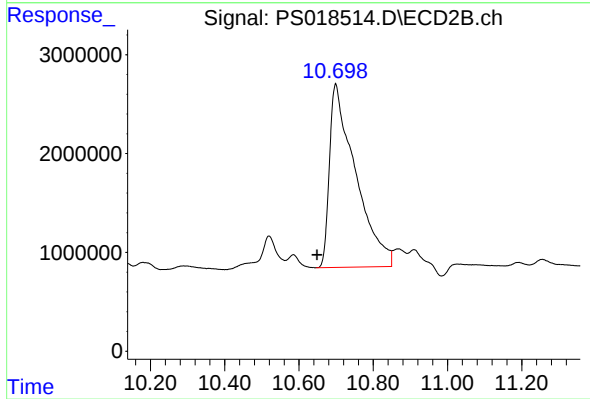

#15 Picloram

R.T.: 10.699 min
Delta R.T.: 0.050 min
Response: 90120459
Conc: 15.58 ng/ml