

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030822\
 Data File : PS018517.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Mar 2022 15:09
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 08 23:56:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 22 00:27:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.032	6.638	634.8E6	352.0E6	381.476	528.302 #
Target Compounds							
5) T	DICAMBA	7.220	6.795	5015218	5414754	<MDL	1.928 #
9) T	2,4-D	8.192f	7.741f	41014389	2480153	20.106	2.649 #
10) T	Pentachlo...	8.431	8.108	15922541	7891671	<MDL	<MDL #
11) T	2,4,5-TP ...	8.980	8.432	13137610	40522542	1.380	9.815 #
12) T	2,4,5-T	9.221	8.881	61824857	8720731	6.146	2.215 #
13) T	2,4-DB	0.000	9.276f	0	105.2E6	N.D.	194.659
14) T	DINOSEB	10.940	9.667	67926554	5512153	8.743	1.896 #
15) T	Picloram	10.769	10.693f	8103158	146.4E6	<MDL	25.313 #
16) T	DCPA	11.212	10.585	11873979	9829000	<MDL	1.980 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030822\
Data File : PS018517.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Mar 2022 15:09
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 08 23:56:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
Quant Title : 8080.M
QLast Update : Tue Feb 22 00:27:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

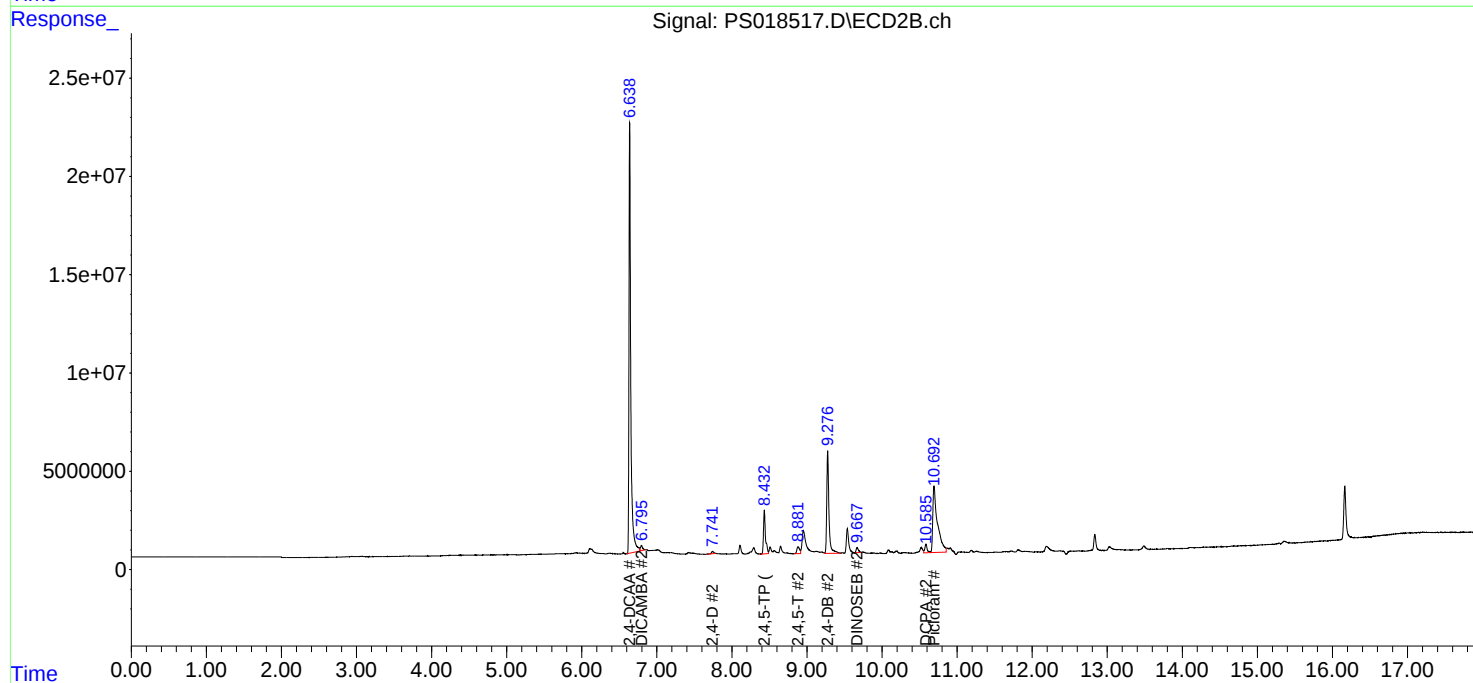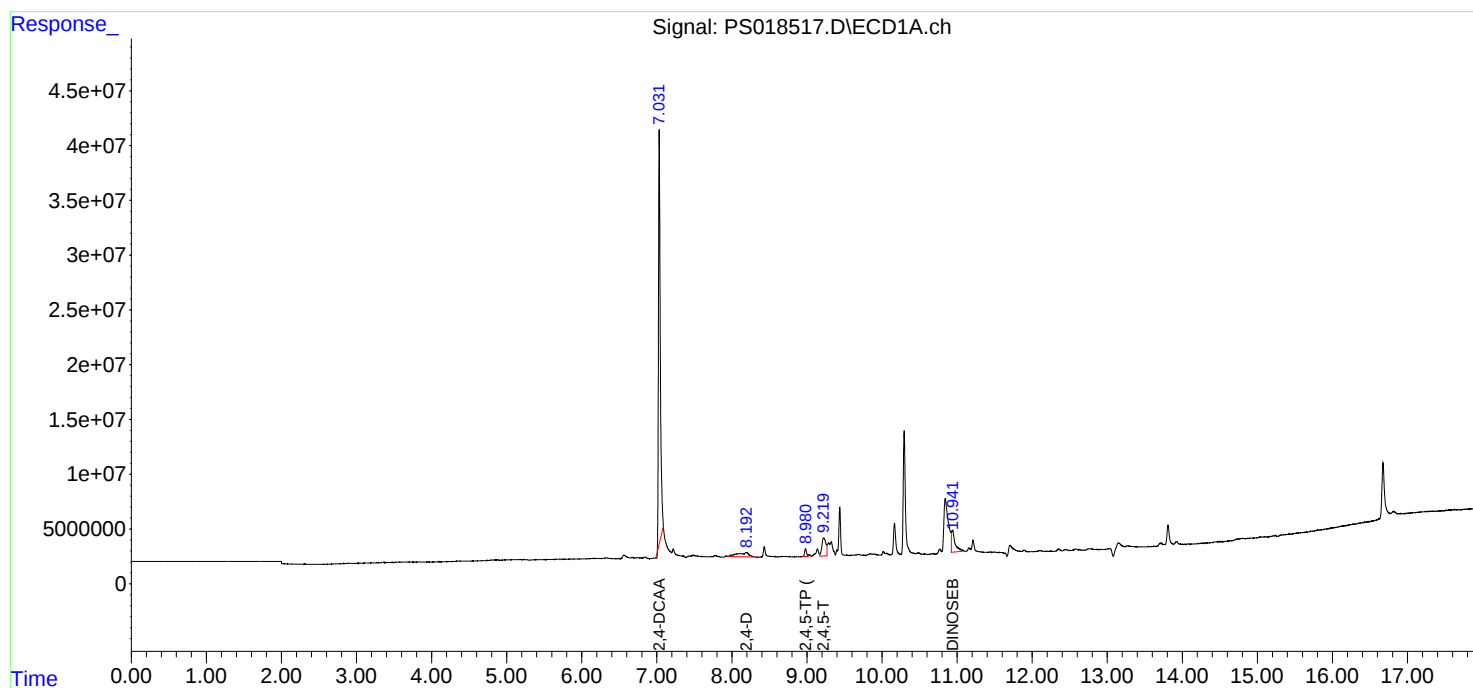


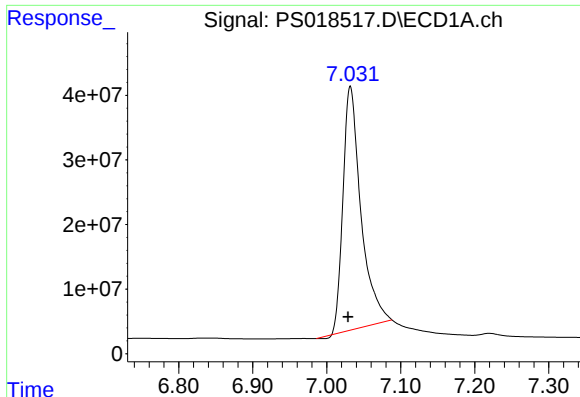

#4 2,4-DCAA


R.T.: 7.032 min
Delta R.T.: 0.003 min
Response: 634794905
Conc: 381.48 ng/ml

Instrument :
ECD_S
ClientSampleId :

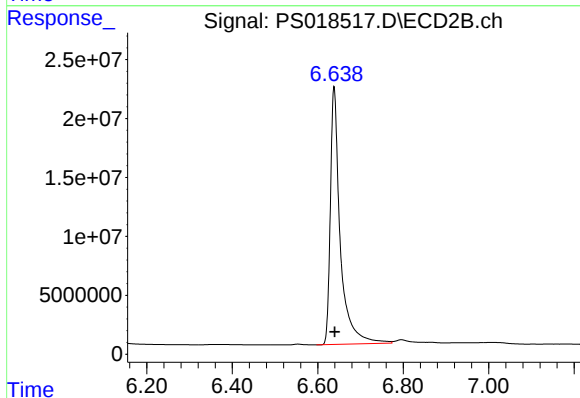


#4 2,4-DCAA

R.T.: 6.638 min
Delta R.T.: -0.002 min
Response: 352029990
Conc: 528.30 ng/ml

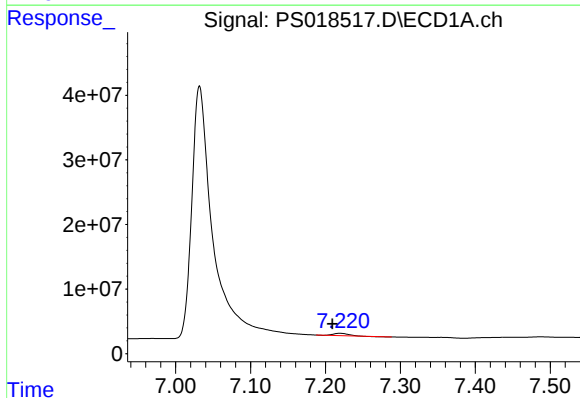


#5 DICAMBA

R.T.: 7.220 min
Delta R.T.: 0.010 min
Response: 5015218
Conc: N.D.

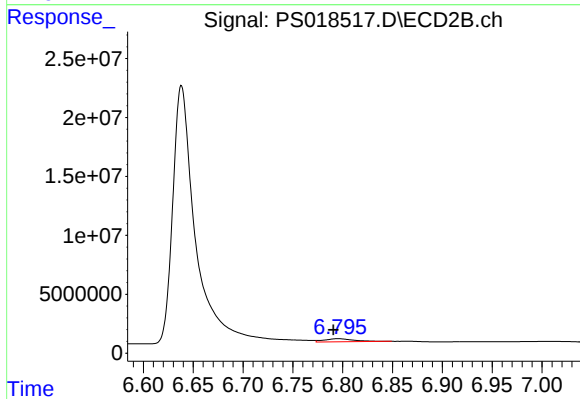

#5 DICAMBA


R.T.: 6.795 min
Delta R.T.: 0.004 min
Response: 5414754
Conc: 1.93 ng/ml

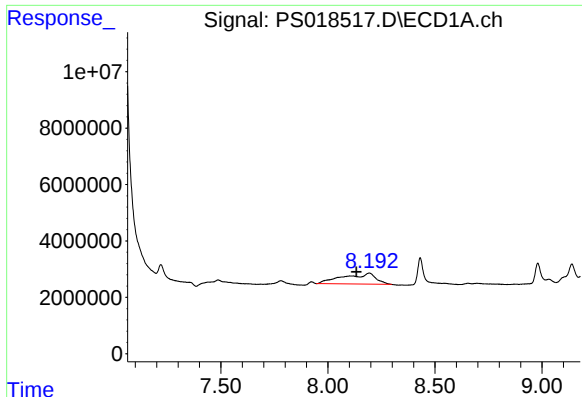

#9 2,4-D


R.T.: 8.192 min
Delta R.T.: 0.060 min
Response: 41014389
Conc: 20.11 ng/ml

Instrument :
ECD_S
ClientSampleId :

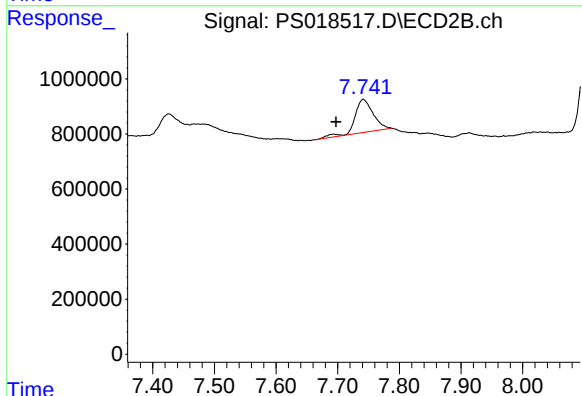


#9 2,4-D

R.T.: 7.741 min
Delta R.T.: 0.044 min
Response: 2480153
Conc: 2.65 ng/ml

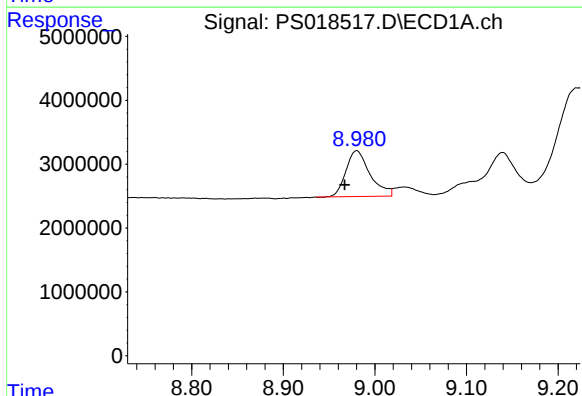


#11 2,4,5-TP (SILVEX)

R.T.: 8.980 min
Delta R.T.: 0.013 min
Response: 13137610
Conc: 1.38 ng/ml

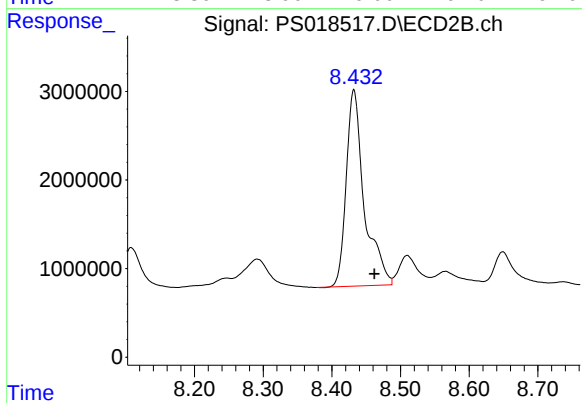

#11 2,4,5-TP (SILVEX)


R.T.: 8.432 min
Delta R.T.: -0.030 min
Response: 40522542
Conc: 9.82 ng/ml

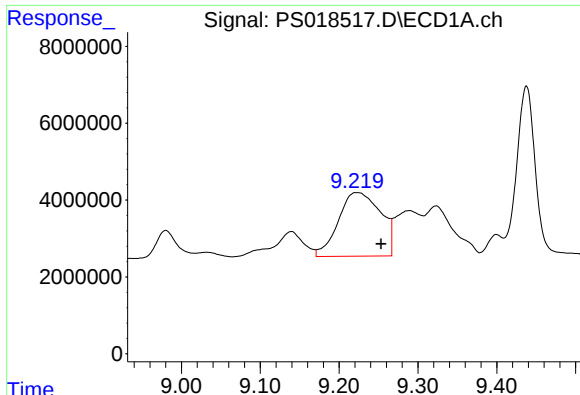

#12 2,4,5-T


R.T.: 9.221 min
Delta R.T.: -0.032 min
Response: 61824857
Conc: 6.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

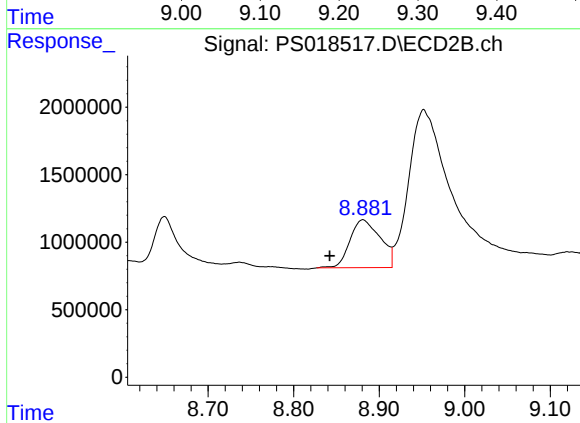


#12 2,4,5-T

R.T.: 8.881 min
Delta R.T.: 0.039 min
Response: 8720731
Conc: 2.22 ng/ml

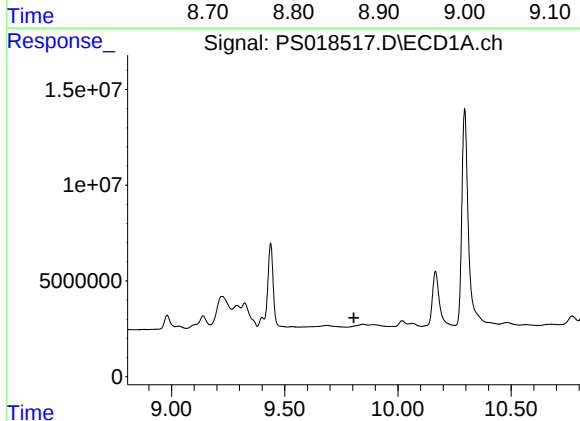


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.806 min
Response: 0
Conc: N.D.

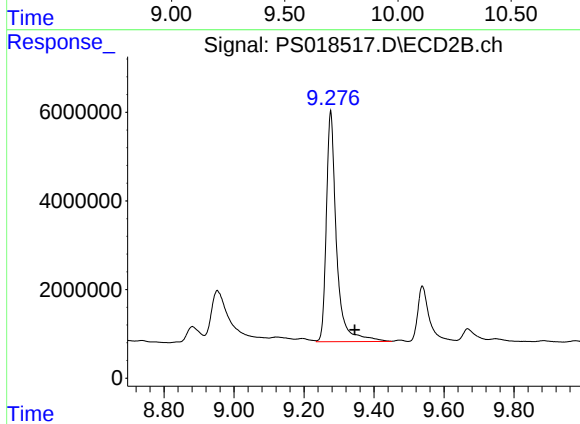

#13 2,4-DB


R.T.: 9.276 min
Delta R.T.: -0.069 min
Response: 105168348
Conc: 194.66 ng/ml

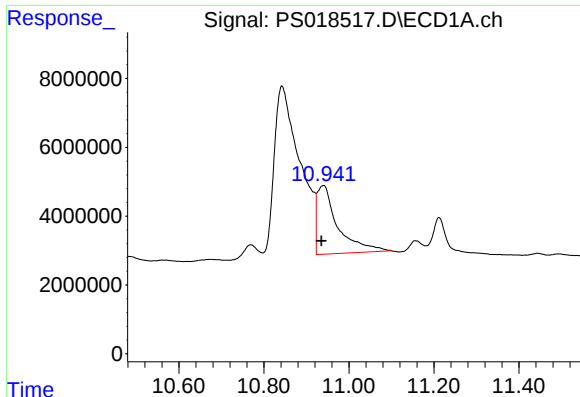

#14 DINoseb


R.T.: 10.940 min
Delta R.T.: 0.005 min
Response: 67926554
Conc: 8.74 ng/ml

Instrument :
ECD_S
ClientSampleId :

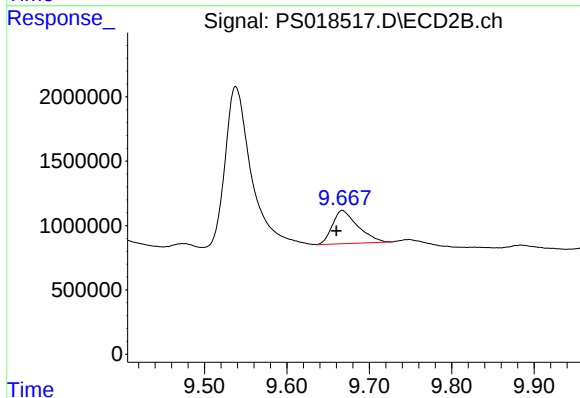


#14 DINoseb

R.T.: 9.667 min
Delta R.T.: 0.007 min
Response: 5512153
Conc: 1.90 ng/ml

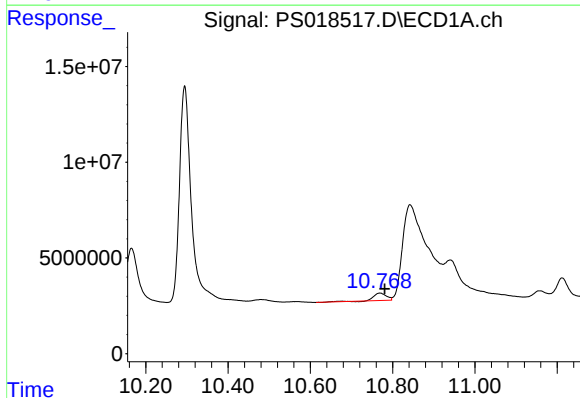


#15 Picloram

R.T.: 10.769 min
Delta R.T.: -0.012 min
Response: 8103158
Conc: N.D.

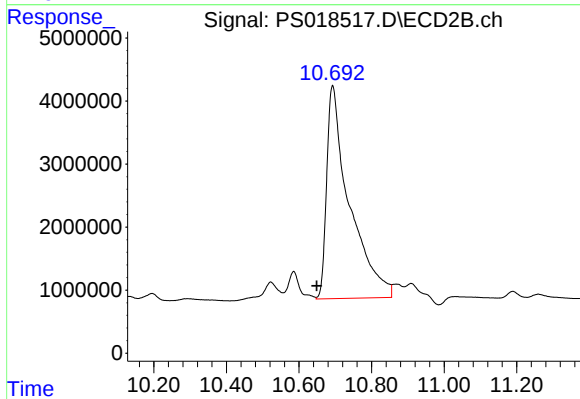

#15 Picloram


R.T.: 10.693 min
Delta R.T.: 0.044 min
Response: 146385453
Conc: 25.31 ng/ml

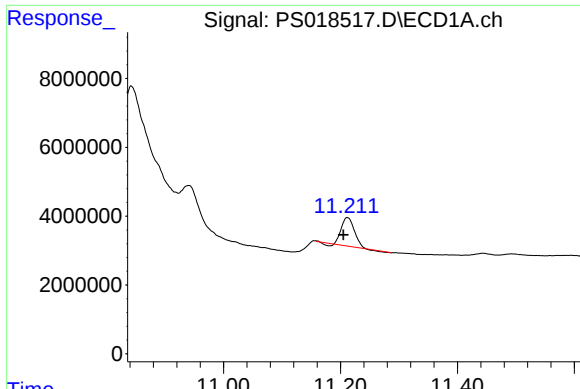

#16 DCPA

R.T.: 11.212 min
Delta R.T.: 0.007 min
Response: 11873979
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

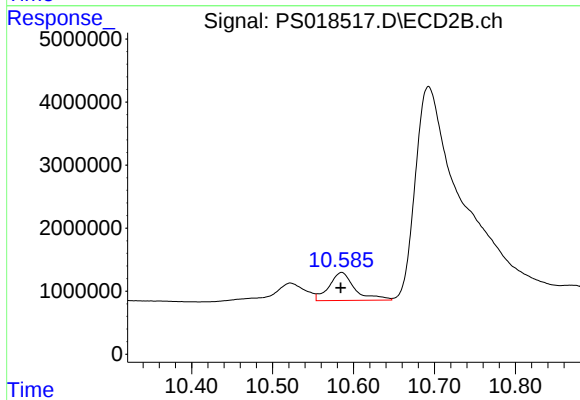

#16 DCPA

R.T.: 10.585 min
Delta R.T.: 0.001 min
Response: 9829000
Conc: 1.98 ng/ml