

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS030920\  
 Data File : PS009190.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 09 Mar 2020 11:58  
 Operator : DD\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 10 03:13:27 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS022020.M  
 Quant Title : 8080.M  
 QLast Update : Thu Feb 20 11:30:26 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound | RT#1  | RT#2   | Resp#1     | Resp#2  | ng/ml   | ng/ml   |
|-----------------------------|----------|-------|--------|------------|---------|---------|---------|
| -----                       |          |       |        |            |         |         |         |
| System Monitoring Compounds |          |       |        |            |         |         |         |
| 4) S                        | 2,4-DCAA | 7.248 | 6.936  | 855.0E6    | 461.9E6 | 391.014 | 479.340 |
| Target Compounds            |          |       |        |            |         |         |         |
| 15) T                       | Picloram | 0.000 | 11.028 | 0 40197738 | N.D.    | 5.532   |         |
| 16) T                       | DCPA     | 0.000 | 11.028 | 0 40197738 | N.D.    | 5.809   |         |
| -----                       |          |       |        |            |         |         |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS030920\  
Data File : PS009190.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 09 Mar 2020 11:58  
Operator : DD\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :  
I.BLK

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Mar 10 03:13:27 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS022020.M  
Quant Title : 8080.M  
QLast Update : Thu Feb 20 11:30:26 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

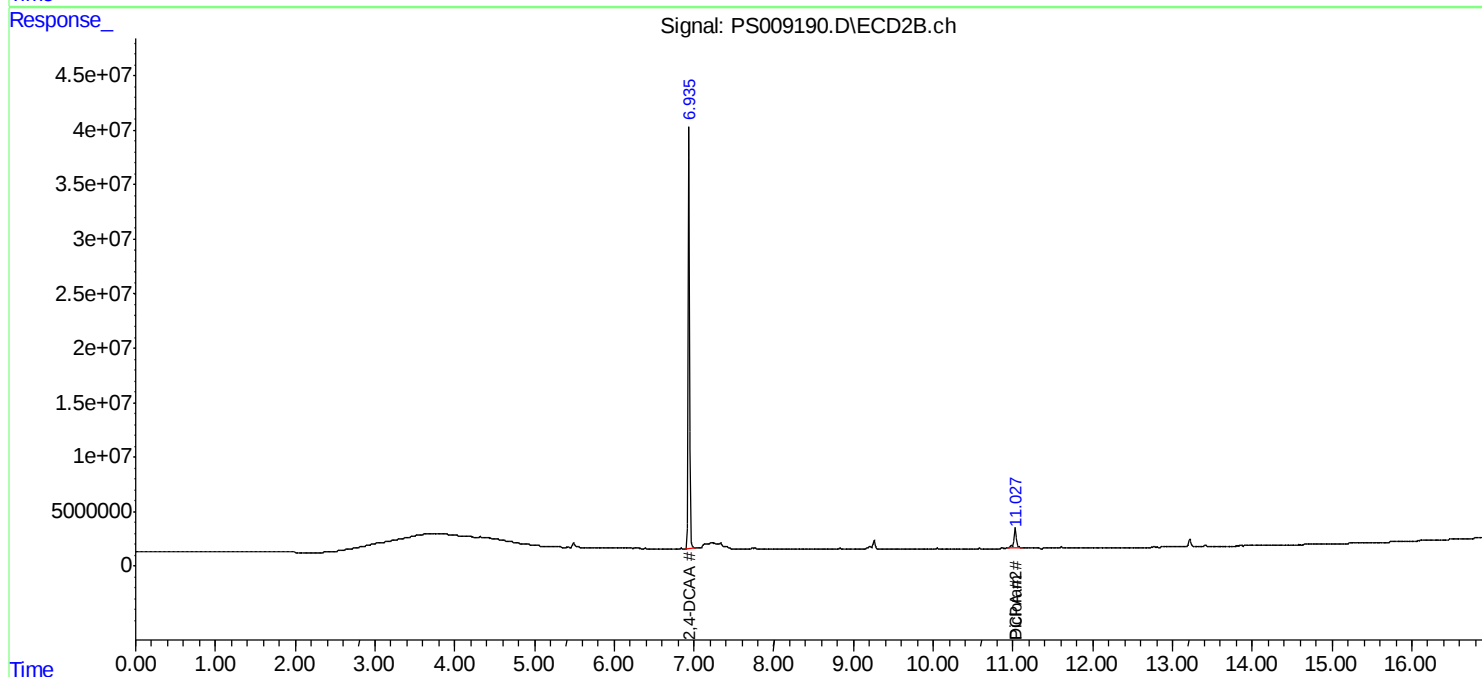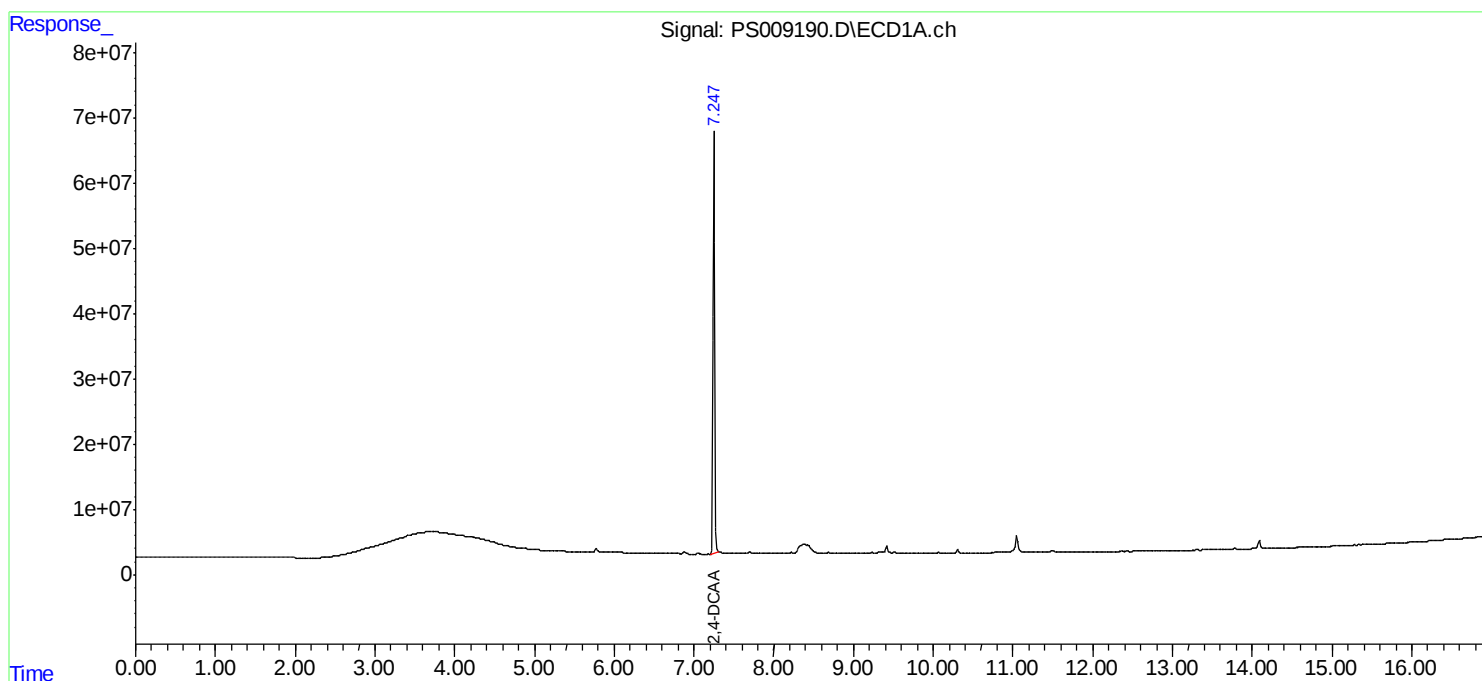


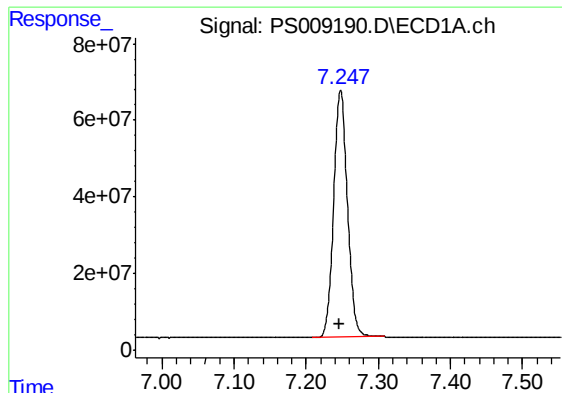

#4 2,4-DCAA


R.T.: 7.248 min  
Delta R.T.: 0.000 min  
Response: 854988265  
Conc: 391.01 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :  
I.BLK

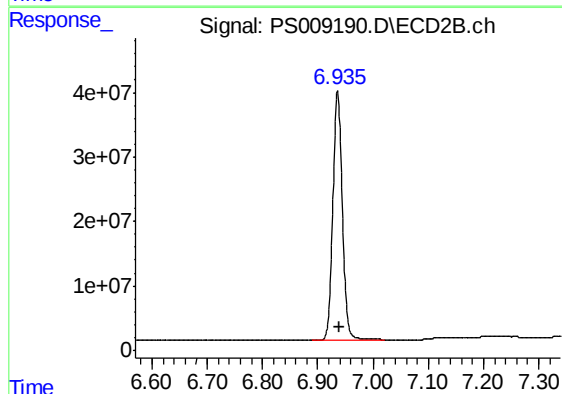


#4 2,4-DCAA

R.T.: 6.936 min  
Delta R.T.: -0.004 min  
Response: 461870794  
Conc: 479.34 ng/ml

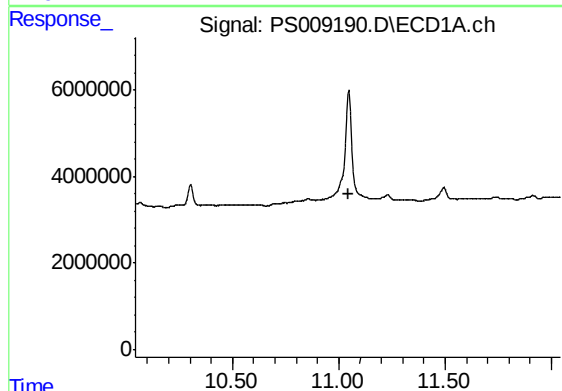


#15 Picloram

R.T.: 0.000 min  
Exp R.T. : 11.043 min  
Response: 0  
Conc: N.D.

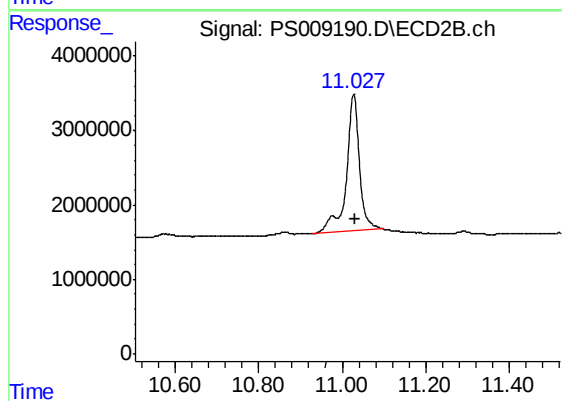

#15 Picloram


R.T.: 11.028 min  
Delta R.T.: -0.003 min  
Response: 40197738  
Conc: 5.53 ng/ml

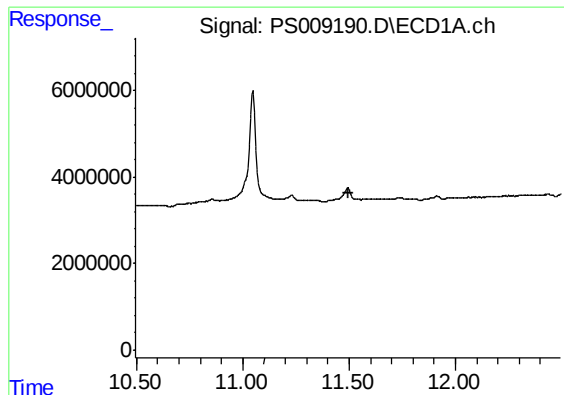

#16 DCPA

R.T.: 0.000 min  
Exp R.T. : 11.495 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :  
I.BLK

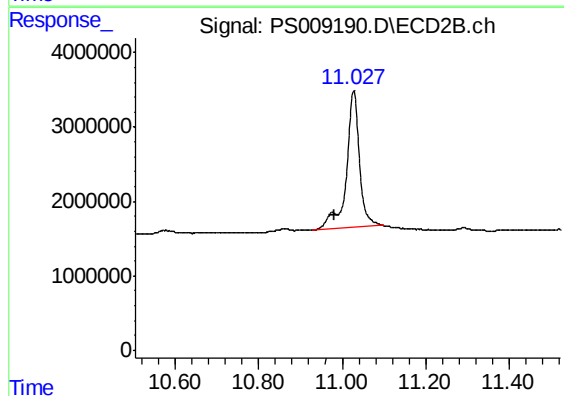

#16 DCPA

R.T.: 11.028 min  
Delta R.T.: 0.045 min  
Response: 40197738  
Conc: 5.81 ng/ml