

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030920\
 Data File : PS009192.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Mar 2020 12:50
 Operator : DD\AJ
 Sample : L1778-05
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 DN1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 03:14:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.248	6.937	624.9E6	282.1E6	285.782	292.767
Target Compounds							
2) T	3,5-DICHL...	0.000	6.112	0 97018177		N.D.	66.484
3) T	4-Nitroph...	0.000	6.566	0 29666538		N.D.	51.323
5) T	DICAMBA	7.377	0.000	150.0E6	0	18.464	N.D. #
7) T	MCPA	7.799	7.405	243.1E6	153.7E6	30.219	34.748
8) T	DICHLORPROP	0.000	7.757	0 75679811		N.D.	75.534
11) T	2,4,5-TP ...	0.000	8.791	0 64444018		N.D.	11.897
12) T	2,4,5-T	0.000	9.255	0 83998459		N.D.	15.518
14) T	DINOSEB	0.000	10.060	0 21122005		N.D.	5.342
15) T	Picloram	11.044	11.027	371.3E6	264.8E6	27.120	36.444 #
16) T	DCPA	0.000	11.027	0 264.8E6		N.D.	38.273



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030920\
Data File : PS009192.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Mar 2020 12:50
Operator : DD\AJ
Sample : L1778-05
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
DN1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 03:14:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

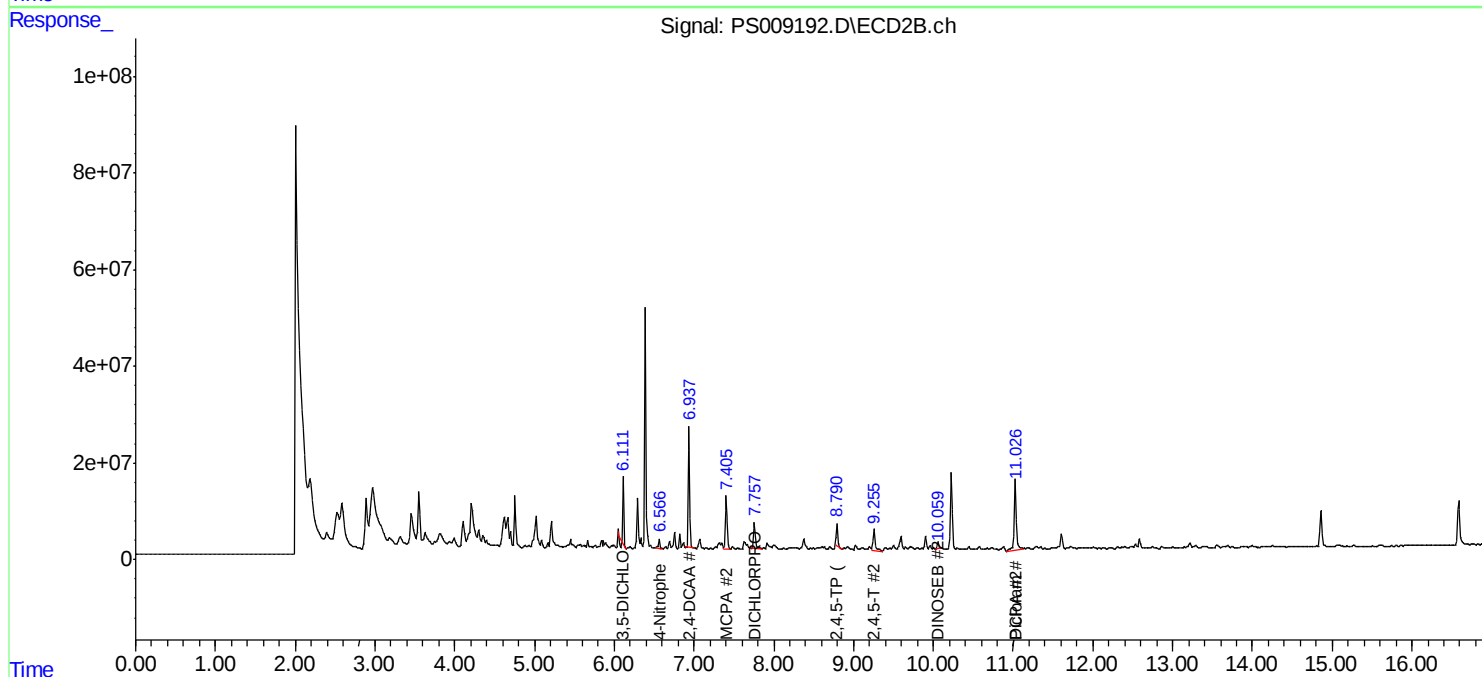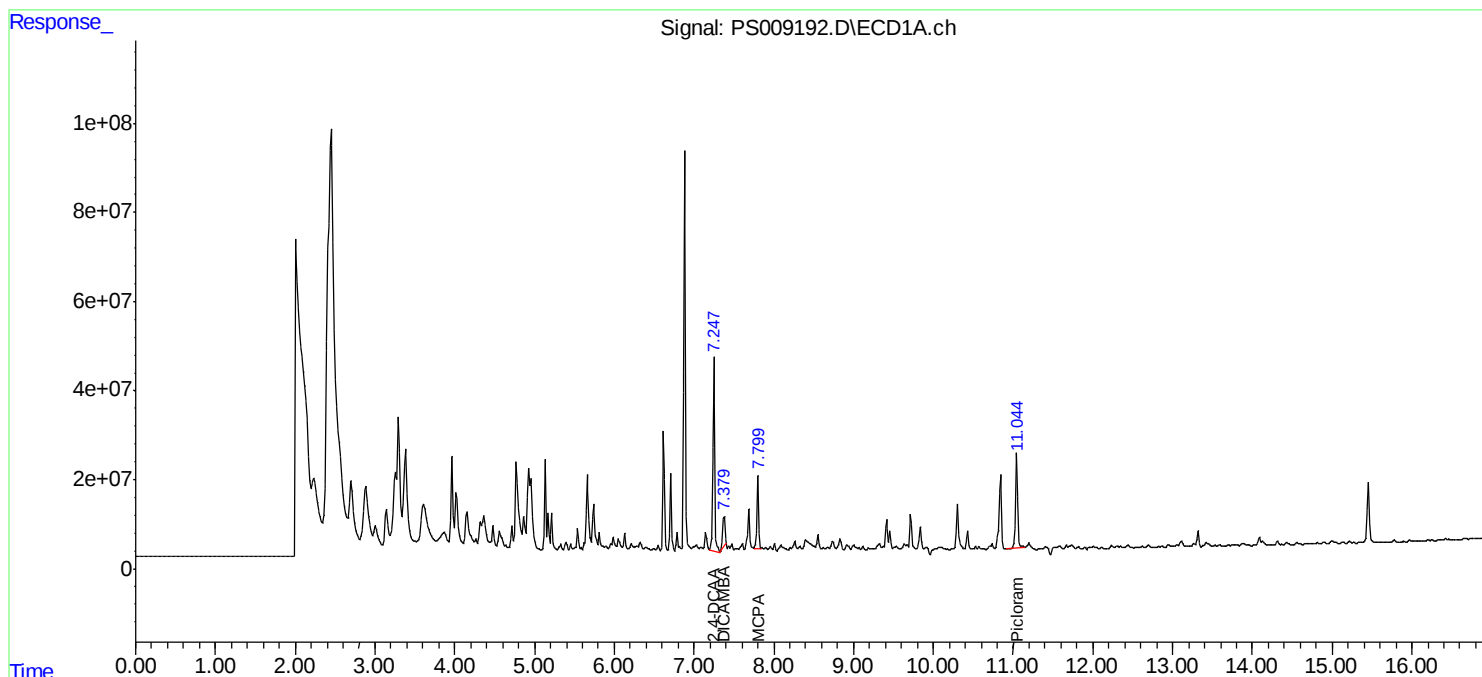


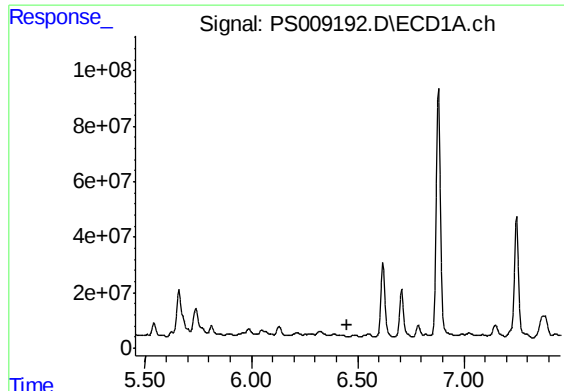

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
DN1

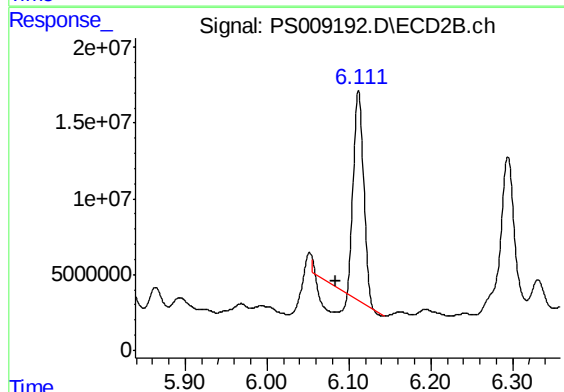


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.112 min
Delta R.T.: 0.028 min
Response: 97018177
Conc: 66.48 ng/ml

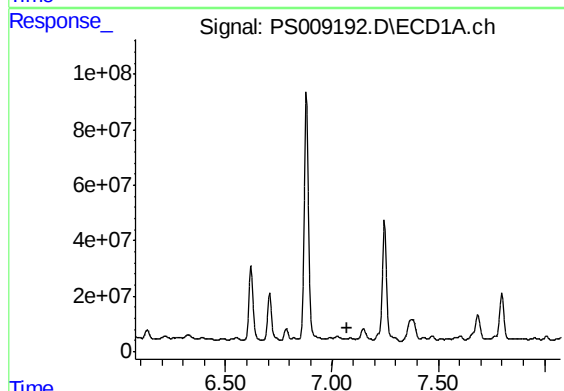


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 7.075 min
Response: 0
Conc: N.D.

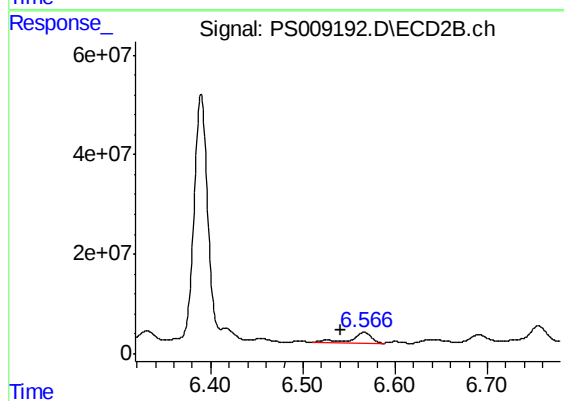

#3 4-Nitrophenol


R.T.: 6.566 min
Delta R.T.: 0.026 min
Response: 29666538
Conc: 51.32 ng/ml

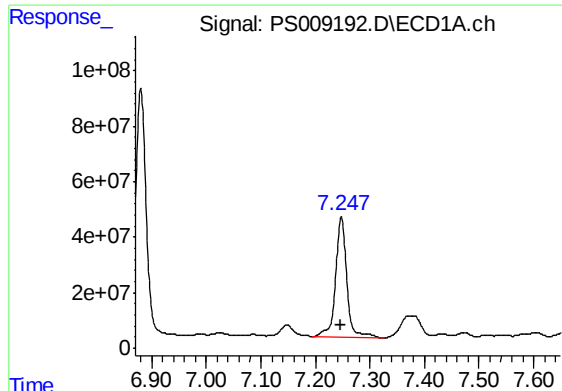

#4 2,4-DCAA


R.T.: 7.248 min
Delta R.T.: 0.000 min
Response: 624888600
Conc: 285.78 ng/ml

Instrument :
ECD_S
ClientSampleId :
DN1

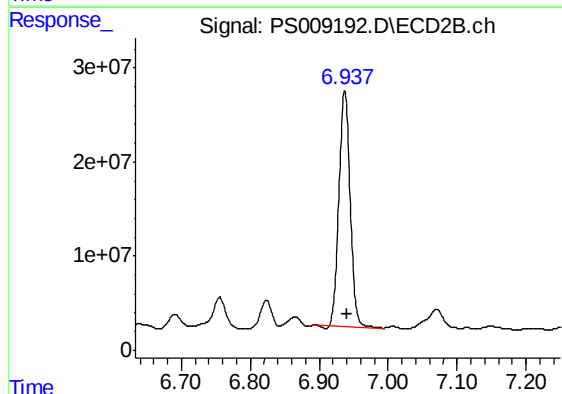


#4 2,4-DCAA

R.T.: 6.937 min
Delta R.T.: -0.003 min
Response: 282096981
Conc: 292.77 ng/ml

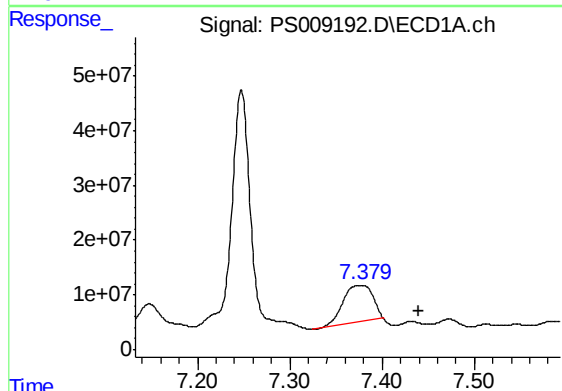


#5 DICAMBA

R.T.: 7.377 min
Delta R.T.: -0.063 min
Response: 150001649
Conc: 18.46 ng/ml

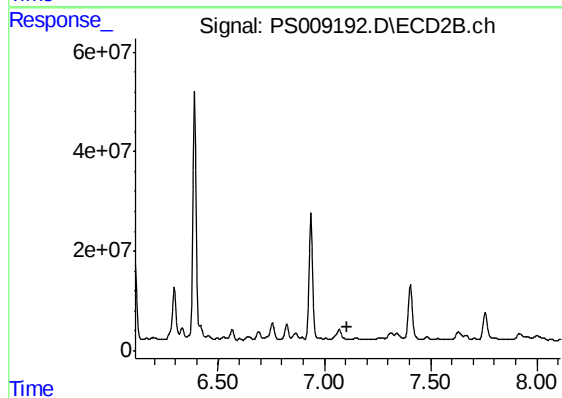

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 7.111 min
Response: 0
Conc: N.D.

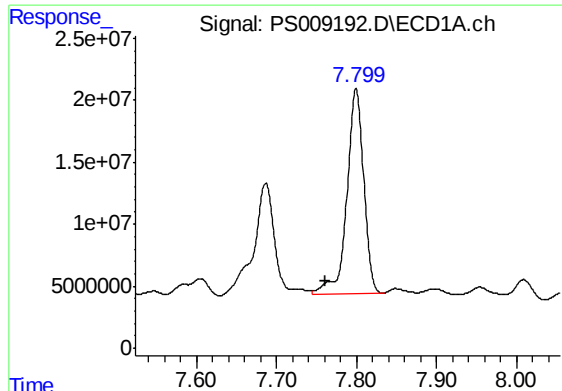

#7 MCPA


R.T.: 7.799 min
Delta R.T.: 0.039 min
Response: 243082903
Conc: 30.22 ug/ml

Instrument :
ECD_S
ClientSampleId :
DN1

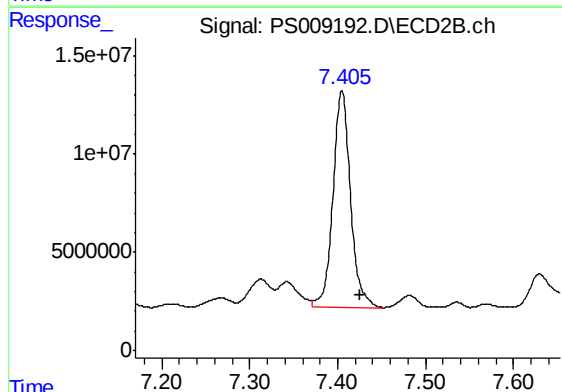


#7 MCPA

R.T.: 7.405 min
Delta R.T.: -0.021 min
Response: 153732496
Conc: 34.75 ug/ml

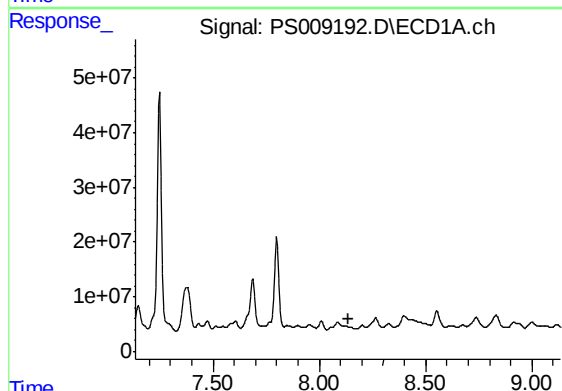


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.135 min
Response: 0
Conc: N.D.

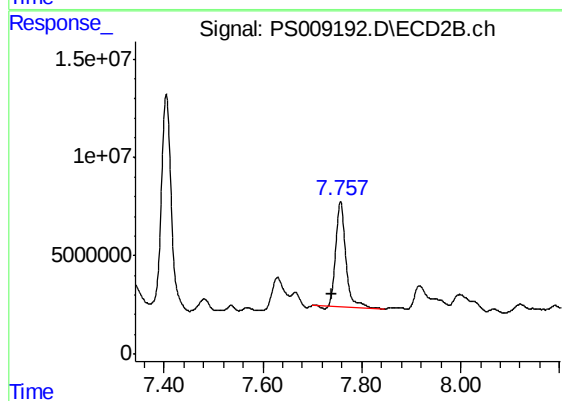

#8 DICHLORPROP


R.T.: 7.757 min
Delta R.T.: 0.018 min
Response: 75679811
Conc: 75.53 ng/ml

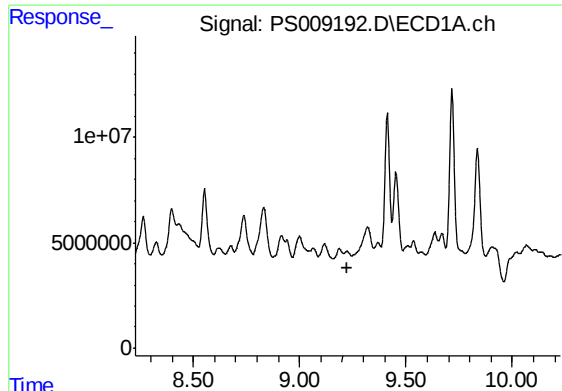

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 9.227 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
DN1

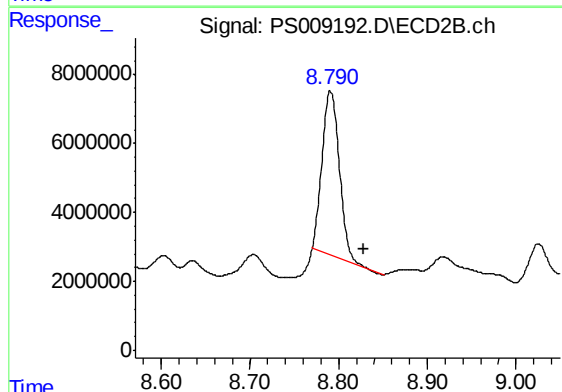


#11 2,4,5-TP (SILVEX)

R.T.: 8.791 min
Delta R.T.: -0.037 min
Response: 64444018
Conc: 11.90 ng/ml

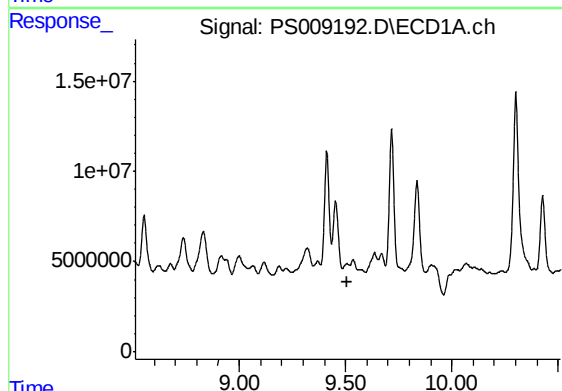


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.511 min
Response: 0
Conc: N.D.

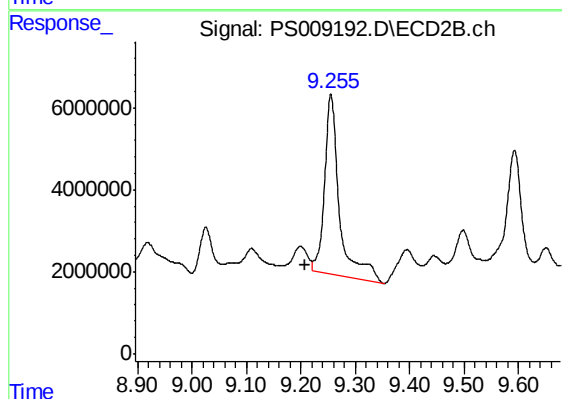

#12 2,4,5-T


R.T.: 9.255 min
Delta R.T.: 0.048 min
Response: 83998459
Conc: 15.52 ng/ml

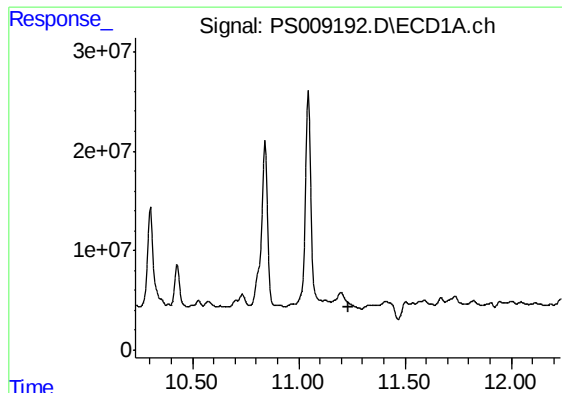

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 11.231 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
DN1

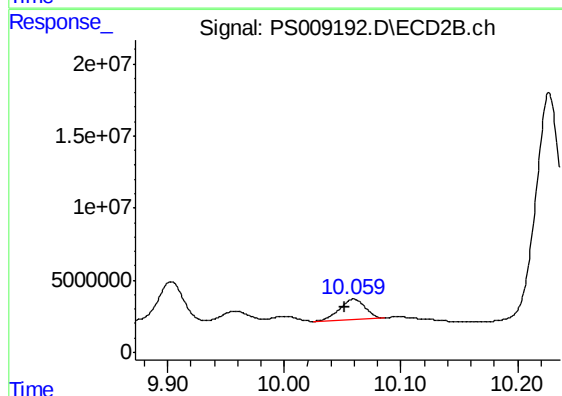


#14 DINOSEB

R.T.: 10.060 min
Delta R.T.: 0.008 min
Response: 21122005
Conc: 5.34 ng/ml

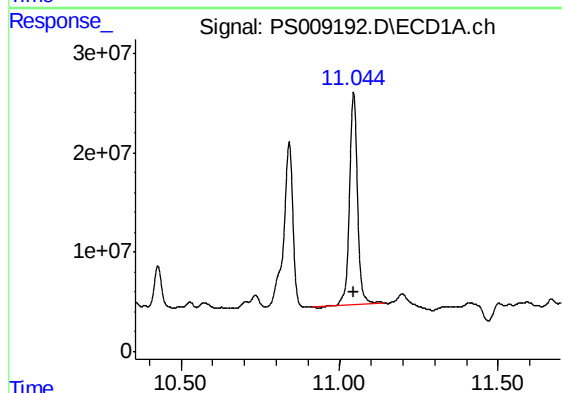


#15 Picloram

R.T.: 11.044 min
Delta R.T.: 0.001 min
Response: 371302850
Conc: 27.12 ng/ml

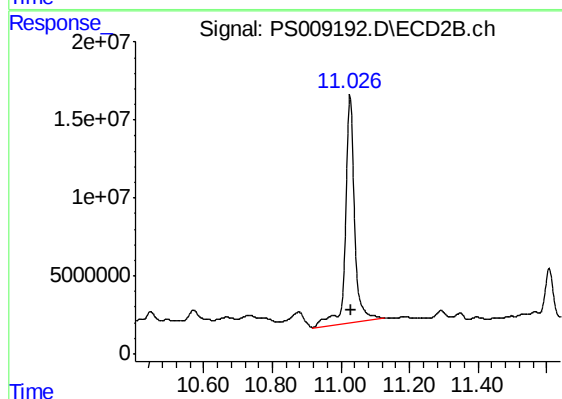

#15 Picloram


R.T.: 11.027 min
Delta R.T.: -0.004 min
Response: 264822060
Conc: 36.44 ng/ml

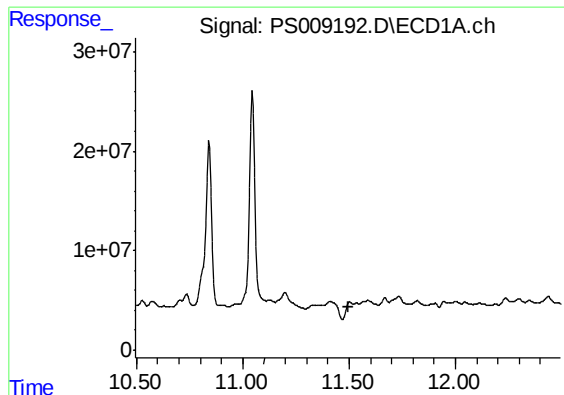

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.495 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
DN1

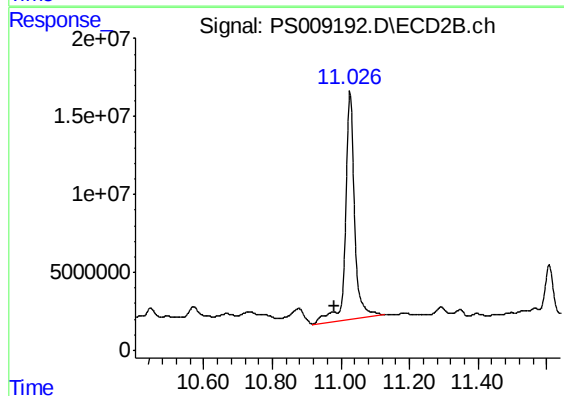

#16 DCPA

R.T.: 11.027 min
Delta R.T.: 0.044 min
Response: 264822060
Conc: 38.27 ng/ml