

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030921\
 Data File : PS014205.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Mar 2021 18:44
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 07:52:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS030521.M
 Quant Title : 8080.M
 QLast Update : Sat Mar 06 03:17:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.207	6.905	441.1E6	204.8E6	438.095	538.348
Target Compounds							
2) T	3,5-DICHL...	6.469f	0.000	6347440	0	4.590	N.D. #
6) T	MCP	0.000	7.139	0	6939794	N.D.	5.236
14) T	DINOSEB	11.201	0.000	2421110	0	<MDL	N.D. #
15) T	Picloram	10.997	10.990	9983496	931444	1.251	<MDL #
16) T	DCPA	0.000	10.885	0	779620	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030921\
Data File : PS014205.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Mar 2021 18:44
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 07:52:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS030521.M
Quant Title : 8080.M
QLast Update : Sat Mar 06 03:17:26 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

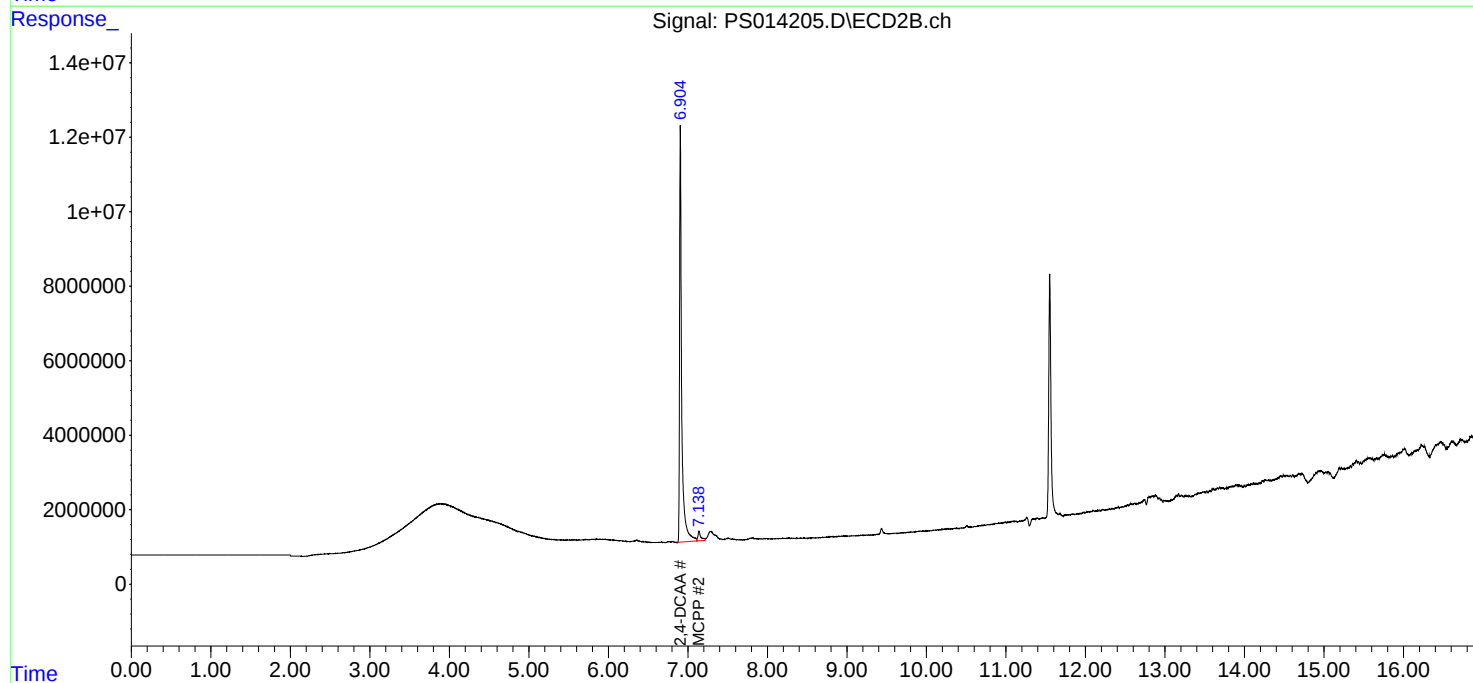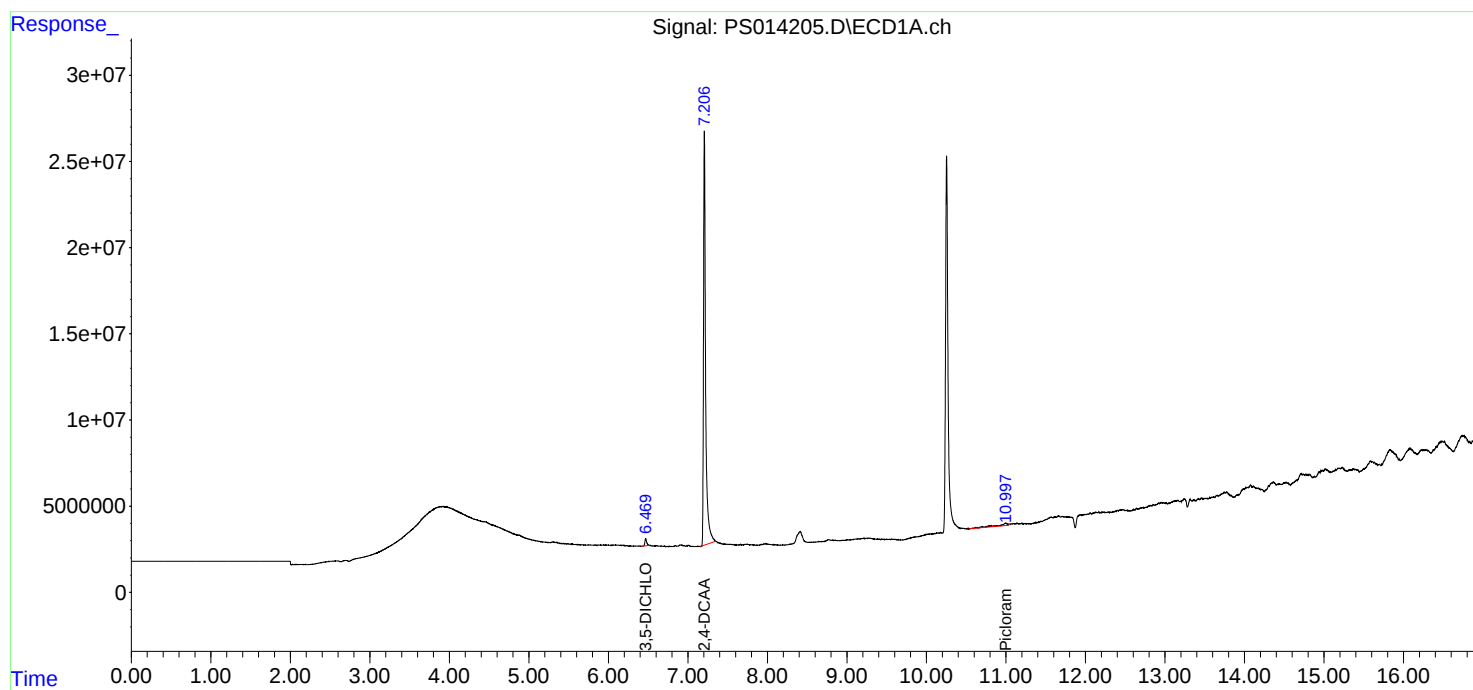


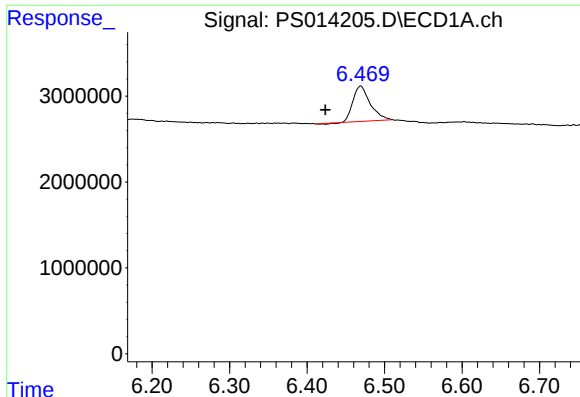

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.469 min
Delta R.T.: 0.045 min
Response: 6347440
Conc: 4.59 ng/ml

Instrument :
ECD_S
ClientSampleId :

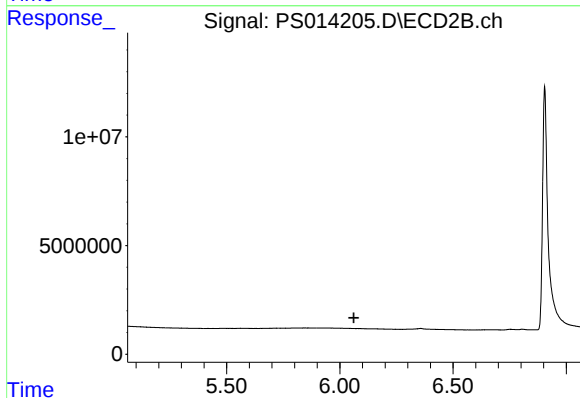


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.062 min
Response: 0
Conc: N.D.

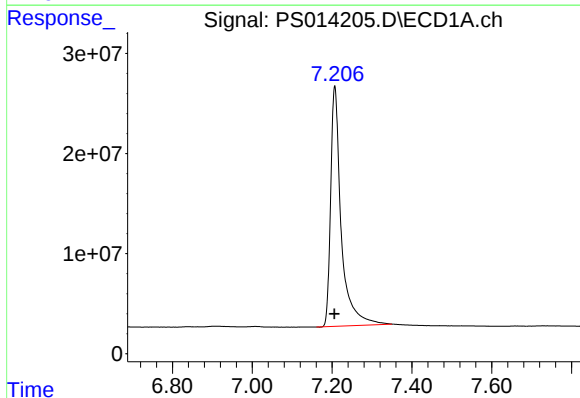


#4 2,4-DCAA

R.T.: 7.207 min
Delta R.T.: 0.001 min
Response: 441149900
Conc: 438.09 ng/ml

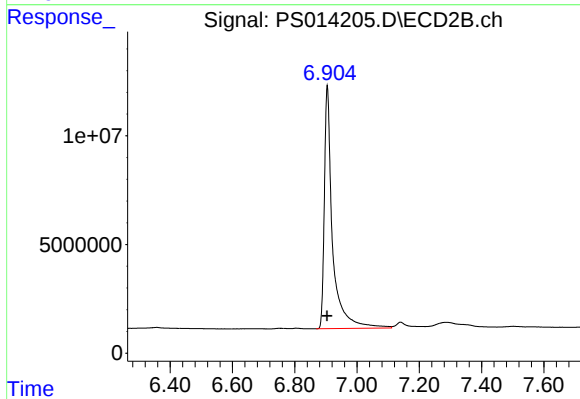

#4 2,4-DCAA


R.T.: 6.905 min
Delta R.T.: 0.000 min
Response: 204812827
Conc: 538.35 ng/ml

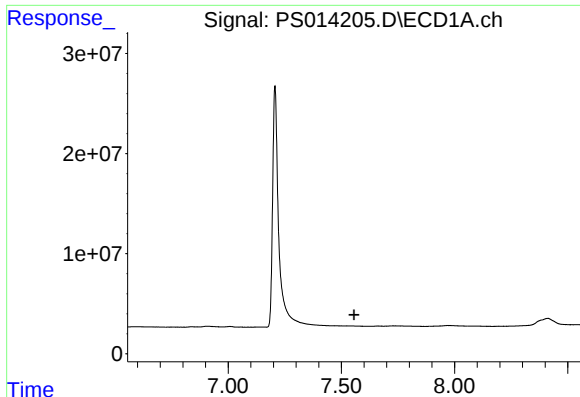

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 7.556 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

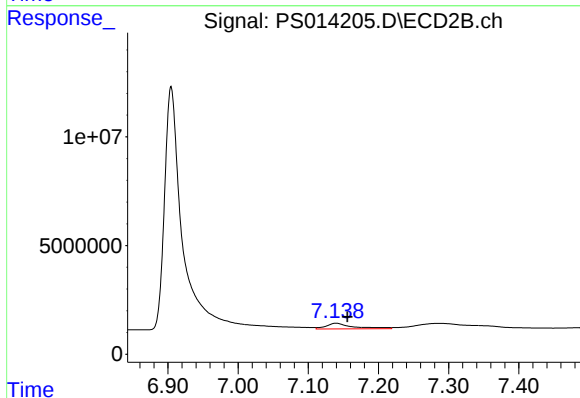


#6 MCPP

R.T.: 7.139 min
Delta R.T.: -0.017 min
Response: 6939794
Conc: 5.24 ug/ml

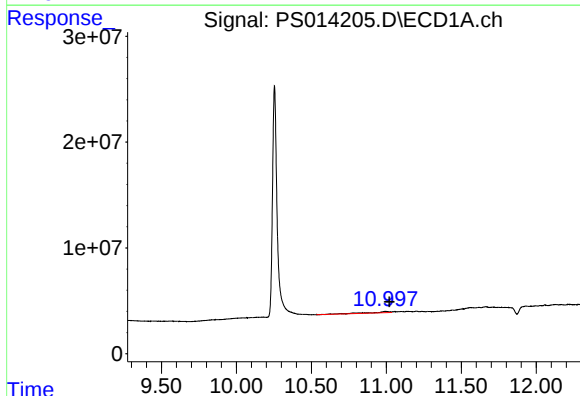

#15 Picloram

R.T.: 10.997 min
Delta R.T.: -0.024 min
Response: 9983496
Conc: 1.25 ng/ml

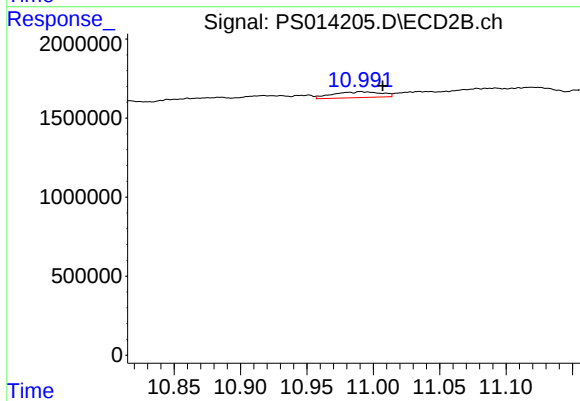

#15 Picloram

R.T.: 10.990 min
Delta R.T.: -0.017 min
Response: 931444
Conc: N.D.