

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030921\
 Data File : PS014203.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Mar 2021 17:58
 Operator : DD\AJ
 Sample : M1590-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 FK-EF-01-018-ABCD

Manual Integrations
 APPROVED

Ankita
 3/10/2021 10:16:23 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 07:51:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS030521.M
 Quant Title : 8080.M
 QLast Update : Sat Mar 06 03:17:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.203	6.900	242.3E6	100.1E6	240.640	263.114m

Target Compounds

 (f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030921\
Data File : PS014203.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Mar 2021 17:58
Operator : DD\AJ
Sample : M1590-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
FK-EF-01-018-ABCD


Manual Integrations
APPROVED

Ankita
3/10/2021 10:16:23 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 07:51:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS030521.M
Quant Title : 8080.M
QLast Update : Sat Mar 06 03:17:26 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

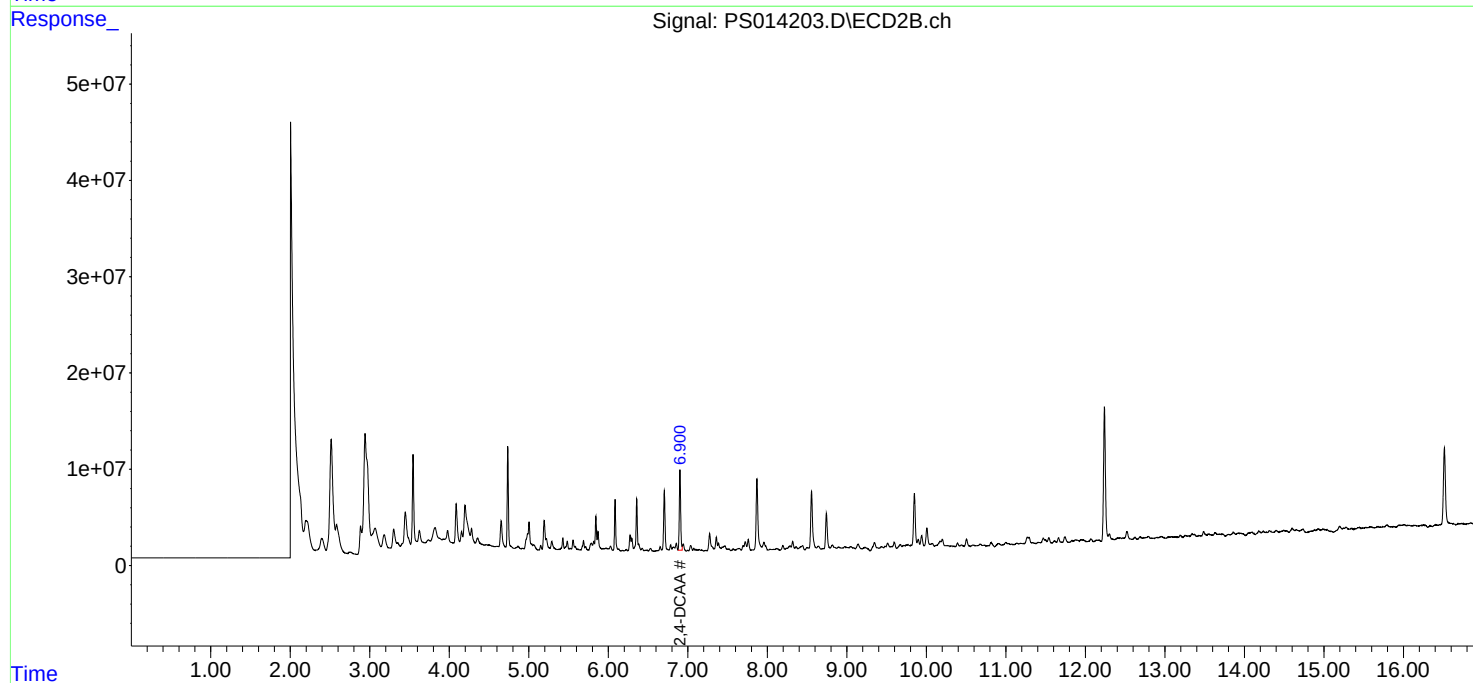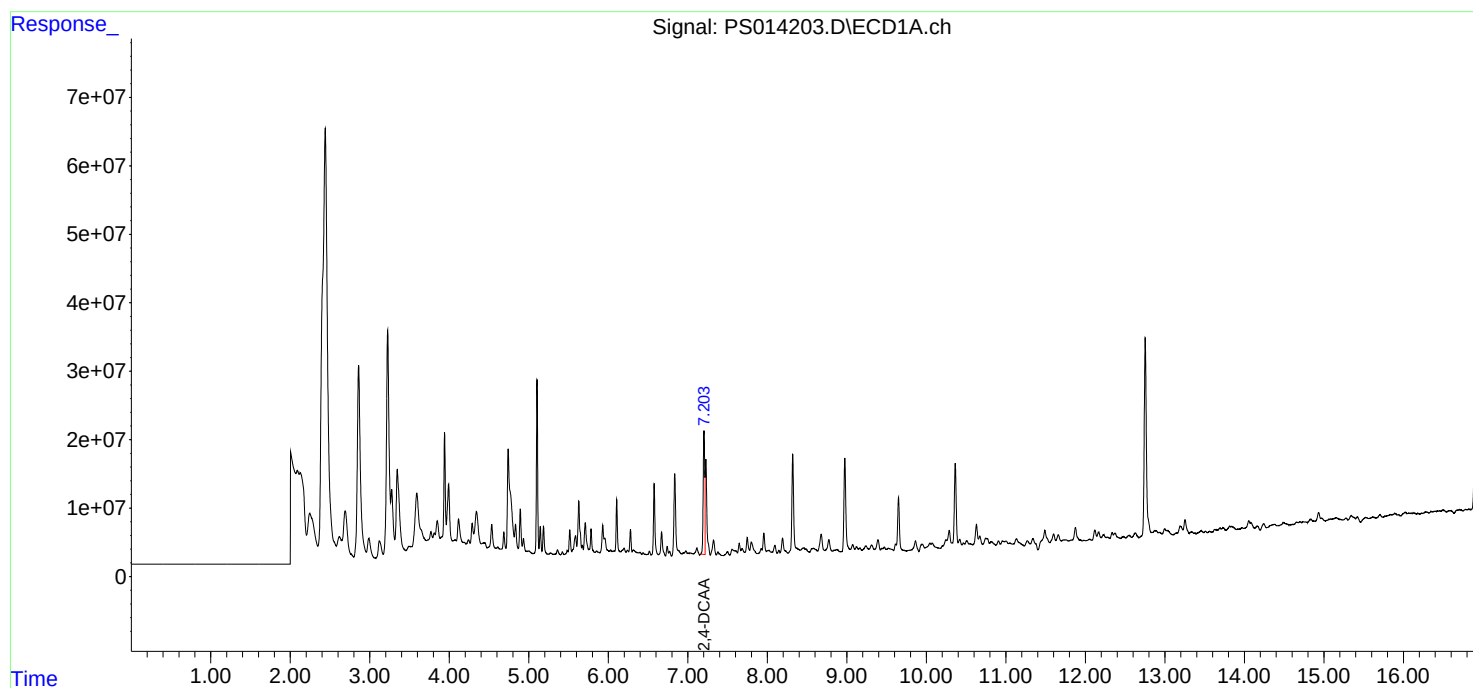

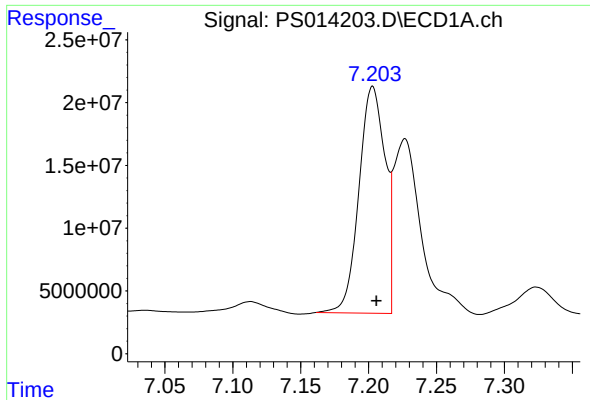


#4 2,4-DCAA

R.T.: 7.203 min
Delta R.T.: -0.003 min
Response: 242318622
Conc: 240.64 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-EF-01-018-ABCD

Manual Integrations
APPROVED

Ankita
3/10/2021 10:16:23 AM

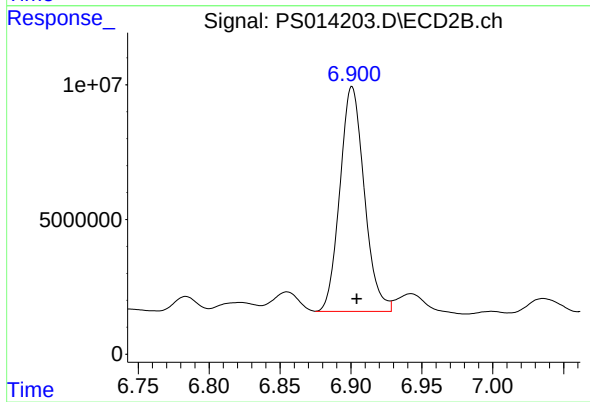

#4 2,4-DCAA

R.T.: 6.900 min
Delta R.T.: -0.004 min
Response: 100100851
Conc: 263.11 ng/ml m