

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031021\
 Data File : PS014208.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Mar 2021 08:37
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 12:49:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS030521.M
 Quant Title : 8080.M
 QLast Update : Sat Mar 06 03:17:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.207	6.905	445.4E6	209.5E6	442.321	550.736
Target Compounds							
2) T	3,5-DICHL...	6.470f	0.000	8289950	0	5.995	N.D. #
6) T	MCP	0.000	7.139	0	9707111	N.D.	7.323
15) T	Picloram	11.085f	11.071f	19690210	10258869	2.467	3.108 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031021\
Data File : PS014208.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Mar 2021 08:37
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 12:49:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS030521.M
Quant Title : 8080.M
QLast Update : Sat Mar 06 03:17:26 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

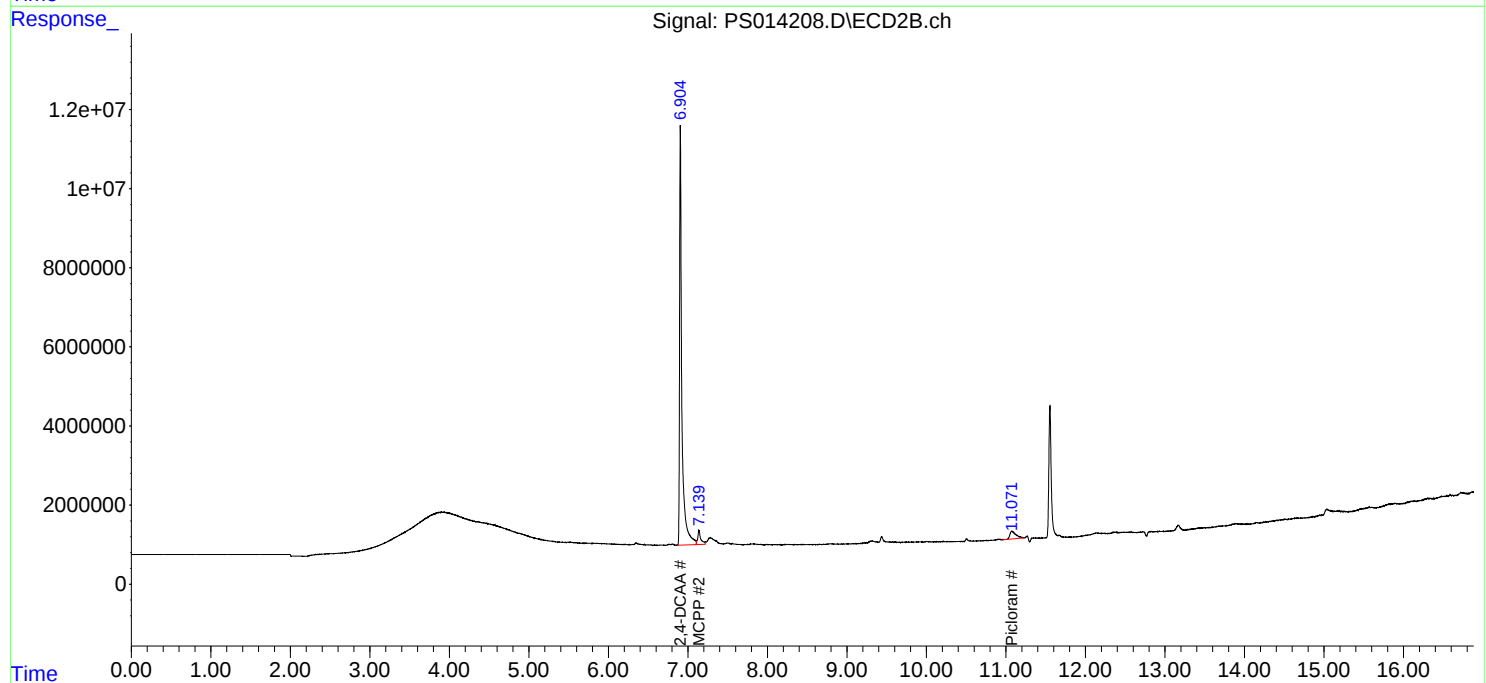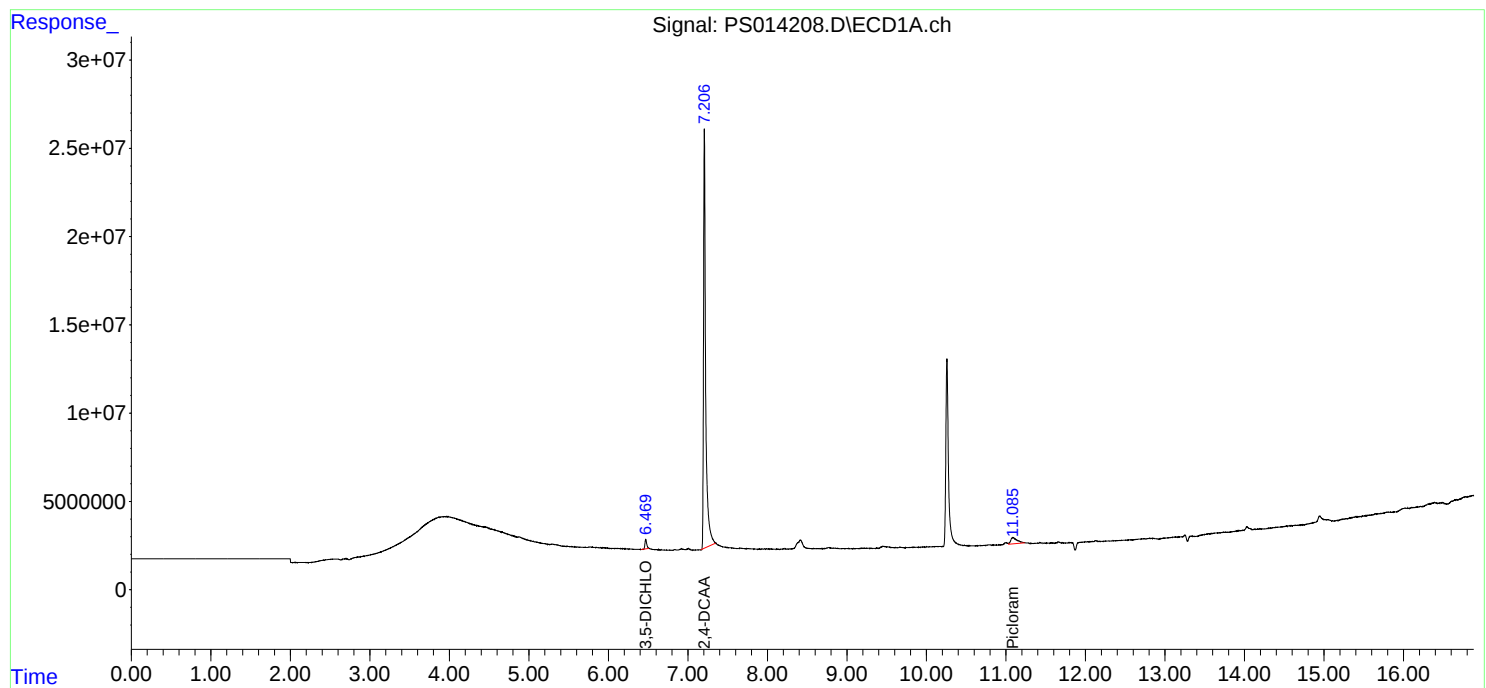


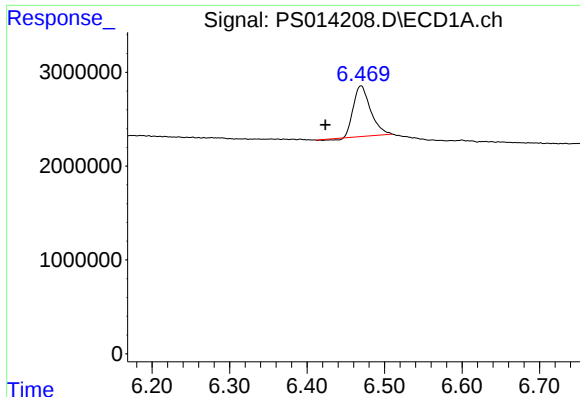

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.470 min
Delta R.T.: 0.046 min
Response: 8289950
Conc: 5.99 ng/ml

Instrument :
ECD_S
ClientSampleId :

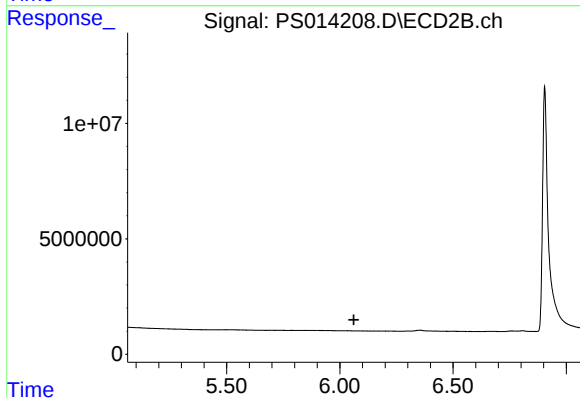


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.062 min
Response: 0
Conc: N.D.

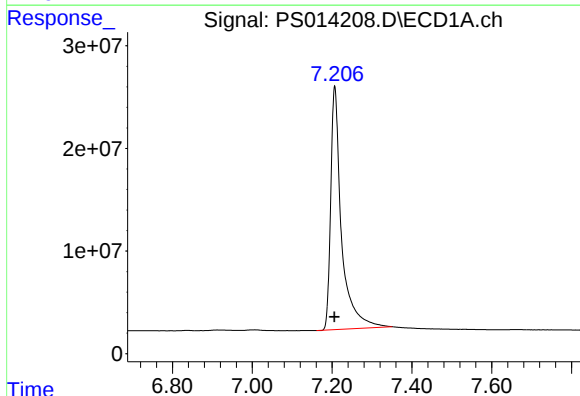


#4 2,4-DCAA

R.T.: 7.207 min
Delta R.T.: 0.000 min
Response: 445405787
Conc: 442.32 ng/ml

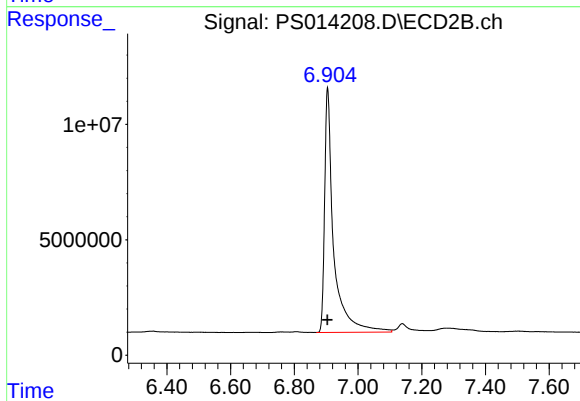

#4 2,4-DCAA


R.T.: 6.905 min
Delta R.T.: 0.000 min
Response: 209526098
Conc: 550.74 ng/ml

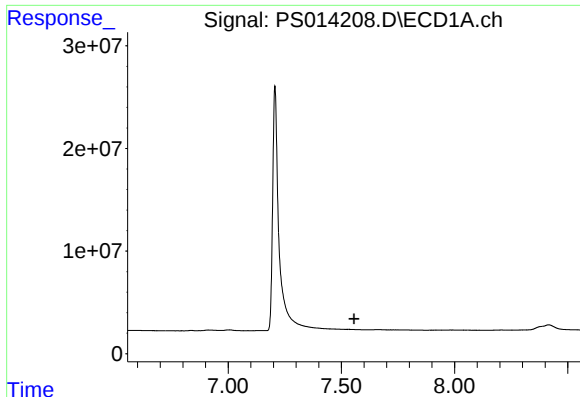

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.556 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

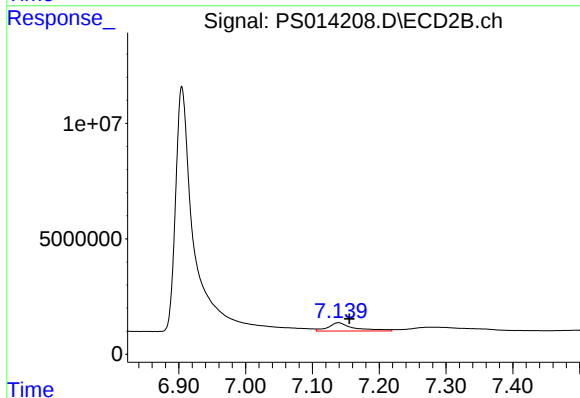


#6 MCP

R.T.: 7.139 min
Delta R.T.: -0.017 min
Response: 9707111
Conc: 7.32 ug/ml

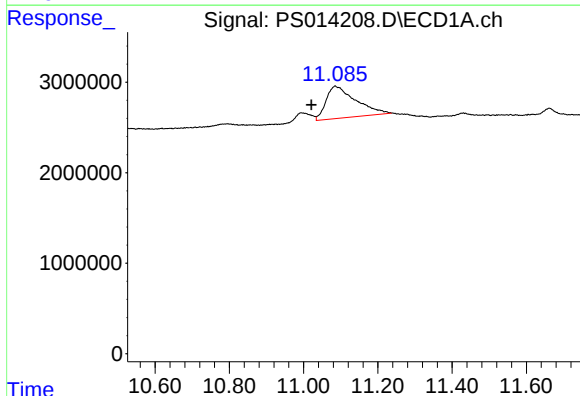

#15 Picloram

R.T.: 11.085 min
Delta R.T.: 0.064 min
Response: 19690210
Conc: 2.47 ng/ml

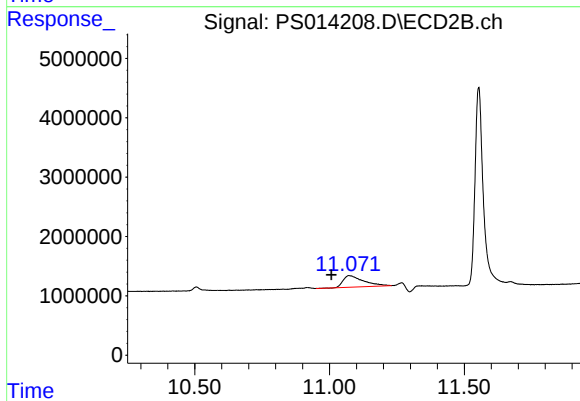

#15 Picloram

R.T.: 11.071 min
Delta R.T.: 0.064 min
Response: 10258869
Conc: 3.11 ng/ml