

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS031021\  
 Data File : PS014215.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 10 Mar 2021 13:40  
 Operator : DD\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 10 17:20:14 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS030521.M  
 Quant Title : 8080.M  
 QLast Update : Sat Mar 06 03:17:26 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound     | RT#1    | RT#2   | Resp#1   | Resp#2  | ng/ml   | ng/ml   |
|-----------------------------|--------------|---------|--------|----------|---------|---------|---------|
| -----                       |              |         |        |          |         |         |         |
| System Monitoring Compounds |              |         |        |          |         |         |         |
| 4) S                        | 2,4-DCAA     | 7.207   | 6.900  | 451.0E6  | 196.9E6 | 447.875 | 517.491 |
| Target Compounds            |              |         |        |          |         |         |         |
| 2) T                        | 3,5-DICHL... | 6.468f  | 0.000  | 11694059 | 0       | 8.456   | N.D. #  |
| 5) T                        | DICAMBA      | 0.000   | 7.055  | 0        | 331709  | N.D.    | <MDL    |
| 6) T                        | MCP          | 0.000   | 7.133  | 0        | 7760431 | N.D.    | 5.855   |
| 8) T                        | DICHLORPROP  | 8.123   | 0.000  | 4538875  | 0       | 4.649   | N.D. #  |
| 15) T                       | Picloram     | 10.976f | 10.988 | 3798125  | 1058093 | <MDL    | <MDL #  |
| 16) T                       | DCPA         | 0.000   | 10.914 | 0        | 1130849 | N.D.    | <MDL    |
| -----                       |              |         |        |          |         |         |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS031021\  
Data File : PS014215.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 10 Mar 2021 13:40  
Operator : DD\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Mar 10 17:20:14 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS030521.M  
Quant Title : 8080.M  
QLast Update : Sat Mar 06 03:17:26 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

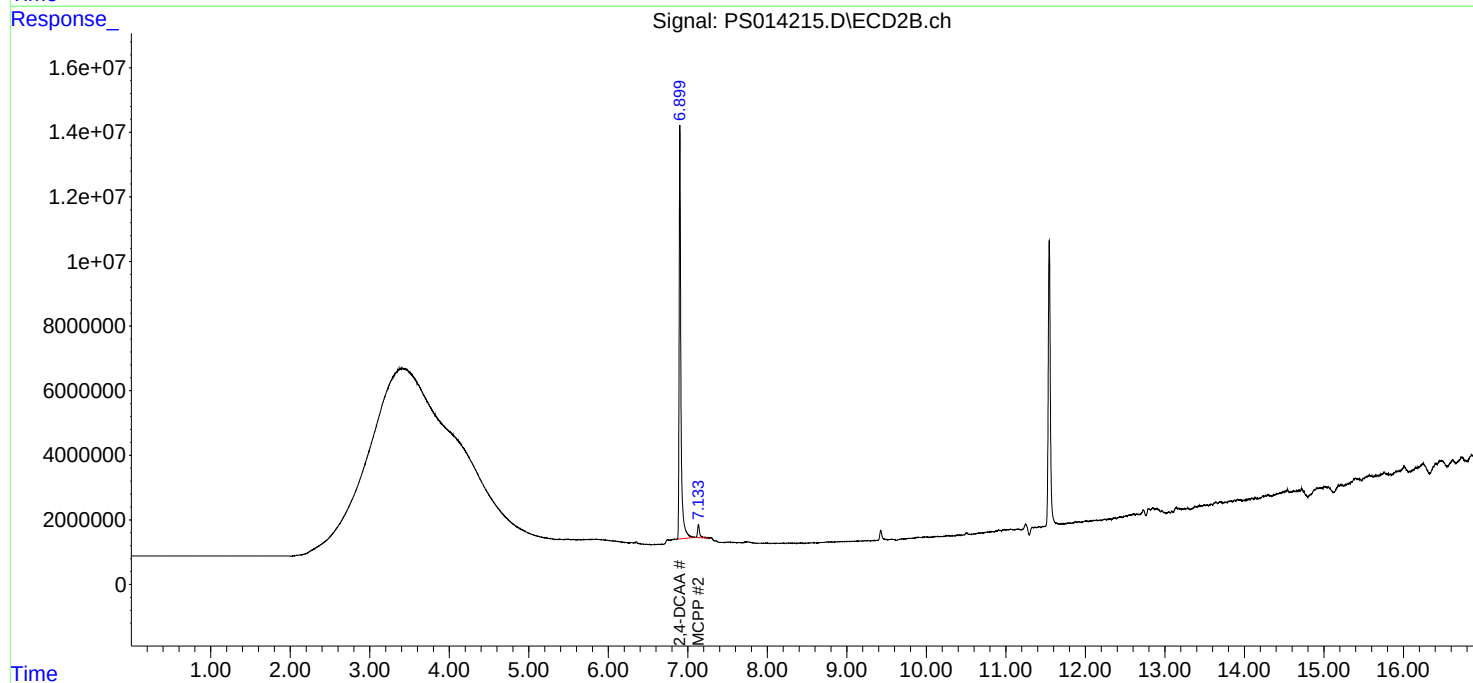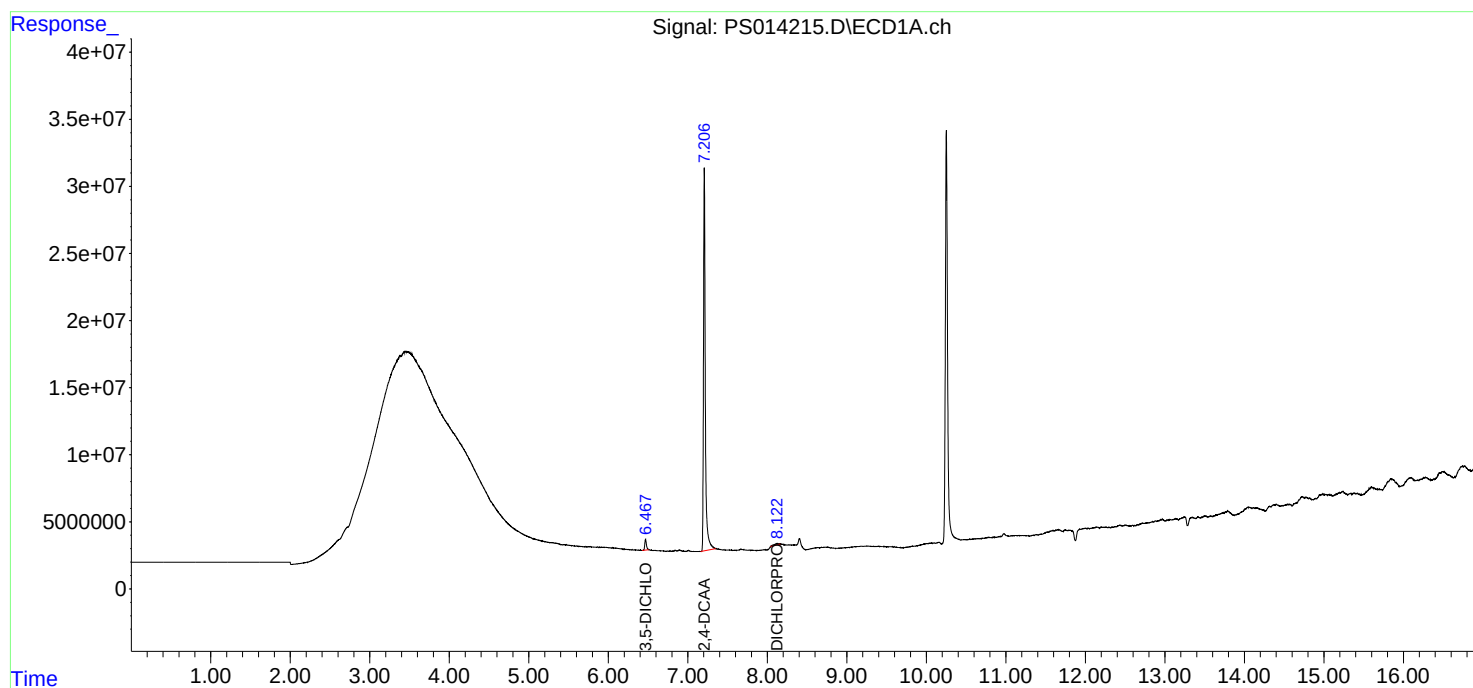


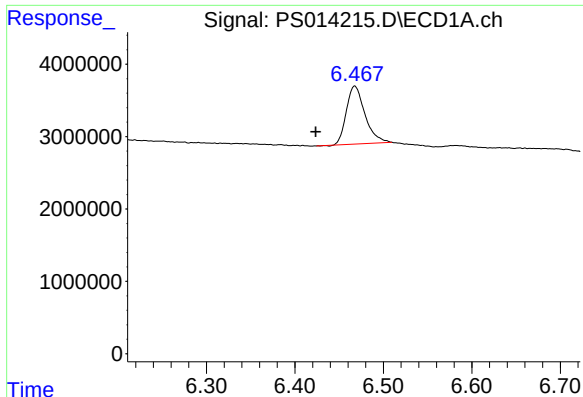

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.468 min  
Delta R.T.: 0.044 min  
Response: 11694059  
Conc: 8.46 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

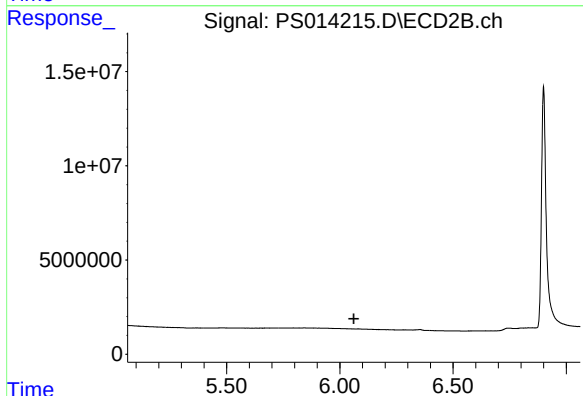


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min  
Exp R.T. : 6.062 min  
Response: 0  
Conc: N.D.

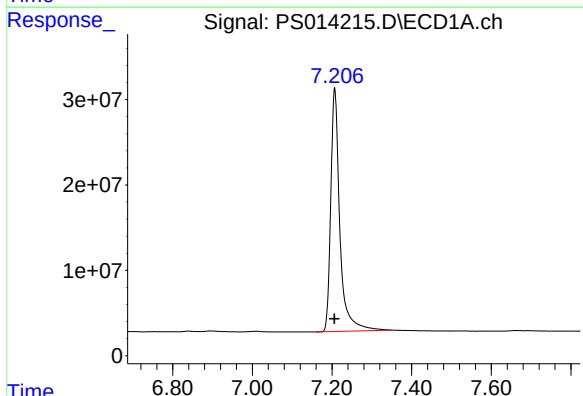


#4 2,4-DCAA

R.T.: 7.207 min  
Delta R.T.: 0.001 min  
Response: 450998189  
Conc: 447.87 ng/ml

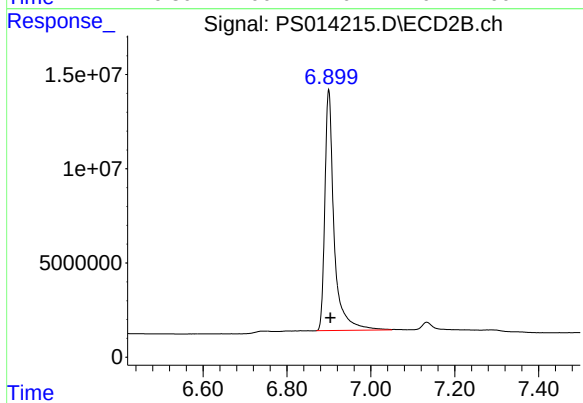

#4 2,4-DCAA


R.T.: 6.900 min  
Delta R.T.: -0.004 min  
Response: 196878040  
Conc: 517.49 ng/ml

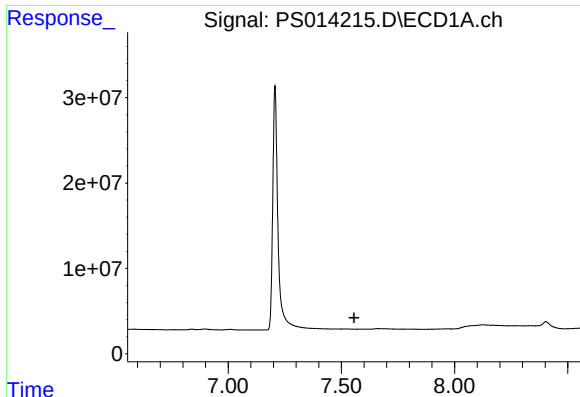

#6 MCPP


R.T.: 0.000 min  
Exp R.T.: 7.556 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :

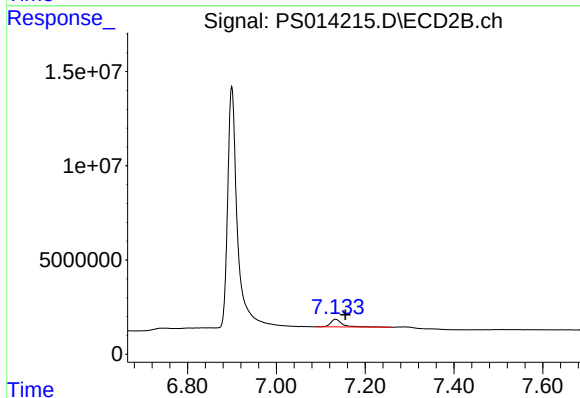


#6 MCPP

R.T.: 7.133 min  
Delta R.T.: -0.023 min  
Response: 7760431  
Conc: 5.85 ug/ml

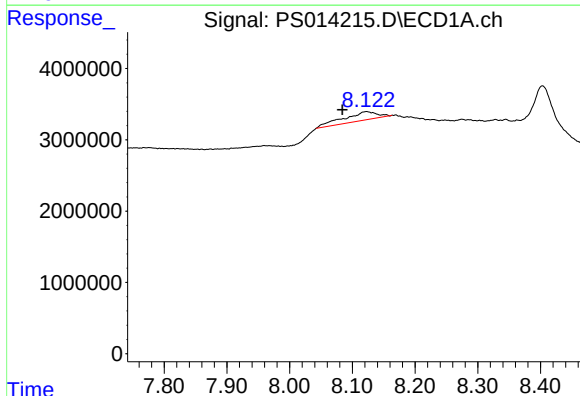

#8 DICHLORPROP

R.T.: 8.123 min  
Delta R.T.: 0.038 min  
Response: 4538875  
Conc: 4.65 ng/ml

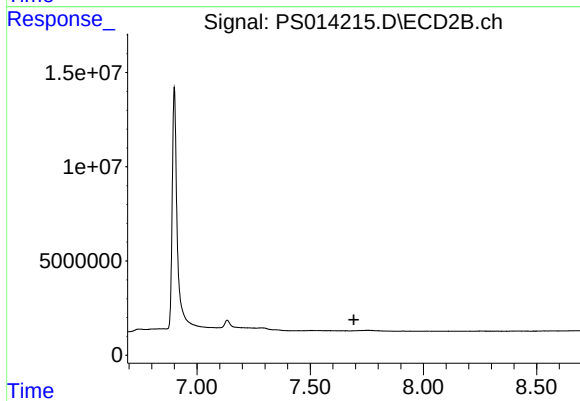

#8 DICHLORPROP

R.T.: 0.000 min  
Exp R.T.: 7.693 min  
Response: 0  
Conc: N.D.