

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031021\
 Data File : PS014210.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Mar 2021 10:13
 Operator : DD\AJ
 Sample : M1589-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 FK-GF-02-067-A

Manual Integrations
 APPROVED

Ankita
 3/11/2021 9:21:41 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 12:50:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS030521.M
 Quant Title : 8080.M
 QLast Update : Sat Mar 06 03:17:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.203	6.896	675.8E6	284.8E6	671.109m	748.702m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031021\
Data File : PS014210.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Mar 2021 10:13
Operator : DD\AJ
Sample : M1589-01
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
FK-GF-02-067-A


Manual Integrations
APPROVED

Ankita
3/11/2021 9:21:41 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 12:50:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS030521.M
Quant Title : 8080.M
QLast Update : Sat Mar 06 03:17:26 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

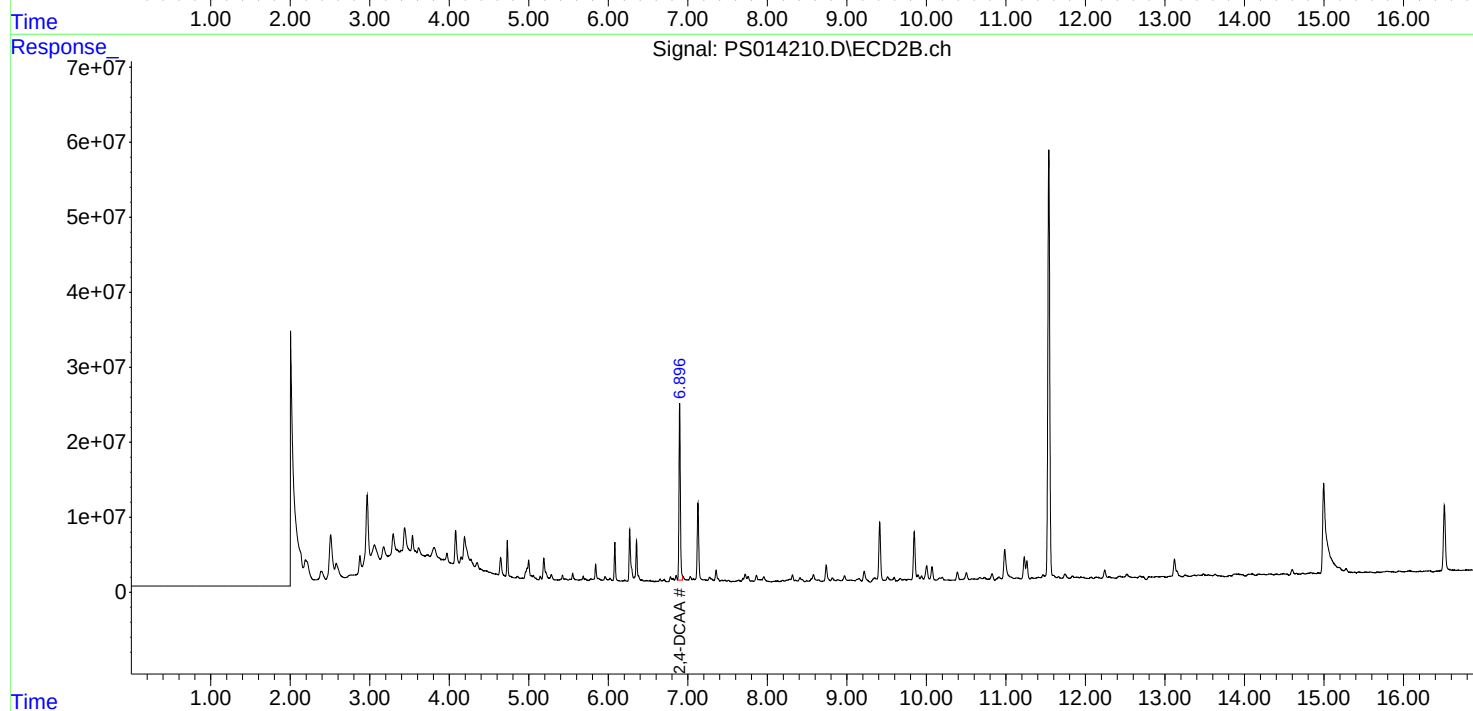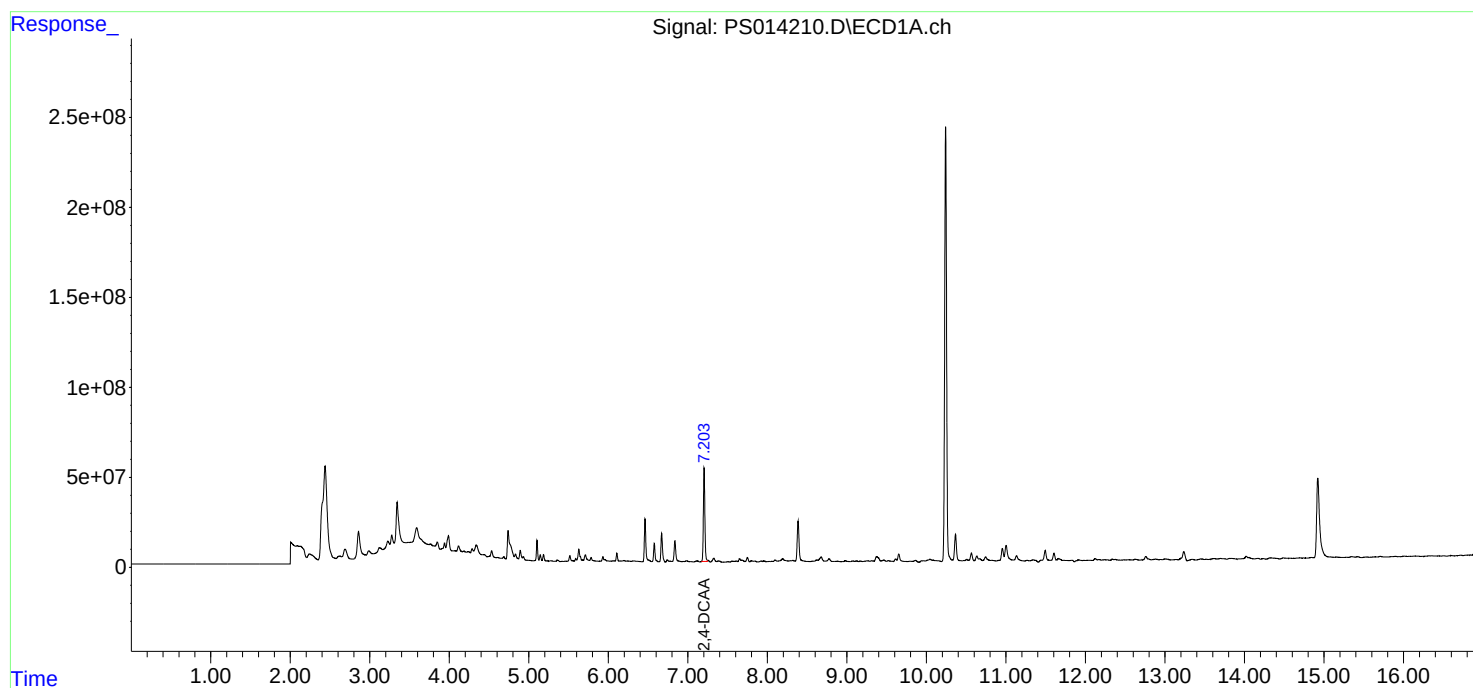

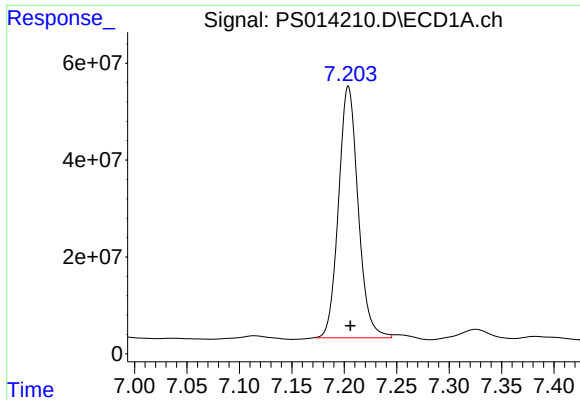


#4 2,4-DCAA

R.T.: 7.203 min
Delta R.T.: -0.002 min
Response: 675789753
Conc: 671.11 ng/ml m

Instrument :
ECD_S
ClientSampleId :
FK-GF-02-067-A

Manual Integrations
APPROVED

Ankita
3/11/2021 9:21:41 AM

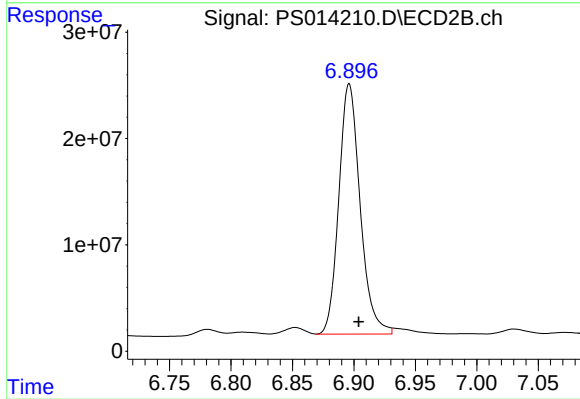

#4 2,4-DCAA

R.T.: 6.896 min
Delta R.T.: -0.008 min
Response: 284841593
Conc: 748.70 ng/ml m