

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031119\
 Data File : PS003490.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2019 09:21
 Operator : EI\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 01:15:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	10.794	0	1151470	N.D.	2.452 #
Target Compounds							
2) T	3,5-DICHL...	0.000	8.951	0	2248414	N.D.	3.641 #
5) T	DICAMBA	0.000	11.064	0	2339648	N.D.	1.400 #
8) T	DICHLORPROP	0.000	12.199	0	65174	N.D.	0.158 #
9) T	2,4-D	0.000	12.694	0	1065390	N.D.	2.030 #
10) T	Pentachlo...	13.515	13.198	9032417	6575471	1.279	0.998
11) T	2,4,5-TP ...	14.398	13.829	4054263	7166947	1.509	2.815 #
14) T	DINOSEB	17.003	15.465	3671326	2820853	1.635	1.580
15) T	Picloram	0.000	16.723	0	3468944	N.D.	1.367 #
16) T	DCPA	17.348	16.639	5389088	6211791	1.635	1.997



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031119\
Data File : PS003490.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2019 09:21
Operator : EI\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 01:15:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

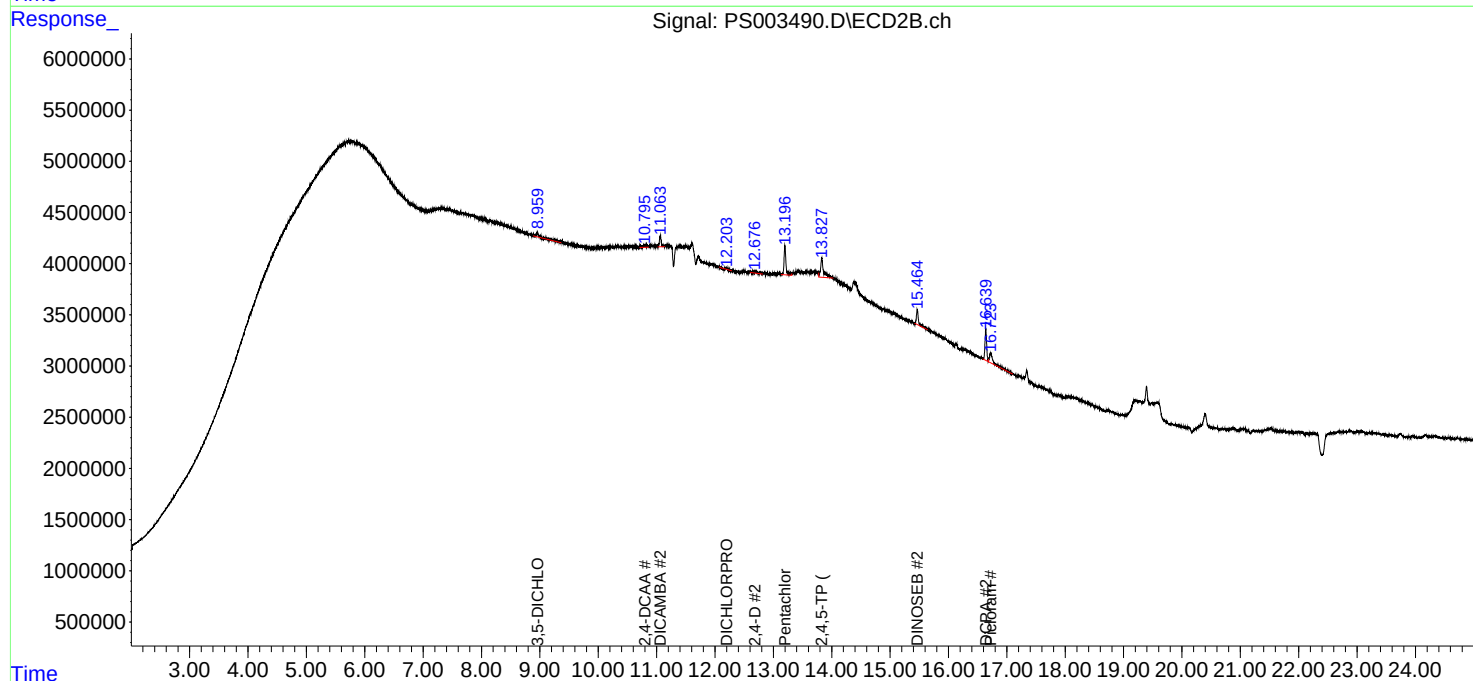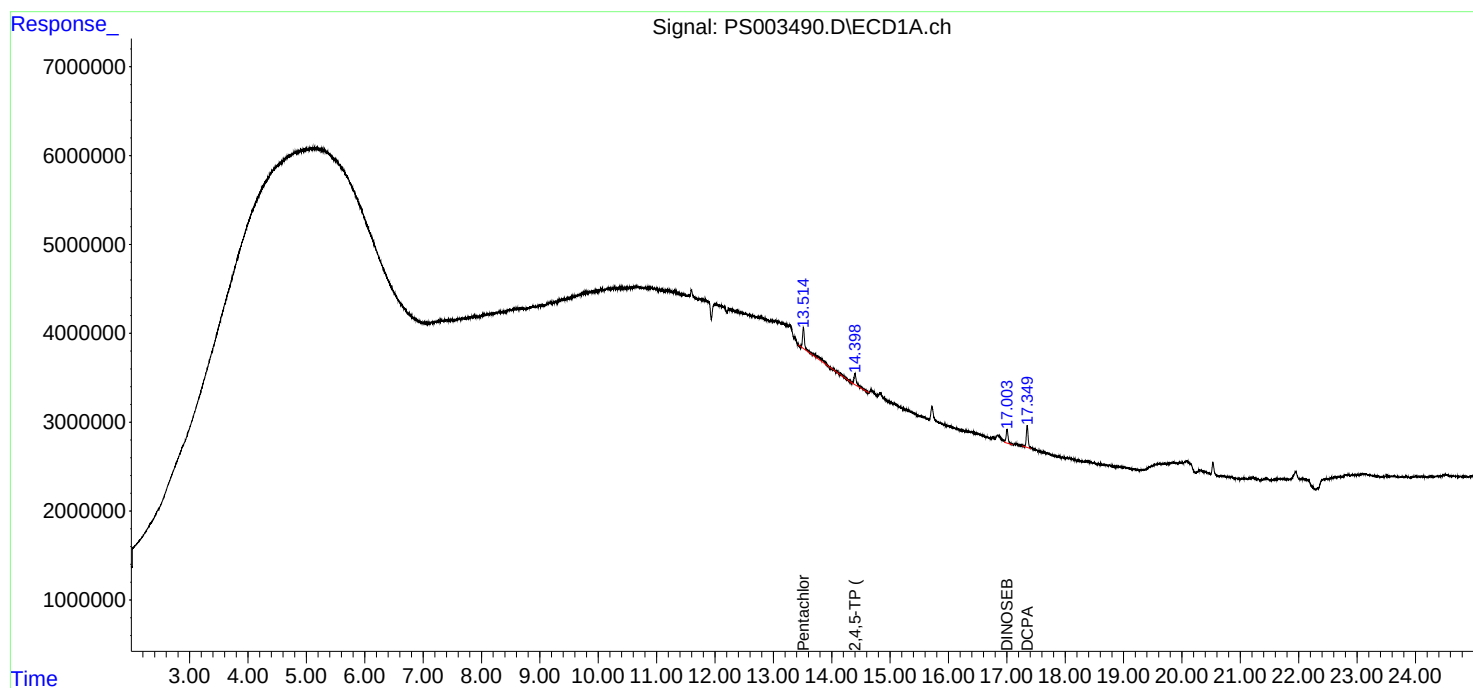


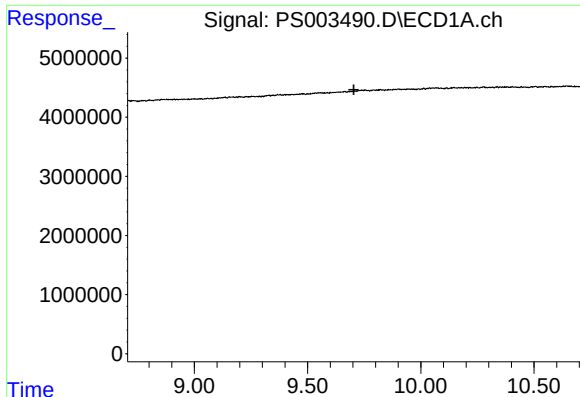

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.705 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

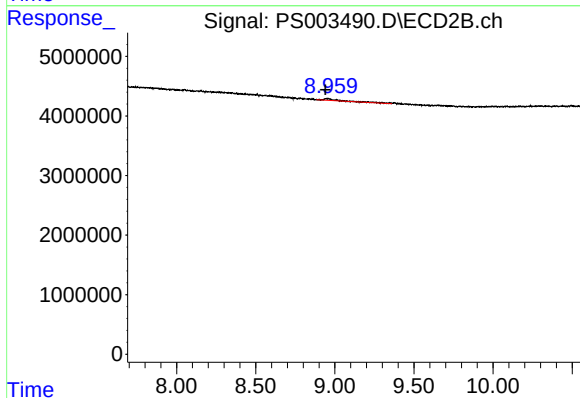


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 8.951 min
Delta R.T.: 0.012 min
Response: 2248414
Conc: 3.64 ng/ml

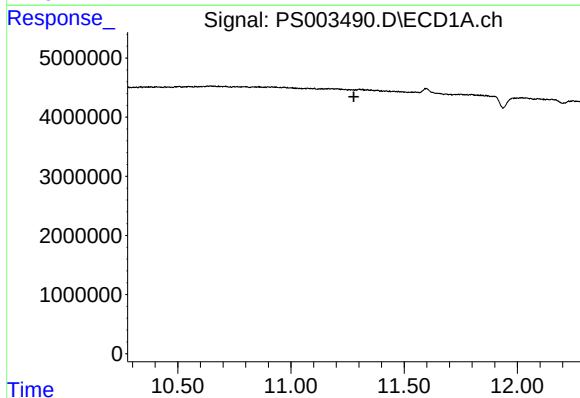


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 11.278 min
Response: 0
Conc: N.D.

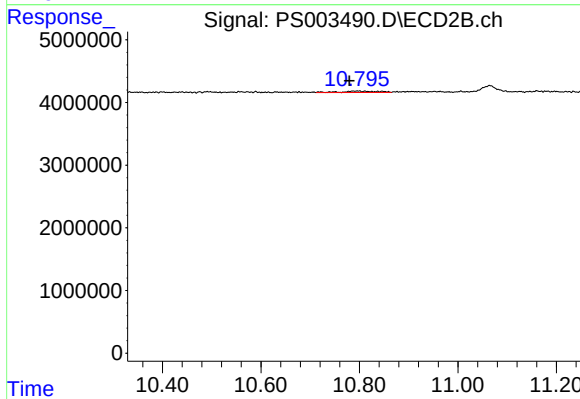

#4 2,4-DCAA


R.T.: 10.794 min
Delta R.T.: 0.014 min
Response: 1151470
Conc: 2.45 ng/ml

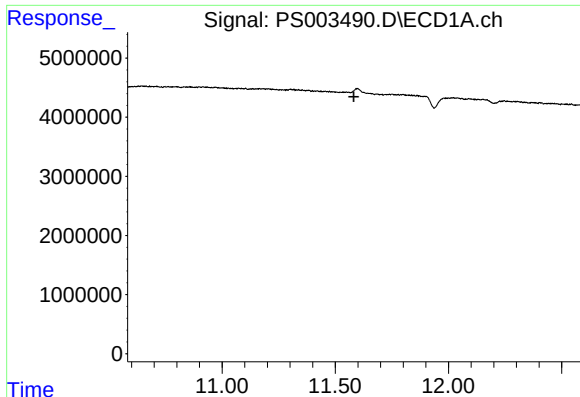

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.582 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

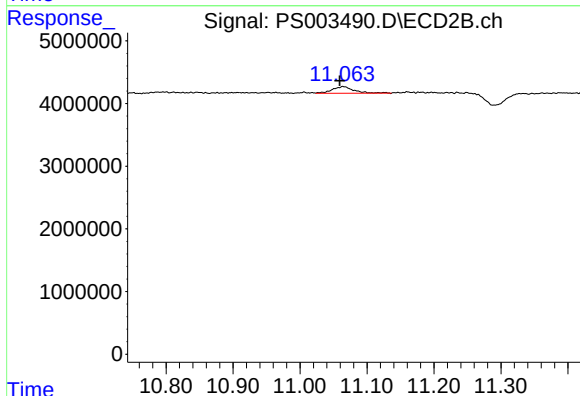


#5 DICAMBA

R.T.: 11.064 min
Delta R.T.: 0.004 min
Response: 2339648
Conc: 1.40 ng/ml

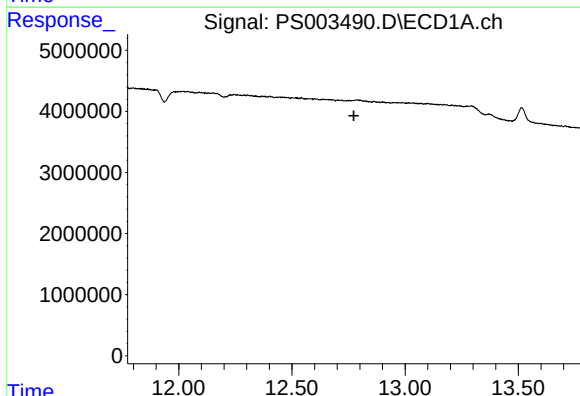


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 12.773 min
Response: 0
Conc: N.D.

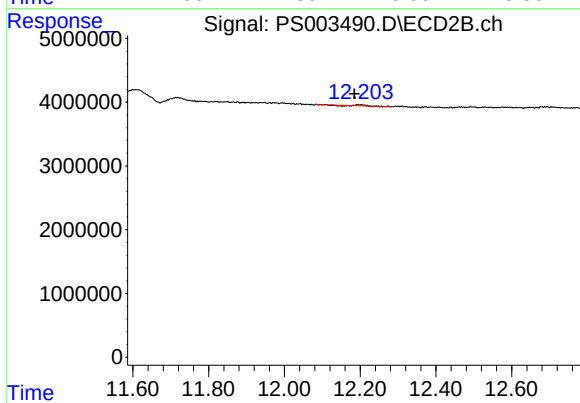

#8 DICHLORPROP


R.T.: 12.199 min
Delta R.T.: 0.014 min
Response: 65174
Conc: 0.16 ng/ml

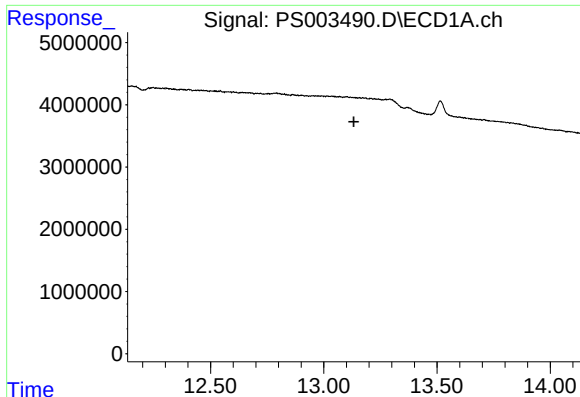

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.133 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

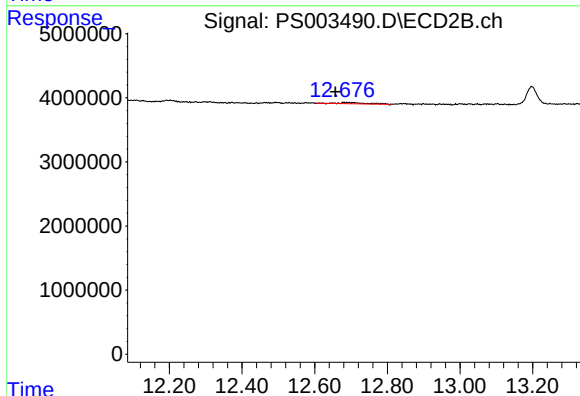


#9 2,4-D

R.T.: 12.694 min
Delta R.T.: 0.037 min
Response: 1065390
Conc: 2.03 ng/ml

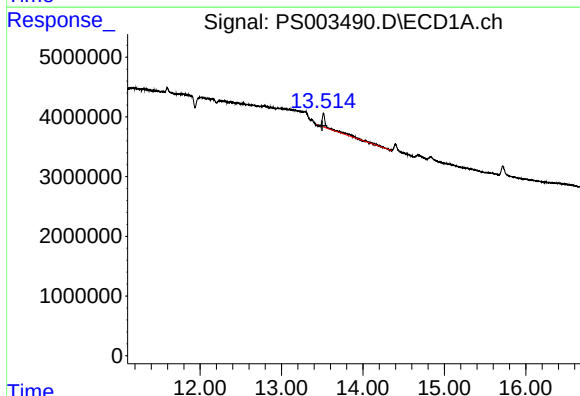


#10 Pentachlorophenol

R.T.: 13.515 min
Delta R.T.: 0.016 min
Response: 9032417
Conc: 1.28 ng/ml

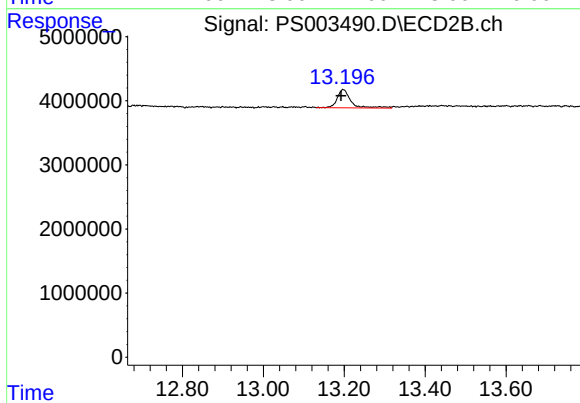

#10 Pentachlorophenol


R.T.: 13.198 min
Delta R.T.: 0.006 min
Response: 6575471
Conc: 1.00 ng/ml

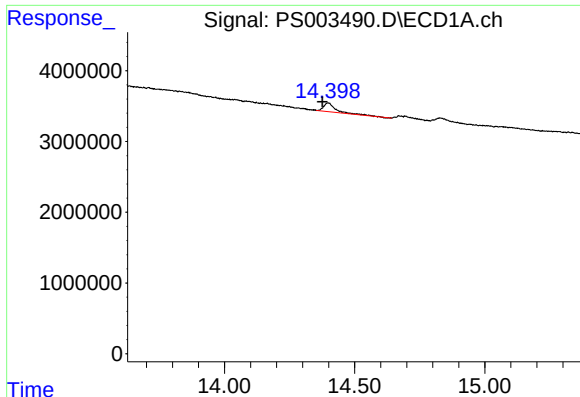

#11 2,4,5-TP (SILVEX)


R.T.: 14.398 min
Delta R.T.: 0.022 min
Response: 4054263
Conc: 1.51 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

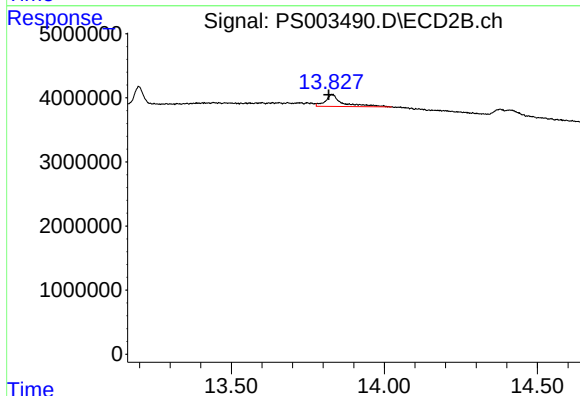


#11 2,4,5-TP (SILVEX)

R.T.: 13.829 min
Delta R.T.: 0.012 min
Response: 7166947
Conc: 2.81 ng/ml

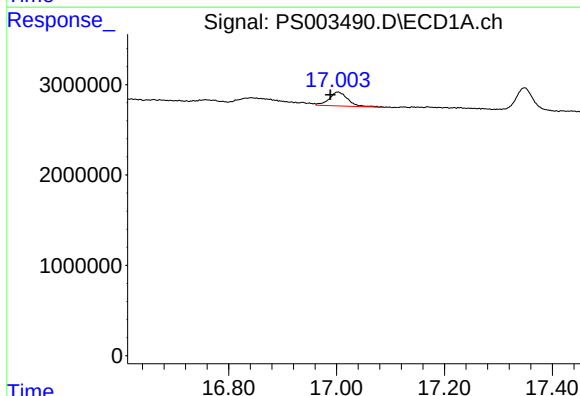


#14 DINOSEB

R.T.: 17.003 min
Delta R.T.: 0.014 min
Response: 3671326
Conc: 1.64 ng/ml

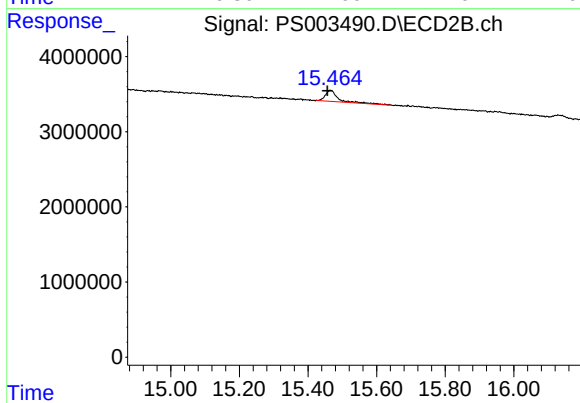

#14 DINOSEB


R.T.: 15.465 min
Delta R.T.: 0.009 min
Response: 2820853
Conc: 1.58 ng/ml

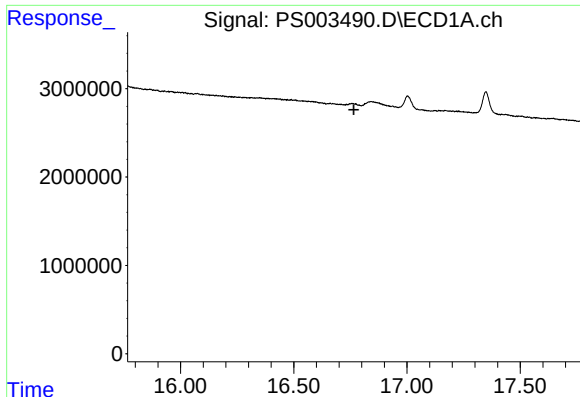

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 16.765 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

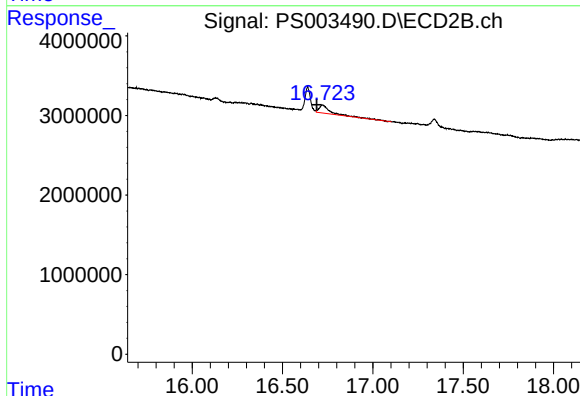


#15 Picloram

R.T.: 16.723 min
Delta R.T.: 0.034 min
Response: 3468944
Conc: 1.37 ng/ml

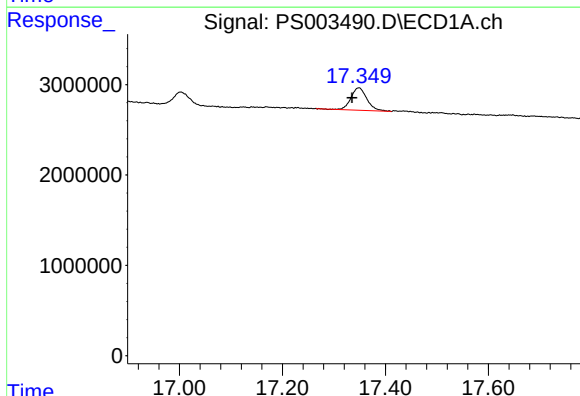

#16 DCPA

R.T.: 17.348 min
Delta R.T.: 0.013 min
Response: 5389088
Conc: 1.64 ng/ml

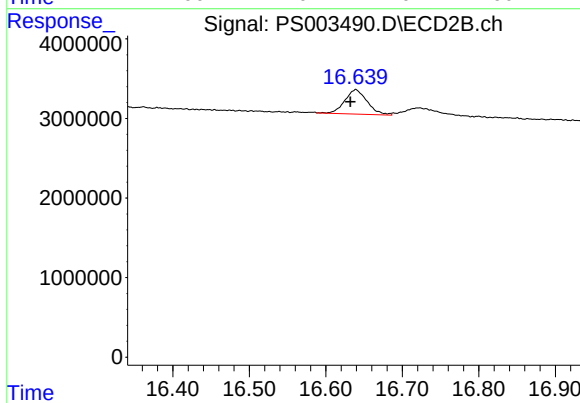

#16 DCPA

R.T.: 16.639 min
Delta R.T.: 0.007 min
Response: 6211791
Conc: 2.00 ng/ml