

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031119\
 Data File : PS003496.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2019 12:31
 Operator : EI\SJ
 Sample : K1693-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 01:17:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.294	10.795	182.4E6	201.3E6	415.568	428.612
Target Compounds							
1) T	Dalapon	2.807	2.292	19543766	12788167	30.070	20.197 #
2) T	3,5-DICHL...	0.000	8.959	0	6896476	N.D.	11.169 #
5) T	DICAMBA	0.000	11.036	0	4224965	N.D.	2.529 #
6) T	MCP	0.000	11.288	0	306641	N.D.	0.260 #
9) T	2,4-D	13.149	12.655	3771696	1607599	8.132	3.063 #
11) T	2,4,5-TP ...	0.000	13.805	0	1537489	N.D.	0.604 #
12) T	2,4,5-T	0.000	14.395	0	4608032	N.D.	2.285 #
13) T	2,4-DB	15.481	15.029	4182303	1806281	17.662	7.074 #
14) T	DINOSEB	0.000	15.438	0	1067624	N.D.	0.598 #
15) T	Picloram	0.000	16.744	0	12541408	N.D.	4.941 #
16) T	DCPA	0.000	16.563	0	4713484	N.D.	1.515 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031119\
Data File : PS003496.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2019 12:31
Operator : EI\SJ
Sample : K1693-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 01:17:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

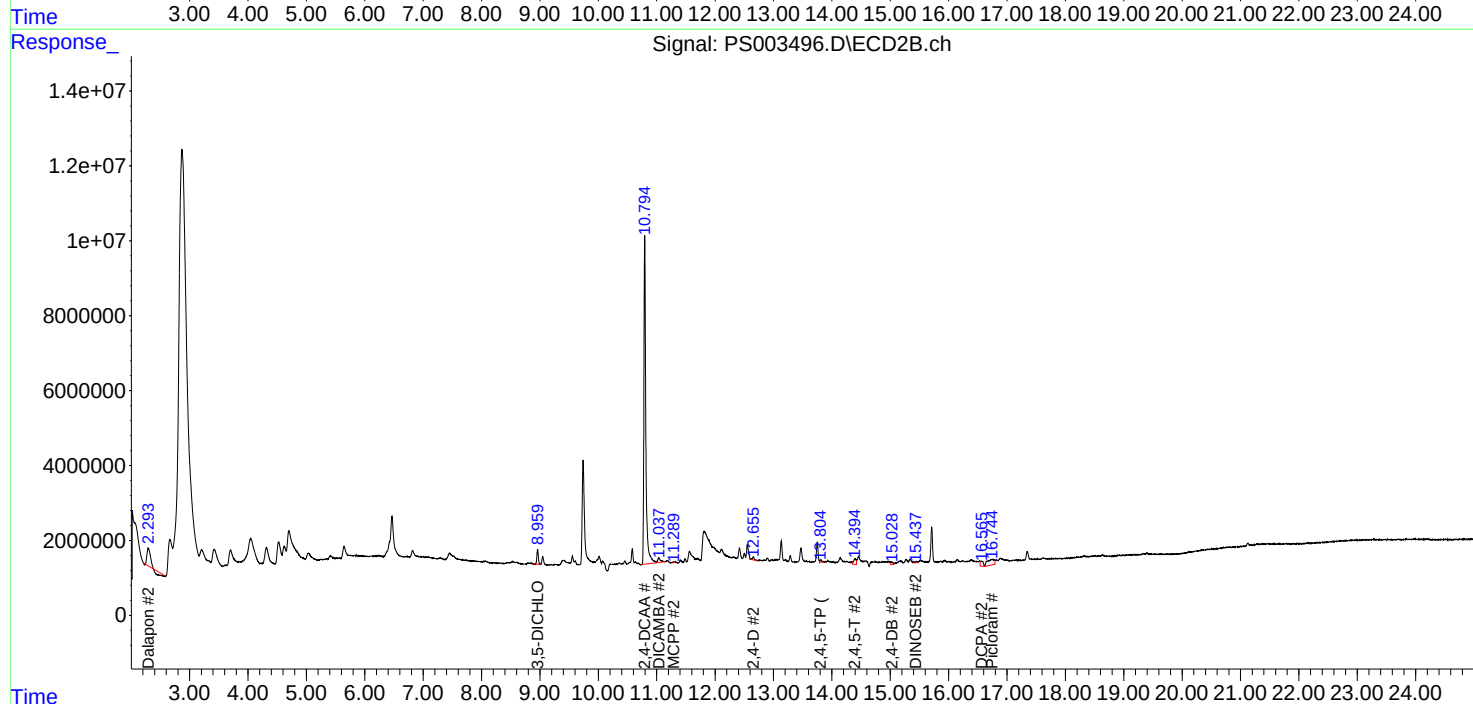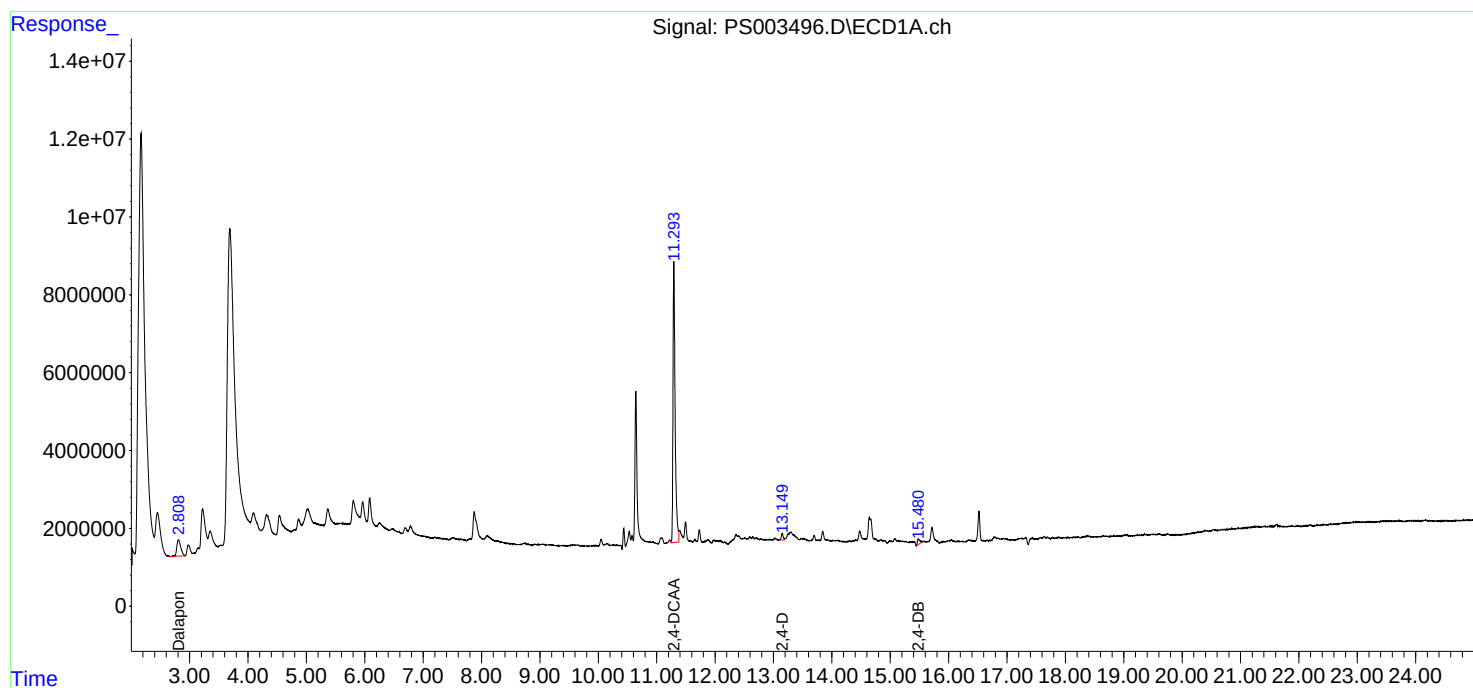


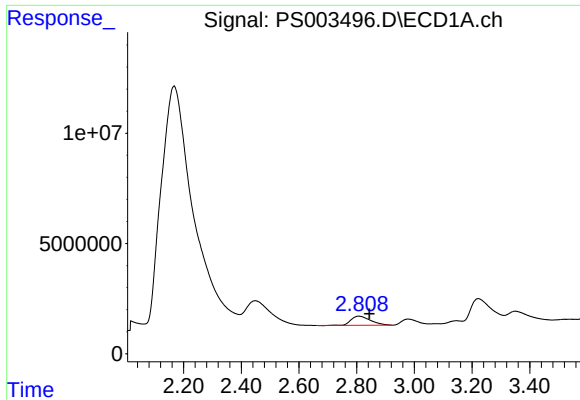

#1 Dalapon


R.T.: 2.807 min
Delta R.T.: -0.037 min
Response: 19543766
Conc: 30.07 ng/ml

Instrument :
ECD_S
ClientSampleId :

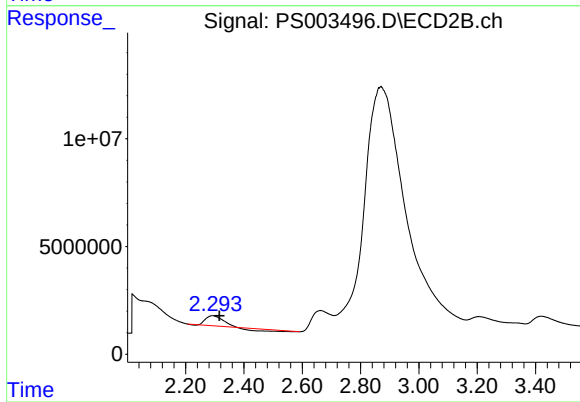


#1 Dalapon

R.T.: 2.292 min
Delta R.T.: -0.024 min
Response: 12788167
Conc: 20.20 ng/ml

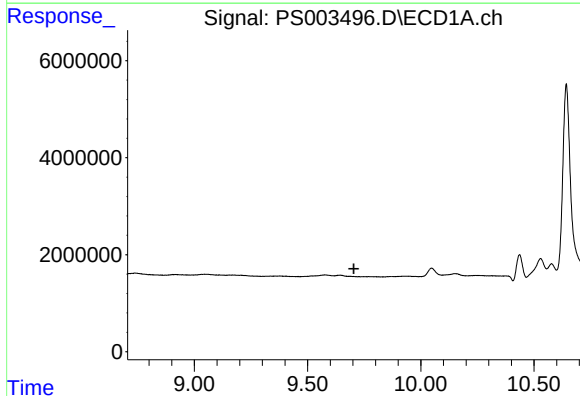


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.705 min
Response: 0
Conc: N.D.

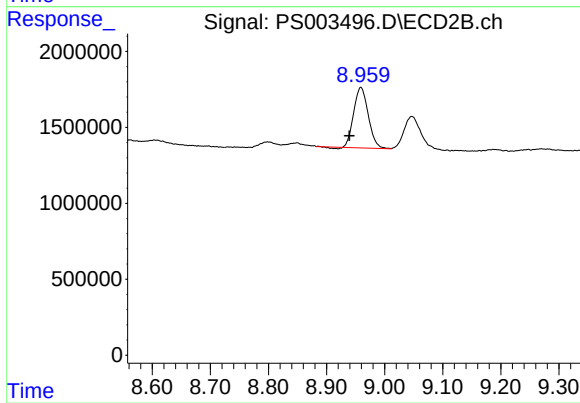

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.959 min
Delta R.T.: 0.020 min
Response: 6896476
Conc: 11.17 ng/ml

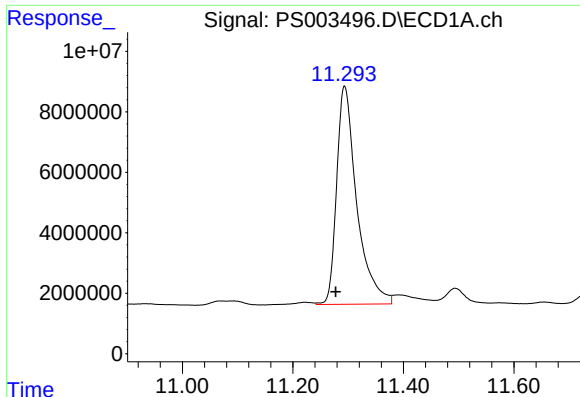

#4 2,4-DCAA


R.T.: 11.294 min
Delta R.T.: 0.016 min
Response: 182444694
Conc: 415.57 ng/ml

Instrument :
ECD_S
ClientSampleId :

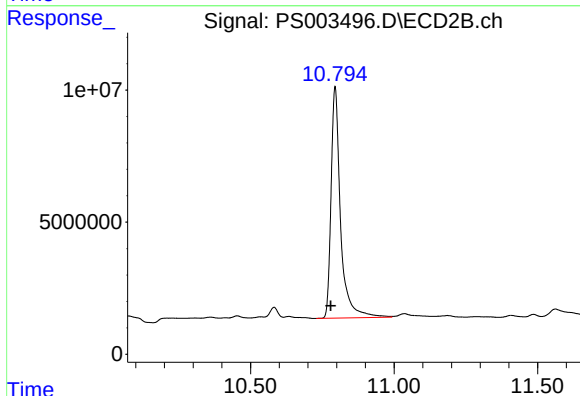


#4 2,4-DCAA

R.T.: 10.795 min
Delta R.T.: 0.015 min
Response: 201262981
Conc: 428.61 ng/ml

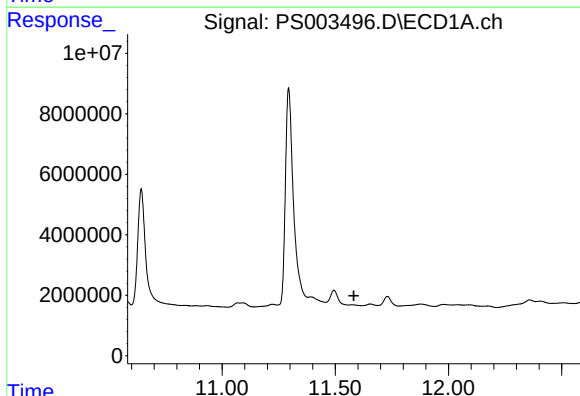


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.582 min
Response: 0
Conc: N.D.

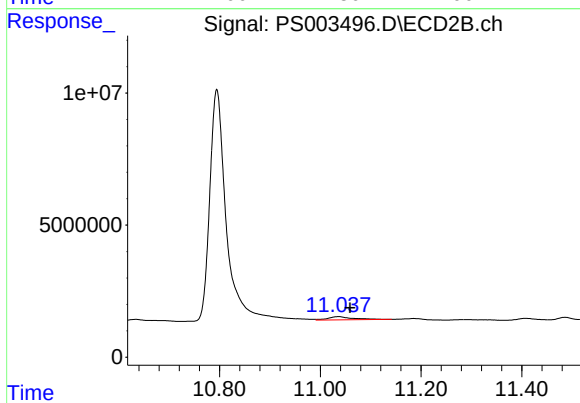

#5 DICAMBA


R.T.: 11.036 min
Delta R.T.: -0.023 min
Response: 4224965
Conc: 2.53 ng/ml

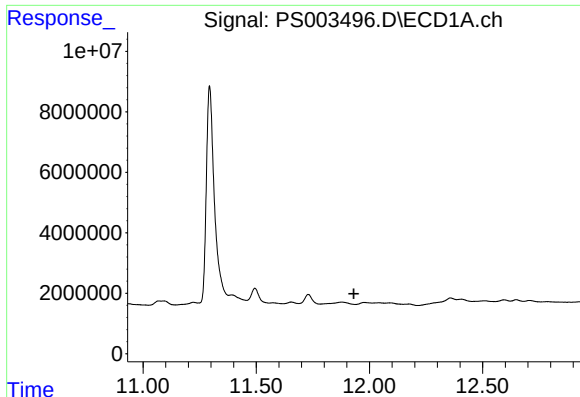

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.931 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

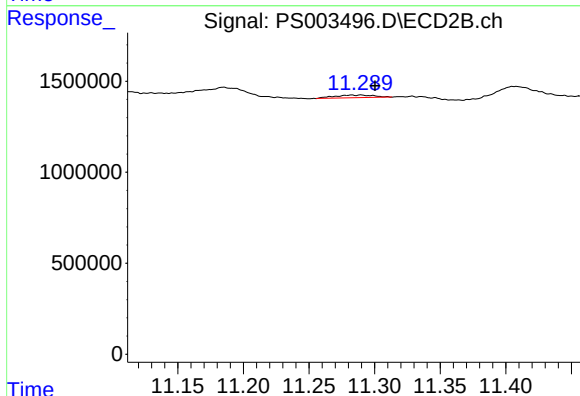


#6 MCP

R.T.: 11.288 min
Delta R.T.: -0.012 min
Response: 306641
Conc: 0.26 ug/ml

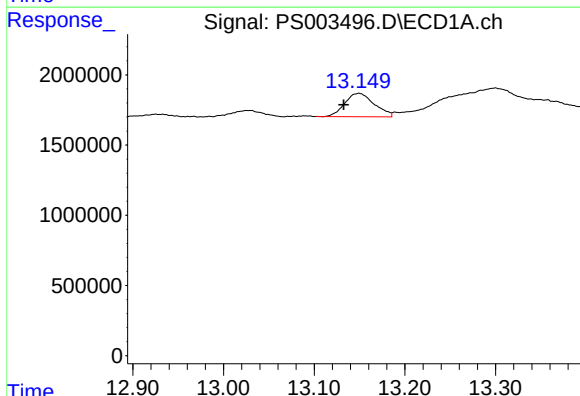


#9 2,4-D

R.T.: 13.149 min
Delta R.T.: 0.016 min
Response: 3771696
Conc: 8.13 ng/ml

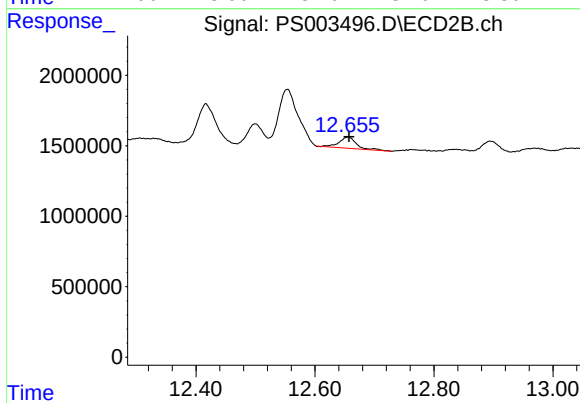

#9 2,4-D


R.T.: 12.655 min
Delta R.T.: -0.002 min
Response: 1607599
Conc: 3.06 ng/ml

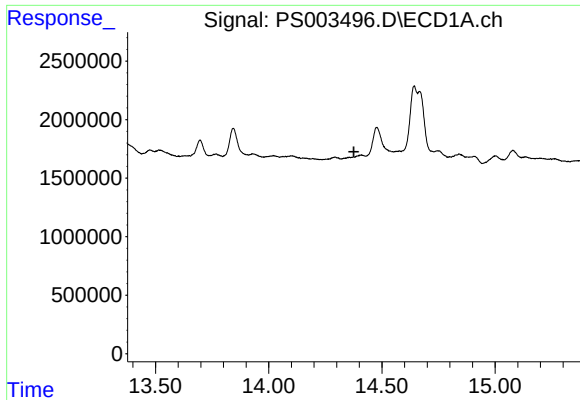

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

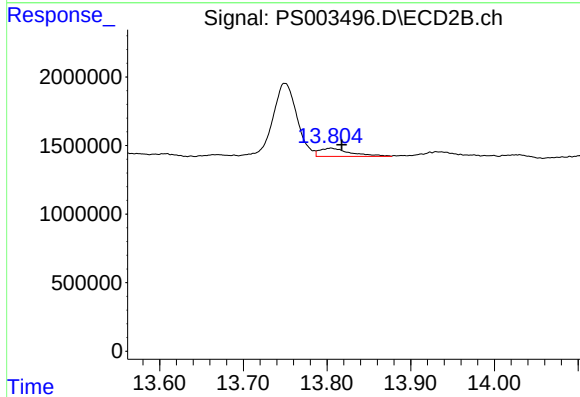


#11 2,4,5-TP (SILVEX)

R.T.: 13.805 min
Delta R.T.: -0.013 min
Response: 1537489
Conc: 0.60 ng/ml

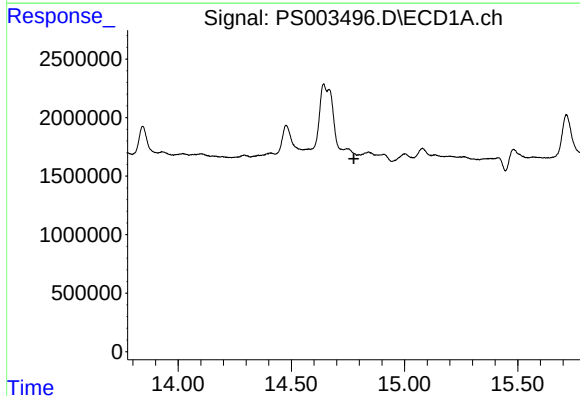


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

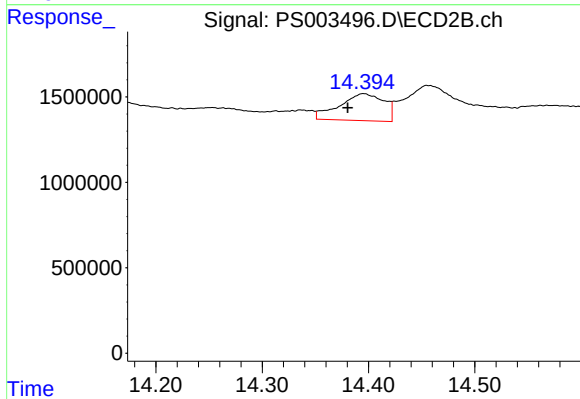

#12 2,4,5-T


R.T.: 14.395 min
Delta R.T.: 0.015 min
Response: 4608032
Conc: 2.28 ng/ml

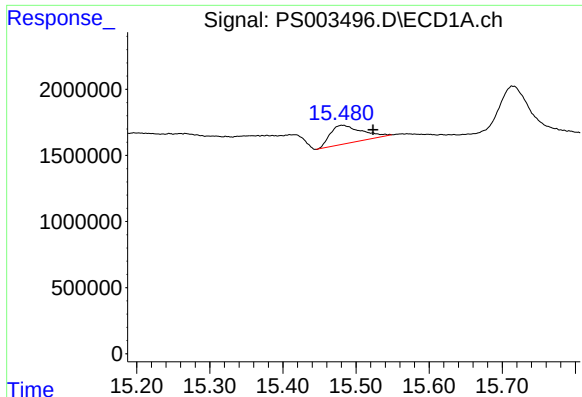

#13 2,4-DB


R.T.: 15.481 min
Delta R.T.: -0.042 min
Response: 4182303
Conc: 17.66 ng/ml

Instrument :
ECD_S
ClientSampleId :

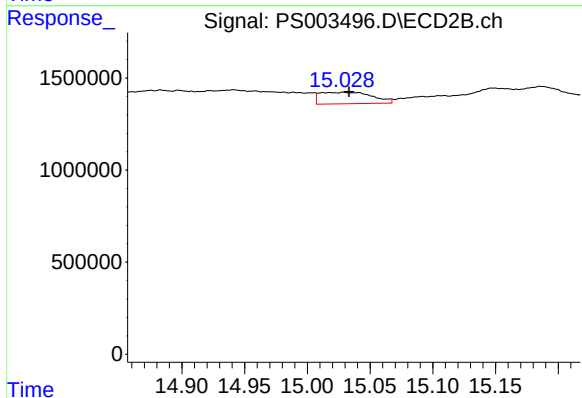


#13 2,4-DB

R.T.: 15.029 min
Delta R.T.: -0.004 min
Response: 1806281
Conc: 7.07 ng/ml

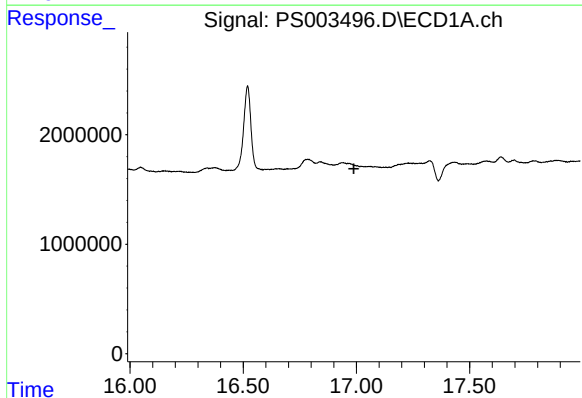


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 16.989 min
Response: 0
Conc: N.D.

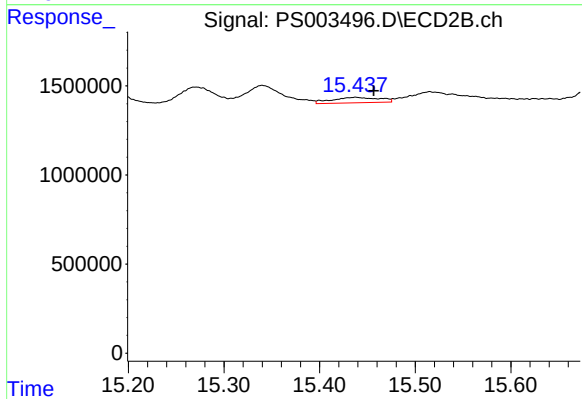

#14 DINOSEB


R.T.: 15.438 min
Delta R.T.: -0.019 min
Response: 1067624
Conc: 0.60 ng/ml

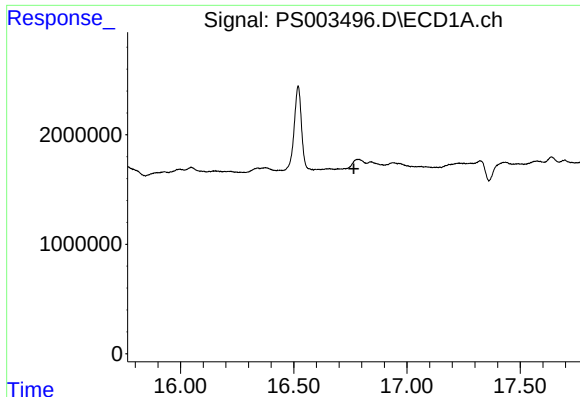

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.765 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

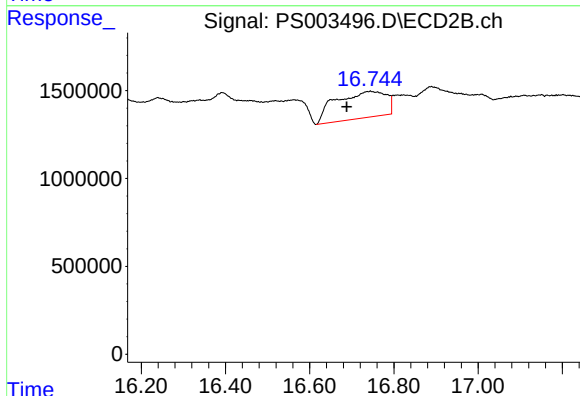


#15 Picloram

R.T.: 16.744 min
Delta R.T.: 0.056 min
Response: 12541408
Conc: 4.94 ng/ml

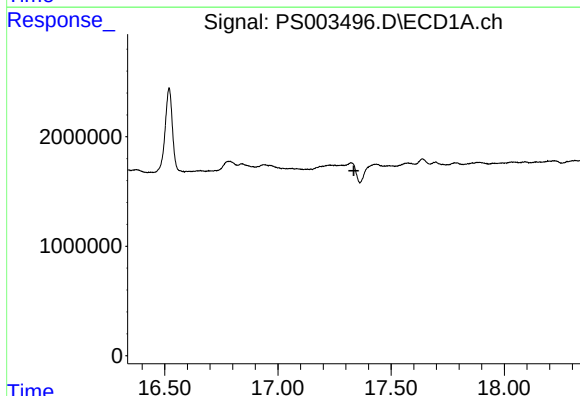

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.335 min
Response: 0
Conc: N.D.

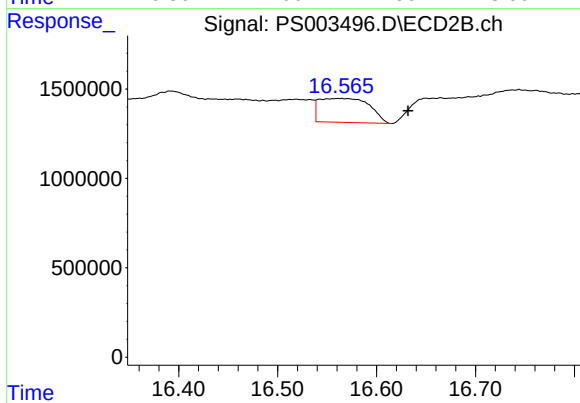

#16 DCPA

R.T.: 16.563 min
Delta R.T.: -0.069 min
Response: 4713484
Conc: 1.52 ng/ml